


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022421\
Data File : VN065991.D
Acq On : 24 Feb 2021 9:01
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Title : SW846 8260
Last Update : Wed Feb 17 15:48:13 2021

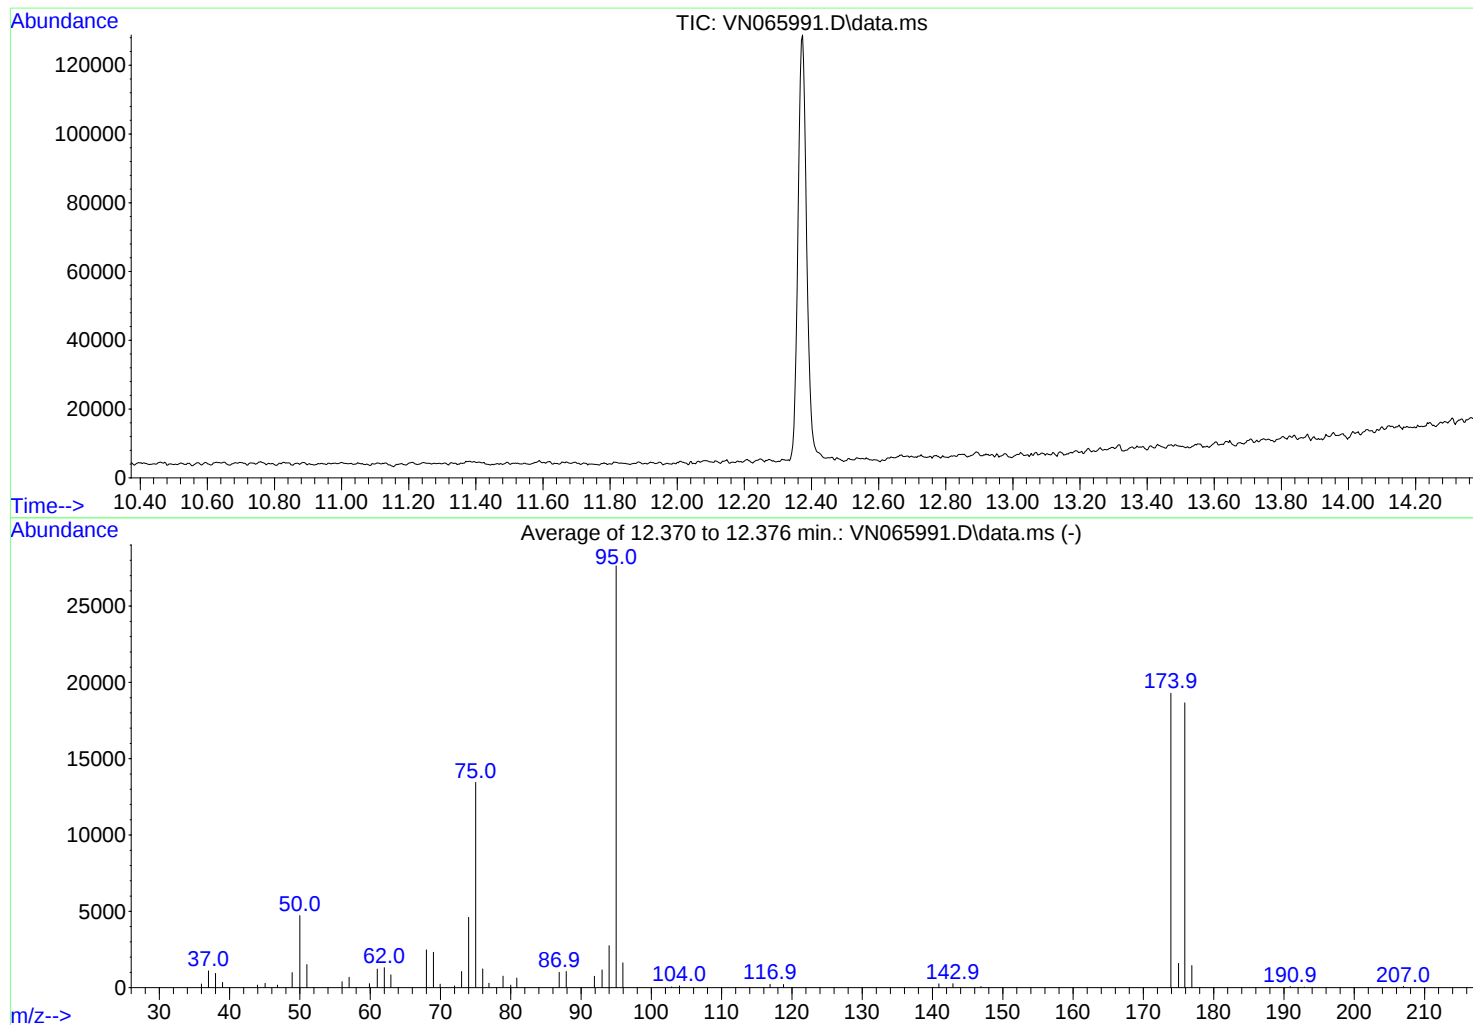

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.1	4714	PASS
75	95	30	60	48.7	13447	PASS
95	95	100	100	100.0	27637	PASS
96	95	5	9	5.9	1628	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	69.8	19291	PASS
175	174	5	9	8.3	1594	PASS
176	174	95	101	96.7	18659	PASS
177	176	5	9	7.7	1445	PASS