

Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN022519\
 Data File : VN053941.D
 Acq On : 25 Feb 2019 20:30
 Operator : JC/SP
 Sample : K1595-04
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11

Quant Time: Feb 26 06:20:17 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 26 05:37:40 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	597984	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1087063	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1052718	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	387992	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.03	65	382533	54.57	ug/l	0.00
Spiked Amount			Recovery	=	109.14%	
35) Dibromofluoromethane	7.59	113	353516	50.29	ug/l	0.00
Spiked Amount			Recovery	=	100.58%	
50) Toluene-d8	10.09	98	1378681	52.69	ug/l	0.00
Spiked Amount			Recovery	=	105.38%	
62) 4-Bromofluorobenzene	12.40	95	453420	52.01	ug/l	0.00
Spiked Amount			Recovery	=	104.02%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
11) Tert butyl alcohol	4.77	59	251	0.565	ug/l #	73
13) Acrolein	3.62	56	217	0.472	ug/l #	49
16) Acetone	3.82	43	33383	6.131	ug/l	93
18) Methyl Acetate	4.33	43	3684	0.752	ug/l #	71
20) Methylene Chloride	4.55	84	13044	1.880	ug/l	91
25) 2-Butanone	6.85	43	11121	4.041	ug/l #	87
29) Tetrahydrofuran	7.21	42	1089	0.594	ug/l #	31
31) Cyclohexane	7.67	56	10063	0.492	ug/l #	1
36) 1,1-Dichloropropene	7.66	75	41526	4.108	ug/l #	46
37) Ethyl Acetate	6.85	43	11121	1.541	ug/l #	67
38) Carbon Tetrachloride	7.67	117	51745	4.922	ug/l #	17
43) Isopropyl Acetate	8.17	43	31510	2.585	ug/l #	91
45) 1,2-Dichloropropane	9.27	63	1817	0.217	ug/l #	44
48) Methyl methacrylate	9.18	41	10858	1.937	ug/l #	12
51) 4-Methyl-2-Pentanone	10.02	43	8894	1.420	ug/l #	34
54) cis-1,3-Dichloropropene	9.91	75	68088	5.790	ug/l #	68
56) Ethyl methacrylate	10.54	69	1375	2.102	ug/l #	1
57) 1,3-Dichloropropane	10.77	76	11555	1.001	ug/l #	43
59) 2-Hexanone	10.76	43	172250	42.288	ug/l #	48
71) Bromoform	12.40	173	3590	0.644	ug/l #	1
76) 1,2,3-Trichloropropane	12.40	75	218144	35.048	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	218144	110.775	ug/l #	15
93) 1,2,4-Trichlorobenzene	14.91	180	65	2.231	ug/l #	11
95) Naphthalene	15.13	128	2786	3.382	ug/l #	87


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA_N\DATA\VN022519\
Data File : VN053941.D
Acq On : 25 Feb 2019 20:30
Operator : JC/SP
Sample : K1595-04
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
TP-CBF-B11

Quant Time: Feb 26 06:20:17 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 26 05:37:40 2019
Response via : Initial Calibration

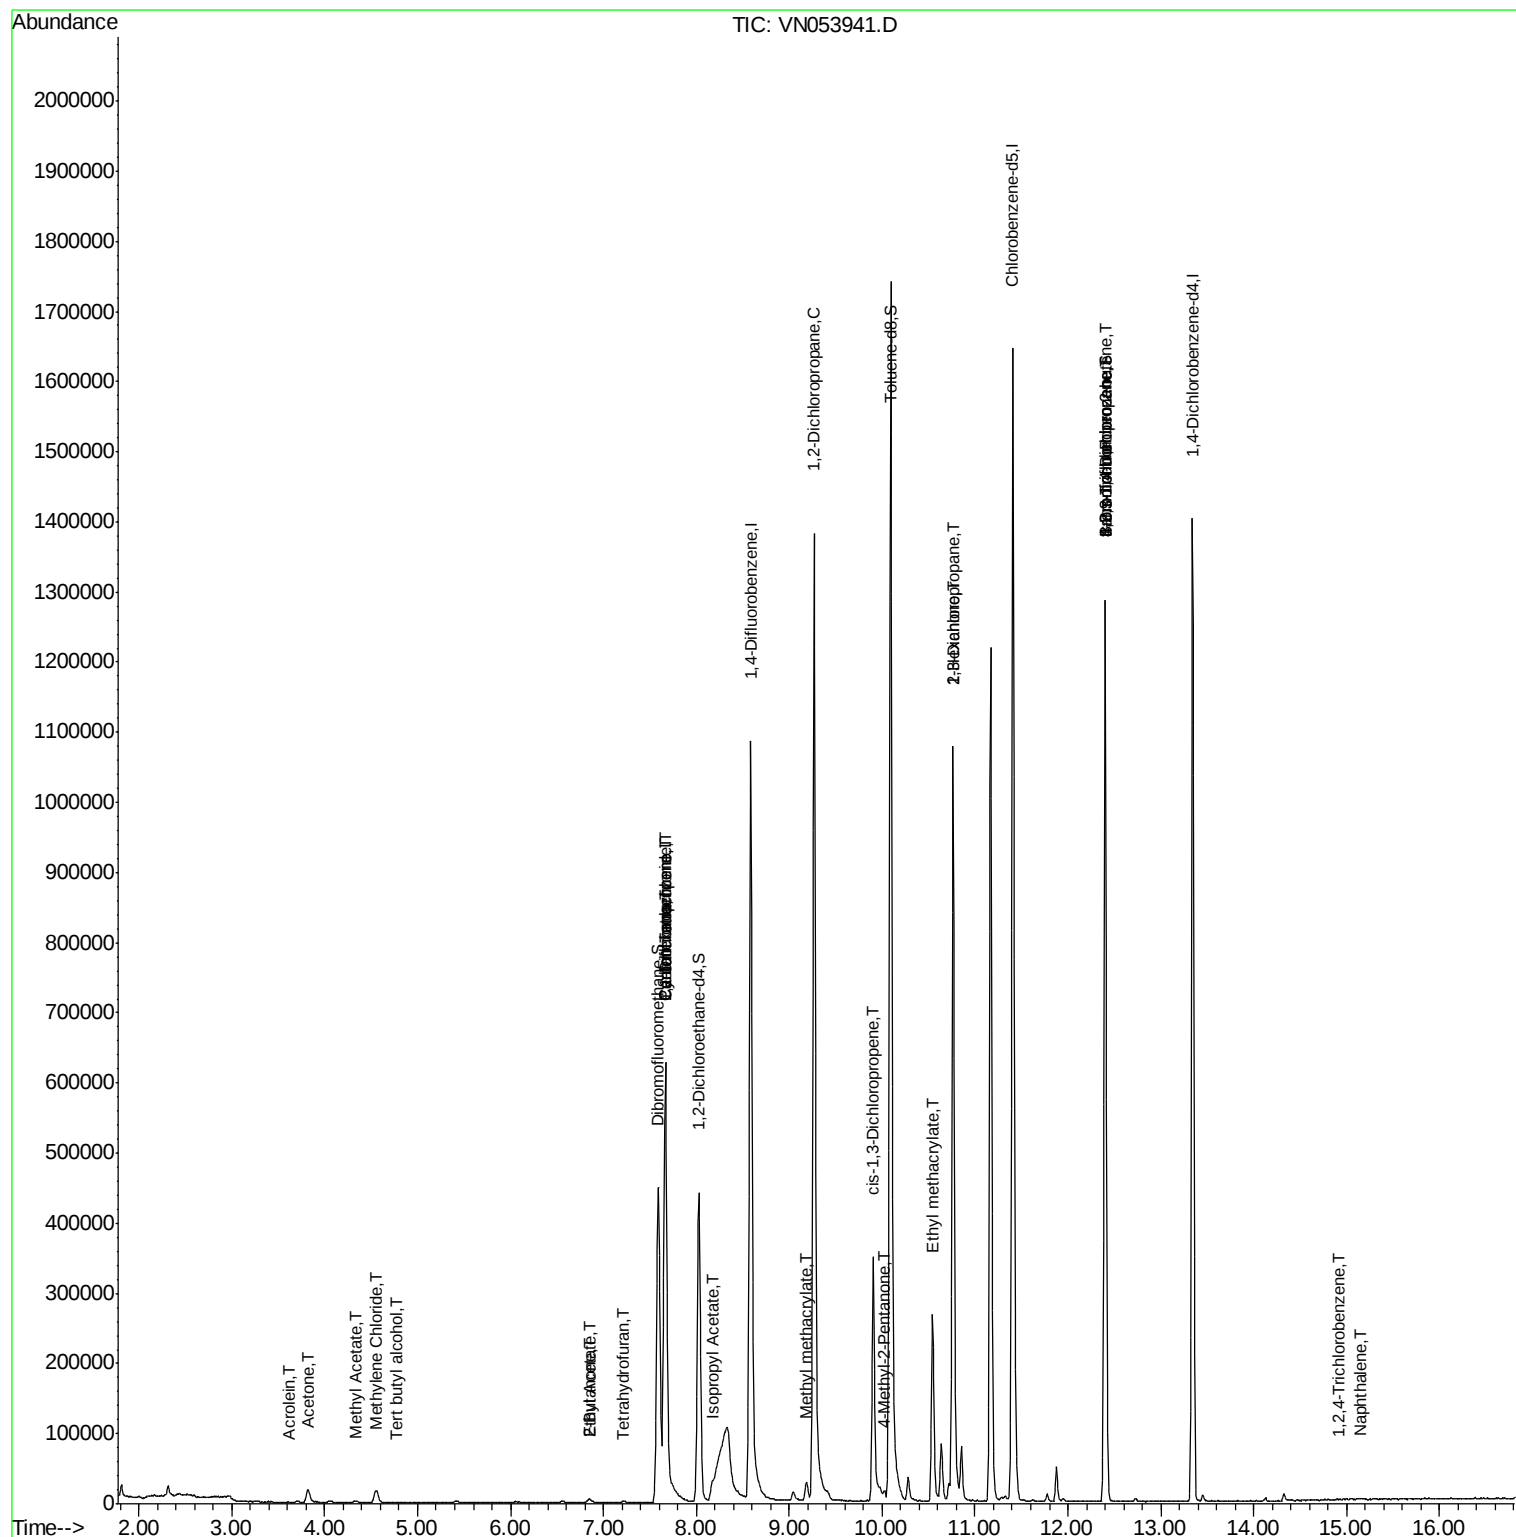

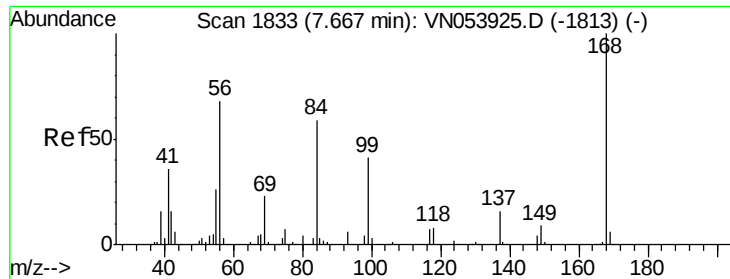

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampleId :


TP-CBF-B11

Tgt Ion:168 Resp: 597984

Ion Ratio Lower Upper




168 100

99 51.5 36.9 55.3

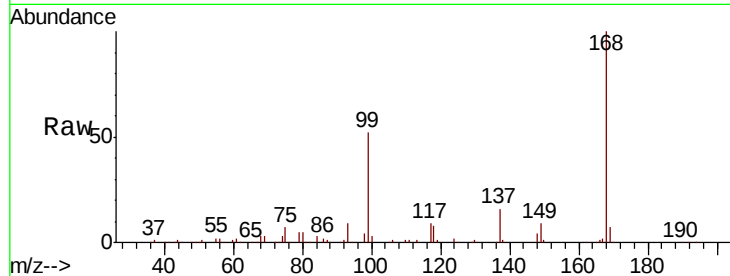

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN0

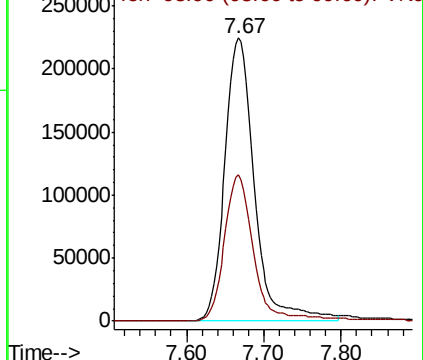

#11

Tert butyl alcohol

Concen: 0.565 ug/l

RT: 4.77 min Scan# 931

Delta R.T. -0.01 min

Lab File: VN053941.D


Acq: 25 Feb 2019 20:30

Tgt Ion: 59 Resp: 251

Ion Ratio Lower Upper



59 100


57 0.0 8.1 12.1#



Abundance Ion 59.00 (58.70 to 59.70): VN0

Ion 57.00 (56.70 to 57.70): VN0

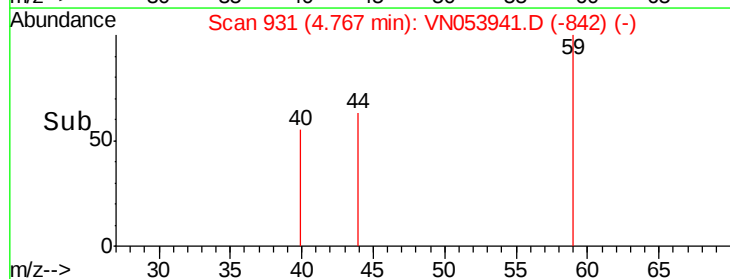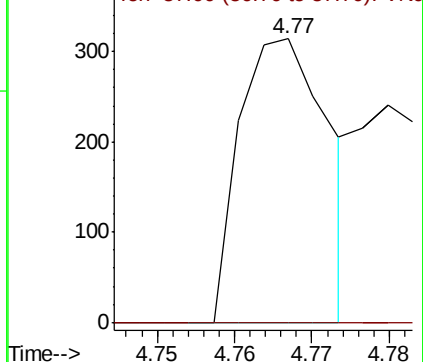

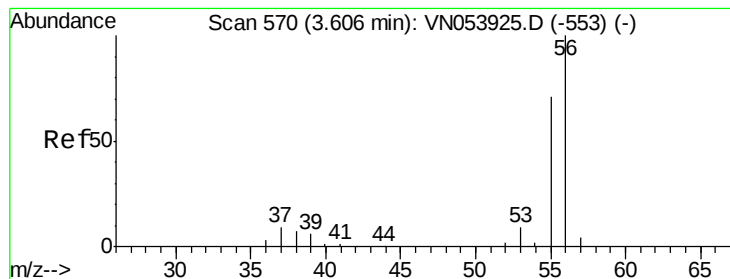

#13

Acrolein

Concen: 0.472 ug/l

RT: 3.62 min Scan# 574

Delta R.T. 0.01 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampleId :


TP-CBF-B11

Tgt Ion: 56 Resp: 217




Ion Ratio Lower Upper

56 100

55 28.1 56.3 84.5#



Abundance Ion 56.00 (55.70 to 56.70): VN053925.D (-553) (-)

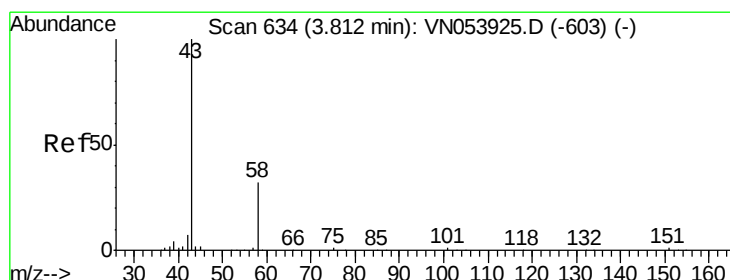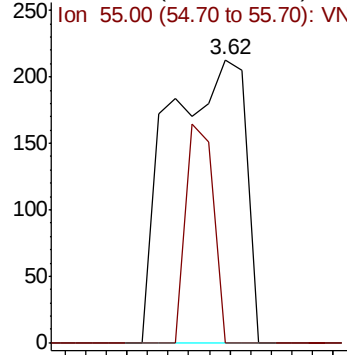

#16

Acetone

Concen: 6.131 ug/l

RT: 3.82 min Scan# 636

Delta R.T. 0.01 min

Lab File: VN053941.D


Acq: 25 Feb 2019 20:30

Tgt Ion: 43 Resp: 33383



Ion Ratio Lower Upper


43 100

58 30.7 27.6 41.4



Abundance Ion 43.00 (42.70 to 43.70): VN053925.D (-603) (-)




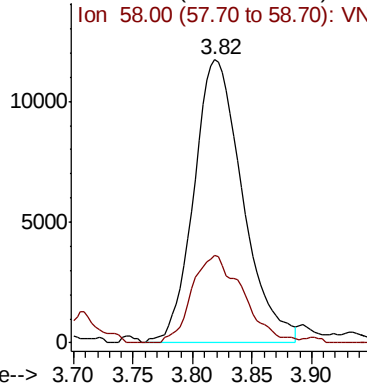


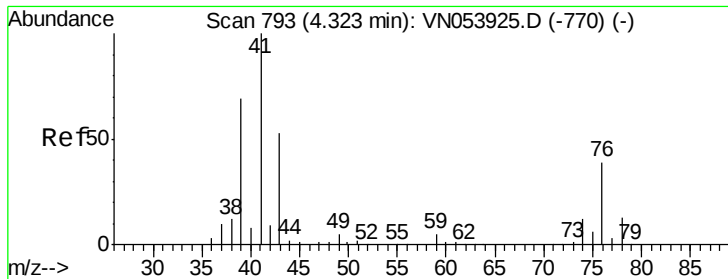

#18
Methyl Acetate
Concen: 0.752 ug/l
RT: 4.33 min Scan# 796
Delta R.T. 0.01 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30




Instrument :
MSVOA_N
ClientSampled :
TP-CBF-B11


Tgt Ion: 43 Resp: 3684
Ion Ratio Lower Upper
43 100
74 11.2 20.5 30.7#

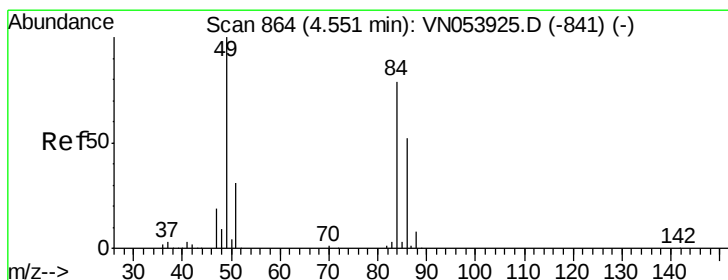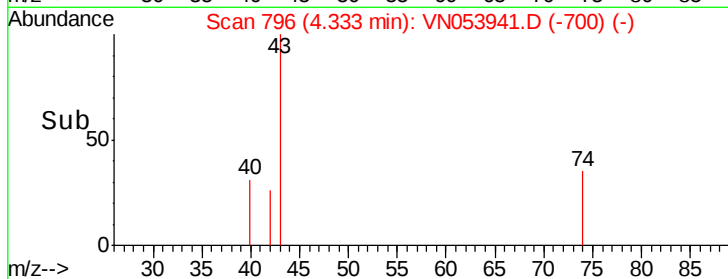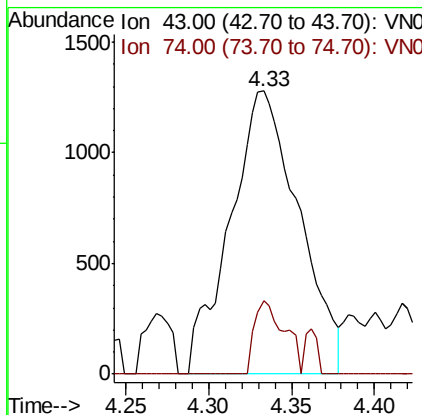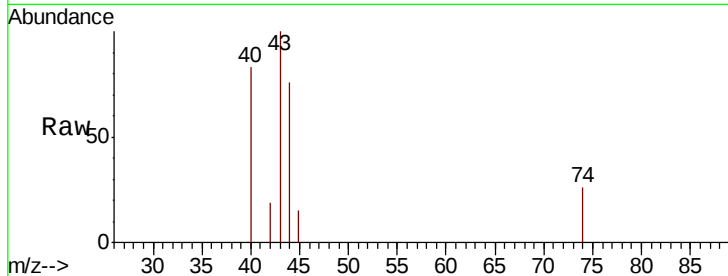

#20
Methylene Chloride
Concen: 1.880 ug/l
RT: 4.55 min Scan# 865
Delta R.T. 0.00 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30

Tgt Ion: 84 Resp: 13044
Ion Ratio Lower Upper
84 100
49 120.9 89.7 134.5
51 39.3 27.8 41.8
86 54.6 51.3 76.9

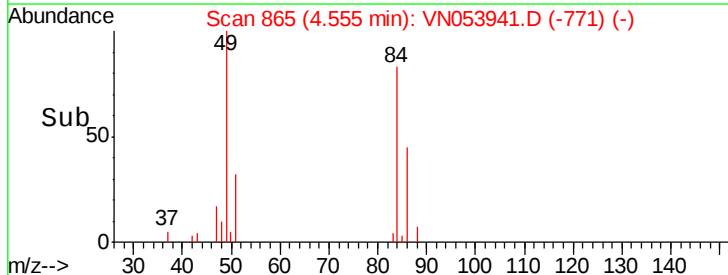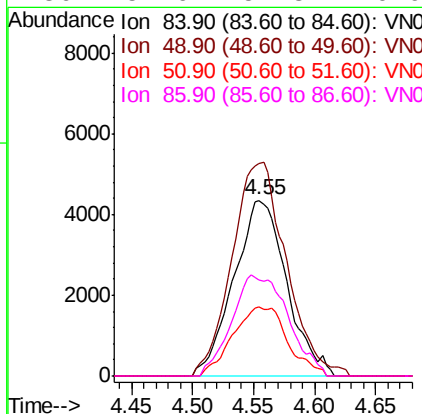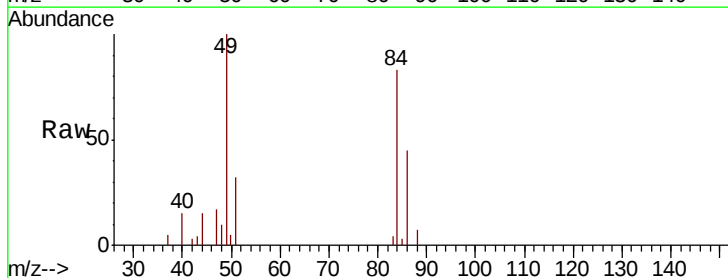

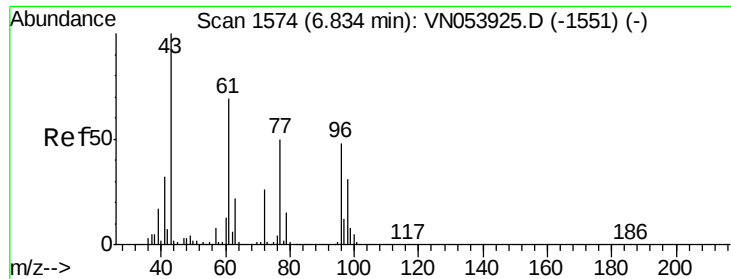

#25

2-Butanone

Concen: 4.041 ug/l

RT: 6.85 min Scan# 1578

Delta R.T. 0.01 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampled :





TP-CBF-B11

Tgt Ion: 43 Resp: 11121

Ion Ratio Lower Upper

43 100

72 20.9 22.1 33.1#

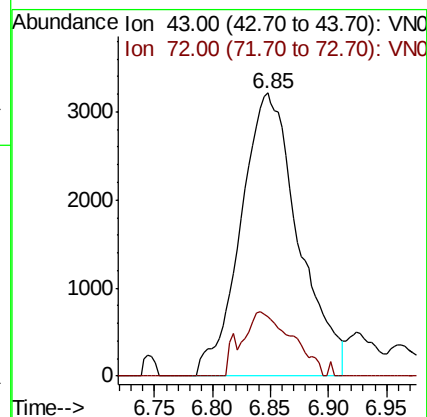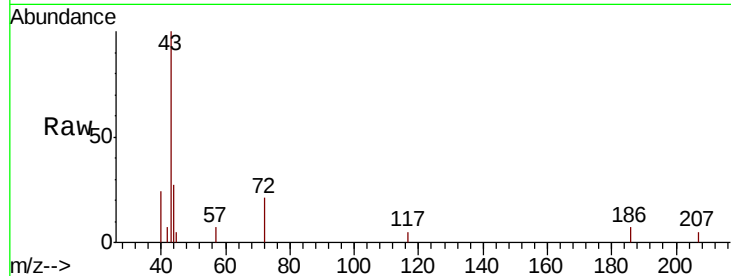

#29

Tetrahydrofuran

Concen: 0.594 ug/l

RT: 7.21 min Scan# 1691

Delta R.T. 0.00 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30




Tgt Ion: 42 Resp: 1089


Ion Ratio Lower Upper

42 100

72 0.0 36.9 55.3#

71 0.0 34.6 52.0#

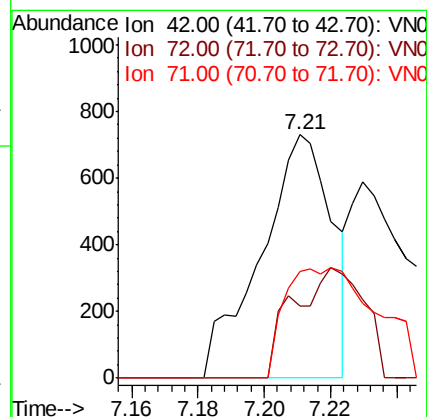

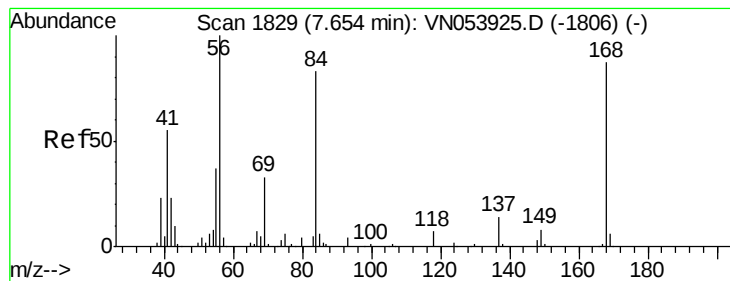

#31

Cyclohexane

Concen: 0.492 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.01 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampleId :

TP-CBF-B11


Tgt Ion: 56 Resp: 10063

Ion Ratio Lower Upper

56 100

69 186.2 26.0 39.0#




84 146.4 69.1 103.7#



Abundance Ion 56.00 (55.70 to 56.70): VN0

Ion 69.00 (68.70 to 69.70): VN0

Ion 84.00 (83.70 to 84.70): VN0

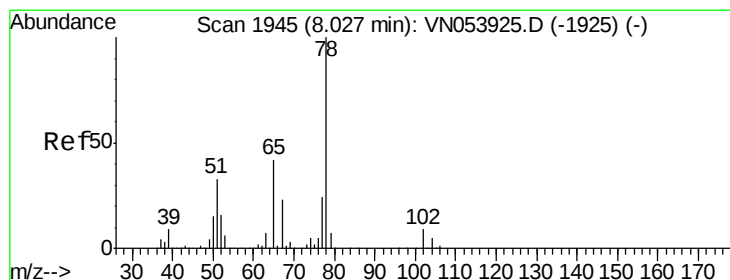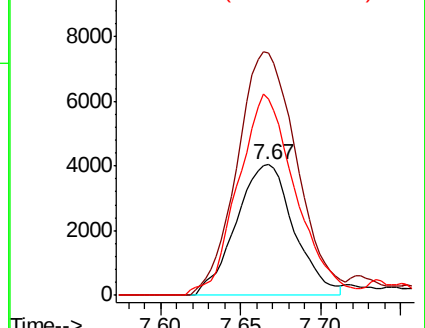

#33

1,2-Dichloroethane-d4

Concen: 54.572 ug/l

RT: 8.03 min Scan# 1945

Delta R.T. 0.00 min

Lab File: VN053941.D


Acq: 25 Feb 2019 20:30

Tgt Ion: 65 Resp: 382533

Ion Ratio Lower Upper



65 100


67 53.5 0.0 111.8

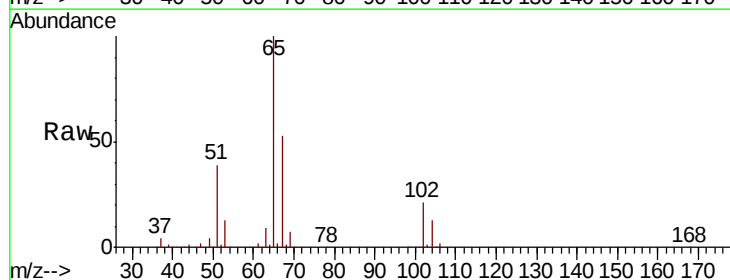

Abundance Ion 64.90 (64.60 to 65.60): VN0

Ion 66.90 (66.60 to 67.60): VN0

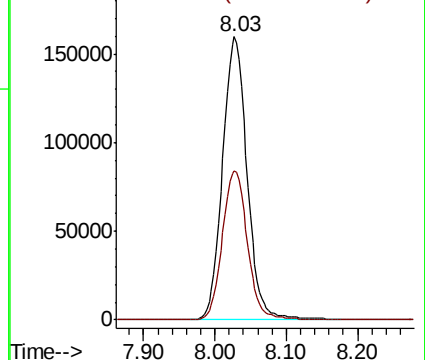


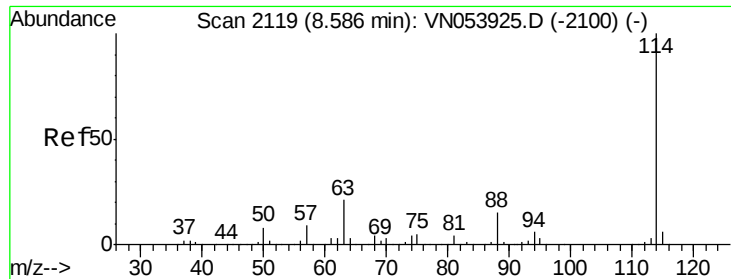




#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11

Tgt Ion:114 Resp: 1087063
 Ion Ratio Lower Upper
 114 100
 63 20.6 0.0 37.4
 88 15.4 0.0 30.4

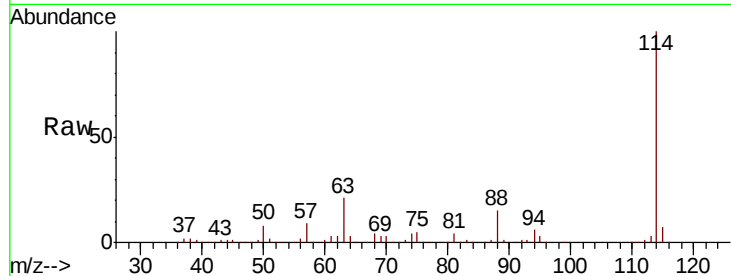


Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN


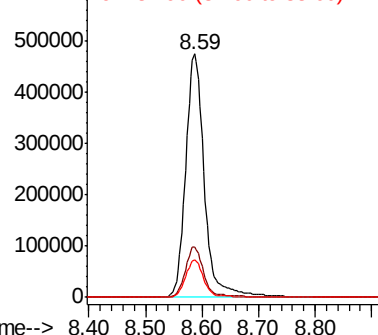



#35
 Dibromofluoromethane
 Concen: 50.290 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. 0.00 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Tgt Ion:113 Resp: 353516
 Ion Ratio Lower Upper
 113 100
 111 102.1 81.1 121.7
 192 22.0 18.8 28.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

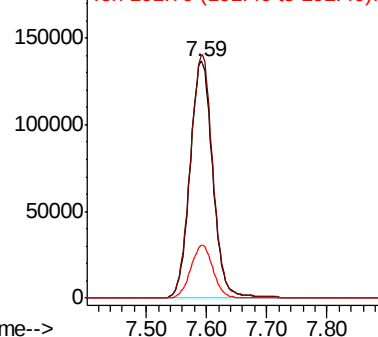

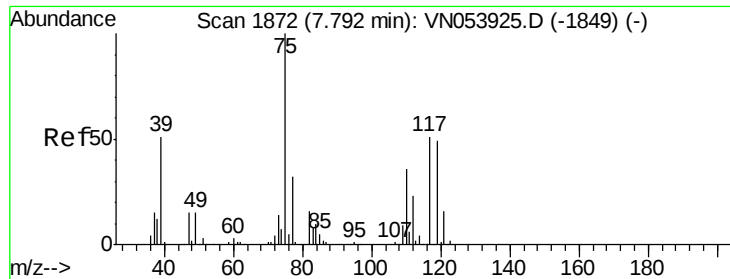

#36

1,1-Dichloropropene

Concen: 4.108 ug/l

RT: 7.66 min Scan# 1832

Delta R.T. -0.13 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampled :

TP-CBF-B11


Tgt Ion: 75 Resp: 41526

Ion Ratio Lower Upper

75 100

110 7.2 19.0 57.0#

77 0.0 25.4 38.0#



Abundance Ion 74.90 (74.60 to 75.60): VN053925.D (-1849) (-)

Ion 109.90 (109.60 to 110.60): VN053925.D (-1849) (-)

Ion 76.90 (76.60 to 77.60): VN053925.D (-1849) (-)

7.66

15000



10000

5000

0

7.60 7.70 7.80

Time-->



#37

Ethyl Acetate

Concen: 1.541 ug/l

RT: 6.85 min Scan# 1578

Delta R.T. -0.08 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30


Tgt Ion: 43 Resp: 11121

Ion Ratio Lower Upper

43 100

61 0.0 12.0 18.0#

70 0.0 8.7 13.1#



Abundance Ion 43.00 (42.70 to 43.70): VN053925.D (-1591) (-)

Ion 60.90 (60.60 to 61.60): VN053925.D (-1591) (-)

Ion 70.00 (69.70 to 70.70): VN053925.D (-1591) (-)

6.85

4000

3000


2000


1000

0

6.75 6.80 6.85 6.90 6.95

Time-->



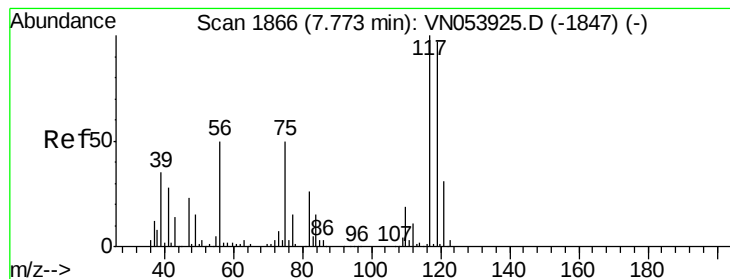

#38

Carbon Tetrachloride

Concen: 4.922 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. -0.11 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampled :

TP-CBF-B11


Tgt Ion:117 Resp: 51745

Ion Ratio Lower Upper

117 100

119 6.0 76.2 114.2#




121 0.0 24.6 36.8#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

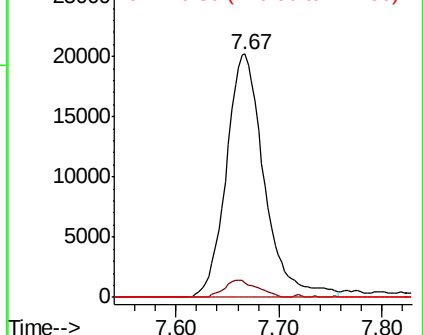

#43

Isopropyl Acetate

Concen: 2.585 ug/l

RT: 8.17 min Scan# 1989

Delta R.T. 0.01 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30


Tgt Ion: 43 Resp: 31510

Ion Ratio Lower Upper

43 100

61 18.1 17.4 26.0



87 10.2 11.5 17.3#




Abundance Ion 43.00 (42.70 to 43.70): V

Ion 61.00 (60.70 to 61.70): V

Ion 87.00 (86.70 to 87.70): V



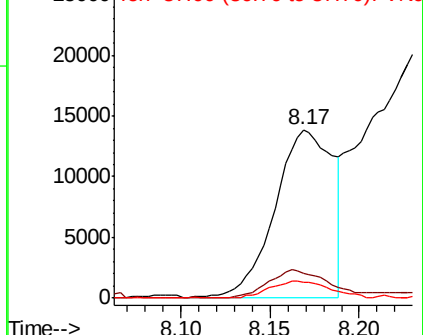



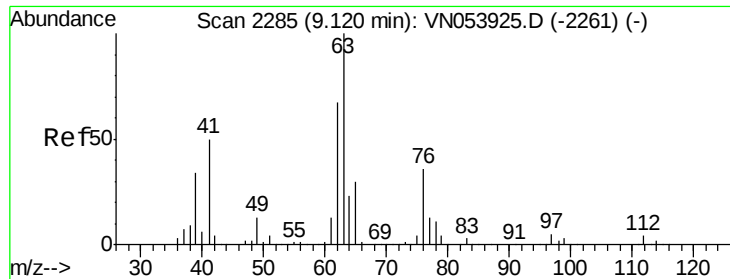

#45
 1,2-Dichloropropane
 Concen: 0.217 ug/l
 RT: 9.27 min Scan# 2330
 Delta R.T. 0.14 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11


Tgt Ion: 63 Resp: 1817
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.3 36.5#

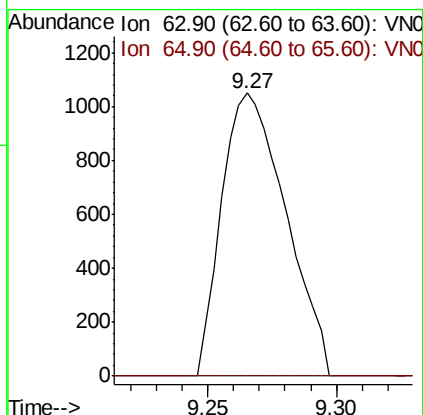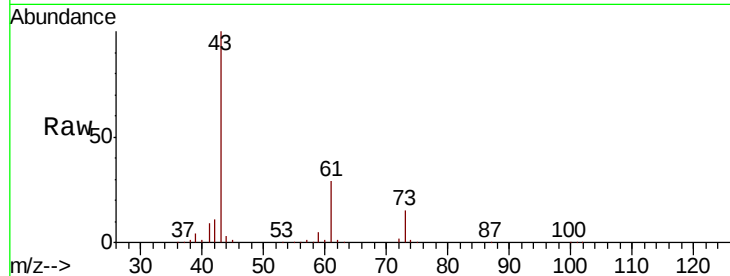

#48
 Methyl methacrylate
 Concen: 1.937 ug/l
 RT: 9.18 min Scan# 2303
 Delta R.T. -0.02 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Tgt Ion: 41 Resp: 10858
 Ion Ratio Lower Upper
 41 100
 69 0.0 74.8 112.2#
 39 0.0 39.0 58.6#


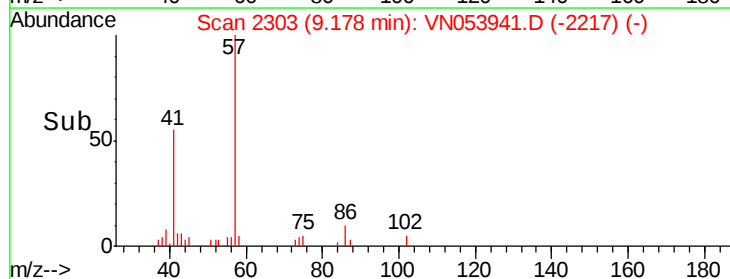
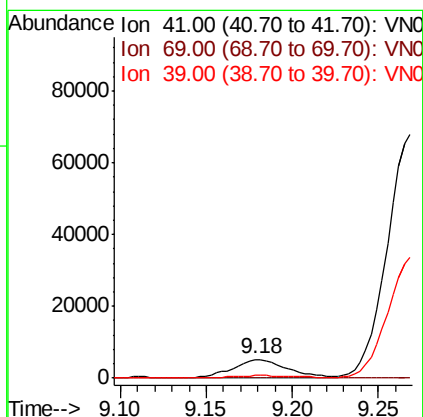





#50
Toluene-d8
Concen: 52.686 ug/l
RT: 10.09 min Scan# 2587
Delta R.T. 0.00 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30




Instrument :
MSVOA_N
ClientSampled :
TP-CBF-B11


Tgt Ion: 98 Resp: 1378681
Ion Ratio Lower Upper
98 100
100 63.2 51.9 77.9

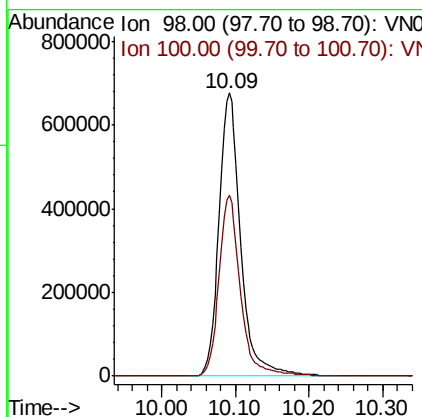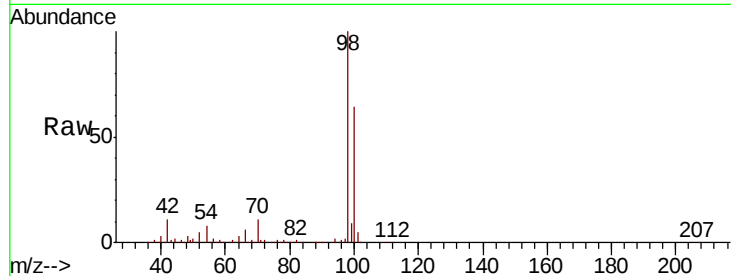

#51
4-Methyl-2-Pentanone
Concen: 1.420 ug/l
RT: 10.02 min Scan# 2566
Delta R.T. 0.04 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30

Tgt Ion: 43 Resp: 8894
Ion Ratio Lower Upper
43 100
58 0.0 32.7 49.1#



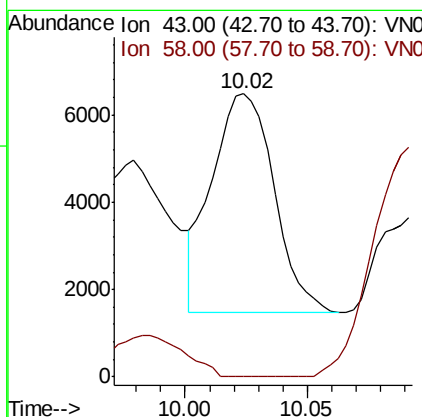



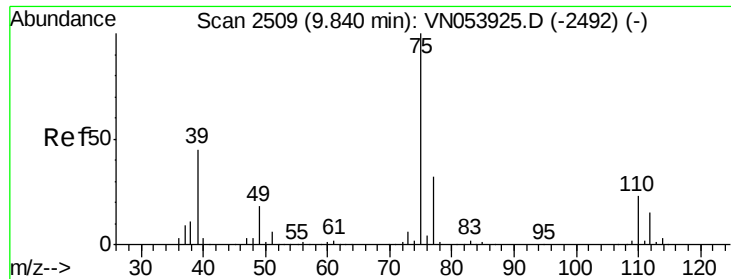

#54
 cis-1,3-Dichloropropene
 Concen: 5.790 ug/l
 RT: 9.91 min Scan# 2529
 Delta R.T. 0.06 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11


Tgt Ion: 75 Resp: 68088
 Ion Ratio Lower Upper
 75 100
 77 0.6 25.8 38.6#
 39 31.6 31.4 47.0

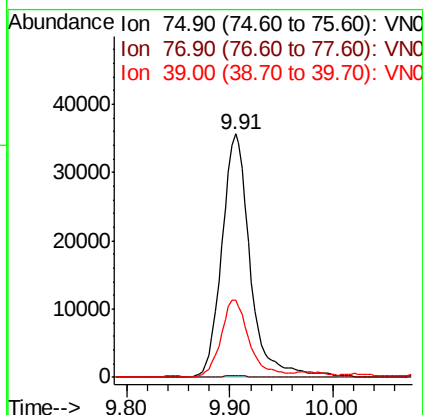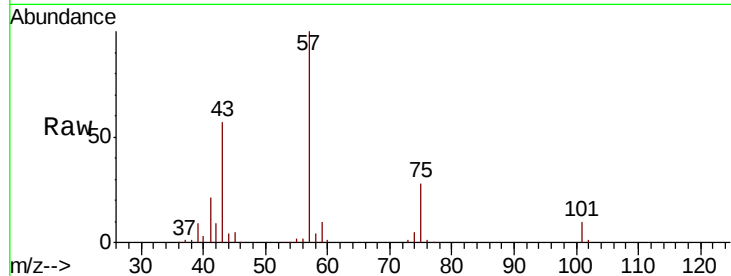

#56
 Ethyl methacrylate
 Concen: 2.102 ug/l
 RT: 10.54 min Scan# 2726
 Delta R.T. 0.11 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Tgt Ion: 69 Resp: 1375
 Ion Ratio Lower Upper
 69 100
 41 3841.3 47.5 71.3#
 39 1614.5 23.4 35.0#


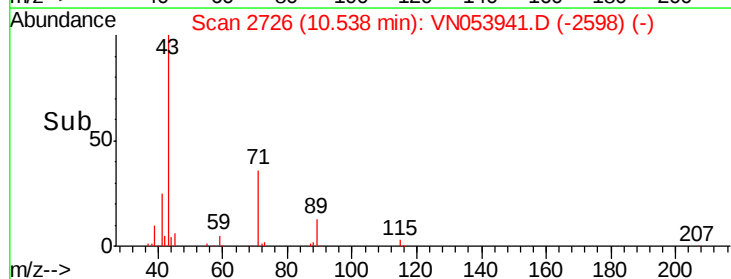
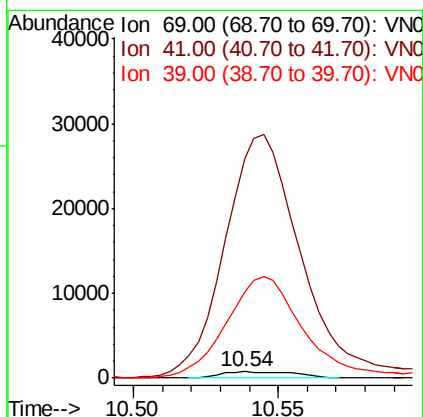



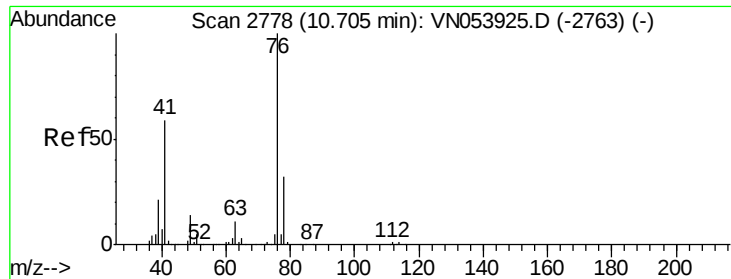

#57
 1,3-Dichloropropane
 Concen: 1.001 ug/l
 RT: 10.77 min Scan# 2797
 Delta R.T. 0.06 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30




Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11


Tgt Ion: 76 Resp: 11555
 Ion Ratio Lower Upper
 76 100
 78 0.0 25.2 37.8#

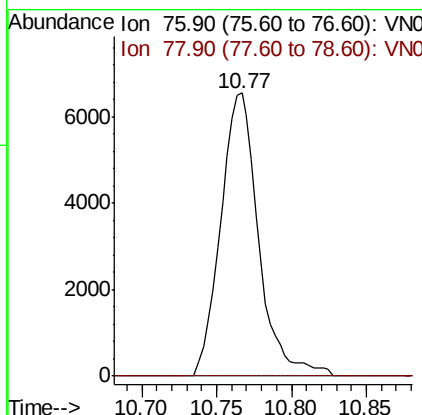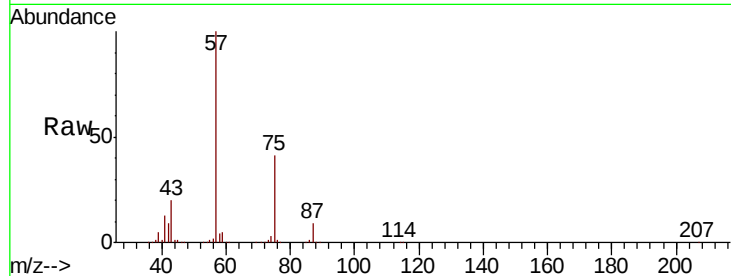

#59
 2-Hexanone
 Concen: 42.288 ug/l
 RT: 10.76 min Scan# 2796
 Delta R.T. 0.01 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Tgt Ion: 43 Resp: 172250
 Ion Ratio Lower Upper
 43 100
 58 19.3 29.1 87.4#



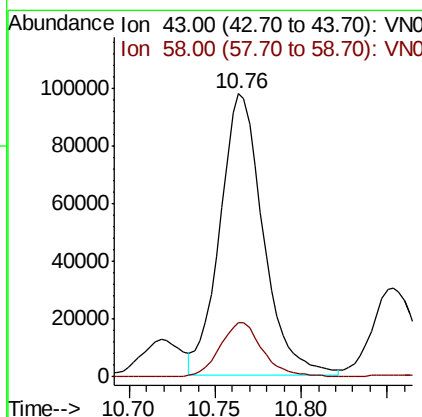





#62
4-Bromofluorobenzene
Concen: 52.007 ug/l
RT: 12.40 min Scan# 3305
Delta R.T. -0.00 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30




Instrument :
MSVOA_N
ClientSampleId :
TP-CBF-B11


Tgt Ion: 95 Resp: 453420
Ion Ratio Lower Upper
95 100
174 88.8 0.0 188.8
176 84.5 0.0 182.6

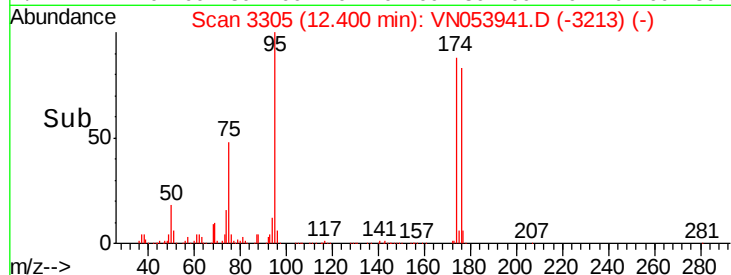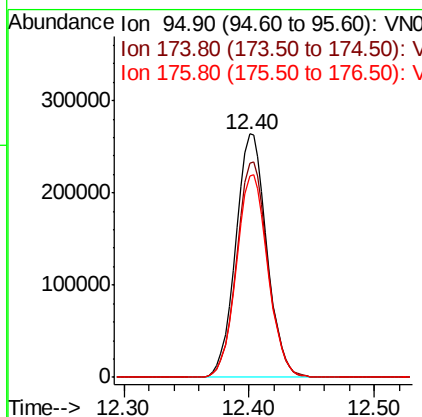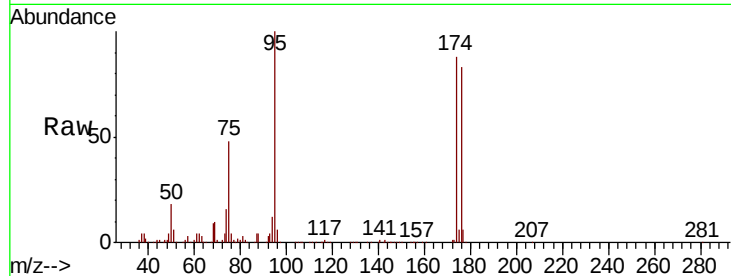

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN053941.D
Acq: 25 Feb 2019 20:30

Tgt Ion: 117 Resp: 1052718
Ion Ratio Lower Upper
117 100
82 55.8 41.4 62.2
119 31.6 25.3 37.9

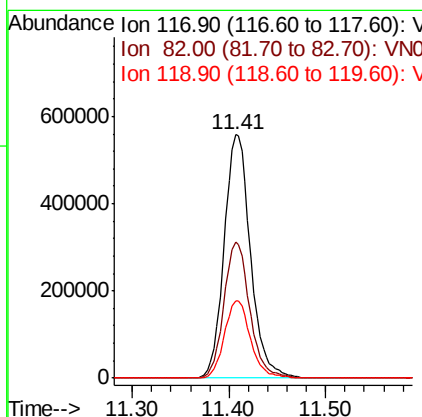



#71

Bromoform

Concen: 0.644 ug/l

RT: 12.40 min Scan# 3306

Delta R.T. 0.28 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampleId :

TP-CBF-B11


Tgt Ion:173 Resp: 3590

Ion Ratio Lower Upper

173 100

175 712.2 24.3 72.8#




254 0.0 0.2 0.2#

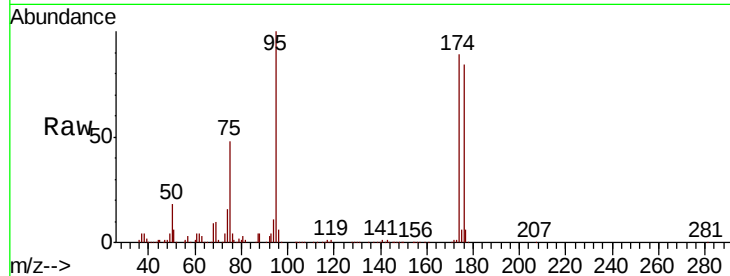

Abundance Ion 172.70 (172.40 to 173.40): V

Ion 174.70 (174.40 to 175.40): V

Ion 254.40 (254.10 to 255.10): V

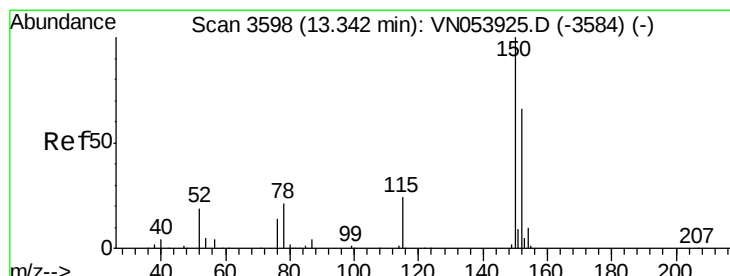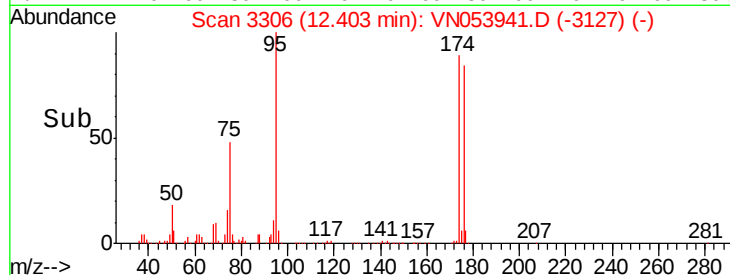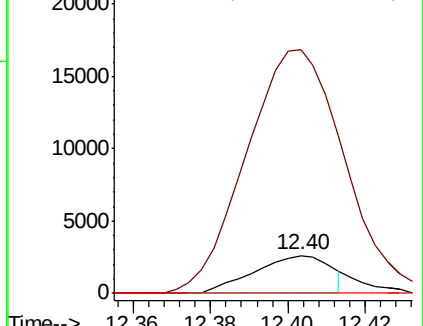

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3598

Delta R.T. 0.00 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30


Tgt Ion:152 Resp: 387992

Ion Ratio Lower Upper

152 100

115 57.0 27.2 81.6



150 156.6 0.0 348.2

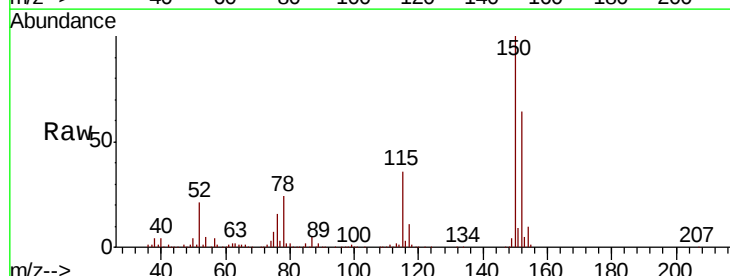


Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

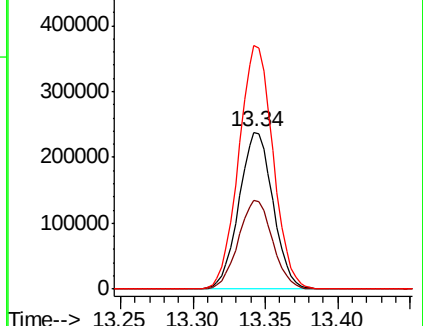



#76

1,2,3-Trichloropropane

Concen: 35.048 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.15 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30

Instrument :

MSVOA_N

ClientSampleId :


TP-CBF-B11

Tgt Ion: 75 Resp: 218144

Ion Ratio Lower Upper

75 100

77 1.2 0.0 0.0#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

150000



12.40

100000

50000

0

Time--> 12.30 12.40 12.50



#81

trans-1,4-Dichloro-2-butene

Concen: 110.775 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. 0.10 min

Lab File: VN053941.D

Acq: 25 Feb 2019 20:30


Tgt Ion: 75 Resp: 218144

Ion Ratio Lower Upper

75 100

53 0.0 68.6 102.8#

89 0.0 35.3 52.9#



Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0

150000


12.40


100000

50000

0

Time--> 12.30 12.40 12.50









#93
 1,2,4-Trichlorobenzene
 Concen: 2.231 ug/l
 RT: 14.91 min Scan# 4087
 Delta R.T. 0.01 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Instrument :
 MSVOA_N
 ClientSampleId :
 TP-CBF-B11

Tgt Ion:180 Resp: 65
 Ion Ratio Lower Upper
 180 100
 182 0.0 48.6 145.9#
 145 0.0 13.8 41.3#




Abundance Ion 179.80 (179.50 to 180.50): V
 Ion 181.80 (181.50 to 182.50): V
 Ion 144.80 (144.50 to 145.50): V

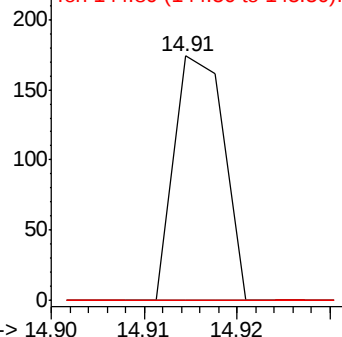

#95
 Naphthalene
 Concen: 3.382 ug/l
 RT: 15.13 min Scan# 4155
 Delta R.T. 0.00 min
 Lab File: VN053941.D
 Acq: 25 Feb 2019 20:30

Tgt Ion:128 Resp: 2786
 Ion Ratio Lower Upper
 128 100
 127 8.6 10.2 15.2#
 129 4.7 8.6 12.8#



Abundance Ion 128.00 (127.70 to 128.70): V
 Ion 127.00 (126.70 to 127.70): V
 Ion 129.00 (128.70 to 129.70): V

