



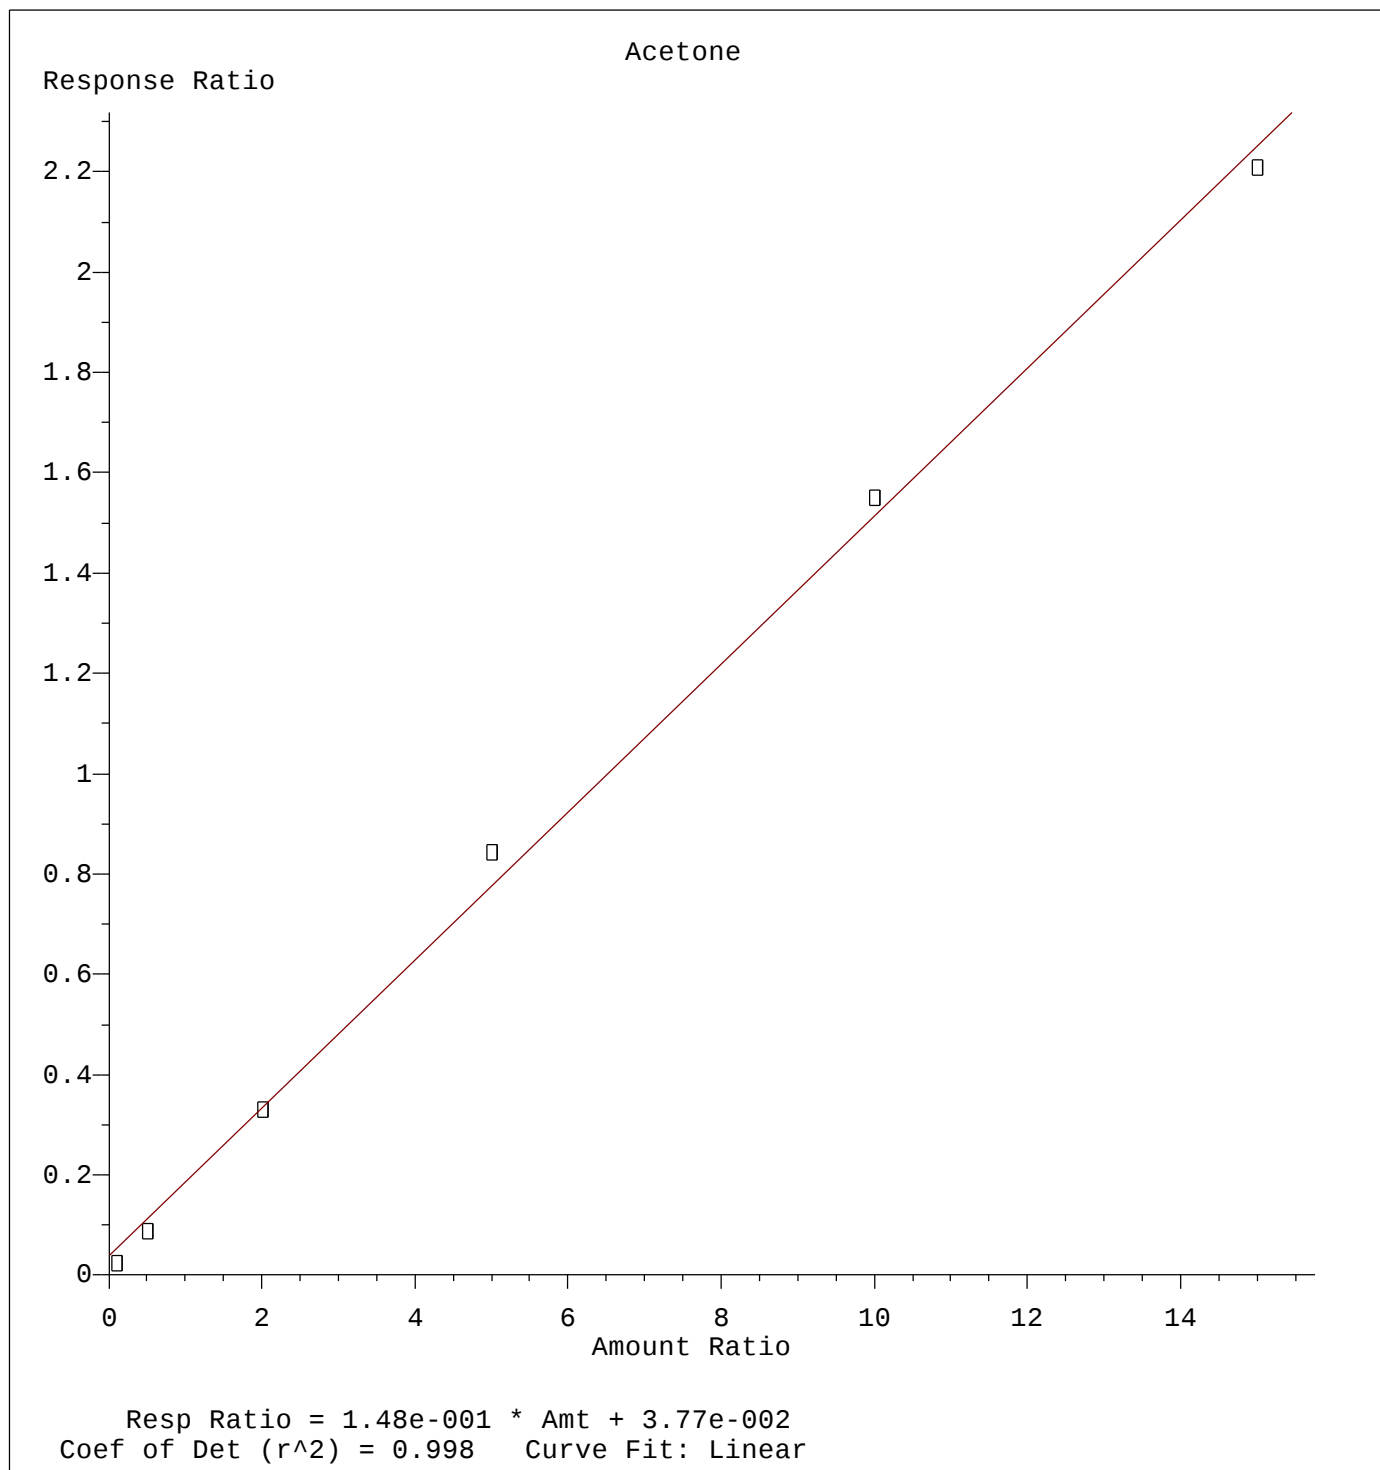

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019

1,2,3-Trichlorobenzene

Response Ratio

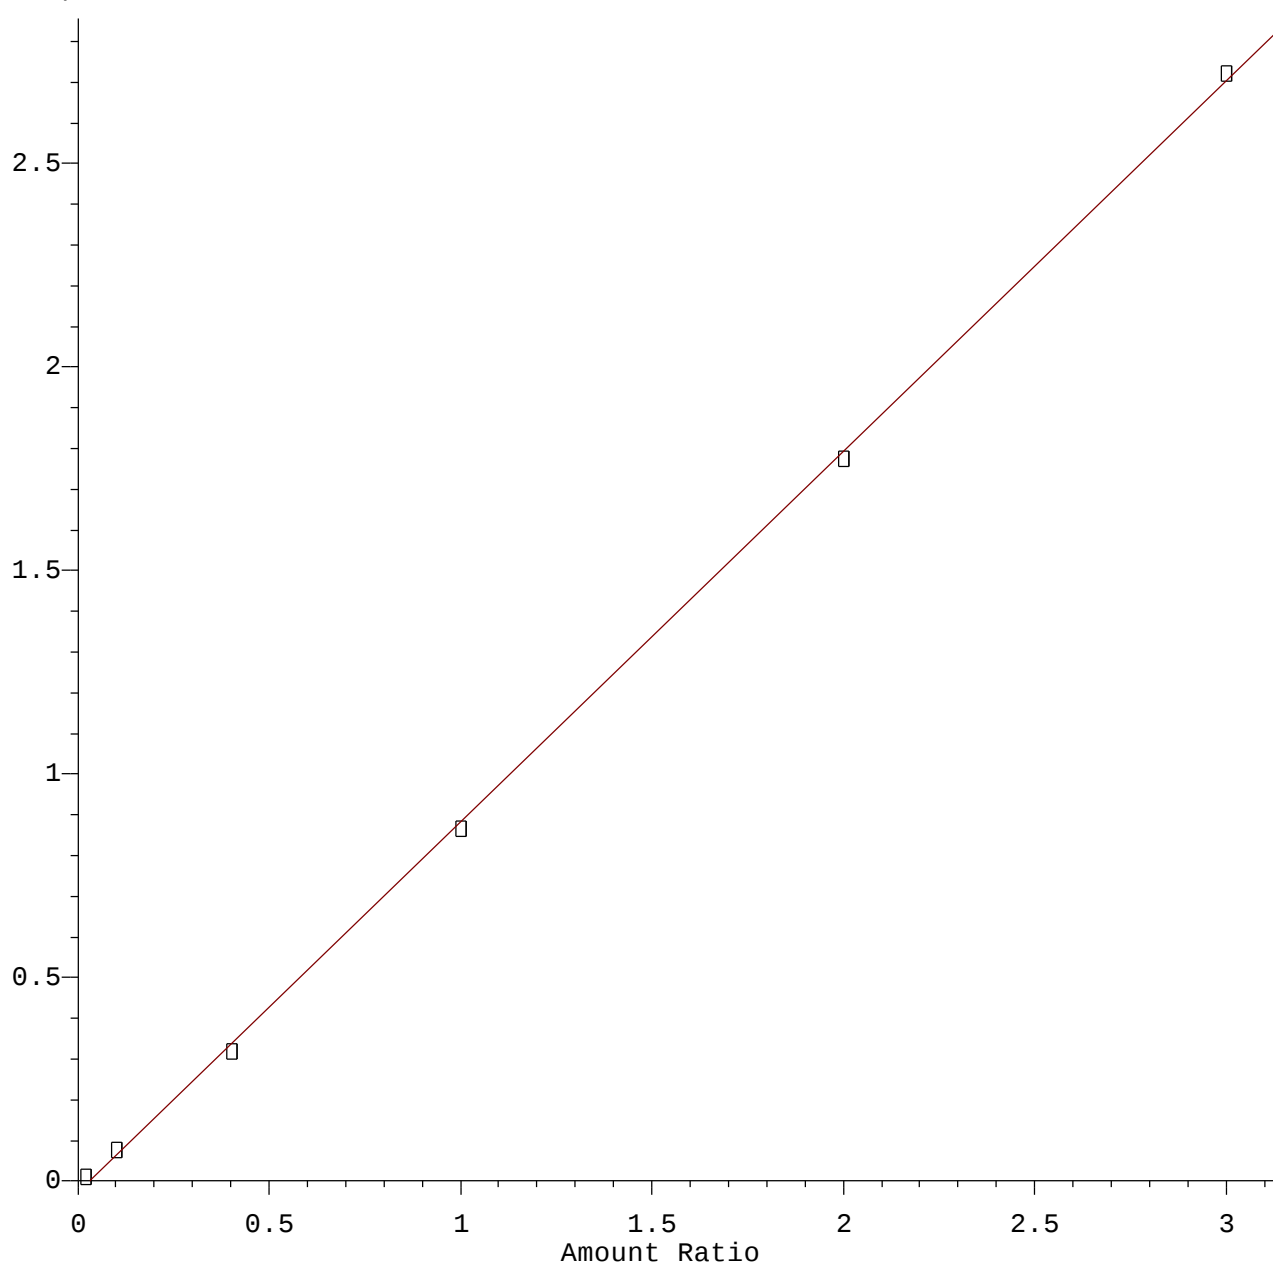


Resp Ratio = $9.10 \times 10^{-1} \times \text{Amt} - 2.83 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019

Naphthalene

Response Ratio

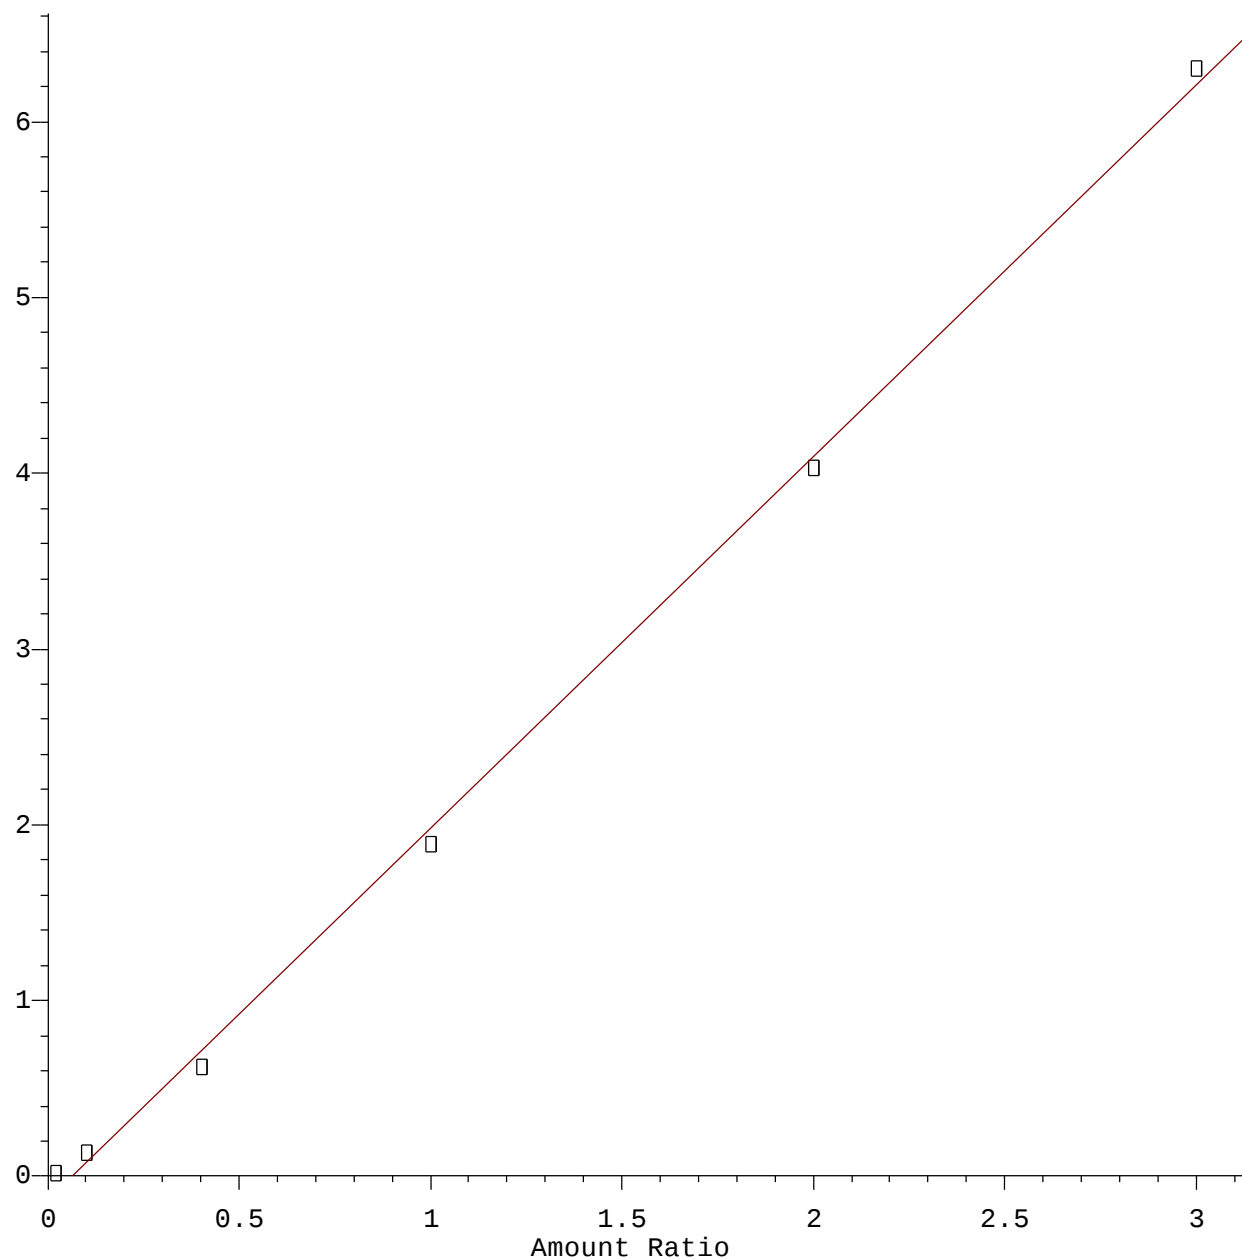


Resp Ratio = 2.12×10^0 * Amt - 1.36×10^{-1}
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019

1,2,4-Trichlorobenzene

Response Ratio

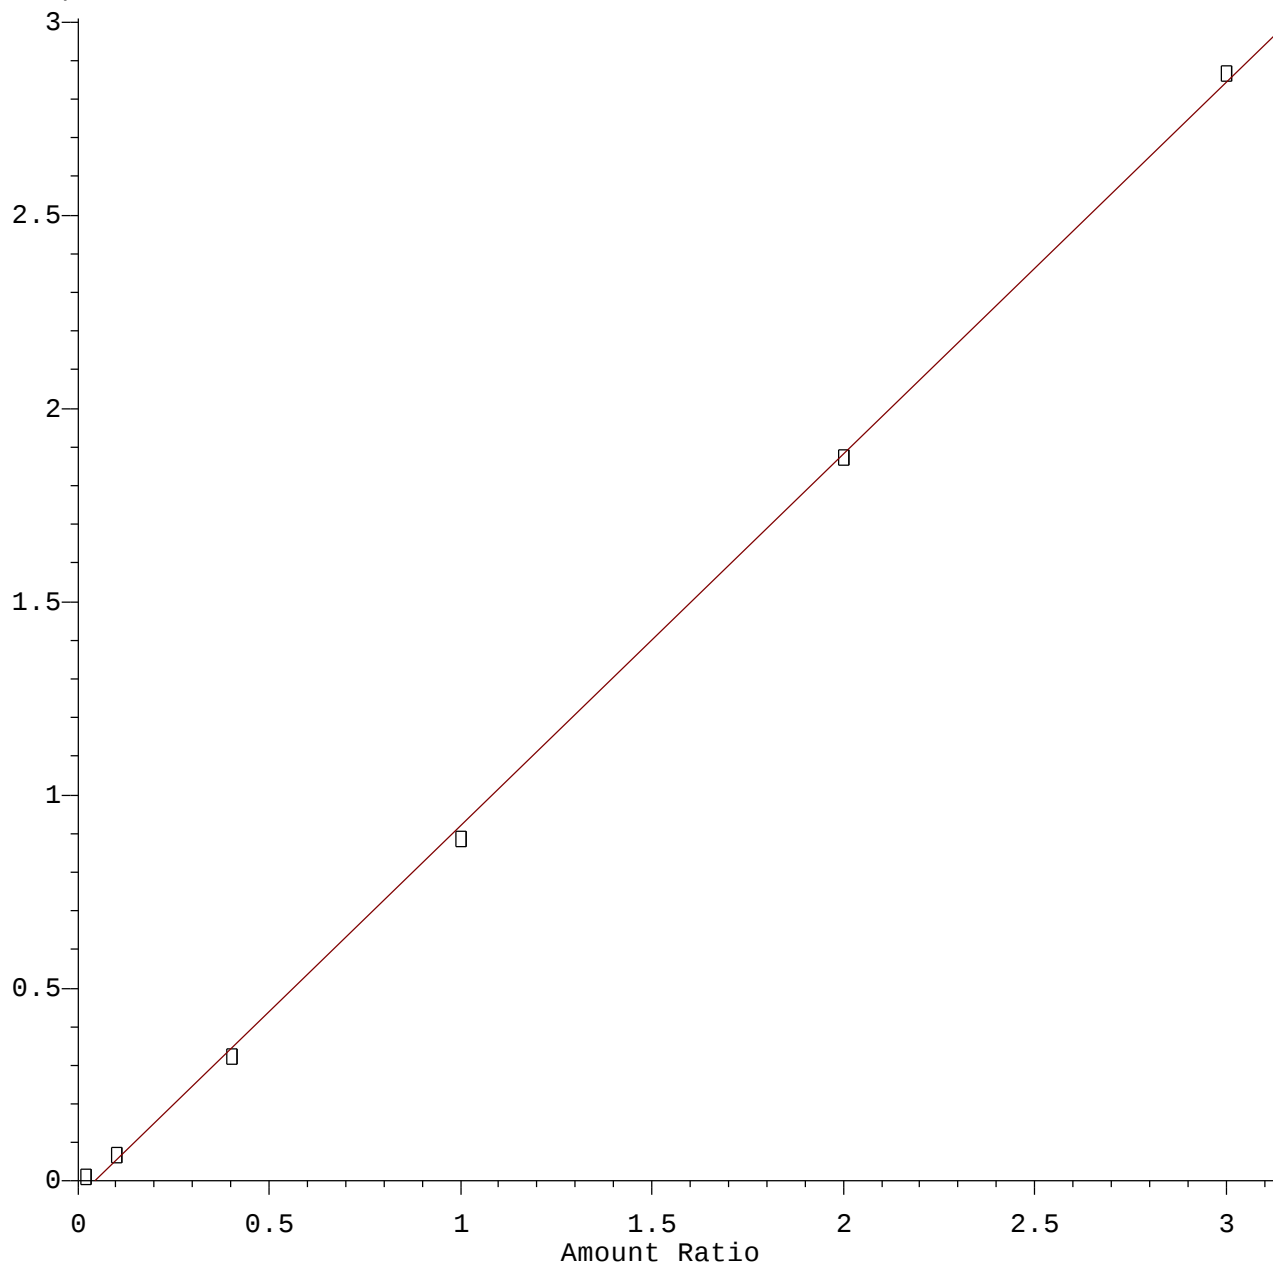


Resp Ratio = $9.62 \times 10^{-1} \times \text{Amt} - 4.28 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019


2-Chloroethyl Vinyl ether

Response Ratio

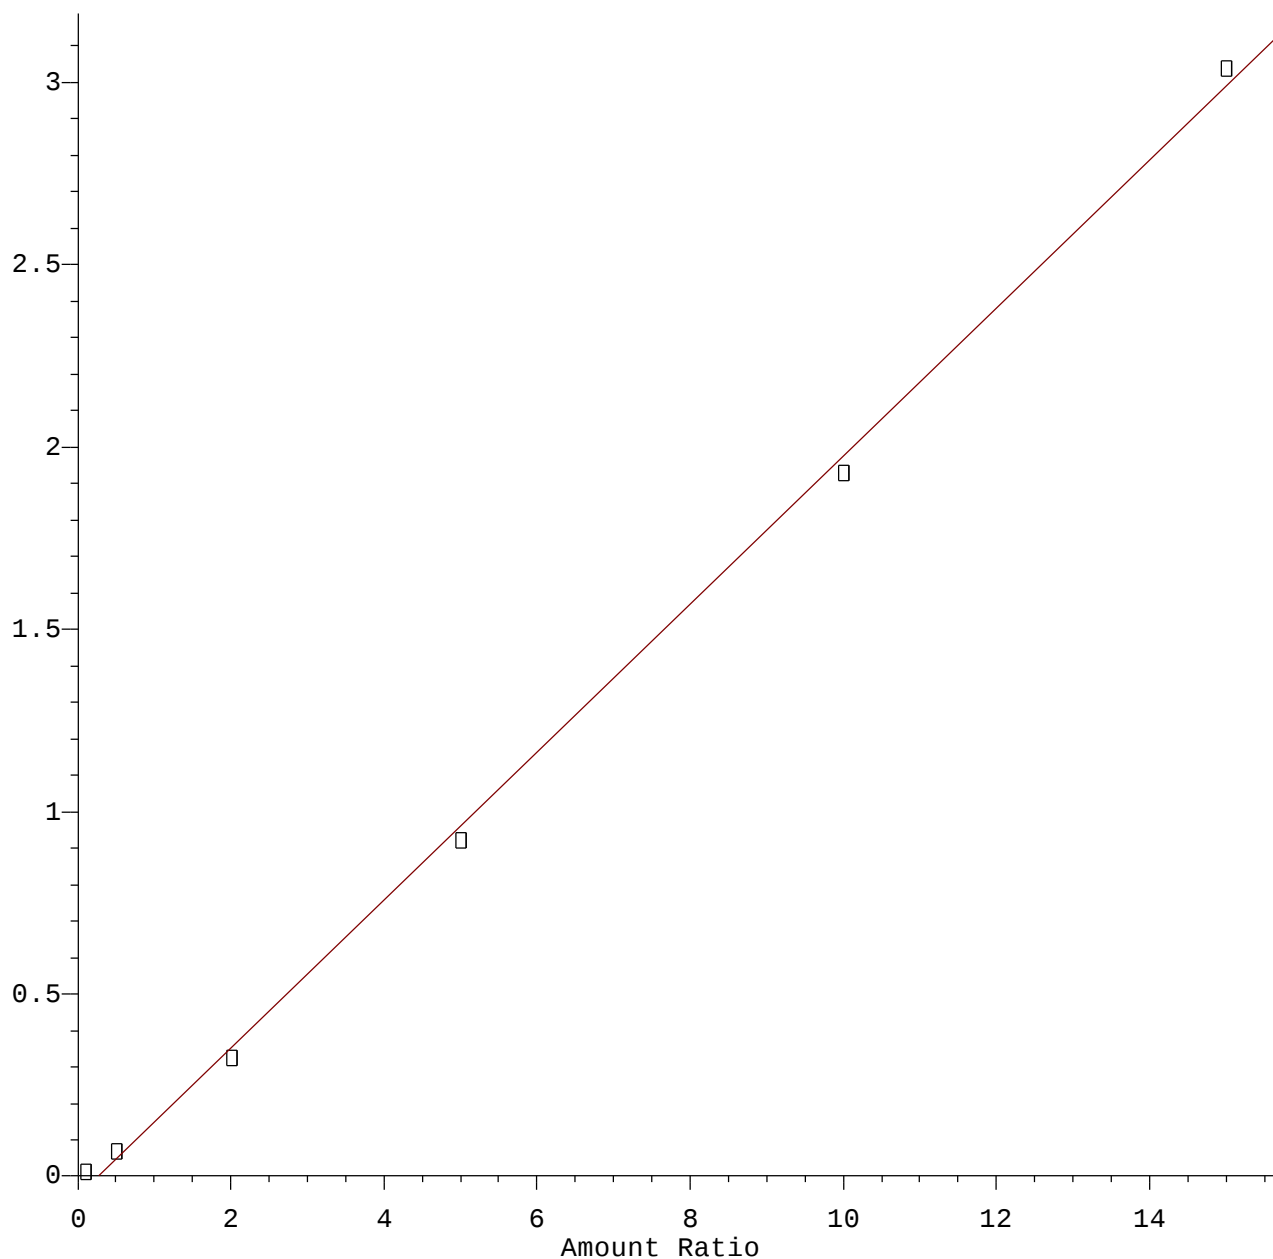


Resp Ratio = $2.03 \times 10^{-1} \times \text{Amt} - 5.52 \times 10^{-2}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019

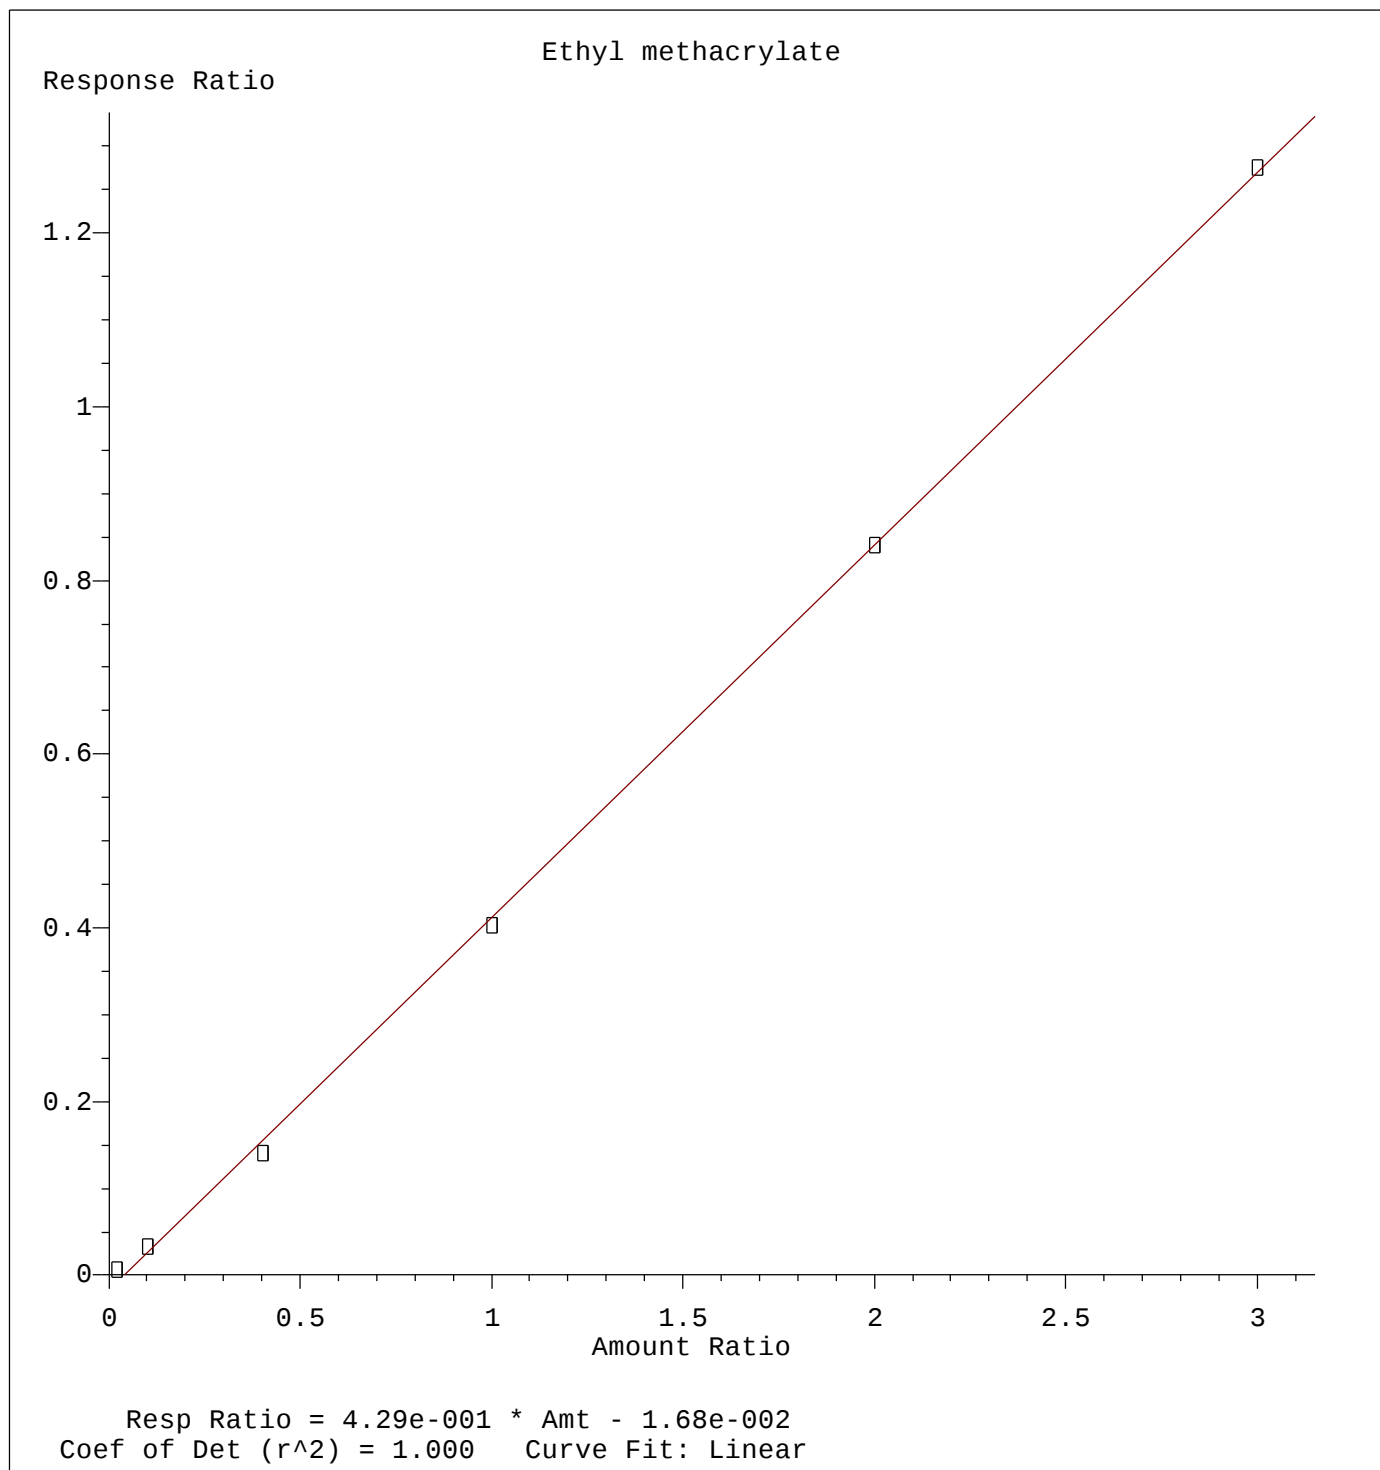

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019

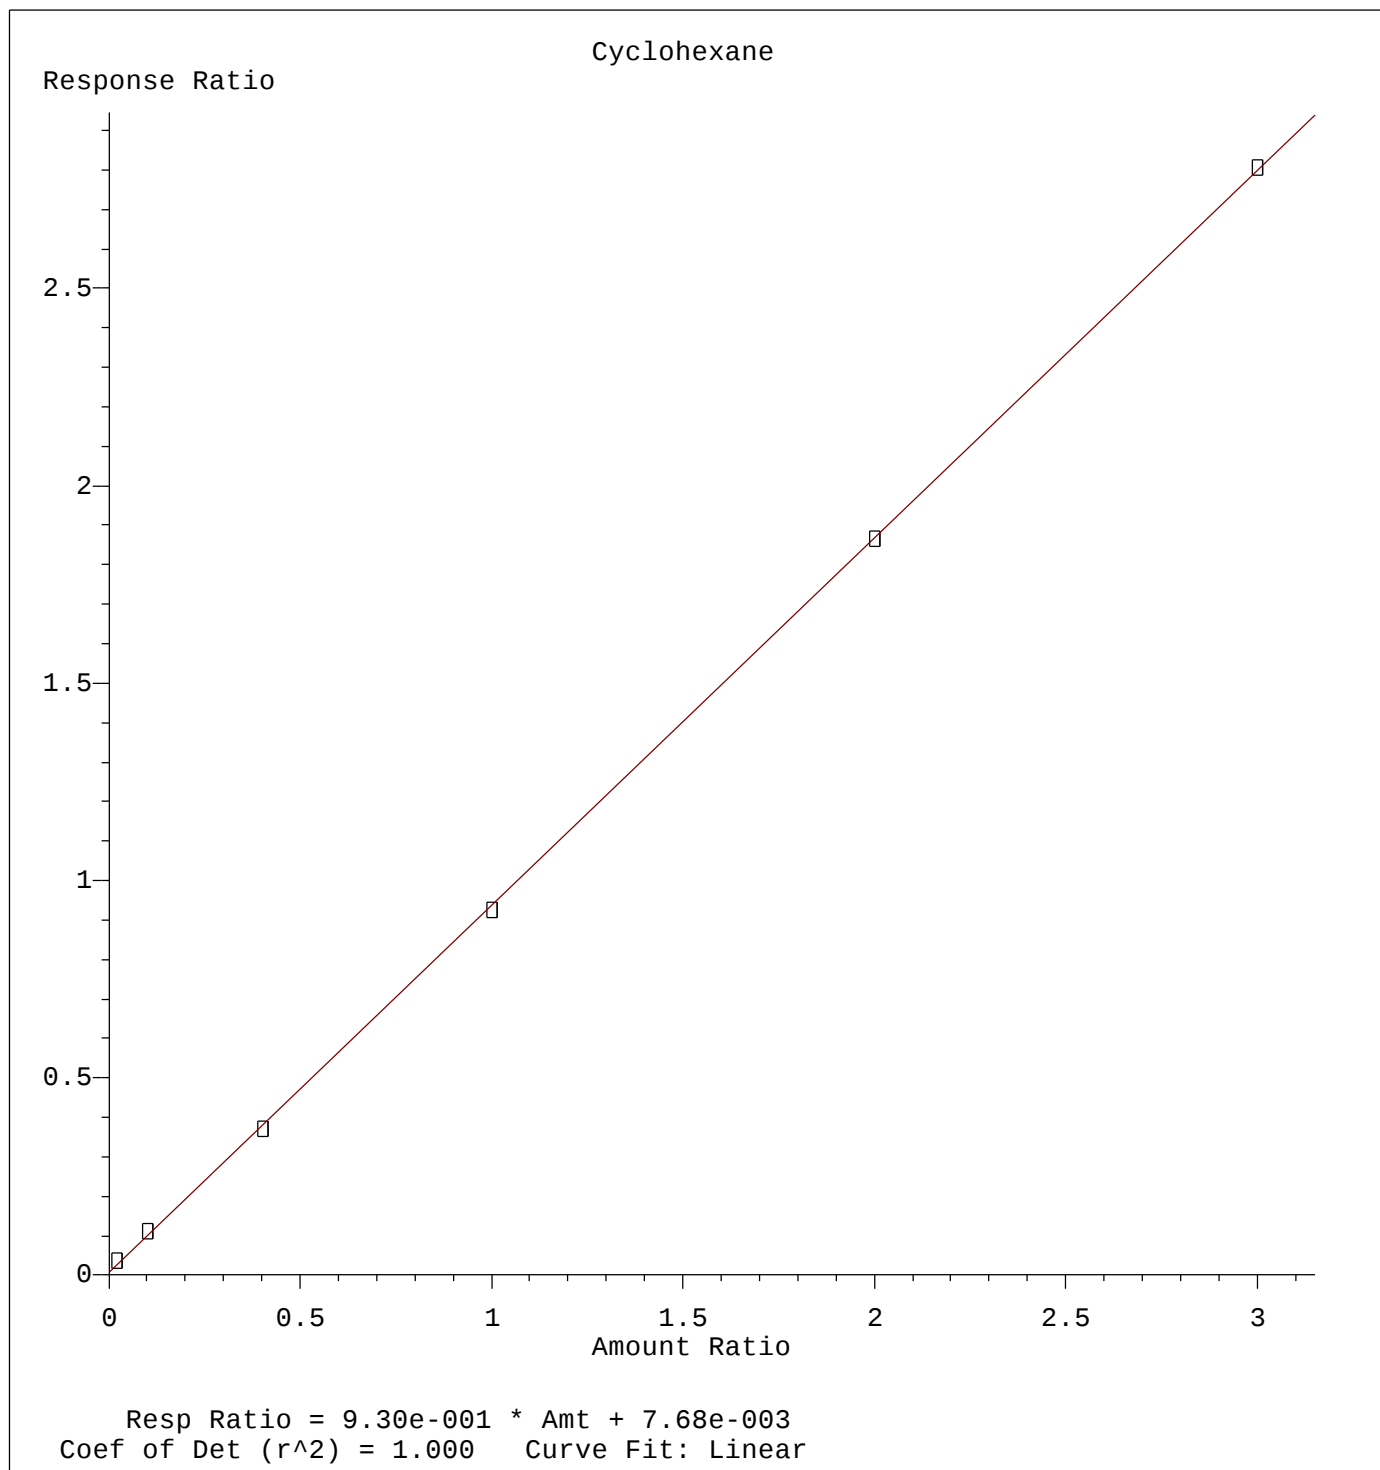

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Calibration Table Last Updated: Thu Feb 28 04:05:45 2019