

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022521\
 Data File : VN066019.D
 Acq On : 25 Feb 2021 11:11
 Operator : JC/MD
 Sample : VN0225WBL01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0225WBL01

Quant Time: Feb 26 01:16:42 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.627	168	121090	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	199306	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	181198	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	74944	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	80798	47.72	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	95.44%
35) Dibromofluoromethane	7.553	113	59704	48.40	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	96.80%
50) Toluene-d8	10.058	98	241036	47.60	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.20%
62) 4-Bromofluorobenzene	12.373	95	87386	45.97	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	91.94%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022521\
Data File : VN066019.D
Acq On : 25 Feb 2021 11:11
Operator : JC/MD
Sample : VN0225WBL01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0225WBL01

Quant Time: Feb 26 01:16:42 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




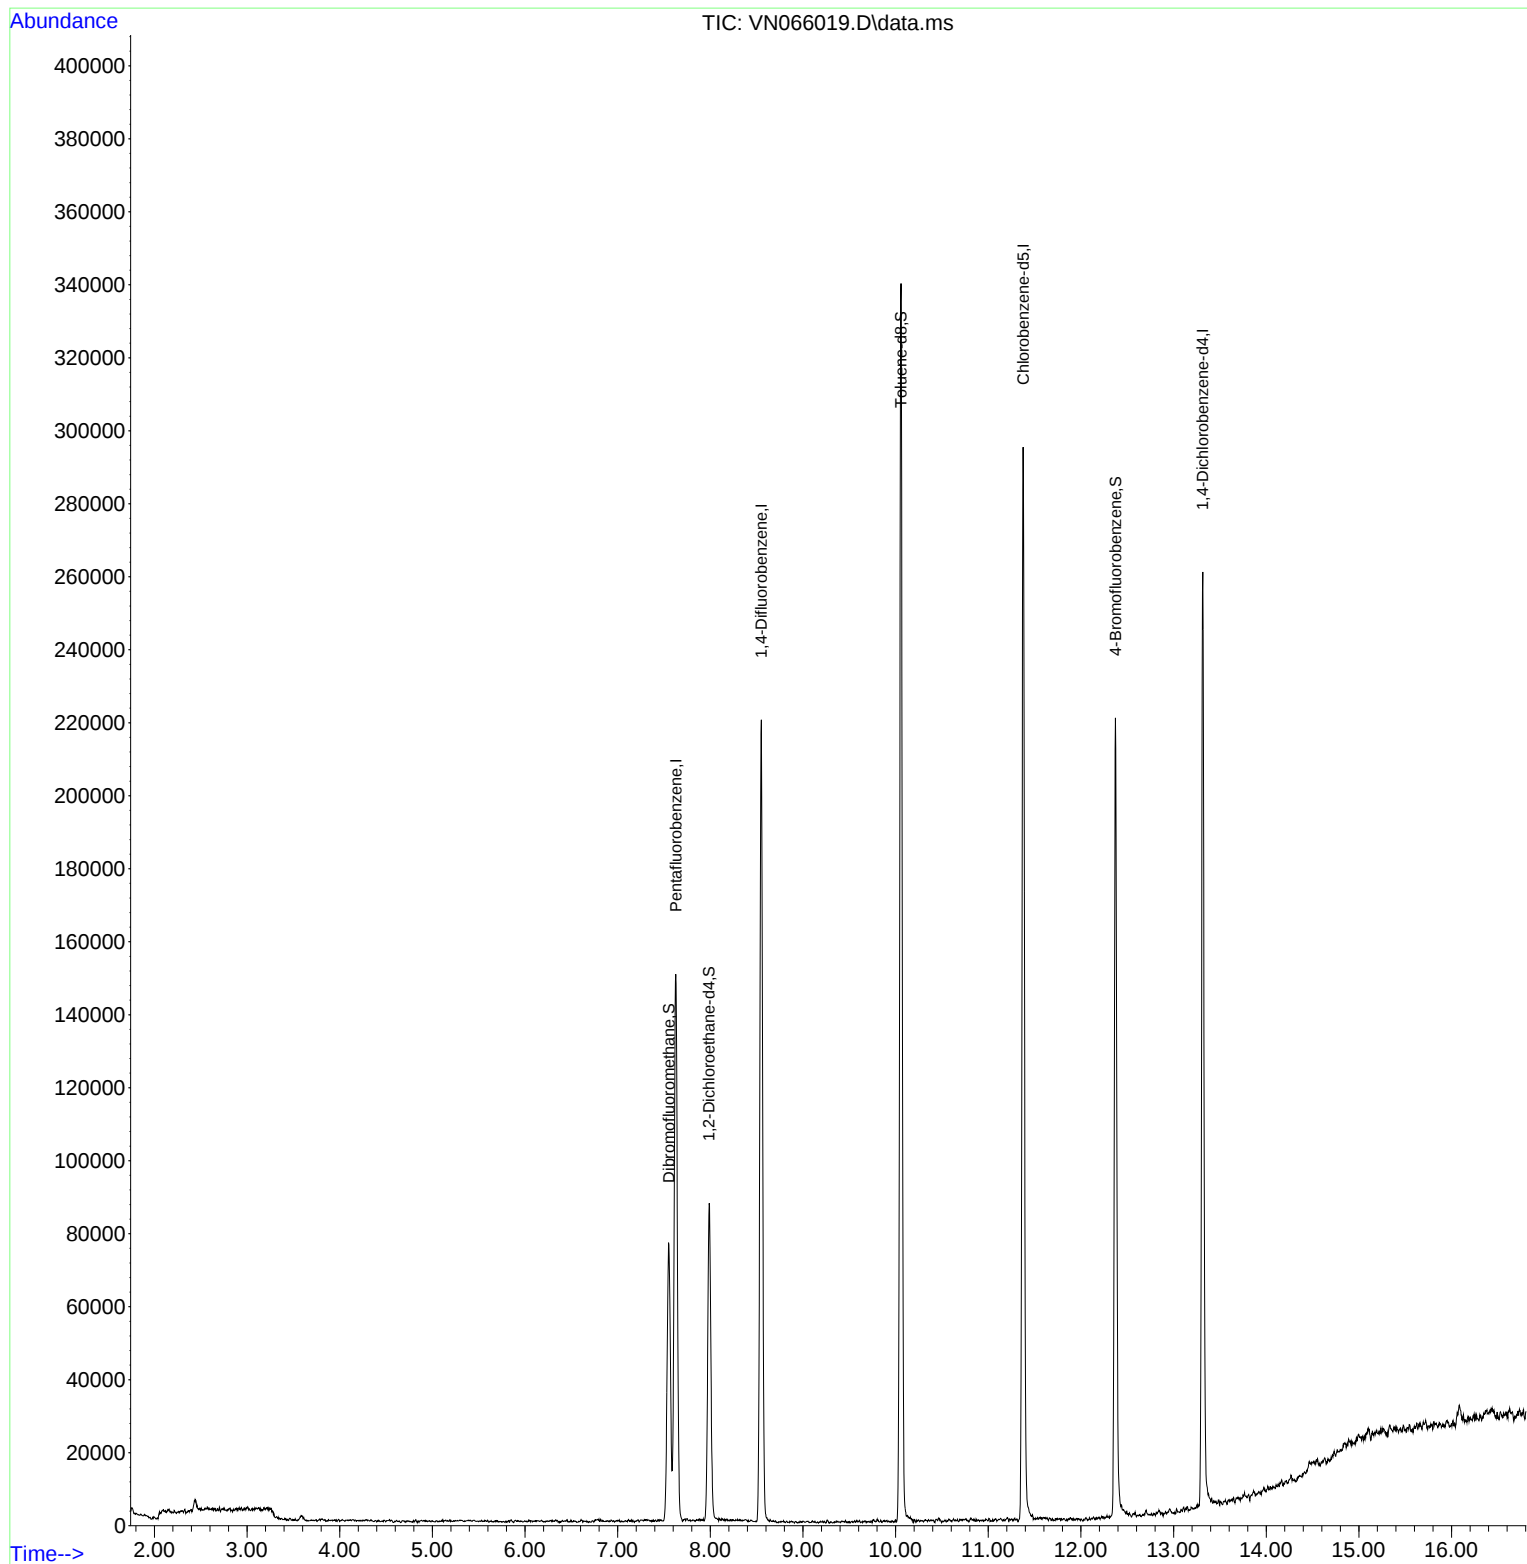


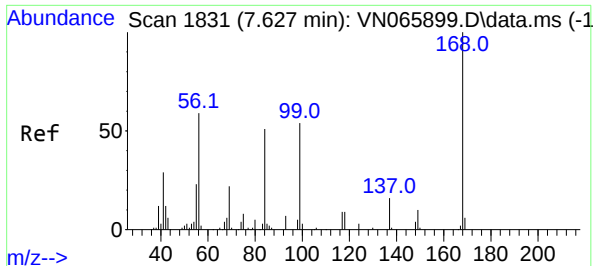

#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11




Instrument :
MSVOA_N
ClientSampleId :
VN0225WBL01


Tgt Ion:168 Resp: 121090
Ion Ratio Lower Upper
168 100
99 59.0 42.6 63.8

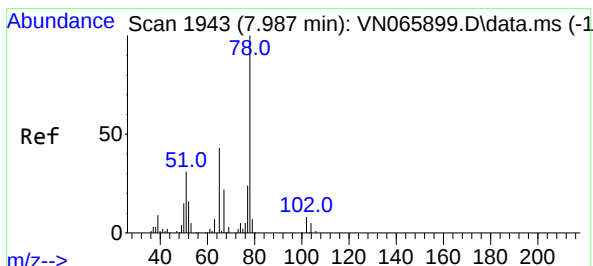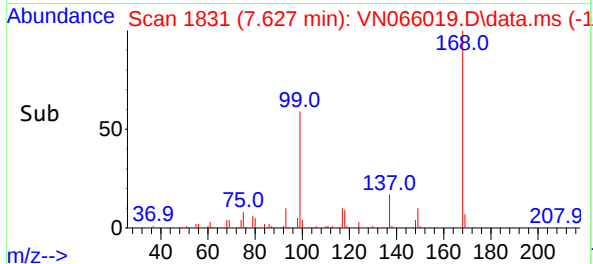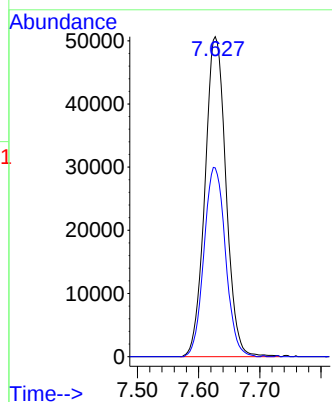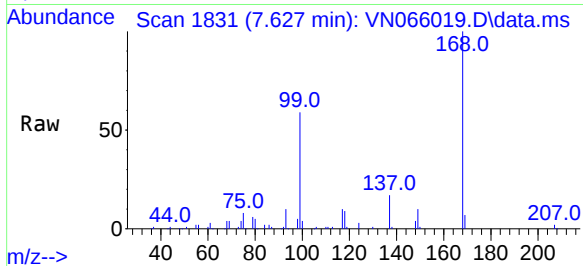

#33
1,2-Dichloroethane-d4
Concen: 47.72 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11

Tgt Ion: 65 Resp: 80798
Ion Ratio Lower Upper
65 100
67 52.1 0.0 107.2


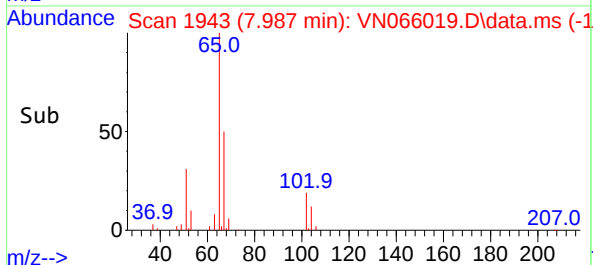
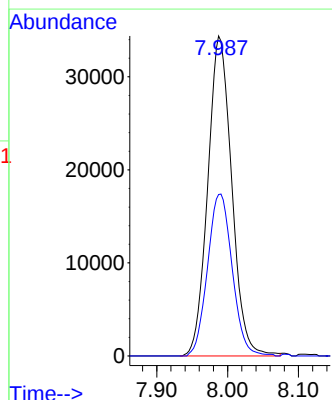
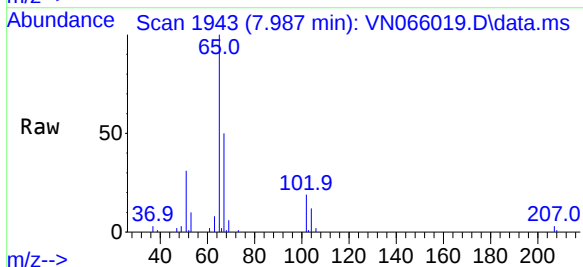


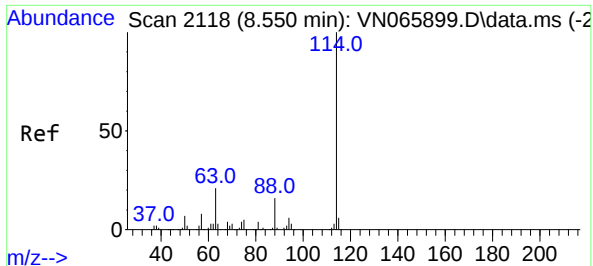

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11




Instrument :
MSVOA_N
ClientSampleId :
VN0225WBL01


Tgt Ion:	114	Resp:	199306
Ion	Ratio	Lower	Upper
114	100		
63	20.0	0.0	38.6
88	16.9	0.0	30.6

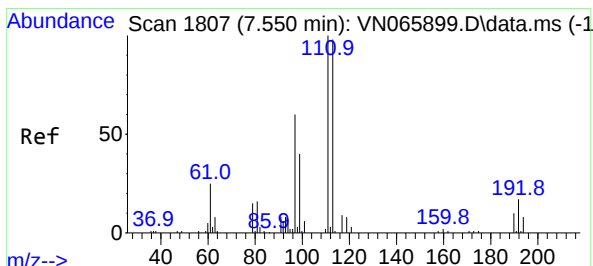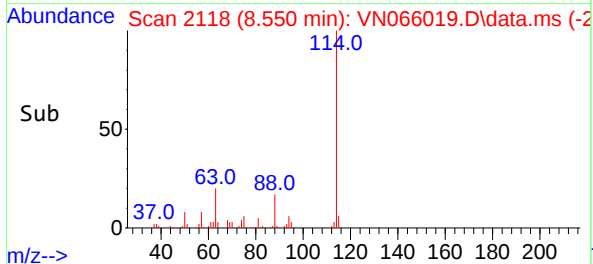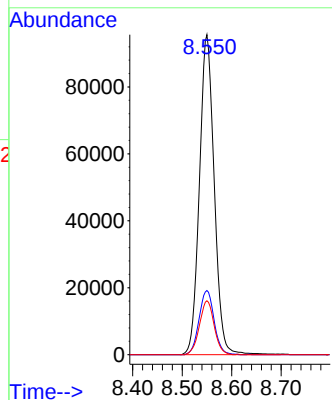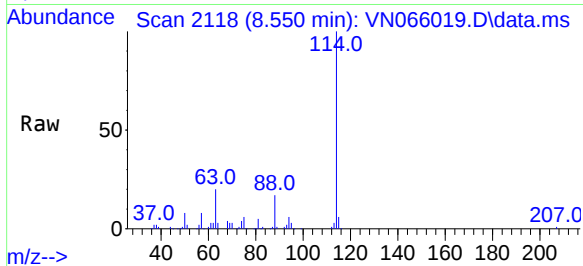

#35
Dibromofluoromethane
Concen: 48.40 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11

Tgt Ion:	113	Resp:	59704
Ion	Ratio	Lower	Upper
113	100		
111	102.4	82.2	123.2
192	18.2	15.4	23.0


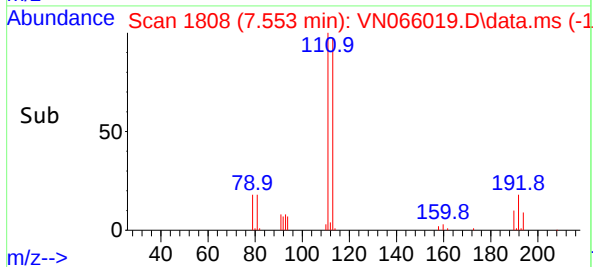
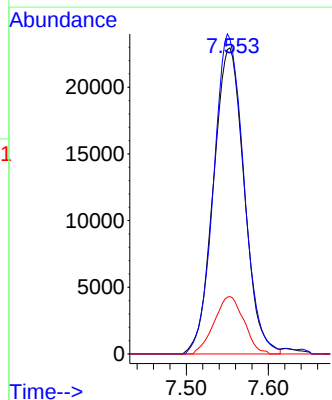
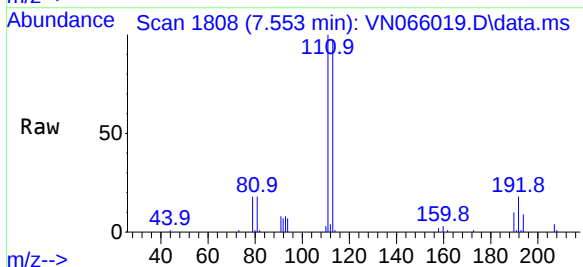


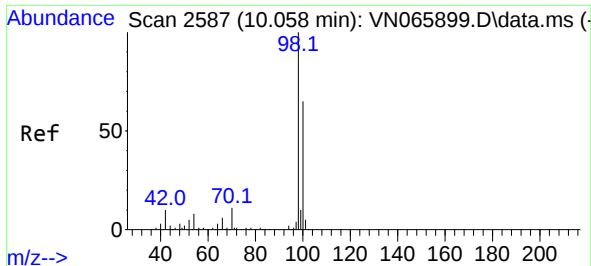

#50
Toluene-d8
Concen: 47.60 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11




Instrument :
MSVOA_N
ClientSampleId :
VN0225WBL01


Tgt Ion: 98 Resp: 241036
Ion Ratio Lower Upper
98 100
100 66.1 50.5 75.7

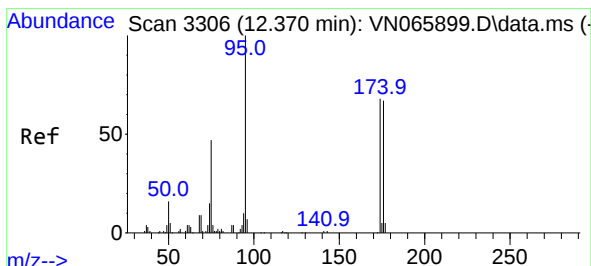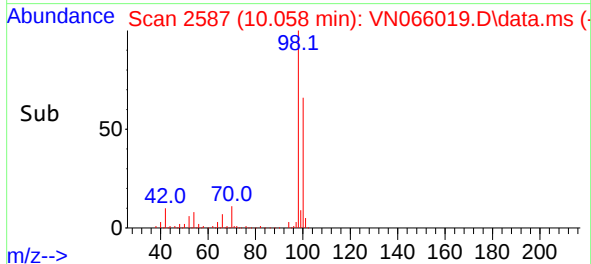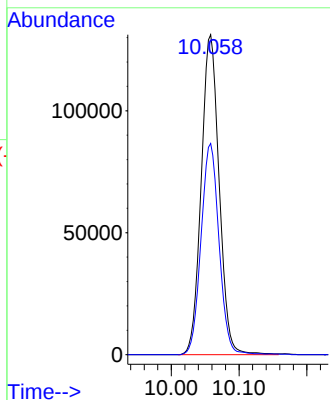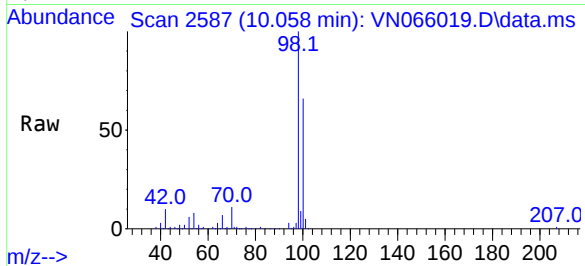

#62
4-Bromofluorobenzene
Concen: 45.97 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11

Tgt Ion: 95 Resp: 87386
Ion Ratio Lower Upper
95 100
174 71.7 0.0 169.0
176 70.1 0.0 162.4


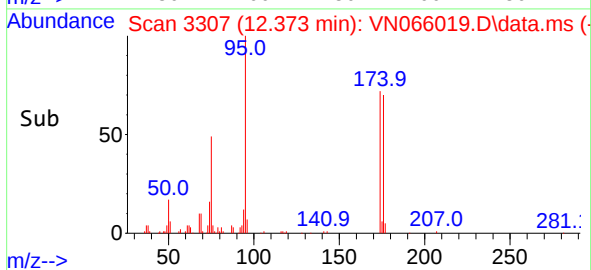
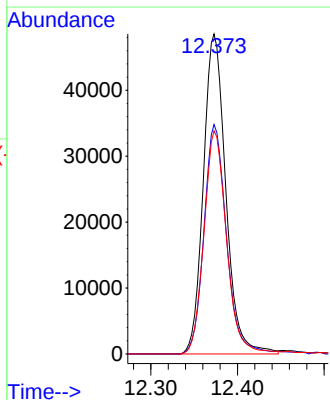
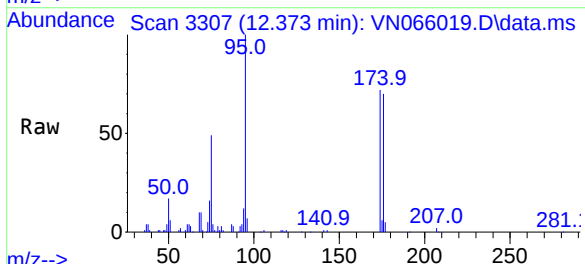


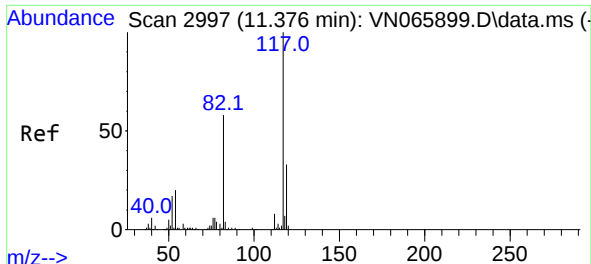

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11

Instrument :
MSVOA_N
ClientSampleId :
VN0225WBL01

Tgt Ion:	117	Resp:	181198
Ion	Ratio	Lower	Upper
117	100		
82	56.1	43.7	65.5
119	31.9	26.1	39.1

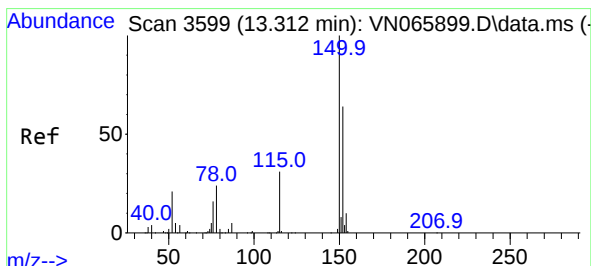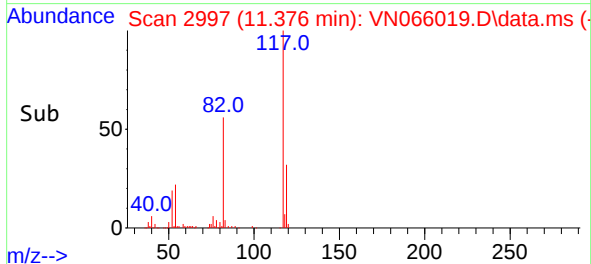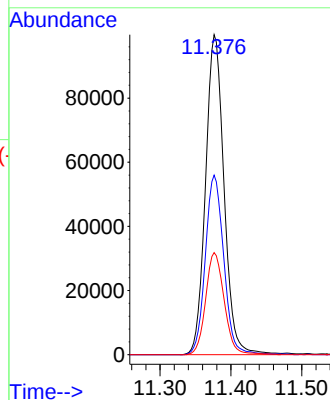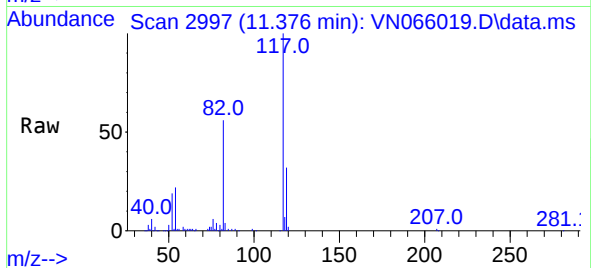

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN066019.D
Acq: 25 Feb 2021 11:11

Tgt Ion:	152	Resp:	74944
Ion	Ratio	Lower	Upper
152	100		
115	63.5	28.5	85.6
150	157.5	0.0	347.6

