

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN022522\  
 Data File : VN071083.D  
 Acq On : 25 Feb 2022 20:34  
 Operator : JC\MD  
 Sample : N1664-32  
 Misc : 5.0mL/MSVOA\_N/WATER  
 ALS Vial : 17 Sample Multiplier: 1

Instrument :  
 MSVOA\_N  
 ClientSampleId :  
 TP-11

Quant Time: Feb 26 03:45:39 2022  
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M  
 Quant Title : SW846 8260  
 QLast Update : Mon Feb 21 07:57:15 2022  
 Response via : Initial Calibration


| Compound                      | R.T.   | QIon  | Response | Conc     | Units      | Dev(Min) |
|-------------------------------|--------|-------|----------|----------|------------|----------|
| -----                         |        |       |          |          |            |          |
| Internal Standards            |        |       |          |          |            |          |
| 1) Pentafluorobenzene         | 8.086  | 168   | 892749   | 50.000   | ug/l       | 0.00     |
| 34) 1,4-Difluorobenzene       | 8.963  | 114   | 1457811  | 50.000   | ug/l       | 0.00     |
| 63) Chlorobenzene-d5          | 11.739 | 117   | 1304873  | 50.000   | ug/l       | 0.00     |
| 72) 1,4-Dichlorobenzene-d4    | 13.668 | 152   | 472147   | 50.000   | ug/l       | 0.00     |
| System Monitoring Compounds   |        |       |          |          |            |          |
| 33) 1,2-Dichloroethane-d4     | 8.434  | 65    | 539131   | 52.866   | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 61 - 141 | Recovery | = 105.740% |          |
| 35) Dibromofluoromethane      | 8.022  | 113   | 418631   | 48.279   | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 69 - 133 | Recovery | = 96.560%  |          |
| 50) Toluene-d8                | 10.439 | 98    | 1779182  | 51.093   | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 65 - 126 | Recovery | = 102.180% |          |
| 62) 4-Bromofluorobenzene      | 12.727 | 95    | 615229   | 49.428   | ug/l       | 0.00     |
| Spiked Amount                 | 50.000 | Range | 58 - 135 | Recovery | = 98.860%  |          |
| Target Compounds              |        |       |          |          |            |          |
|                               |        |       |          |          | Qvalue     |          |
| 3) Chloromethane              | 2.299  | 50    | 2695     | 0.231    | ug/l       | 97       |
| 13) Acrolein                  | 4.034  | 56    | 410      | 0.247    | ug/l #     | 82       |
| 16) Acetone                   | 4.293  | 43    | 50626    | 9.014    | ug/l       | 98       |
| 18) Methyl Acetate            | 4.851  | 43    | 34390    | 2.221    | ug/l       | 97       |
| 20) Methylene Chloride        | 5.098  | 84    | 111293   | 10.904   | ug/l       | 90       |
| 25) 2-Butanone                | 7.345  | 43    | 10682    | 1.430    | ug/l #     | 83       |
| 29) Tetrahydrofuran           | 7.704  | 42    | 1679     | 0.347    | ug/l #     | 75       |
| 31) Cyclohexane               | 8.086  | 56    | 18884    | 1.071    | ug/l #     | 1        |
| 36) 1,1-Dichloropropene       | 8.081  | 75    | 68107    | 4.794    | ug/l #     | 49       |
| 37) Ethyl Acetate             | 7.345  | 43    | 10682    | 0.701    | ug/l #     | 68       |
| 38) Carbon Tetrachloride      | 8.081  | 117   | 86878    | 6.207    | ug/l #     | 17       |
| 43) Isopropyl Acetate         | 8.563  | 43    | 230805   | 9.611    | ug/l #     | 72       |
| 45) 1,2-Dichloropropane       | 9.616  | 63    | 6807     | 0.632    | ug/l #     | 44       |
| 48) Methyl methacrylate       | 9.539  | 41    | 25139    | 2.212    | ug/l #     | 8        |
| 49) 1,4-Dioxane               | 9.563  | 88    | 58       | 0.287    | ug/l #     | 1        |
| 51) 4-Methyl-2-Pentanone      | 10.322 | 43    | 10666    | 0.730    | ug/l #     | 49       |
| 54) cis-1,3-Dichloropropene   | 10.239 | 75    | 141810   | 8.295    | ug/l #     | 59       |
| 57) 1,3-Dichloropropane       | 11.086 | 76    | 80101    | 4.480    | ug/l #     | 43       |
| 59) 2-Hexanone                | 11.086 | 43    | 1236990  | 123.098  | ug/l #     | 49       |
| 74) N-amyl acetate            | 12.345 | 43    | 2607     | 0.215    | ug/l #     | 43       |
| 76) 1,2,3-Trichloropropane    | 12.727 | 75    | 309266   | 27.820   | ug/l #     | 1        |
| 81) trans-1,4-Dichloro-2-b... | 12.727 | 75    | 309266   | 90.149   | ug/l #     | 5        |
| 93) 1,2,4-Trichlorobenzene    | 15.262 | 180   | 285      | 2.030    | ug/l #     | 81       |
| 95) Naphthalene               | 15.509 | 128   | 1416     | 5.050    | ug/l #     | 74       |
| 96) 1,2,3-Trichlorobenzene    | 15.698 | 180   | 132      | 2.532    | ug/l #     | 1        |
| -----                         |        |       |          |          |            |          |


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN022522\  
Data File : VN071083.D  
Acq On : 25 Feb 2022 20:34  
Operator : JC\MD  
Sample : N1664-32  
Misc : 5.0mL/MSVOA\_N/WATER  
ALS Vial : 17 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11

Quant Time: Feb 26 03:45:39 2022  
Quant Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021522W.M  
Quant Title : SW846 8260  
QLast Update : Mon Feb 21 07:57:15 2022  
Response via : Initial Calibration




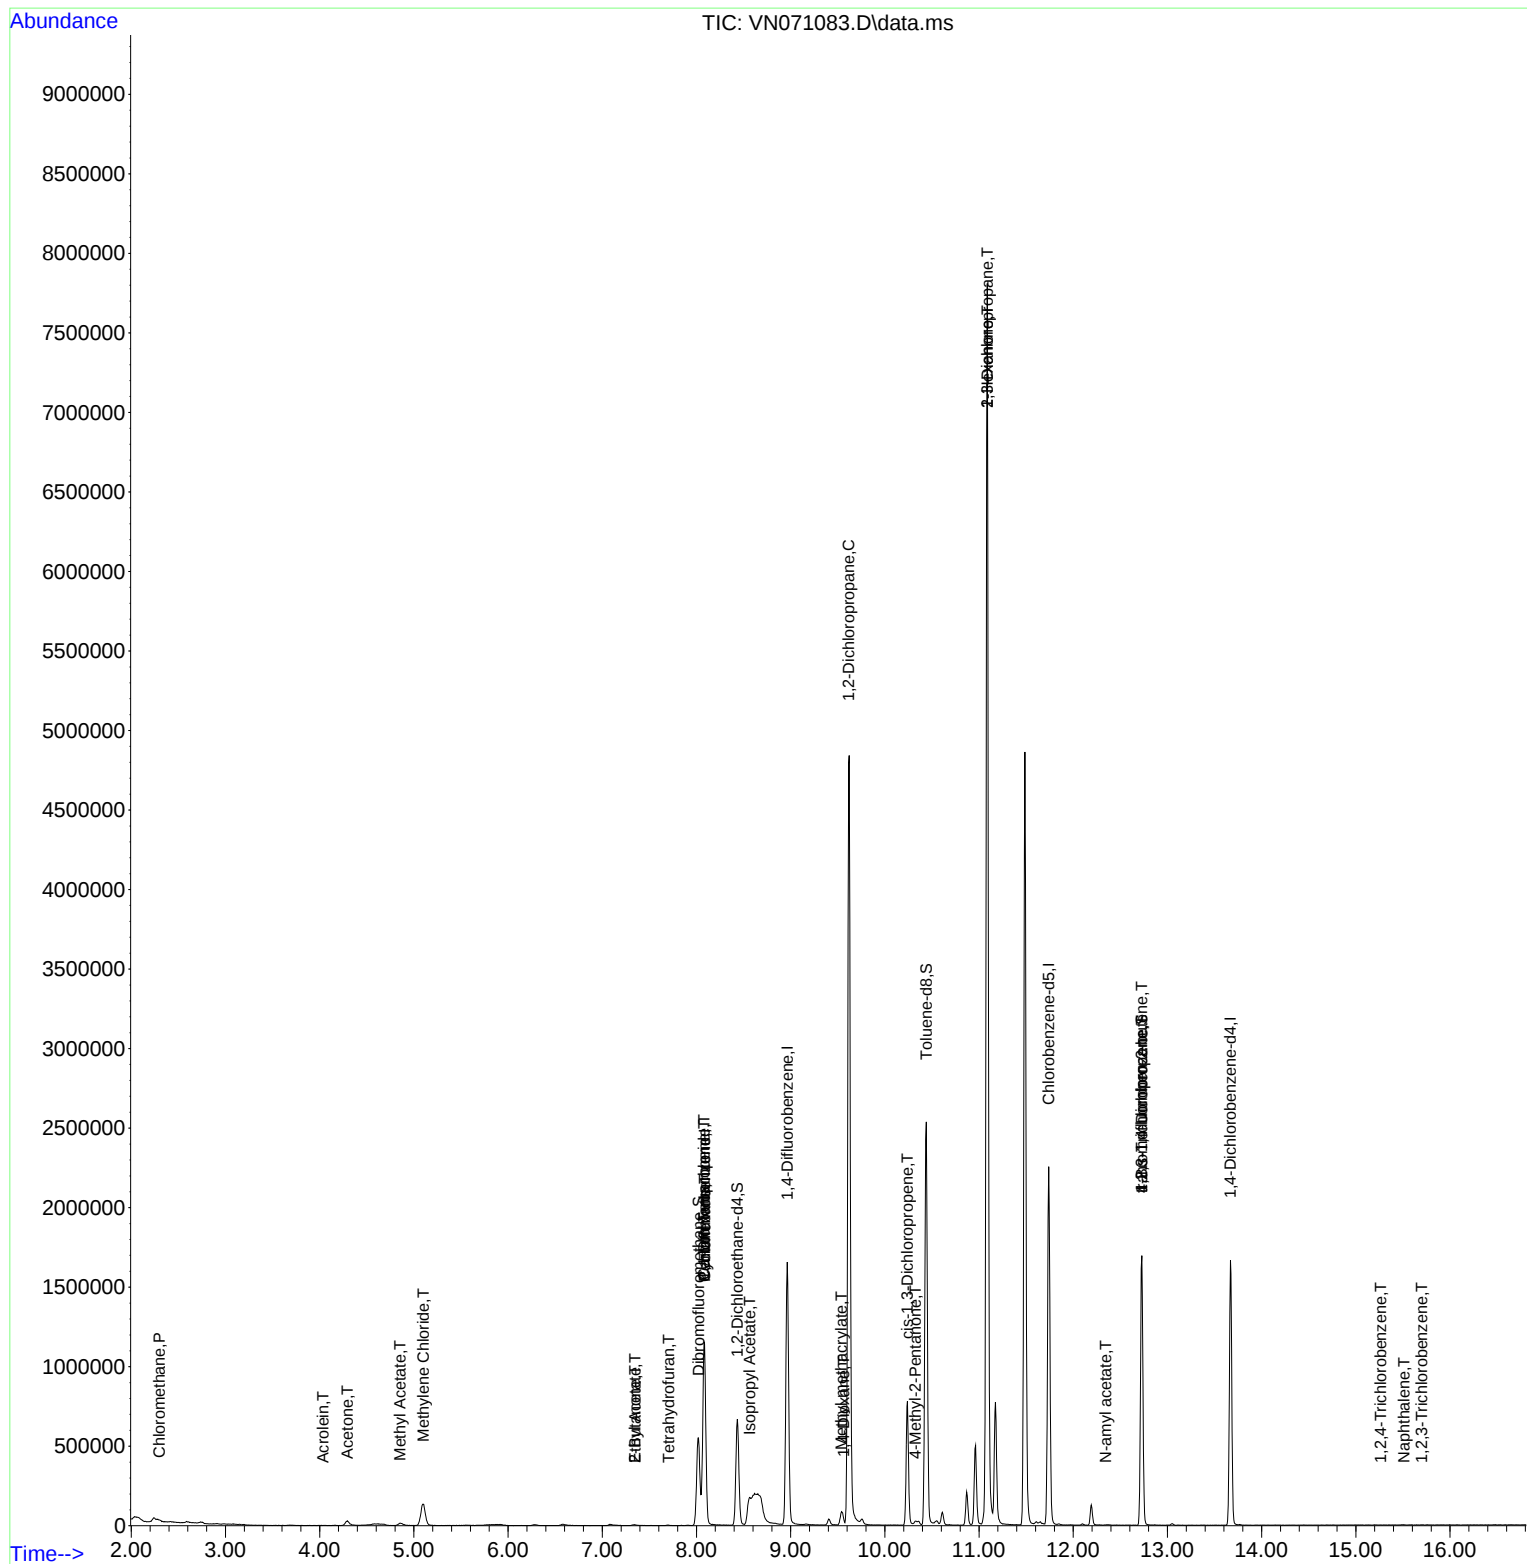




#1  
Pentafluorobenzene  
Concen: 50.000 ug/l  
RT: 8.086 min Scan# 10  
Delta R.T. 0.005 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion:168 Resp: 892749  
Ion Ratio Lower Upper  
168 100  
99 56.7 41.3 61.9

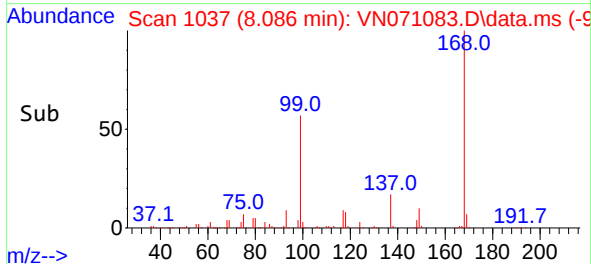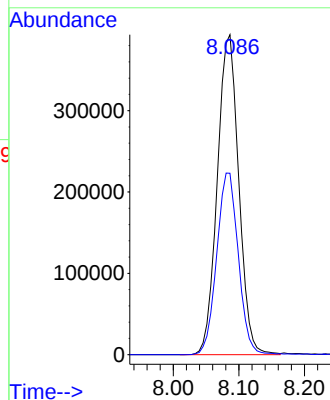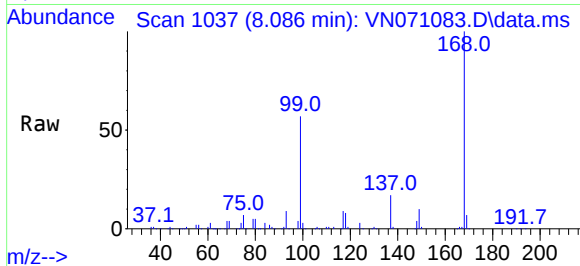

#3  
Chloromethane  
Concen: 0.231 ug/l  
RT: 2.299 min Scan# 53  
Delta R.T. 0.000 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 50 Resp: 2695  
Ion Ratio Lower Upper  
50 100  
52 29.9 25.4 38.0


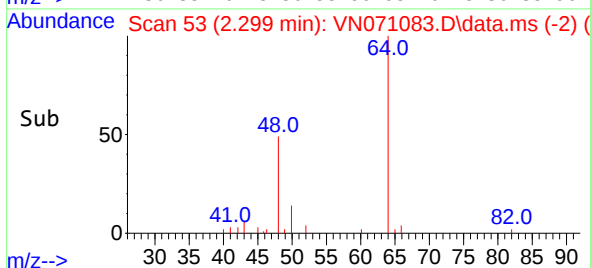
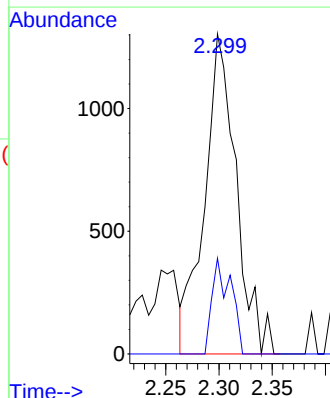
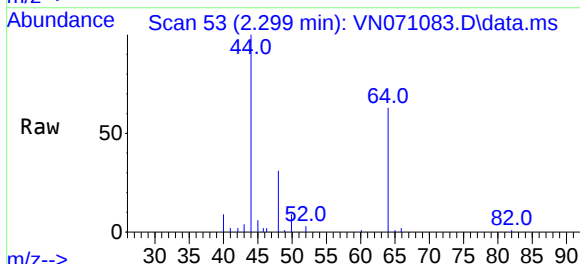




#13  
Acrolein  
Concen: 0.247 ug/l  
RT: 4.034 min Scan# 348  
Delta R.T. -0.000 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 56 Resp: 410  
Ion Ratio Lower Upper  
56 100  
55 55.6 56.6 85.0#

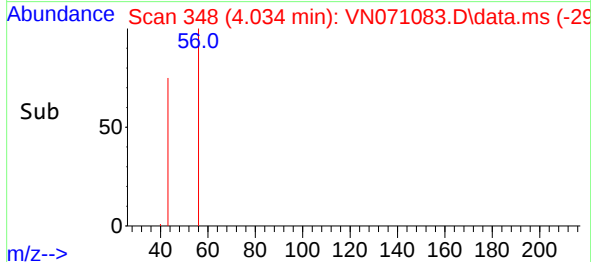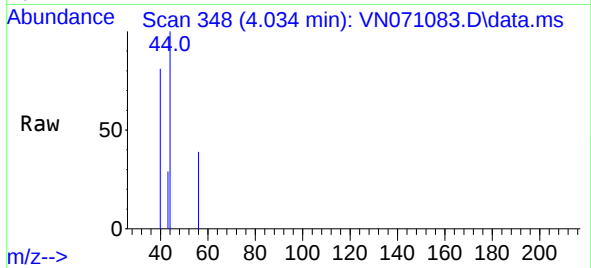

#16  
Acetone  
Concen: 9.014 ug/l  
RT: 4.293 min Scan# 392  
Delta R.T. 0.012 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 43 Resp: 50626  
Ion Ratio Lower Upper  
43 100  
58 30.2 23.1 34.7


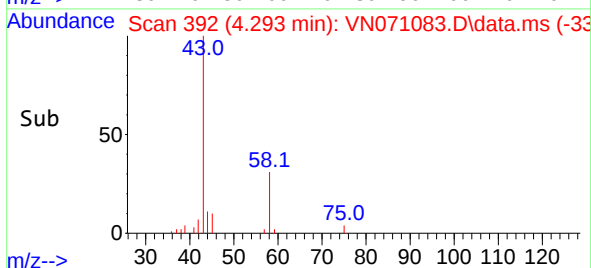
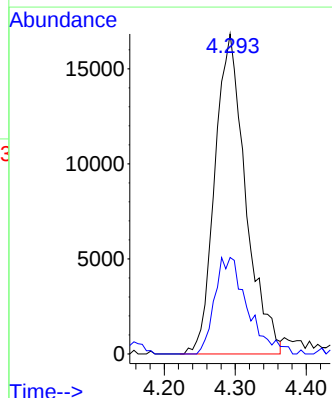
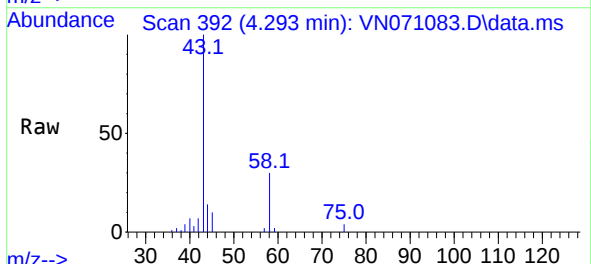




#18  
Methyl Acetate  
Concen: 2.221 ug/l  
RT: 4.851 min Scan# 487  
Delta R.T. 0.006 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 43 Resp: 34390  
Ion Ratio Lower Upper  
43 100  
74 22.7 19.4 29.2

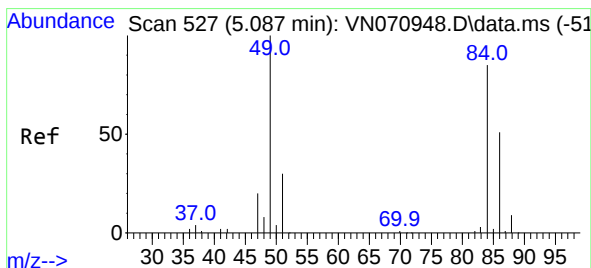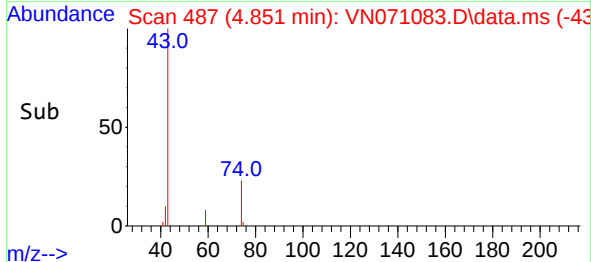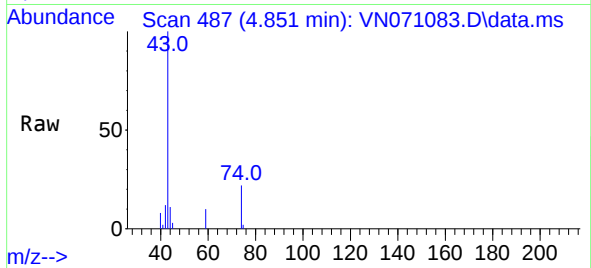

#20  
Methylene Chloride  
Concen: 10.904 ug/l  
RT: 5.098 min Scan# 529  
Delta R.T. 0.012 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 84 Resp: 111293  
Ion Ratio Lower Upper  
84 100  
49 134.9 93.5 140.3  
51 39.4 29.4 44.2  
86 67.3 53.0 79.4


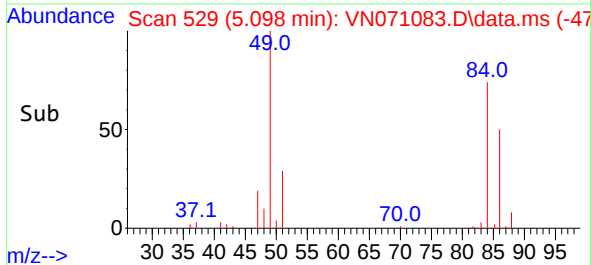

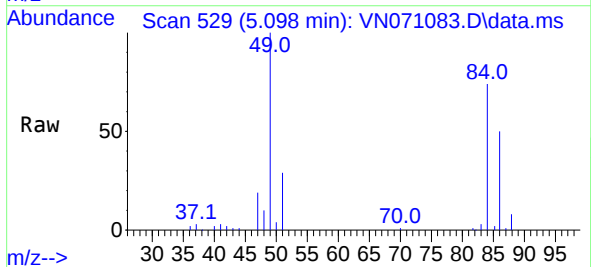




#25  
2-Butanone  
Concen: 1.430 ug/l  
RT: 7.345 min Scan# 911  
Delta R.T. 0.018 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 43 Resp: 10682  
Ion Ratio Lower Upper  
43 100  
72 18.3 21.7 32.5#

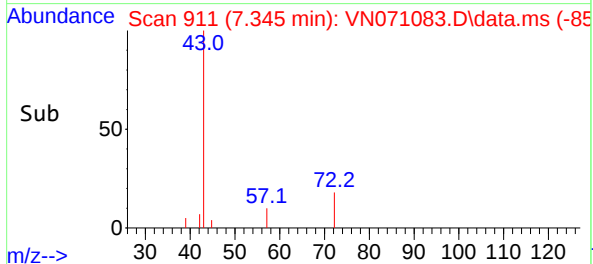

#29  
Tetrahydrofuran  
Concen: 0.347 ug/l  
RT: 7.704 min Scan# 972  
Delta R.T. 0.024 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 42 Resp: 1679  
Ion Ratio Lower Upper  
42 100  
72 30.3 36.3 54.5#  
71 26.3 34.7 52.1#

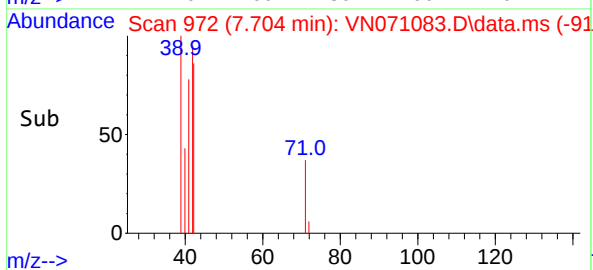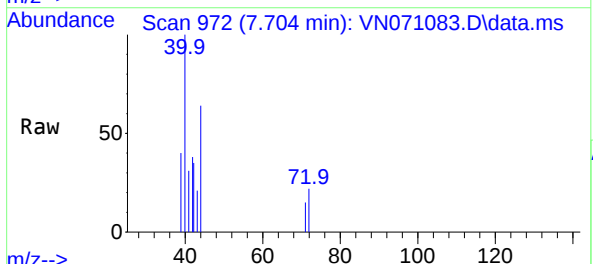



#31

Cyclohexane

Concen: 1.071 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. 0.000 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34

Instrument :

MSVOA\_N

ClientSampleId :

TP-11





Tgt Ion: 56 Resp: 18884

Ion Ratio Lower Upper

56 100

69 169.6 27.1 40.7#

84 157.2 73.4 110.0#

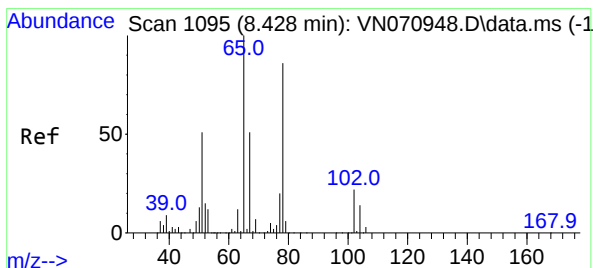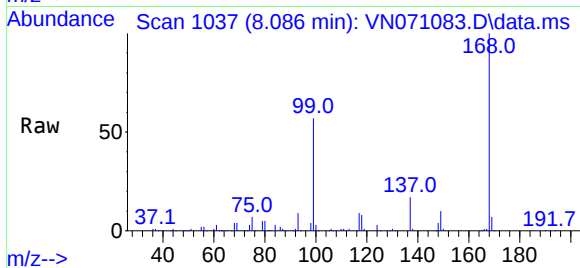

#33

1,2-Dichloroethane-d4

Concen: 52.866 ug/l

RT: 8.434 min Scan# 1096

Delta R.T. 0.006 min

Lab File: VN071083.D




Acq: 25 Feb 2022 20:34


Tgt Ion: 65 Resp: 539131

Ion Ratio Lower Upper

65 100

67 53.3 0.0 103.0

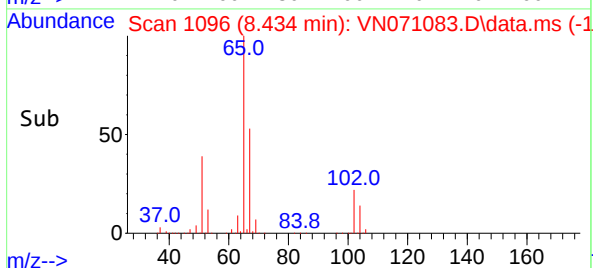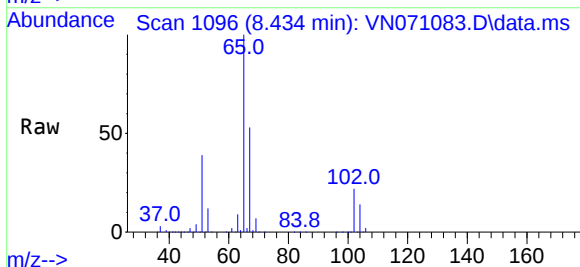



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 8.963 min Scan# 1186

Delta R.T. 0.000 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34

Instrument :

MSVOA\_N

ClientSampleId :

TP-11





Tgt Ion:114 Resp: 1457811

Ion Ratio Lower Upper

114 100

63 21.8 0.0 37.8

88 15.3 0.0 27.4

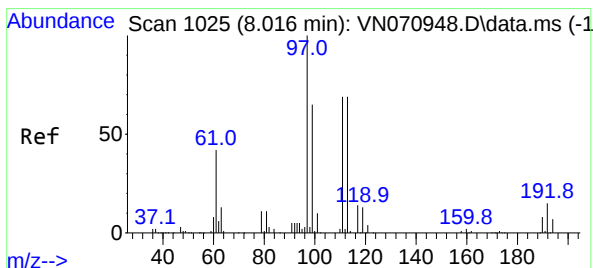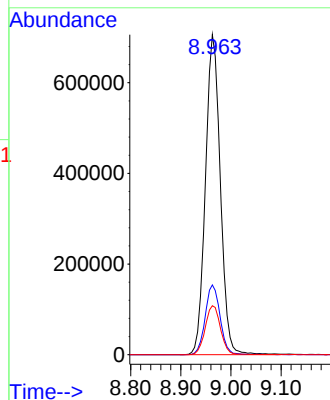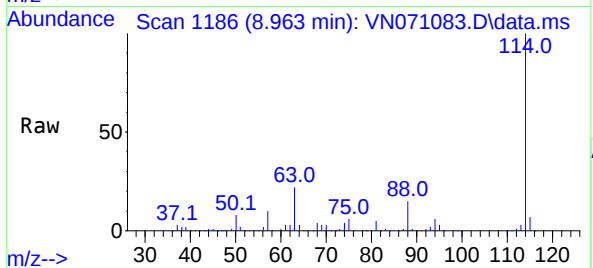

#35

Dibromofluoromethane

Concen: 48.279 ug/l

RT: 8.022 min Scan# 1026

Delta R.T. 0.006 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34




Tgt Ion:113 Resp: 418631


Ion Ratio Lower Upper

113 100

111 102.7 82.2 123.2

192 20.8 16.9 25.3


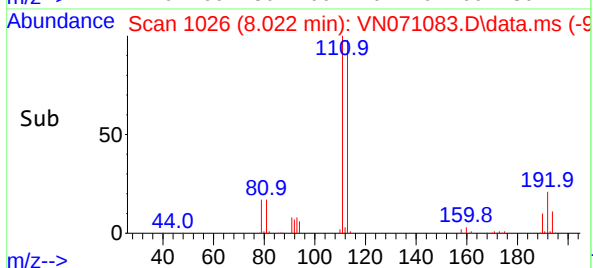
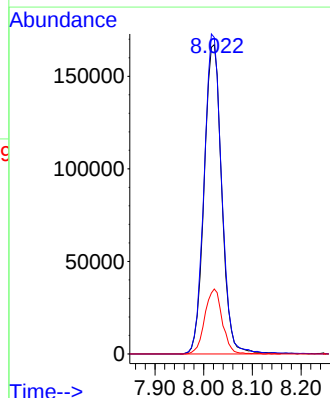
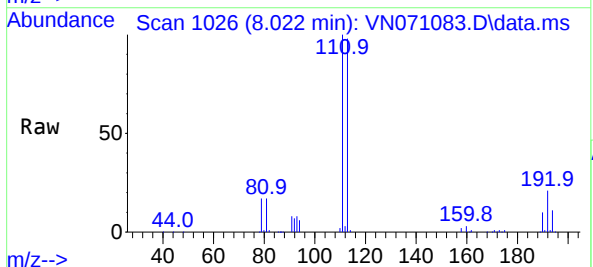




#36  
1,1-Dichloropropene  
Concen: 4.794 ug/l  
RT: 8.081 min Scan# 1059  
Delta R.T. -0.135 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 75 Resp: 68107  
Ion Ratio Lower Upper  
75 100  
110 8.8 18.4 55.2#  
77 0.0 24.4 36.6#

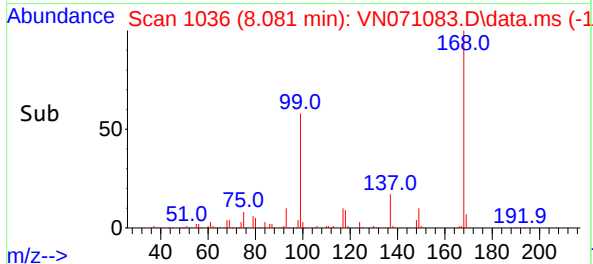

#37  
Ethyl Acetate  
Concen: 0.701 ug/l  
RT: 7.345 min Scan# 911  
Delta R.T. -0.059 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 43 Resp: 10682  
Ion Ratio Lower Upper  
43 100  
61 0.0 11.5 17.3#  
70 0.0 7.9 11.9#


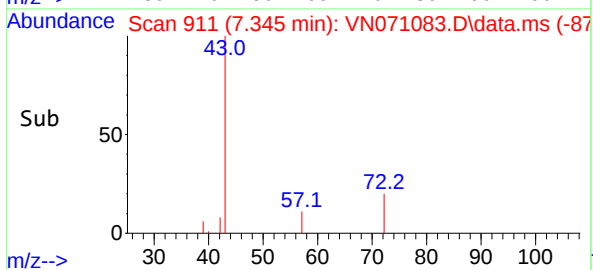

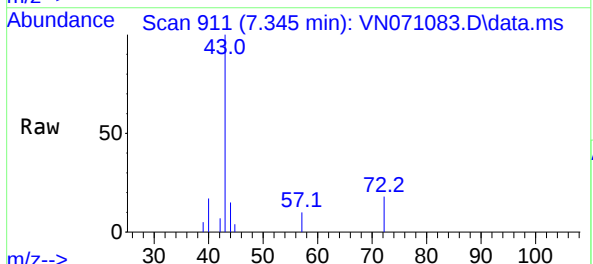




#38  
Carbon Tetrachloride  
Concen: 6.207 ug/l  
RT: 8.081 min Scan# 1107  
Delta R.T. -0.118 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion:117 Resp: 86878  
Ion Ratio Lower Upper  
117 100  
119 5.7 76.1 114.1#  
121 0.0 24.2 36.2#

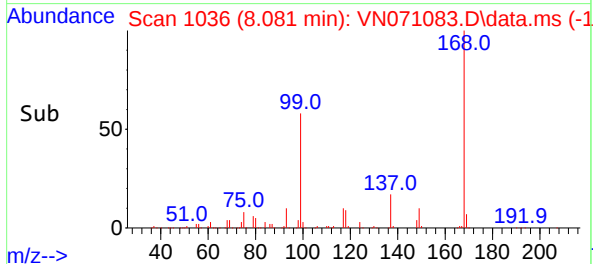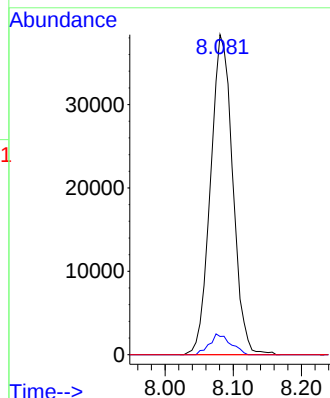

#43  
Isopropyl Acetate  
Concen: 9.611 ug/l  
RT: 8.563 min Scan# 1118  
Delta R.T. 0.006 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 43 Resp: 230805  
Ion Ratio Lower Upper  
43 100  
61 9.3 20.4 30.6#  
87 5.2 11.2 16.8#

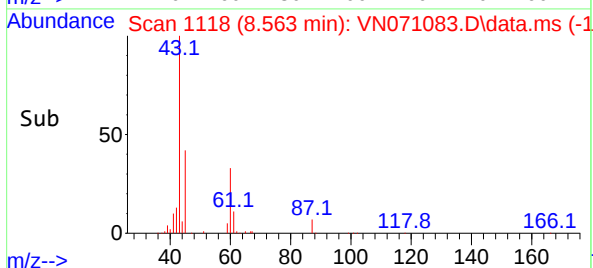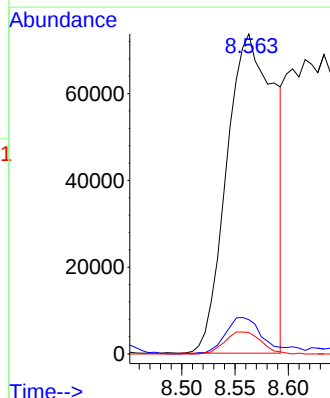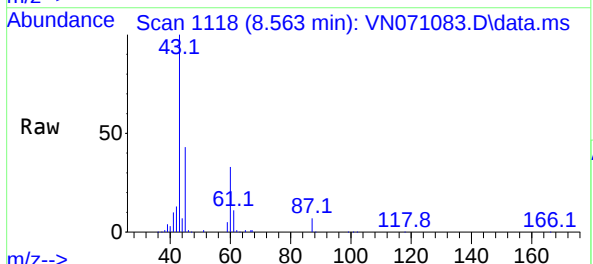



#45

1,2-Dichloropropane

Concen: 0.632 ug/l

RT: 9.616 min Scan# 1297

Delta R.T. 0.135 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34

Instrument :

MSVOA\_N

ClientSampleId :





TP-11

Tgt Ion: 63 Resp: 6807

Ion Ratio Lower Upper

63 100

65 0.0 24.7 37.1#

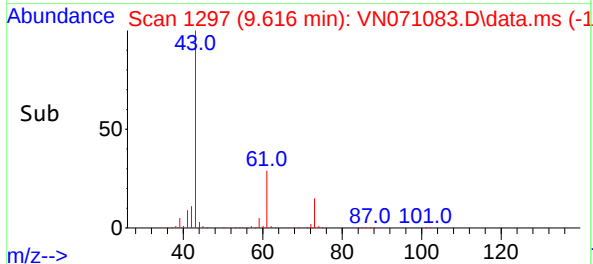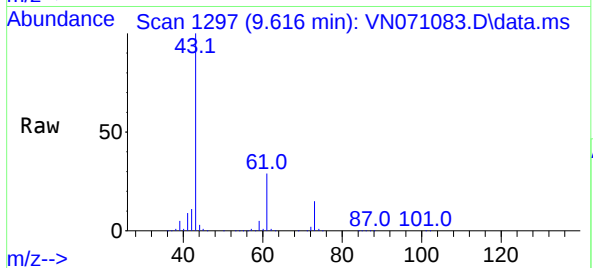

#48

Methyl methacrylate

Concen: 2.212 ug/l

RT: 9.539 min Scan# 1284

Delta R.T. -0.012 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34




Tgt Ion: 41 Resp: 25139


Ion Ratio Lower Upper

41 100

69 0.0 72.4 108.6#

39 0.0 58.4 87.6#


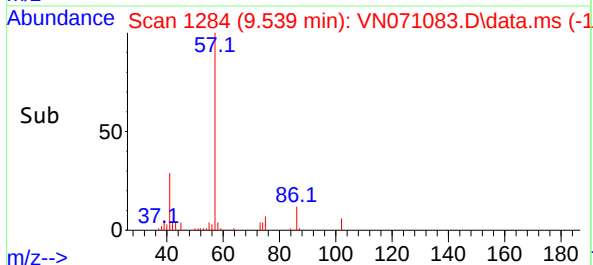
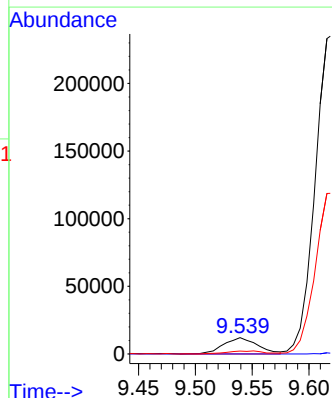
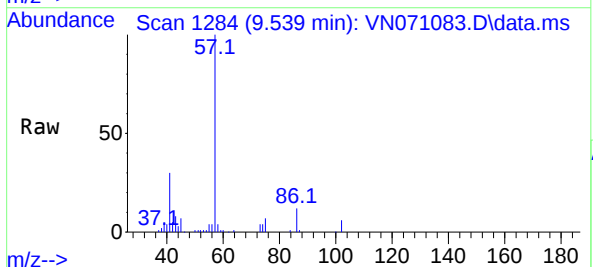




#49  
1,4-Dioxane  
Concen: 0.287 ug/l  
RT: 9.563 min Scan# 11  
Delta R.T. 0.000 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 88 Resp: 58  
Ion Ratio Lower Upper  
88 100  
43 0.0 23.4 35.2#  
58 6334.5 50.6 75.8#

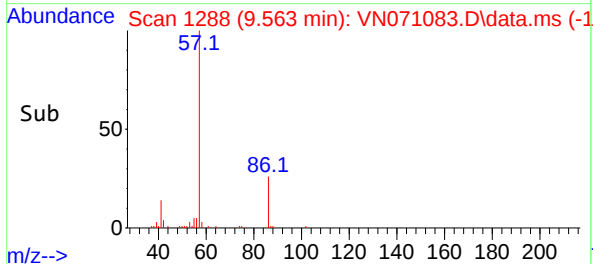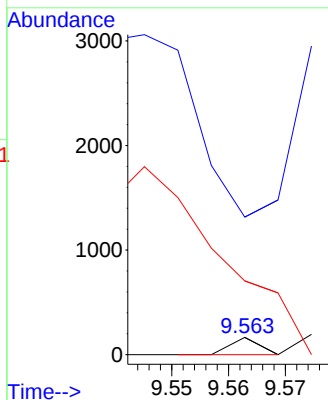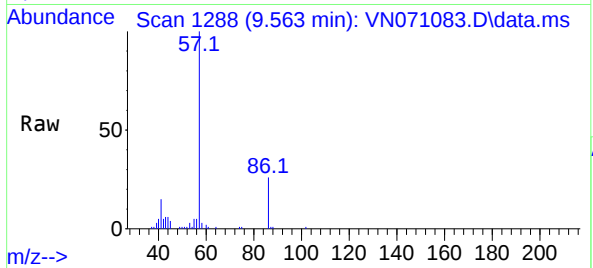

#50  
Toluene-d8  
Concen: 51.093 ug/l  
RT: 10.439 min Scan# 1437  
Delta R.T. 0.006 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 98 Resp: 1779182  
Ion Ratio Lower Upper  
98 100  
100 65.4 50.4 75.6

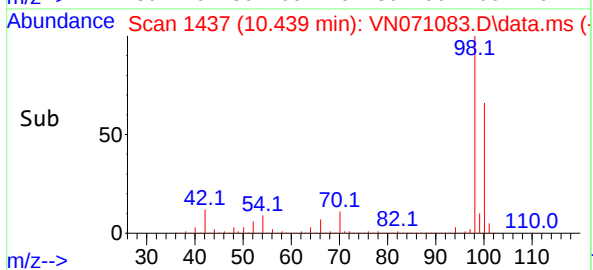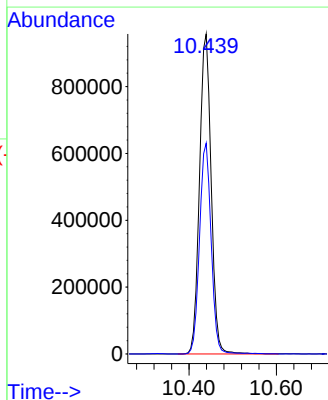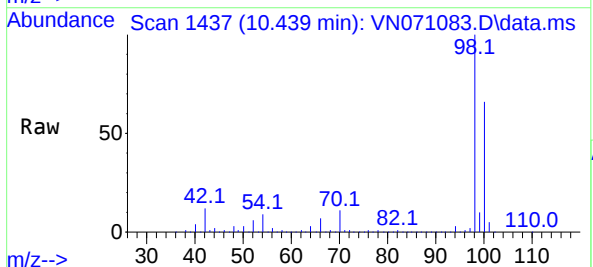

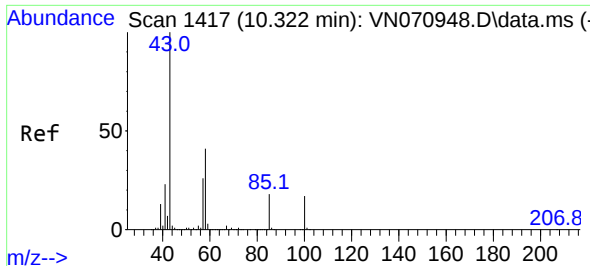

#51

4-Methyl-2-Pentanone

Concen: 0.730 ug/l

RT: 10.322 min Scan# 1417

Delta R.T. 0.000 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34

Instrument :

MSVOA\_N

ClientSampleId :





TP-11

Tgt Ion: 43 Resp: 10666

Ion Ratio Lower Upper

43 100

58 68.6 30.4 45.6#

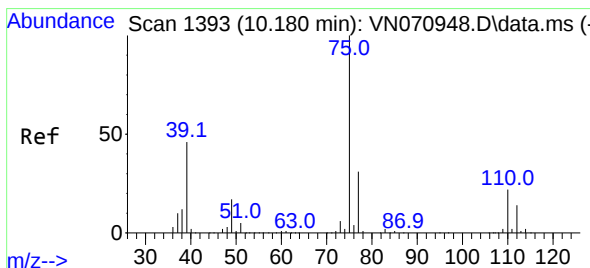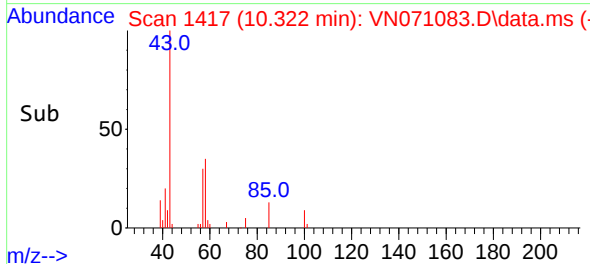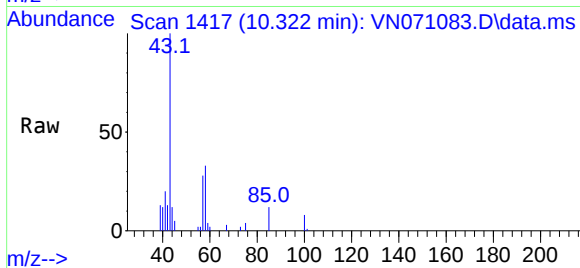

#54

cis-1,3-Dichloropropene

Concen: 8.295 ug/l

RT: 10.239 min Scan# 1403

Delta R.T. 0.059 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34




Tgt Ion: 75 Resp: 141810


Ion Ratio Lower Upper

75 100

77 0.5 26.4 39.6#

39 30.7 42.5 63.7#


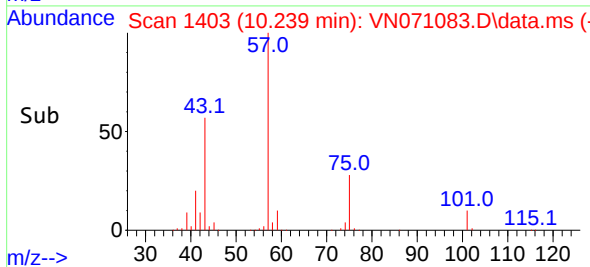

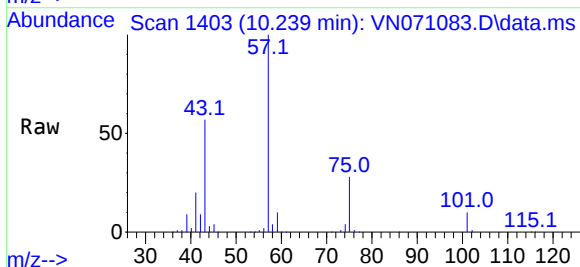


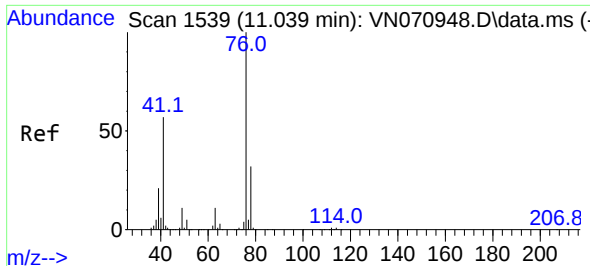

#57  
1,3-Dichloropropane  
Concen: 4.480 ug/l  
RT: 11.086 min Scan# 1547  
Delta R.T. 0.047 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 76 Resp: 80101  
Ion Ratio Lower Upper  
76 100  
78 0.3 25.7 38.5#

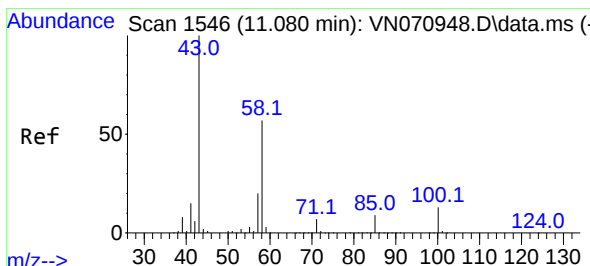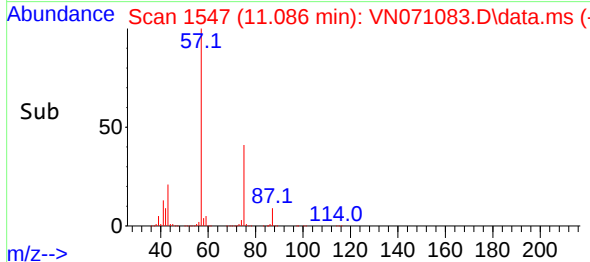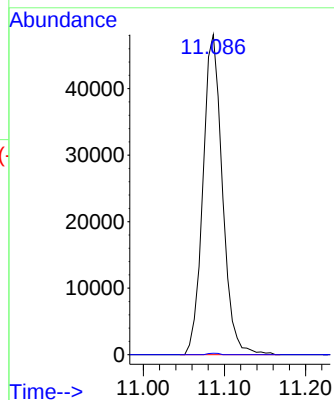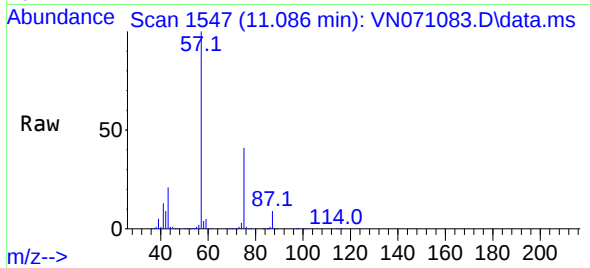

#59  
2-Hexanone  
Concen: 123.098 ug/l  
RT: 11.086 min Scan# 1547  
Delta R.T. 0.006 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 43 Resp: 1236990  
Ion Ratio Lower Upper  
43 100  
58 17.5 26.9 80.7#

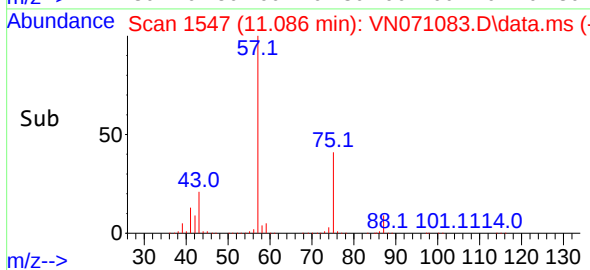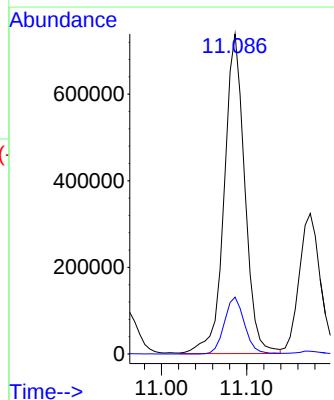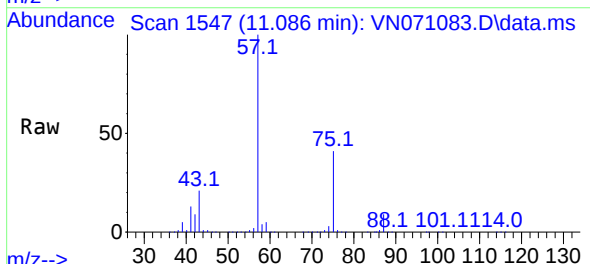




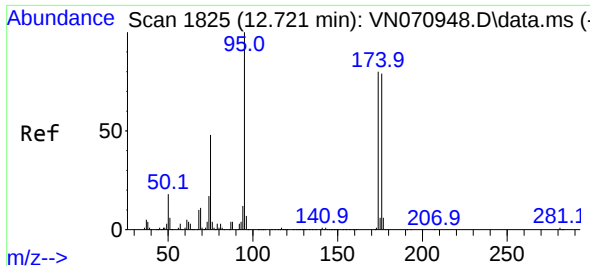


#62  
4-Bromofluorobenzene  
Concen: 49.428 ug/l  
RT: 12.727 min Scan# 1826  
Delta R.T. 0.006 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11

Tgt Ion: 95 Resp: 615229




| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 95  | 100   |       |       |
| 174 | 79.8  | 0.0   | 187.2 |
| 176 | 76.6  | 0.0   | 181.4 |

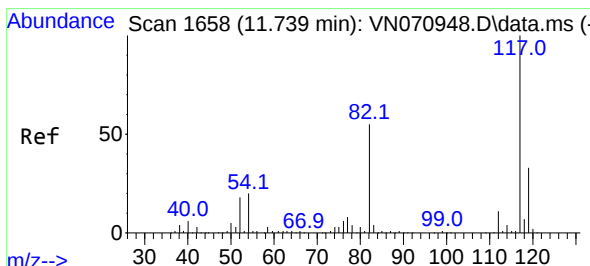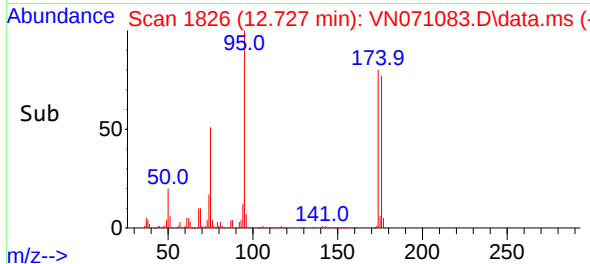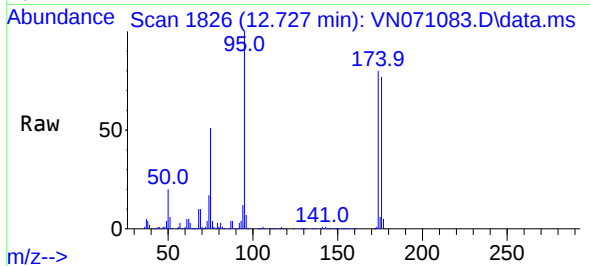


#63  
Chlorobenzene-d5  
Concen: 50.000 ug/l  
RT: 11.739 min Scan# 1658  
Delta R.T. 0.000 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 117 Resp: 1304873


| Ion | Ratio | Lower | Upper |
|-----|-------|-------|-------|
| 117 | 100   |       |       |
| 82  | 58.0  | 42.4  | 63.6  |
| 119 | 32.2  | 25.4  | 38.2  |

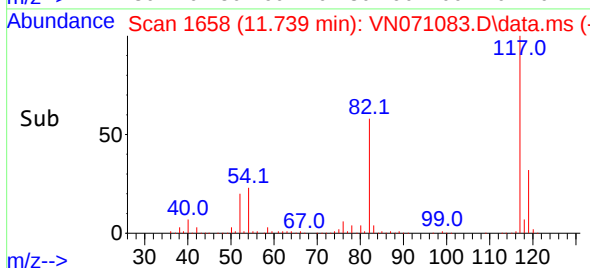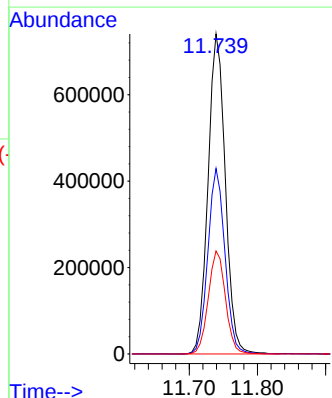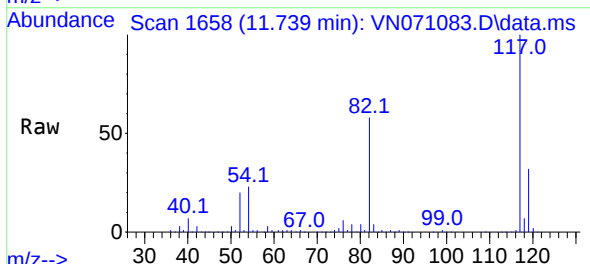






#72  
1,4-Dichlorobenzene-d4  
Concen: 50.000 ug/l  
RT: 13.668 min Scan# 1986  
Delta R.T. 0.000 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34


Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11





Tgt Ion:152 Resp: 472147  
Ion Ratio Lower Upper  
152 100  
115 58.4 27.5 82.5  
150 157.3 0.0 344.4

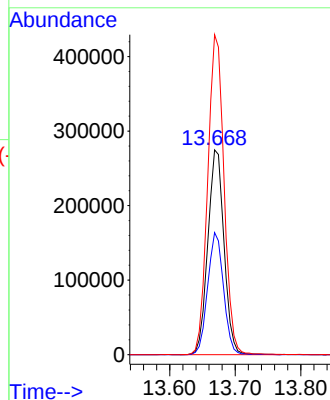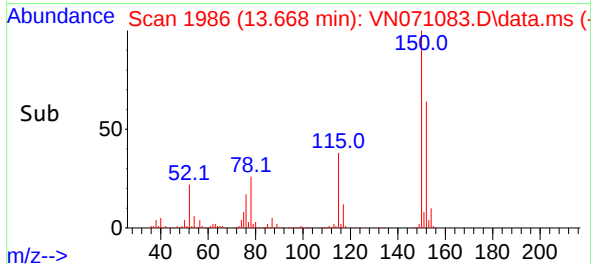


#74  
N-ethyl acetate  
Concen: 0.215 ug/l  
RT: 12.345 min Scan# 1761  
Delta R.T. -0.035 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

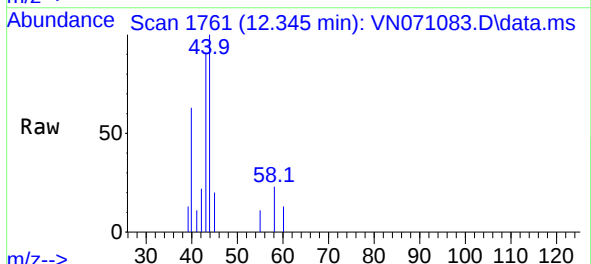

Tgt Ion: 43 Resp: 2607  
Ion Ratio Lower Upper  
43 100  
70 0.0 33.4 50.0#  
55 0.0 19.3 28.9#  
61 0.0 18.5 27.7#



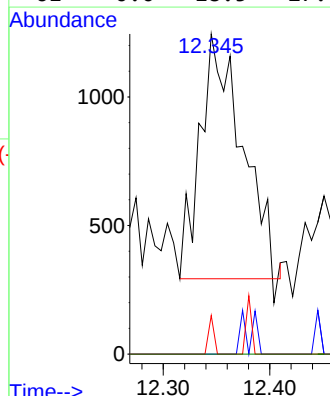



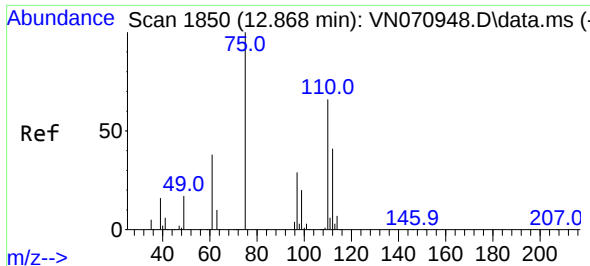

#76  
1,2,3-Trichloropropane  
Concen: 27.820 ug/l  
RT: 12.727 min Scan# 1826  
Delta R.T. -0.141 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34




Instrument :  
MSVOA\_N  
ClientSampleId :  
TP-11


Tgt Ion: 75 Resp: 309266  
Ion Ratio Lower Upper  
75 100  
77 1.3 82.6 247.8#

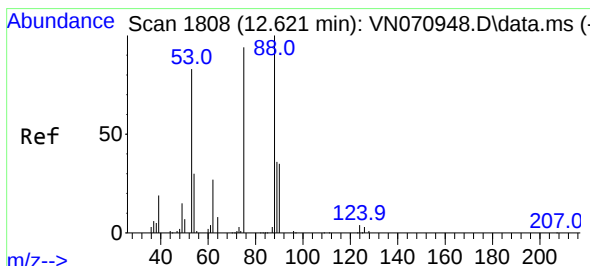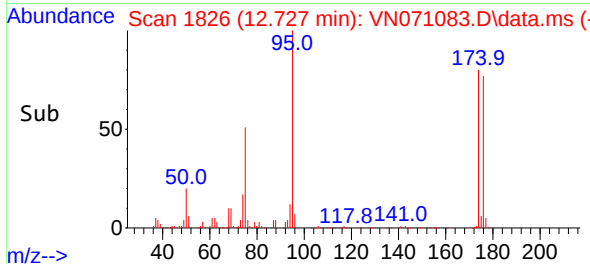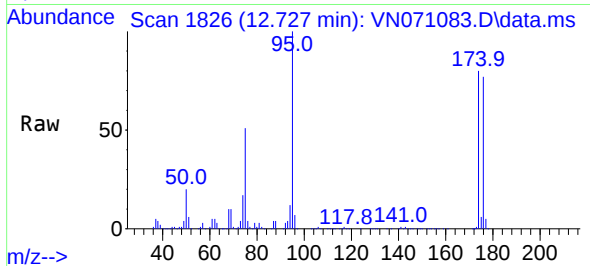

#81  
trans-1,4-Dichloro-2-butene  
Concen: 90.149 ug/l  
RT: 12.727 min Scan# 1826  
Delta R.T. 0.106 min  
Lab File: VN071083.D  
Acq: 25 Feb 2022 20:34

Tgt Ion: 75 Resp: 309266  
Ion Ratio Lower Upper  
75 100  
53 0.1 90.5 135.7#  
89 0.0 38.2 57.4#

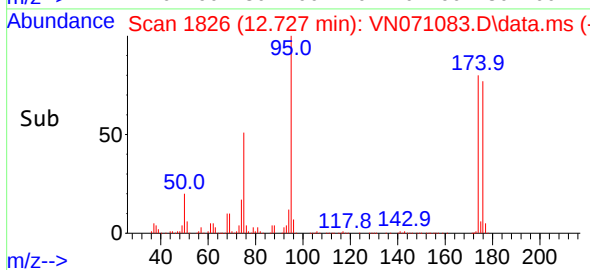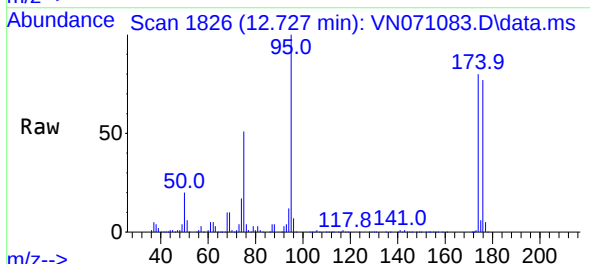



#93

1,2,4-Trichlorobenzene

Concen: 2.030 ug/l

RT: 15.262 min Scan# 21

Delta R.T. 0.005 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34





Instrument :

MSVOA\_N

ClientSampleId :

TP-11

|             |       |            |
|-------------|-------|------------|
| Tgt Ion:180 | Resp: | 285        |
| Ion Ratio   | Lower | Upper      |
| 180         | 100   |            |
| 182         | 104.2 | 48.3 144.9 |
| 145         | 0.0   | 14.5 43.5# |

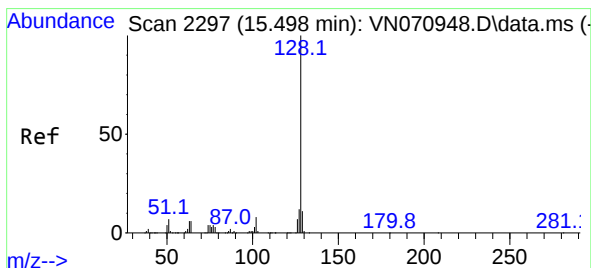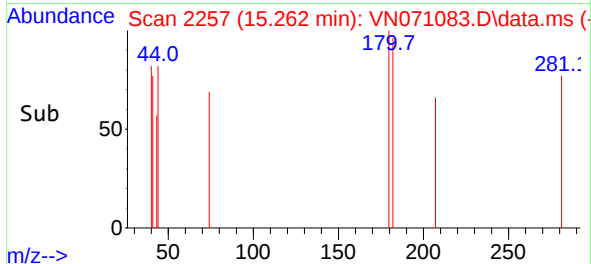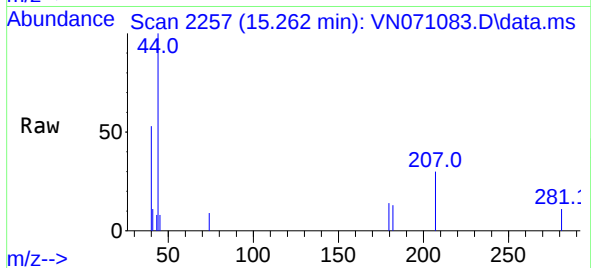

#95

Naphthalene

Concen: 5.050 ug/l




RT: 15.509 min Scan# 2299


Delta R.T. 0.011 min

Lab File: VN071083.D

Acq: 25 Feb 2022 20:34

|             |       |            |
|-------------|-------|------------|
| Tgt Ion:128 | Resp: | 1416       |
| Ion Ratio   | Lower | Upper      |
| 128         | 100   |            |
| 127         | 4.0   | 10.5 15.7# |
| 129         | 0.0   | 8.7 13.1#  |

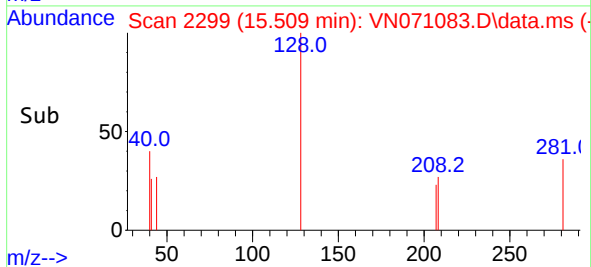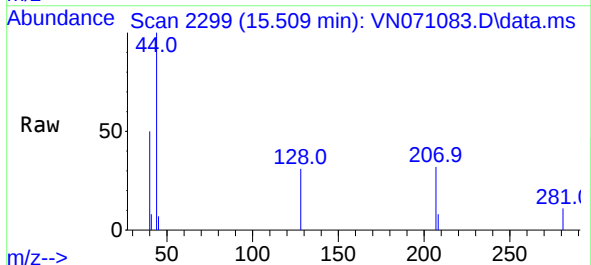



#96

1,2,3-Trichlorobenzene

Concen: 2.532 ug/l

RT: 15.698 min Scan# 21

Delta R.T. 0.006 min

Lab File: VN071083.D


Acq: 25 Feb 2022 20:34

Instrument :

MSVOA\_N

ClientSampleId :

TP-11

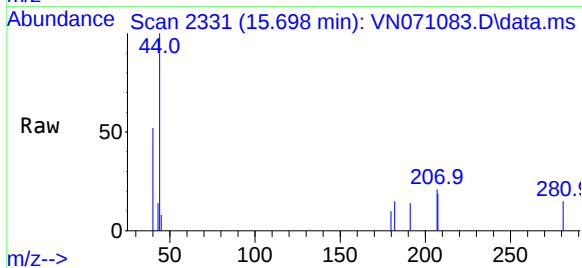

Tgt Ion:180 Resp: 132

Ion Ratio Lower Upper

180 100

182 228.0 47.4 142.2#

145 0.0 15.0 45.1#

