

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022522\
 Data File : VN071069.D
 Acq On : 25 Feb 2022 13:02
 Operator : JC\MD
 Sample : VN0225MBL01
 Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0225MBL01

Quant Time: Feb 26 03:41:51 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 21 07:57:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	842824	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1339964	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1181308	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	408355	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	501639	52.104	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	104.200%
35) Dibromofluoromethane	8.022	113	395322	49.601	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	99.200%
50) Toluene-d8	10.439	98	1590306	49.686	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.380%
62) 4-Bromofluorobenzene	12.727	95	486009	42.480	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	84.960%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022522\
Data File : VN071069.D
Acq On : 25 Feb 2022 13:02
Operator : JC\MD
Sample : VN0225MBL01
Misc : 5.00g/10.0mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01

Quant Time: Feb 26 03:41:51 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 21 07:57:15 2022
Response via : Initial Calibration




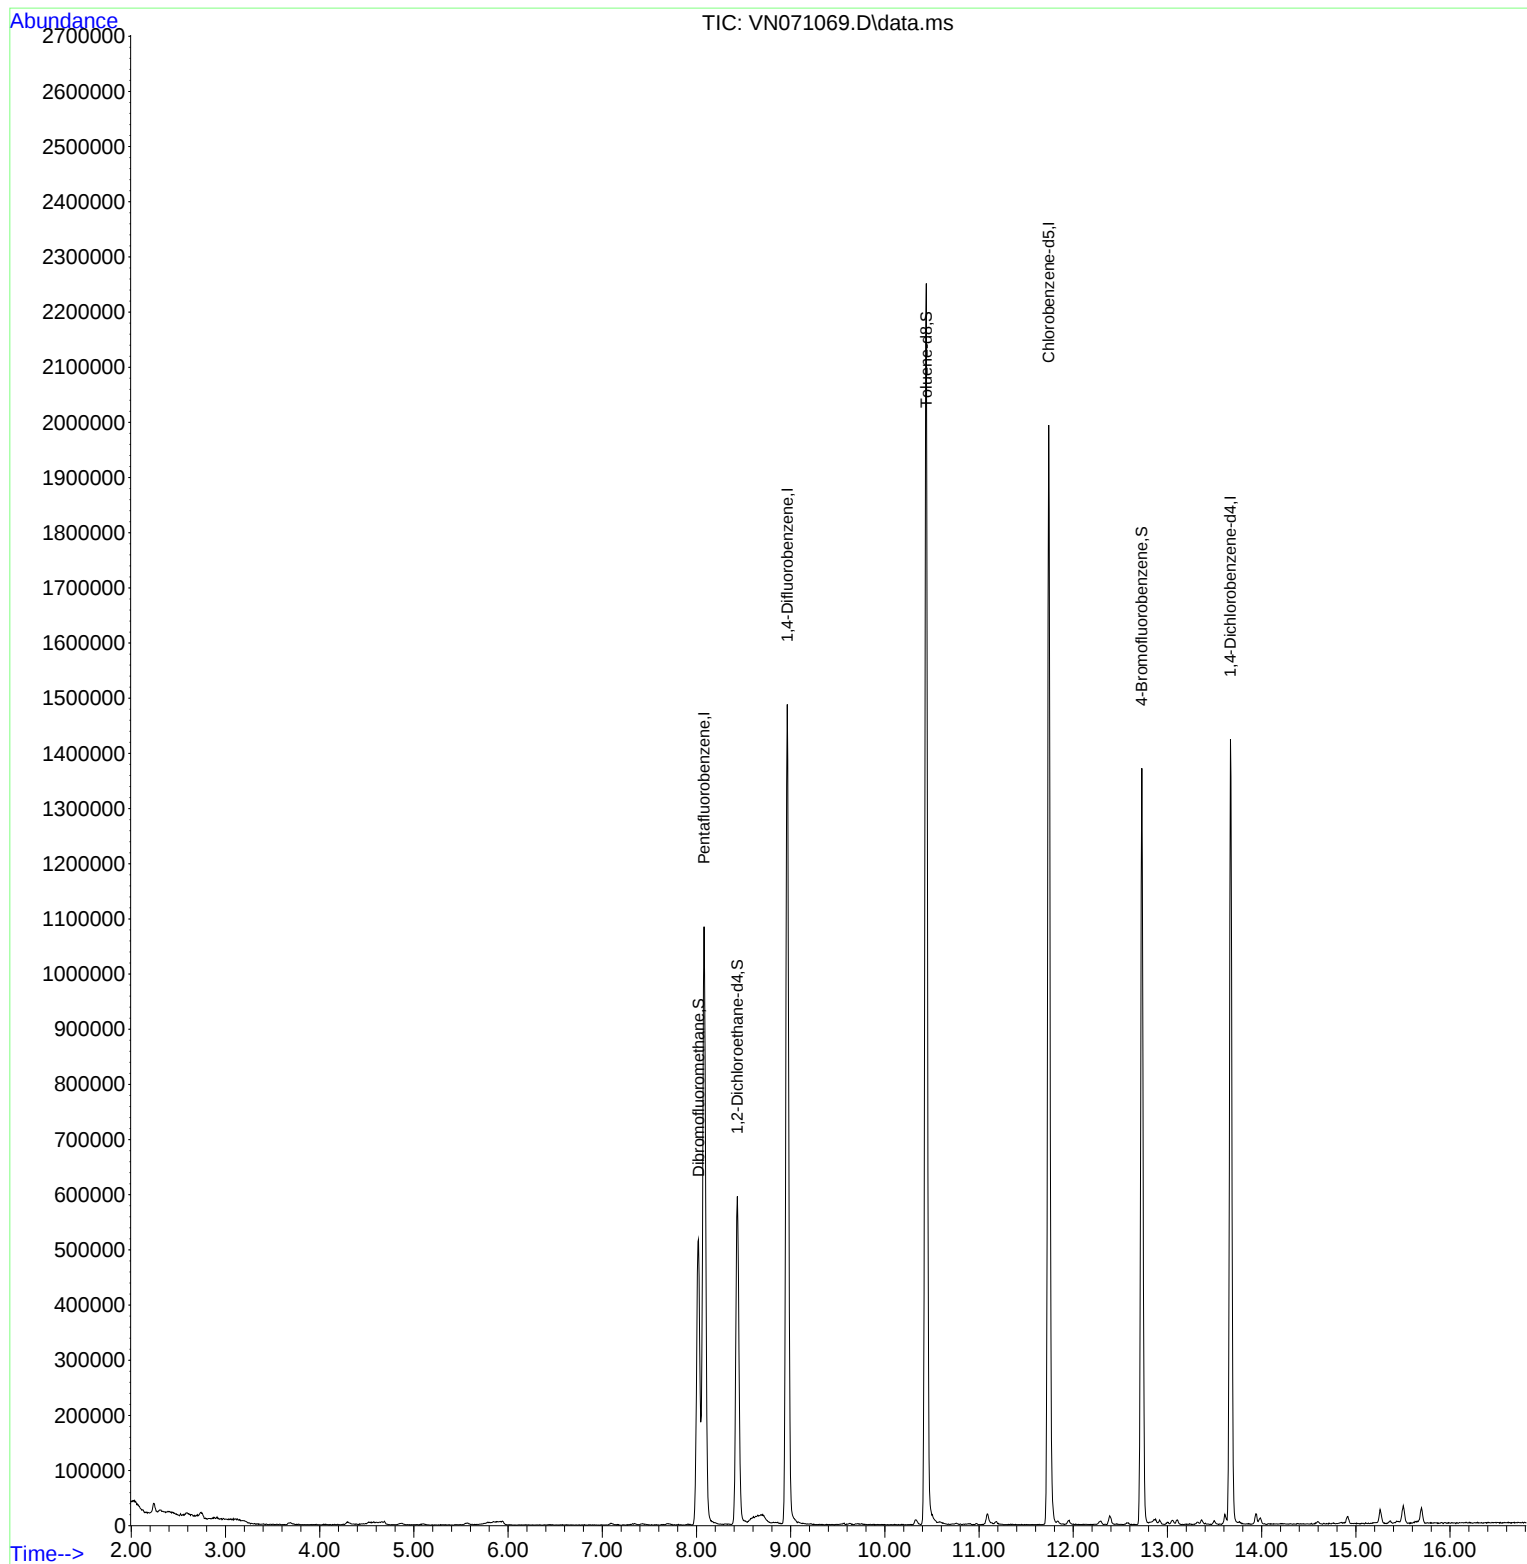


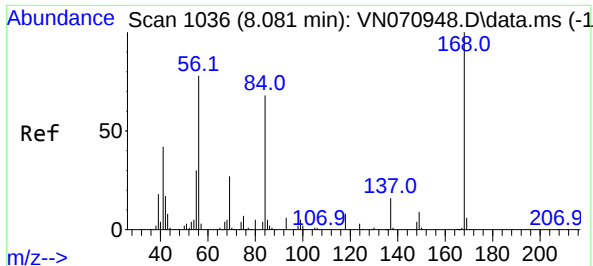

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.000 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02




Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01


Tgt Ion:168 Resp: 842824
Ion Ratio Lower Upper
168 100
99 56.4 41.3 61.9

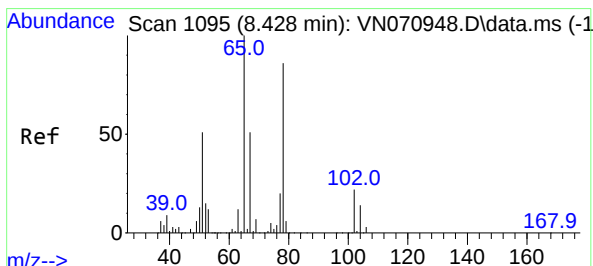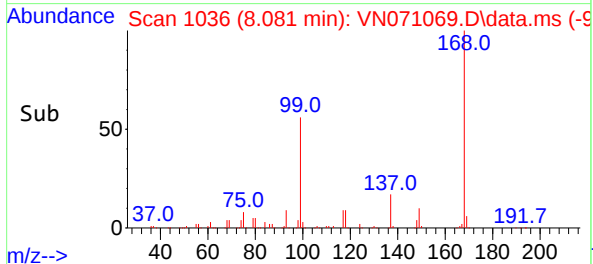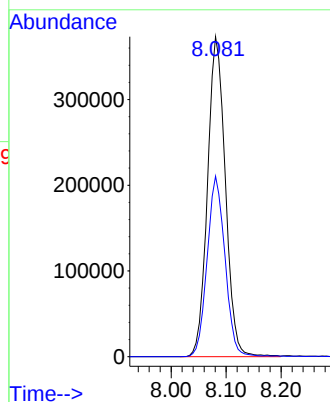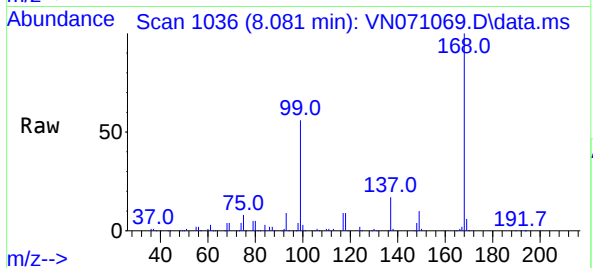

#33
1,2-Dichloroethane-d4
Concen: 52.104 ug/l
RT: 8.433 min Scan# 1096
Delta R.T. 0.006 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02

Tgt Ion: 65 Resp: 501639
Ion Ratio Lower Upper
65 100
67 52.9 0.0 103.0


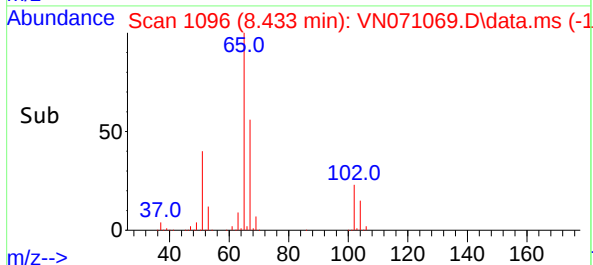
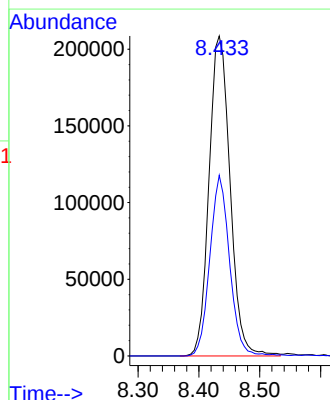
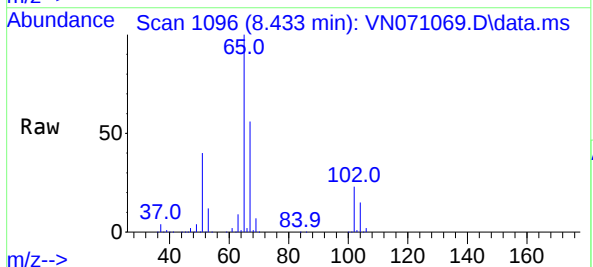


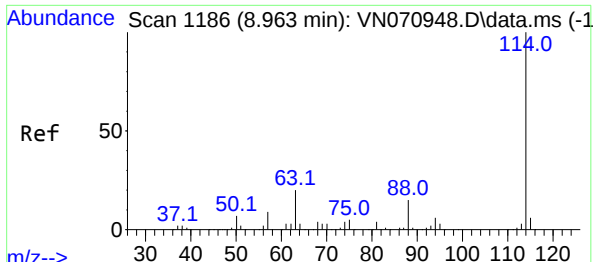

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02




Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01


Tgt Ion:114 Resp: 1339964
Ion Ratio Lower Upper
114 100
63 21.8 0.0 37.8
88 15.6 0.0 27.4

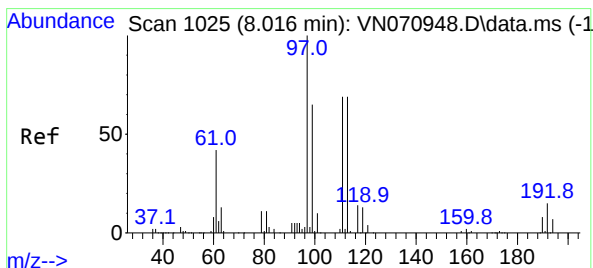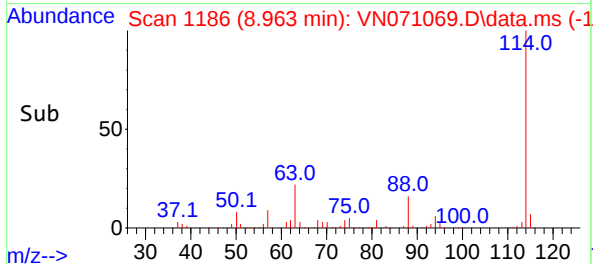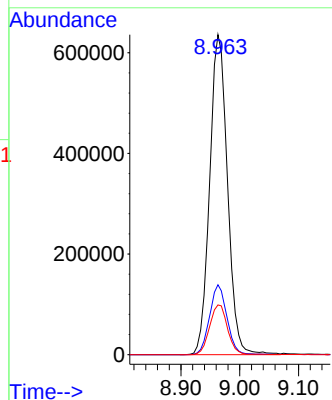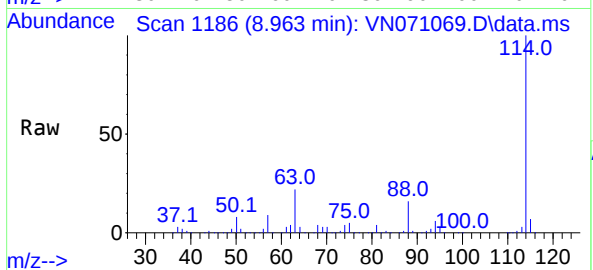

#35
Dibromofluoromethane
Concen: 49.601 ug/l
RT: 8.022 min Scan# 1026
Delta R.T. 0.006 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02

Tgt Ion:113 Resp: 395322
Ion Ratio Lower Upper
113 100
111 101.5 82.2 123.2
192 20.8 16.9 25.3


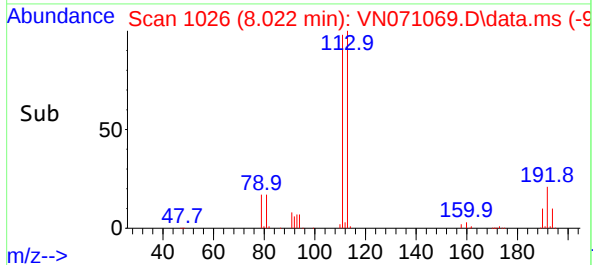
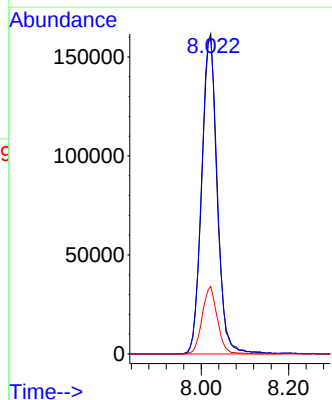
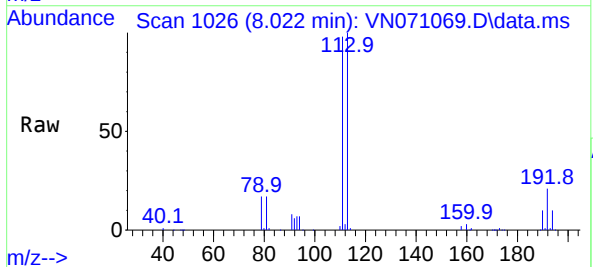


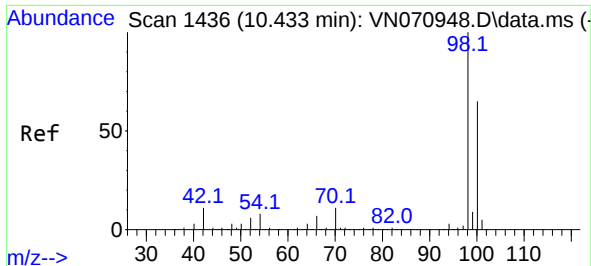

#50
Toluene-d8
Concen: 49.686 ug/l
RT: 10.439 min Scan# 1436
Delta R.T. 0.006 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02




Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01


Tgt Ion: 98 Resp: 1590306
Ion Ratio Lower Upper
98 100
100 66.2 50.4 75.6

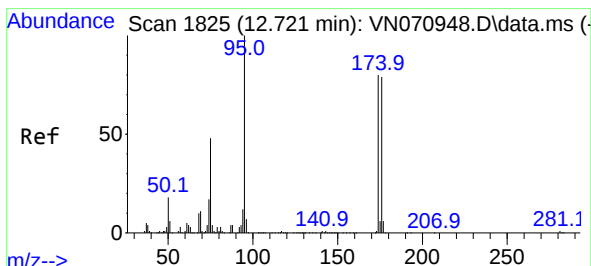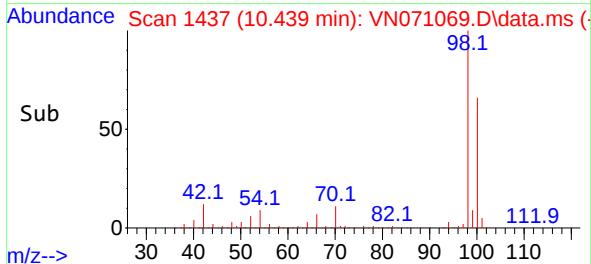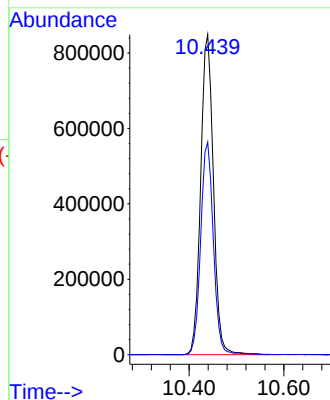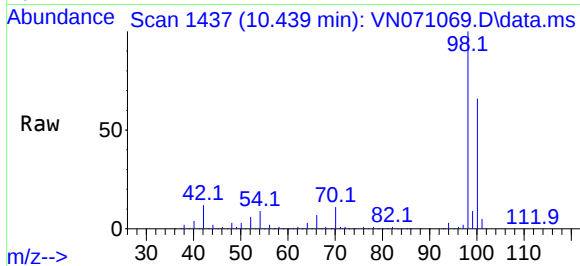

#62
4-Bromofluorobenzene
Concen: 42.480 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.006 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02

Tgt Ion: 95 Resp: 486009
Ion Ratio Lower Upper
95 100
174 80.8 0.0 187.2
176 76.7 0.0 181.4


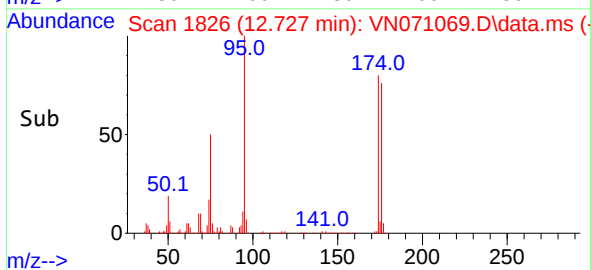
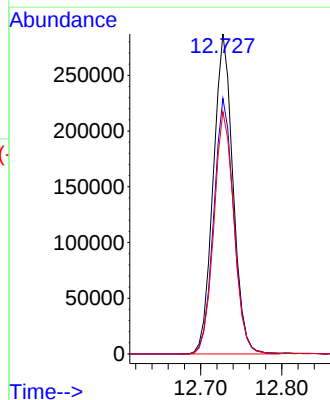
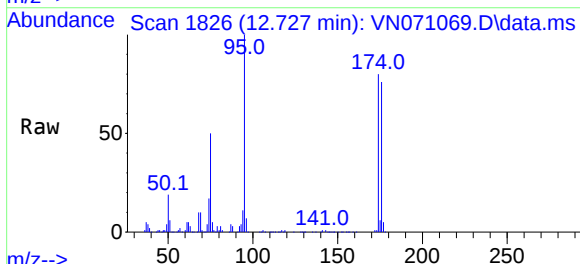


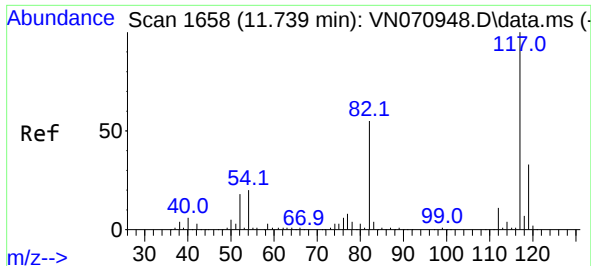

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02

Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01

Tgt Ion:117 Resp: 1181308
Ion Ratio Lower Upper
117 100
82 57.3 42.4 63.6
119 31.4 25.4 38.2

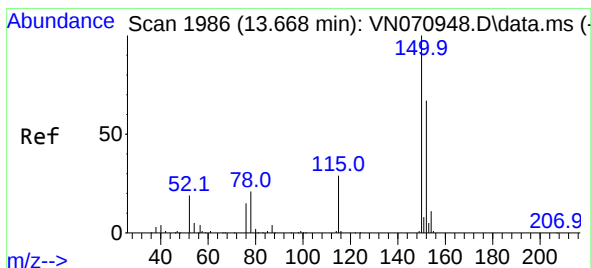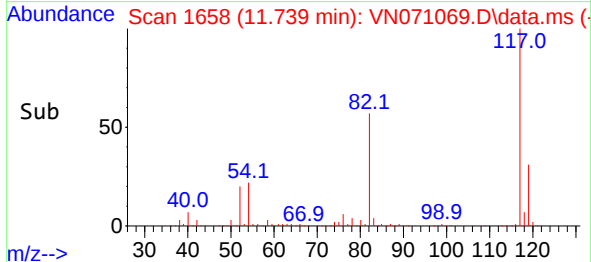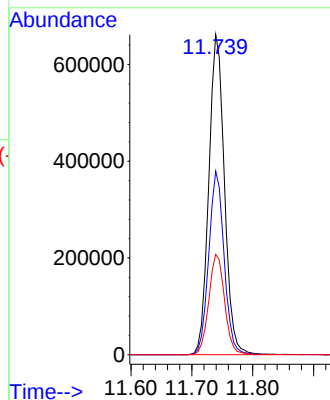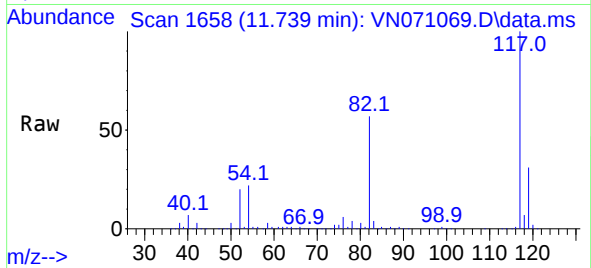

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN071069.D
Acq: 25 Feb 2022 13:02

Tgt Ion:152 Resp: 408355
Ion Ratio Lower Upper
152 100
115 56.8 27.5 82.5
150 155.9 0.0 344.4

