

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022525\
 Data File : VN085848.D
 Acq On : 25 Feb 2025 11:19
 Operator : JC\MD
 Sample : VN0225MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0225MBL01

Quant Time: Feb 25 23:23:16 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	212309	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	398494	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	358977	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	138211	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	172010	62.492	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	124.980%
35) Dibromofluoromethane	8.165	113	151153	57.967	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	115.940%
50) Toluene-d8	10.565	98	495454	52.224	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	104.440%
62) 4-Bromofluorobenzene	12.847	95	142420	45.563	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	91.120%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022525\
Data File : VN085848.D
Acq On : 25 Feb 2025 11:19
Operator : JC\MD
Sample : VN0225MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01


Quant Time: Feb 25 23:23:16 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration

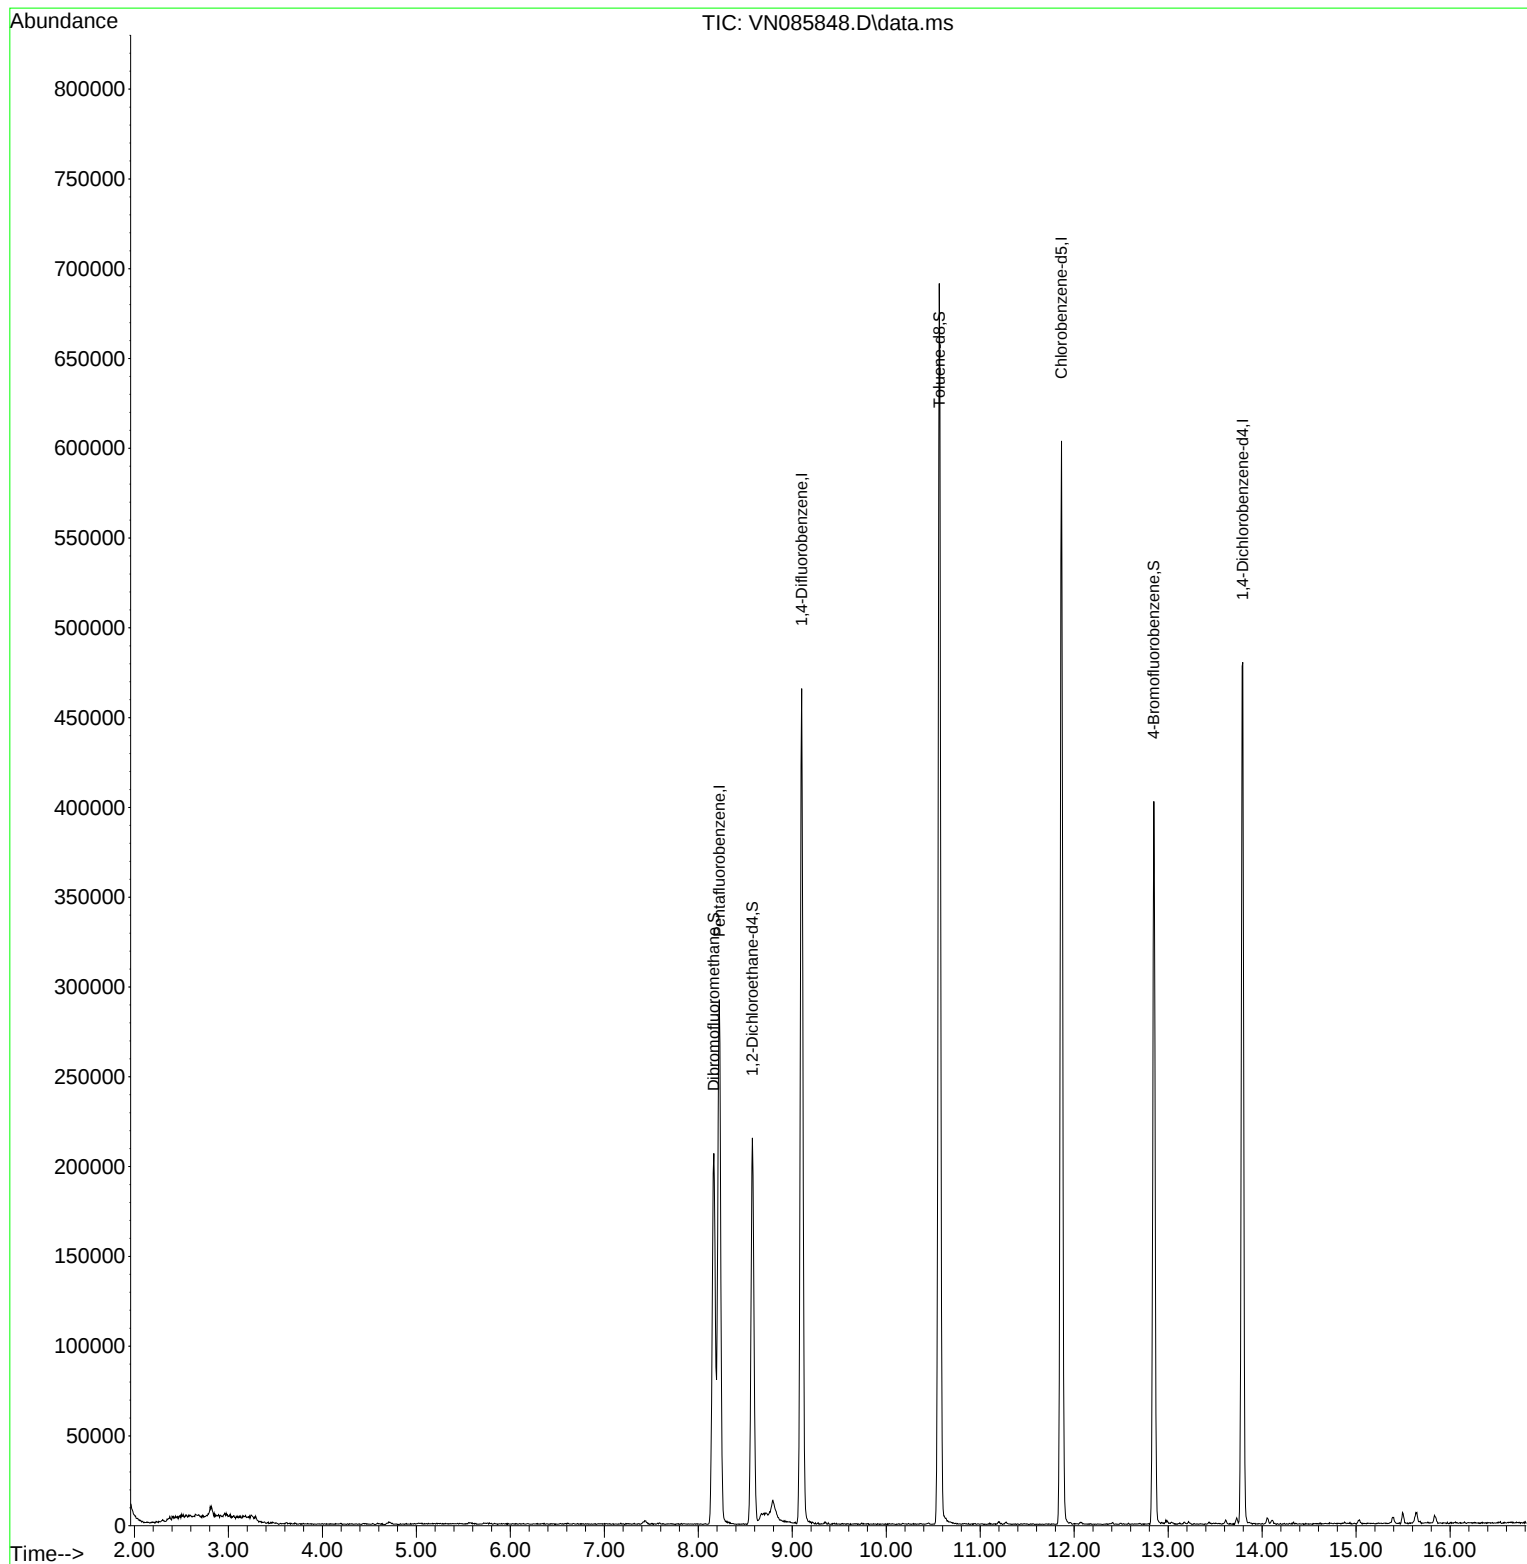



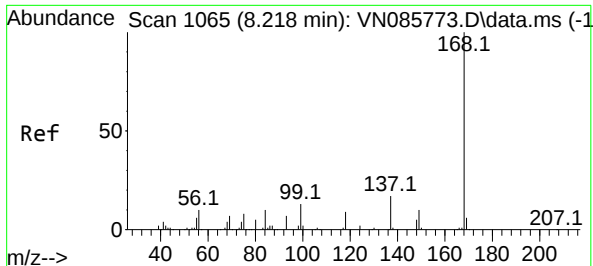


#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1125
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19

Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01



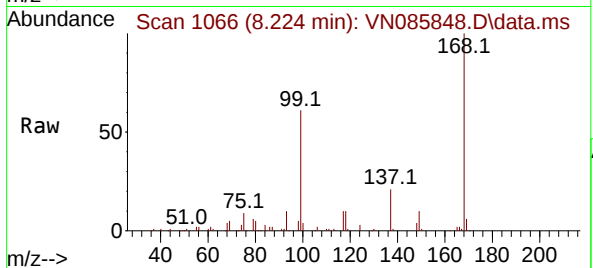



Tgt Ion:168 Resp: 212309
Ion Ratio Lower Upper
168 100
99 61.2 47.9 71.9

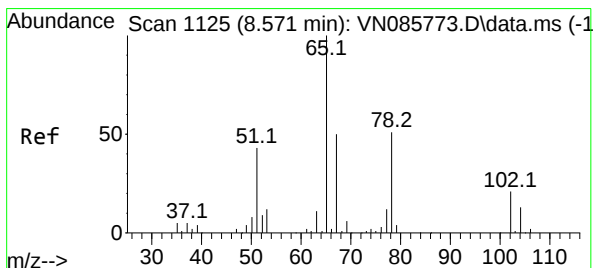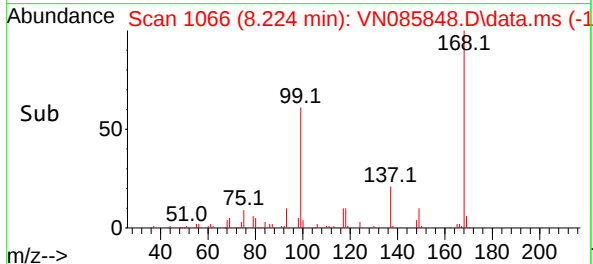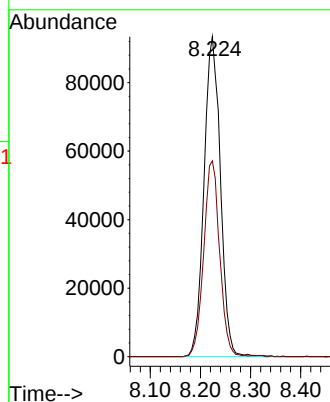

#33
1,2-Dichloroethane-d4
Concen: 62.492 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19

Tgt Ion: 65 Resp: 172010
Ion Ratio Lower Upper
65 100
67 53.6 0.0 106.2

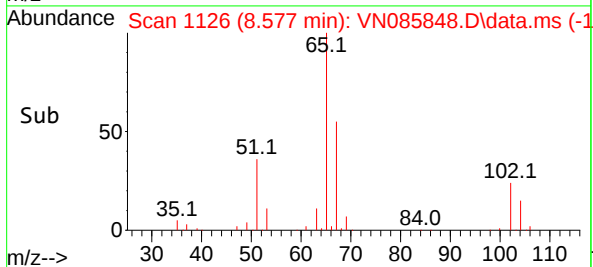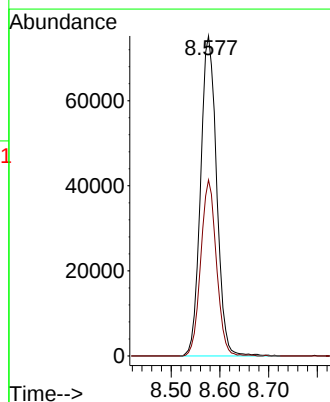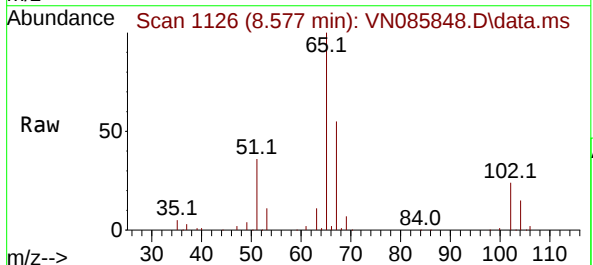

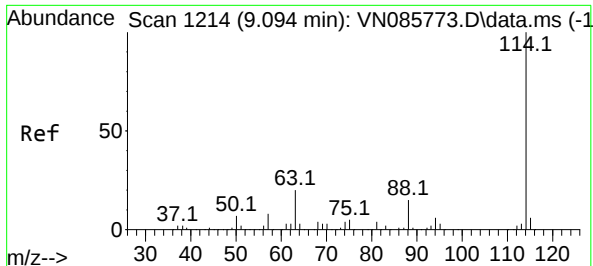

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085848.D

Acq: 25 Feb 2025 11:19

Instrument :

MSVOA_N

ClientSampleId :

VN0225MBL01





Tgt Ion:114 Resp: 398494

Ion Ratio Lower Upper

114 100

63 20.4 0.0 39.2

88 16.1 0.0 30.0

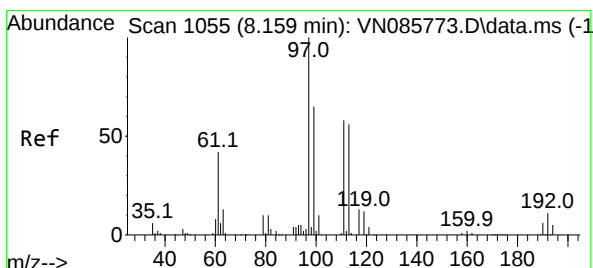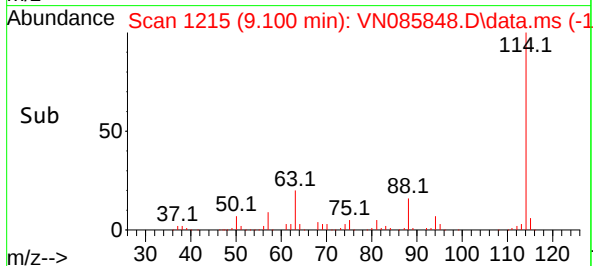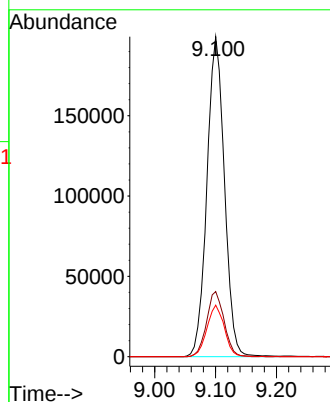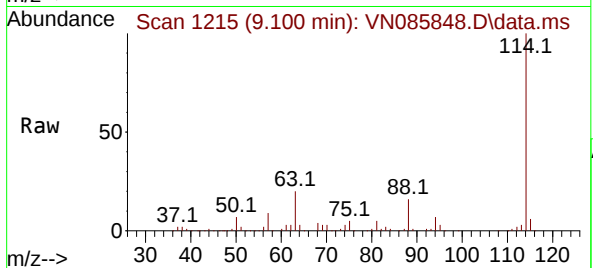

#35

Dibromofluoromethane

Concen: 57.967 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085848.D

Acq: 25 Feb 2025 11:19




Tgt Ion:113 Resp: 151153


Ion Ratio Lower Upper

113 100

111 102.6 82.2 123.4

192 18.9 14.7 22.1


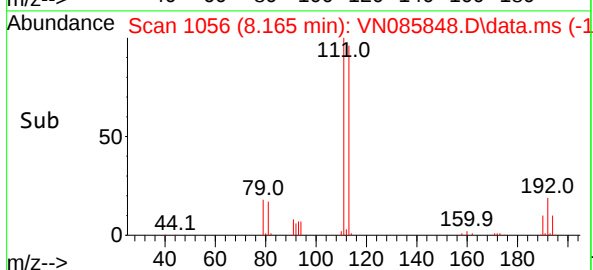
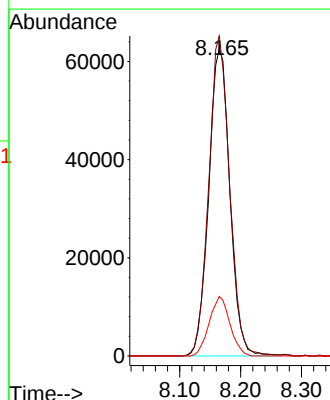
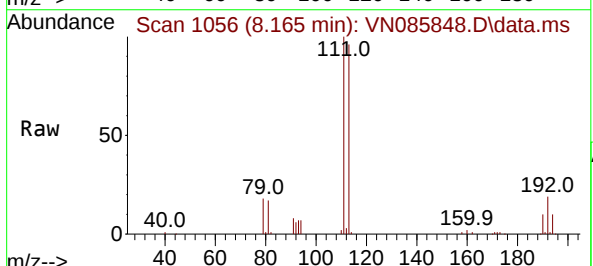


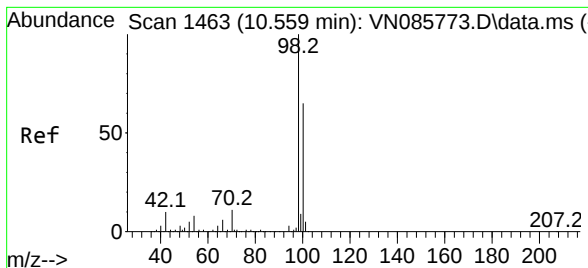

#50
Toluene-d8
Concen: 52.224 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19




Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01


Tgt Ion: 98 Resp: 495454
Ion Ratio Lower Upper
98 100
100 63.1 52.1 78.1

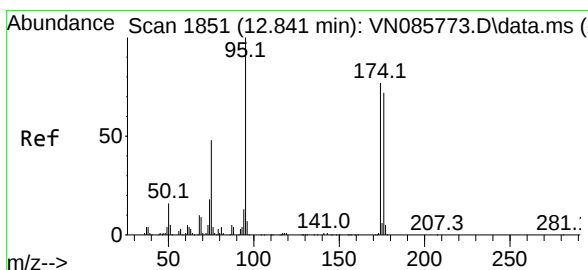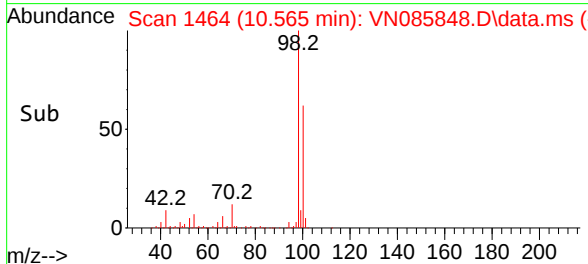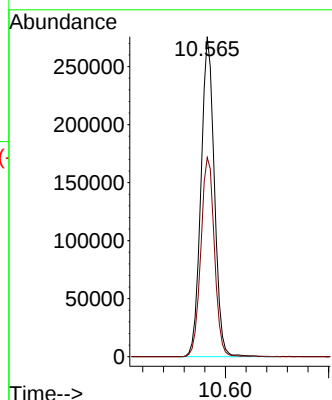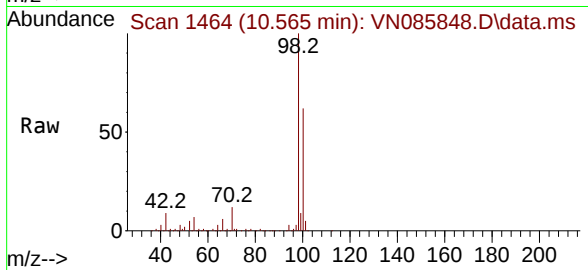

#62
4-Bromofluorobenzene
Concen: 45.563 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19


Tgt Ion: 95 Resp: 142420
Ion Ratio Lower Upper
95 100
174 79.6 0.0 152.4
176 74.8 0.0 146.6

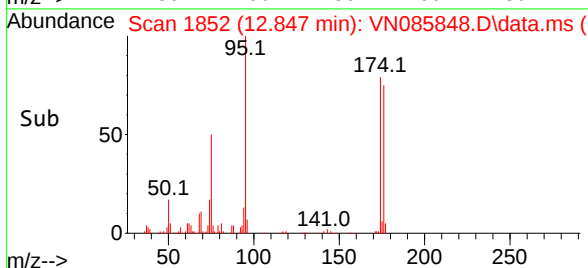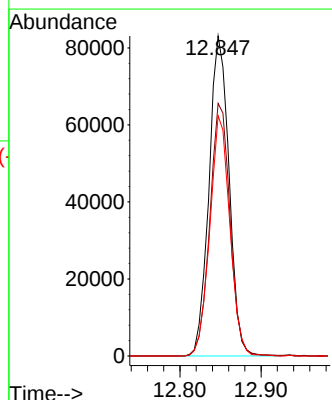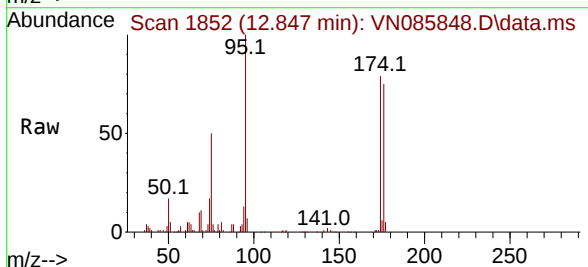



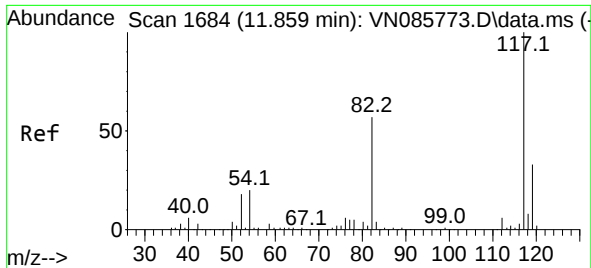


#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19

Instrument :
MSVOA_N
ClientSampleId :
VN0225MBL01

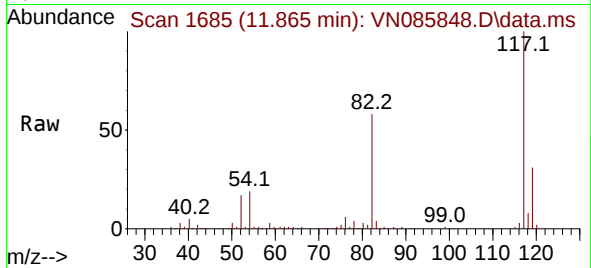

Tgt Ion:117 Resp: 358977
Ion Ratio Lower Upper
117 100
82 58.0 45.7 68.5
119 31.5 26.2 39.2

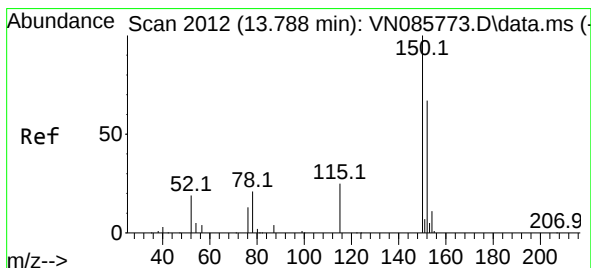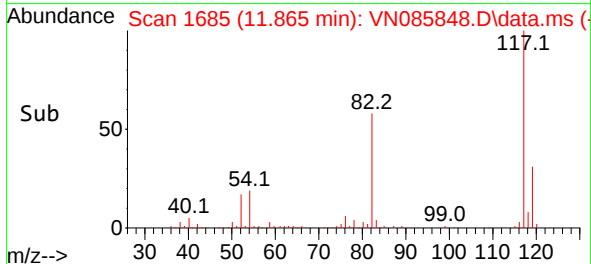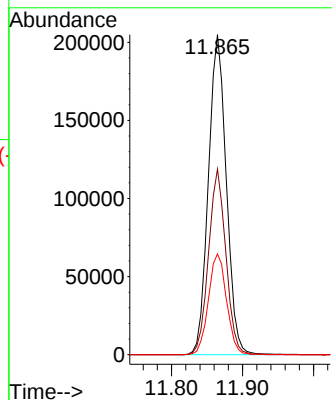

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.006 min
Lab File: VN085848.D
Acq: 25 Feb 2025 11:19

Tgt Ion:152 Resp: 138211
Ion Ratio Lower Upper
152 100
115 62.0 30.4 91.3
150 159.1 0.0 345.4

