


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022525\
Data File : VN085846.D
Acq On : 25 Feb 2025 10:11
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

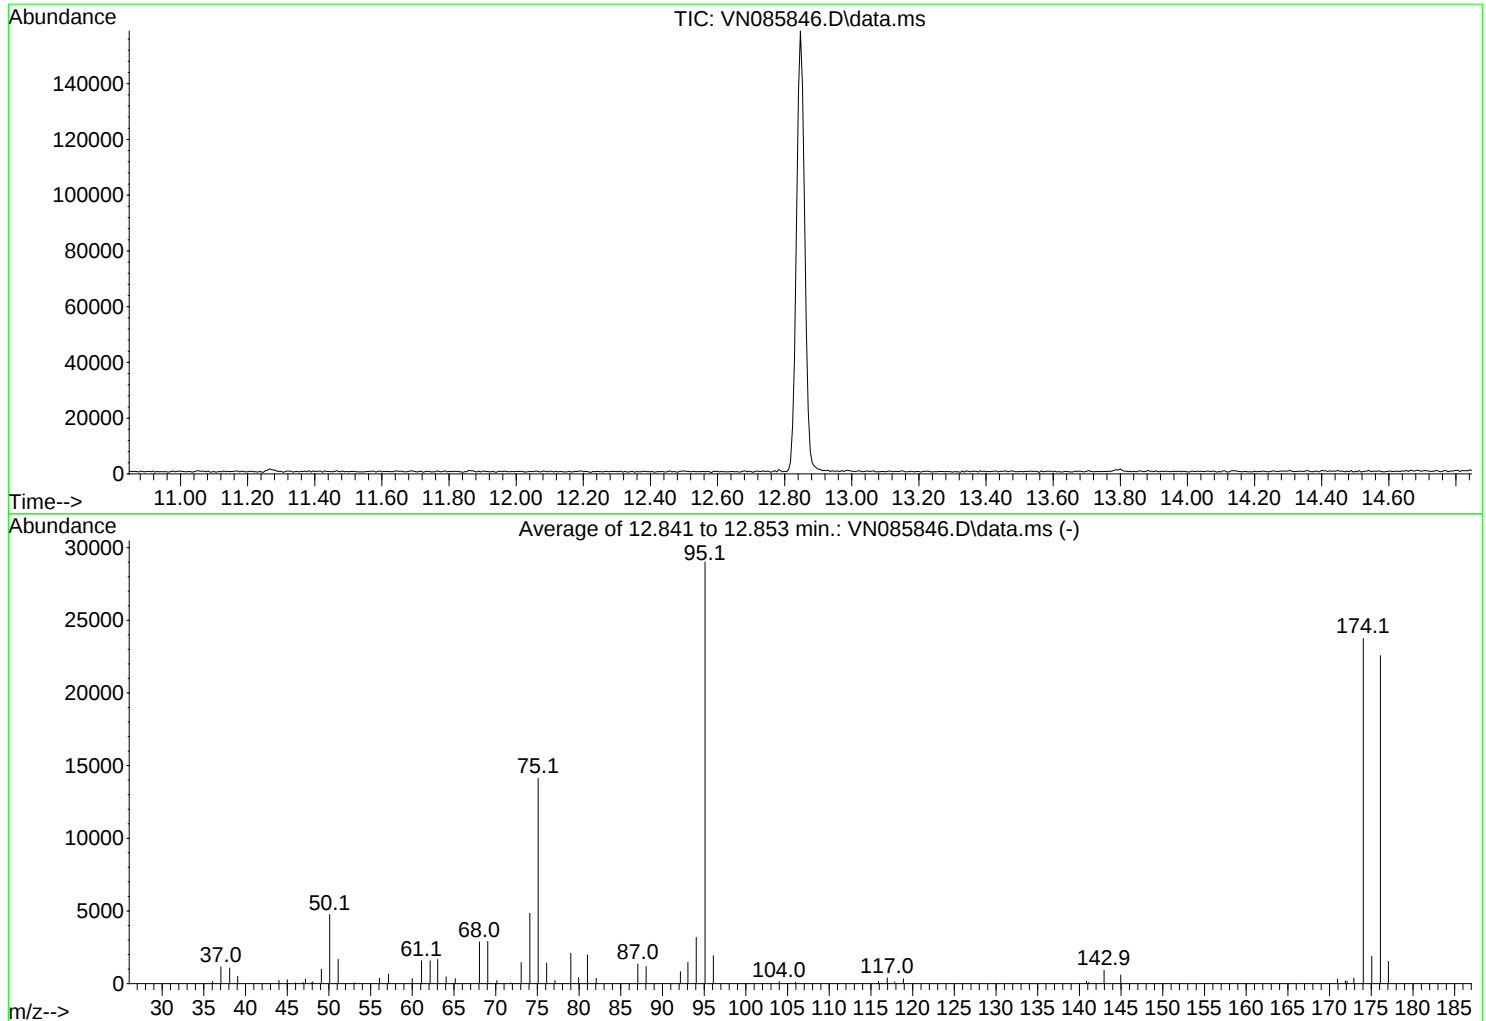

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.4	4759	PASS
75	95	30	60	48.7	14129	PASS
95	95	100	100	100.0	29021	PASS
96	95	5	9	6.7	1930	PASS
173	174	0.00	2	1.6	388	PASS
174	95	50	100	81.9	23757	PASS
175	174	5	9	7.9	1877	PASS
176	174	95	101	95.0	22573	PASS
177	176	5	9	6.8	1536	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	142	49.10	986	65.15	351	79.95	401
37.05	1157	50.10	4759	68.05	2879	81.00	1981
38.10	1078	51.10	1676	69.05	2904	82.05	361
39.05	494	53.10	51	70.15	215	87.05	135
44.00	221	56.05	375	71.80	60	88.05	1176
45.00	264	57.15	649	73.05	1450	92.15	831
46.00	54	60.00	355	74.10	4848	93.05	1464
46.90	62	61.10	1575	75.10	14129	94.05	3185
47.20	324	62.15	1570	76.10	1409	95.10	29021
47.90	52	63.05	1668	77.10	221	96.10	1930
48.05	126	64.05	479	79.00	2081	104.00	134

Average of 12.841 to 12.853 min.: VN085846.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
105.95	113	172.10	179				
115.90	157	172.90	388				
116.95	399	174.05	23757				
117.85	126	175.05	1877				
118.90	331	176.10	22573				
140.85	178	177.05	1536				
141.10	73						
142.95	914						
144.95	593						
170.95	319						
171.90	204						

Instrument :

MSVOA_N

ClientSampleId :

BFB