


Data Path : Z:\VOASRV\HPCHEM1\MSVOA_N\DATA\VN022619\
 Data File : VN053945.D
 Acq On : 26 Feb 2019 9:50
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
 Title : SW846 8260
 Last Update : Thu Feb 28 04:05:45 2019

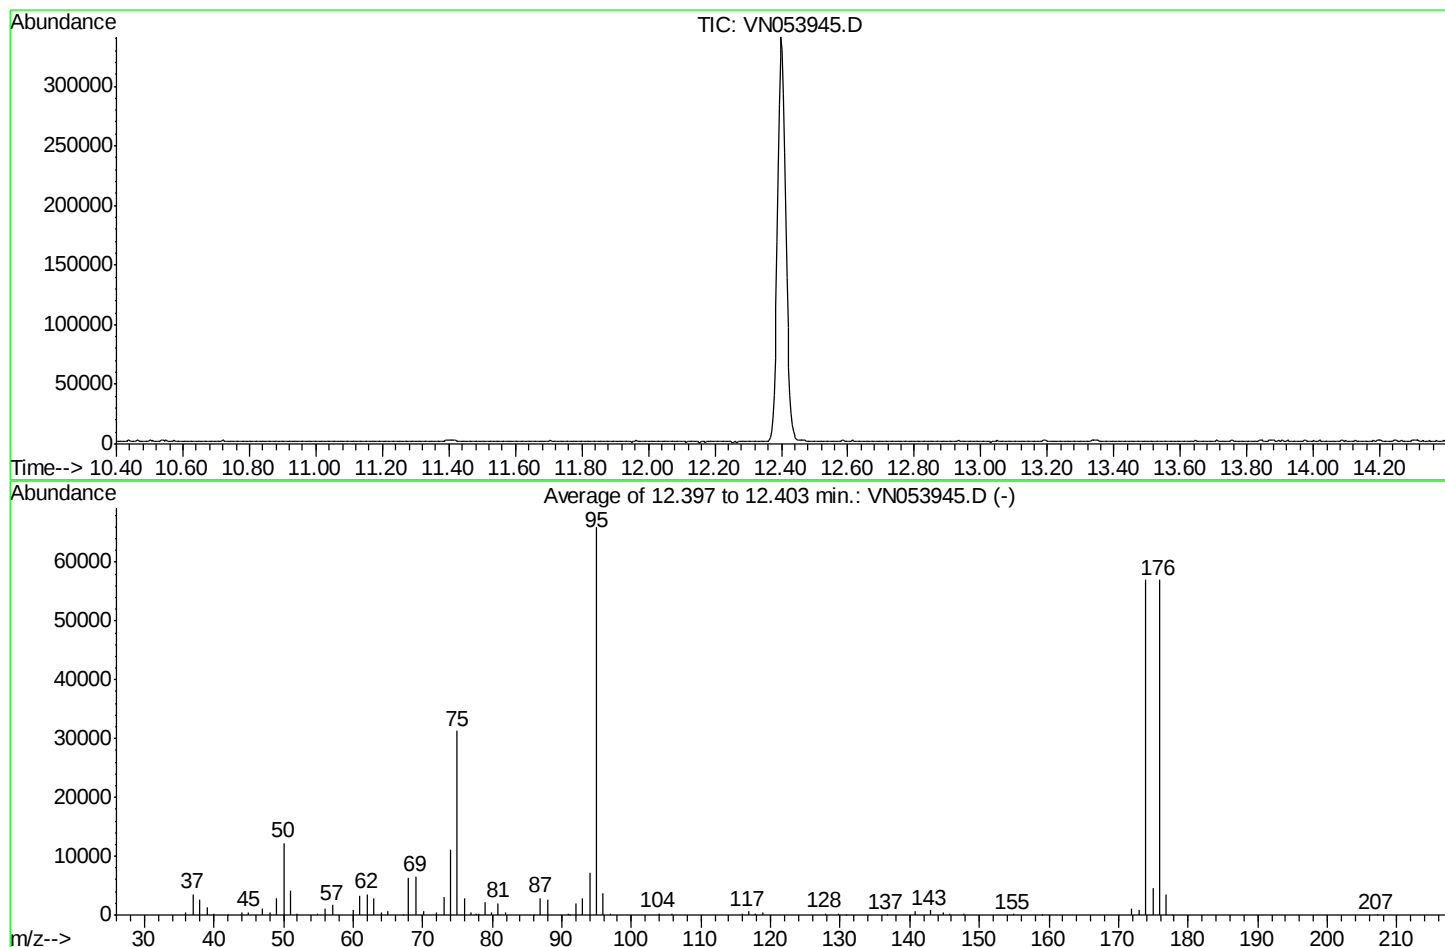

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.6	12234	PASS
75	95	30	60	47.4	31261	PASS
95	95	100	100	100.0	65925	PASS
96	95	5	9	5.6	3703	PASS
173	174	0.00	2	1.7	945	PASS
174	95	50	100	86.4	56992	PASS
175	174	5	9	7.9	4488	PASS
176	174	95	101	100.1	57021	PASS
177	176	5	9	6.3	3564	PASS