

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022621\
 Data File : VN066064.D
 Acq On : 26 Feb 2021 20:16
 Operator : JC/MD
 Sample : M1503-05
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SEDGWICK-AVE

Quant Time: Feb 26 23:38:11 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.627	168	113912	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	185983	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	170274	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	74267	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.991	65	78825	49.48	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery =	98.96%		
35) Dibromofluoromethane	7.553	113	58016	50.40	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery =	100.80%		
50) Toluene-d8	10.058	98	224896	47.60	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery =	95.20%		
62) 4-Bromofluorobenzene	12.373	95	85118	47.99	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery =	95.98%		
Target Compounds						Qvalue
3) Chloromethane	2.062	50	542	0.29	ug/l #	42
13) Acrolein	3.582	56	717	3.54	ug/l	86
16) Acetone	3.791	43	7051	12.57	ug/l	100
18) Methyl Acetate	4.299	43	651	0.49	ug/l #	51
20) Methylene Chloride	4.515	84	4541	3.07	ug/l	95
25) 2-Butanone	6.804	43	1121	1.42	ug/l #	46
31) Cyclohexane	7.624	56	2271	0.96	ug/l #	10
36) 1,1-Dichloropropene	7.630	75	8526	4.65	ug/l #	45
37) Ethyl Acetate	6.804	43	1121	0.68	ug/l #	68
38) Carbon Tetrachloride	7.630	117	11558	6.78	ug/l #	16
39) Methylcyclohexane	9.045	83	1095	0.53	ug/l	95
43) Isopropyl Acetate	8.126	43	7135	2.70	ug/l #	83
45) 1,2-Dichloropropane	9.228	63	297	0.21	ug/l #	44
48) Methyl methacrylate	9.145	41	1687	1.26	ug/l #	10
51) 4-Methyl-2-Pentanone	9.945	43	1377	0.86	ug/l	89
52) Toluene	10.122	92	878	0.25	ug/l	99
54) cis-1,3-Dichloropropene	9.871	75	12985	5.86	ug/l #	61
55) 1,1,2-Trichloroethane	10.508	97	540	0.42	ug/l #	15
57) 1,3-Dichloropropane	10.733	76	6430	2.82	ug/l #	43
59) 2-Hexanone	10.733	43	87614	76.59	ug/l #	49
67) Ethyl Benzene	11.482	91	39335	6.10	ug/l	98
68) m/p-Xylenes	11.585	106	9207	3.83	ug/l	93
69) o-Xylene	11.920	106	4521	1.95	ug/l	88
71) Bromoform	12.379	173	183	2.69	ug/l #	1
73) Isopropylbenzene	12.219	105	8253	1.36	ug/l	99
76) 1,2,3-Trichloropropane	12.373	75	44061	24.70	ug/l #	100
78) n-propylbenzene	12.563	91	13091	1.90	ug/l	95
79) 2-Chlorotoluene	12.627	91	6952	1.61	ug/l #	40
80) 1,3,5-Trimethylbenzene	12.704	105	17739	3.44	ug/l	99
81) trans-1,4-Dichloro-2-b...	12.373	75	44061	78.71	ug/l #	12
82) 4-Chlorotoluene	12.701	91	2128	0.49	ug/l #	40
83) tert-Butylbenzene	12.968	119	1037	0.24	ug/l #	79
84) 1,2,4-Trimethylbenzene	13.010	105	28320	5.48	ug/l	99
85) sec-Butylbenzene	13.138	105	2095	0.38	ug/l	97
86) p-Isopropyltoluene	13.260	119	2792	0.56	ug/l	88
89) n-Butylbenzene	13.553	91	1302	0.31	ug/l #	1

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022621\
Data File : VN066064.D
Acq On : 26 Feb 2021 20:16
Operator : JC/MD
Sample : M1503-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE

Quant Time: Feb 26 23:38:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)
90) Hexachloroethane	13.858	117	3039	3.58	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.251	75	155	1.28	ug/l #	1
95) Naphthalene	15.100	128	71587	18.66	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022621\
Data File : VN066064.D
Acq On : 26 Feb 2021 20:16
Operator : JC/MD
Sample : M1503-05
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE

Quant Time: Feb 26 23:38:11 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




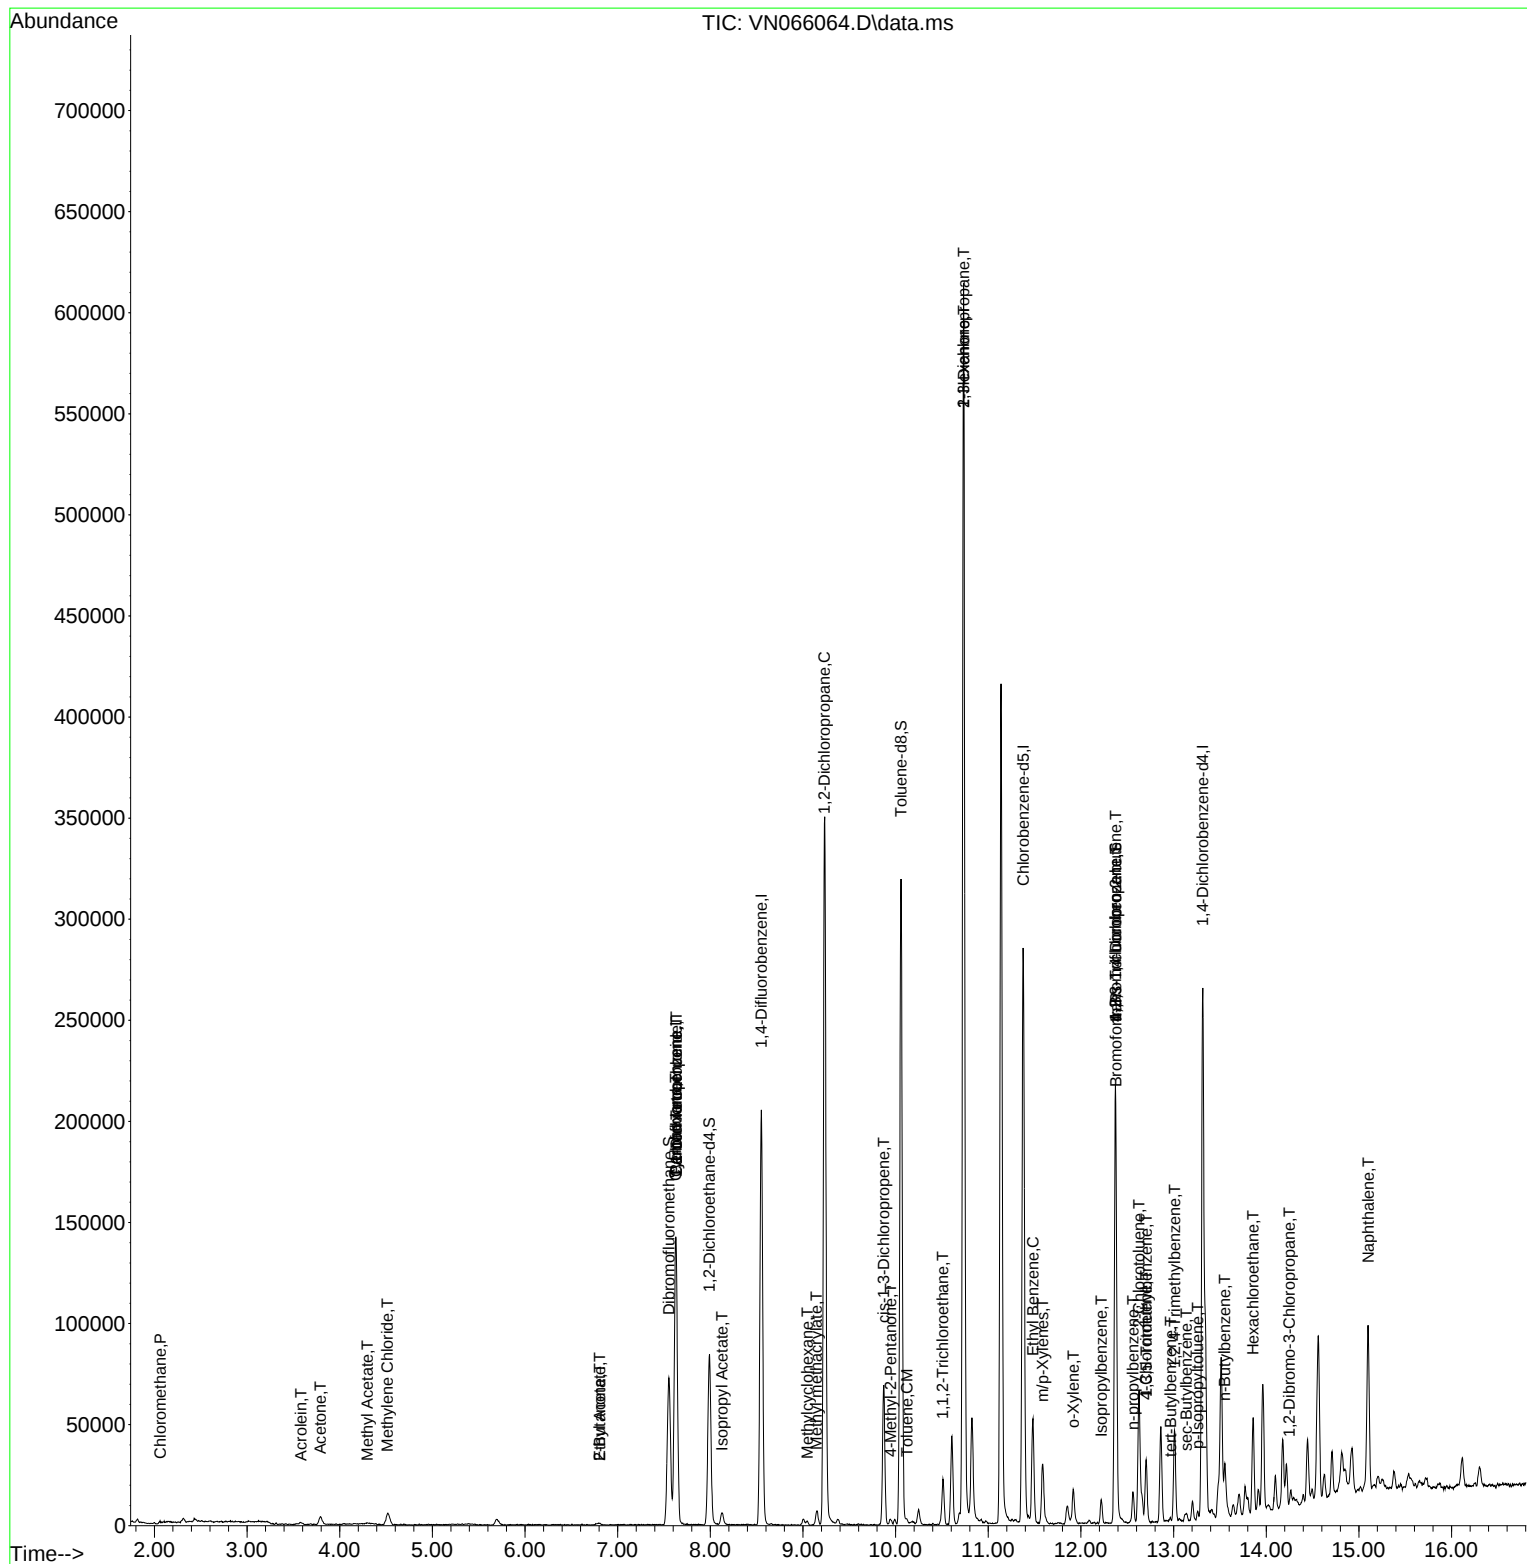




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:168 Resp: 113912
Ion Ratio Lower Upper
168 100
99 63.3 42.6 63.8

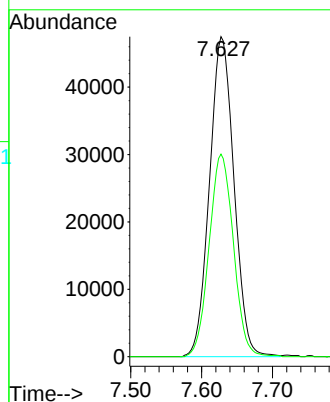

#3
Chloromethane
Concen: 0.29 ug/l
RT: 2.062 min Scan# 100
Delta R.T. 0.013 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16


Tgt Ion: 50 Resp: 542
Ion Ratio Lower Upper
50 100
52 0.0 25.8 38.8#

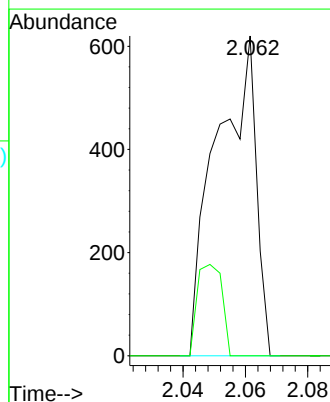






#13
Acrolein
Concen: 3.54 ug/l
RT: 3.582 min Scan# 573
Delta R.T. 0.006 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE







Tgt Ion: 56 Resp: 717
Ion Ratio Lower Upper
56 100
55 81.2 56.0 84.0



#16
Acetone
Concen: 12.57 ug/l
RT: 3.791 min Scan# 638
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 43 Resp: 7051
Ion Ratio Lower Upper
43 100
58 33.8 27.0 40.6









#18
Methyl Acetate
Concen: 0.49 ug/l
RT: 4.299 min Scan# 796
Delta R.T. 0.006 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 43 Resp: 651
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#

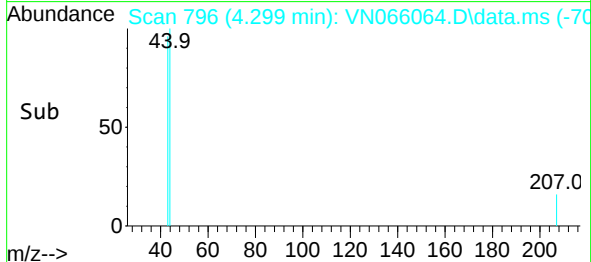

#20
Methylene Chloride
Concen: 3.07 ug/l
RT: 4.515 min Scan# 863
Delta R.T. 0.010 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 84 Resp: 4541
Ion Ratio Lower Upper
84 100
49 122.6 94.6 141.8
51 42.6 29.9 44.9
86 69.3 51.4 77.2




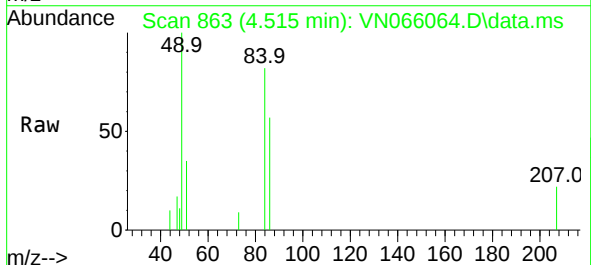


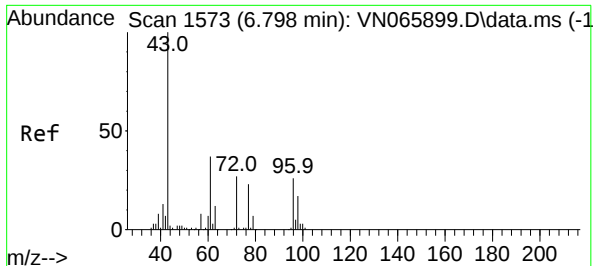

#25
2-Butanone
Concen: 1.42 ug/l
RT: 6.804 min Scan# 1575
Delta R.T. 0.006 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 43 Resp: 1121
Ion Ratio Lower Upper
43 100
72 0.0 23.1 34.7#

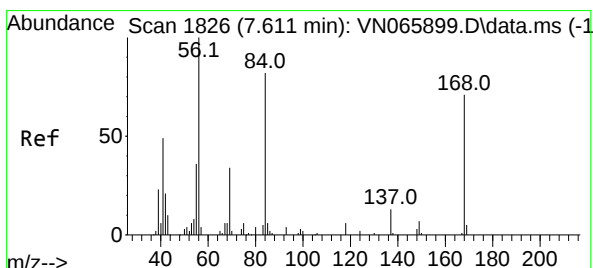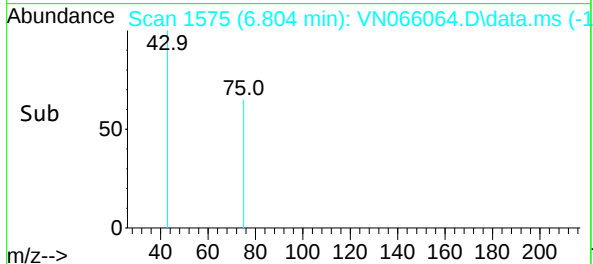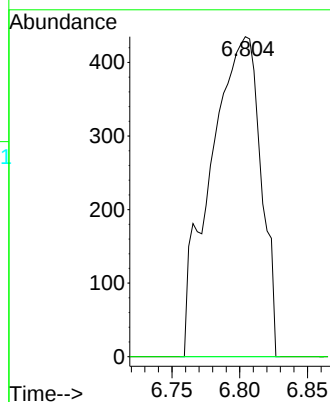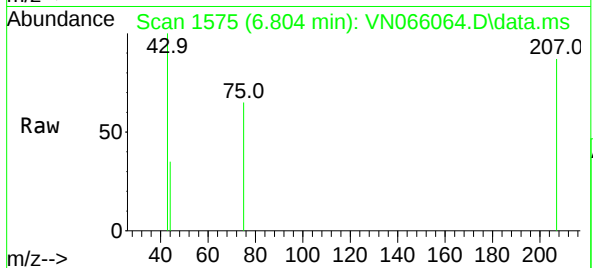

#31
Cyclohexane
Concen: 0.96 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.013 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 56 Resp: 2271
Ion Ratio Lower Upper
56 100
69 189.7 26.6 39.8#
84 106.3 70.4 105.6#


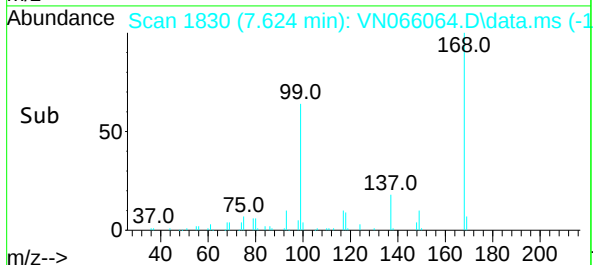
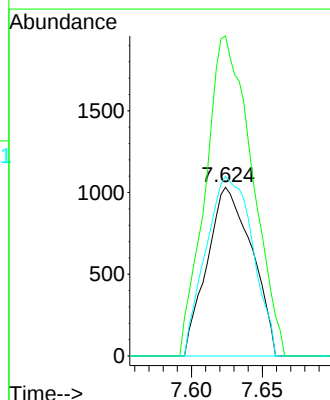
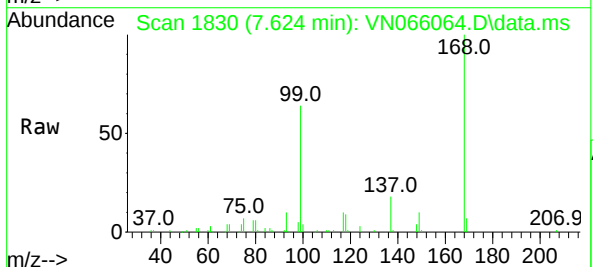


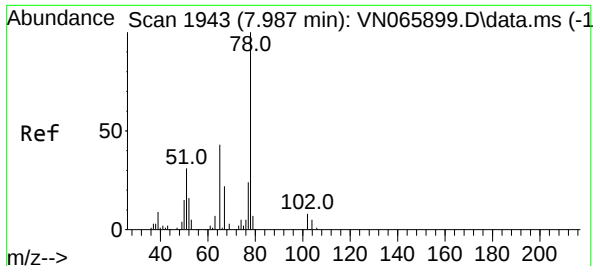

#33
1,2-Dichloroethane-d4
Concen: 49.48 ug/l
RT: 7.991 min Scan# 1944
Delta R.T. 0.004 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 65 Resp: 78825
Ion Ratio Lower Upper
65 100
67 50.9 0.0 107.2

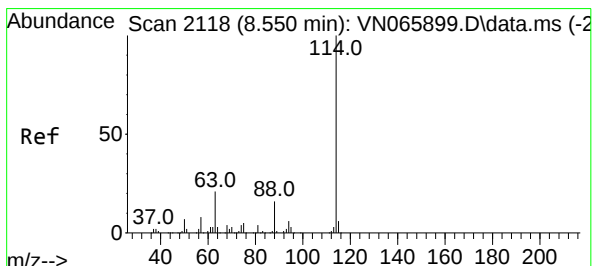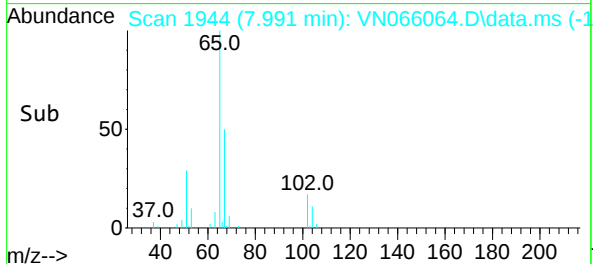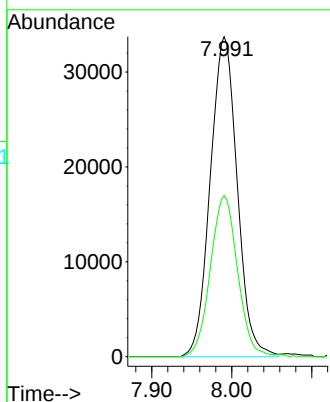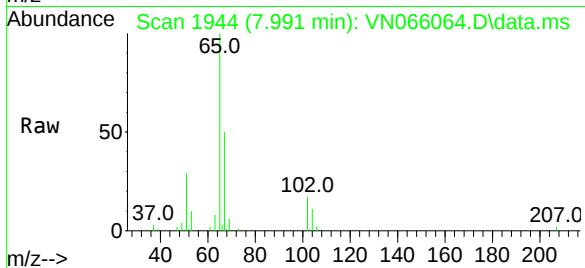

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. -0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 114 Resp: 185983
Ion Ratio Lower Upper
114 100
63 20.2 0.0 38.6
88 16.9 0.0 30.6


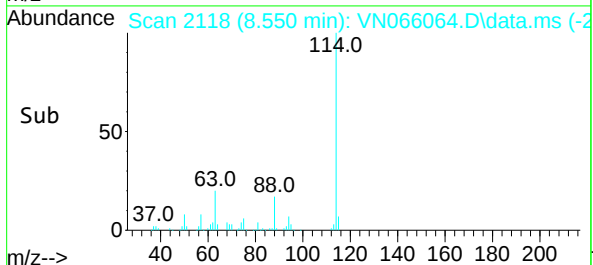
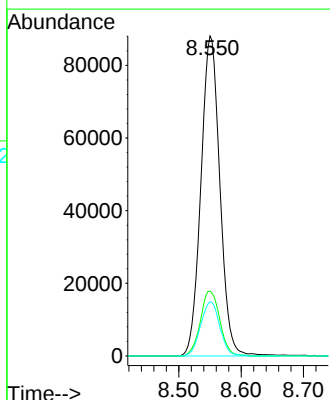
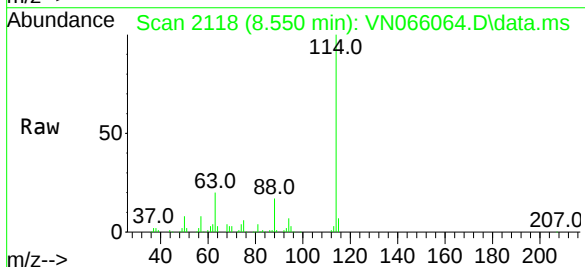


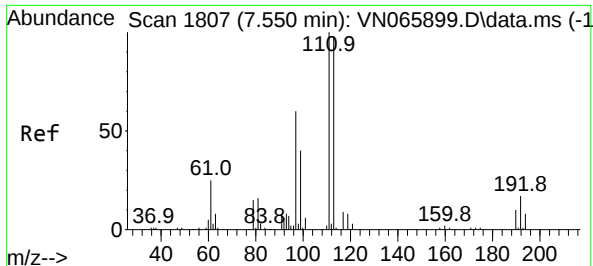

#35
Dibromofluoromethane
Concen: 50.40 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:113 Resp: 58016
Ion Ratio Lower Upper
113 100
111 101.2 82.2 123.2
192 17.9 15.4 23.0

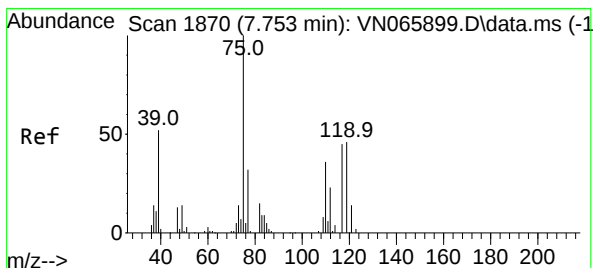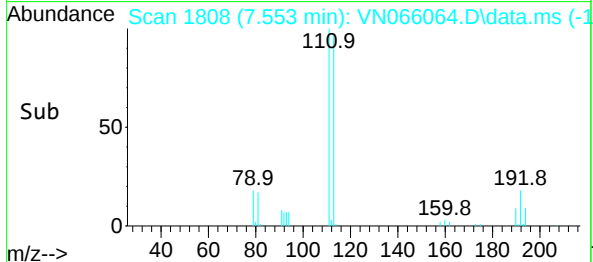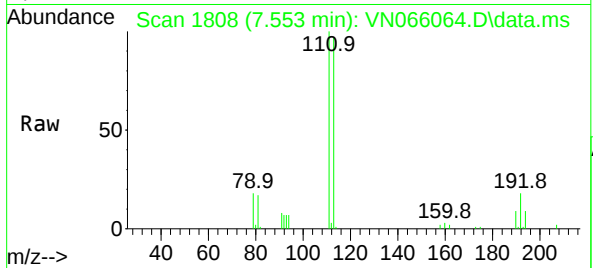

#36
1,1-Dichloropropene
Concen: 4.65 ug/l
RT: 7.630 min Scan# 1832
Delta R.T. -0.123 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 75 Resp: 8526
Ion Ratio Lower Upper
75 100
110 4.6 18.2 54.6#
77 0.0 24.9 37.3#

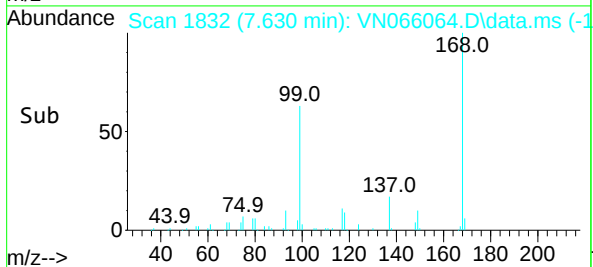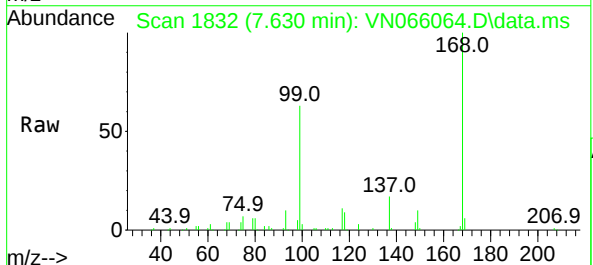

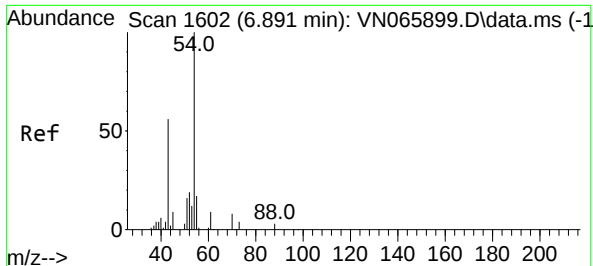

#37

Ethyl Acetate

Concen: 0.68 ug/l

RT: 6.804 min Scan# 1575





Delta R.T. -0.087 min

Lab File: VN066064.D

Acq: 26 Feb 2021 20:16

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE

Tgt Ion: 43	Resp: 1121
Ion Ratio	Lower Upper
43 100	
61 0.0	11.6 17.4#
70 0.0	8.6 13.0#

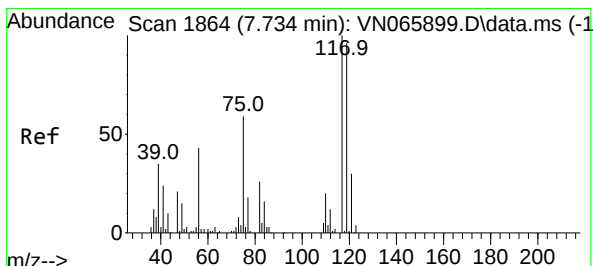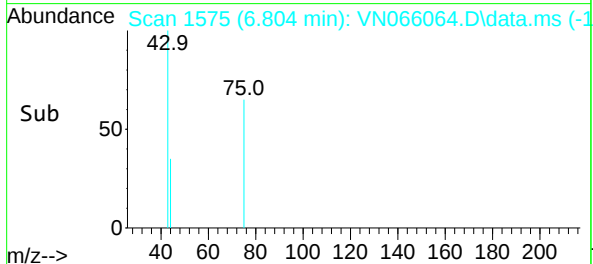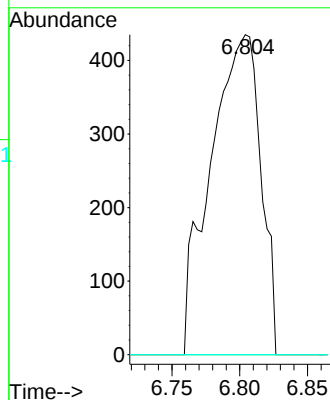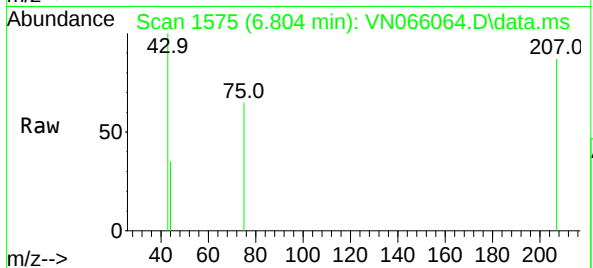

#38

Carbon Tetrachloride

Concen: 6.78 ug/l




RT: 7.630 min Scan# 1832


Delta R.T. -0.104 min

Lab File: VN066064.D

Acq: 26 Feb 2021 20:16


Tgt Ion: 117	Resp: 11558
Ion Ratio	Lower Upper
117 100	
119 4.5	76.0 114.0#
121 0.0	24.5 36.7#

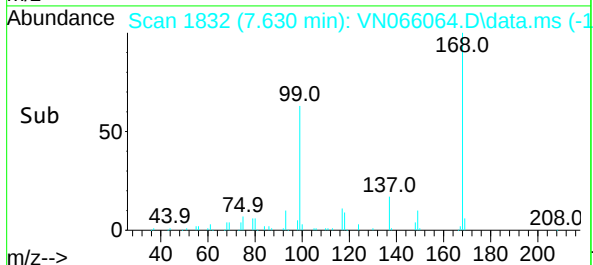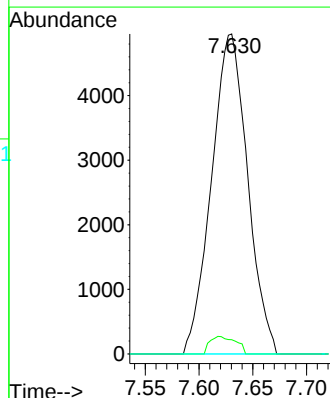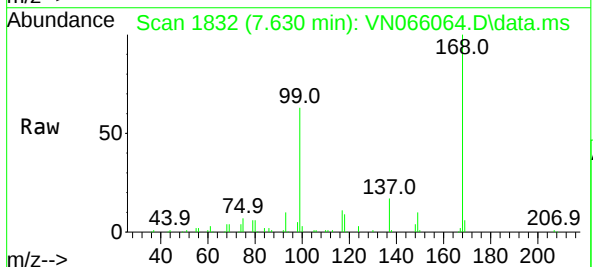






#39
Methylcyclohexane
Concen: 0.53 ug/l
RT: 9.045 min Scan# 2272
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE







Tgt Ion: 83	Resp: 1095
Ion Ratio	Lower Upper
83 100	
55 69.9	58.9 88.3
98 41.7	35.9 53.9

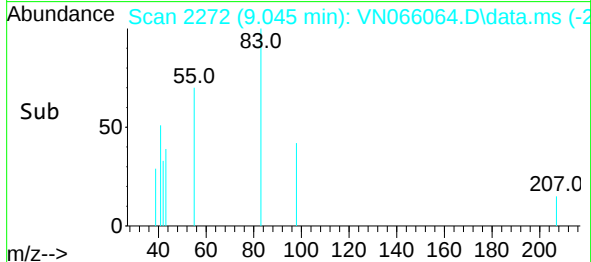

#43
Isopropyl Acetate
Concen: 2.70 ug/l
RT: 8.126 min Scan# 1986
Delta R.T. -0.006 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 43	Resp: 7135
Ion Ratio	Lower Upper
43 100	
61 19.3	22.5 33.7#
87 6.4	11.1 16.7#

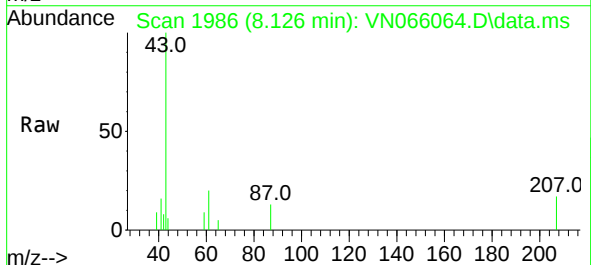



#45

1,2-Dichloropropane

Concen: 0.21 ug/l

RT: 9.228 min Scan# 2329

Delta R.T. 0.144 min

Lab File: VN066064.D





Acq: 26 Feb 2021 20:16

Tgt Ion: 63 Resp: 297

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

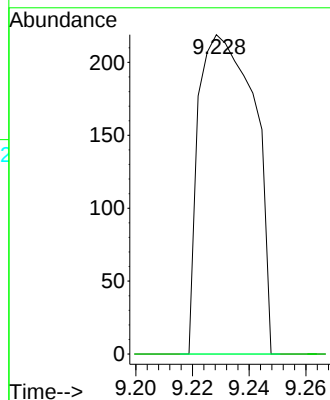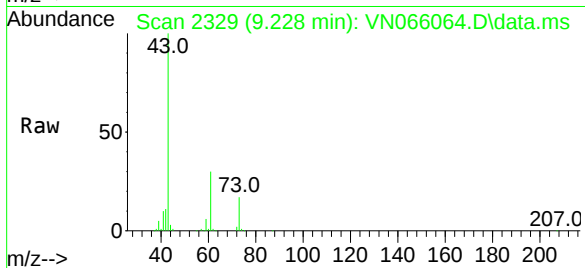

#48

Methyl methacrylate

Concen: 1.26 ug/l

RT: 9.145 min Scan# 2303

Delta R.T. -0.023 min

Lab File: VN066064.D

Acq: 26 Feb 2021 20:16




Tgt Ion: 41 Resp: 1687


Ion Ratio Lower Upper

41 100

69 0.0 75.9 113.9#

39 0.0 46.6 69.8#



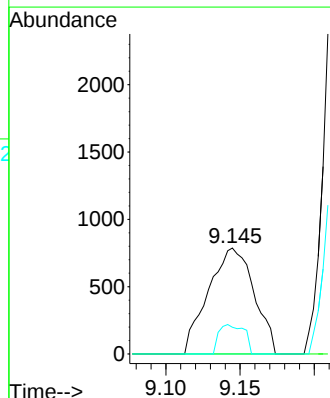
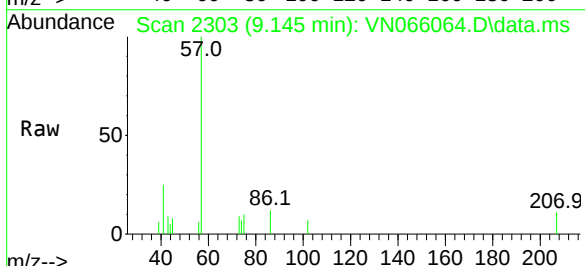




#50
Toluene-d8
Concen: 47.60 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. -0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 98 Resp: 224896
Ion Ratio Lower Upper
98 100
100 66.3 50.5 75.7



#51
4-Methyl-2-Pentanone
Concen: 0.86 ug/l
RT: 9.945 min Scan# 2552
Delta R.T. -0.007 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 43 Resp: 1377
Ion Ratio Lower Upper
43 100
58 33.6 32.5 48.7









#52
Toluene
Concen: 0.25 ug/l
RT: 10.122 min Scan# 2607
Delta R.T. 0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 92 Resp: 878
Ion Ratio Lower Upper
92 100
91 173.8 140.7 211.1



#54
cis-1,3-Dichloropropene
Concen: 5.86 ug/l
RT: 9.871 min Scan# 2529
Delta R.T. 0.064 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 75 Resp: 12985
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#
39 27.8 36.2 54.4#









#55
1,1,2-Trichloroethane
Concen: 0.42 ug/l
RT: 10.508 min Scan# 2727
Delta R.T. -0.023 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 97	Resp:	540
Ion Ratio	Lower	Upper
97	100	
83	0.0	67.7 101.5#
85	0.0	44.5 66.7#
99	0.0	49.4 74.0#

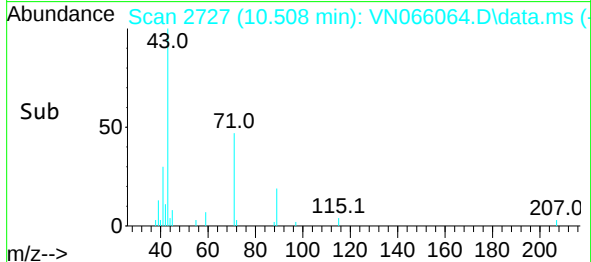

#57
1,3-Dichloropropane
Concen: 2.82 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.057 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 76	Resp:	6430
Ion Ratio	Lower	Upper
76	100	
78	0.0	25.7 38.5#




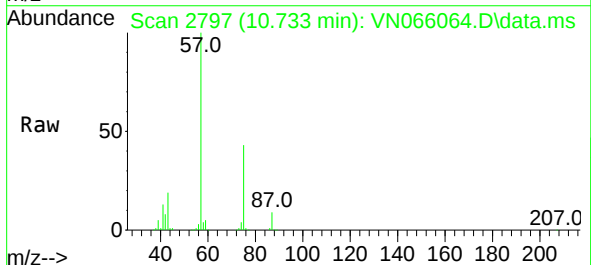


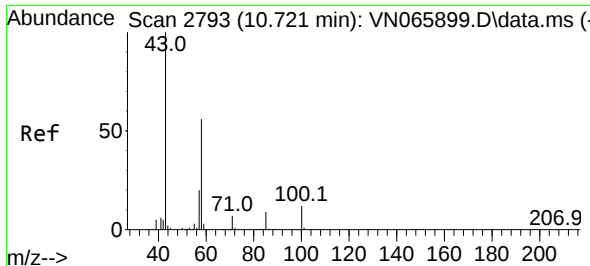

#59
2-Hexanone
Concen: 76.59 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.012 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 43 Resp: 87614
Ion Ratio Lower Upper
43 100
58 19.0 28.1 84.3#

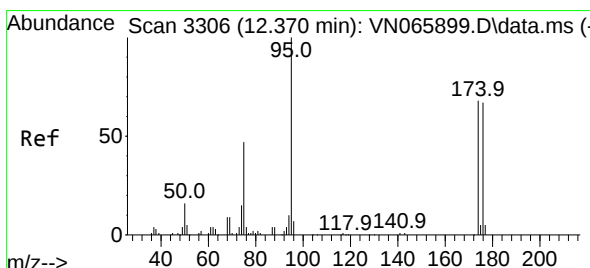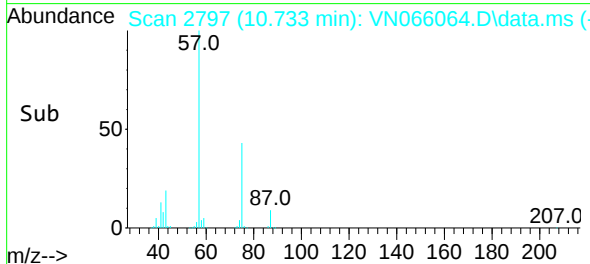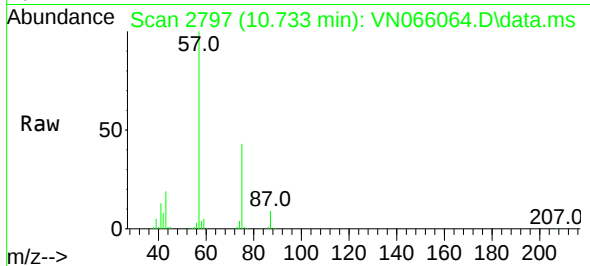

#62
4-Bromofluorobenzene
Concen: 47.99 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 95 Resp: 85118
Ion Ratio Lower Upper
95 100
174 72.4 0.0 169.0
176 68.9 0.0 162.4


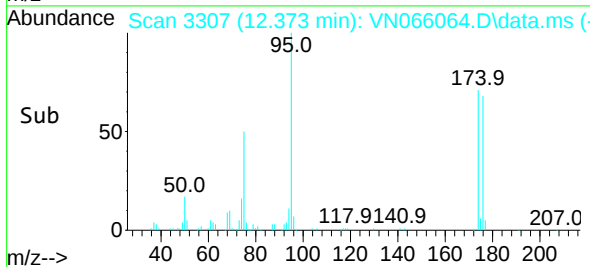

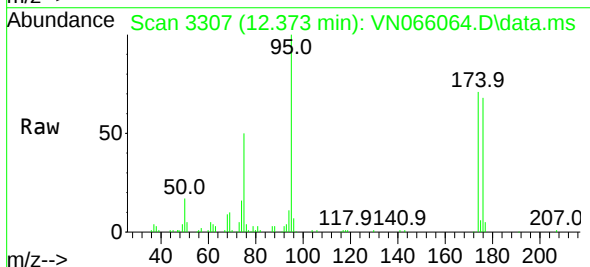


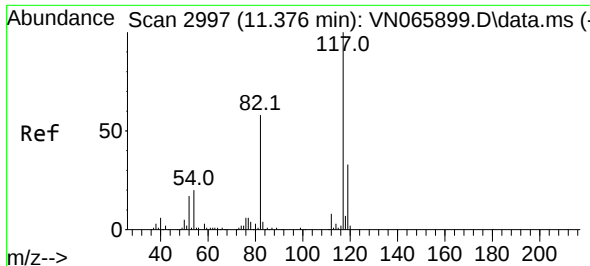

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:117 Resp: 170274
Ion Ratio Lower Upper
117 100
82 57.5 43.7 65.5
119 32.2 26.1 39.1

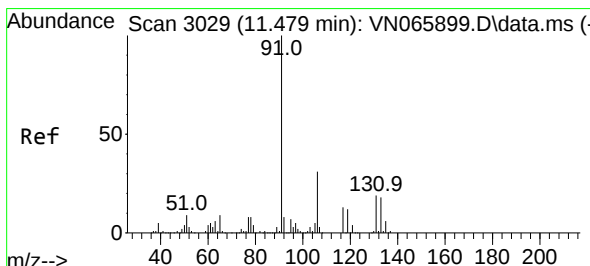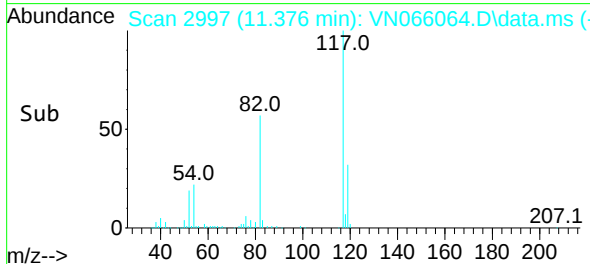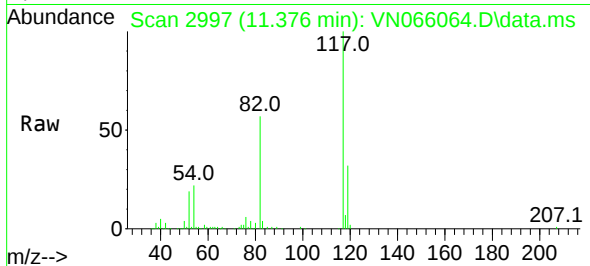

#67
Ethyl Benzene
Concen: 6.10 ug/l
RT: 11.482 min Scan# 3030
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 91 Resp: 39335
Ion Ratio Lower Upper
91 100
106 31.0 25.5 38.3


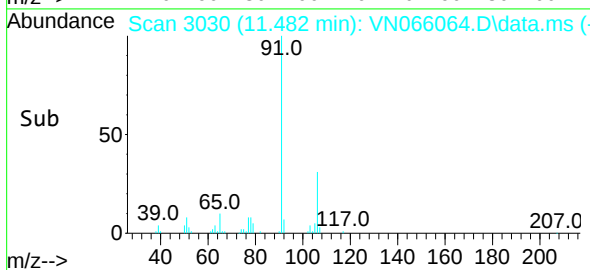

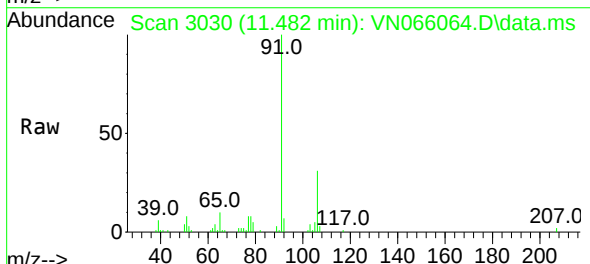




#68
m/p-Xylenes
Concen: 3.83 ug/l
RT: 11.585 min Scan# 3062
Delta R.T. -0.007 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:106 Resp: 9207
Ion Ratio Lower Upper
106 100
91 212.5 161.4 242.0



#69
o-Xylene
Concen: 1.95 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion:106 Resp: 4521
Ion Ratio Lower Upper
106 100
91 232.3 106.8 320.4


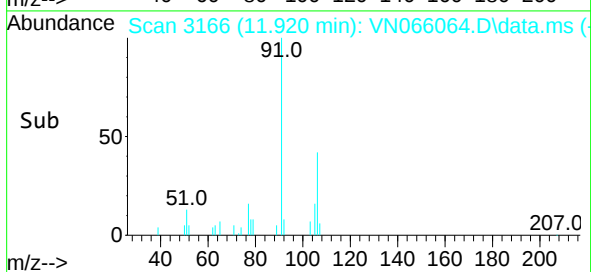




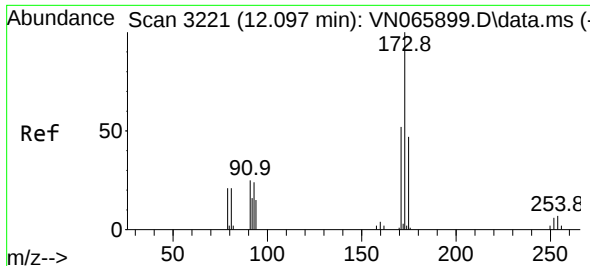

#71
Bromoform
Concen: 2.69 ug/l
RT: 12.379 min Scan# 3309
Delta R.T. 0.282 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:173 Resp: 183
Ion Ratio Lower Upper
173 100
175 2074.9 23.8 71.2#
254 0.0 0.0 0.0

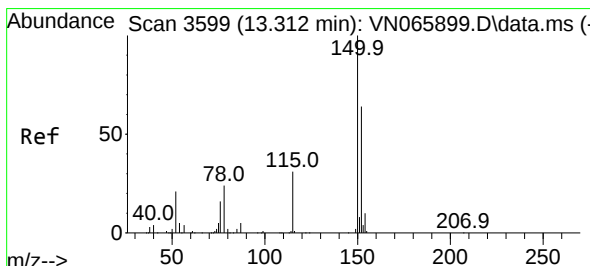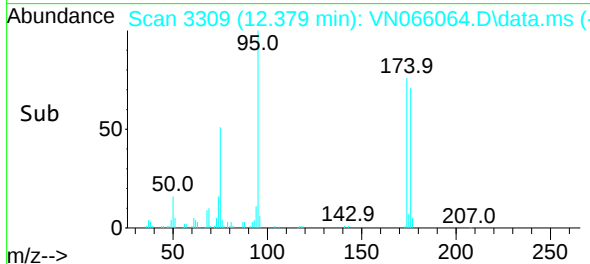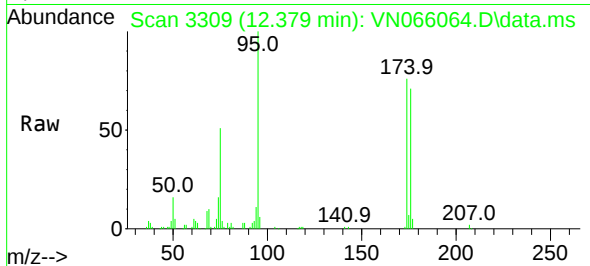

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion:152 Resp: 74267
Ion Ratio Lower Upper
152 100
115 66.3 28.5 85.6
150 157.3 0.0 347.6


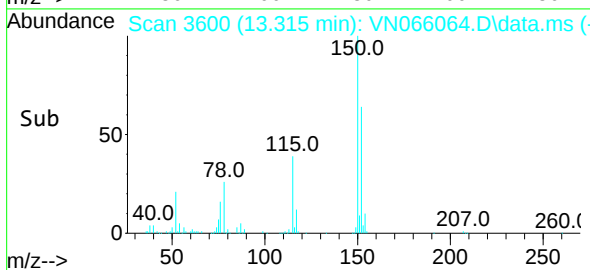

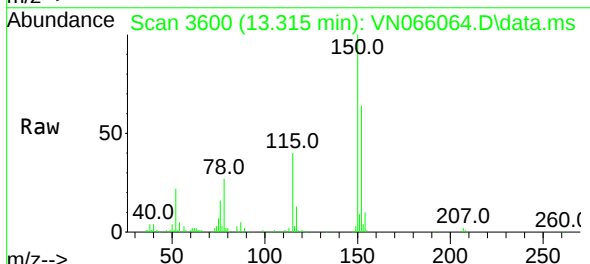




#73
Isopropylbenzene
Concen: 1.36 ug/l
RT: 12.219 min Scan# 3259
Delta R.T. -0.000 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:105 Resp: 8253
Ion Ratio Lower Upper
105 100
120 26.9 13.3 39.9

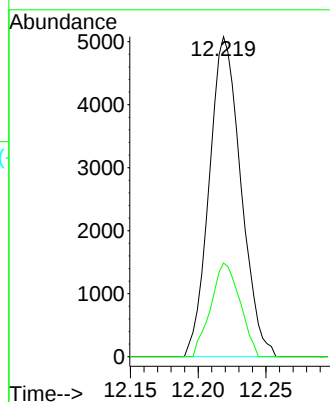

#76
1,2,3-Trichloropropane
Concen: 24.70 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 75 Resp: 44061
Ion Ratio Lower Upper
75 100
77 1.4 0.0 0.0#



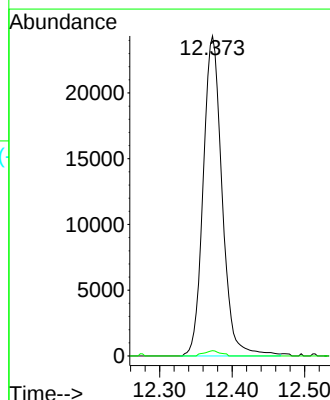
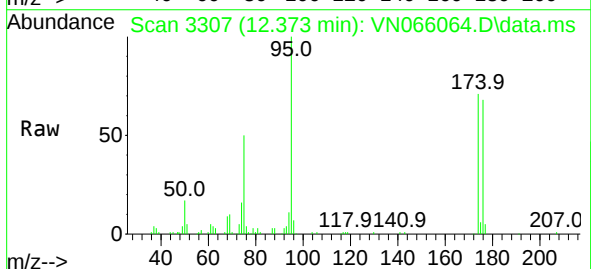




#78
n-propylbenzene
Concen: 1.90 ug/l
RT: 12.563 min Scan# 3366
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 91 Resp: 13091
Ion Ratio Lower Upper
91 100
120 21.1 11.8 35.3



#79
2-Chlorotoluene
Concen: 1.61 ug/l
RT: 12.627 min Scan# 3386
Delta R.T. -0.016 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 91 Resp: 6952
Ion Ratio Lower Upper
91 100
126 0.0 17.4 52.3#









#80
1,3,5-Trimethylbenzene
Concen: 3.44 ug/l
RT: 12.704 min Scan# 3410
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:105 Resp: 17739
Ion Ratio Lower Upper
105 100
120 47.7 24.3 72.8

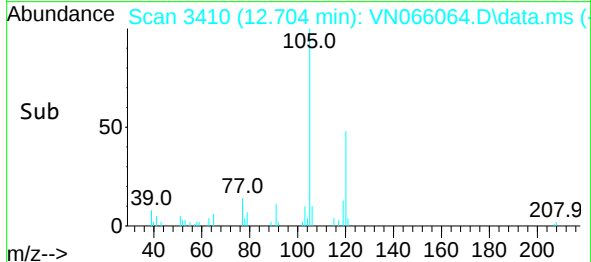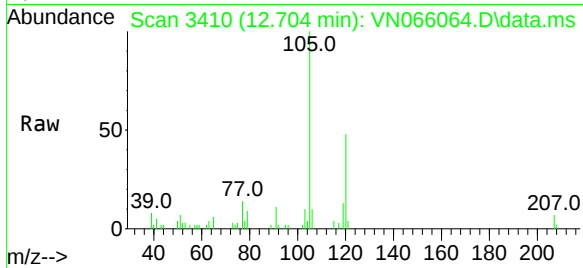

#81
trans-1,4-Dichloro-2-butene
Concen: 78.71 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 75 Resp: 44061
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#




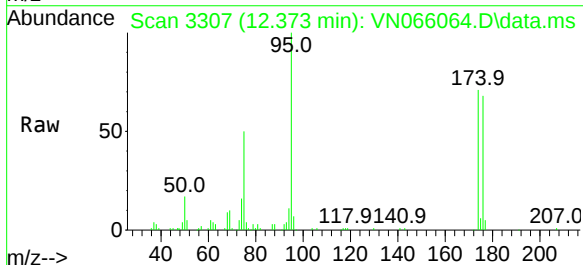




#82
4-Chlorotoluene
Concen: 0.49 ug/l
RT: 12.701 min Scan# 3409
Delta R.T. -0.042 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion: 91 Resp: 2128
Ion Ratio Lower Upper
91 100
126 0.0 17.2 51.6#

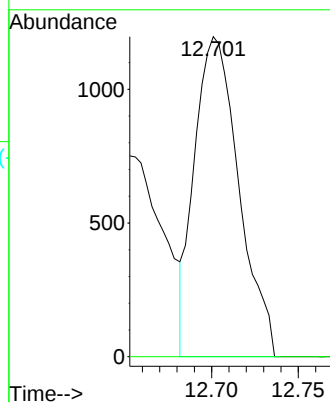

#83
tert-Butylbenzene
Concen: 0.24 ug/l
RT: 12.968 min Scan# 3492
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 119 Resp: 1037
Ion Ratio Lower Upper
119 100
91 52.2 33.0 98.9
134 9.5 12.7 38.1#

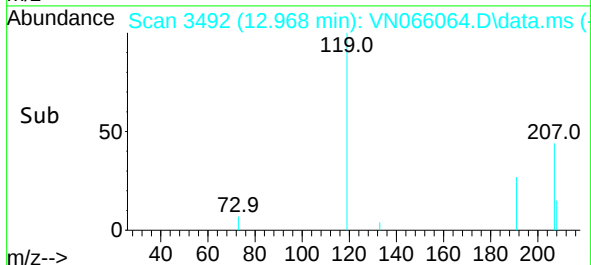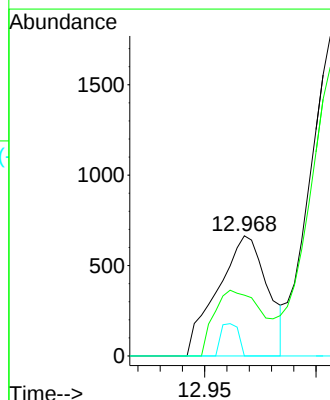



#84

1,2,4-Trimethylbenzene

Concen: 5.48 ug/l

RT: 13.010 min Scan# 3505

Delta R.T. -0.000 min

Lab File: VN066064.D

Acq: 26 Feb 2021 20:16

Tgt Ion:105 Resp: 28320

Ion Ratio Lower Upper

105 100





120 44.2 22.4 67.0

Instrument :

MSVOA_N

ClientSampleId :

SEDGWICK-AVE

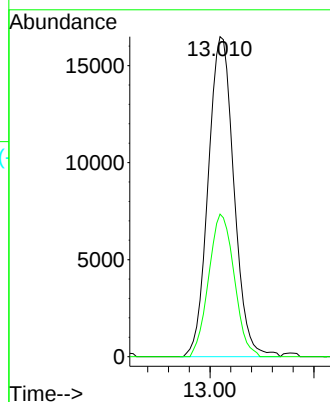

#85

sec-Butylbenzene

Concen: 0.38 ug/l

RT: 13.138 min Scan# 3545

Delta R.T. -0.004 min

Lab File: VN066064.D




Acq: 26 Feb 2021 20:16


Tgt Ion:105 Resp: 2095

Ion Ratio Lower Upper

105 100

134 21.3 10.0 30.0



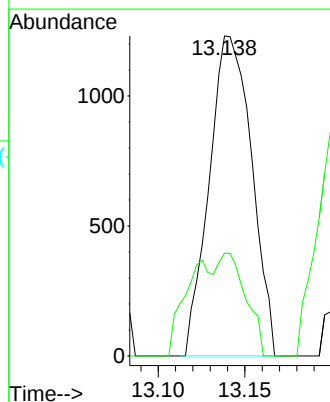



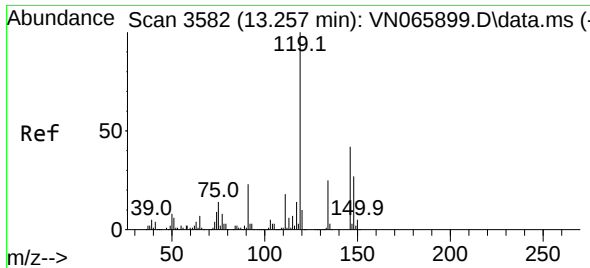

#86
p-Isopropyltoluene
Concen: 0.56 ug/l
RT: 13.260 min Scan# 3583
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:	119	Resp:	2792
Ion	Ratio	Lower	Upper
119	100		
134	22.8	13.3	39.8
91	32.2	11.8	35.3

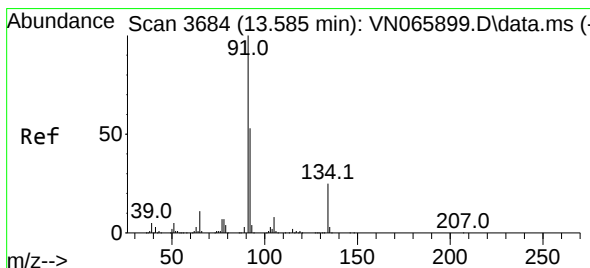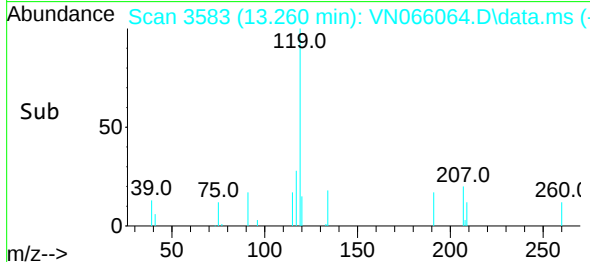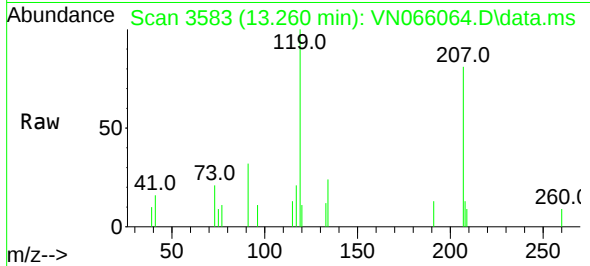

#89
n-Butylbenzene
Concen: 0.31 ug/l
RT: 13.553 min Scan# 3674
Delta R.T. -0.032 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion:	91	Resp:	1302
Ion	Ratio	Lower	Upper
91	100		
92	0.0	26.1	78.3#
134	441.5	13.0	38.9#


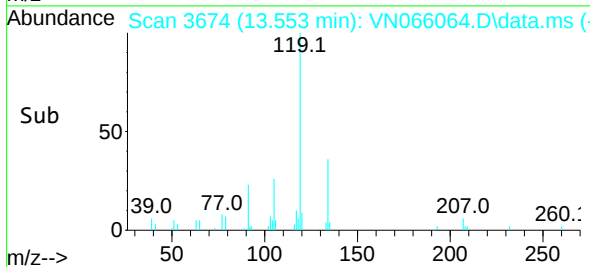

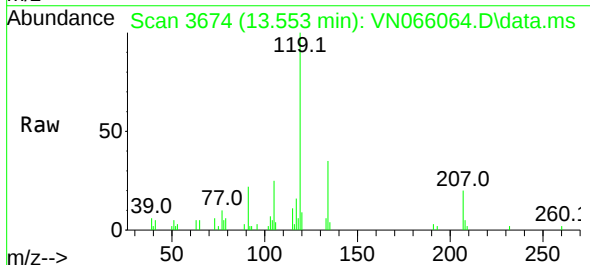




#90
Hexachloroethane
Concen: 3.58 ug/l
RT: 13.858 min Scan# 3769
Delta R.T. 0.015 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16




Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE


Tgt Ion:117 Resp: 3039
Ion Ratio Lower Upper
117 100
201 0.0 37.8 113.3#



#92
1,2-Dibromo-3-Chloropropane
Concen: 1.28 ug/l
RT: 14.251 min Scan# 3891
Delta R.T. 0.013 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Tgt Ion: 75 Resp: 155
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#



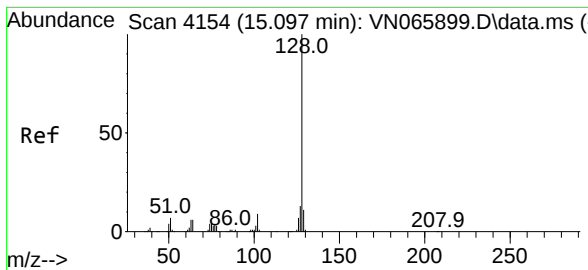

#95
Naphthalene
Concen: 18.66 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. 0.003 min
Lab File: VN066064.D
Acq: 26 Feb 2021 20:16

Instrument :
MSVOA_N
ClientSampleId :
SEDGWICK-AVE

Tgt Ion:	128	Resp:	71587
Ion	Ratio	Lower	Upper
128	100		
127	12.6	10.2	15.2
129	10.7	8.6	13.0

