
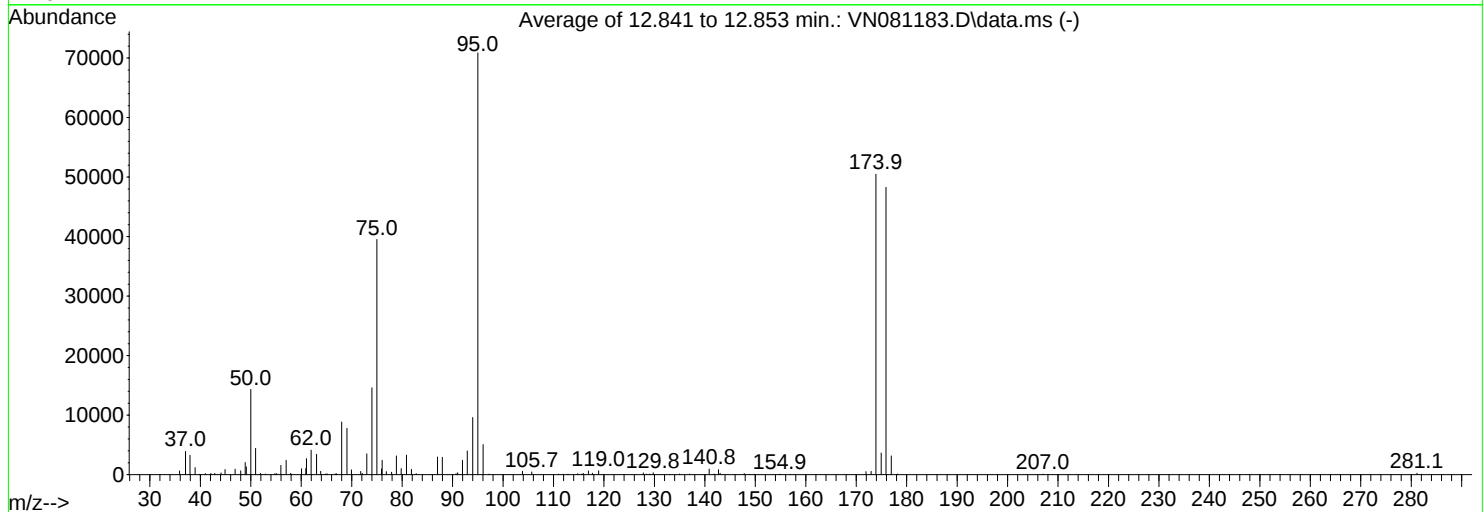


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022624\
Data File : VN081183.D
Acq On : 26 Feb 2024 08:27
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

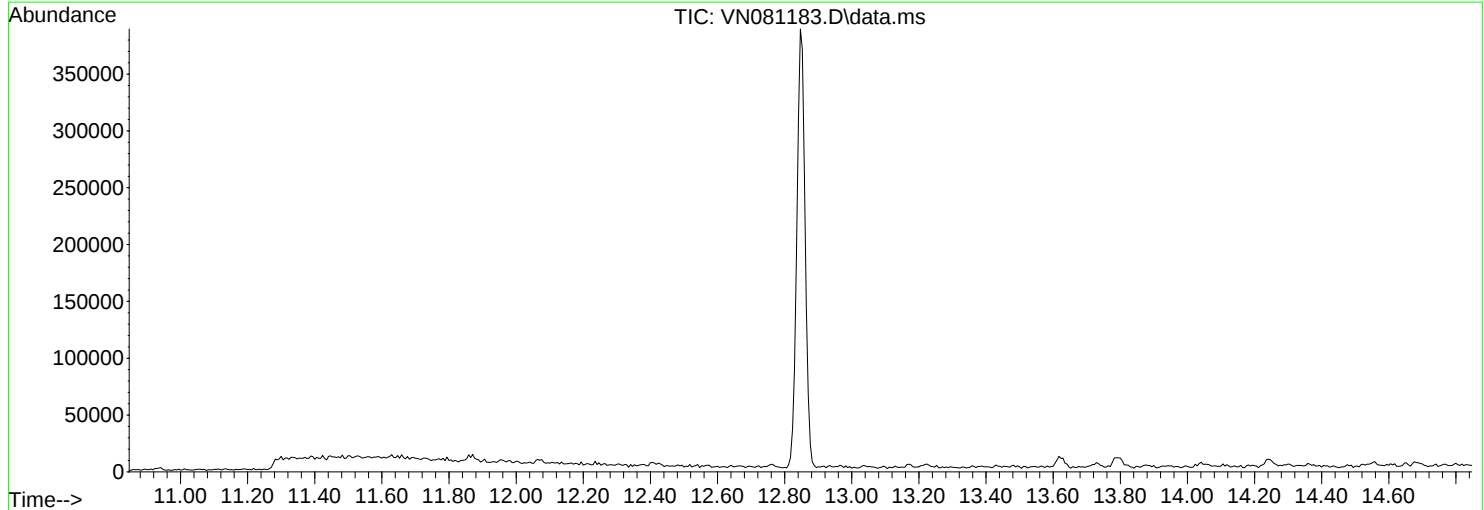

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.2	14322	PASS
75	95	30	60	55.8	39515	PASS
95	95	100	100	100.0	70875	PASS
96	95	5	9	7.2	5069	PASS
173	174	0.00	2	1.1	575	PASS
174	95	50	100	71.2	50488	PASS
175	174	5	9	7.2	3636	PASS
176	174	95	101	95.6	48288	PASS
177	176	5	9	6.5	3144	PASS

Average of 12.841 to 12.853 min.: VN081183.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	613	48.00	645	57.90	217	66.75	121
37.05	3903	48.90	2045	58.10	92	67.00	15
37.95	3251	49.10	1321	60.05	1003	68.00	883
38.95	1189	50.00	14322	60.90	1023	69.05	778
39.80	56	50.95	4423	61.05	2700	69.95	813
41.00	178	51.90	207	61.95	4122	71.80	539
42.10	211	52.90	107	63.05	3431	72.10	203
42.85	224	54.80	188	63.85	556	73.00	3495
44.10	299	55.15	194	64.70	50	74.00	14598
44.90	850	55.95	1573	64.90	127	75.00	39515
46.90	922	57.00	2422	65.20	116	75.90	982

Average of 12.841 to 12.853 min.: VN081183.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
76.05	2413	91.00	319	112.80	55	129.75	333
76.85	513	91.95	2410	113.00	62	133.00	50
77.90	410	92.90	3992	114.80	168	135.00	119
78.85	3140	94.00	9603	115.60	97	136.95	121
79.80	1023	95.00	70875	115.90	217	140.85	937
80.85	3276	96.05	5069	116.90	627	141.80	116
81.85	887	97.20	80	117.70	259	142.70	833
82.80	171	103.85	575	118.95	655	143.00	235
87.00	2959	105.70	470	127.80	303	147.80	177
87.95	2906	111.00	80	128.50	79	148.90	64
90.70	159	111.90	87	129.10	100	149.90	78

Average of 12.841 to 12.853 min.: VN081183.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
154.90	74	282.00	84				
156.90	62						
171.95	504						
172.95	575						
173.90	50488						
174.95	3636						
175.90	48288						
176.95	3144						
178.15	121						
207.00	75						
281.15	240						

Instrument :

MSVOA_N

ClientSampleId :

BFB