

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022625\
 Data File : VN085864.D
 Acq On : 26 Feb 2025 12:09
 Operator : JC\MD
 Sample : VN0226WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0226WBL01

Quant Time: Feb 26 22:51:25 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	270093	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	493199	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	432412	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	165756	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	186374	53.224	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	106.440%
35) Dibromofluoromethane	8.165	113	162991	50.505	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	101.000%
50) Toluene-d8	10.565	98	543688	46.304	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.600%
62) 4-Bromofluorobenzene	12.847	95	175574	45.384	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	90.760%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022625\
Data File : VN085864.D
Acq On : 26 Feb 2025 12:09
Operator : JC\MD
Sample : VN0226WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0226WBL01

Quant Time: Feb 26 22:51:25 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




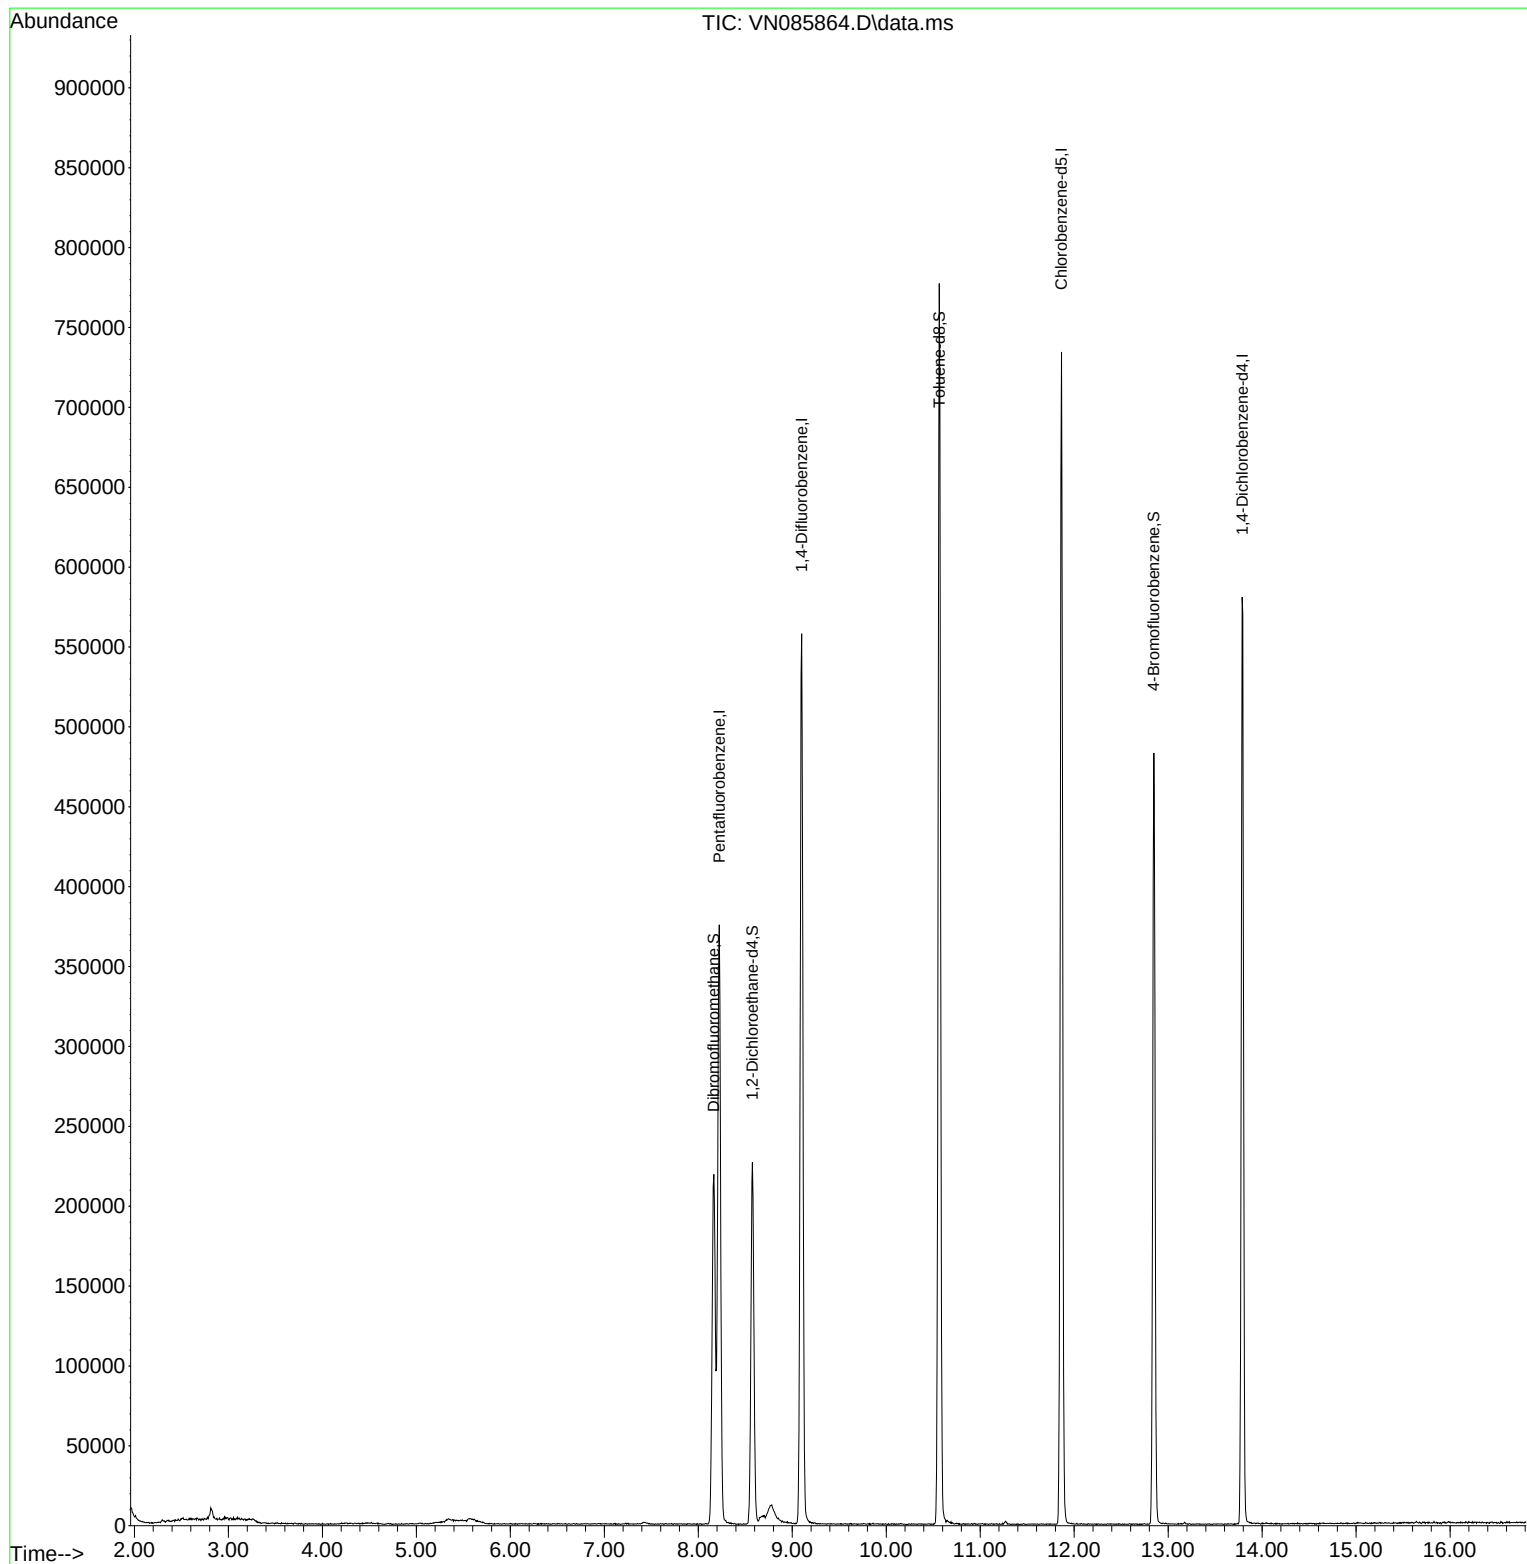


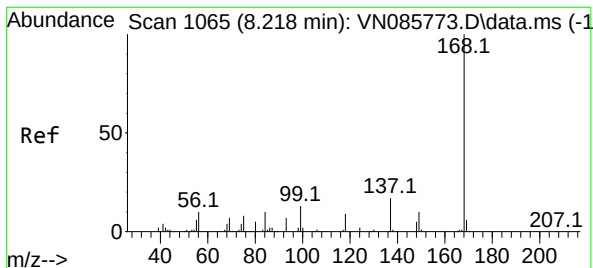

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1106
Delta R.T. 0.006 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0226WBL01


Tgt Ion:168 Resp: 270093
Ion Ratio Lower Upper
168 100
99 59.9 47.9 71.9

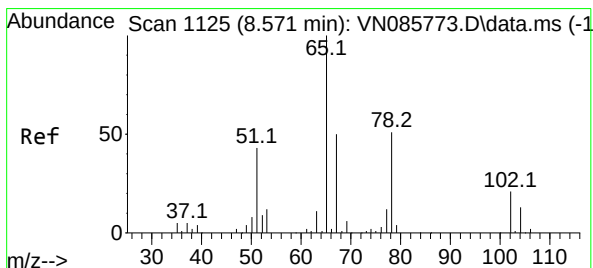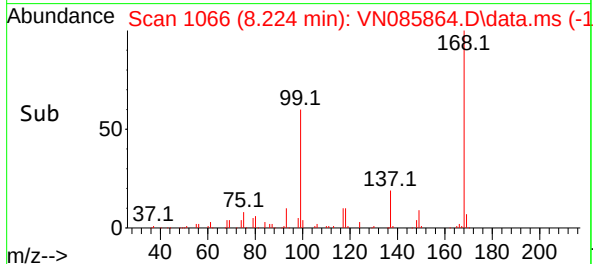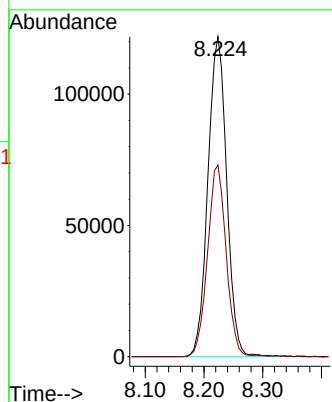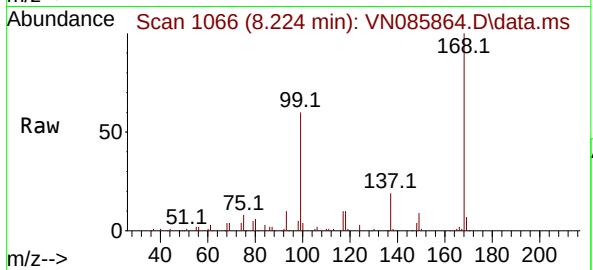

#33
1,2-Dichloroethane-d4
Concen: 53.224 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09

Tgt Ion: 65 Resp: 186374
Ion Ratio Lower Upper
65 100
67 52.6 0.0 106.2

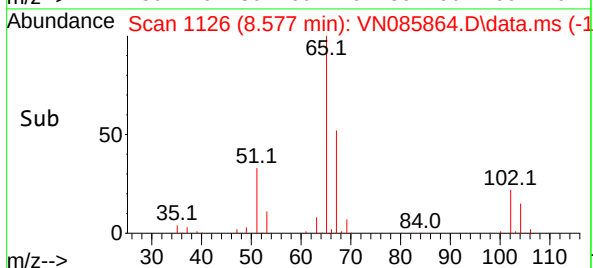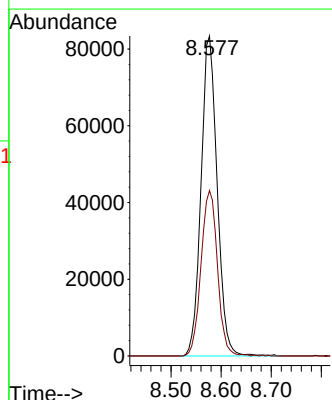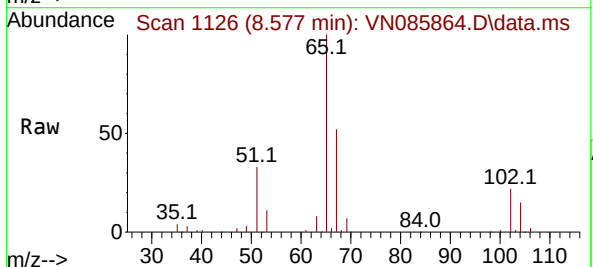

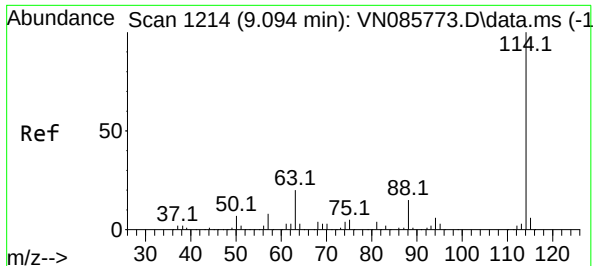

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085864.D

Acq: 26 Feb 2025 12:09

Instrument :

MSVOA_N

ClientSampleId :

VN0226WBL01





Tgt Ion:114 Resp: 493199

Ion Ratio Lower Upper

114 100

63 20.3 0.0 39.2

88 16.6 0.0 30.0

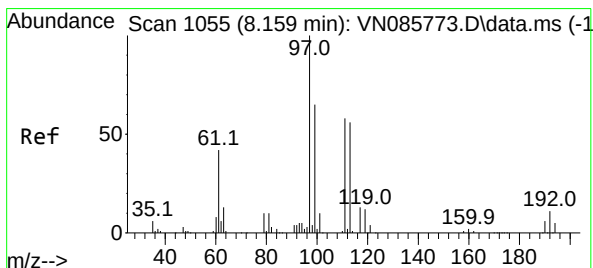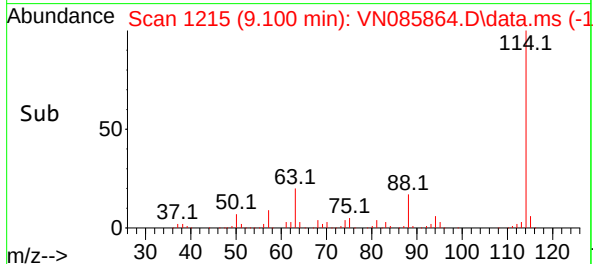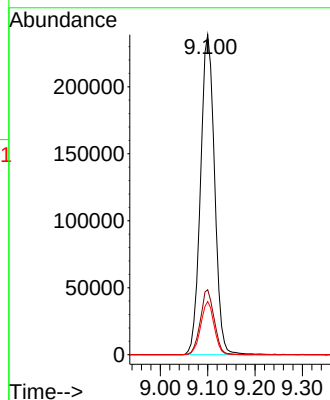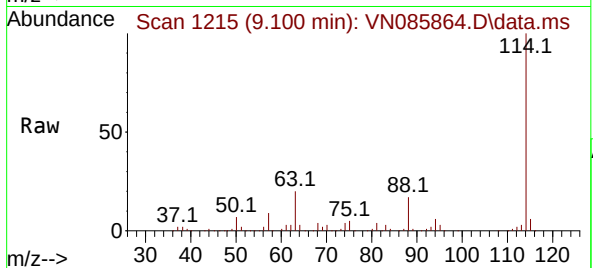

#35

Dibromofluoromethane

Concen: 50.505 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085864.D

Acq: 26 Feb 2025 12:09




Tgt Ion:113 Resp: 162991


Ion Ratio Lower Upper

113 100

111 103.6 82.2 123.4

192 18.8 14.7 22.1


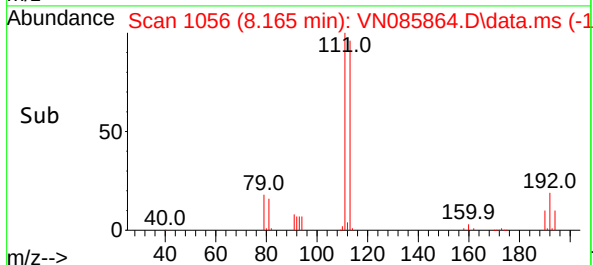
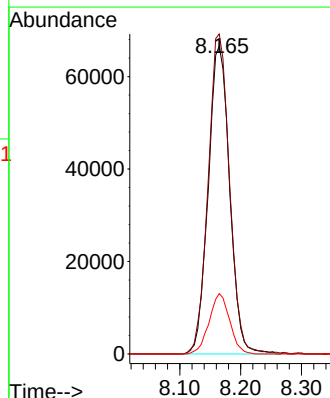
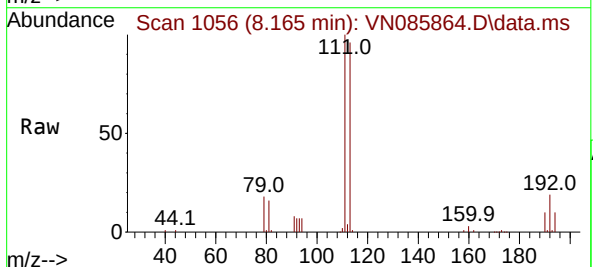


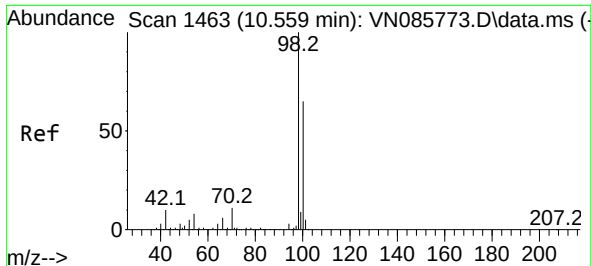

#50
Toluene-d8
Concen: 46.304 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09




Instrument :
MSVOA_N
ClientSampleId :
VN0226WBL01


Tgt Ion: 98 Resp: 543688
Ion Ratio Lower Upper
98 100
100 65.0 52.1 78.1

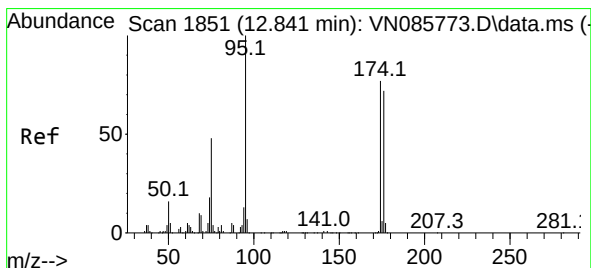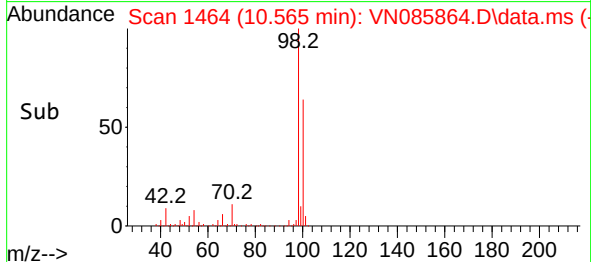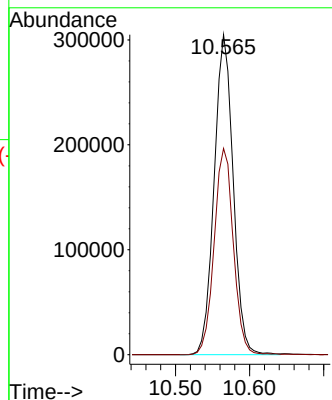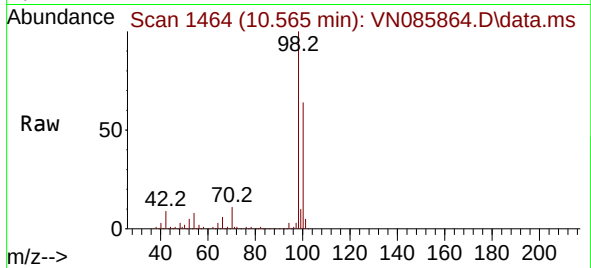

#62
4-Bromofluorobenzene
Concen: 45.384 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.006 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09

Tgt Ion: 95 Resp: 175574
Ion Ratio Lower Upper
95 100
174 78.8 0.0 152.4
176 73.7 0.0 146.6


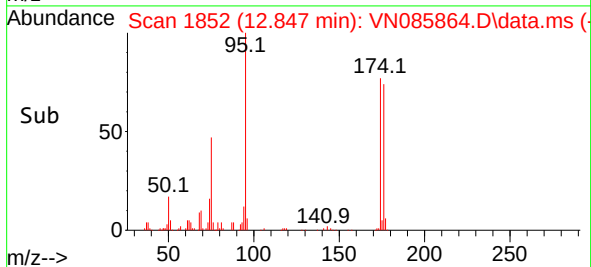
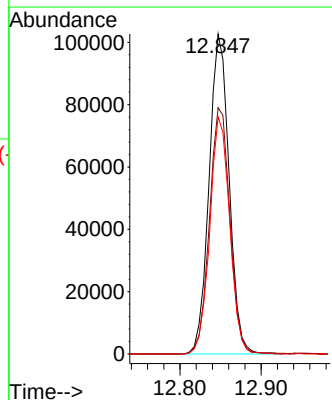
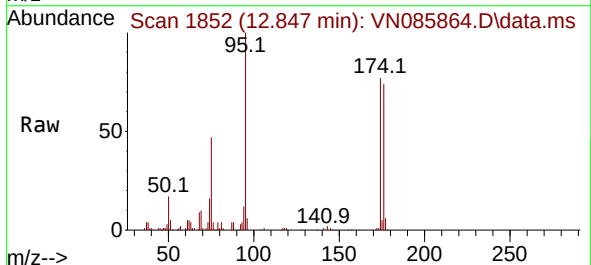


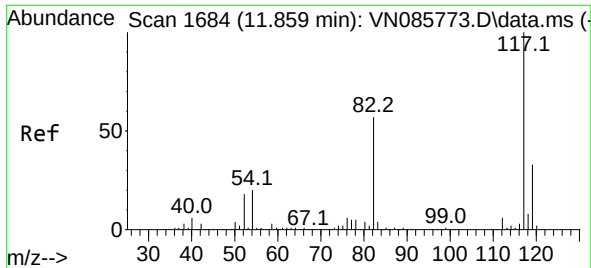

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09

Instrument :
MSVOA_N
ClientSampleId :
VN0226WBL01

Tgt Ion:117 Resp: 432412
Ion Ratio Lower Upper
117 100
82 54.6 45.7 68.5
119 31.6 26.2 39.2

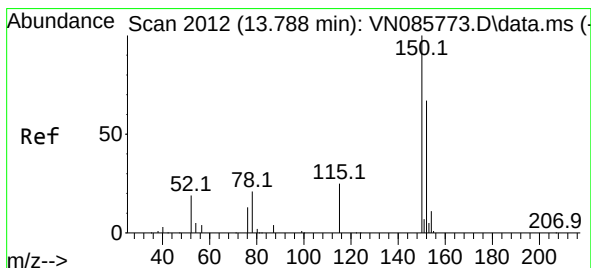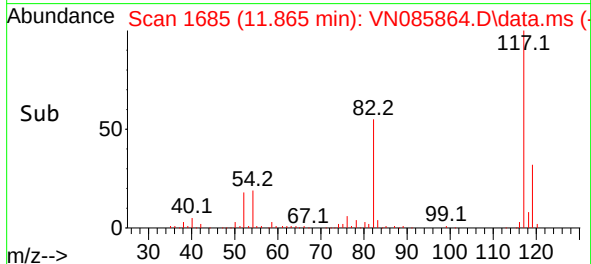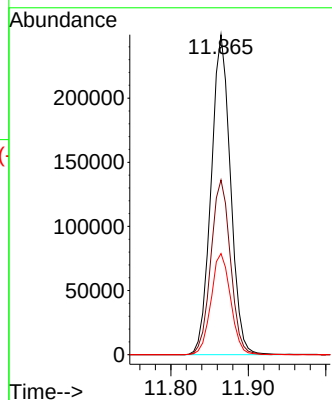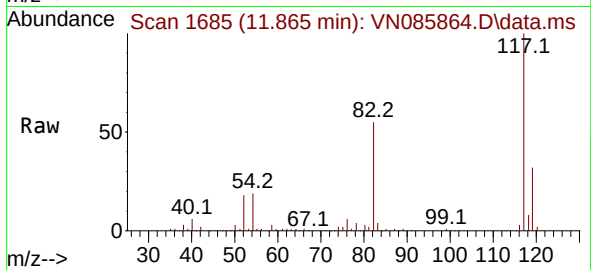

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN085864.D
Acq: 26 Feb 2025 12:09

Tgt Ion:152 Resp: 165756
Ion Ratio Lower Upper
152 100
115 59.8 30.4 91.3
150 157.7 0.0 345.4

