

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022625\
 Data File : VN085869.D
 Acq On : 26 Feb 2025 14:20
 Operator : JC\MD
 Sample : Q1421-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 P001-CLAY-CF01-01

Quant Time: Feb 26 23:00:15 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	266570	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	497524	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	429240	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	167346	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	182347	52.763	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	105.520%
35) Dibromofluoromethane	8.165	113	160657	49.349	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	98.700%
50) Toluene-d8	10.565	98	545079	46.019	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	92.040%
62) 4-Bromofluorobenzene	12.847	95	179218	45.923	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	=	91.840%
Target Compounds						
						Qvalue
16) Acetone	4.430	43	42483	38.849	ug/l	93
20) Methylene Chloride	5.277	84	8227	2.339	ug/l	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022625\
Data File : VN085869.D
Acq On : 26 Feb 2025 14:20
Operator : JC\MD
Sample : Q1421-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
P001-CLAY-CF01-01

Quant Time: Feb 26 23:00:15 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




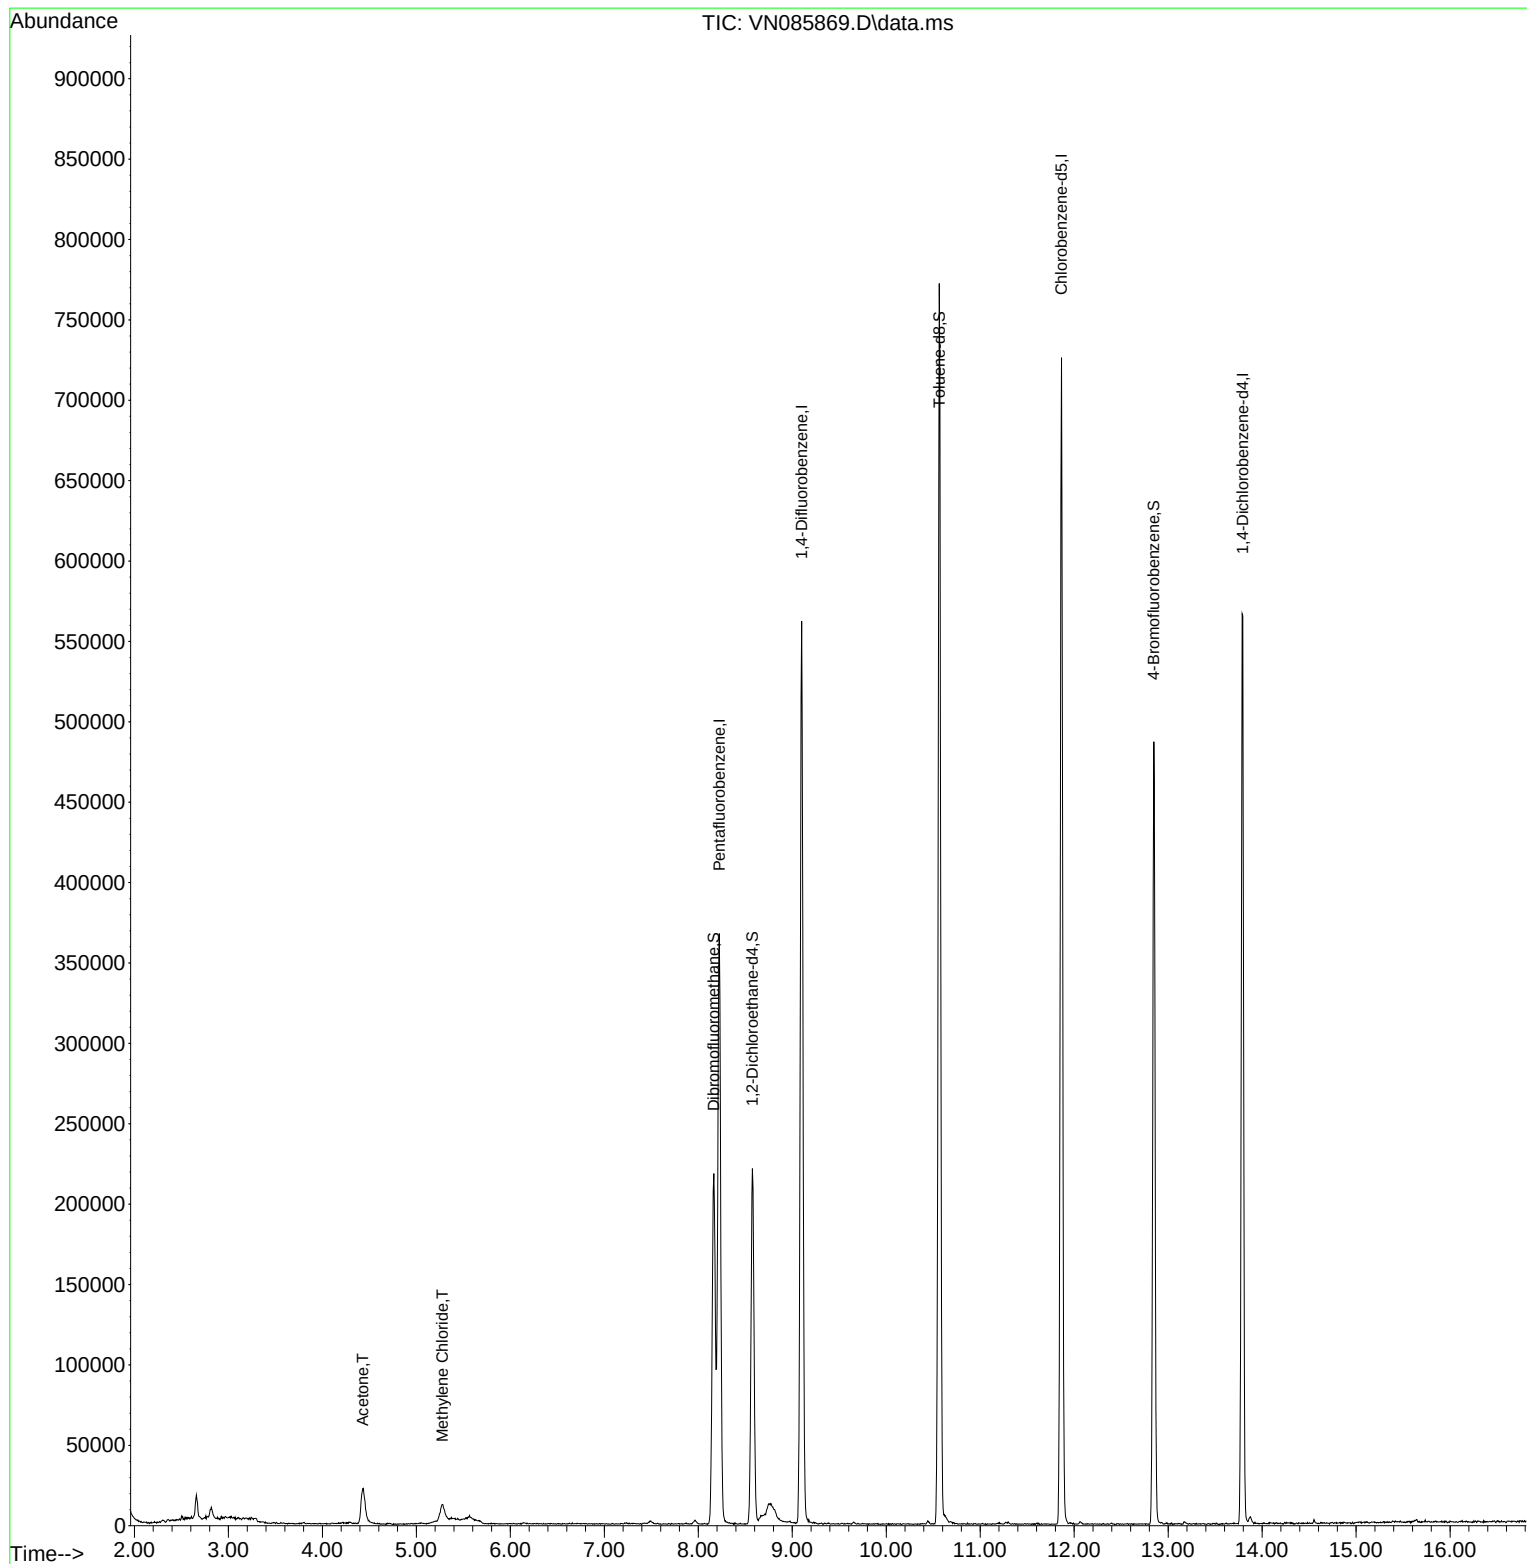


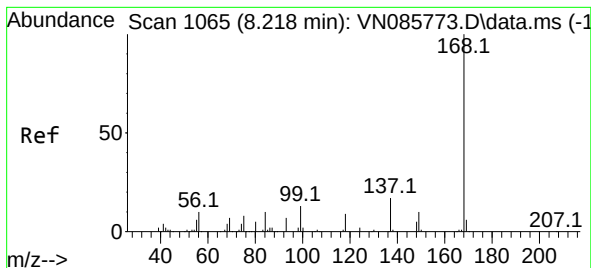

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20




Instrument :
MSVOA_N
ClientSampleId :
P001-CLAY-CF01-01


Tgt Ion:168 Resp: 266570
Ion Ratio Lower Upper
168 100
99 59.8 47.9 71.9

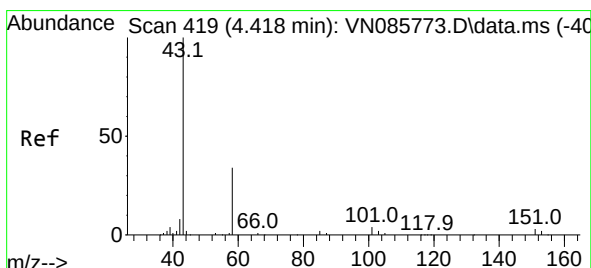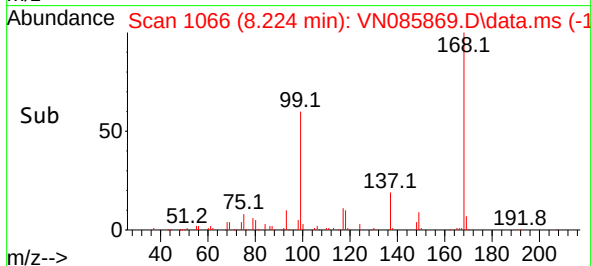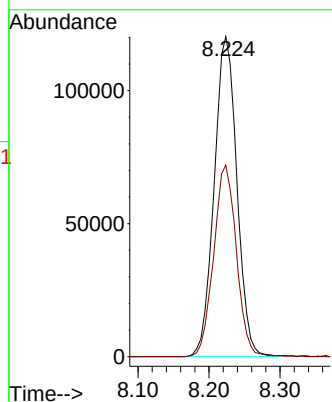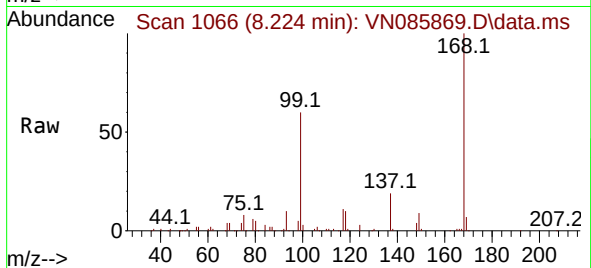

#16
Acetone
Concen: 38.849 ug/l
RT: 4.430 min Scan# 421
Delta R.T. 0.012 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20

Tgt Ion: 43 Resp: 42483
Ion Ratio Lower Upper
43 100
58 38.6 27.5 41.3


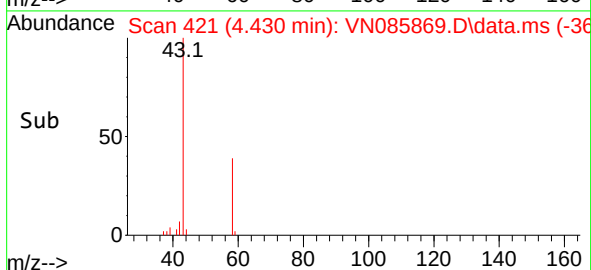
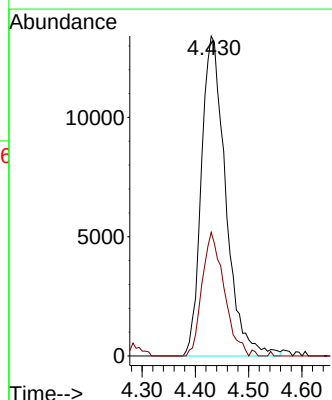
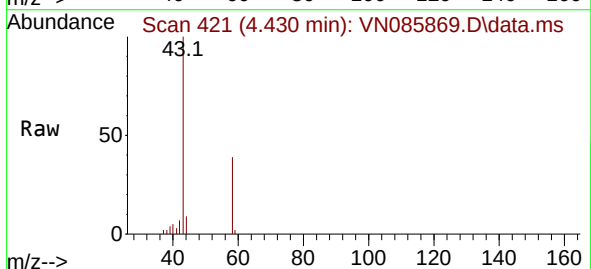


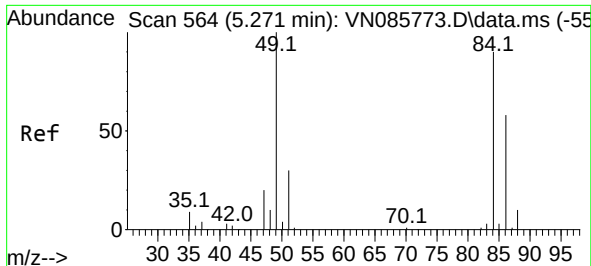

#20
Methylene Chloride
Concen: 2.339 ug/l
RT: 5.277 min Scan# 51
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20




Instrument :
MSVOA_N
ClientSampleId :
P001-CLAY-CF01-01


Tgt Ion: 84	Resp: 8227
Ion Ratio	Lower Upper
84 100	
49 103.4	88.4 132.6
51 28.1	26.6 40.0
86 73.7	51.0 76.6

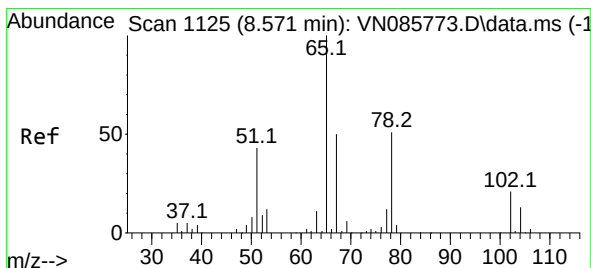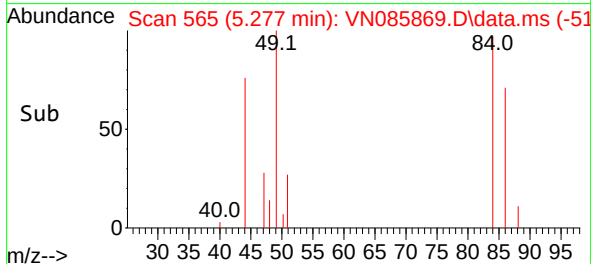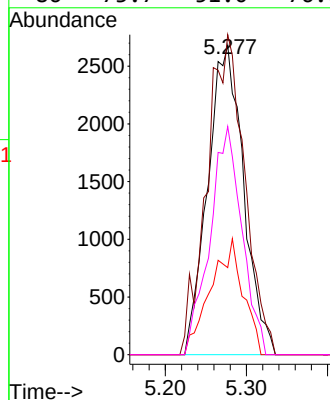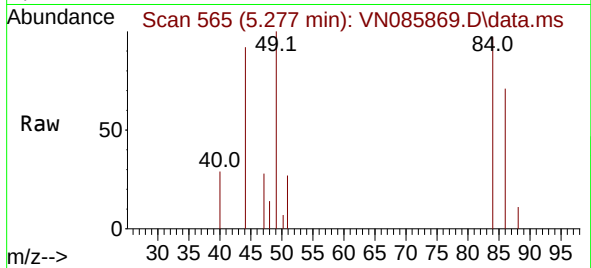

#33
1,2-Dichloroethane-d4
Concen: 52.763 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20

Tgt Ion: 65	Resp: 182347
Ion Ratio	Lower Upper
65 100	
67 52.4	0.0 106.2

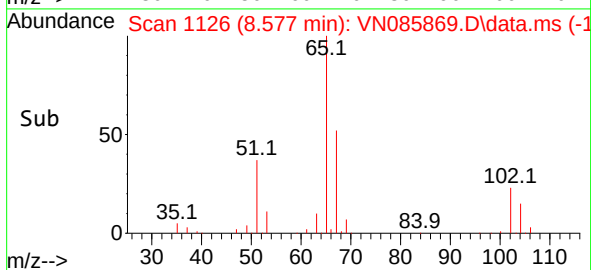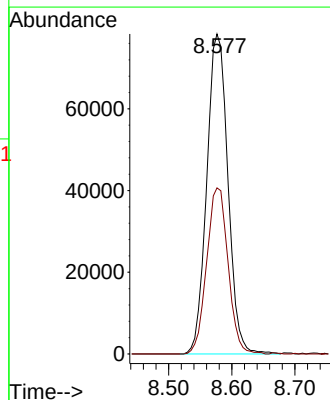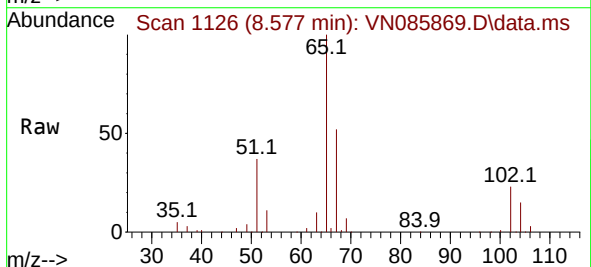

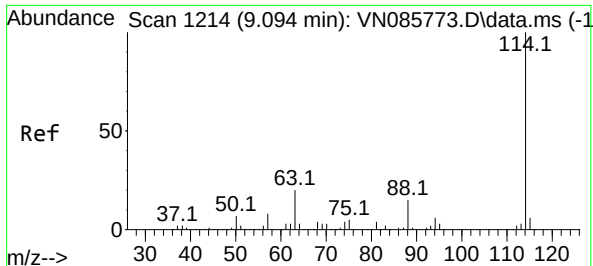

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 11

Delta R.T. 0.006 min

Lab File: VN085869.D

Acq: 26 Feb 2025 14:20

Instrument :

MSVOA_N

ClientSampleId :

P001-CLAY-CF01-01





Tgt Ion:114 Resp: 497524

Ion Ratio Lower Upper

114 100

63 19.3 0.0 39.2

88 16.4 0.0 30.0

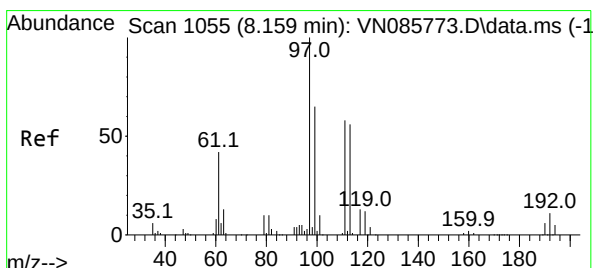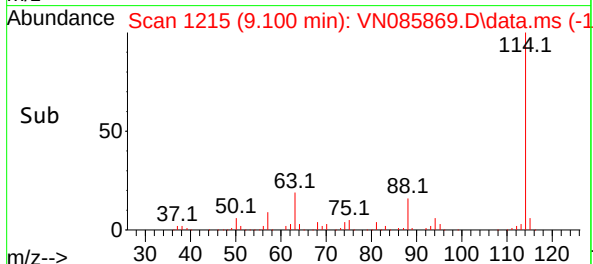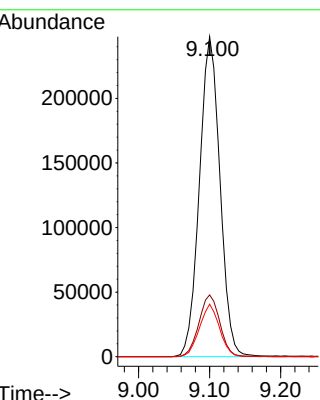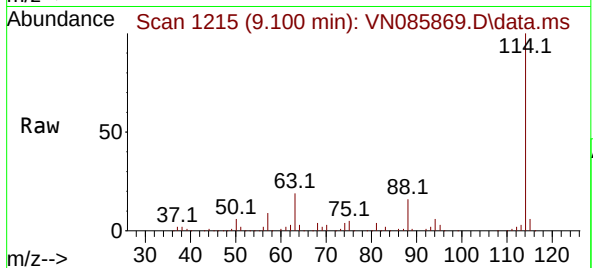

#35

Dibromofluoromethane

Concen: 49.349 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085869.D

Acq: 26 Feb 2025 14:20




Tgt Ion:113 Resp: 160657


Ion Ratio Lower Upper

113 100

111 104.4 82.2 123.4

192 19.4 14.7 22.1


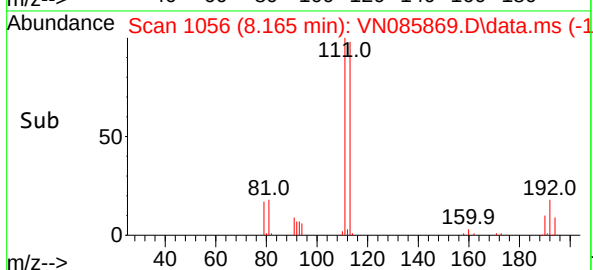
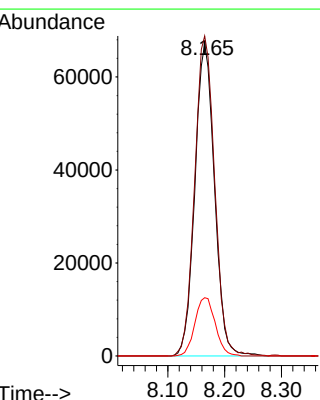
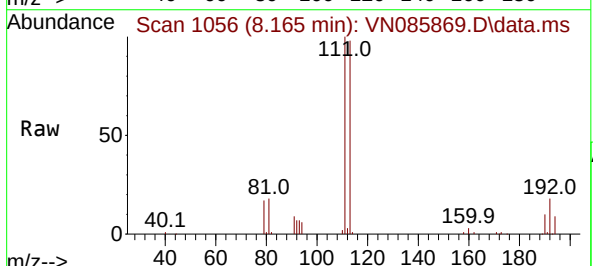


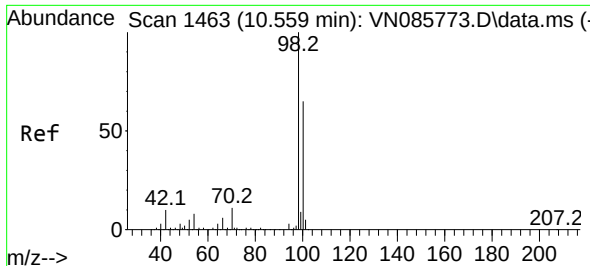

#50
Toluene-d8
Concen: 46.019 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20




Instrument :
MSVOA_N
ClientSampleId :
P001-CLAY-CF01-01


Tgt Ion: 98 Resp: 545079
Ion Ratio Lower Upper
98 100
100 63.9 52.1 78.1

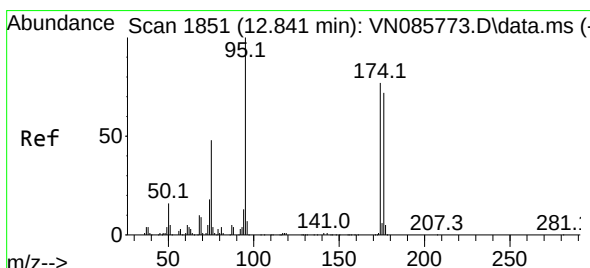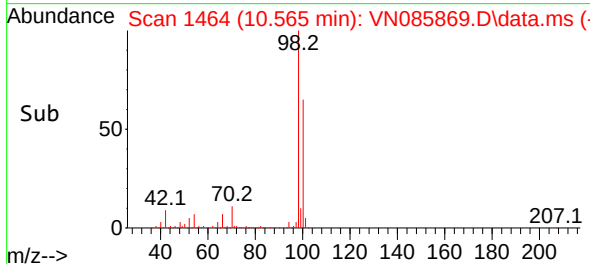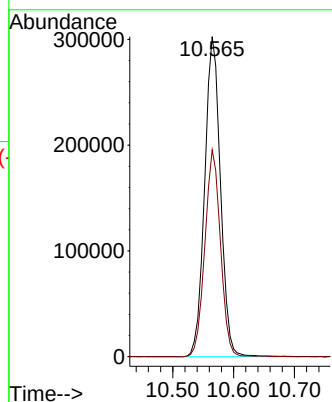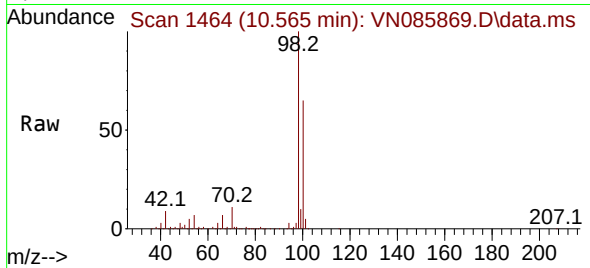

#62
4-Bromofluorobenzene
Concen: 45.923 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20

Tgt Ion: 95 Resp: 179218
Ion Ratio Lower Upper
95 100
174 76.6 0.0 152.4
176 73.0 0.0 146.6


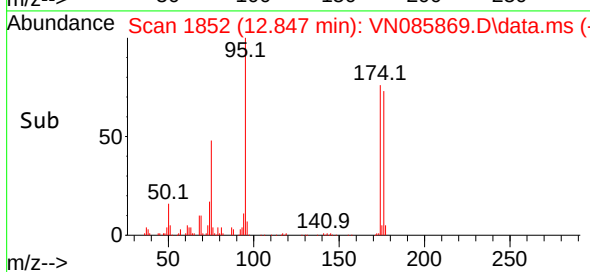
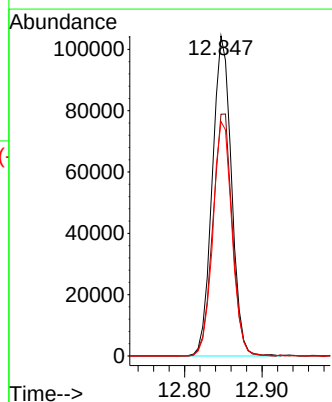
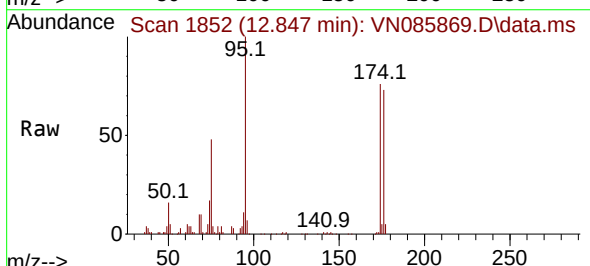


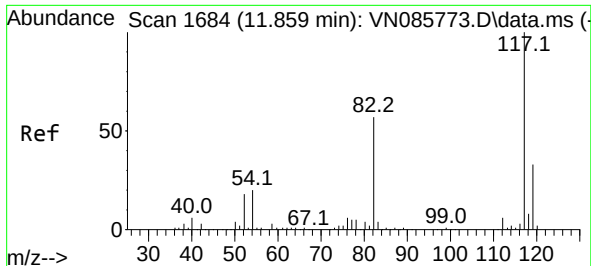

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20

Instrument :
MSVOA_N
ClientSampleId :
P001-CLAY-CF01-01

Tgt Ion:117 Resp: 429240
Ion Ratio Lower Upper
117 100
82 56.1 45.7 68.5
119 32.5 26.2 39.2

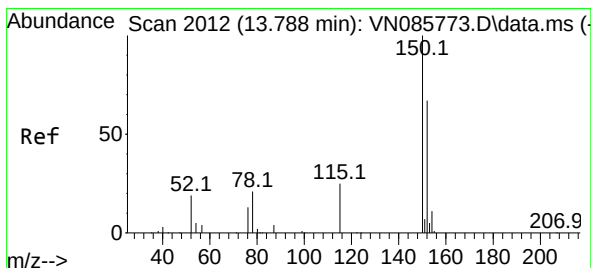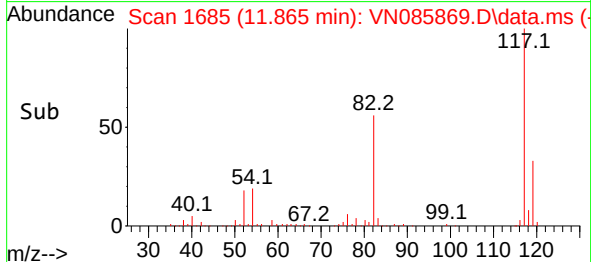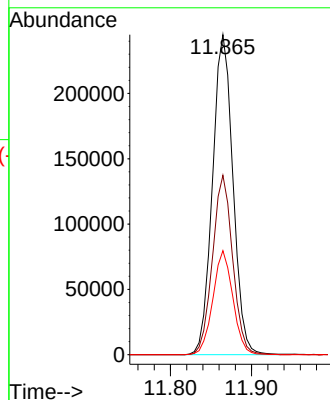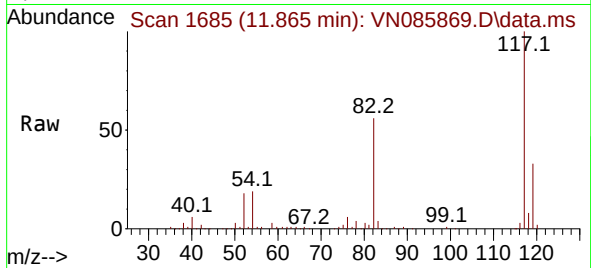

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.006 min
Lab File: VN085869.D
Acq: 26 Feb 2025 14:20

Tgt Ion:152 Resp: 167346
Ion Ratio Lower Upper
152 100
115 59.2 30.4 91.3
150 153.8 0.0 345.4

