


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022625\
Data File : VN085861.D
Acq On : 26 Feb 2025 10:08
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

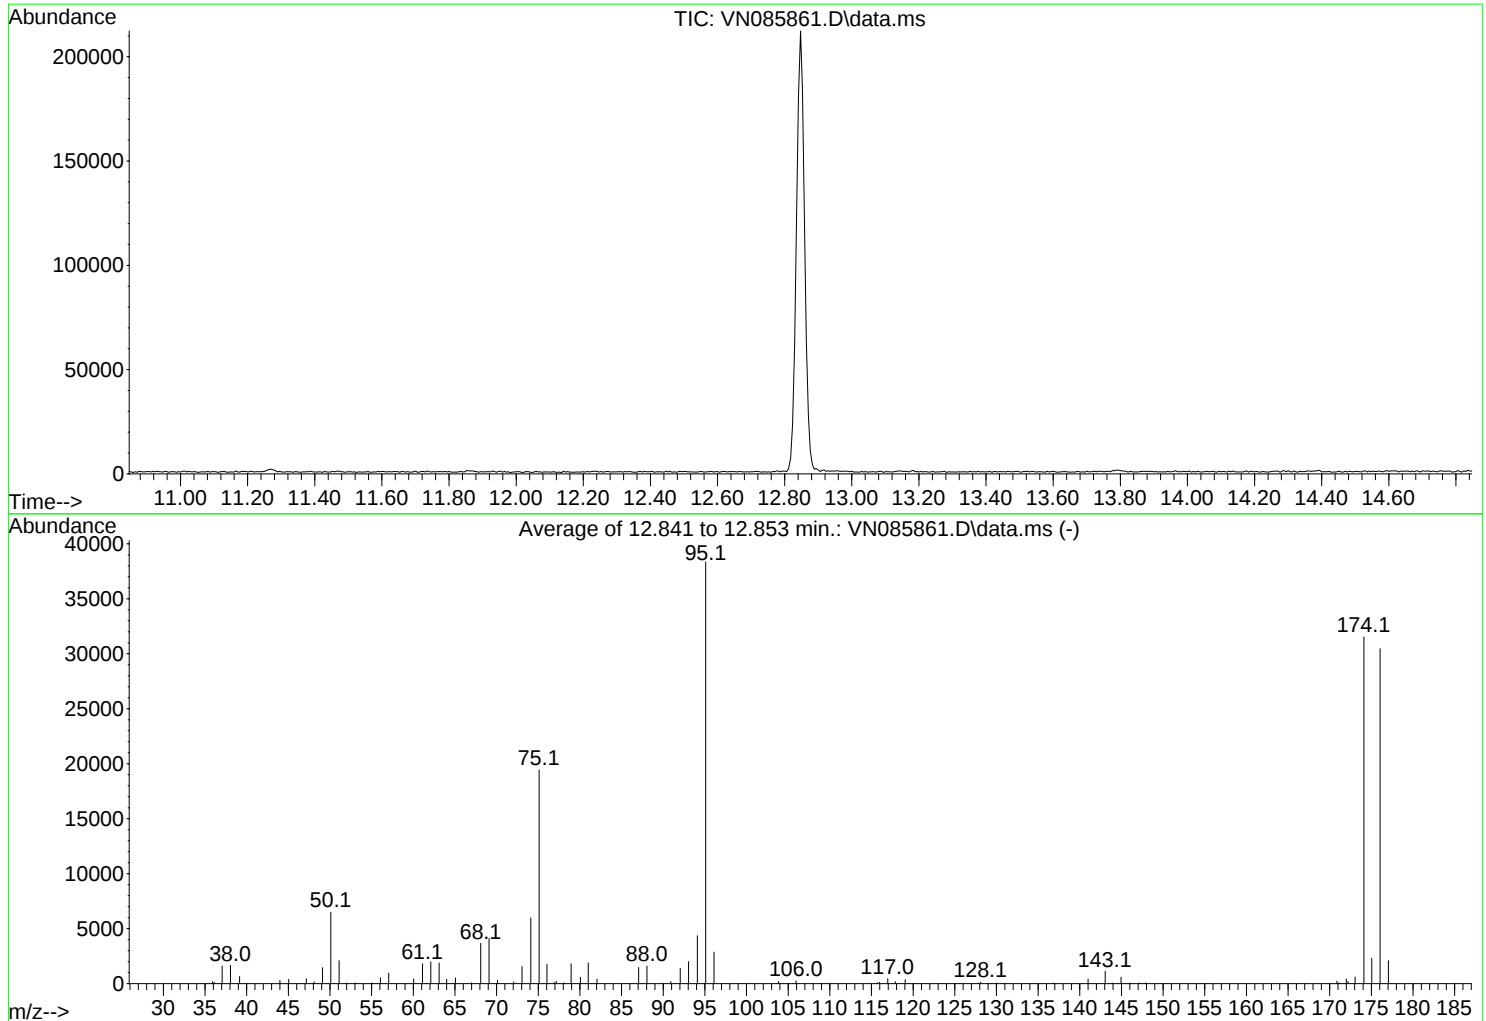

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	16.9	6493	PASS
75	95	30	60	50.6	19424	PASS
95	95	100	100	100.0	38363	PASS
96	95	5	9	7.5	2866	PASS
173	174	0.00	2	1.9	610	PASS
174	95	50	100	82.2	31531	PASS
175	174	5	9	7.3	2299	PASS
176	174	95	101	96.6	30467	PASS
177	176	5	9	6.9	2091	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	175	51.10	2094	65.05	523	76.90	111
36.10	116	52.00	61	67.00	78	77.15	211
37.05	1594	53.10	60	68.10	3666	78.10	7
38.05	1659	55.10	60	69.10	4098	78.95	180
39.15	662	56.05	520	70.10	300	80.05	583
44.00	302	57.05	968	72.05	164	81.00	1899
45.05	396	60.05	434	72.30	51	82.05	422
47.15	455	61.10	1803	73.05	1564	87.05	1466
48.10	167	62.10	1985	74.10	5977	88.05	1594
49.10	1457	63.10	1881	75.10	19424	90.90	190
50.10	6493	64.00	390	76.05	1769	92.05	1400

Average of 12.841 to 12.853 min.: VN085861.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
93.05	2005	127.80	53	170.85	238		
94.10	4363	128.10	131	171.10	75		
95.10	38363	130.00	64	172.00	434		
96.10	2866	136.80	58	172.20	204		
103.85	210	141.00	427	173.05	610		
105.95	264	143.05	1119	174.10	31531		
115.70	76	143.90	54	175.05	2299		
115.95	122	144.95	601	176.05	30467		
116.95	448	146.00	55	177.05	2091		
117.85	184	147.20	61				
119.05	370	147.90	68				

Instrument :
MSVOA_N
ClientSampleId :
BFB