


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022719\
 Data File : VN053970.D
 Acq On : 27 Feb 2019 15:41
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
 Title : SW846 8260
 Last Update : Thu Feb 28 04:05:45 2019

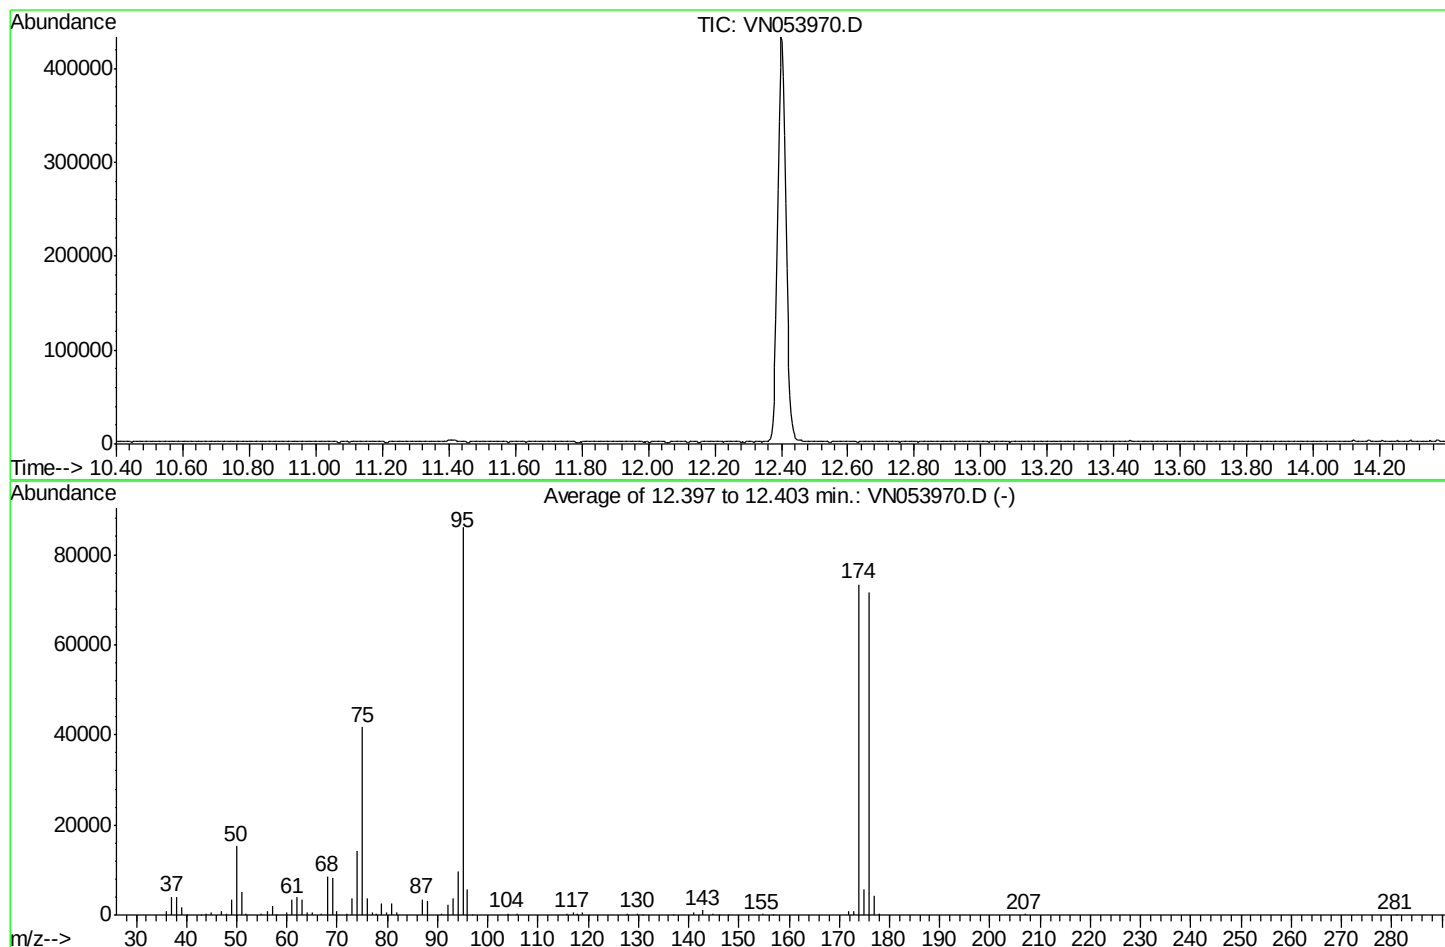

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.8	15350	PASS
75	95	30	60	48.4	41688	PASS
95	95	100	100	100.0	86080	PASS
96	95	5	9	6.5	5615	PASS
173	174	0.00	2	1.3	920	PASS
174	95	50	100	85.2	73333	PASS
175	174	5	9	7.6	5565	PASS
176	174	95	101	97.7	71621	PASS
177	176	5	9	6.1	4388	PASS