



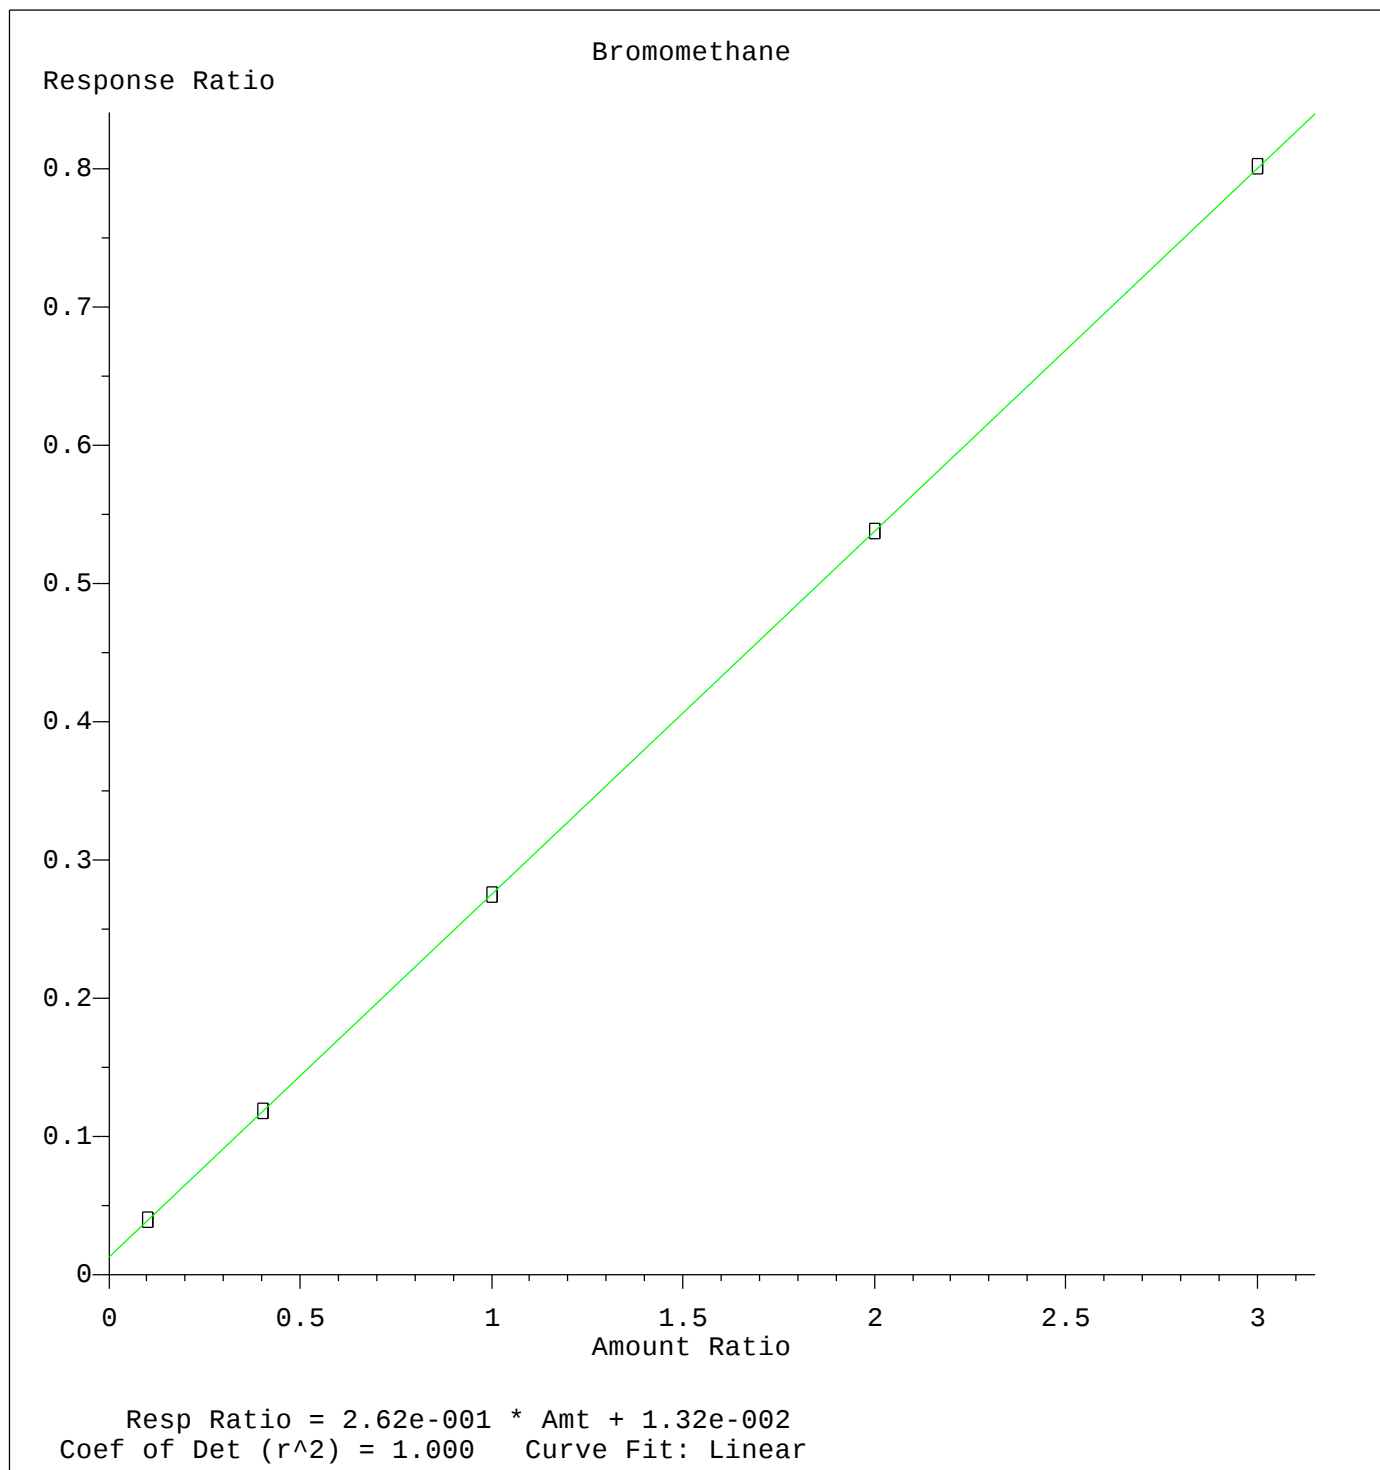

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020


trans-1,2-Dichloroethene

Response Ratio

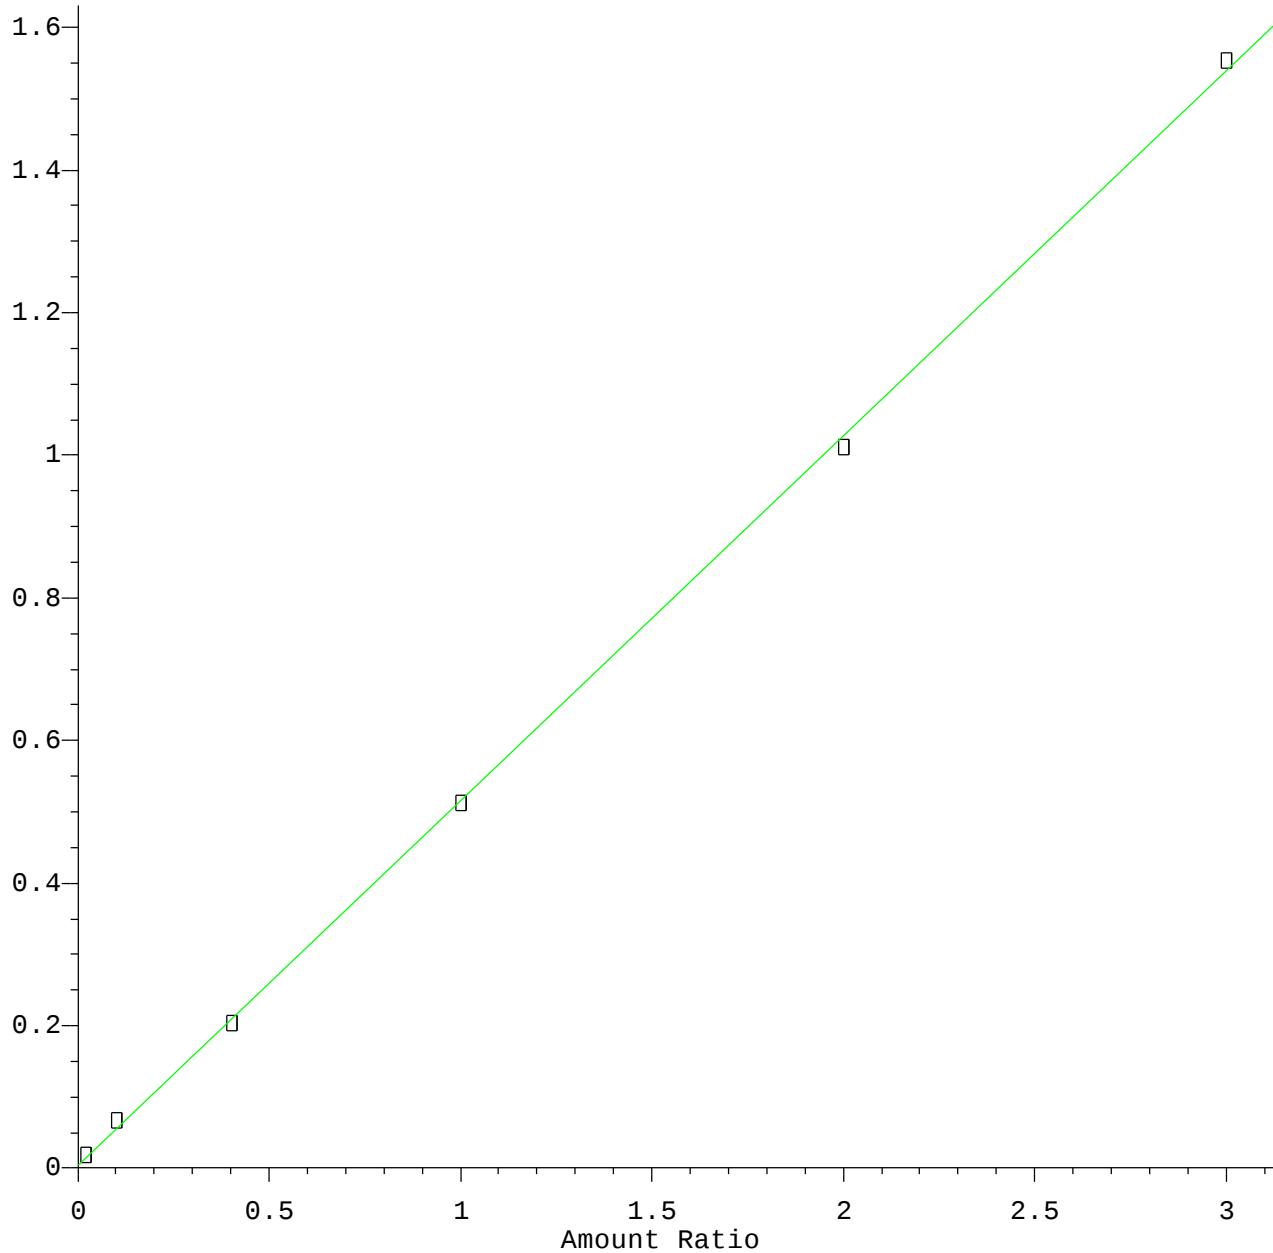

Resp Ratio = 5.12e-001 * Amt + 4.40e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

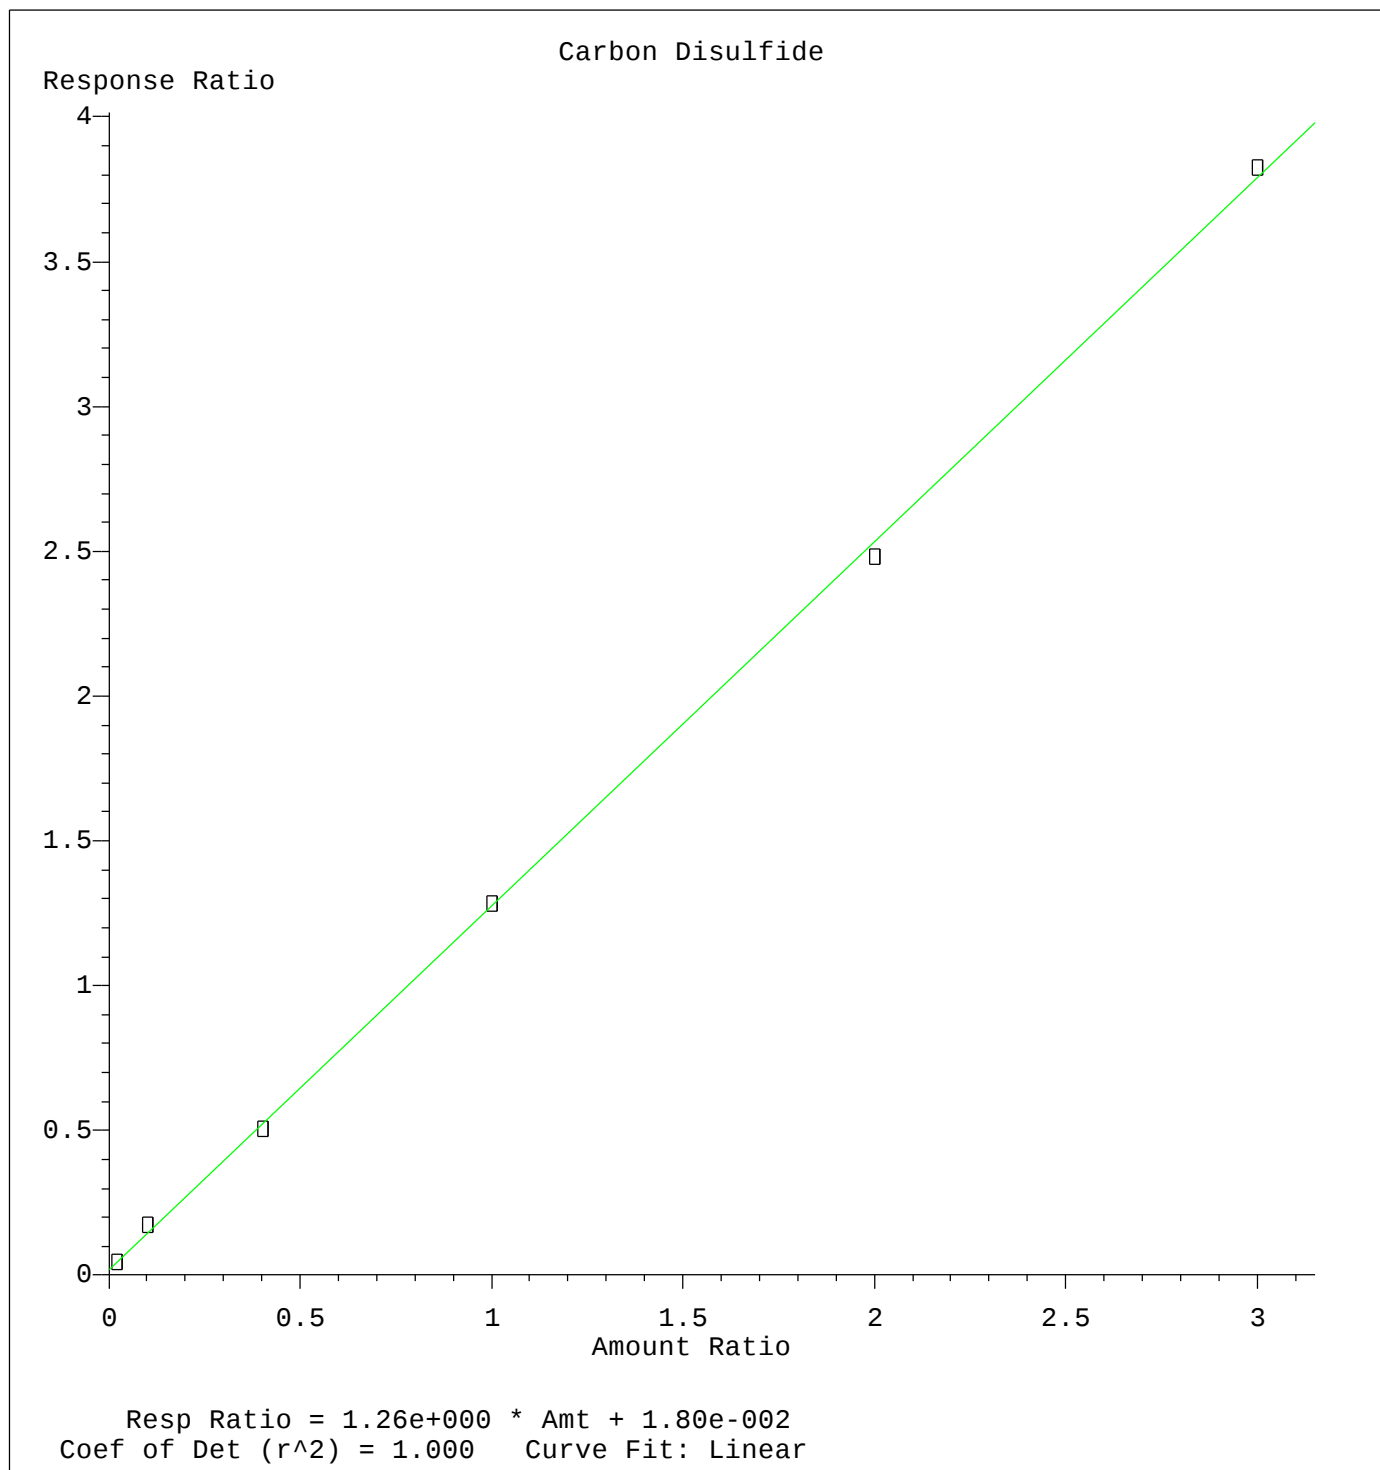

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

1,1-Dichloroethene

Response Ratio

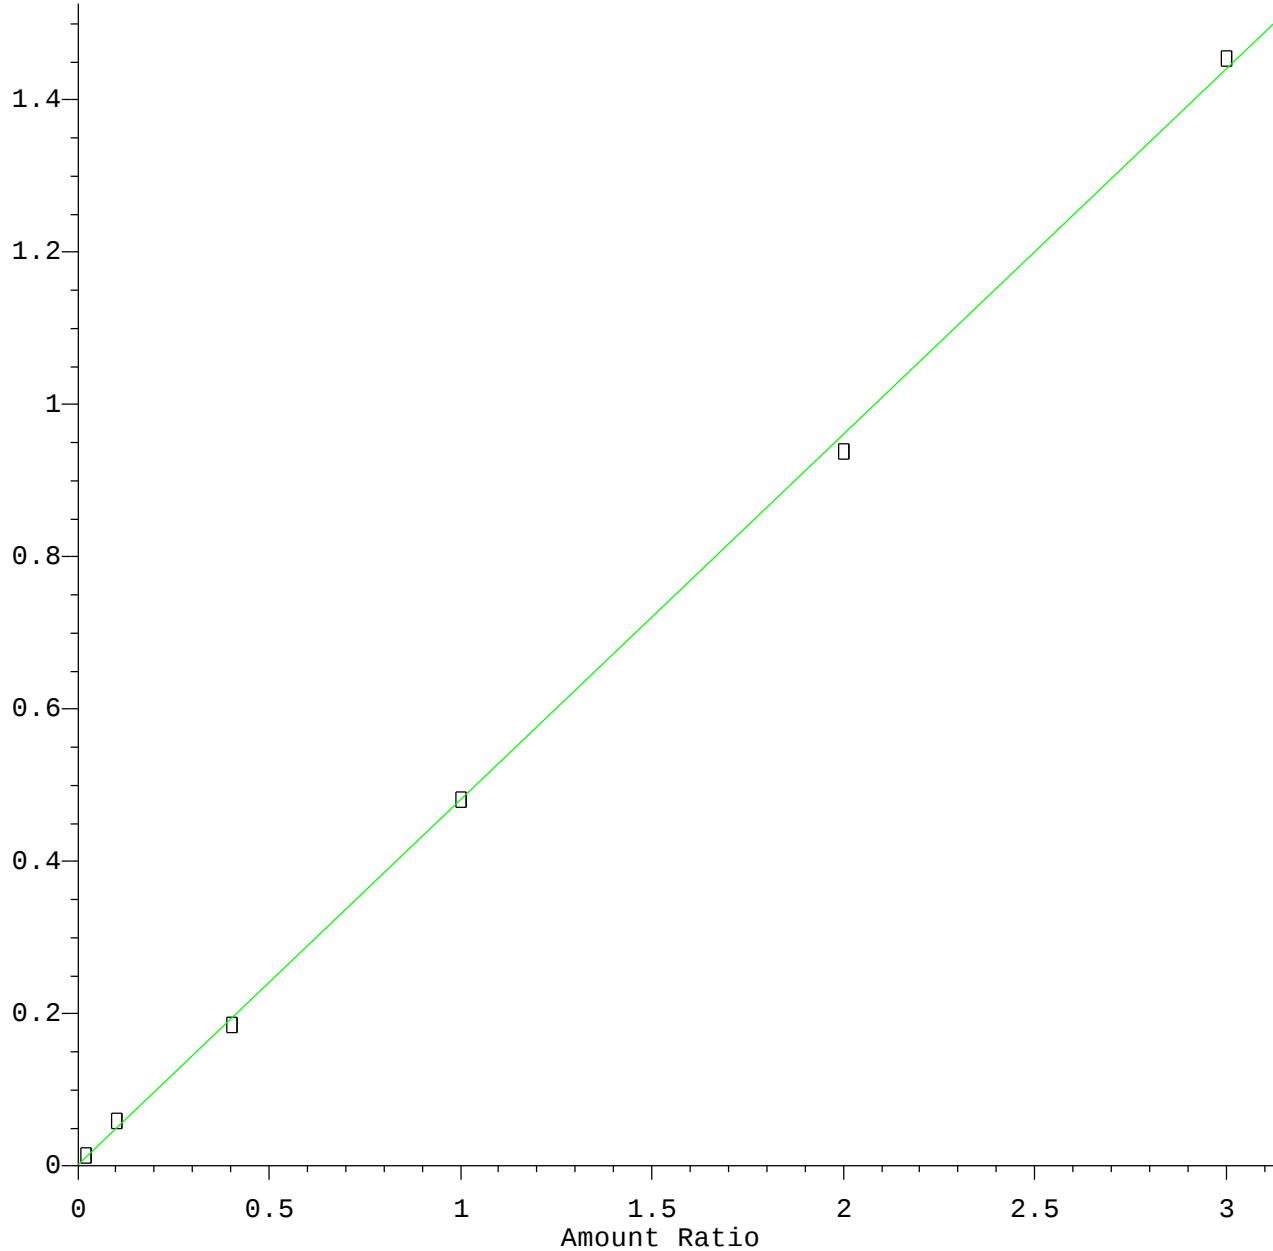


Resp Ratio = $4.80 \times 10^{-1} \times \text{Amt} + 7.43 \times 10^{-4}$
Coef of Det (r^2) = 0.999 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

1,2,3-Trichlorobenzene

Response Ratio

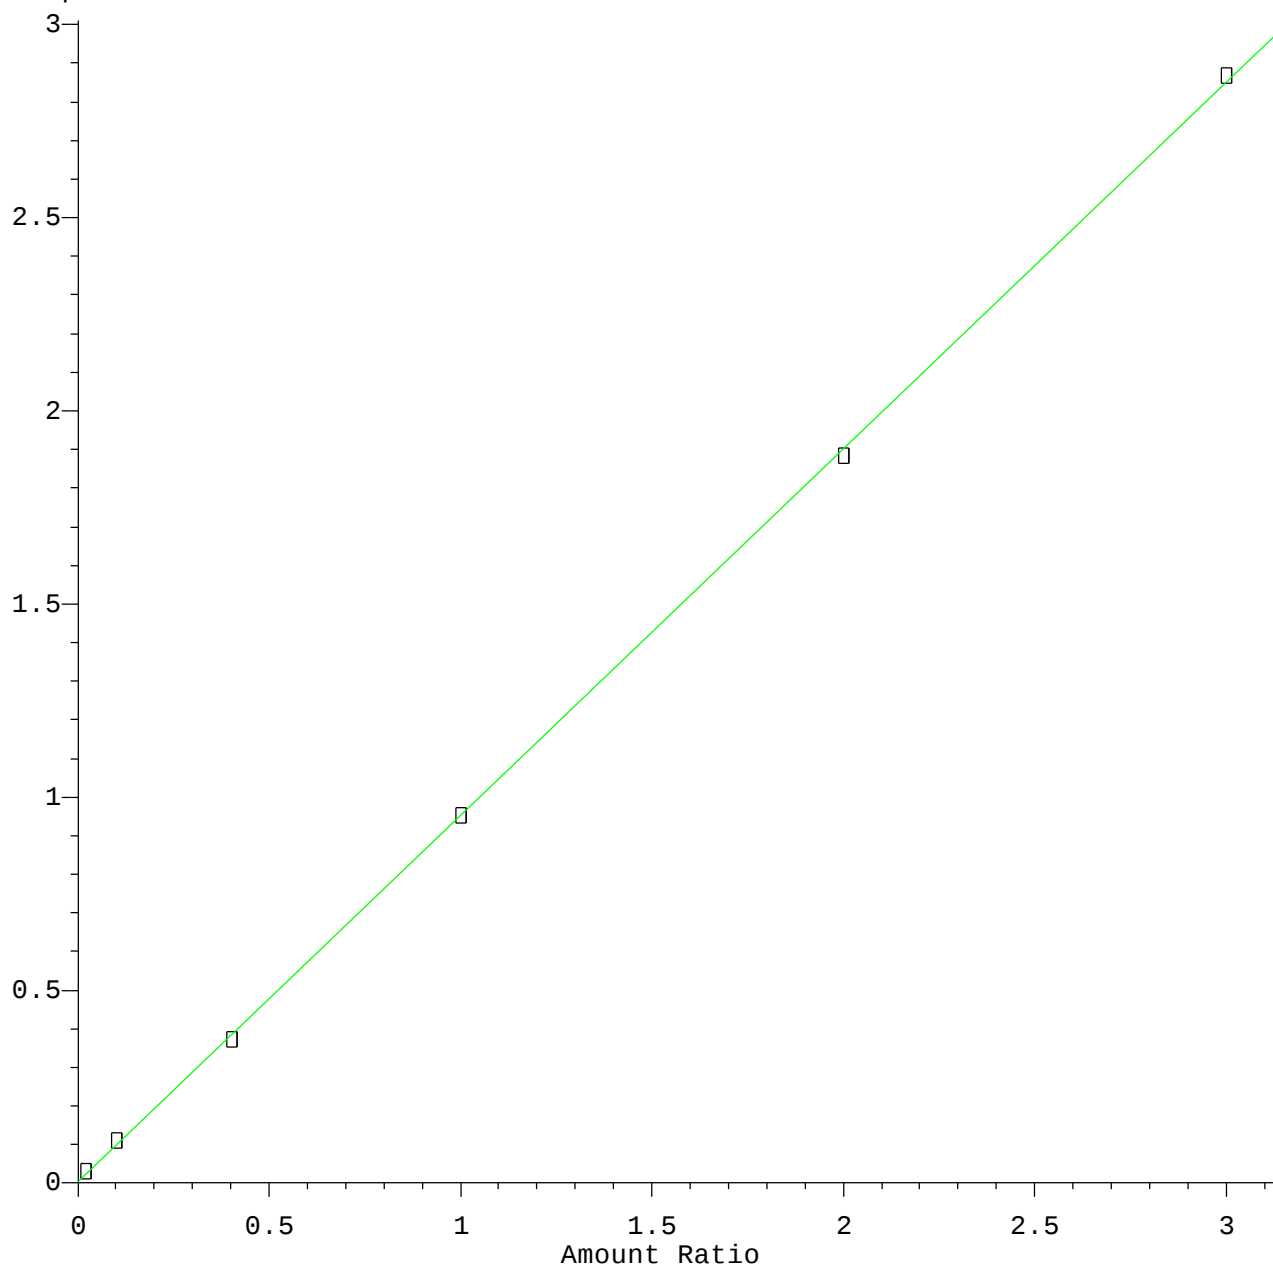


Resp Ratio = 9.49e-001 * Amt + 3.47e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020


Naphthalene

Response Ratio

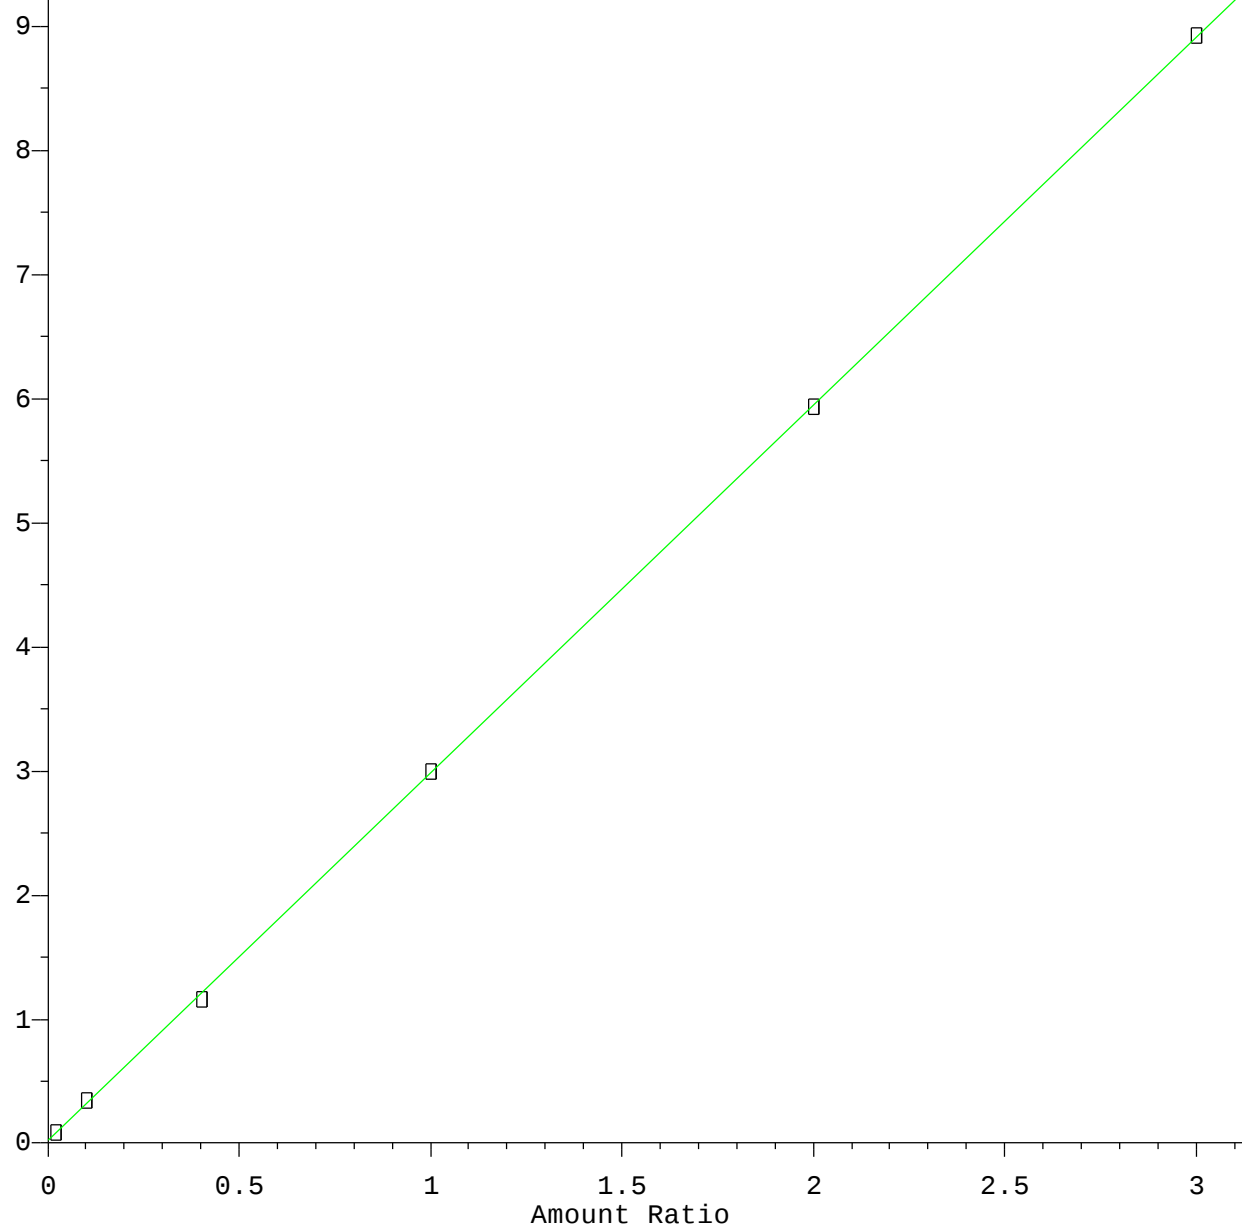

Resp Ratio = 2.96e+000 * Amt + 1.62e-002
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

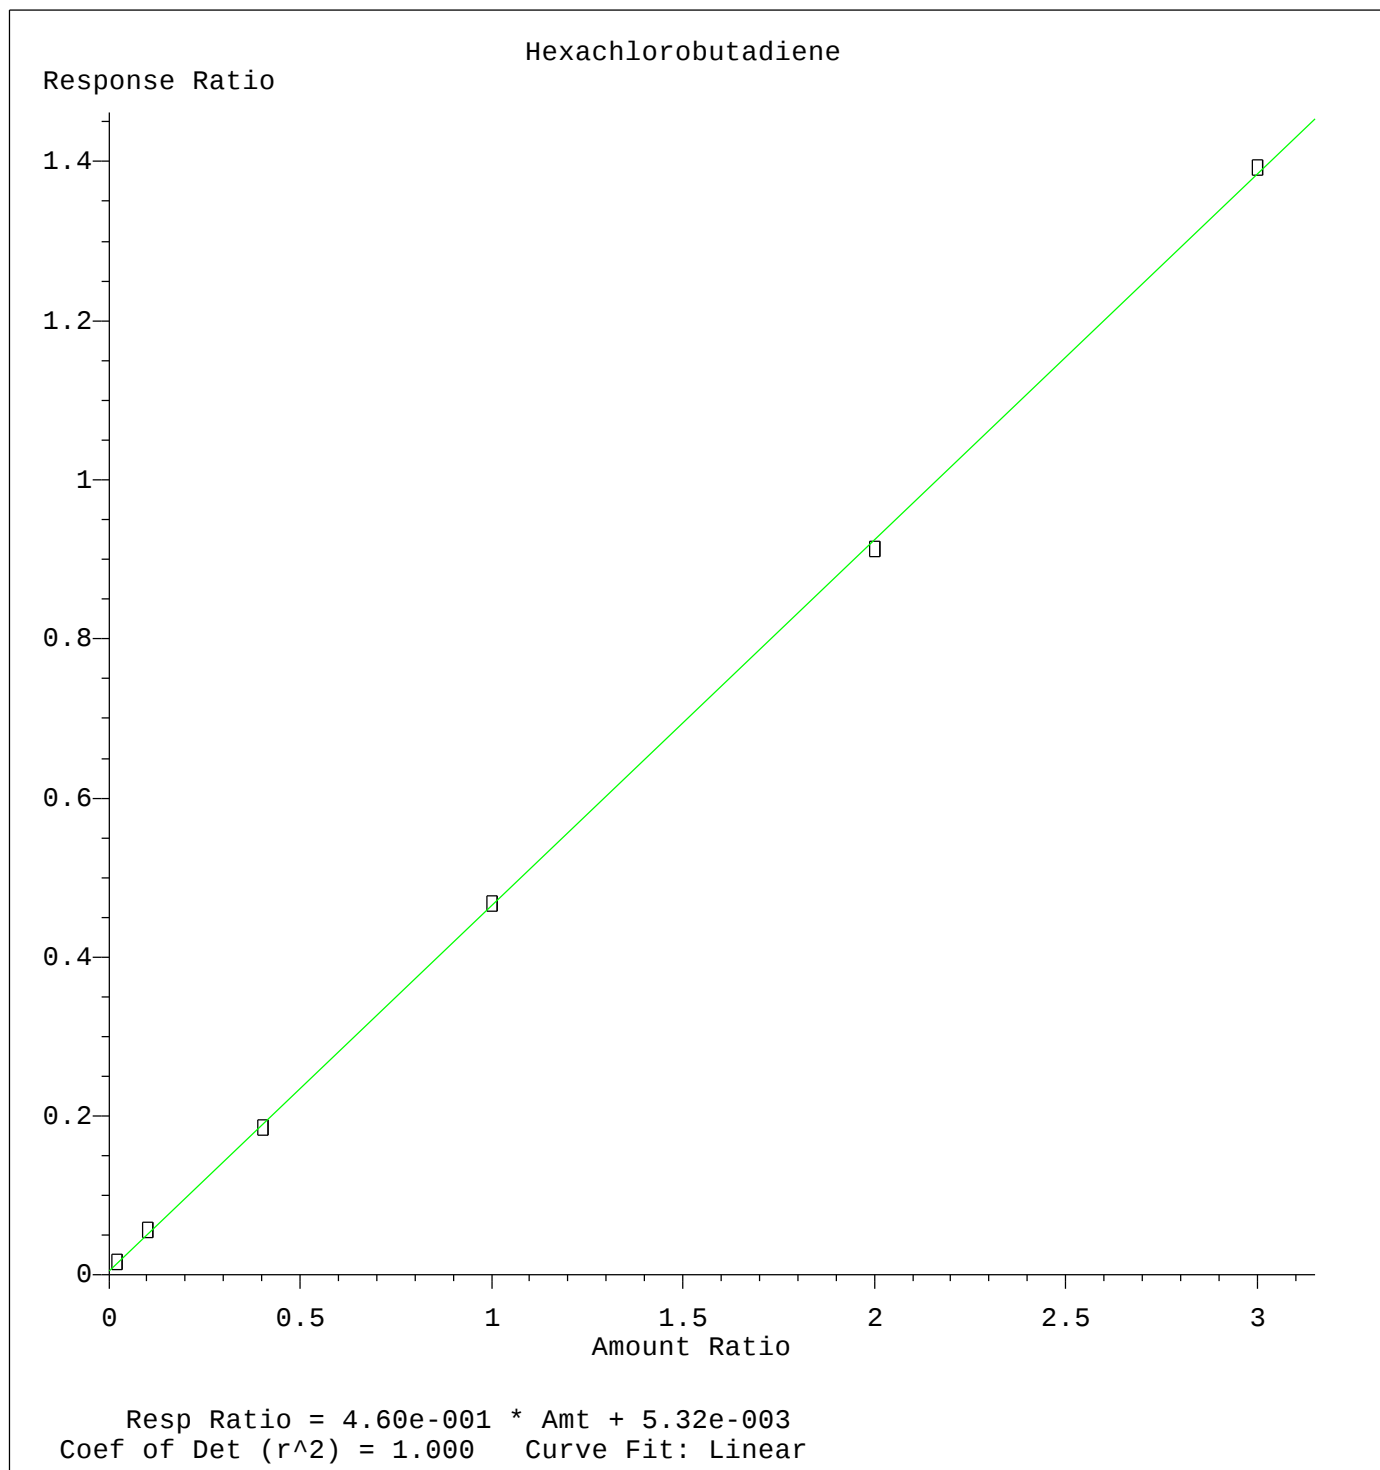

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020


1,2,4-Trichlorobenzene

Response Ratio

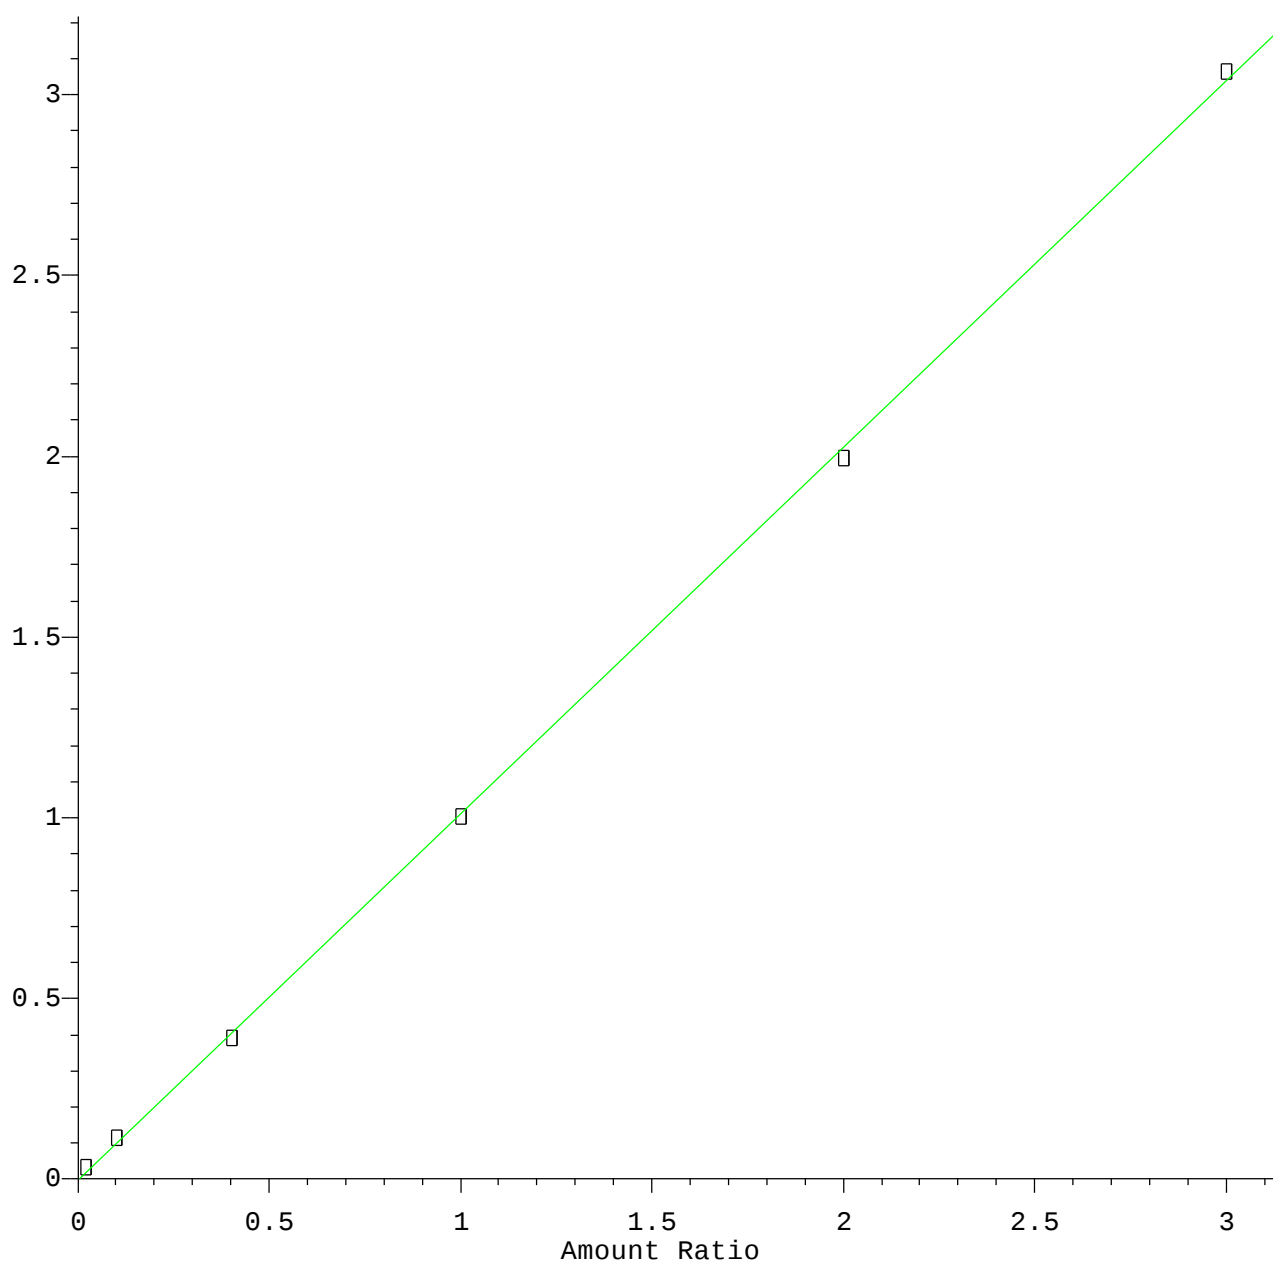

Resp Ratio = 1.01e+000 * Amt - 1.79e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear


Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

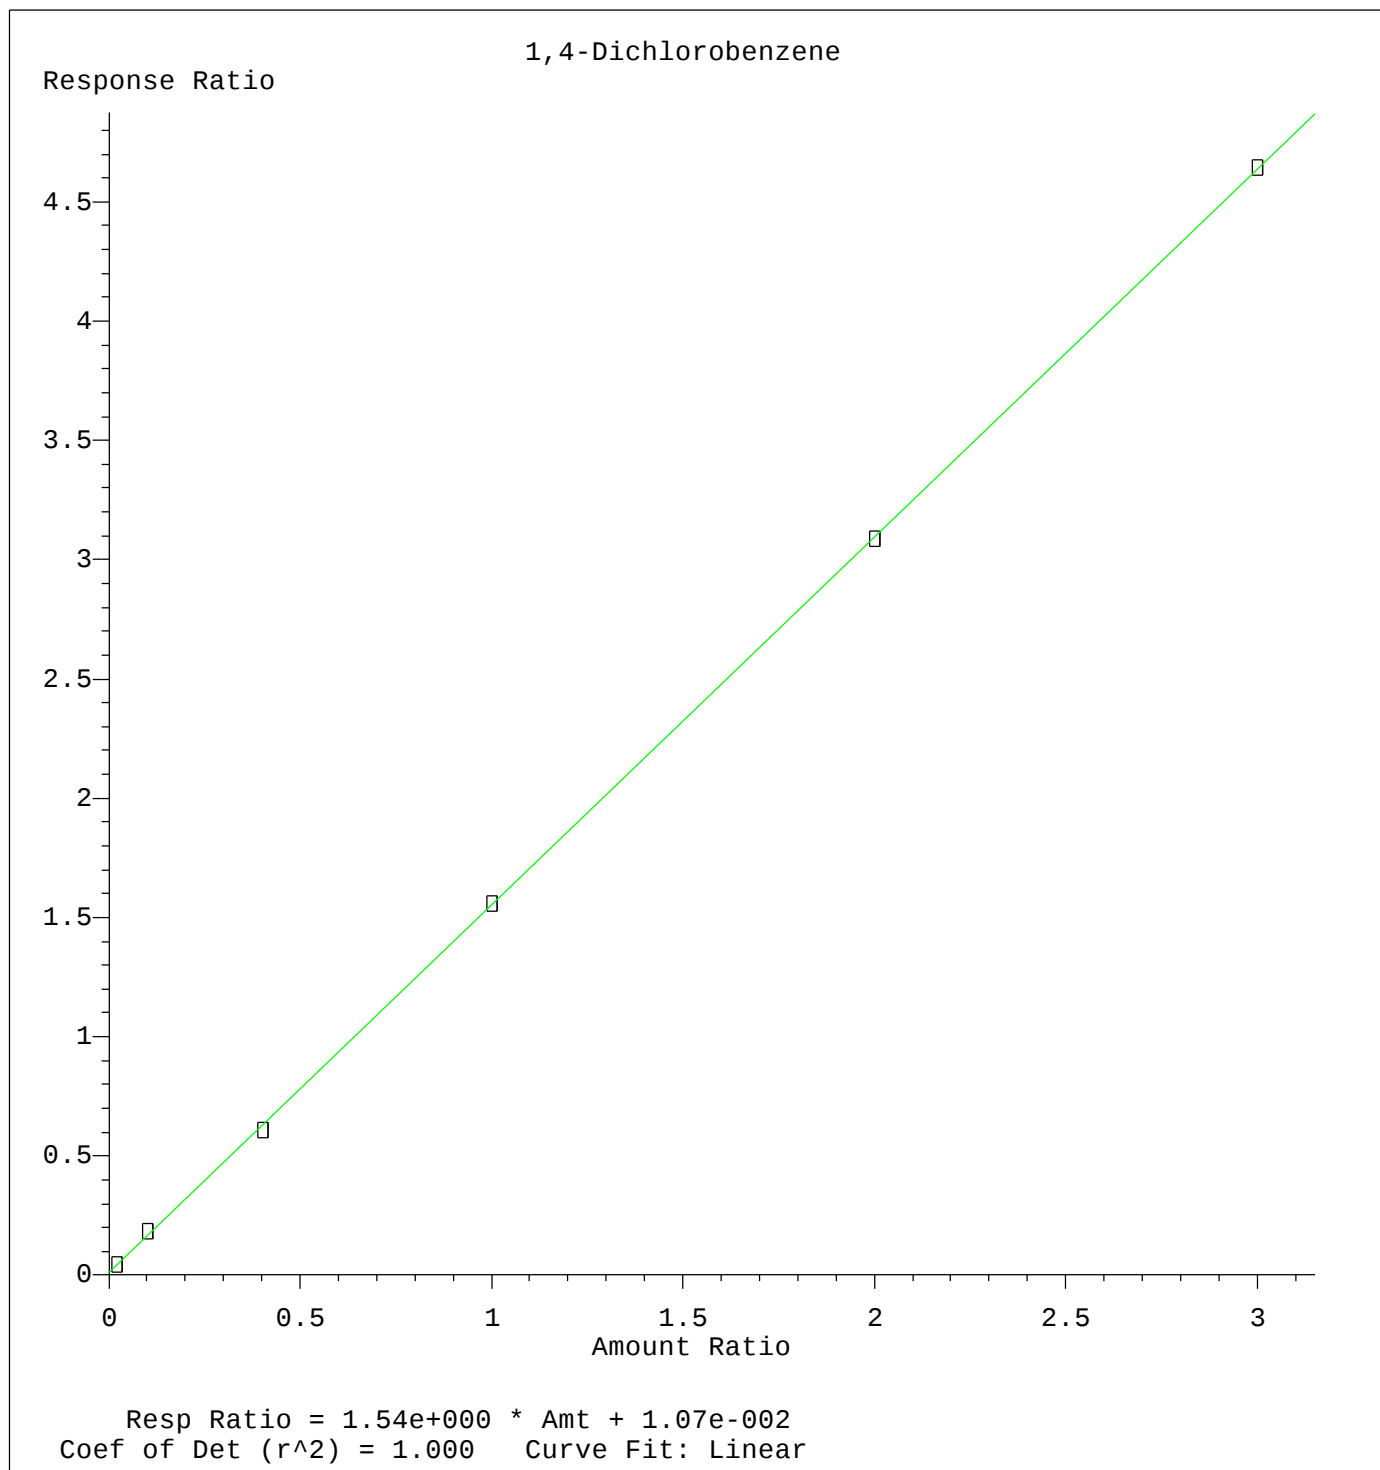

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

1,3-Dichlorobenzene

Response Ratio

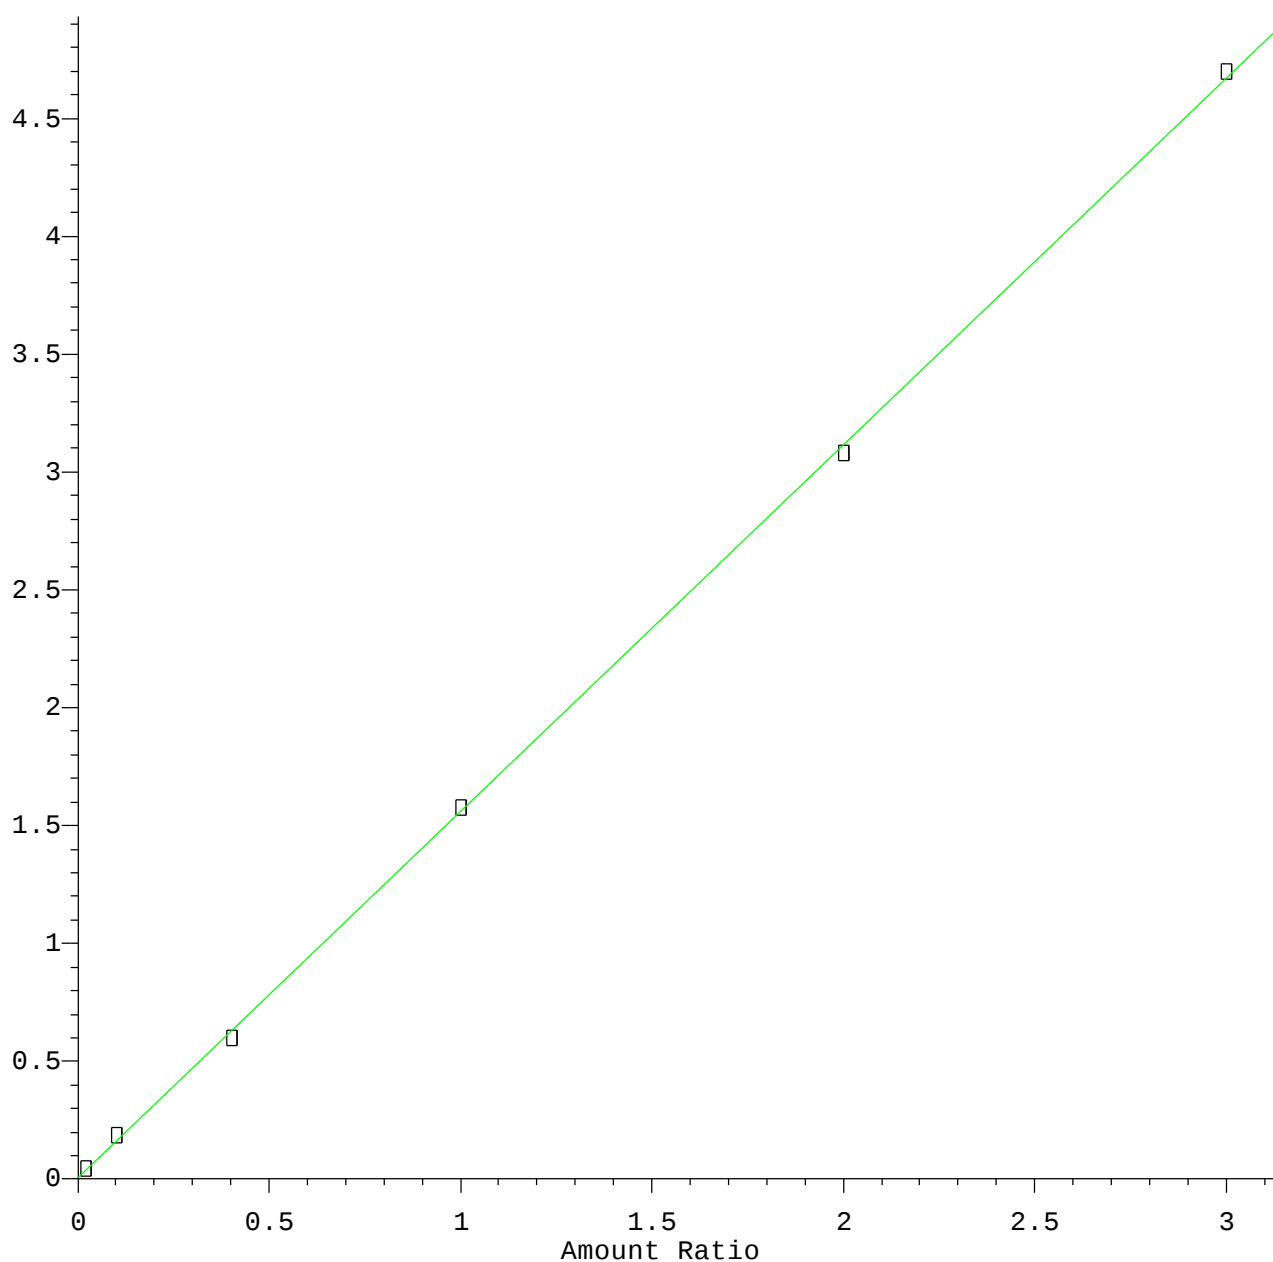


Resp Ratio = 1.56e+000 * Amt + 5.93e-003
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020


Tetrachloroethene

Response Ratio

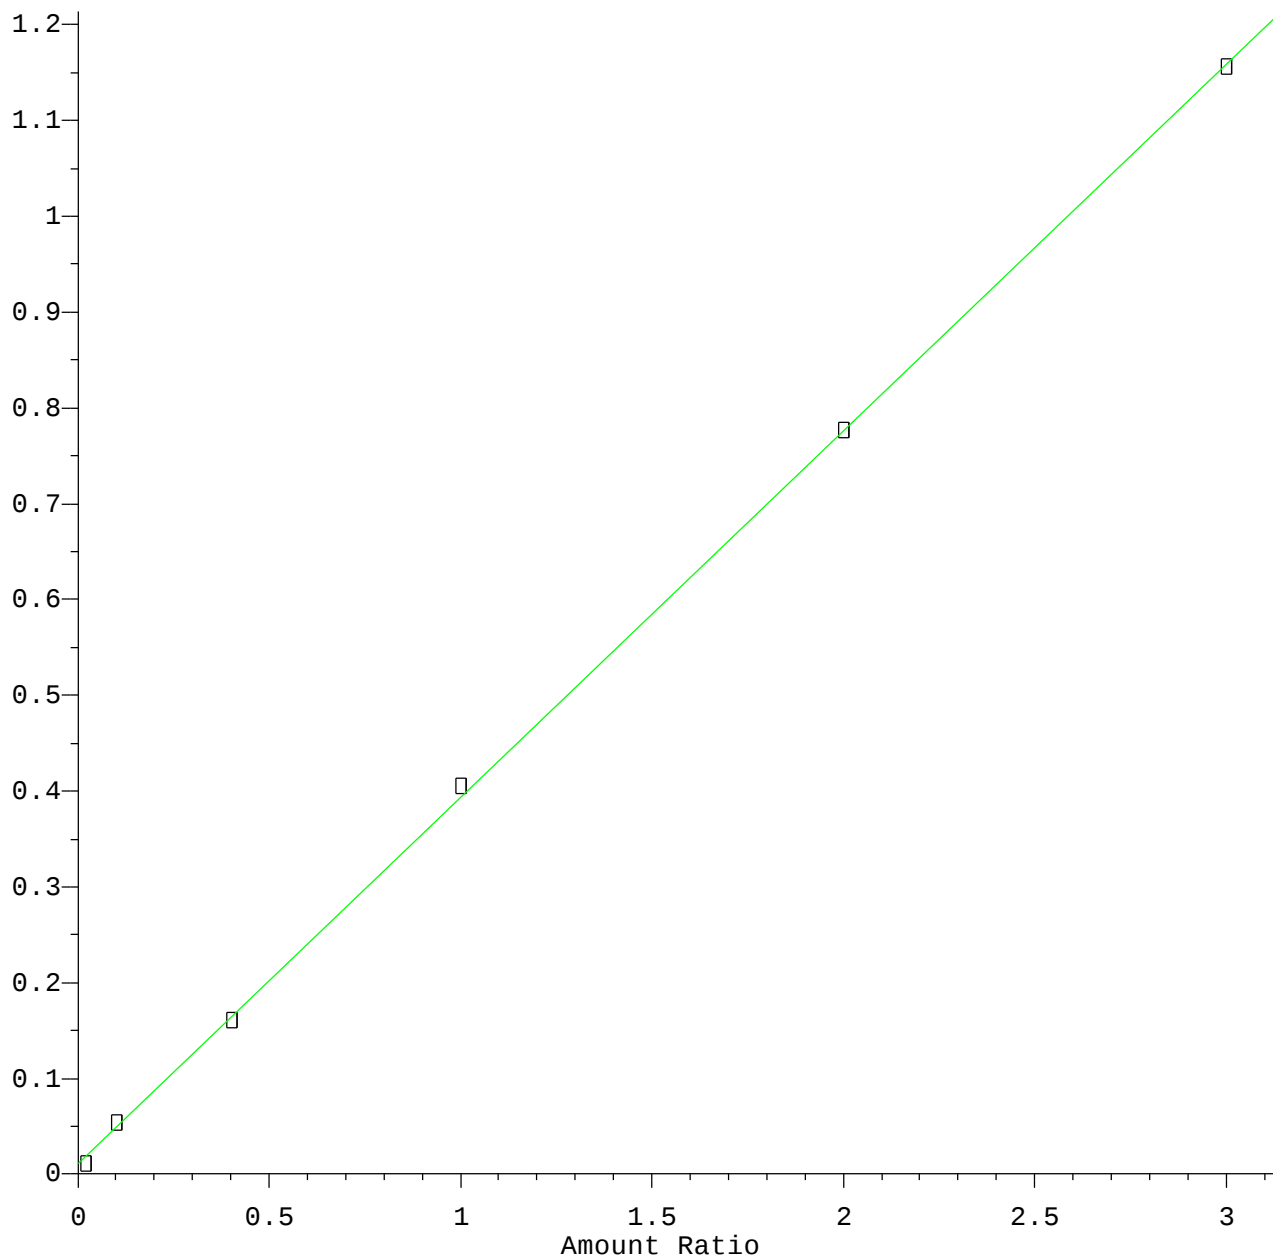

Resp Ratio = $3.83 \times 10^{-1} \times \text{Amt} + 1.11 \times 10^{-2}$
Coef of Det (r^2) = 1.000 Curve Fit: Linear

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020

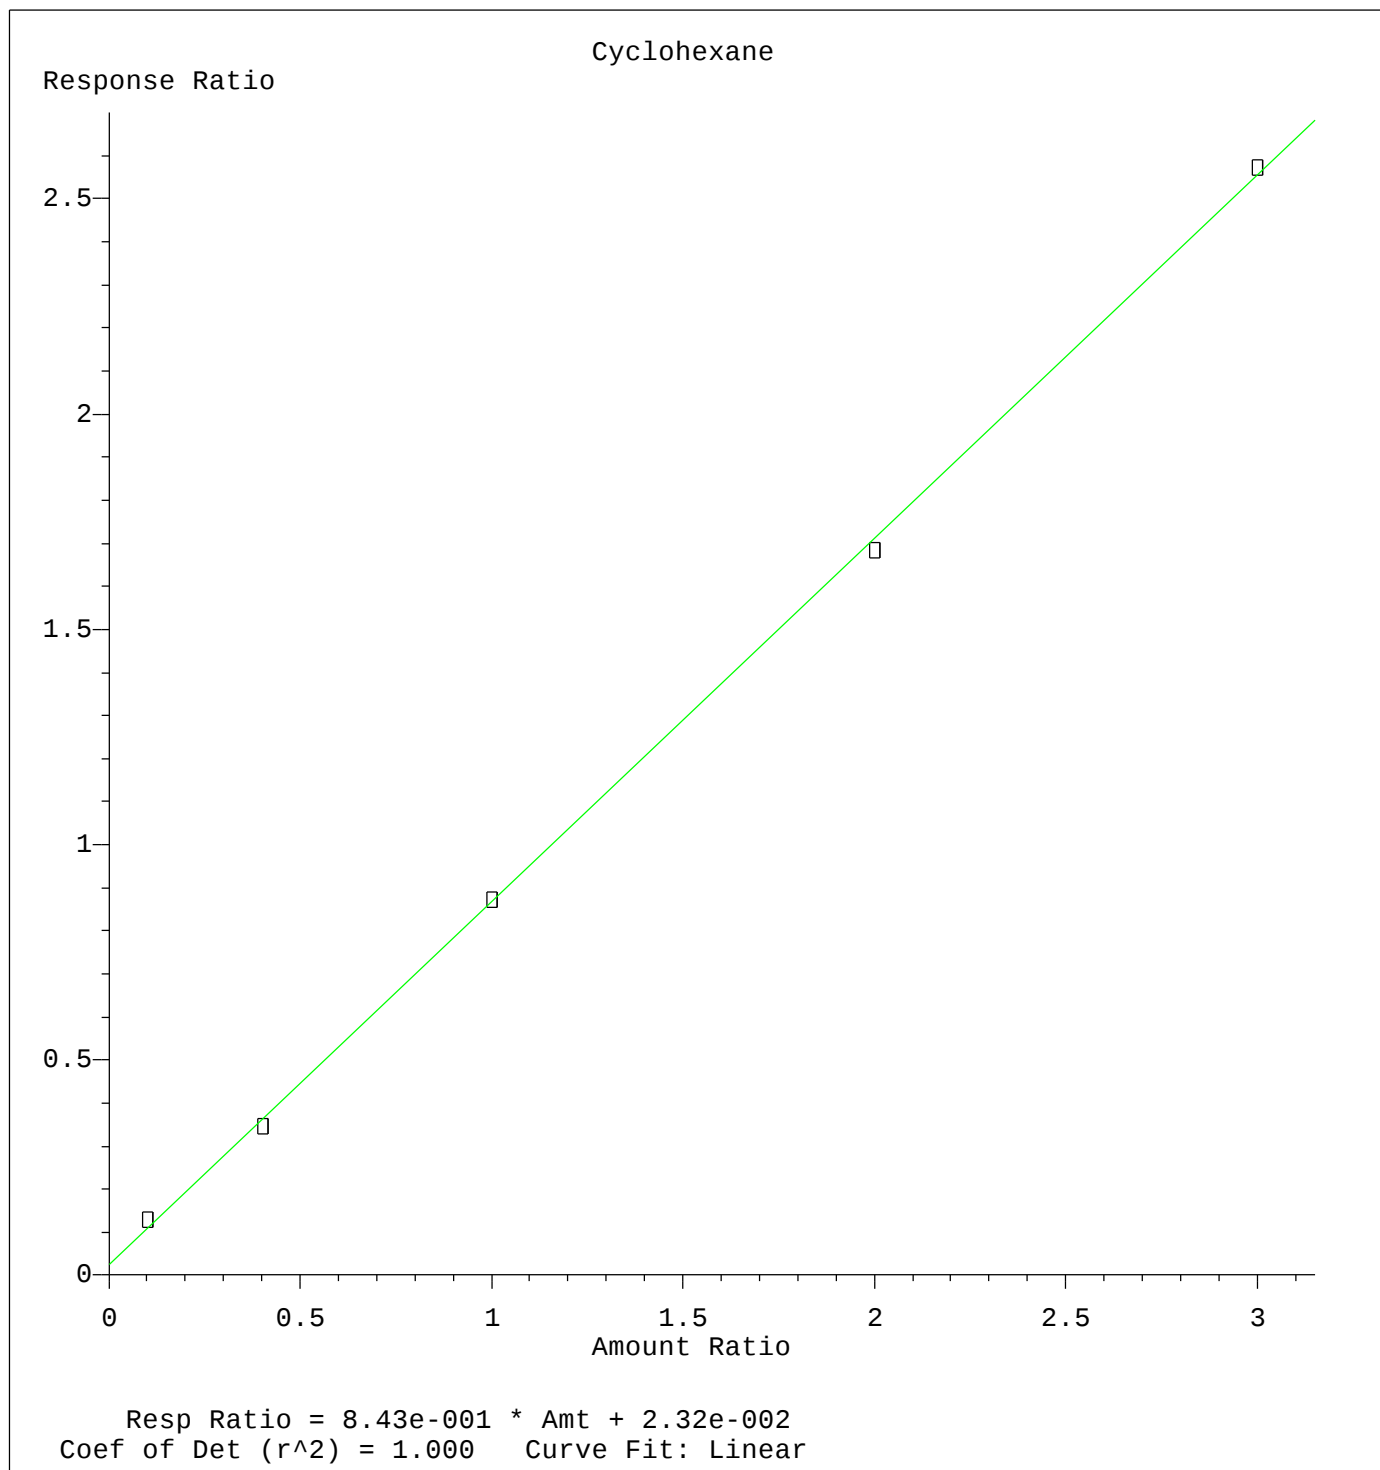

Method Name: Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Calibration Table Last Updated: Thu Feb 27 13:52:50 2020