
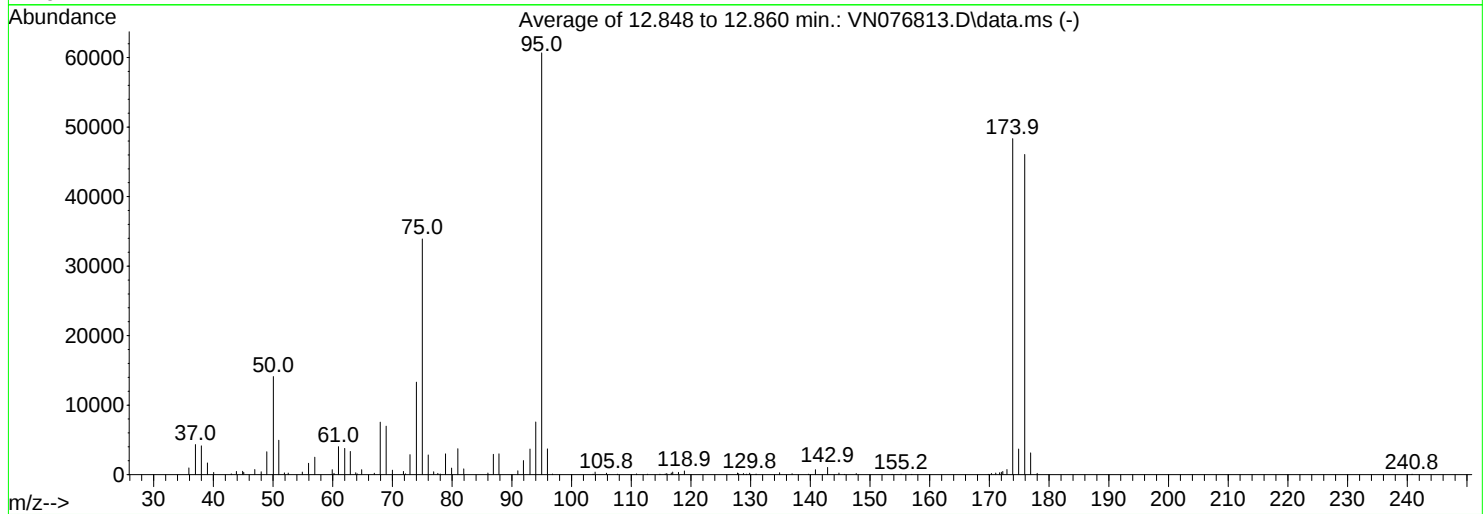


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022723\
Data File : VN076813.D
Acq On : 27 Feb 2023 08:59
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

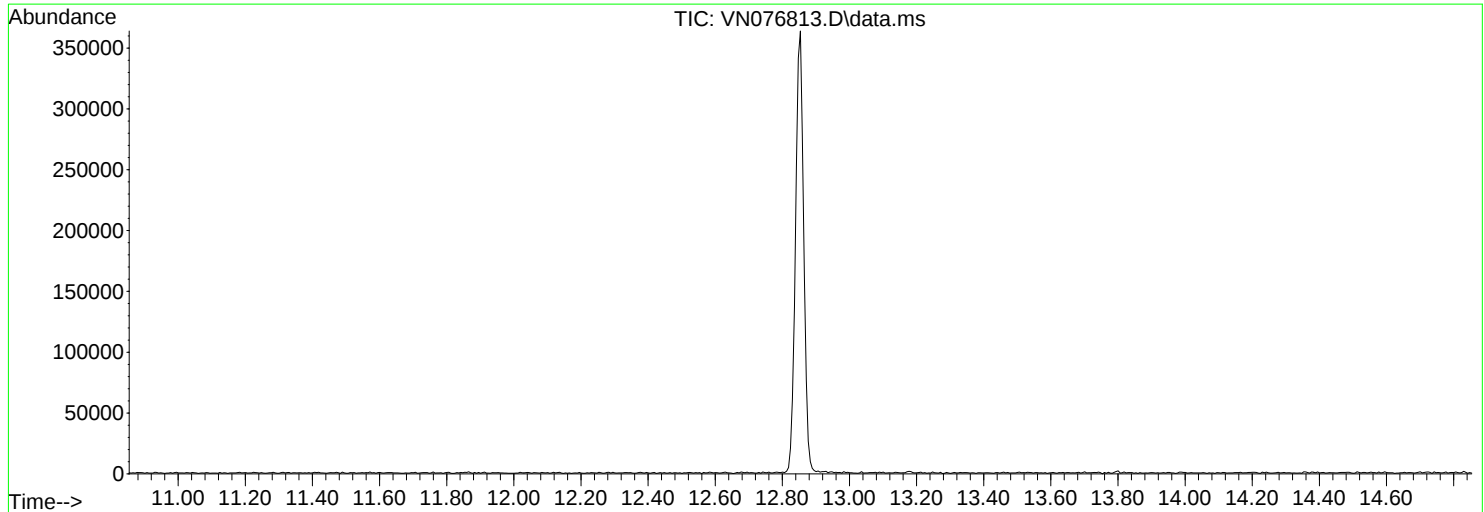

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	23.3	14112	PASS
75	95	30	60	55.9	33917	PASS
95	95	100	100	100.0	60683	PASS
96	95	5	9	6.1	3715	PASS
173	174	0.00	2	1.5	744	PASS
174	95	50	100	79.7	48344	PASS
175	174	5	9	7.6	3674	PASS
176	174	95	101	95.3	46051	PASS
177	176	5	9	6.8	3138	PASS

Average of 12.848 to 12.860 min.: VN076813.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	972	48.95	3289	62.00	3775	72.95	2881
37.00	4325	50.05	14112	62.95	3334	74.00	1330
38.00	4147	50.95	4941	63.85	267	75.00	3391
39.00	1674	51.90	245	64.10	111	76.00	284
40.05	328	52.55	240	64.85	707	76.90	417
43.00	125	54.90	363	66.95	201	77.60	178
43.85	455	55.95	1647	67.95	7556	78.00	97
44.90	478	57.00	2511	68.95	6976	78.90	2995
45.10	323	59.90	720	70.00	650	79.90	943
46.95	735	60.20	191	71.85	453	80.95	3741
48.00	418	60.95	4031	72.20	118	81.95	834

Average of 12.848 to 12.860 min.: VN076813.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.00	221	103.95	368	118.90	528	142.90	1047
86.90	2916	105.85	202	127.80	236	144.80	236
87.85	2999	107.70	61	128.00	151	145.70	59
91.00	543	110.90	120	128.80	162	147.70	157
91.95	2030	112.70	65	129.30	76	153.70	53
93.05	3676	114.80	74	129.85	207	155.20	60
94.00	7573	115.70	91	130.90	84	157.00	55
95.00	60683	115.95	153	134.85	266	169.80	51
95.95	3715	116.70	229	136.95	129	170.35	153
96.80	101	116.95	366	139.70	66	171.05	229
103.60	74	117.90	319	140.85	713	171.70	268

Average of 12.848 to 12.860 min.: VN076813.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.00	337						
172.25	467						
172.95	744						
173.90	48344						
174.90	3674						
175.90	46051						
176.90	3138						
178.00	174						
240.80	67						

Instrument :

MSVOA_N

ClientSampleId :

BFB