


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022724\
Data File : VN081207.D
Acq On : 27 Feb 2024 09:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

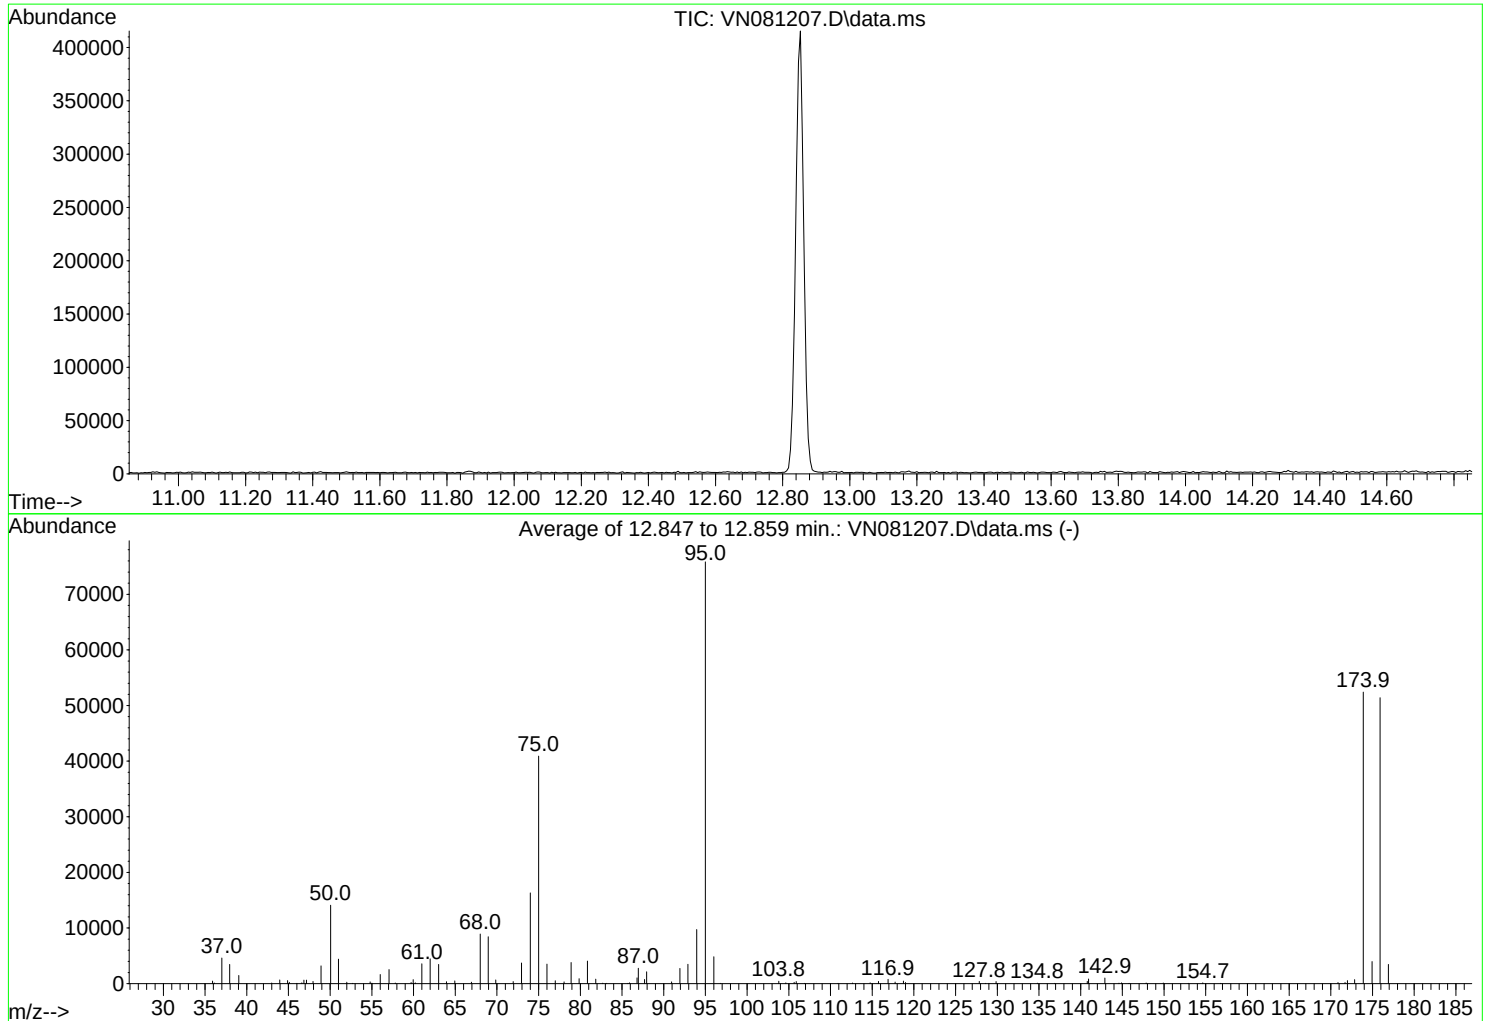

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	18.6	14099	PASS
75	95	30	60	53.9	40893	PASS
95	95	100	100	100.0	75832	PASS
96	95	5	9	6.4	4824	PASS
173	174	0.00	2	1.4	729	PASS
174	95	50	100	69.1	52413	PASS
175	174	5	9	7.6	3982	PASS
176	174	95	101	98.1	51400	PASS
177	176	5	9	6.7	3447	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.90	459	46.85	630	57.05	2527	68.00	891
36.10	107	47.15	641	57.80	121	68.95	844
37.00	4596	47.95	405	59.70	217	69.85	66
37.95	3446	48.90	3201	59.95	727	71.95	37
39.05	1458	50.05	14099	60.20	153	72.95	3705
43.00	122	51.00	4415	61.00	3576	74.00	16316
43.95	657	52.00	254	62.00	4471	75.00	40893
44.90	537	52.70	58	63.00	3466	76.00	3504
45.10	230	54.80	318	63.95	347	77.00	516
46.00	70	55.00	101	64.95	487	78.05	313
46.60	139	56.00	1632	66.95	264	78.90	3807

Average of 12.847 to 12.859 min.: VN081207.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.85	899	90.95	322	106.90	58	129.00	70
80.85	4067	91.95	2720	110.90	67	129.85	380
81.85	800	92.90	3492	112.65	129	134.80	94
82.70	91	93.95	9717	114.75	139	136.90	65
83.10	54	95.00	75832	115.75	415	140.80	393
85.70	61	96.00	4824	116.90	767	140.95	833
85.90	153	96.80	60	117.75	282	142.90	1017
86.80	1025	103.80	430	118.75	452	144.60	77
86.95	2769	104.65	148	119.00	193	144.90	153
87.70	754	105.65	223	127.85	394	145.80	58
87.95	2140	105.90	367	128.60	54	147.85	113

Average of 12.847 to 12.859 min.: VN081207.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
149.90	125	176.90	3447				
152.90	63						
154.65	134						
156.80	65						
170.85	211						
171.70	217						
172.00	556						
172.85	729						
173.90	52413						
174.95	3982						
175.90	51400						

Instrument :

MSVOA_N

ClientSampleId :

BFB