
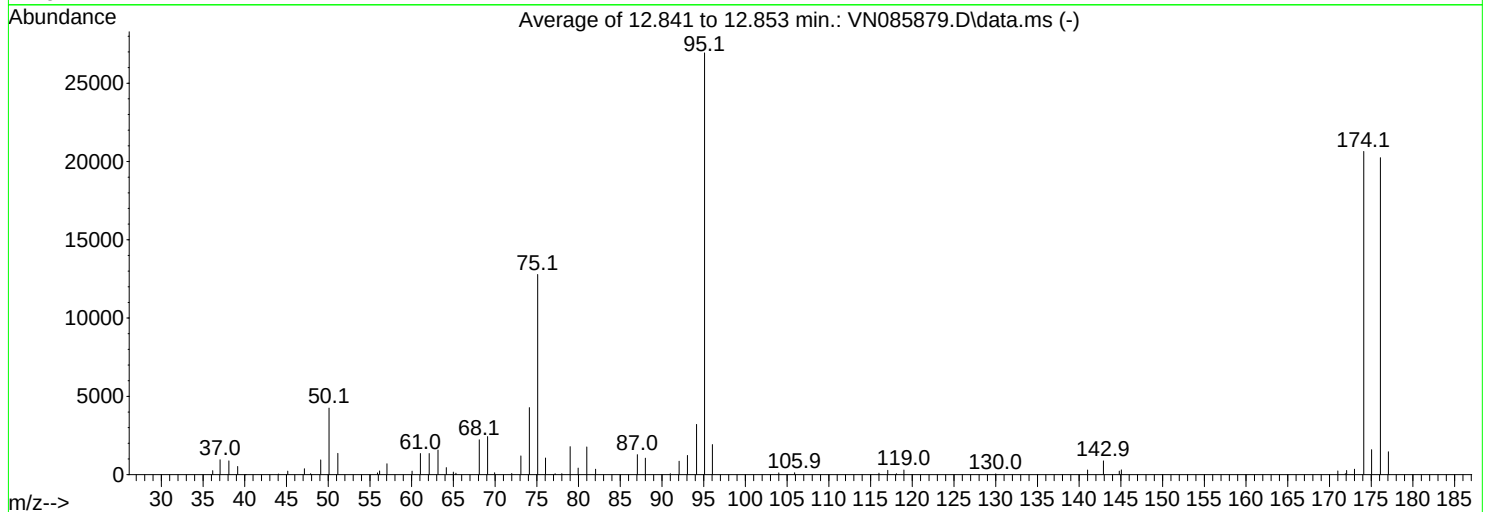


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022725\
Data File : VN085879.D
Acq On : 27 Feb 2025 09:45
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Title : SW846 8260
Last Update : Wed Feb 19 03:43:32 2025

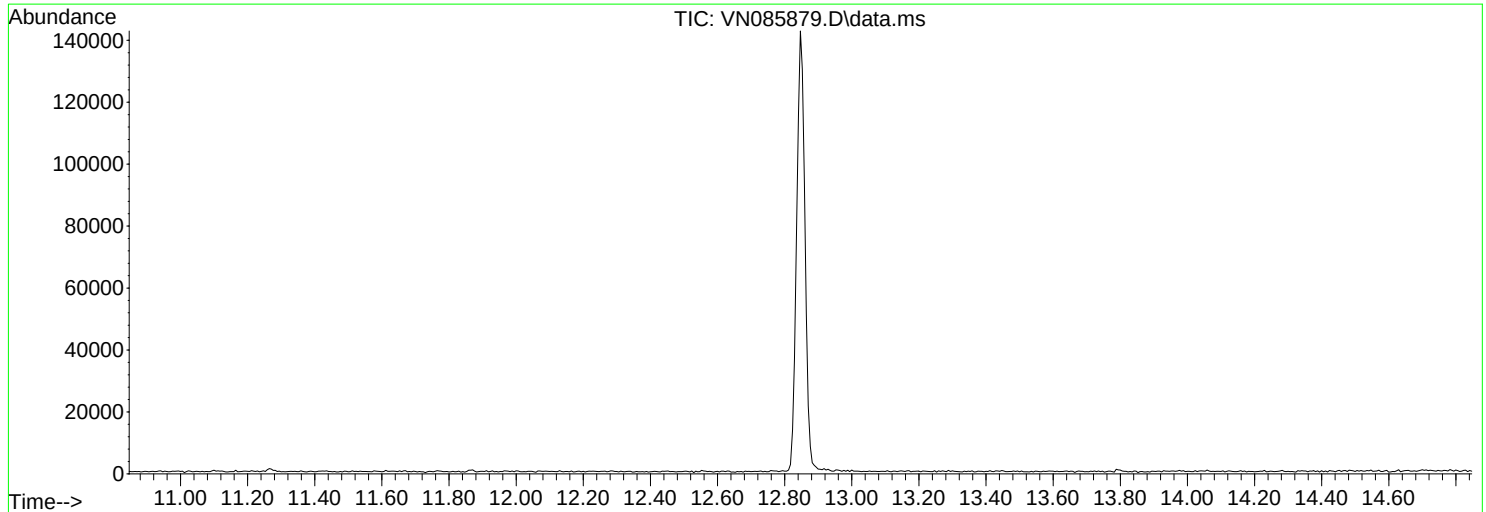

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	15.8	4251	PASS
75	95	30	60	47.5	12785	PASS
95	95	100	100	100.0	26939	PASS
96	95	5	9	7.1	1926	PASS
173	174	0.00	2	1.7	348	PASS
174	95	50	100	76.6	20640	PASS
175	174	5	9	7.7	1592	PASS
176	174	95	101	98.1	20243	PASS
177	176	5	9	7.2	1466	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.15	251	51.15	1358	68.10	2230	79.95	411
37.05	952	55.90	109	69.10	2431	81.00	1777
38.10	877	56.15	232	69.95	121	82.05	341
39.15	517	57.05	700	72.00	69	87.05	1280
40.05	5	60.05	228	73.10	1198	88.00	1057
44.05	39	61.05	1353	74.10	4284	91.00	59
45.15	222	62.10	1354	75.10	12785	92.05	854
47.15	377	63.15	1570	76.05	1066	93.05	1224
47.90	65	64.15	454	77.20	61	94.15	3205
49.10	944	65.00	160	78.00	58	95.10	26939
50.10	4251	65.30	90	79.00	1793	96.05	1926

Average of 12.841 to 12.853 min.: VN085879.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
104.00	116	171.00	235				
105.90	118	171.90	63				
116.00	90	172.05	264				
117.05	272	173.00	348				
118.10	60	174.10	20640				
119.00	294	175.05	1592				
130.00	56	176.10	20243				
141.00	299	177.05	1466				
142.90	879						
144.80	226						
145.05	308						

Instrument :

MSVOA_N

ClientSampleId :

BFB