

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN022819\
 Data File : VN053998.D
 Acq On : 28 Feb 2019 12:33
 Operator : JC/SP
 Sample : K1645-12
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 SR-9-D

Manual Integrations
 APPROVED

MMDadoda
 3/1/2019 4:10:21 PM

Quant Time: Mar 01 04:31:58 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 28 04:05:45 2019
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	587180	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1086646	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1066363	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	401295	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	391715	56.91	ug/l	0.00
Spiked Amount 50.000			Recovery	=	113.82%	
35) Dibromofluoromethane	7.59	113	360114	51.25	ug/l	0.00
Spiked Amount 50.000			Recovery	=	102.50%	
50) Toluene-d8	10.09	98	1391766	53.21	ug/l	0.00
Spiked Amount 50.000			Recovery	=	106.42%	
62) 4-Bromofluorobenzene	12.40	95	459164	52.69	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.38%	
Target Compounds						
20) Methylene Chloride	4.55	84	534449	78.453	ug/l	91
43) Isopropyl Acetate	8.17	43	28510m	2.340	ug/l	
84) 1,2,4-Trimethylbenzene	13.04	105	32529	1.274	ug/l	96
95) Naphthalene	15.13	128	122439	10.423	ug/l	98

(#) = qualifier out of range (m) = manual integration (+) = signals summed


Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN022819\
Data File : VN053998.D
Acq On : 28 Feb 2019 12:33
Operator : JC/SP
Sample : K1645-12
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 7 Sample Multiplier: 1


Instrument :
MSVOA_N
ClientSampleId :
SR-9-D

Manual Integrations
APPROVED

MMDadoda
3/1/2019 4:10:21 PM

Quant Time: Mar 01 04:31:58 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 28 04:05:45 2019
Response via : Initial Calibration

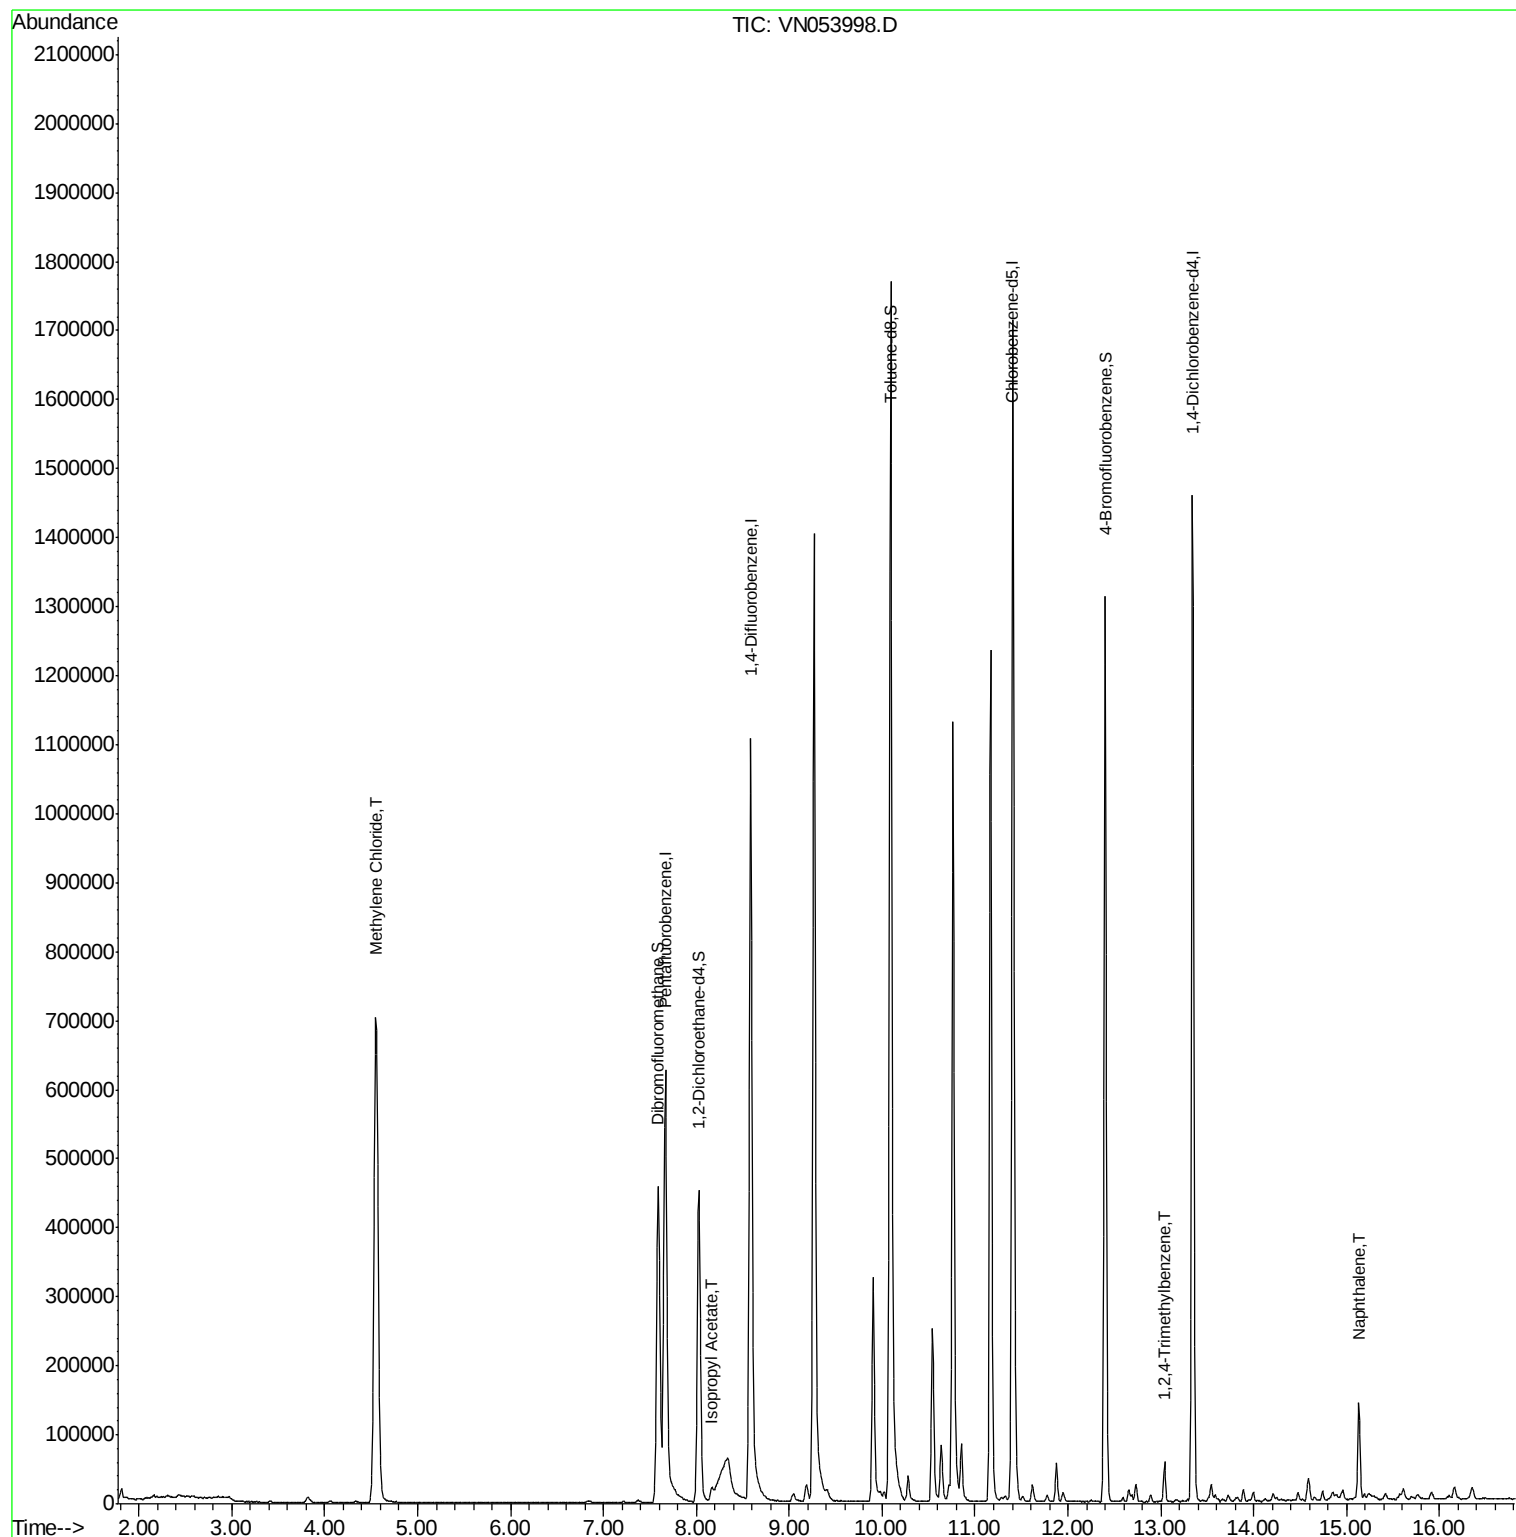

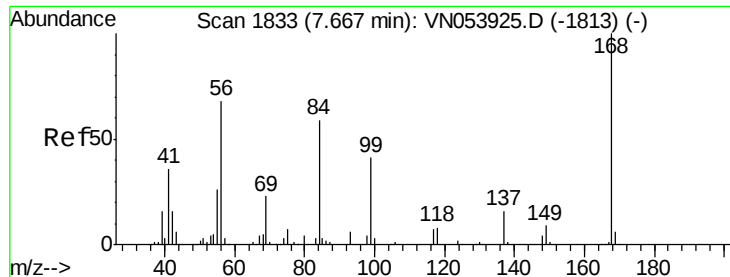

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN053998.D

Acq: 28 Feb 2019 12:33

Instrument :

MSVOA_N

ClientSampled :

SR-9-D

Tot Ion:168 Resp: 587180

Ion Ratio Lower Upper

168 100


99 52.6 36.9 55.3

Manual Integrations

APPROVED

MMDadoda

3/1/2019 4:10:21 PM

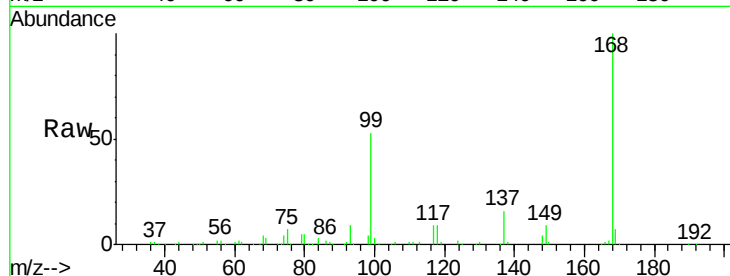

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

7.67

250000

200000



150000

100000

50000

0

Time--> 7.50 7.60 7.70 7.80

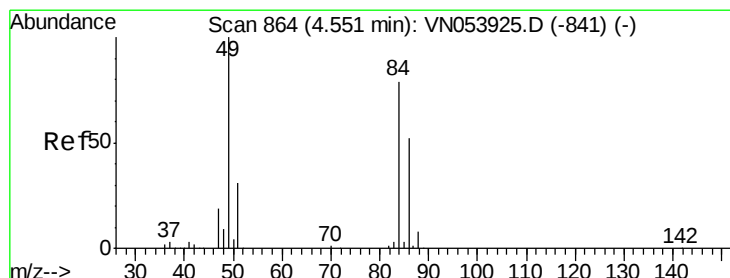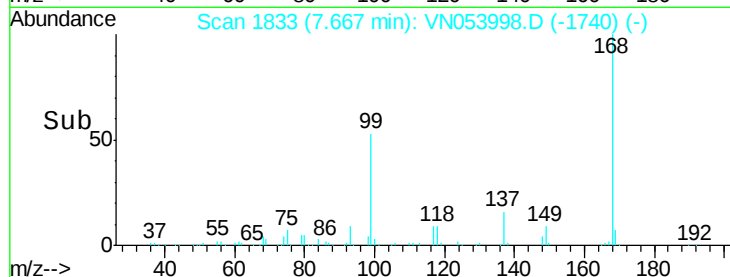

#20

Methylene Chloride

Concen: 78.453 ug/l

RT: 4.55 min Scan# 864

Delta R.T. 0.00 min

Lab File: VN053998.D

Acq: 28 Feb 2019 12:33

Tgt Ion: 84 Resp: 534449


Ion Ratio Lower Upper

84 100

49 127.3 89.7 134.5

51 39.2 27.8 41.8

86 64.0 51.3 76.9

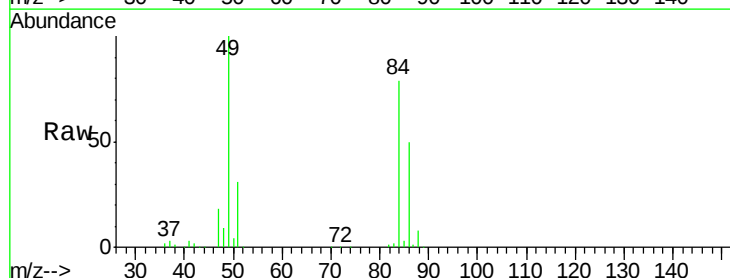

Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO

4.55


300000


200000

100000

0

Time--> 4.40 4.50 4.60 4.70

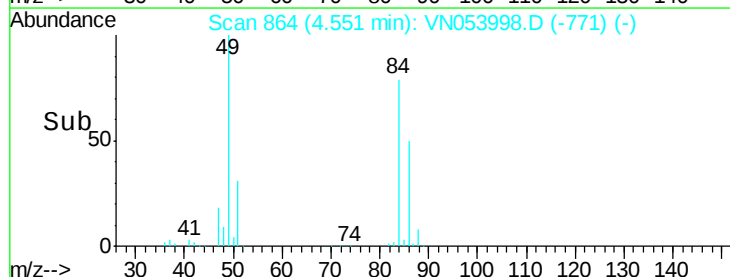

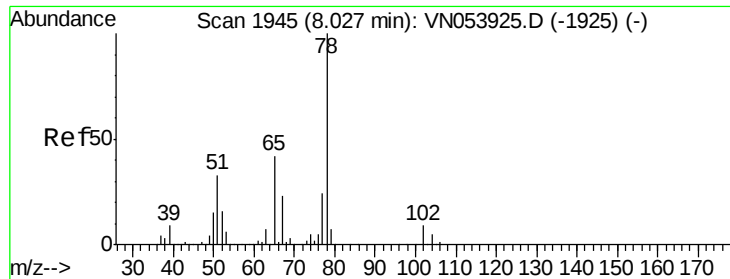





#33
 1,2-Dichloroethane-d4
 Concen: 56.910 ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Instrument :
 MSVOA_N
 ClientSampleId :
 SR-9-D

Tot Ion	Ratio	Resp	Lower	Upper
65	100	391715		
67	55.0	0.0	111.8	




Manual Integrations
 APPROVED


MMDadoda
 3/1/2019 4:10:21 PM

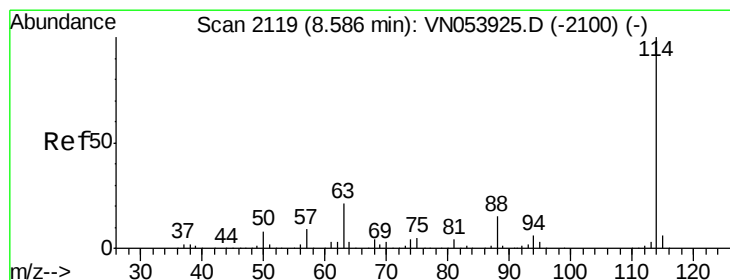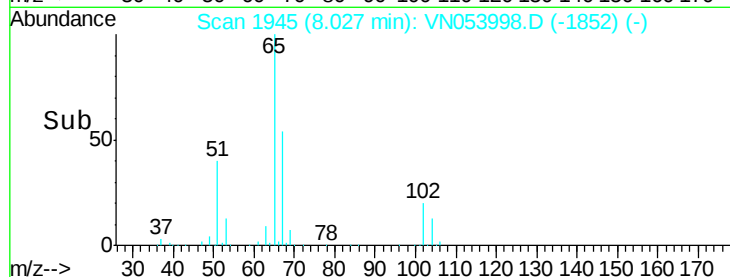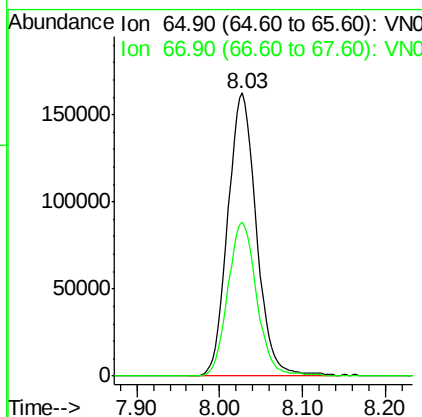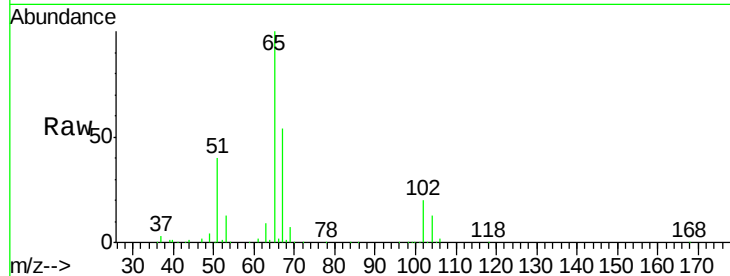

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Tgt Ion	Ratio	Resp	Lower	Upper
114	100	1086646		
63	21.1	0.0	37.4	
88	15.5	0.0	30.4	

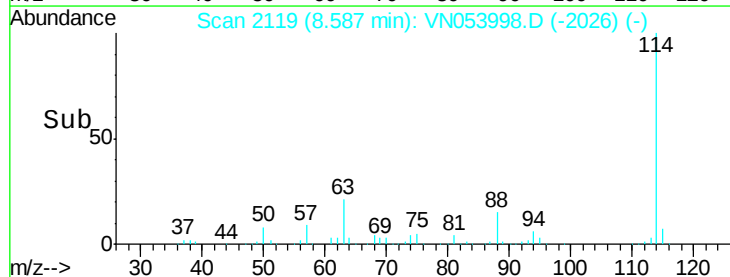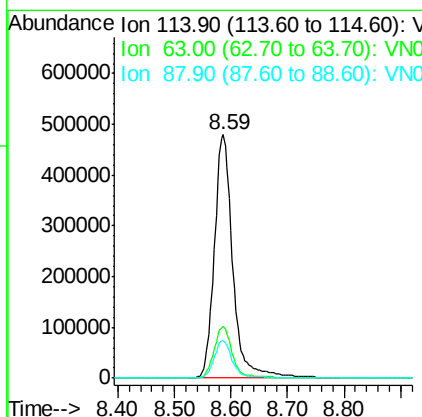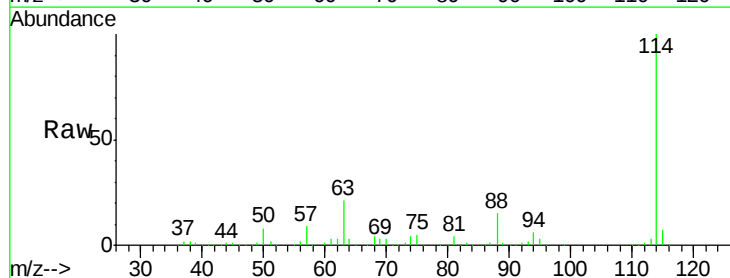

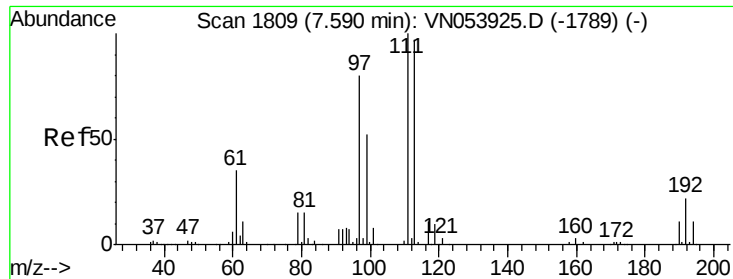





#35
 Dibromofluoromethane
 Concen: 51.248 ug/l
 RT: 7.59 min Scan# 1809
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Instrument :
 MSVOA_N
 ClientSampleId :
 SR-9-D

Tot Ion	Ratio	Resp	Lower	Upper
113	100	360114		
111	102.1	81.1	121.7	
192	21.6	18.8	28.2	




Manual Integrations
 APPROVED


MMDadoda
 3/1/2019 4:10:21 PM

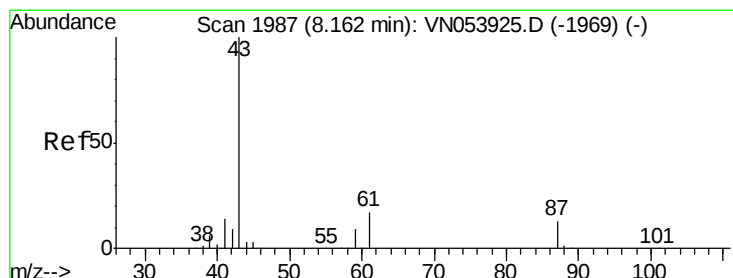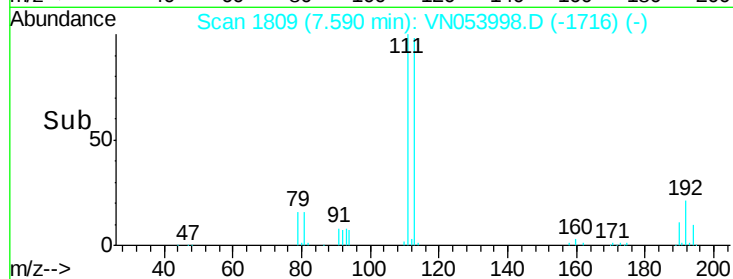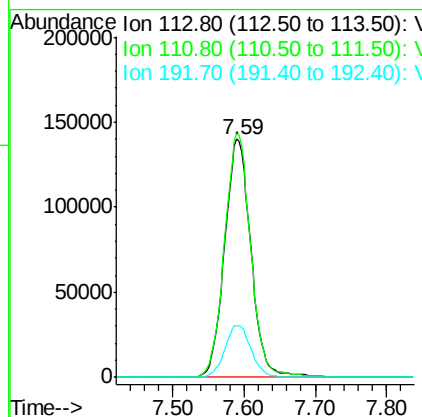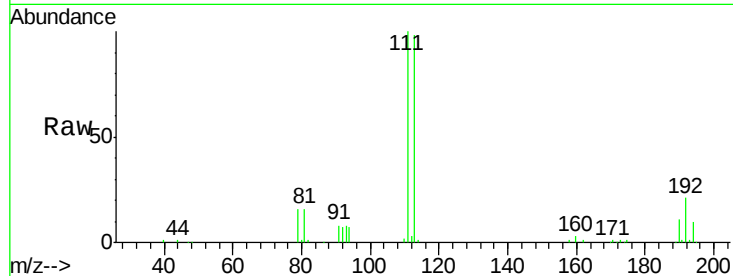

#43
 Isopropyl Acetate
 Concen: 2.340 ug/l m
 RT: 8.17 min Scan# 1988
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Tgt Ion	Ratio	Resp	Lower	Upper
43	100	28510		
61	0.0	17.4	26.0#	
87	0.0	11.5	17.3#	

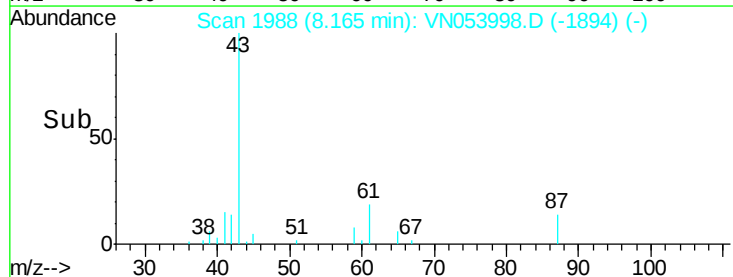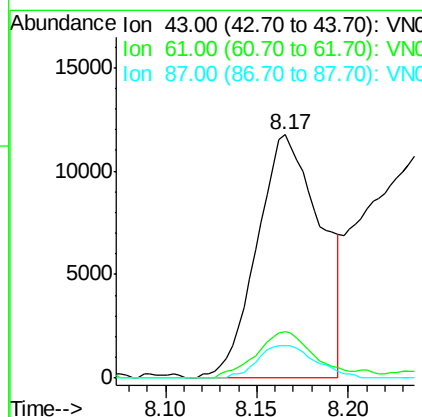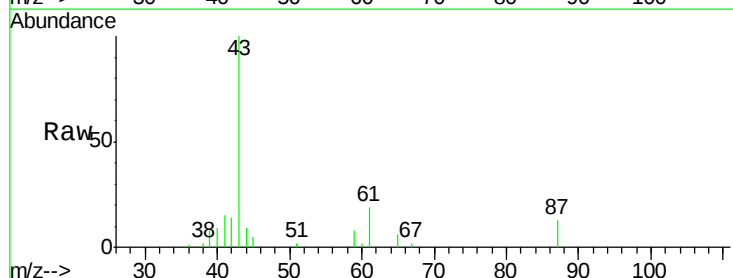

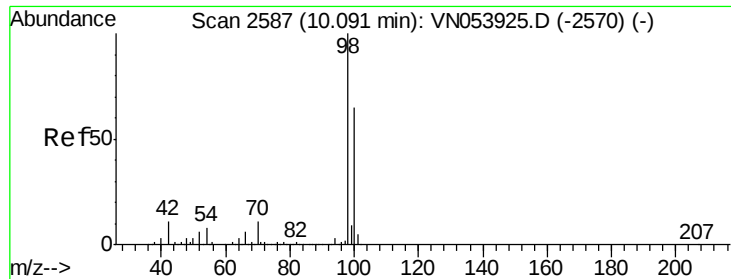

#50

Toluene-d8

Concen: 53.206 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN053998.D

Acq: 28 Feb 2019 12:33

Instrument :

MSVOA_N

ClientSampleId :

SR-9-D

Tot Ion: 98 Resp: 1391766





Ion Ratio Lower Upper

98 100

100 64.2 51.9 77.9

Manual Integrations
APPROVED

MMDadoda
3/1/2019 4:10:21 PM

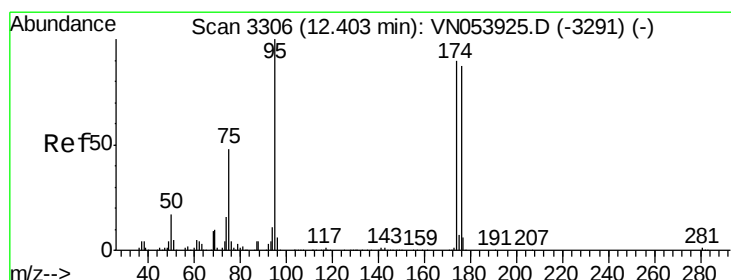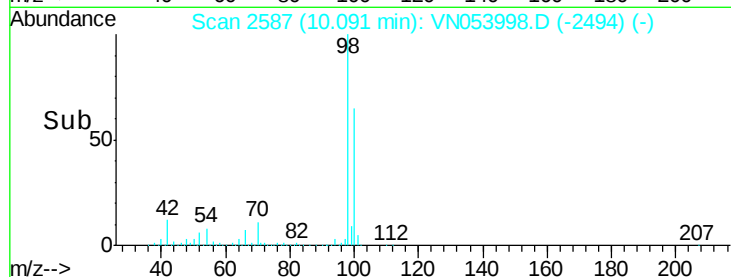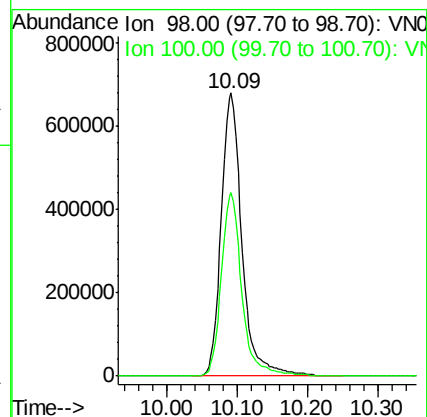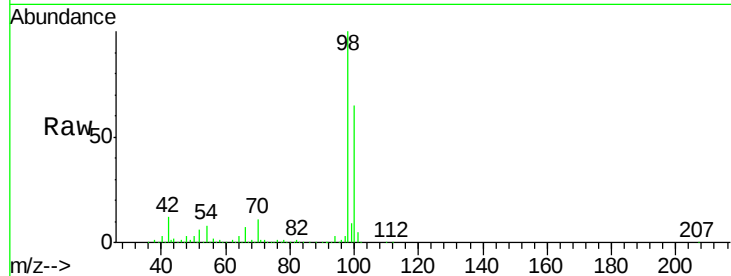

#62

4-Bromofluorobenzene

Concen: 52.686 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN053998.D

Acq: 28 Feb 2019 12:33




Tgt Ion: 95 Resp: 459164


Ion Ratio Lower Upper

95 100

174 87.7 0.0 188.8

176 84.2 0.0 182.6

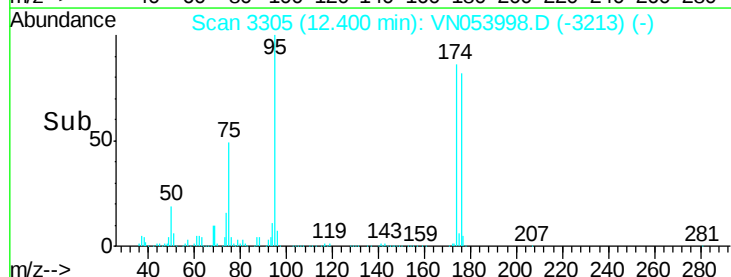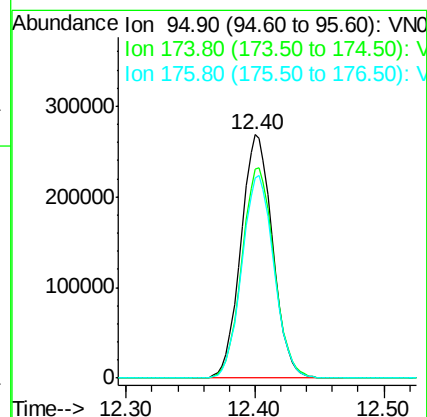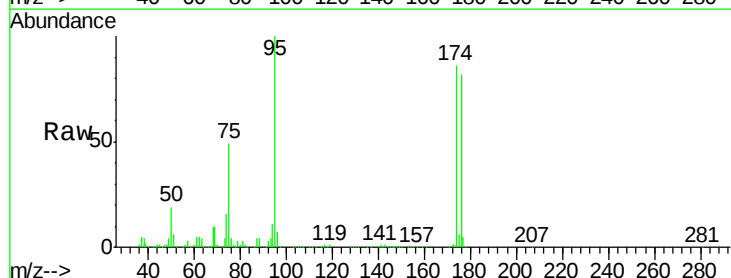

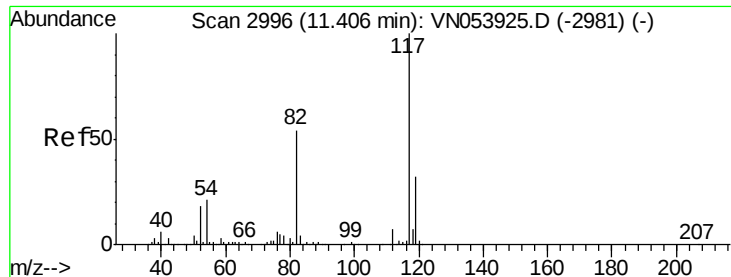





#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN053998.D
Acq: 28 Feb 2019 12:33

Instrument :
MSVOA_N
ClientSampled :
SR-9-D

Tot Ion	Ratio	Lower	Upper
117	100		
82	54.8	41.4	62.2
119	32.1	25.3	37.9




Manual Integrations
APPROVED


MMDadoda
3/1/2019 4:10:21 PM

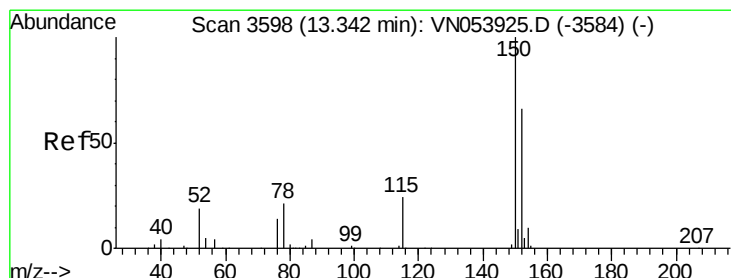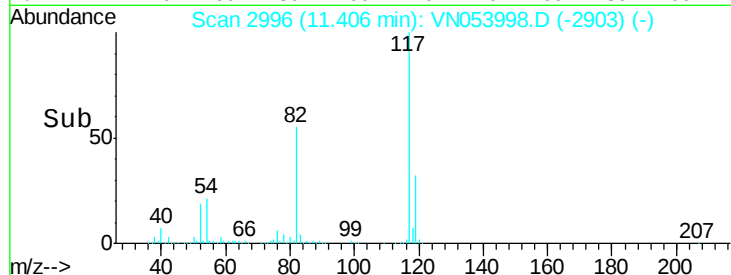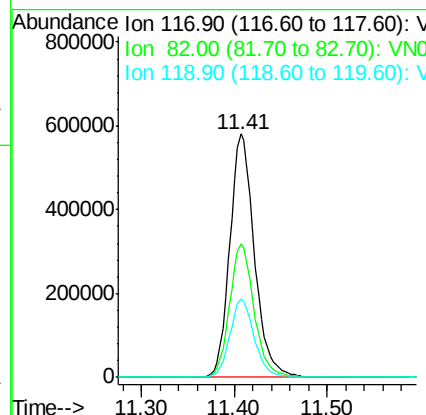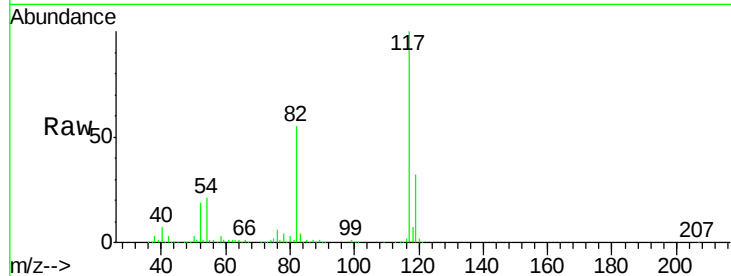

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN053998.D
Acq: 28 Feb 2019 12:33

Tgt Ion	Ratio	Lower	Upper
152	100		
115	57.3	27.2	81.6
150	156.5	0.0	348.2

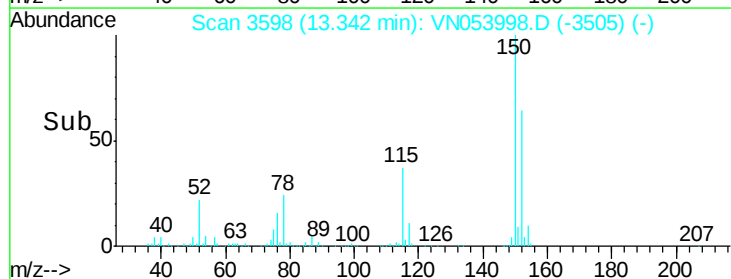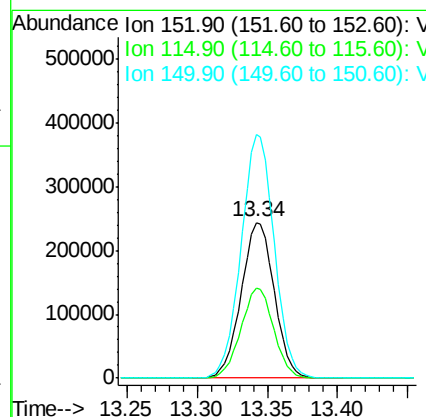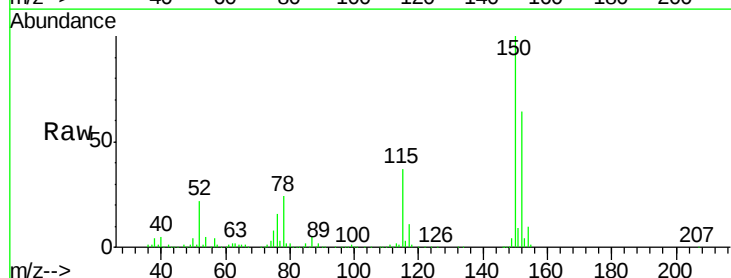

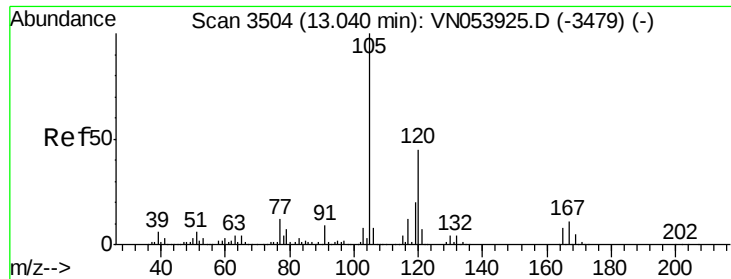





#84
 1,2,4-Trimethylbenzene
 Concen: 1.274 ug/l
 RT: 13.04 min Scan# 3504
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Instrument :
 MSVOA_N
 ClientSampleId :
 SR-9-D

Tot Ion	Ratio	Lower	Upper
105	100		
120	43.8	23.2	69.5

Manual Integrations
 APPROVED

MMDadoda
 3/1/2019 4:10:21 PM

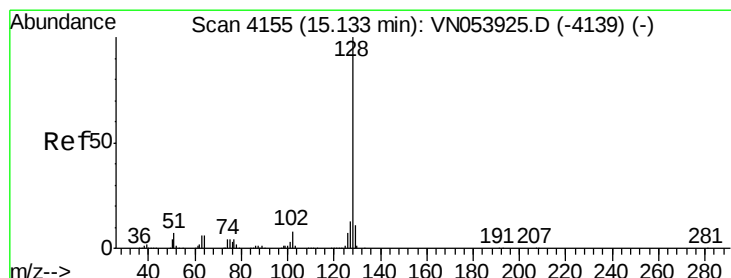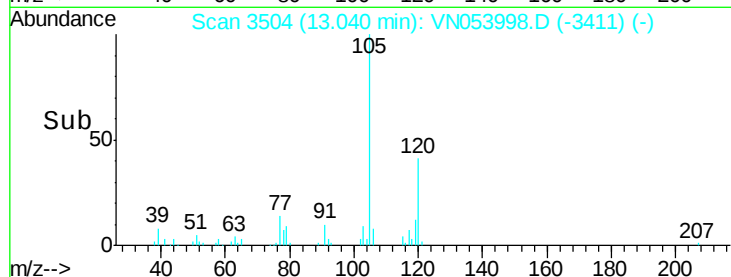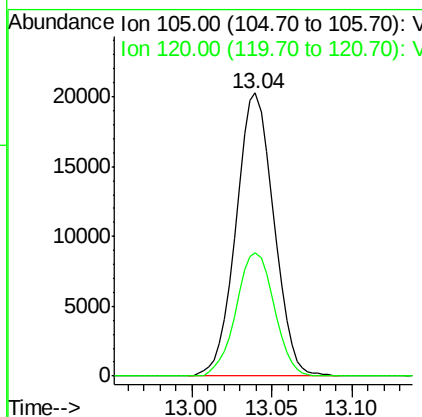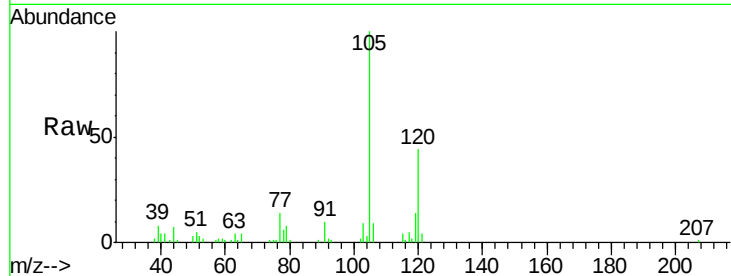

#95
 Naphthalene
 Concen: 10.423 ug/l
 RT: 15.13 min Scan# 4155
 Delta R.T. 0.00 min
 Lab File: VN053998.D
 Acq: 28 Feb 2019 12:33

Tgt Ion	Ratio	Lower	Upper
128	100		
127	13.4	10.2	15.2
129	11.3	8.6	12.8

