

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022822\
 Data File : VN071104.D
 Acq On : 28 Feb 2022 19:08
 Operator : JC\MD
 Sample : N1689-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-40

Quant Time: Mar 01 04:24:13 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 21 07:57:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	911745	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1452810	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1303817	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.668	152	466302	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.433	65	545950	52.419	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 104.840%			
35) Dibromofluoromethane	8.016	113	419211	48.512	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.020%			
50) Toluene-d8	10.439	98	1767955	50.946	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 101.900%			
62) 4-Bromofluorobenzene	12.727	95	613283	49.441	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 98.880%			
Target Compounds						Qvalue
3) Chloromethane	2.304	50	2858	0.240	ug/l #	87
11) Tert butyl alcohol	5.357	59	763233	402.109	ug/l	97
13) Acrolein	4.040	56	442	0.261	ug/l #	14
15) Acrylonitrile	5.604	53	3415	0.611	ug/l #	28
16) Acetone	4.293	43	19995	3.486	ug/l	99
18) Methyl Acetate	4.857	43	7191	Below Cal	#	51
19) Methyl tert-butyl Ether	5.616	73	273823	8.745	ug/l #	90
22) Diisopropyl ether	6.492	45	209187	6.407	ug/l	88
23) Vinyl Acetate	6.492	43	104820	3.793	ug/l #	72
25) 2-Butanone	7.345	43	3789	0.497	ug/l #	57
29) Tetrahydrofuran	7.686	42	4167	0.843	ug/l #	78
31) Cyclohexane	8.086	56	27317	1.517	ug/l #	41
36) 1,1-Dichloropropene	8.081	75	70701	4.994	ug/l #	49
38) Carbon Tetrachloride	8.081	117	89305	6.402	ug/l #	16
40) Benzene	8.457	78	2503774	59.788	ug/l	99
41) Methacrylonitrile	7.692	41	4401	0.550	ug/l #	39
43) Isopropyl Acetate	8.528	43	19309	0.807	ug/l #	55
51) 4-Methyl-2-Pentanone	10.322	43	3346	0.230	ug/l	97
52) Toluene	10.498	92	9503	0.361	ug/l	99
58) 2-Chloroethyl Vinyl ether	9.963	63	95	31.825	ug/l #	45
59) 2-Hexanone	11.127	43	16250	1.623	ug/l	89
67) Ethyl Benzene	11.839	91	23575	0.479	ug/l	100
68) m/p-Xylenes	11.951	106	9009	0.474	ug/l	99
69) o-Xylene	12.280	106	9842	0.530	ug/l	91
73) Isopropylbenzene	12.574	105	20382	0.543	ug/l	99
76) 1,2,3-Trichloropropane	12.727	75	312336	28.448	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	8124	0.267	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.727	75	312336	92.185	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	17743	0.593	ug/l	99
90) Hexachloroethane	14.280	117	2241	0.402	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.251	180	812	2.090	ug/l #	10
95) Naphthalene	15.498	128	20614	5.880	ug/l	97
96) 1,2,3-Trichlorobenzene	15.698	180	549	2.582	ug/l #	34

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Instrument :

MSVOA_N


ClientSampleId :


MW-40

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022822\
Data File : VN071104.D
Acq On : 28 Feb 2022 19:08
Operator : JC\MD
Sample : N1689-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Time: Mar 01 04:24:13 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 21 07:57:15 2022
Response via : Initial Calibration




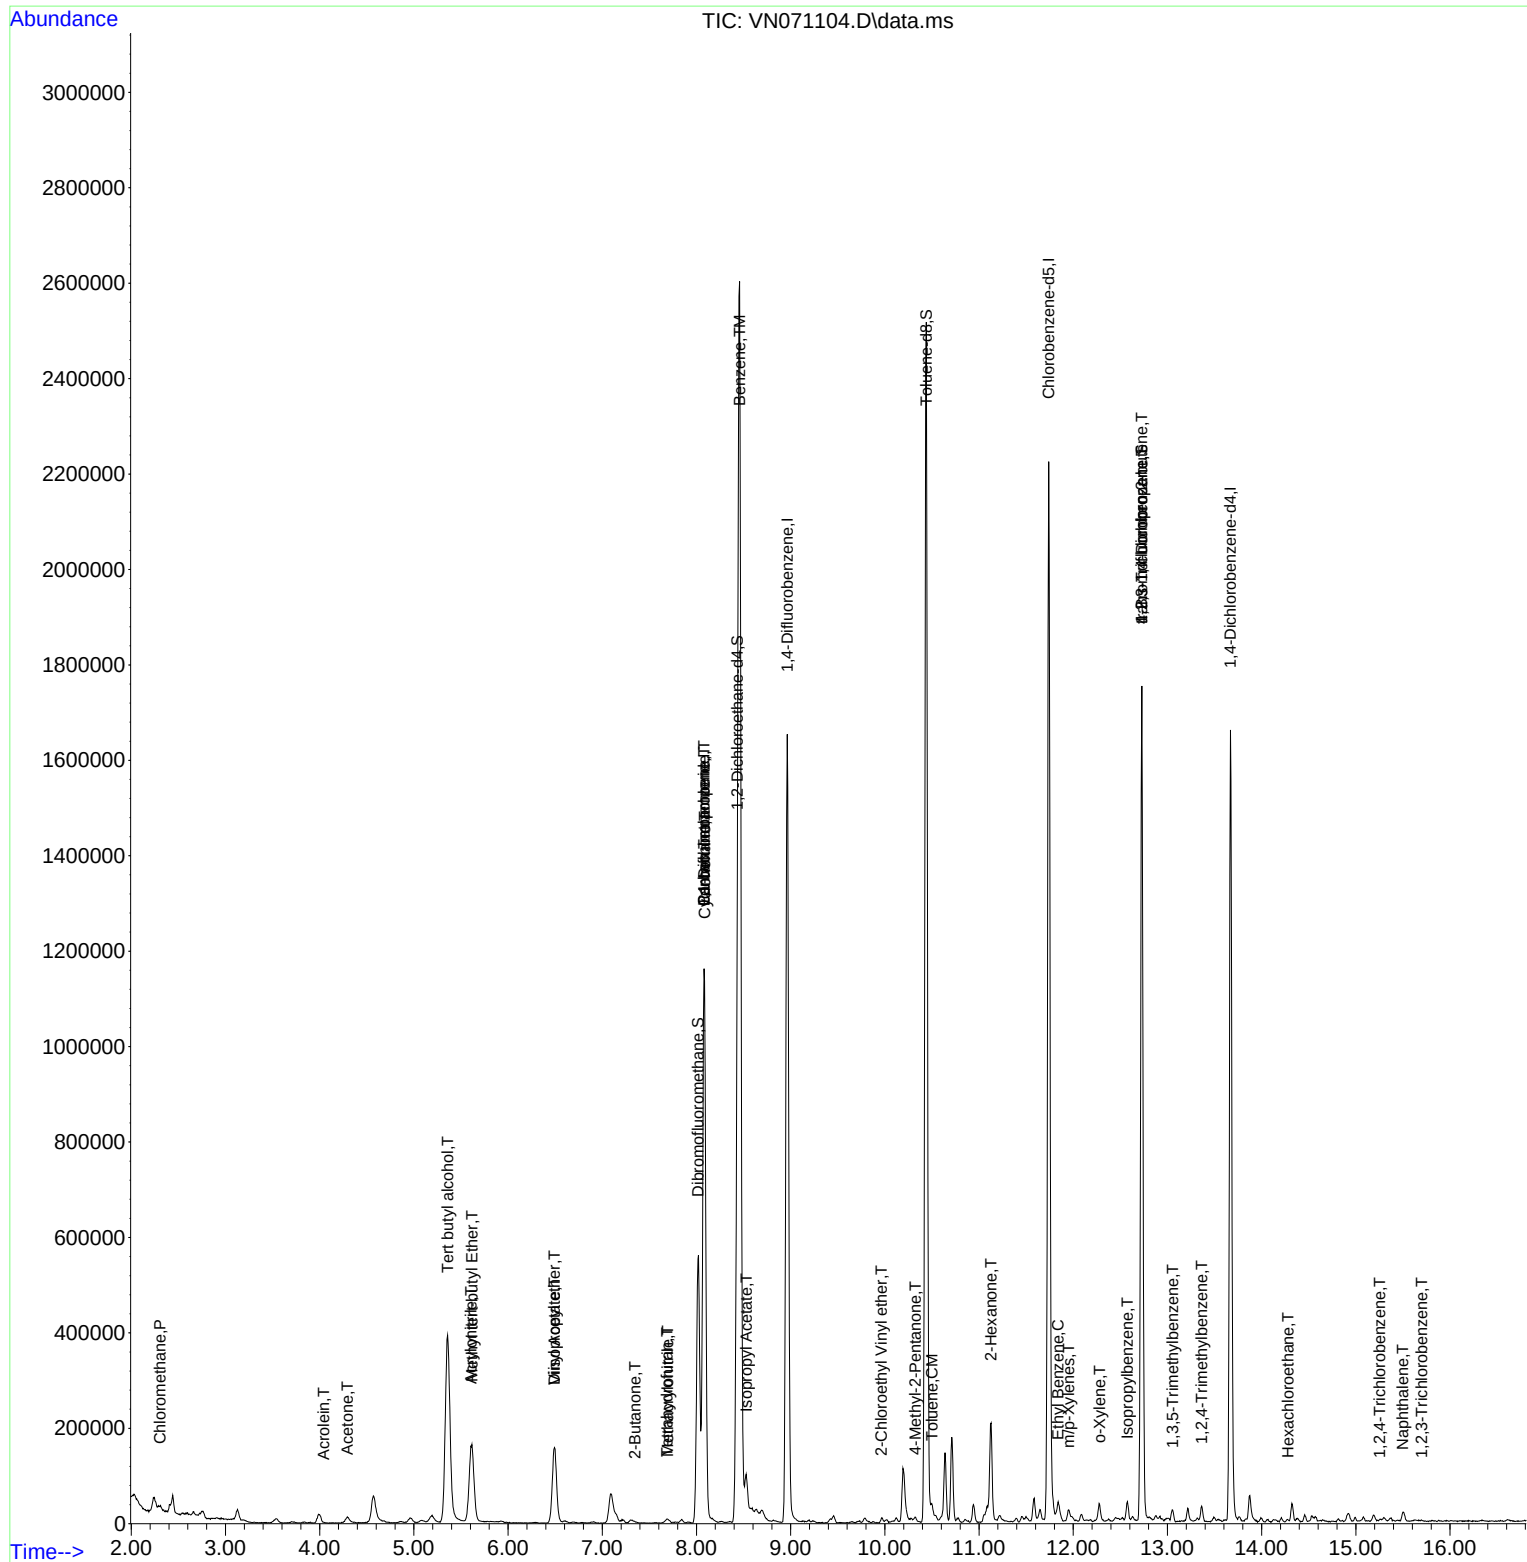




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 911745
Ion Ratio Lower Upper
168 100
99 55.9 41.3 61.9

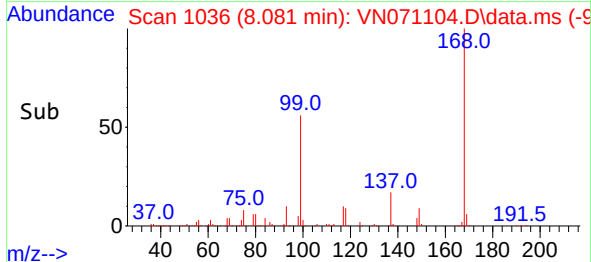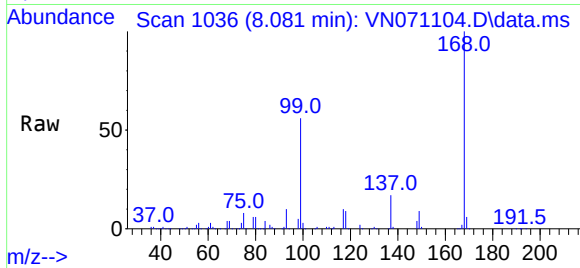

#3
Chloromethane
Concen: 0.240 ug/l
RT: 2.304 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 50 Resp: 2858
Ion Ratio Lower Upper
50 100
52 38.6 25.4 38.0#


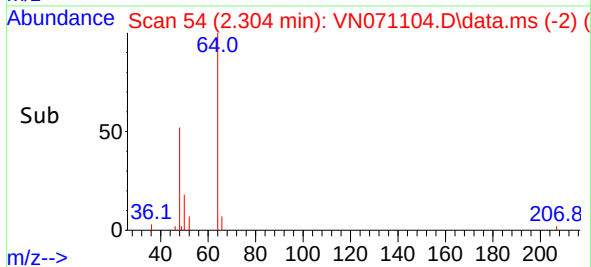

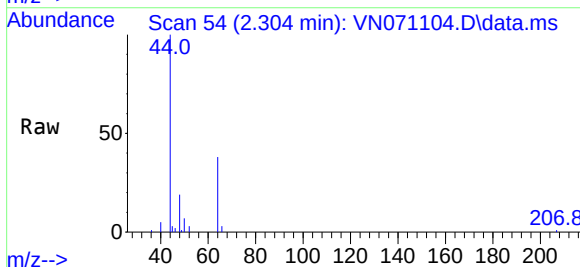




#11
Tert butyl alcohol
Concen: 402.109 ug/l
RT: 5.357 min Scan# 51
Delta R.T. -0.012 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 59 Resp: 763233
Ion Ratio Lower Upper
59 100
57 9.9 8.7 13.1

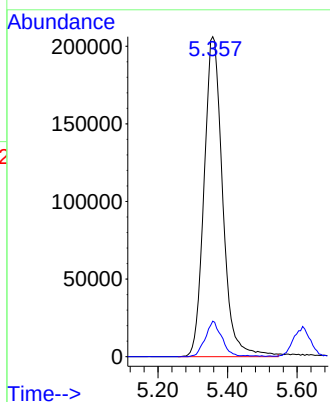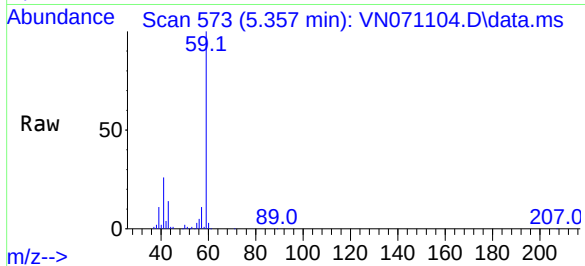

#13
Acrolein
Concen: 0.261 ug/l
RT: 4.040 min Scan# 349
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 56 Resp: 442
Ion Ratio Lower Upper
56 100
55 0.0 56.6 85.0#


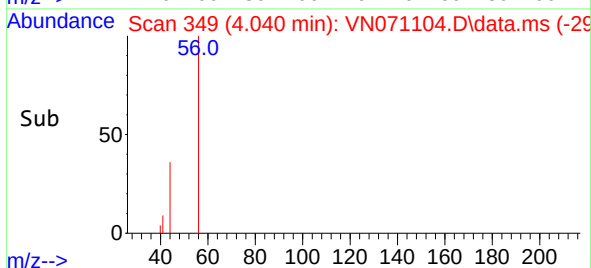

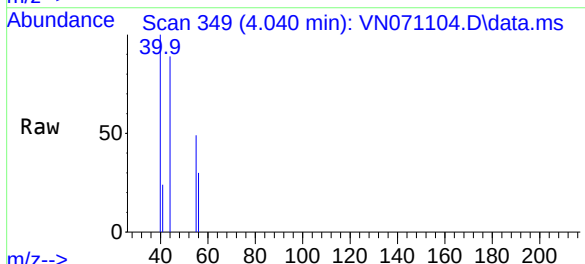




#15
Acrylonitrile
Concen: 0.611 ug/l
RT: 5.604 min Scan# 615
Delta R.T. 0.059 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 53 Resp: 3415
Ion Ratio Lower Upper
53 100
52 10.0 66.2 99.2#
51 67.6 29.6 44.4#

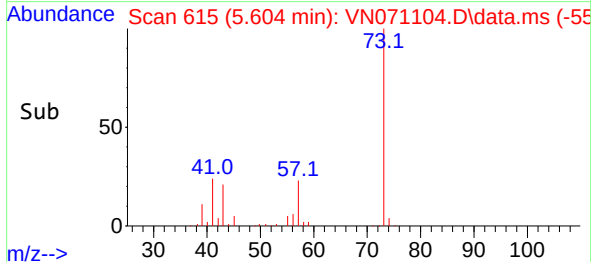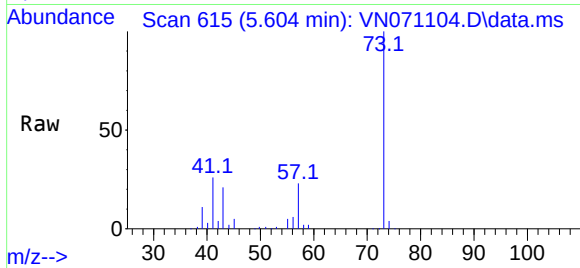

#16
Acetone
Concen: 3.486 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.012 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 43 Resp: 19995
Ion Ratio Lower Upper
43 100
58 28.5 23.1 34.7


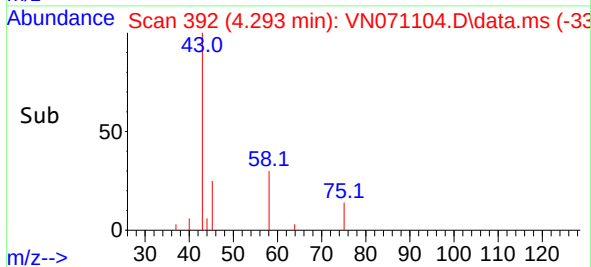

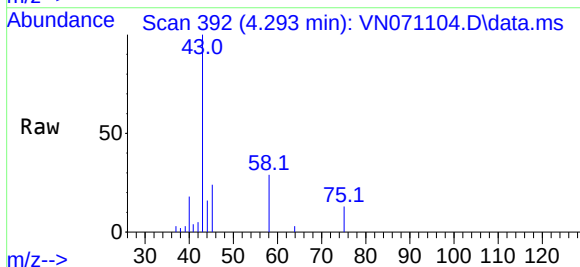




#19
Methyl tert-butyl Ether
Concen: 8.745 ug/l
RT: 5.616 min Scan# 616
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 73 Resp: 273823
Ion Ratio Lower Upper
73 100
57 25.8 16.8 25.2#

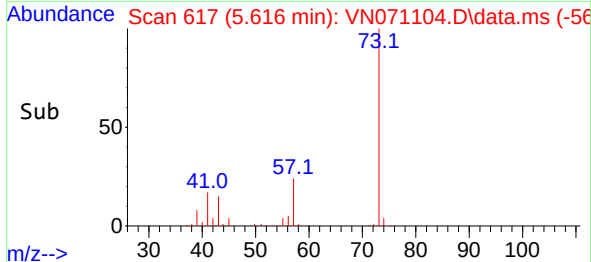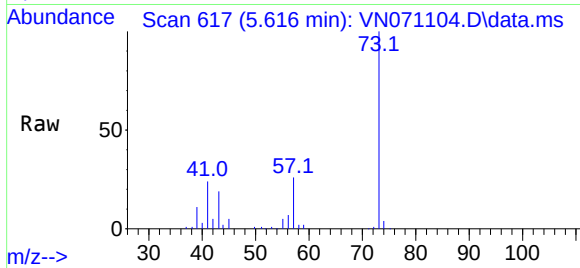

#22
Diisopropyl ether
Concen: 6.407 ug/l
RT: 6.492 min Scan# 766
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 45 Resp: 209187
Ion Ratio Lower Upper
45 100
43 53.6 51.7 77.5
87 23.5 23.2 34.8
59 9.6 9.4 14.0


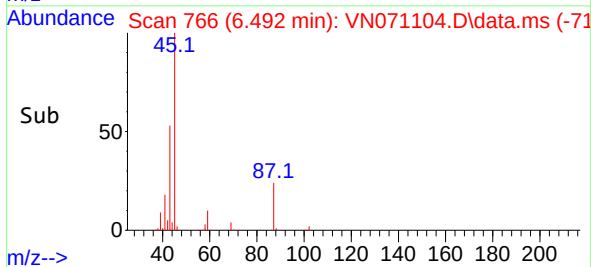

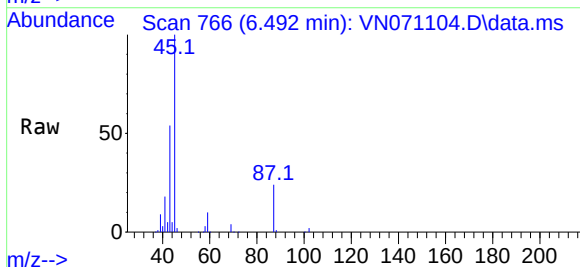




#23
Vinyl Acetate
Concen: 3.793 ug/l
RT: 6.492 min Scan# 70
Delta R.T. 0.065 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 104820
Ion Ratio Lower Upper
43 100
86 0.0 8.5 12.7#



#25
2-Butanone
Concen: 0.497 ug/l
RT: 7.345 min Scan# 911
Delta R.T. 0.018 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 43 Resp: 3789
Ion Ratio Lower Upper
43 100
72 49.2 21.7 32.5#

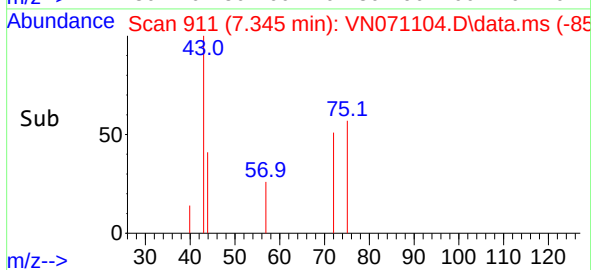



#29

Tetrahydrofuran

Concen: 0.843 ug/l

RT: 7.686 min Scan# 9

Delta R.T. 0.006 min

Lab File: VN071104.D

Acq: 28 Feb 2022 19:08

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion: 42 Resp: 4167

Ion Ratio Lower Upper

42 100

72 38.5 36.3 54.5

71 21.0 34.7 52.1#

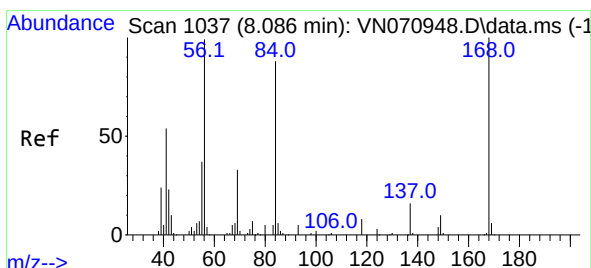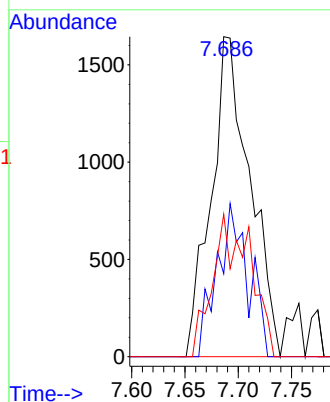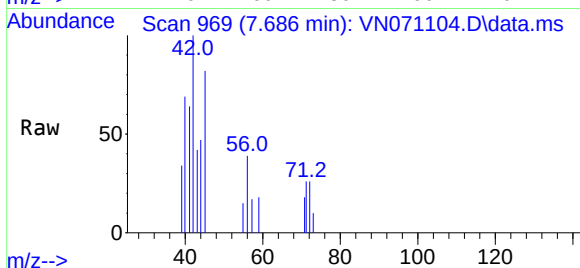

#31

Cyclohexane

Concen: 1.517 ug/l

RT: 8.086 min Scan# 1037

Delta R.T. -0.000 min

Lab File: VN071104.D

Acq: 28 Feb 2022 19:08




Tgt Ion: 56 Resp: 27317


Ion Ratio Lower Upper

56 100

69 125.7 27.1 40.7#

84 112.6 73.4 110.0#


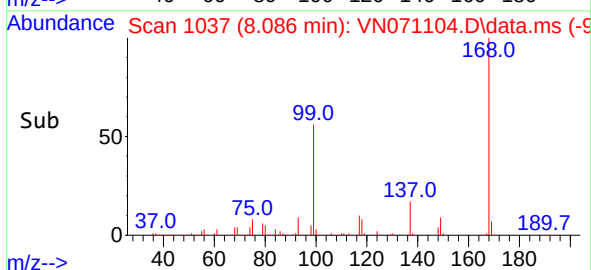

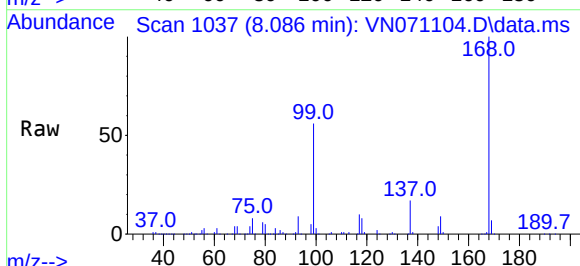


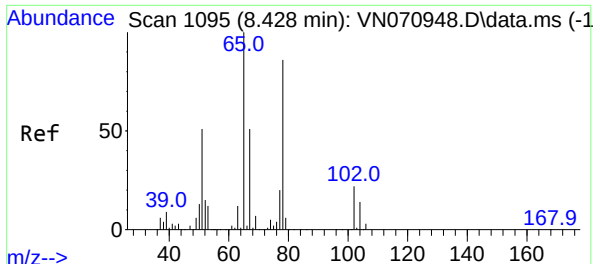

#33
1,2-Dichloroethane-d4
Concen: 52.419 ug/l
RT: 8.433 min Scan# 1095
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 65 Resp: 545950
Ion Ratio Lower Upper
65 100
67 52.7 0.0 103.0

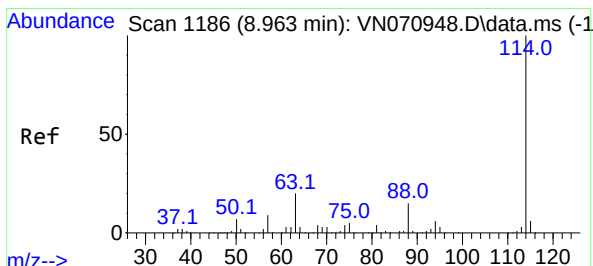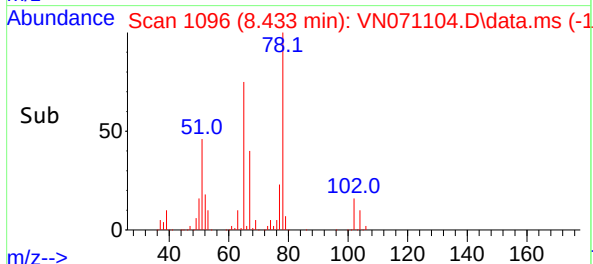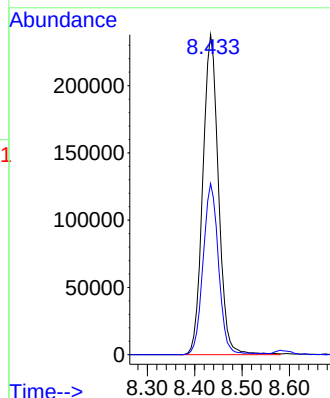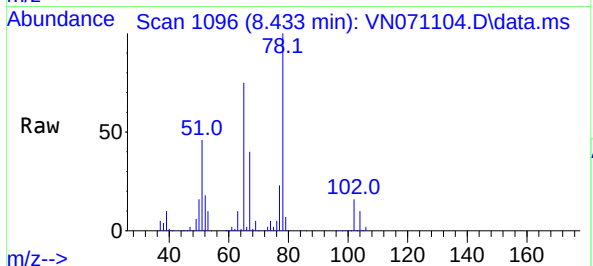

#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 114 Resp: 1452810
Ion Ratio Lower Upper
114 100
63 21.5 0.0 37.8
88 15.9 0.0 27.4


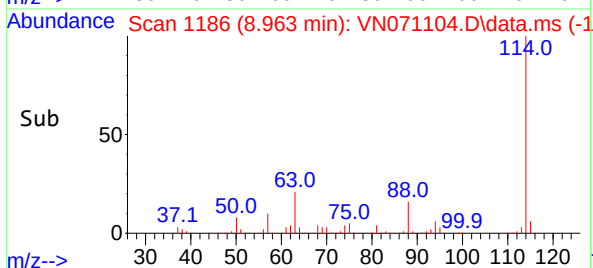

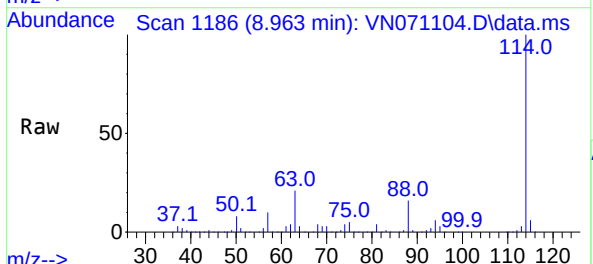


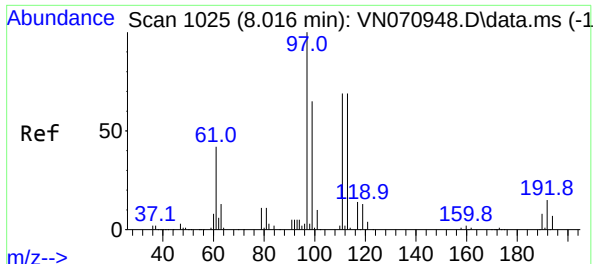

#35
Dibromofluoromethane
Concen: 48.512 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:113 Resp: 419211
Ion Ratio Lower Upper
113 100
111 103.1 82.2 123.2
192 20.4 16.9 25.3

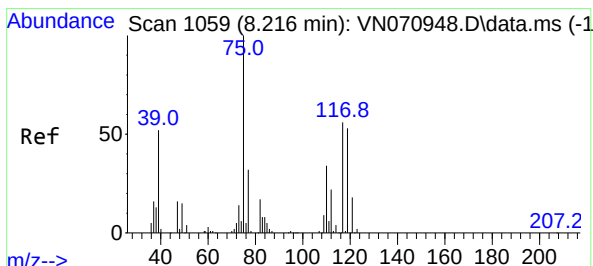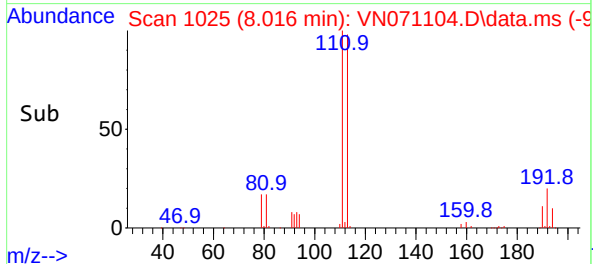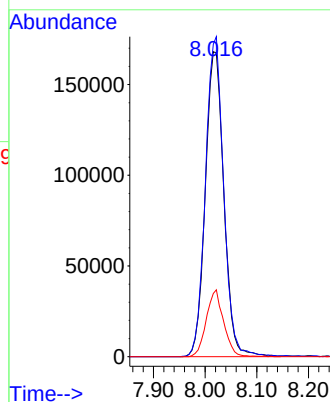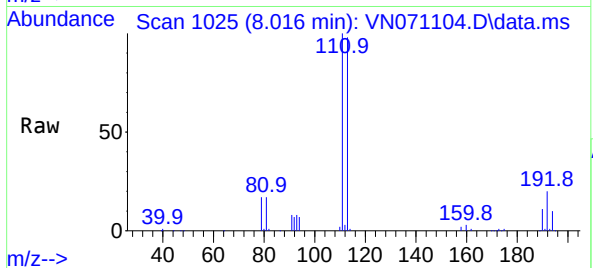

#36
1,1-Dichloropropene
Concen: 4.994 ug/l
RT: 8.081 min Scan# 1036
Delta R.T. -0.135 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 75 Resp: 70701
Ion Ratio Lower Upper
75 100
110 9.3 18.4 55.2#
77 0.0 24.4 36.6#


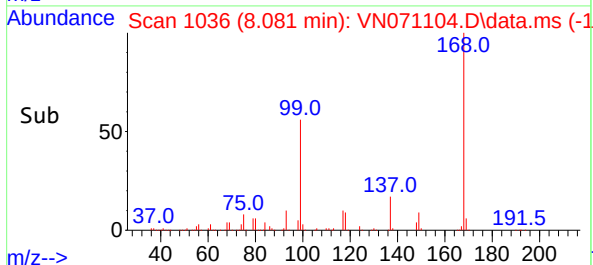

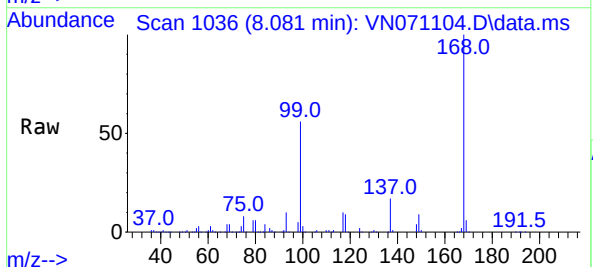


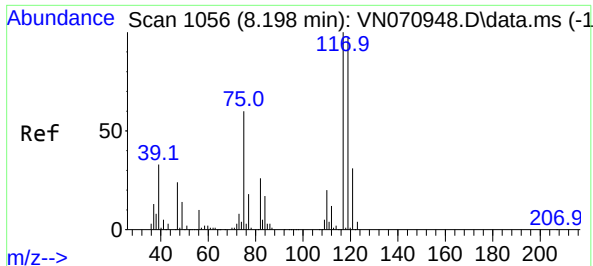

#38
Carbon Tetrachloride
Concen: 6.402 ug/l
RT: 8.081 min Scan# 1100
Delta R.T. -0.118 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 89305
Ion Ratio Lower Upper
117 100
119 5.0 76.1 114.1#
121 0.0 24.2 36.2#

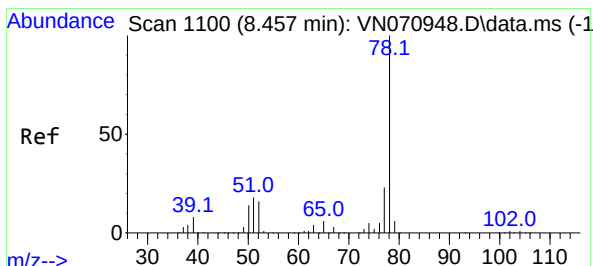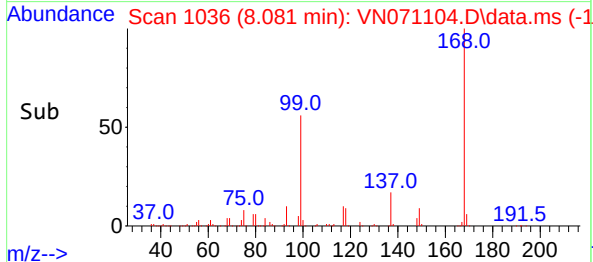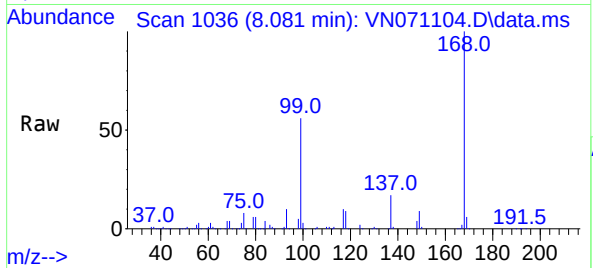

#40
Benzene
Concen: 59.788 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 78 Resp: 2503774
Ion Ratio Lower Upper
78 100
77 23.6 18.6 27.8


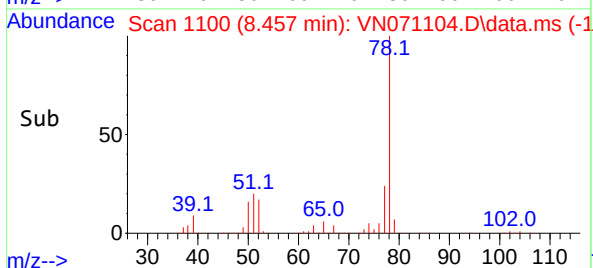
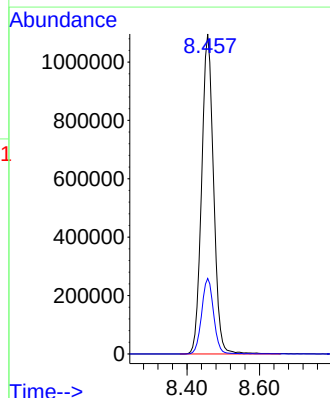
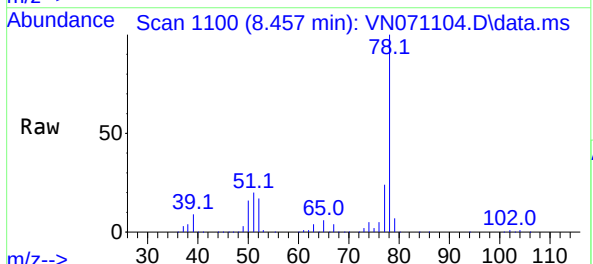




#41
Methacrylonitrile
Concen: 0.550 ug/l
RT: 7.692 min Scan# 91
Delta R.T. 0.065 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:	41	Resp:	4401
Ion	Ratio	Lower	Upper
41	100		
39	49.1	48.1	72.1
67	0.0	68.3	102.5#
52	0.0	29.6	44.4#

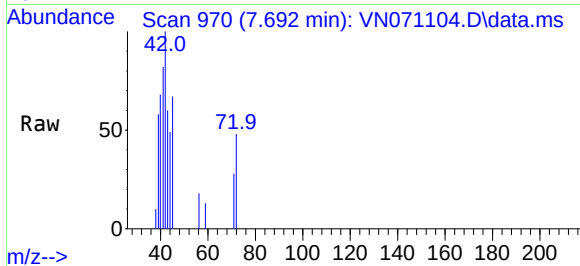

#43
Isopropyl Acetate
Concen: 0.807 ug/l
RT: 8.528 min Scan# 1112
Delta R.T. -0.029 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion:	43	Resp:	19309
Ion	Ratio	Lower	Upper
43	100		
61	0.0	20.4	30.6#
87	0.0	11.2	16.8#


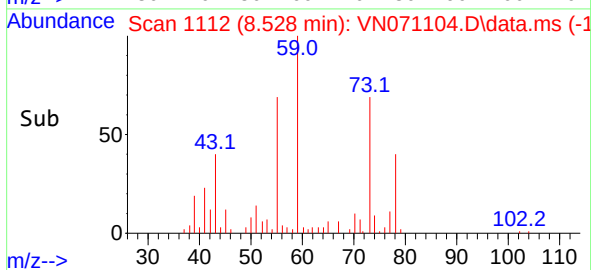

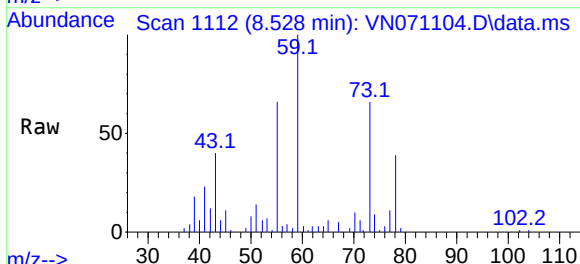




#50
Toluene-d8
Concen: 50.946 ug/l
RT: 10.439 min Scan# 1436
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 98 Resp: 1767955
Ion Ratio Lower Upper
98 100
100 65.6 50.4 75.6

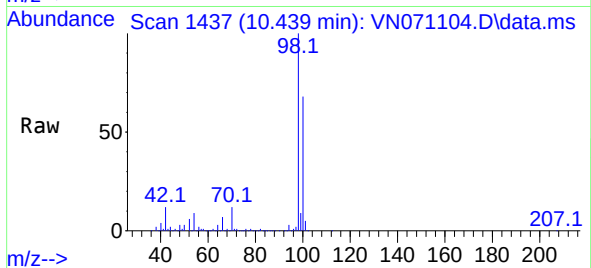

#51
4-Methyl-2-Pentanone
Concen: 0.230 ug/l
RT: 10.322 min Scan# 1417
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 43 Resp: 3346
Ion Ratio Lower Upper
43 100
58 40.1 30.4 45.6


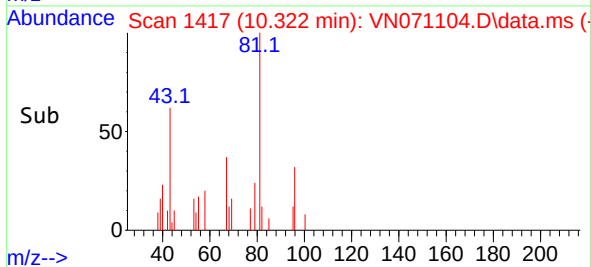

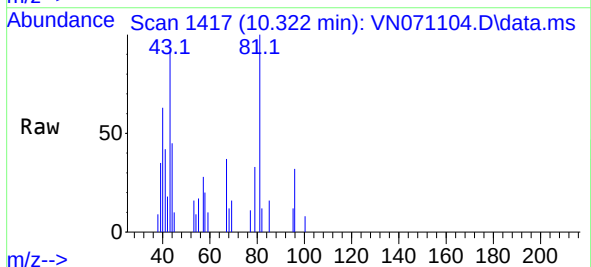




#52
Toluene
Concen: 0.361 ug/l
RT: 10.498 min Scan# 1447
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 92 Resp: 9503
Ion Ratio Lower Upper
92 100
91 175.9 142.0 213.0

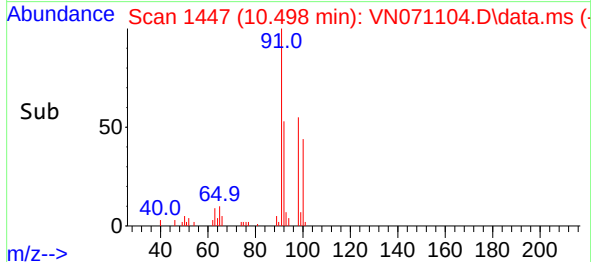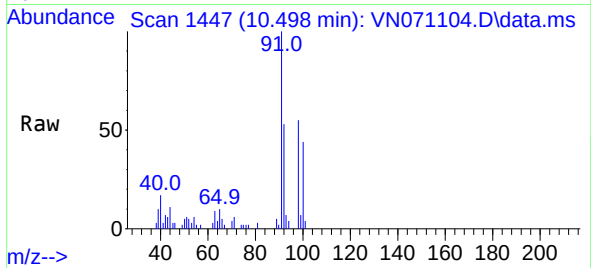

#58
2-Chloroethyl Vinyl ether
Concen: 31.825 ug/l
RT: 9.963 min Scan# 1356
Delta R.T. -0.070 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 63 Resp: 95
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


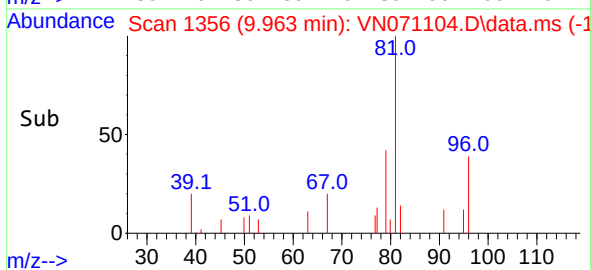






#59
2-Hexanone
Concen: 1.623 ug/l
RT: 11.127 min Scan# 11
Delta R.T. 0.047 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 16250
Ion Ratio Lower Upper
43 100
58 61.8 26.9 80.7

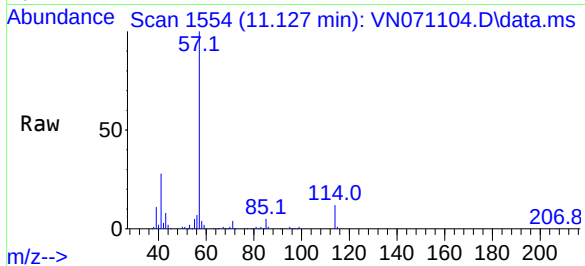

#62
4-Bromofluorobenzene
Concen: 49.441 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 95 Resp: 613283
Ion Ratio Lower Upper
95 100
174 79.8 0.0 187.2
176 77.6 0.0 181.4


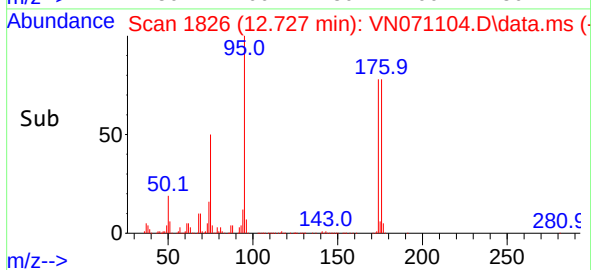

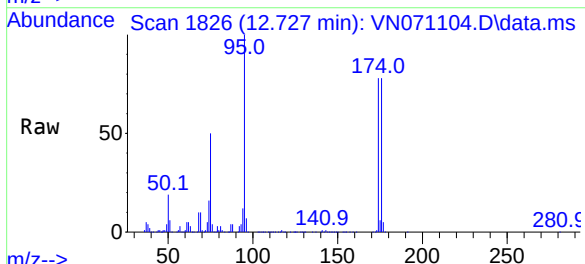




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 1303817
Ion Ratio Lower Upper
117 100
82 57.0 42.4 63.6
119 31.9 25.4 38.2

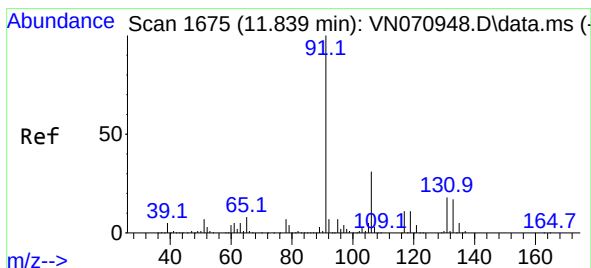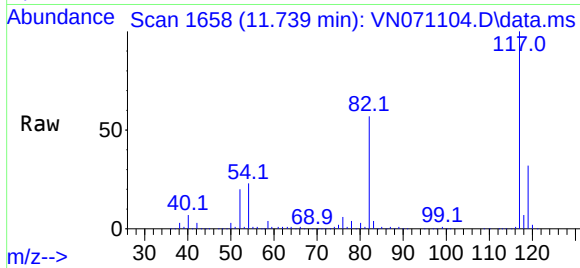

#67
Ethyl Benzene
Concen: 0.479 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 91 Resp: 23575
Ion Ratio Lower Upper
91 100
106 32.1 25.7 38.5


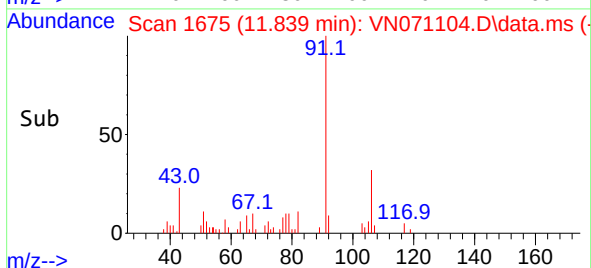

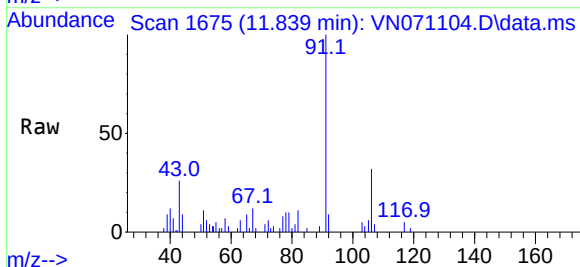




#68
m/p-Xylenes
Concen: 0.474 ug/l
RT: 11.951 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:106 Resp: 9009
Ion Ratio Lower Upper
106 100
91 202.8 160.6 240.8

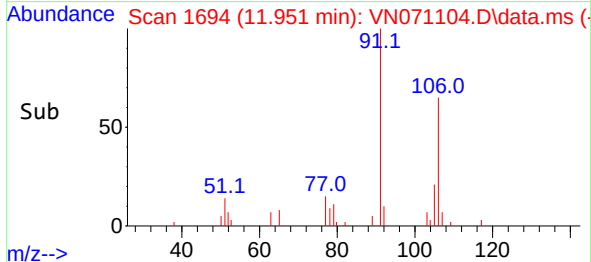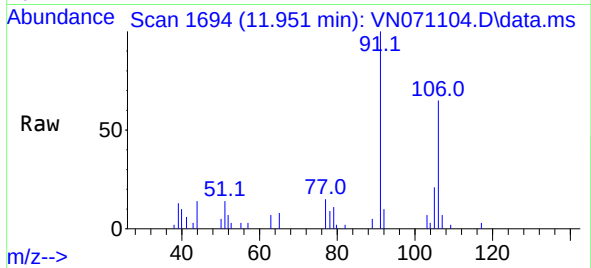

#69
o-Xylene
Concen: 0.530 ug/l
RT: 12.280 min Scan# 1750
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion:106 Resp: 9842
Ion Ratio Lower Upper
106 100
91 225.9 105.8 317.3


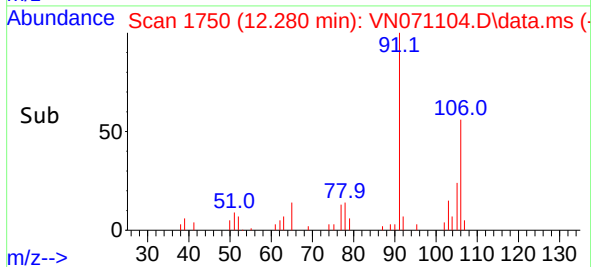

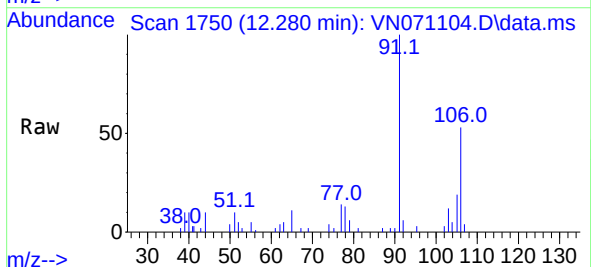




#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.668 min Scan# 1986
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:152 Resp: 466302
Ion Ratio Lower Upper
152 100
115 58.6 27.5 82.5
150 157.1 0.0 344.4



#73
Isopropylbenzene
Concen: 0.543 ug/l
RT: 12.574 min Scan# 1800
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion:105 Resp: 20382
Ion Ratio Lower Upper
105 100
120 26.4 13.4 40.1


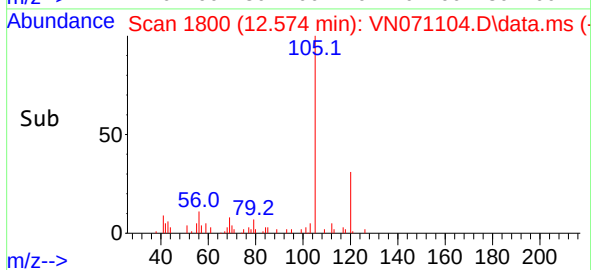






#76
1,2,3-Trichloropropane
Concen: 28.448 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.141 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 312336
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#

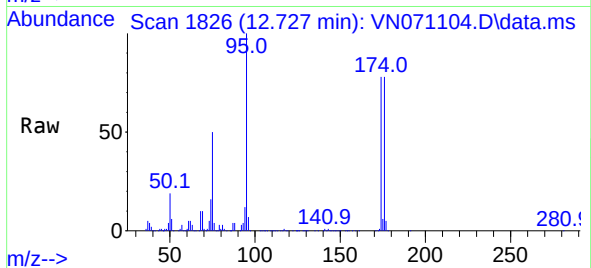

#80
1,3,5-Trimethylbenzene
Concen: 0.267 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 105 Resp: 8124
Ion Ratio Lower Upper
105 100
120 55.1 24.6 73.6


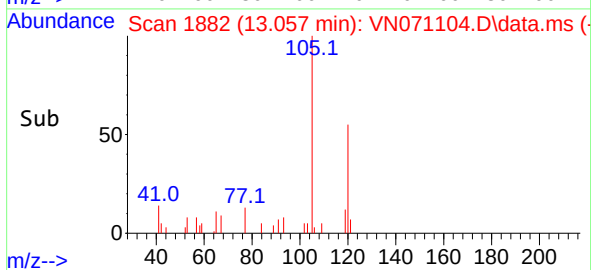




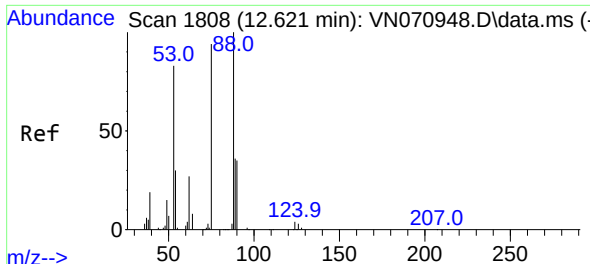

#81
trans-1,4-Dichloro-2-butene
Concen: 92.185 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 312336
Ion Ratio Lower Upper
75 100
53 0.2 90.5 135.7#
89 0.0 38.2 57.4#

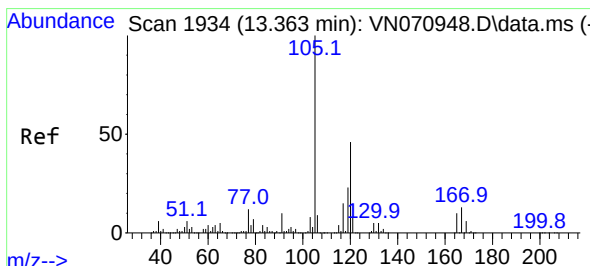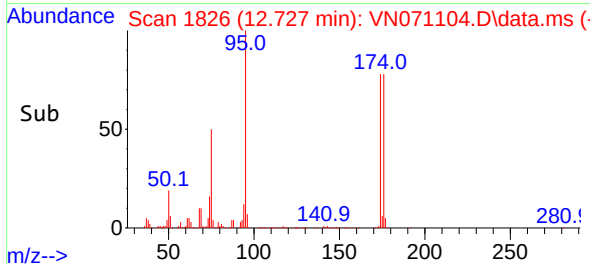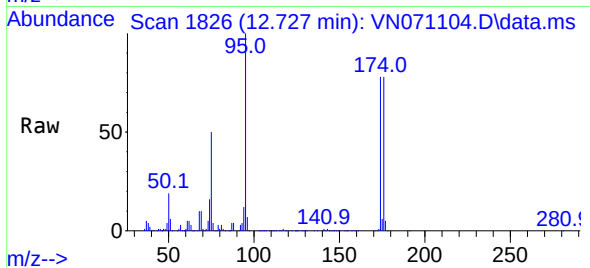

#84
1,2,4-Trimethylbenzene
Concen: 0.593 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion: 105 Resp: 17743
Ion Ratio Lower Upper
105 100
120 46.5 22.8 68.4


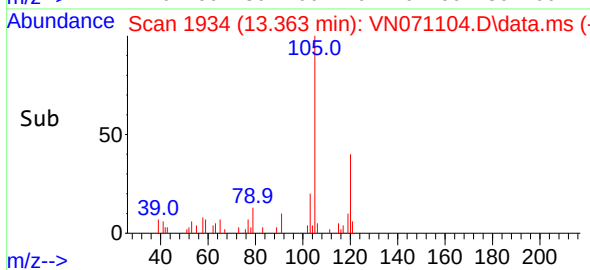

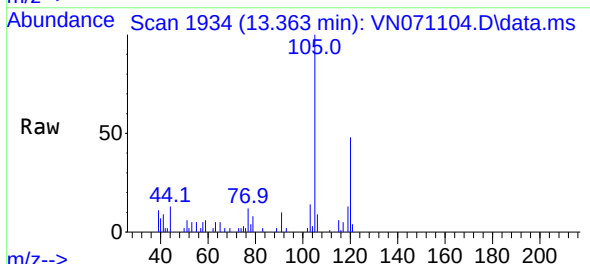




#90
Hexachloroethane
Concen: 0.402 ug/l
RT: 14.280 min Scan# 2077
Delta R.T. 0.076 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 2241
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

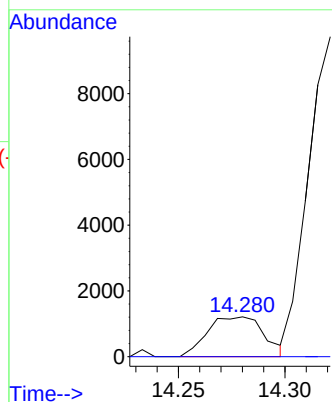

#93
1,2,4-Trichlorobenzene
Concen: 2.090 ug/l
RT: 15.251 min Scan# 2255
Delta R.T. -0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion:180 Resp: 812
Ion Ratio Lower Upper
180 100
182 88.1 48.3 144.9
145 221.6 14.5 43.5#


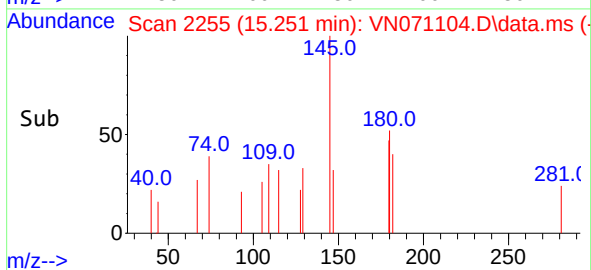






#95
Naphthalene
Concen: 5.880 ug/l
RT: 15.498 min Scan# 2297
Delta R.T. -0.000 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Tgt Ion:	128	Resp:	20614
Ion	Ratio	Lower	Upper
128	100		
127	14.7	10.5	15.7
129	11.9	8.7	13.1



#96
1,2,3-Trichlorobenzene
Concen: 2.582 ug/l
RT: 15.698 min Scan# 2331
Delta R.T. 0.006 min
Lab File: VN071104.D
Acq: 28 Feb 2022 19:08

Tgt Ion:	180	Resp:	549
Ion	Ratio	Lower	Upper
180	100		
182	161.7	47.4	142.2#
145	0.0	15.0	45.1#

