

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022823\
 Data File : VN076824.D
 Acq On : 28 Feb 2023 13:34
 Operator : JC\MD
 Sample : VN0228MBL01
 Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0228MBL01

Quant Time: Mar 01 01:25:33 2023
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
 Quant Title : SW846 8260
 QLast Update : Tue Feb 14 01:44:47 2023
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.231	168	279698	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.107	114	497561	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.866	117	439949	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.795	152	168547	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	199538	51.664	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	103.320%
35) Dibromofluoromethane	8.172	113	158503	48.644	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	97.280%
50) Toluene-d8	10.566	98	601442	49.425	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	98.840%
62) 4-Bromofluorobenzene	12.854	95	179160	44.453	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	88.900%


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022823\
Data File : VN076824.D
Acq On : 28 Feb 2023 13:34
Operator : JC\MD
Sample : VN0228MBL01
Misc : 5.00g/10mL/100uL/5.00mL/MSVOA_N/MEOH
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0228MBL01

Quant Time: Mar 01 01:25:33 2023
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Quant Title : SW846 8260
QLast Update : Tue Feb 14 01:44:47 2023
Response via : Initial Calibration




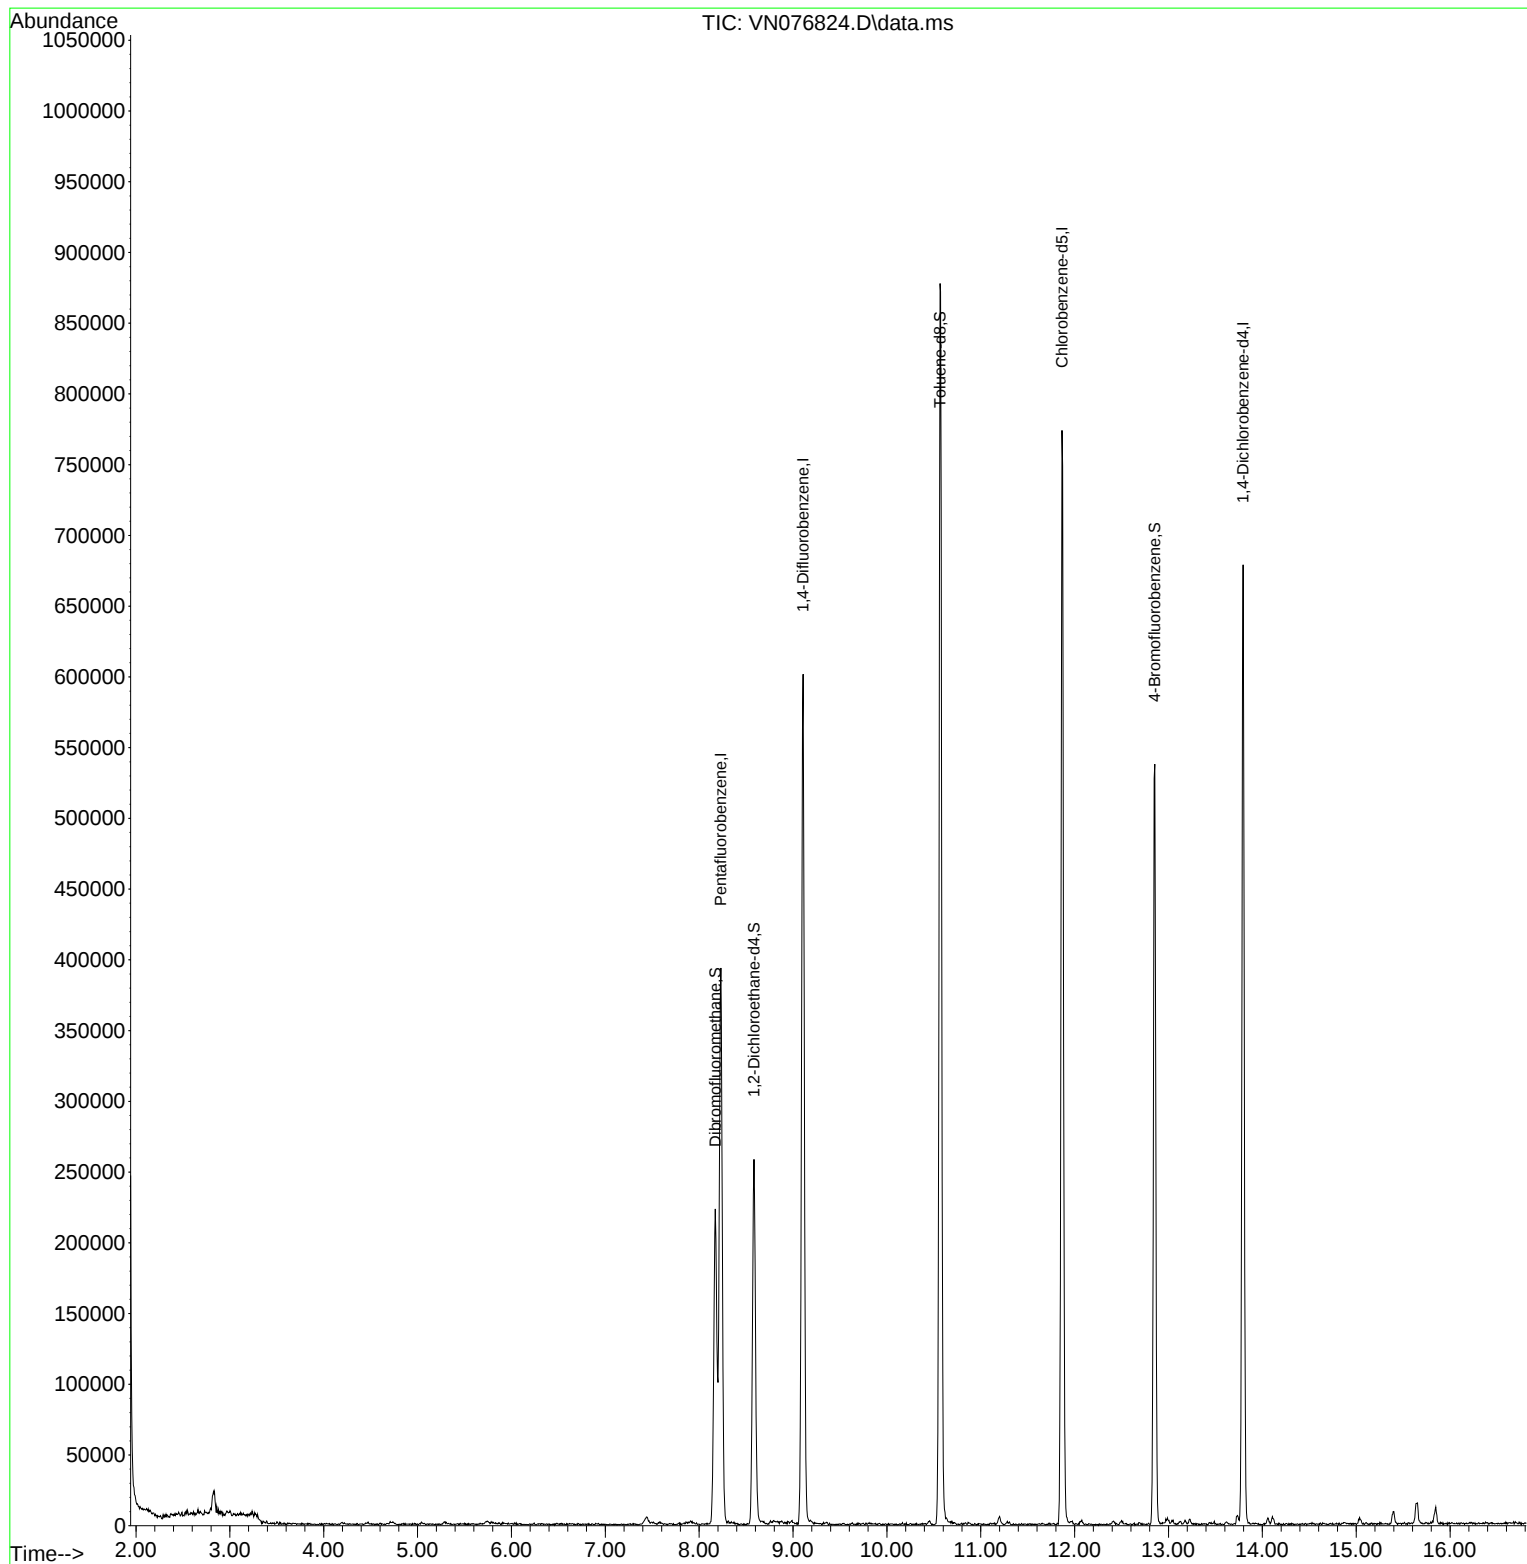


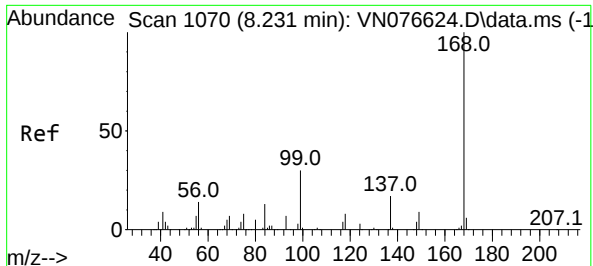

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.231 min Scan# 1107
Delta R.T. -0.000 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34




Instrument :
MSVOA_N
ClientSampleId :
VN0228MBL01


Tgt Ion:168 Resp: 279698
Ion Ratio Lower Upper
168 100
99 55.9 44.8 67.2

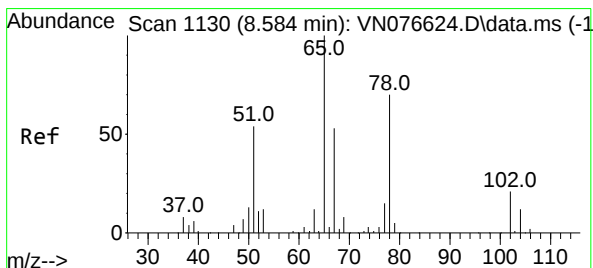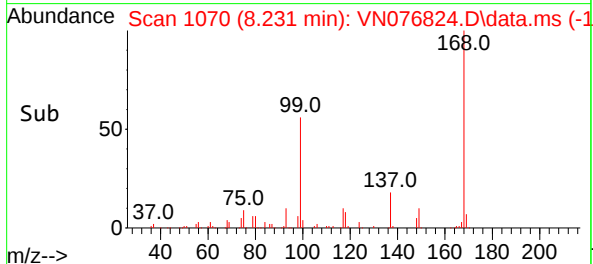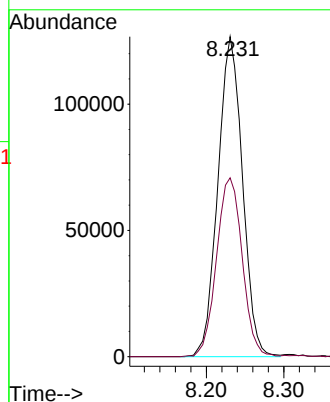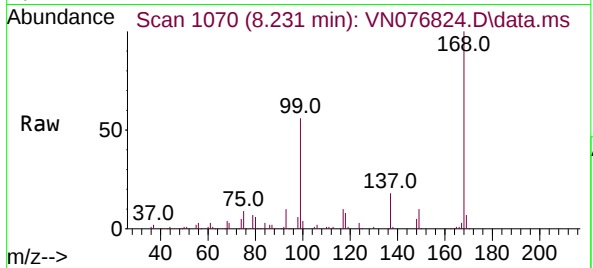

#33
1,2-Dichloroethane-d4
Concen: 51.664 ug/l
RT: 8.583 min Scan# 1130
Delta R.T. -0.001 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34

Tgt Ion: 65 Resp: 199538
Ion Ratio Lower Upper
65 100
67 51.6 0.0 105.6

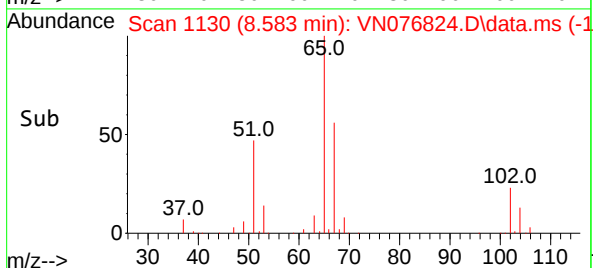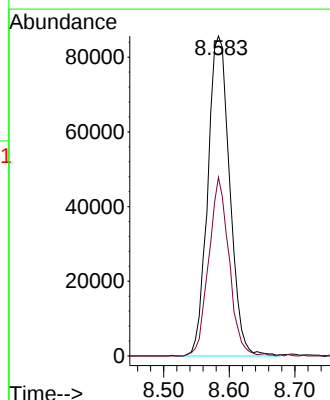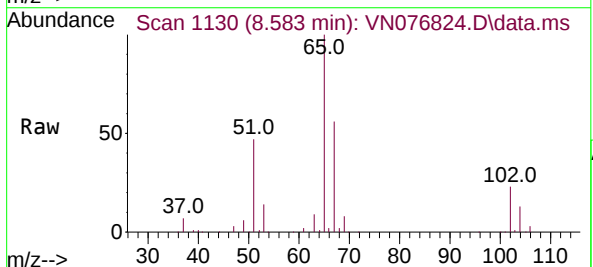

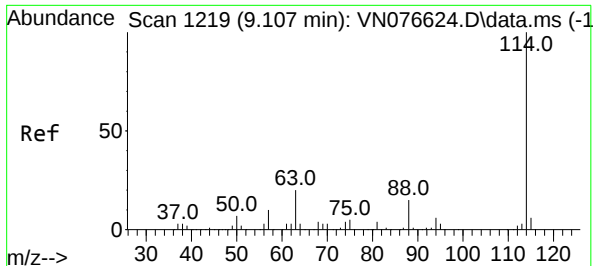

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.107 min Scan# 1

Delta R.T. -0.000 min

Lab File: VN076824.D

Acq: 28 Feb 2023 13:34

Instrument :

MSVOA_N

ClientSampleId :

VN0228MBL01





Tgt Ion:114 Resp: 497561

Ion Ratio Lower Upper

114 100

63 21.9 0.0 40.0

88 14.6 0.0 29.6

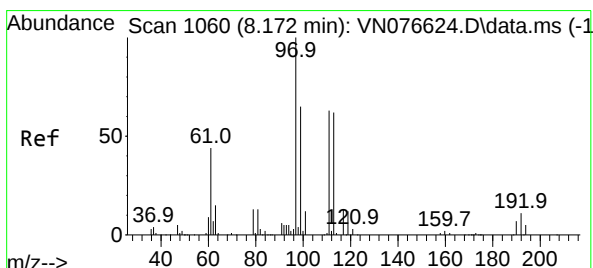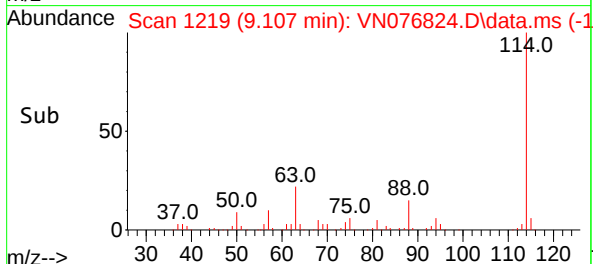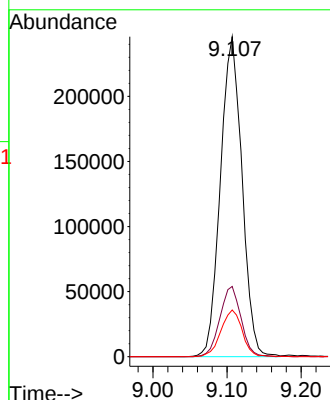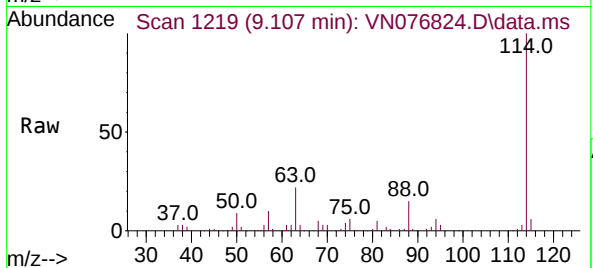

#35

Dibromofluoromethane

Concen: 48.644 ug/l

RT: 8.172 min Scan# 1060

Delta R.T. -0.000 min

Lab File: VN076824.D

Acq: 28 Feb 2023 13:34




Tgt Ion:113 Resp: 158503


Ion Ratio Lower Upper

113 100

111 100.6 83.1 124.7

192 16.4 15.6 23.4


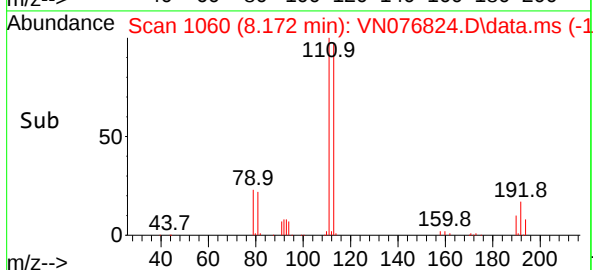
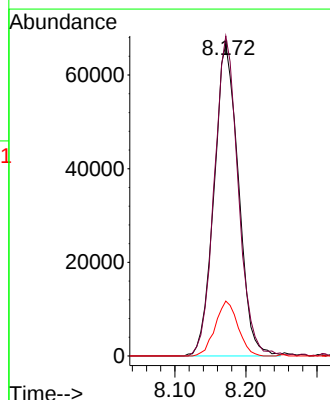
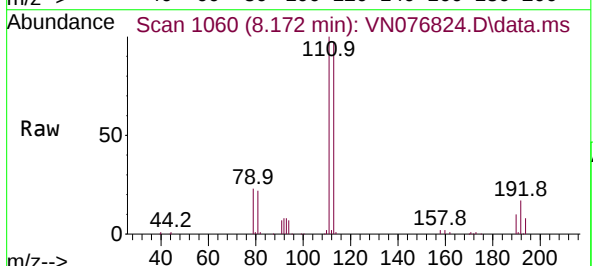


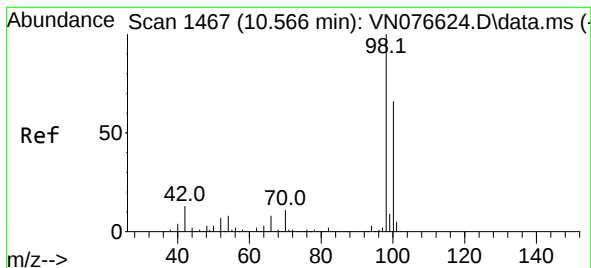

#50
Toluene-d8
Concen: 49.425 ug/l
RT: 10.566 min Scan# 1467
Delta R.T. -0.000 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34




Instrument :
MSVOA_N
ClientSampleId :
VN0228MBL01


Tgt Ion: 98 Resp: 601442
Ion Ratio Lower Upper
98 100
100 65.9 52.9 79.3

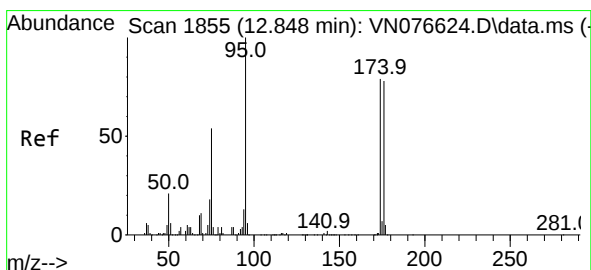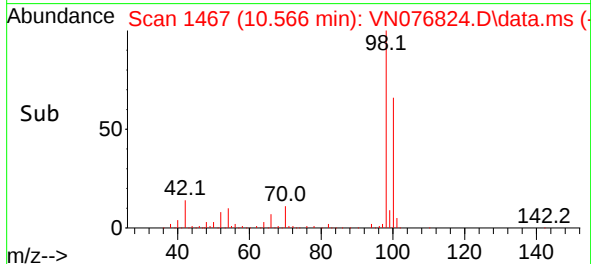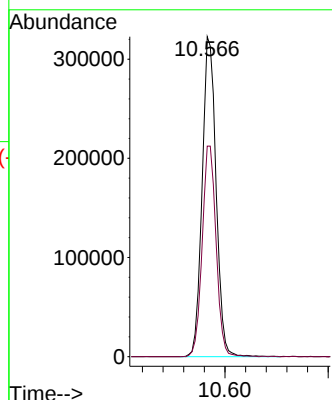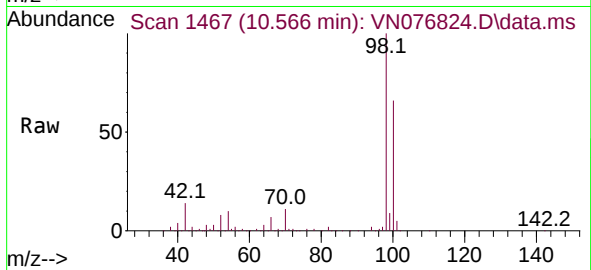

#62
4-Bromofluorobenzene
Concen: 44.453 ug/l
RT: 12.854 min Scan# 1856
Delta R.T. 0.006 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34

Tgt Ion: 95 Resp: 179160
Ion Ratio Lower Upper
95 100
174 76.4 0.0 169.2
176 73.9 0.0 163.4


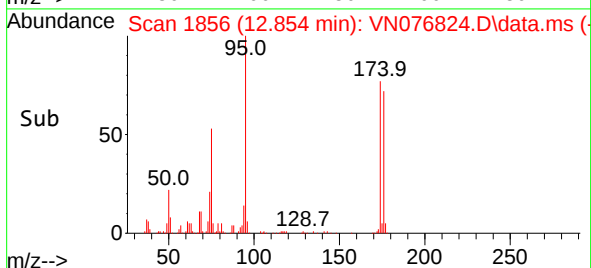
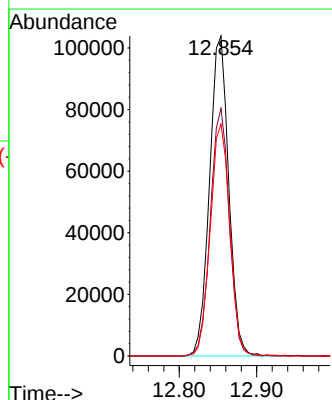
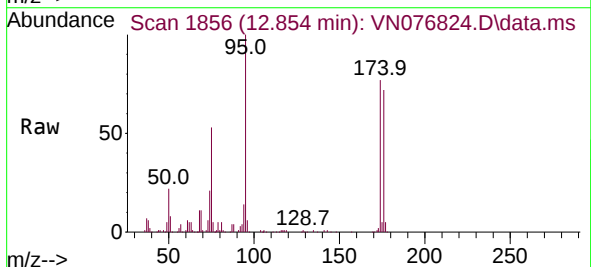


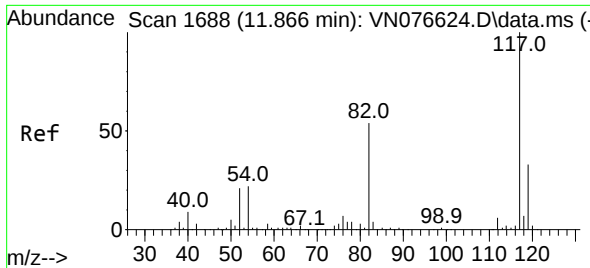

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.866 min Scan# 117
Delta R.T. -0.000 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34

Instrument :
MSVOA_N
ClientSampleId :
VN0228MBL01

Tgt Ion:117 Resp: 439949
Ion Ratio Lower Upper
117 100
82 55.8 43.4 65.2
119 32.1 26.1 39.1

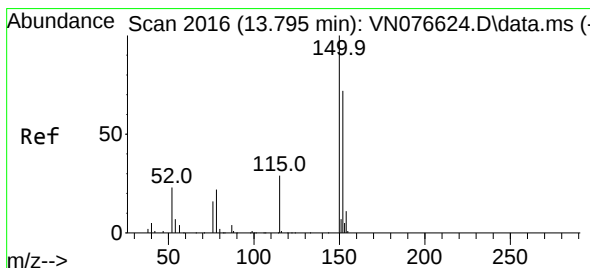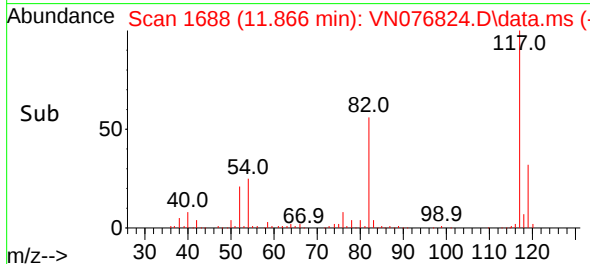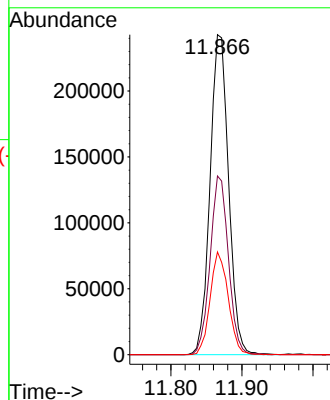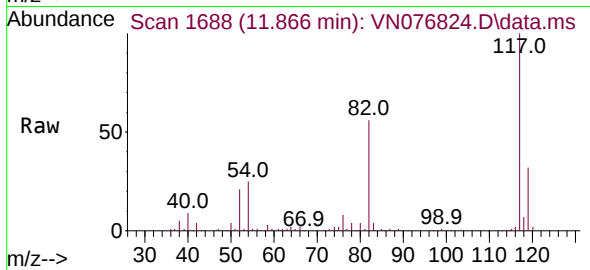

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.795 min Scan# 2016
Delta R.T. -0.000 min
Lab File: VN076824.D
Acq: 28 Feb 2023 13:34

Tgt Ion:152 Resp: 168547
Ion Ratio Lower Upper
152 100
115 59.6 29.3 87.9
150 157.9 0.0 349.8

