
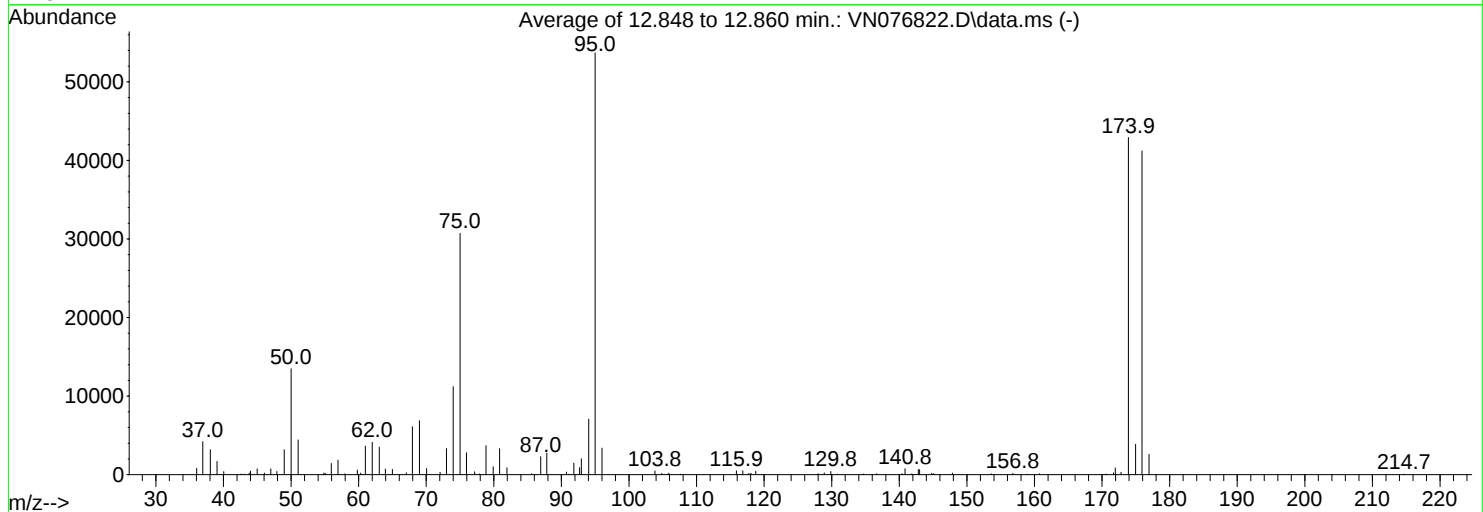


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022823\
Data File : VN076822.D
Acq On : 28 Feb 2023 10:34
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021323W.M
Title : SW846 8260
Last Update : Tue Feb 14 01:44:47 2023

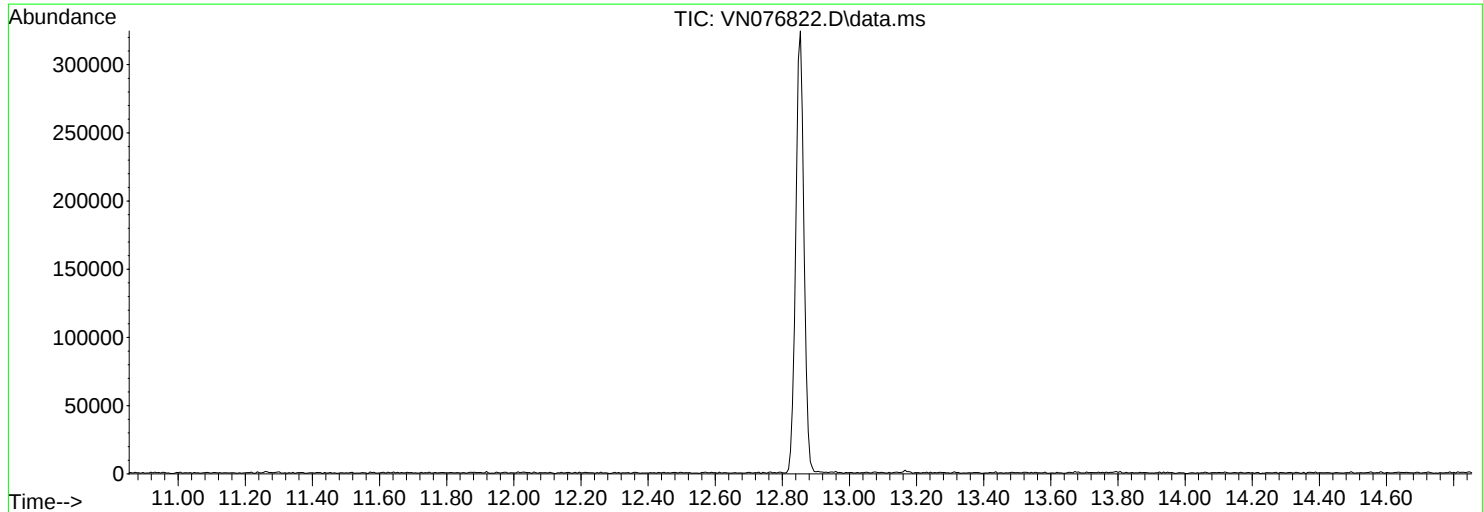

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	25.1	13479	PASS
75	95	30	60	57.2	30723	PASS
95	95	100	100	100.0	53693	PASS
96	95	5	9	6.3	3372	PASS
173	174	0.00	2	0.7	301	PASS
174	95	50	100	79.9	42917	PASS
175	174	5	9	9.0	3851	PASS
176	174	95	101	96.0	41211	PASS
177	176	5	9	6.3	2594	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
36.05	791	47.00	736	60.30	206	73.00	332
36.95	4205	47.90	407	61.00	3622	74.00	1119
38.05	3178	49.00	3185	62.00	4121	75.00	3072
39.05	1701	50.00	13479	63.05	3500	75.95	279
40.05	394	51.05	4424	63.95	716	77.15	376
42.60	89	54.85	197	65.00	681	77.90	104
43.10	52	55.05	193	67.05	242	78.85	3692
43.80	214	55.95	1435	67.95	6104	79.90	992
44.00	459	56.95	1844	69.00	6871	80.85	3308
45.00	742	57.95	108	70.05	771	81.95	870
46.05	212	59.80	590	72.05	317	85.60	118

Average of 12.848 to 12.860 min.: VN076822.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	2291	104.85	166	129.85	416	145.10	142
87.85	2750	105.70	70	130.90	60	147.85	213
90.75	327	105.90	213	134.70	83	153.60	112
91.10	61	107.60	57	136.65	132	156.80	165
91.85	1463	115.90	494	140.40	116	158.90	52
92.70	892	116.85	491	140.85	751	160.70	132
92.95	2020	117.75	172	141.80	80	169.90	51
94.05	7075	118.05	177	142.00	69	170.50	50
95.00	53693	118.75	427	142.80	654	170.70	67
96.00	3372	128.00	121	143.00	629	171.70	224
103.85	468	128.90	222	144.80	193	171.95	862

Average of 12.848 to 12.860 min.: VN076822.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.80	301						
173.90	42917						
174.95	3851						
175.90	41211						
176.95	2594						
214.70	54						

Instrument :

MSVOA_N

ClientSampleId :

BFB