

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022824\
 Data File : VN081253.D
 Acq On : 28 Feb 2024 19:17
 Operator : JC\MD
 Sample : P1587-04 50X
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 1326

Quant Time: Feb 28 23:31:13 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 16 23:45:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	308384	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.106	114	573576	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.871	117	518718	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	225851	50.000	ug/l	0.00


System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.583	65	214593	56.772	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 113.540%	
35) Dibromofluoromethane	8.165	113	170368	52.528	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 105.060%	
50) Toluene-d8	10.571	98	638255	55.406	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 110.820%	
62) 4-Bromofluorobenzene	12.853	95	220751	50.999	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	= 102.000%	

Target Compounds			Qvalue			
3) Chloromethane	2.377	50	646	Below Cal	#	50
6) Chloroethane	3.112	64	167	Below Cal	#	42
13) Acrolein	4.183	56	722	1.938	ug/l #	56
16) Acetone	4.418	43	1298	0.873	ug/l #	44
20) Methylene Chloride	5.283	84	891	Below Cal		88
25) 2-Butanone	7.500	43	3036	1.264	ug/l #	88
31) Cyclohexane	8.230	56	9040	1.385	ug/l #	3
36) 1,1-Dichloropropene	8.230	75	30148	5.426	ug/l #	51
37) Ethyl Acetate	7.500	43	3036	0.605	ug/l #	70
38) Carbon Tetrachloride	8.230	117	35174	6.257	ug/l #	19
39) Methylcyclohexane	9.612	83	1333	0.206	ug/l #	17
40) Benzene	8.612	78	7713	0.480	ug/l #	88
52) Toluene	10.635	92	416476	40.903	ug/l	97
53) t-1,3-Dichloropropene	10.635	75	4355	0.706	ug/l #	1
67) Ethyl Benzene	11.965	91	332738	16.563	ug/l	97
68) m/p-Xylenes	12.071	106	555863	72.189	ug/l	95
69) o-Xylene	12.400	106	267525	35.049	ug/l	96
70) Styrene	12.400	104	14723	1.217	ug/l #	1
73) Isopropylbenzene	12.700	105	21971	1.112	ug/l	98
76) 1,2,3-Trichloropropane	12.853	75	120122	23.409	ug/l #	1
78) n-propylbenzene	13.041	91	61356	2.697	ug/l	93
79) 2-Chlorotoluene	13.100	91	38640	2.769	ug/l #	45
80) 1,3,5-Trimethylbenzene	13.176	105	121580	7.588	ug/l	98
81) trans-1,4-Dichloro-2-b...	12.853	75	120122	60.252	ug/l #	14
82) 4-Chlorotoluene	13.176	91	14763	1.082	ug/l #	44
83) tert-Butylbenzene	13.488	119	56349	4.067	ug/l #	67
84) 1,2,4-Trimethylbenzene	13.488	105	467190	29.263	ug/l	96
85) sec-Butylbenzene	13.488	105	467190	24.258	ug/l #	60
86) p-Isopropyltoluene	13.676	119	6946	0.434	ug/l	90
89) n-Butylbenzene	14.059	91	3797	0.272	ug/l #	78
90) Hexachloroethane	14.335	117	3794	1.435	ug/l #	21
95) Naphthalene	15.647	128	101710	6.196	ug/l	99

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Quant Time: Feb 28 23:31:13 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 16 23:45:20 2024
Response via : Initial Calibration









#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:168 Resp: 308384
Ion Ratio Lower Upper
168 100
99 65.2 59.9 89.9

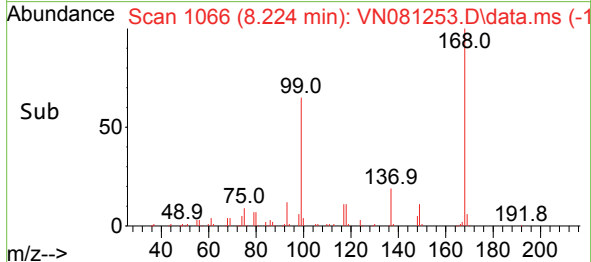

#3
Chloromethane
Concen: Below Cal
RT: 2.377 min Scan# 72
Delta R.T. 0.012 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 50 Resp: 646
Ion Ratio Lower Upper
50 100
52 59.0 25.0 37.4#









#6
Chloroethane
Concen: Below Cal
RT: 3.112 min Scan# 197
Delta R.T. -0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 64 Resp: 167
Ion Ratio Lower Upper
64 100
66 0.0 26.4 39.6#

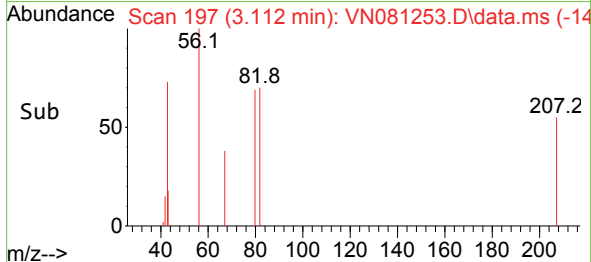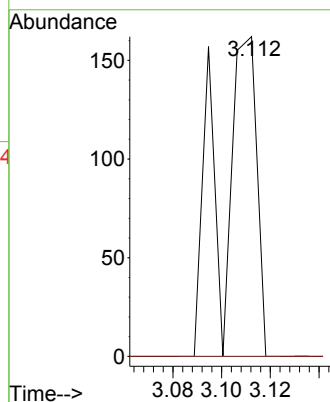

#13
Acrolein
Concen: 1.938 ug/l
RT: 4.183 min Scan# 379
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 56 Resp: 722
Ion Ratio Lower Upper
56 100
55 33.4 55.3 82.9#



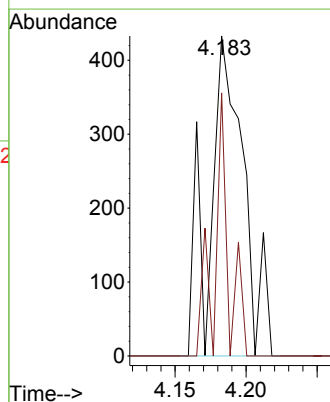





#16
Acetone
Concen: 0.873 ug/l
RT: 4.418 min Scan# 419
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 43 Resp: 1298
Ion Ratio Lower Upper
43 100
58 0.0 24.8 37.2#

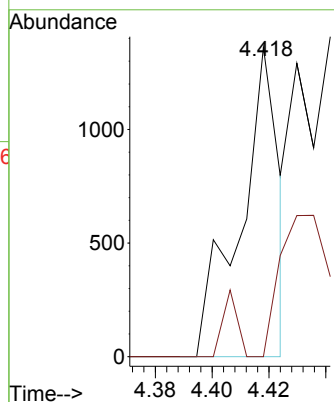

#20
Methylene Chloride
Concen: Below Cal
RT: 5.283 min Scan# 566
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 84 Resp: 891
Ion Ratio Lower Upper
84 100
49 152.9 108.1 162.1
51 42.8 32.9 49.3
86 68.2 48.6 73.0



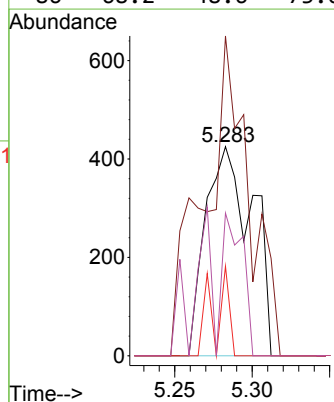





#25
2-Butanone
Concen: 1.264 ug/l
RT: 7.500 min Scan# 94
Delta R.T. 0.023 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 43 Resp: 3036
Ion Ratio Lower Upper
43 100
72 18.3 19.5 29.3#

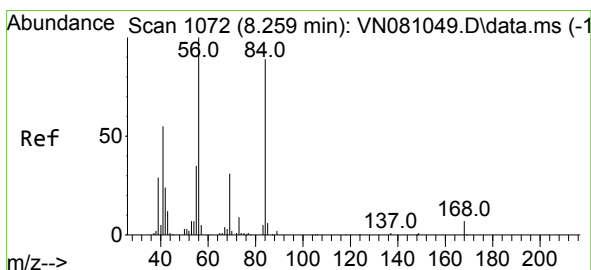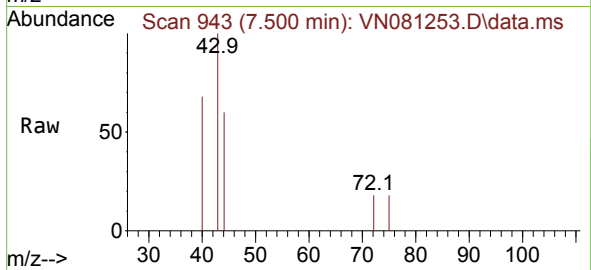

#31
Cyclohexane
Concen: 1.385 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.029 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 56 Resp: 9040
Ion Ratio Lower Upper
56 100
69 131.2 20.1 30.1#
84 118.6 56.9 85.3#









#33
 1,2-Dichloroethane-d4
 Concen: 56.772 ug/l
 RT: 8.583 min Scan# 1126
 Delta R.T. 0.006 min
 Lab File: VN081253.D
 Acq: 28 Feb 2024 19:17




Instrument :
 MSVOA_N
 ClientSampleId :
 1326


Tgt Ion: 65 Resp: 214593
 Ion Ratio Lower Upper
 65 100
 67 52.8 0.0 102.4

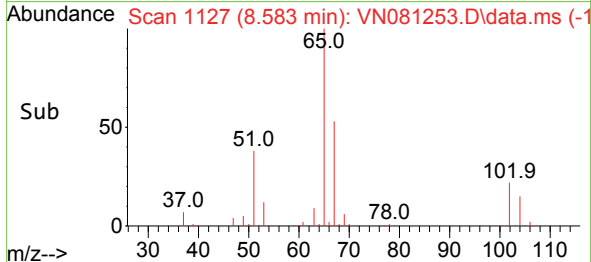

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 9.106 min Scan# 1216
 Delta R.T. 0.006 min
 Lab File: VN081253.D
 Acq: 28 Feb 2024 19:17

Tgt Ion: 114 Resp: 573576
 Ion Ratio Lower Upper
 114 100
 63 21.8 0.0 48.0
 88 15.6 0.0 34.8









#35
Dibromofluoromethane
Concen: 52.528 ug/l
RT: 8.165 min Scan# 1056
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:113 Resp: 170368
Ion Ratio Lower Upper
113 100
111 101.9 82.2 123.4
192 14.6 12.5 18.7

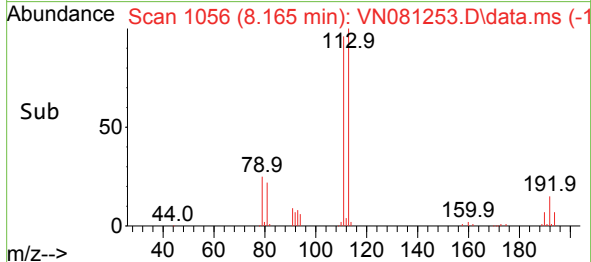

#36
1,1-Dichloropropene
Concen: 5.426 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.141 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 75 Resp: 30148
Ion Ratio Lower Upper
75 100
110 9.1 16.0 48.0#
77 0.0 25.8 38.6#









#37
Ethyl Acetate
Concen: 0.605 ug/l
RT: 7.500 min Scan# 94
Delta R.T. -0.059 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 43 Resp: 3036
Ion Ratio Lower Upper
43 100
61 0.0 10.6 15.8#
70 0.0 8.0 12.0#

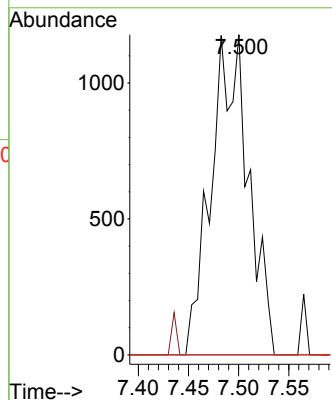

#38
Carbon Tetrachloride
Concen: 6.257 ug/l
RT: 8.230 min Scan# 1067
Delta R.T. -0.129 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 117 Resp: 35174
Ion Ratio Lower Upper
117 100
119 6.5 73.4 110.2#
121 0.0 24.4 36.6#

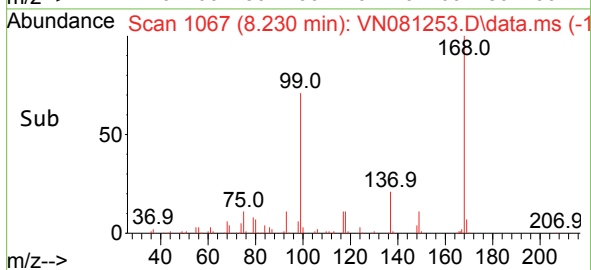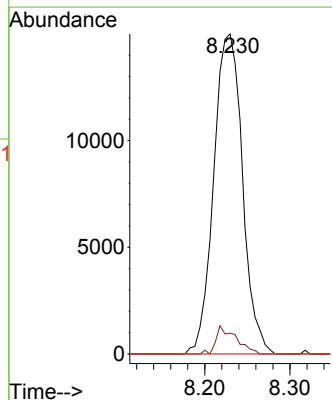



#39

Methylcyclohexane

Concen: 0.206 ug/l

RT: 9.612 min Scan# 1133

Delta R.T. 0.012 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :

1326





Tgt Ion: 83 Resp: 1333

Ion Ratio Lower Upper

83 100

55 0.0 65.7 98.5#

98 0.0 33.8 50.6#

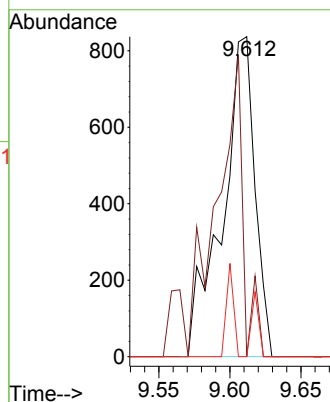

#40

Benzene

Concen: 0.480 ug/l

RT: 8.612 min Scan# 1132

Delta R.T. 0.006 min

Lab File: VN081253.D




Acq: 28 Feb 2024 19:17


Tgt Ion: 78 Resp: 7713

Ion Ratio Lower Upper

78 100

77 31.6 20.4 30.6#


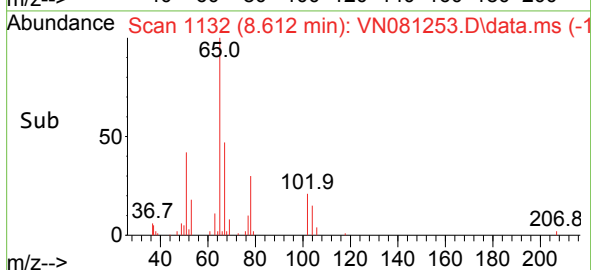






#50
Toluene-d8
Concen: 55.406 ug/l
RT: 10.571 min Scan# 1465
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 98 Resp: 638255
Ion Ratio Lower Upper
98 100
100 65.2 51.4 77.0

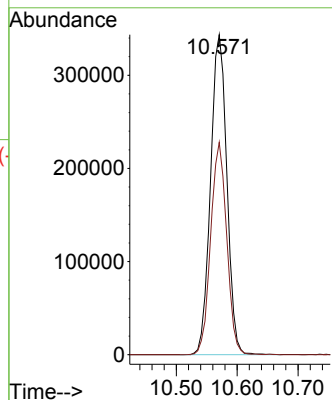

#52
Toluene
Concen: 40.903 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 92 Resp: 416476
Ion Ratio Lower Upper
92 100
91 170.5 139.4 209.0


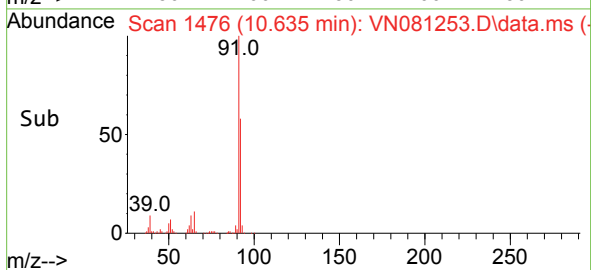
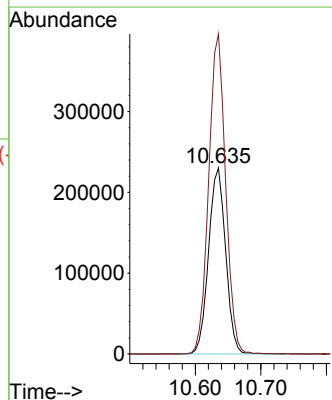





#53
t-1,3-Dichloropropene
Concen: 0.706 ug/l
RT: 10.635 min Scan# 1476
Delta R.T. -0.200 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion: 75 Resp: 4355
Ion Ratio Lower Upper
75 100
77 213.5 25.5 38.3#

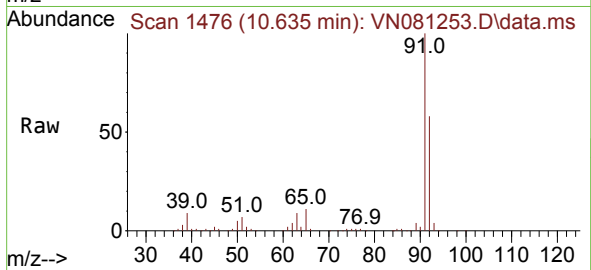

#62
4-Bromofluorobenzene
Concen: 50.999 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 95 Resp: 220751
Ion Ratio Lower Upper
95 100
174 70.6 0.0 120.4
176 65.9 0.0 121.0


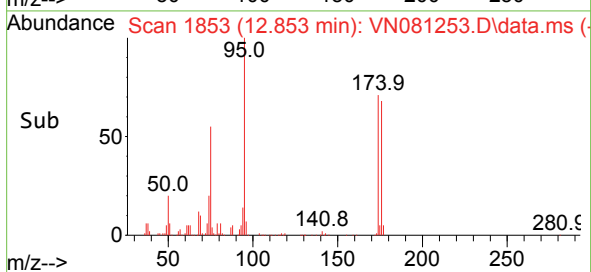






#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.871 min Scan# 1
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:117 Resp: 518718
Ion Ratio Lower Upper
117 100
82 57.9 52.7 79.1
119 31.9 25.3 37.9

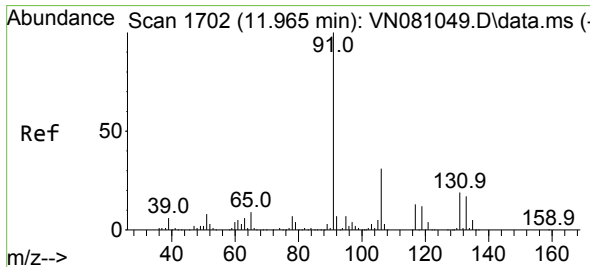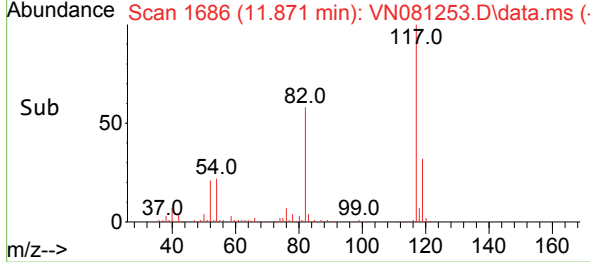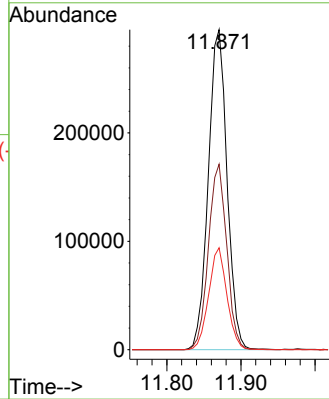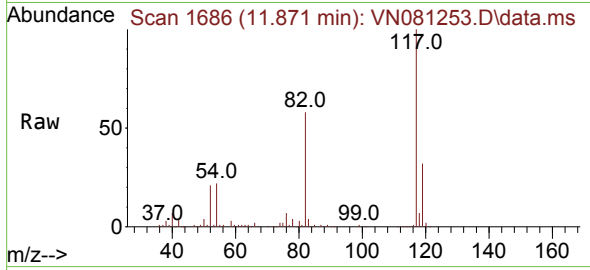

#67
Ethyl Benzene
Concen: 16.563 ug/l
RT: 11.965 min Scan# 1702
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 91 Resp: 332738
Ion Ratio Lower Upper
91 100
106 28.1 23.8 35.6


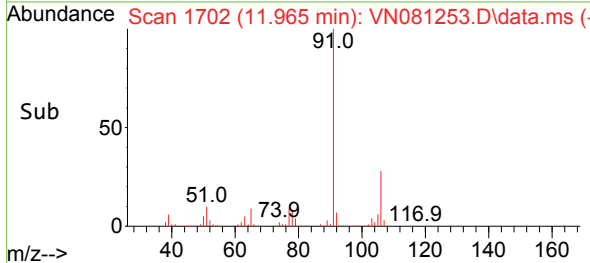
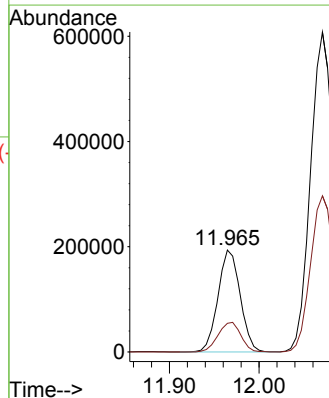
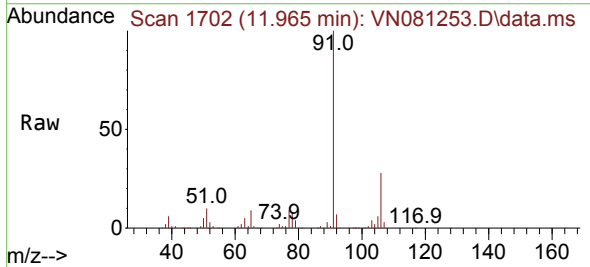




#68
m/p-Xylenes
Concen: 72.189 ug/l
RT: 12.071 min Scan# 1720
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:106 Resp: 555863
Ion Ratio Lower Upper
106 100
91 203.4 169.0 253.6



#69
o-Xylene
Concen: 35.049 ug/l
RT: 12.400 min Scan# 1776
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion:106 Resp: 267525
Ion Ratio Lower Upper
106 100
91 218.3 112.1 336.3

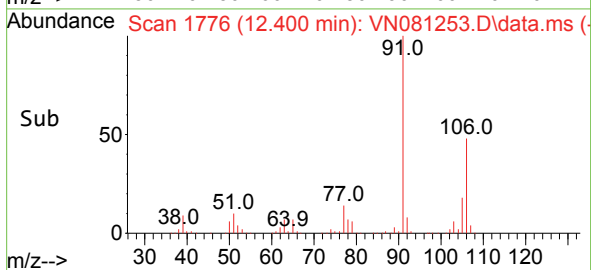



#70

Styrene

Concen: 1.217 ug/l

RT: 12.400 min Scan# 1

Delta R.T. -0.012 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :

1326





Tgt Ion:104 Resp: 14723

Ion Ratio Lower Upper

104 100

78 295.9 43.8 65.8#

103 249.8 44.2 66.2#



#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.794 min Scan# 2013

Delta R.T. -0.000 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17




Tgt Ion:152 Resp: 225851


Ion Ratio Lower Upper

152 100

115 66.0 32.3 96.8

150 154.4 0.0 339.8

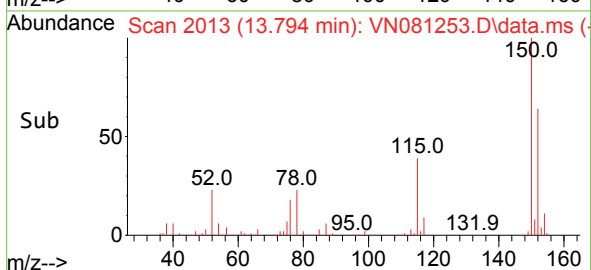



#73

Isopropylbenzene

Concen: 1.112 ug/l

RT: 12.700 min Scan# 1827

Delta R.T. -0.000 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :





1326

Tgt Ion:105 Resp: 21971

Ion Ratio Lower Upper

105 100

120 23.9 12.6 37.6

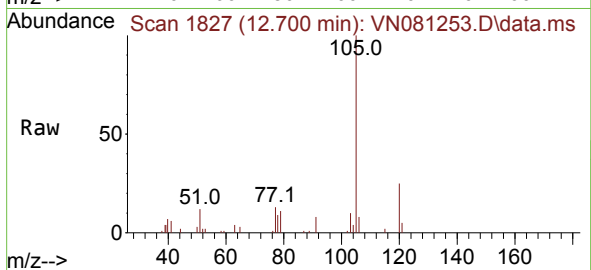

#76

1,2,3-Trichloropropane

Concen: 23.409 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. -0.141 min

Lab File: VN081253.D




Acq: 28 Feb 2024 19:17


Tgt Ion: 75 Resp: 120122

Ion Ratio Lower Upper

75 100

77 1.5 91.0 272.8#

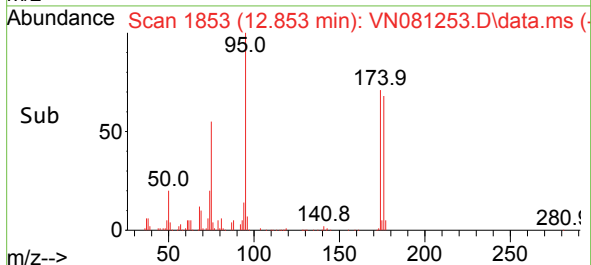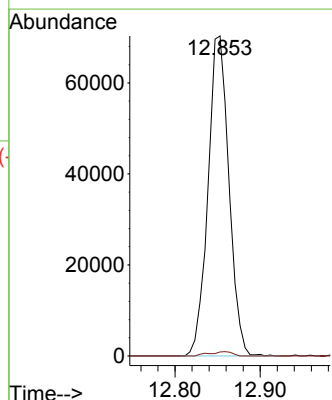



#78

n-propylbenzene

Concen: 2.697 ug/l

RT: 13.041 min Scan# 1885

Delta R.T. 0.006 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :





1326

Tgt Ion: 91 Resp: 61356

Ion Ratio Lower Upper

91 100

120 24.0 10.3 30.9

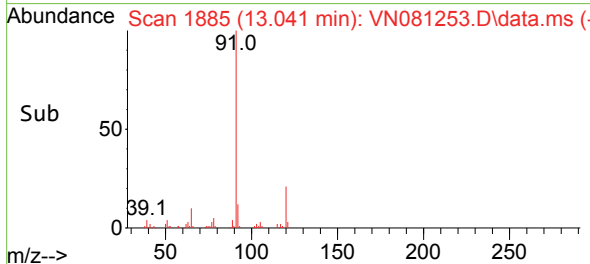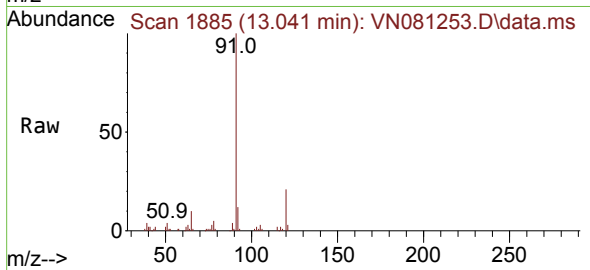

#79

2-Chlorotoluene

Concen: 2.769 ug/l

RT: 13.100 min Scan# 1895

Delta R.T. -0.029 min

Lab File: VN081253.D




Acq: 28 Feb 2024 19:17


Tgt Ion: 91 Resp: 38640

Ion Ratio Lower Upper

91 100

126 0.0 14.8 44.4#

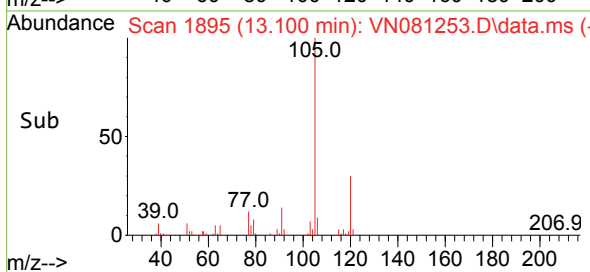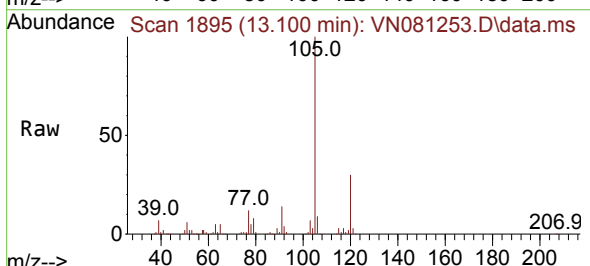



#80

1,3,5-Trimethylbenzene

Concen: 7.588 ug/l

RT: 13.176 min Scan# 1908

Delta R.T. -0.000 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :





1326

Tgt Ion:105 Resp: 121580

Ion Ratio Lower Upper

105 100

120 47.1 23.0 69.0

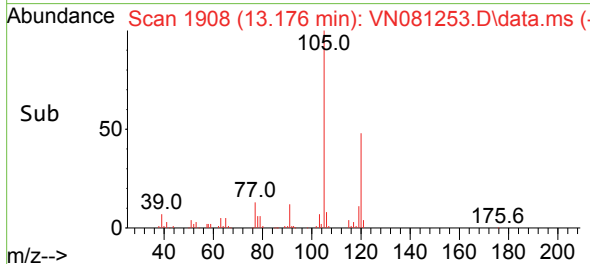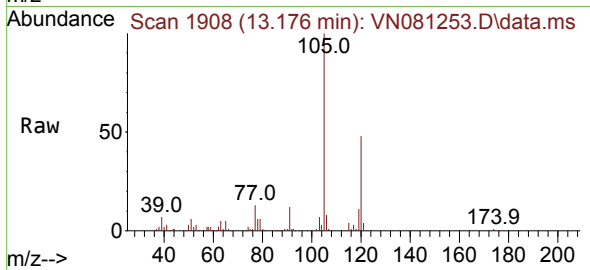

#81

trans-1,4-Dichloro-2-butene

Concen: 60.252 ug/l

RT: 12.853 min Scan# 1853

Delta R.T. 0.112 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17




Tgt Ion: 75 Resp: 120122


Ion Ratio Lower Upper

75 100

53 0.0 71.4 107.2#

89 0.0 33.4 50.0#

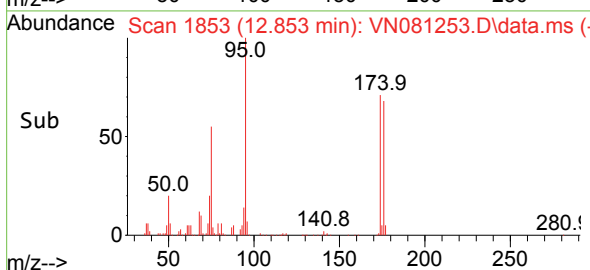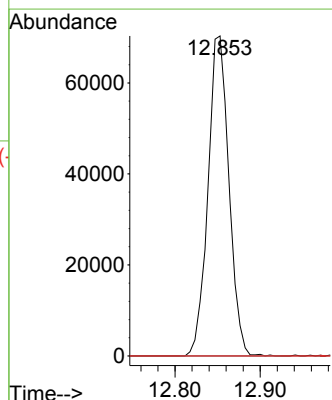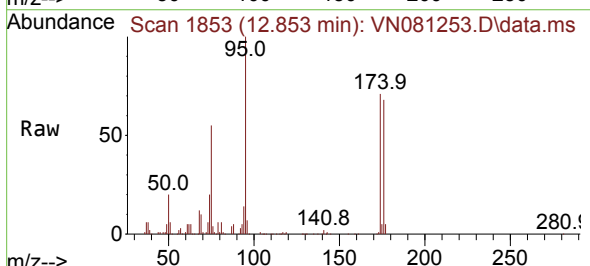



#82

4-Chlorotoluene

Concen: 1.082 ug/l

RT: 13.176 min Scan# 1916

Delta R.T. -0.047 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17

Instrument :

MSVOA_N

ClientSampleId :





1326

Tgt Ion: 91 Resp: 14763

Ion Ratio Lower Upper

91 100

126 0.0 15.3 45.9#

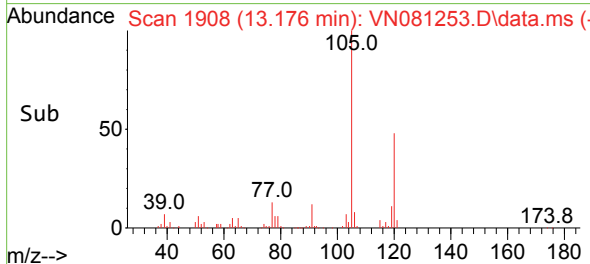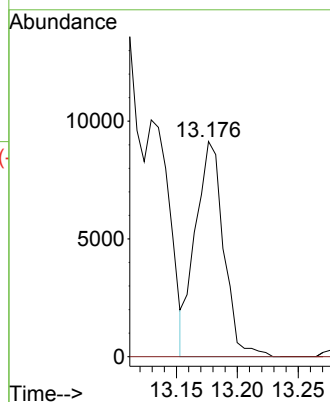

#83

tert-Butylbenzene

Concen: 4.067 ug/l

RT: 13.488 min Scan# 1961

Delta R.T. 0.047 min

Lab File: VN081253.D

Acq: 28 Feb 2024 19:17




Tgt Ion: 119 Resp: 56349


Ion Ratio Lower Upper

119 100

91 97.2 36.8 110.4

134 0.0 12.4 37.4#


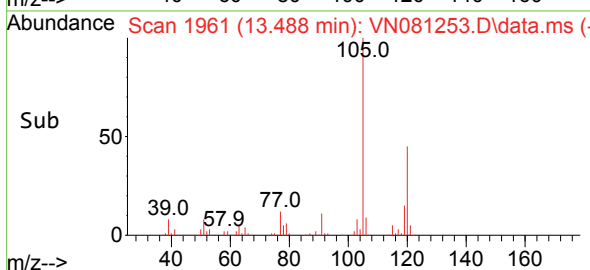

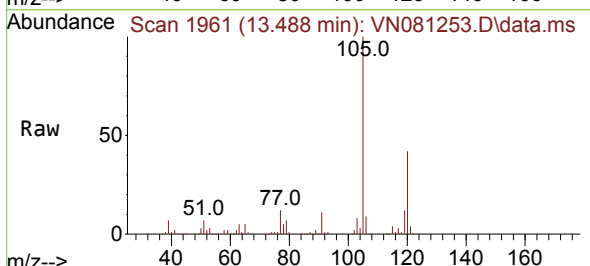




#84
1,2,4-Trimethylbenzene
Concen: 29.263 ug/l
RT: 13.488 min Scan# 1960
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:105 Resp: 467190
Ion Ratio Lower Upper
105 100
120 44.3 20.9 62.7

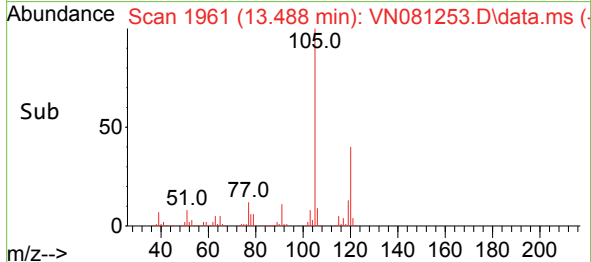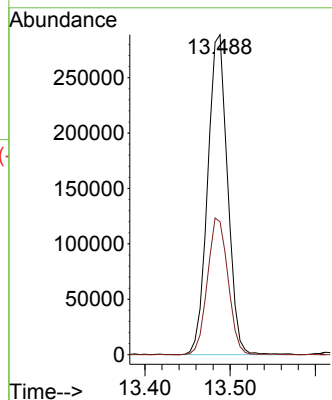

#85
sec-Butylbenzene
Concen: 24.258 ug/l
RT: 13.488 min Scan# 1961
Delta R.T. -0.129 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion:105 Resp: 467190
Ion Ratio Lower Upper
105 100
134 0.0 8.6 25.8#



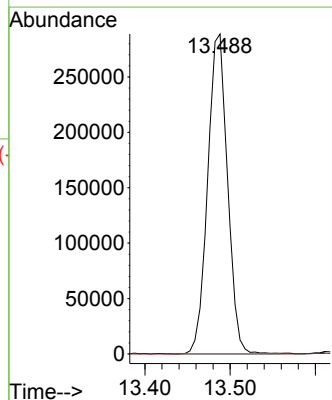





#86
p-Isopropyltoluene
Concen: 0.434 ug/l
RT: 13.676 min Scan# 1993
Delta R.T. -0.053 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17




Instrument :
MSVOA_N
ClientSampleId :
1326


Tgt Ion:119 Resp: 6946
Ion Ratio Lower Upper
119 100
134 24.1 12.4 37.2
91 36.7 13.5 40.4

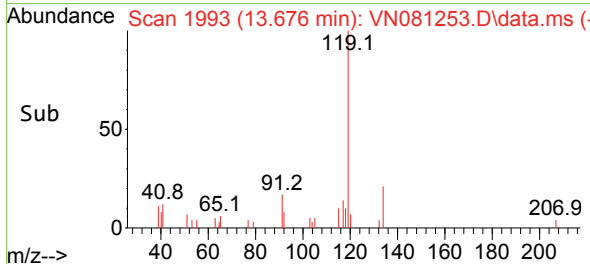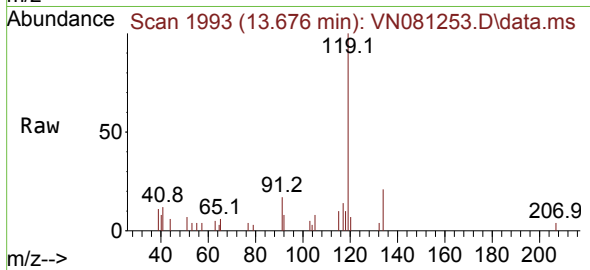

#89
n-Butylbenzene
Concen: 0.272 ug/l
RT: 14.059 min Scan# 2058
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion: 91 Resp: 3797
Ion Ratio Lower Upper
91 100
92 62.1 26.7 80.1
134 0.0 10.8 32.4#


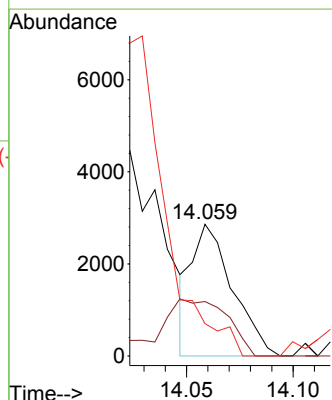
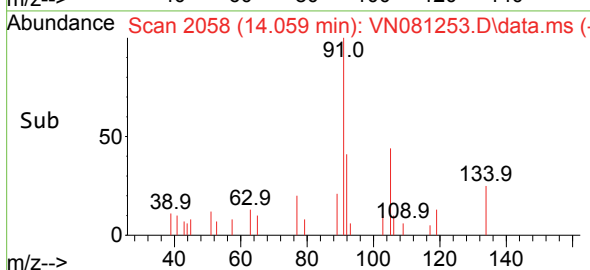
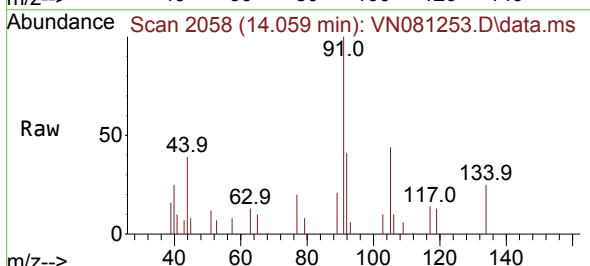




#90
Hexachloroethane
Concen: 1.435 ug/l
RT: 14.335 min Scan# 2105
Delta R.T. -0.000 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Instrument :
MSVOA_N
ClientSampleId :
1326

Tgt Ion:117 Resp: 3794
Ion Ratio Lower Upper
117 100
201 0.0 30.0 90.0#



#95
Naphthalene
Concen: 6.196 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.006 min
Lab File: VN081253.D
Acq: 28 Feb 2024 19:17

Tgt Ion:128 Resp: 101710
Ion Ratio Lower Upper
128 100
127 13.1 10.0 15.0
129 11.3 8.7 13.1

