
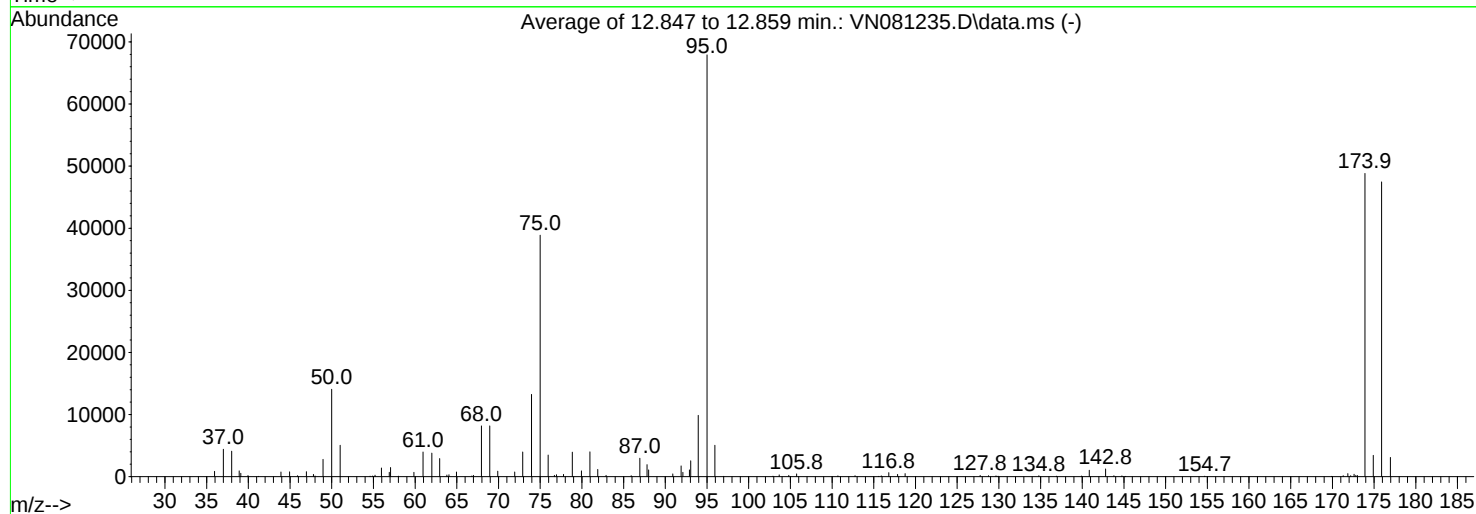


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN022824\
Data File : VN081235.D
Acq On : 28 Feb 2024 10:57
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

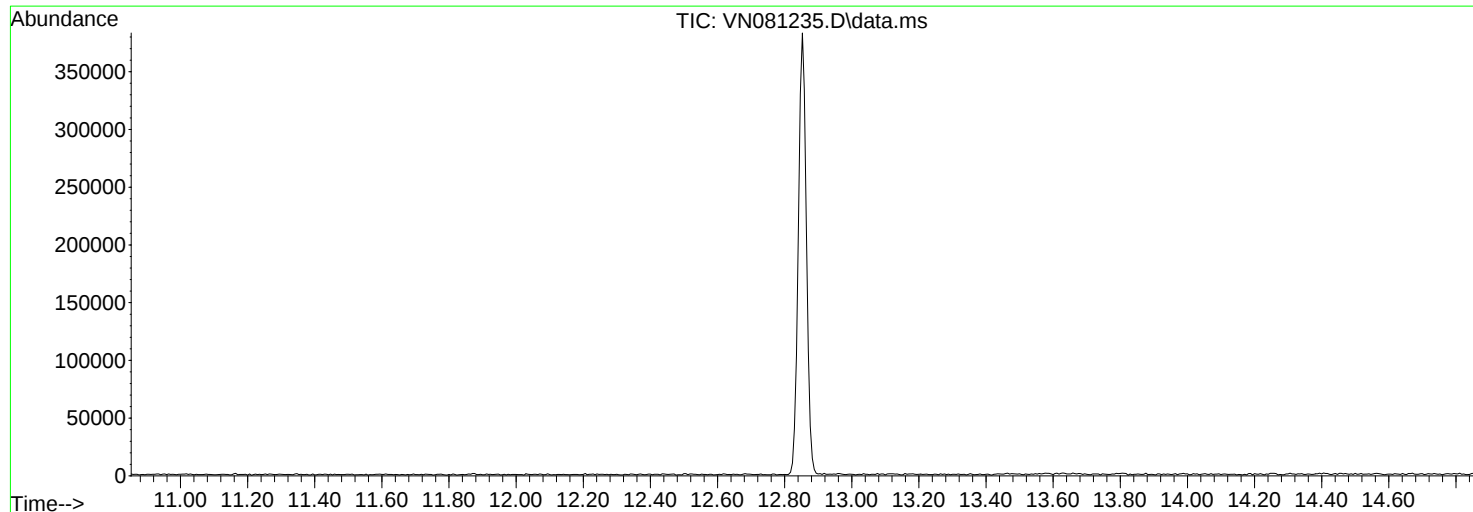

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1844

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.7	14058	PASS
75	95	30	60	57.2	38885	PASS
95	95	100	100	100.0	67923	PASS
96	95	5	9	7.5	5061	PASS
173	174	0.00	2	0.4	196	PASS
174	95	50	100	71.9	48835	PASS
175	174	5	9	7.0	3421	PASS
176	174	95	101	97.2	47461	PASS
177	176	5	9	6.5	3101	PASS

Average of 12.847 to 12.859 min.: VN081235.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	840	47.80	354	58.00	81	68.95	816
37.00	4404	48.00	108	59.85	685	69.90	88
38.00	4088	48.95	2787	60.95	3967	71.95	74
38.90	942	50.00	14058	62.00	3796	72.90	397
39.10	545	51.00	5044	62.95	2920	73.95	13233
39.95	173	54.60	81	63.80	251	75.00	38885
41.20	54	54.90	113	64.05	321	75.95	3483
43.90	752	55.20	227	64.95	742	76.70	216
44.95	765	55.95	1389	66.80	103	76.95	322
45.90	149	56.90	700	67.00	211	77.80	359
46.95	804	57.05	1478	67.95	8156	78.85	3941

Average of 12.847 to 12.859 min.: VN081235.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.95	923	92.90	1073	112.75	165	136.90	77
80.95	3993	93.05	2562	115.60	64	139.90	103
81.90	1159	93.95	9872	115.90	120	140.85	1020
82.90	202	95.00	67923	116.80	645	142.80	1246
85.90	146	95.95	5061	117.85	375	143.80	146
86.95	2954	97.00	59	118.75	480	144.75	130
87.80	1941	102.90	73	127.75	210	145.20	61
88.00	1088	103.65	278	128.75	154	154.70	83
90.90	433	104.80	212	129.65	141	169.90	59
91.90	1720	105.75	438	129.90	74	171.30	150
92.10	685	110.70	133	134.80	145	171.85	482

Average of 12.847 to 12.859 min.: VN081235.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
172.20	170						
172.60	399						
172.80	196						
173.00	172						
173.90	48835						
174.90	3421						
175.90	47461						
176.95	3101						

Instrument :

MSVOA_N

ClientSampleId :

BFB