


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030119\
Data File : VN054015.D
Acq On : 1 Mar 2019 8:17
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N030119W.M
Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
Last Update : Tue Mar 05 00:48:50 2019

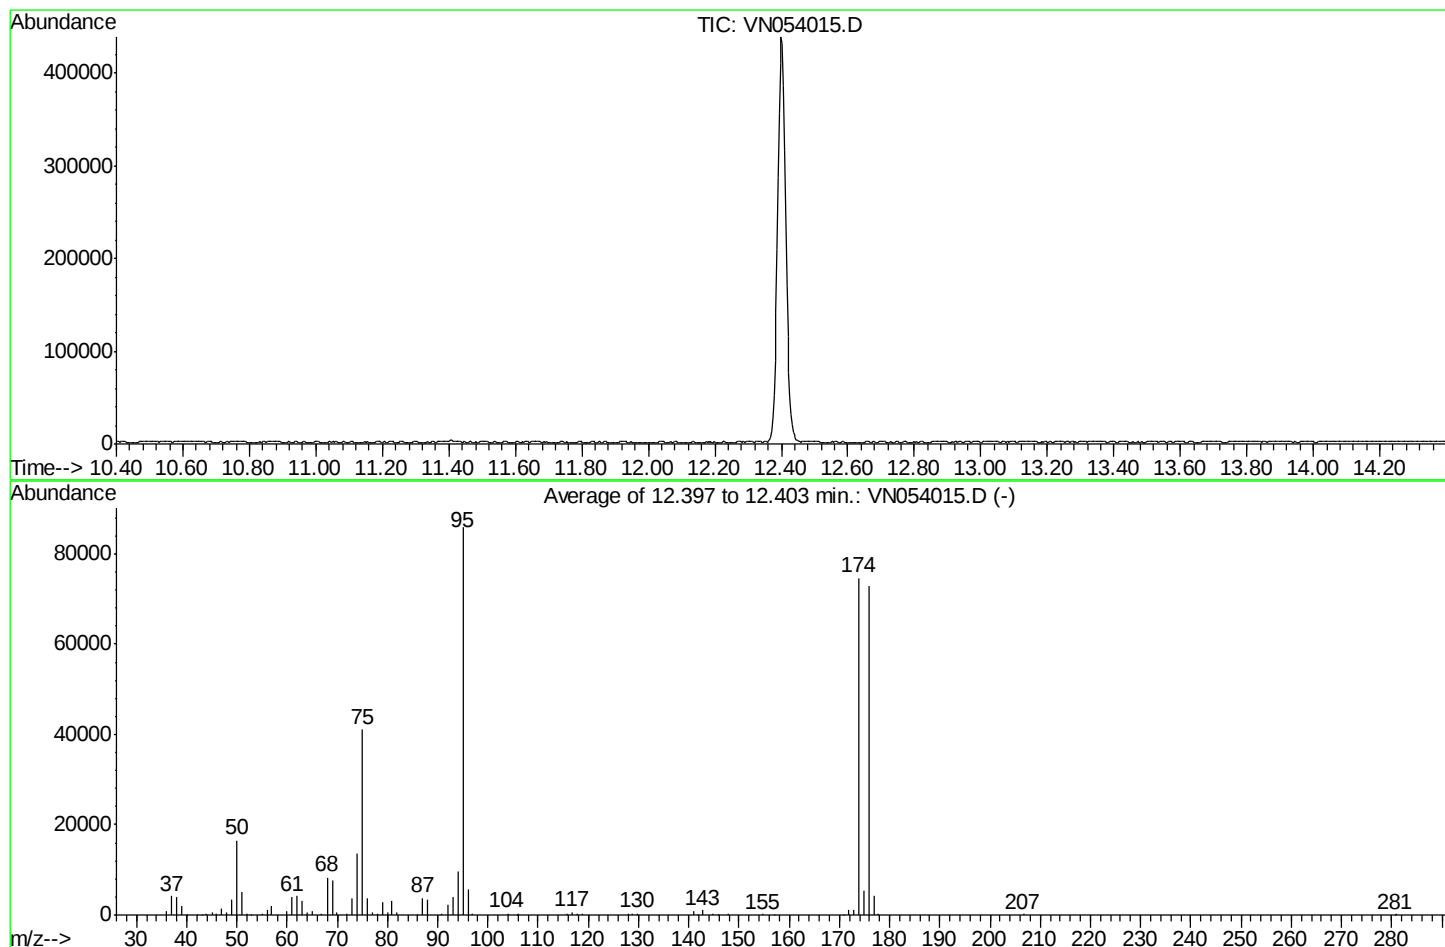

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	16541	PASS
75	95	30	60	47.8	41008	PASS
95	95	100	100	100.0	85874	PASS
96	95	5	9	6.5	5564	PASS
173	174	0.00	2	1.4	1051	PASS
174	95	50	100	86.9	74584	PASS
175	174	5	9	7.1	5315	PASS
176	174	95	101	97.6	72824	PASS
177	176	5	9	5.8	4231	PASS