

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030121\
 Data File : VN066088.D
 Acq On : 1 Mar 2021 19:51
 Operator : JC/MD
 Sample : M1488-01
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 41700

Quant Time: Mar 01 21:46:59 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 17 15:48:13 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.627	168	112824	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.550	114	185309	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	169203	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.315	152	73064	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	78567	49.80	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	99.60%
35) Dibromofluoromethane	7.553	113	56659	49.40	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	98.80%
50) Toluene-d8	10.058	98	225260	47.85	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	95.70%
62) 4-Bromofluorobenzene	12.373	95	83521	47.26	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	94.52%


Target Compounds						Qvalue
3) Chloromethane	2.055	50	705	0.38	ug/l	96
11) Tert butyl alcohol	4.756	59	393	1.79	ug/l #	73
13) Acrolein	3.586	56	1092	5.44	ug/l	98
16) Acetone	3.795	43	20812	40.65	ug/l	91
18) Methyl Acetate	4.303	43	745	0.57	ug/l #	51
20) Methylene Chloride	4.521	84	8433	5.76	ug/l	98
25) 2-Butanone	6.798	43	4136	5.30	ug/l	92
29) Tetrahydrofuran	7.171	42	194	0.36	ug/l #	32
31) Cyclohexane	7.627	56	2366	1.01	ug/l #	27
36) 1,1-Dichloropropene	7.627	75	8423	4.61	ug/l #	48
37) Ethyl Acetate	6.798	43	4136	2.51	ug/l #	68
38) Carbon Tetrachloride	7.627	117	11747	6.92	ug/l #	16
40) Benzene	8.000	78	4927	0.88	ug/l #	87
43) Isopropyl Acetate	8.126	43	8619	3.28	ug/l #	90
45) 1,2-Dichloropropane	9.232	63	446	0.31	ug/l #	44
48) Methyl methacrylate	9.138	41	2073	1.56	ug/l #	10
51) 4-Methyl-2-Pentanone	9.949	43	2786	1.74	ug/l #	81
52) Toluene	10.122	92	5775	1.68	ug/l	99
54) cis-1,3-Dichloropropene	9.872	75	14665	6.64	ug/l #	61
56) Ethyl methacrylate	10.193	69	692	0.36	ug/l #	36
57) 1,3-Dichloropropane	10.733	76	7447	3.28	ug/l #	43
59) 2-Hexanone	10.733	43	102036	89.52	ug/l #	50
67) Ethyl Benzene	11.479	91	1795	0.28	ug/l	97
68) m/p-Xylenes	11.585	106	2228	0.93	ug/l	81
69) o-Xylene	11.920	106	1278	0.55	ug/l	77
74) N-amyl acetate	12.026	43	1110	0.54	ug/l #	44
76) 1,2,3-Trichloropropane	12.373	75	43183	24.60	ug/l #	100
81) trans-1,4-Dichloro-2-b...	12.373	75	43183	78.41	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.013	105	2989	0.59	ug/l	95
85) sec-Butylbenzene	13.013	105	2989	0.55	ug/l #	56
92) 1,2-Dibromo-3-Chloropr...	14.244	75	61	1.02	ug/l #	1
95) Naphthalene	15.100	128	6301	4.45	ug/l	100


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030121\
Data File : VN066088.D
Acq On : 1 Mar 2021 19:51
Operator : JC/MD
Sample : M1488-01
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
41700

Quant Time: Mar 01 21:46:59 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021721W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 17 15:48:13 2021
Response via : Initial Calibration




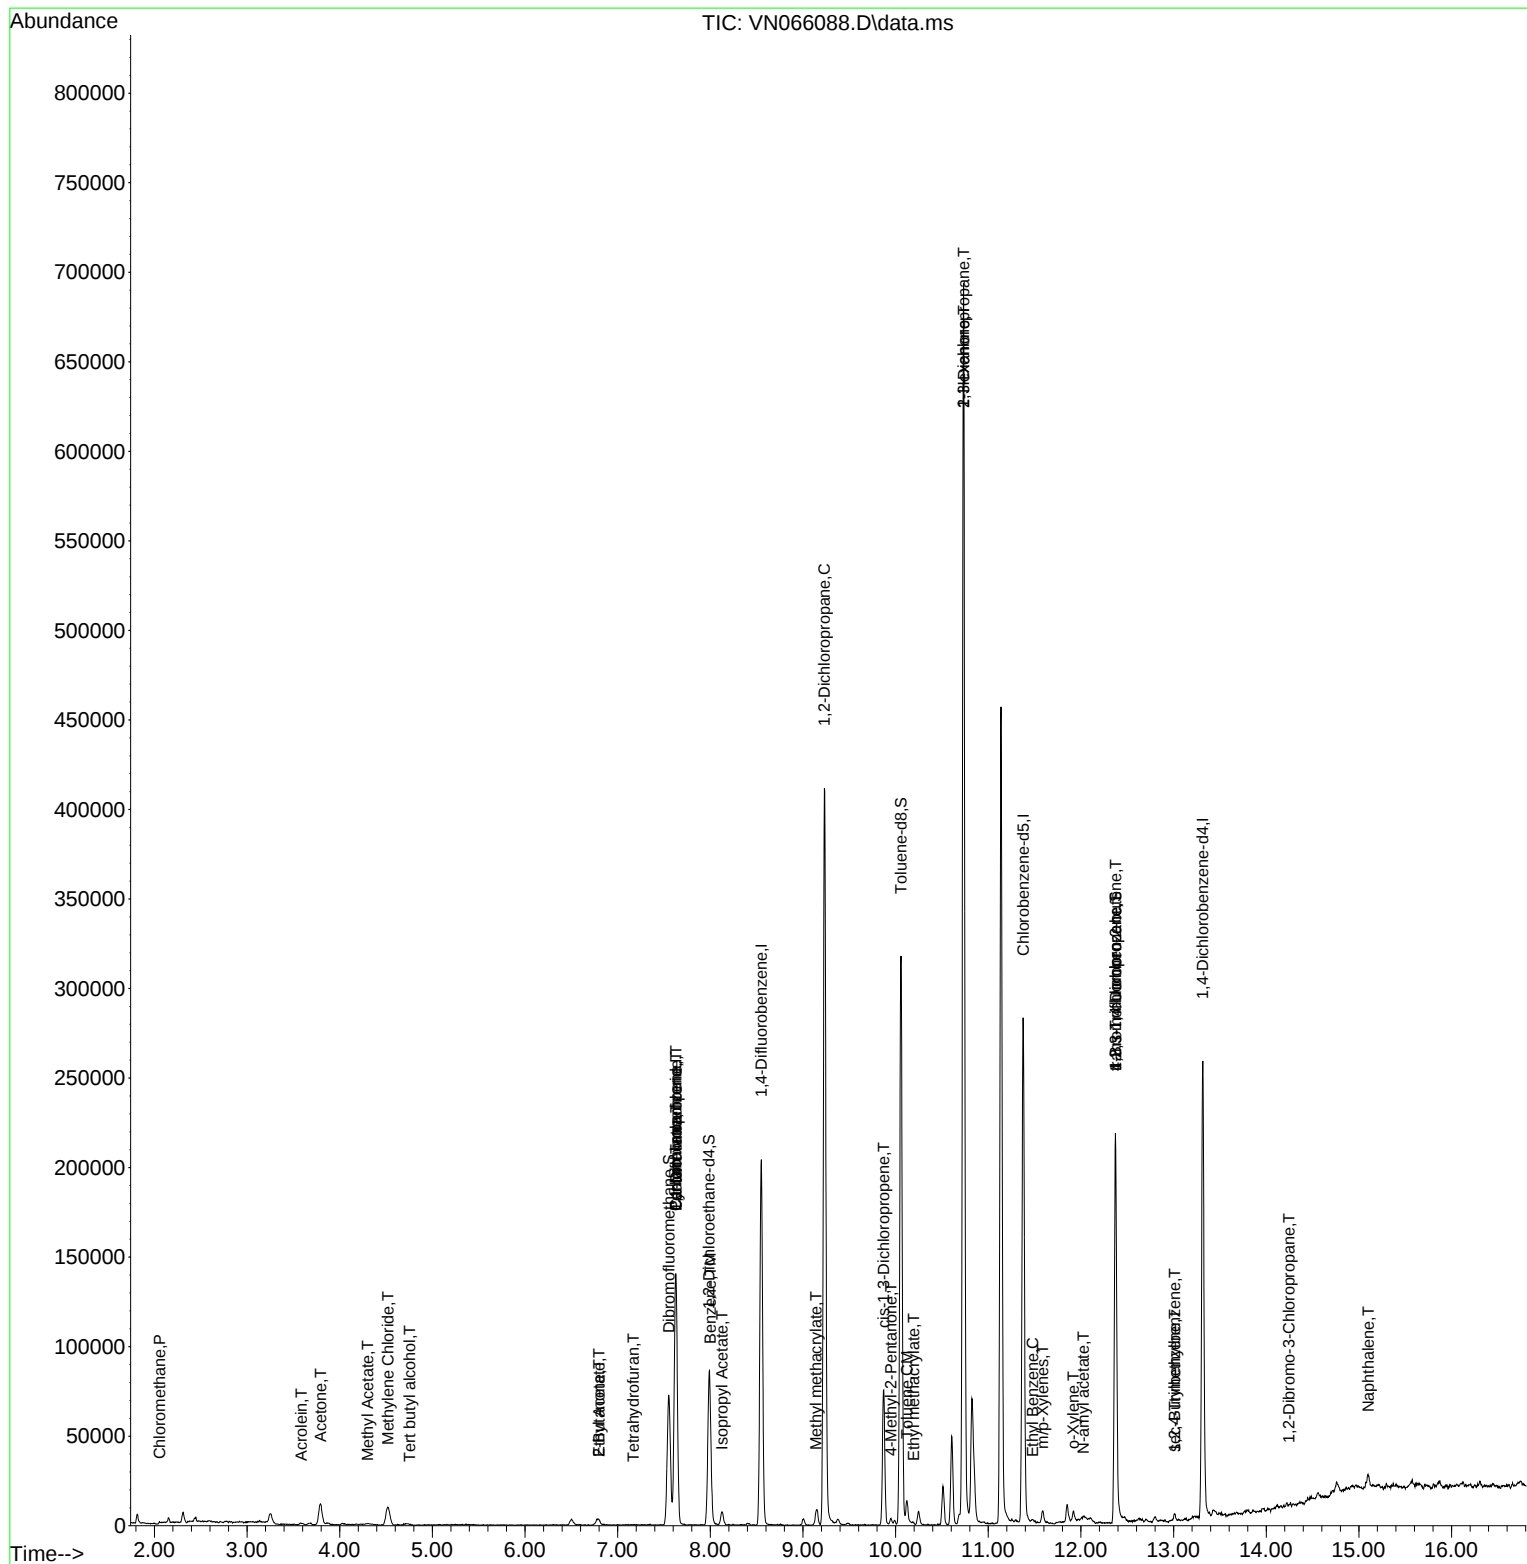




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion:168 Resp: 112824
Ion Ratio Lower Upper
168 100
99 62.1 42.6 63.8

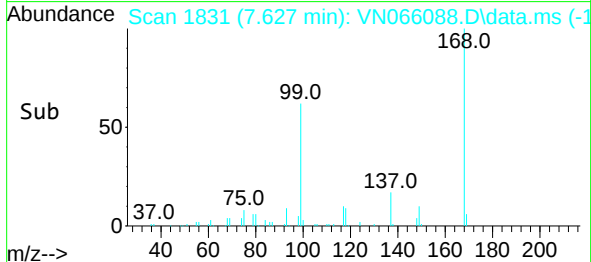

#3
Chloromethane
Concen: 0.38 ug/l
RT: 2.055 min Scan# 98
Delta R.T. 0.006 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 50 Resp: 705
Ion Ratio Lower Upper
50 100
52 30.3 25.8 38.8

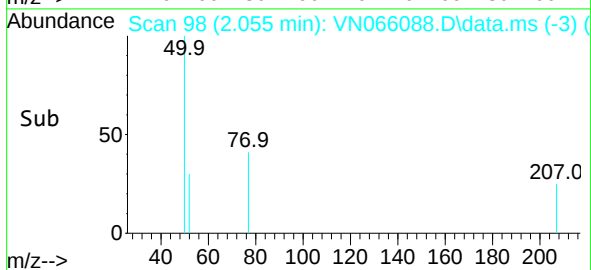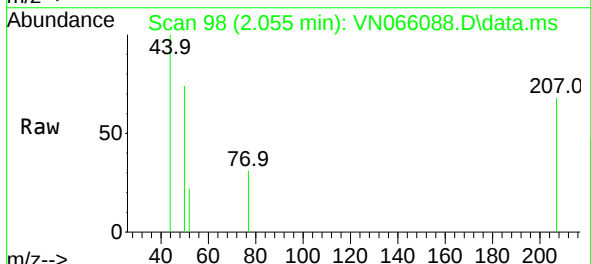


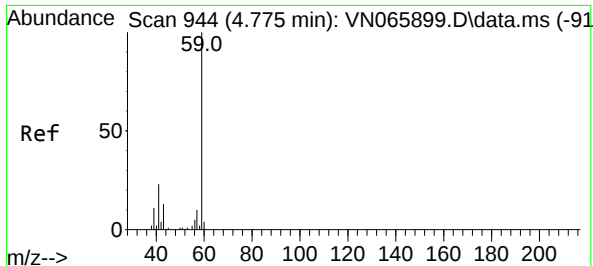




#11

Tert butyl alcohol
Concen: 1.79 ug/l
RT: 4.756 min Scan# 938
Delta R.T. -0.019 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampled :
41700

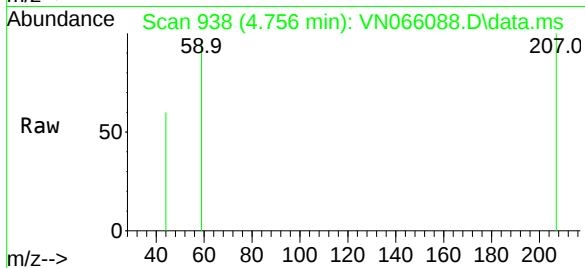




Tgt Ion: 59 Resp: 393
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

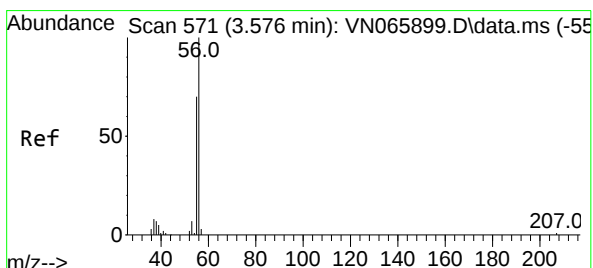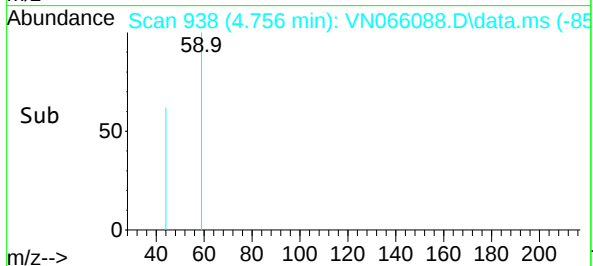


#13

Acrolein
Concen: 5.44 ug/l
RT: 3.586 min Scan# 574
Delta R.T. 0.010 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 56 Resp: 1092
Ion Ratio Lower Upper
56 100
55 67.9 56.0 84.0


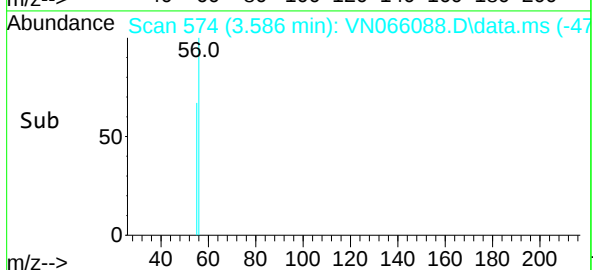

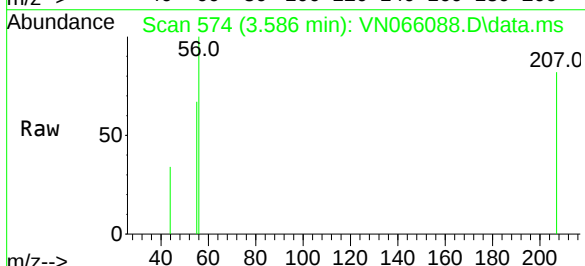


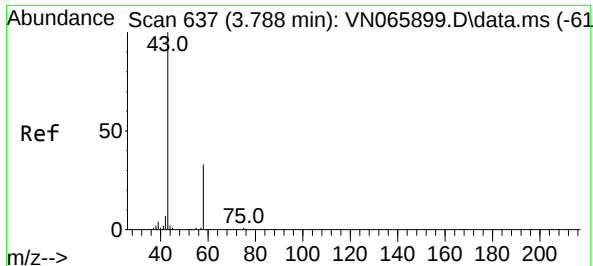

#16
Acetone
Concen: 40.65 ug/l
RT: 3.795 min Scan# 639
Delta R.T. 0.007 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampleId :
41700


Tgt Ion: 43 Resp: 20812
Ion Ratio Lower Upper
43 100
58 28.9 27.0 40.6

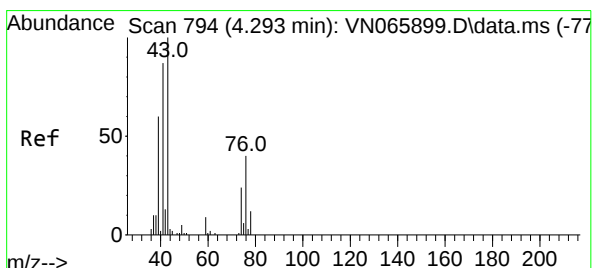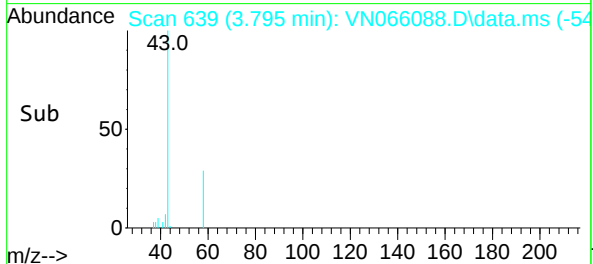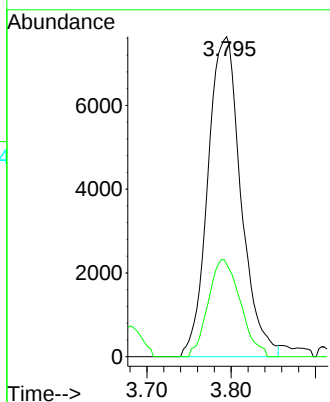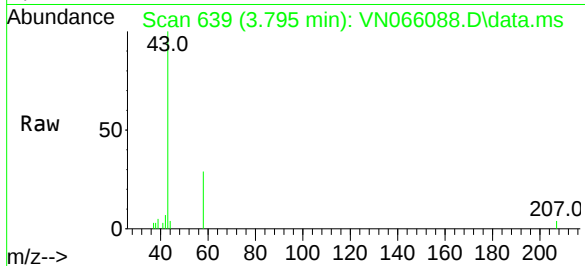

#18
Methyl Acetate
Concen: 0.57 ug/l
RT: 4.303 min Scan# 797
Delta R.T. 0.010 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51


Tgt Ion: 43 Resp: 745
Ion Ratio Lower Upper
43 100
74 0.0 19.5 29.3#

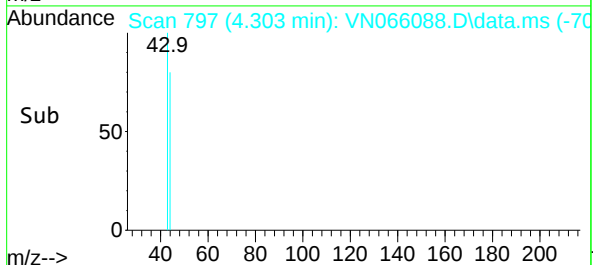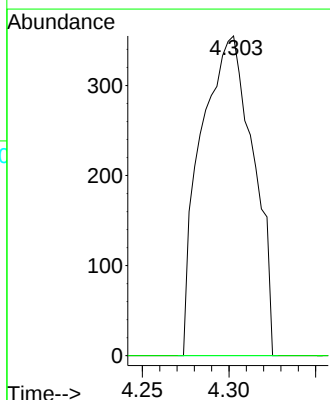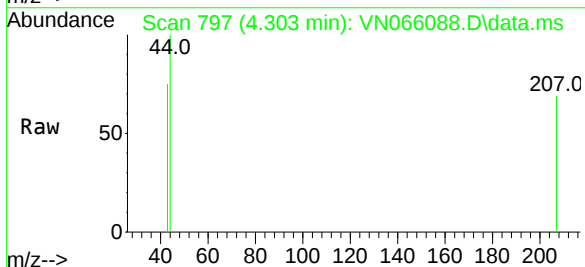






#20
Methylene Chloride
Concen: 5.76 ug/l
RT: 4.521 min Scan# 865
Delta R.T. 0.016 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampleId :
41700







Tgt Ion:	84	Resp:	8433
Ion	Ratio	Lower	Upper
84	100		
49	120.2	94.6	141.8
51	34.8	29.9	44.9
86	63.2	51.4	77.2

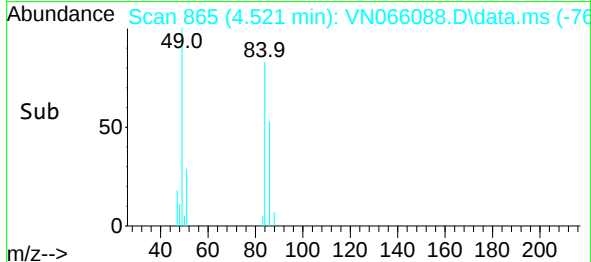

#25
2-Butanone
Concen: 5.30 ug/l
RT: 6.798 min Scan# 1573
Delta R.T. -0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion:	43	Resp:	4136
Ion	Ratio	Lower	Upper
43	100		
72	24.7	23.1	34.7

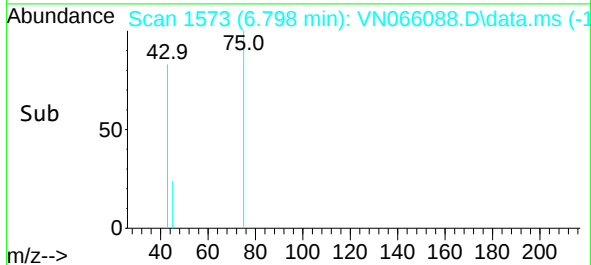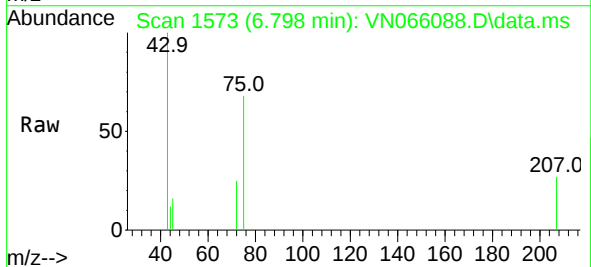

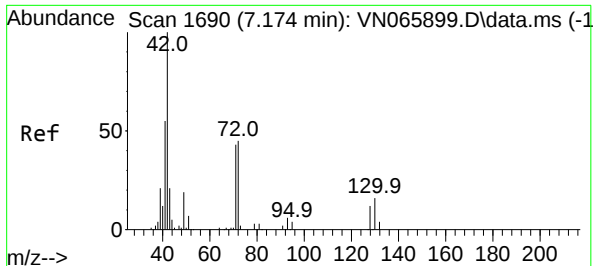

#29

Tetrahydrofuran

Concen: 0.36 ug/l

RT: 7.171 min Scan# 1689





Delta R.T. -0.003 min

Lab File: VN066088.D

Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampled :
41700

Tgt Ion: 42	Resp: 194
Ion Ratio	Lower Upper
42 100	
72 0.0	36.6 55.0#
71 0.0	34.3 51.5#

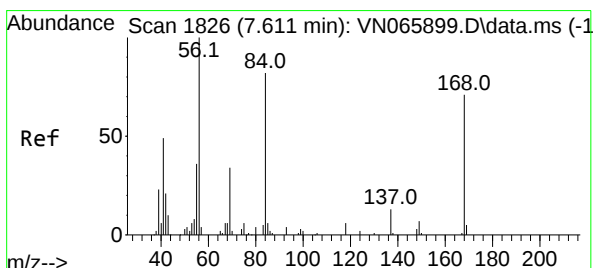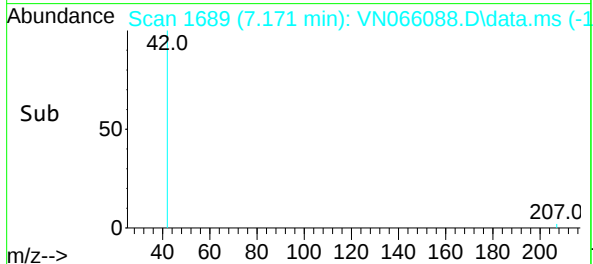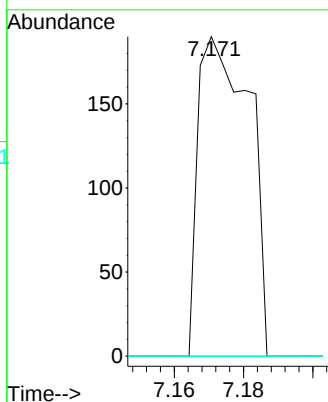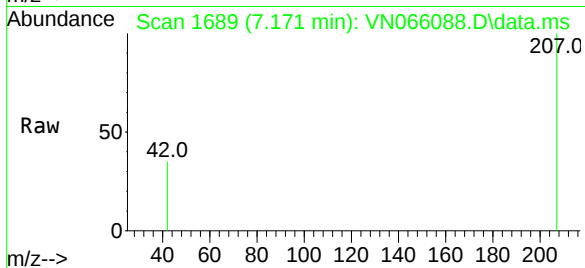

#31

Cyclohexane

Concen: 1.01 ug/l




RT: 7.627 min Scan# 1831


Delta R.T. 0.016 min

Lab File: VN066088.D

Acq: 1 Mar 2021 19:51

Tgt Ion: 56	Resp: 2366
Ion Ratio	Lower Upper
56 100	
69 156.0	26.6 39.8#
84 105.2	70.4 105.6


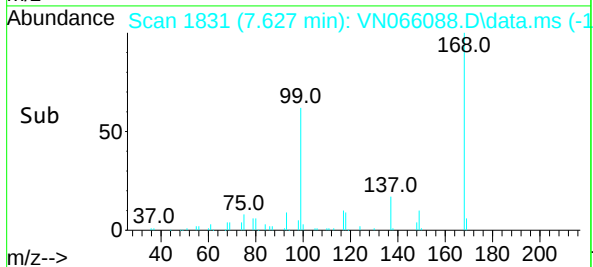
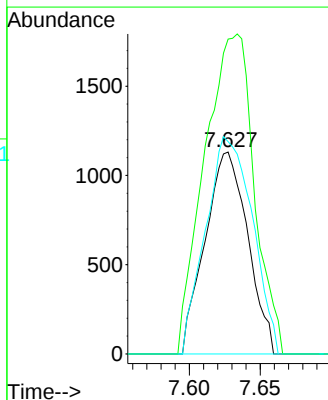
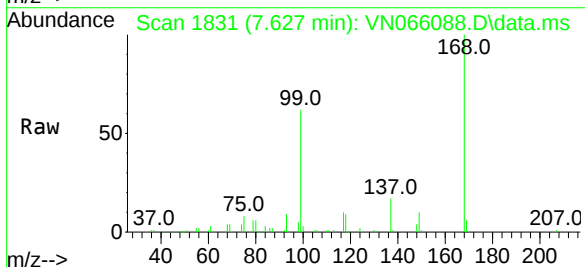




#33
1,2-Dichloroethane-d4
Concen: 49.80 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion: 65 Resp: 78567
Ion Ratio Lower Upper
65 100
67 49.1 0.0 107.2

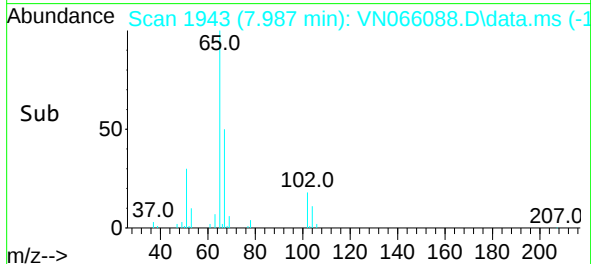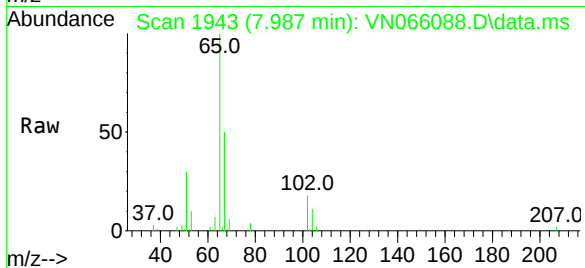

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.550 min Scan# 2118
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 114 Resp: 185309
Ion Ratio Lower Upper
114 100
63 20.7 0.0 38.6
88 16.4 0.0 30.6


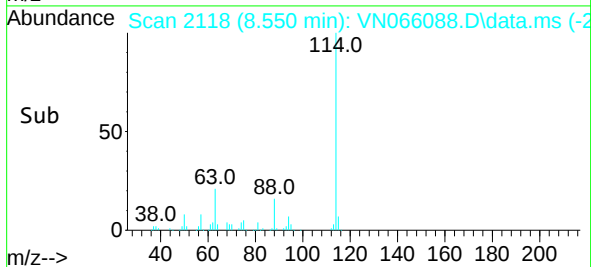

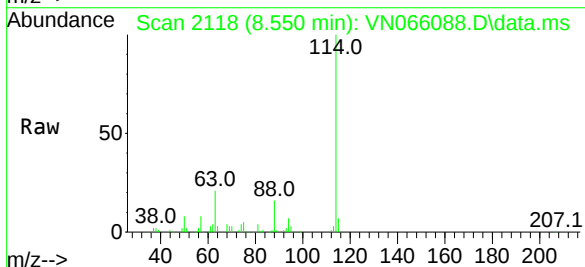


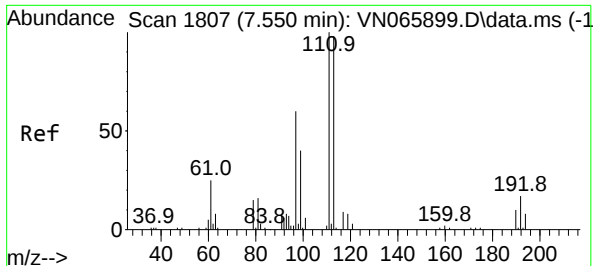

#35
Dibromofluoromethane
Concen: 49.40 ug/l
RT: 7.553 min Scan# 1808
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion:113 Resp: 56659
Ion Ratio Lower Upper
113 100
111 101.9 82.2 123.2
192 18.2 15.4 23.0

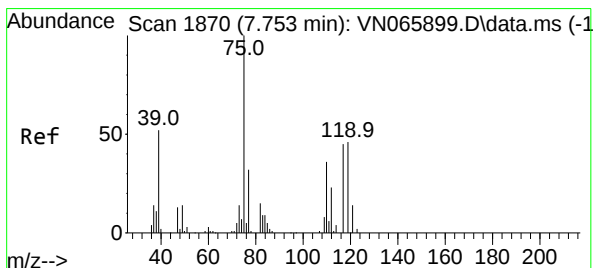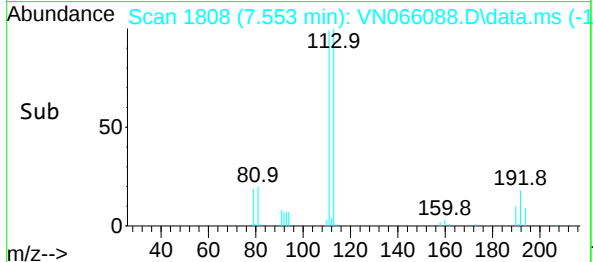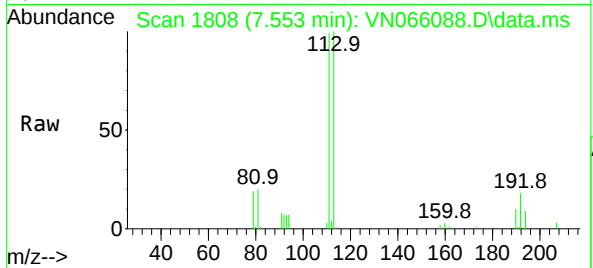

#36
1,1-Dichloropropene
Concen: 4.61 ug/l
RT: 7.627 min Scan# 1831
Delta R.T. -0.126 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 75 Resp: 8423
Ion Ratio Lower Upper
75 100
110 8.3 18.2 54.6#
77 0.0 24.9 37.3#

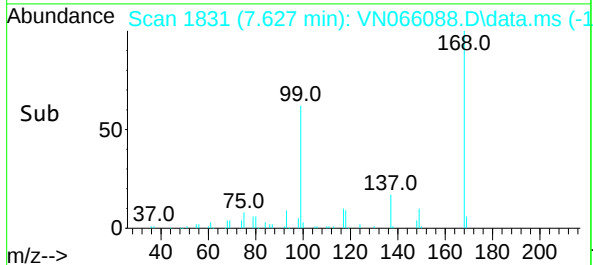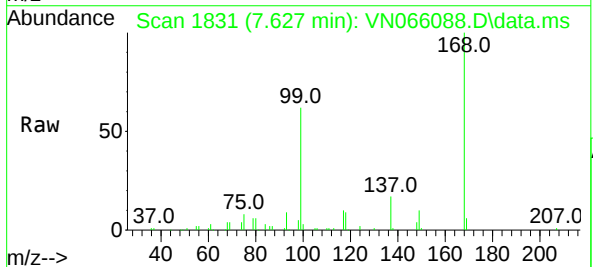

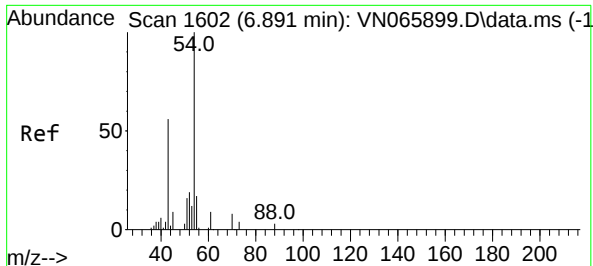

#37

Ethyl Acetate

Concen: 2.51 ug/l

RT: 6.798 min Scan# 1573





Delta R.T. -0.093 min

Lab File: VN066088.D

Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampleId :
41700

Tgt Ion:	43	Resp:	4136
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.6	17.4#
70	0.0	8.6	13.0#

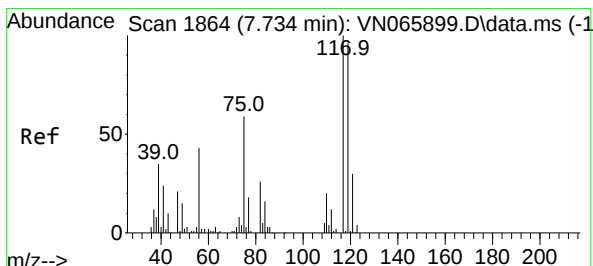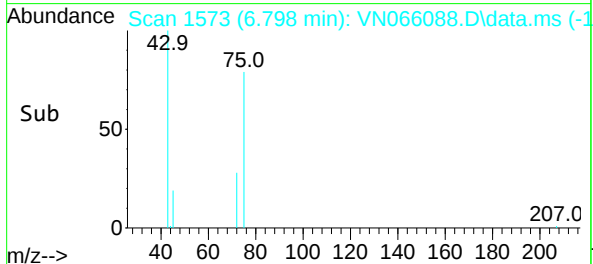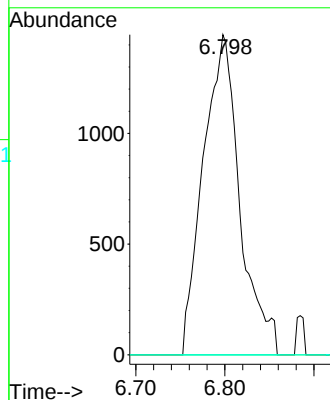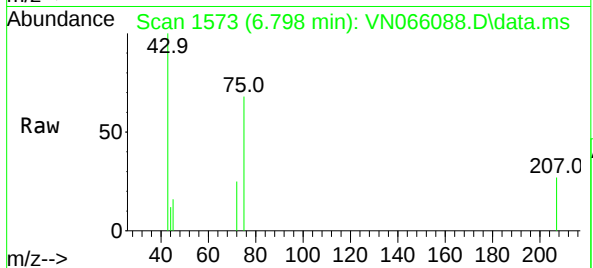

#38

Carbon Tetrachloride

Concen: 6.92 ug/l




RT: 7.627 min Scan# 1831


Delta R.T. -0.107 min

Lab File: VN066088.D

Acq: 1 Mar 2021 19:51

Tgt Ion:	117	Resp:	11747
Ion	Ratio	Lower	Upper
117	100		
119	4.8	76.0	114.0#
121	0.0	24.5	36.7#


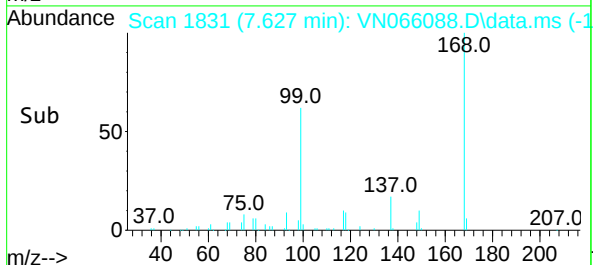
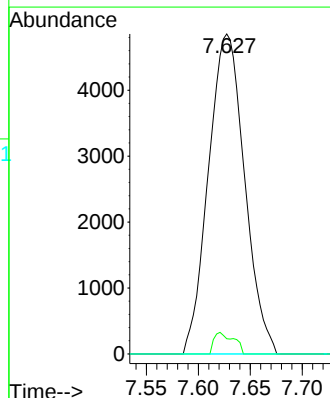
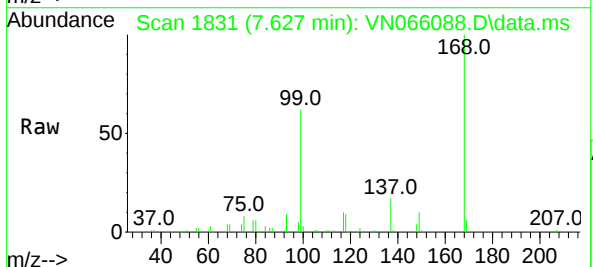


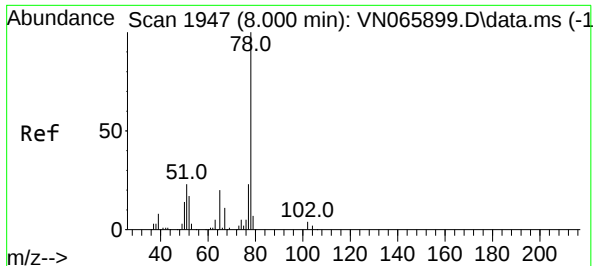

#40
Benzene
Concen: 0.88 ug/l
RT: 8.000 min Scan# 1947
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion: 78 Resp: 4927
Ion Ratio Lower Upper
78 100
77 30.3 19.0 28.4#

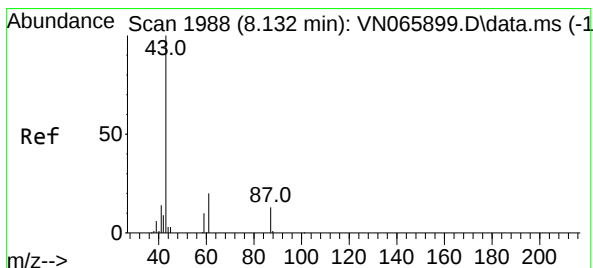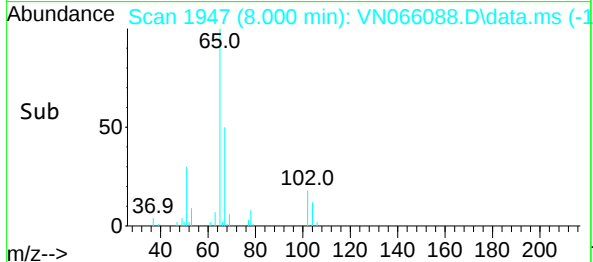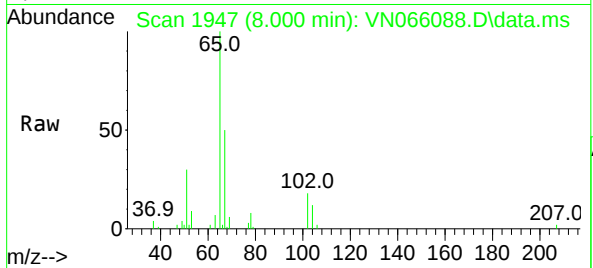

#43
Isopropyl Acetate
Concen: 3.28 ug/l
RT: 8.126 min Scan# 1986
Delta R.T. -0.006 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 43 Resp: 8619
Ion Ratio Lower Upper
43 100
61 20.9 22.5 33.7#
87 13.1 11.1 16.7

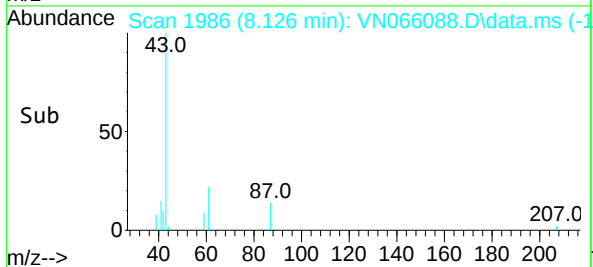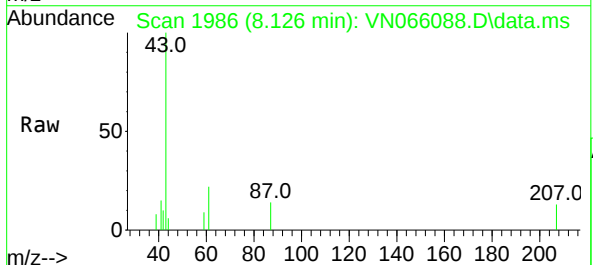



#45

1,2-Dichloropropane

Concen: 0.31 ug/l

RT: 9.232 min Scan# 2330

Delta R.T. 0.148 min

Lab File: VN066088.D





Acq: 1 Mar 2021 19:51

Tgt Ion: 63 Resp: 446

Ion Ratio Lower Upper

63 100

65 0.0 24.9 37.3#

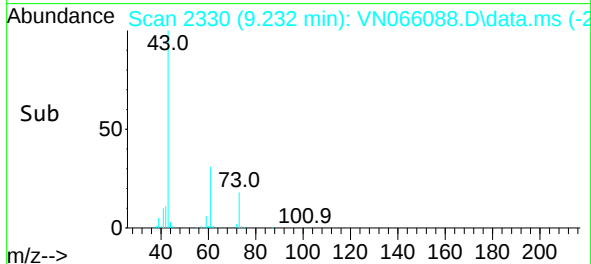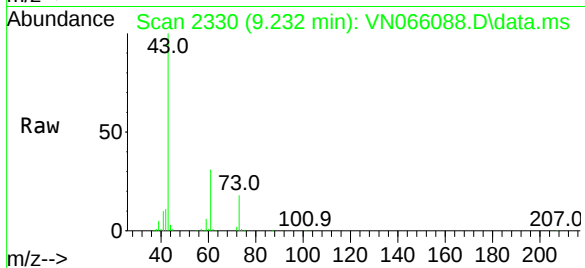

#48

Methyl methacrylate

Concen: 1.56 ug/l

RT: 9.138 min Scan# 2301

Delta R.T. -0.030 min

Lab File: VN066088.D

Acq: 1 Mar 2021 19:51




Tgt Ion: 41 Resp: 2073


Ion Ratio Lower Upper

41 100

69 0.0 75.9 113.9#

39 0.0 46.6 69.8#


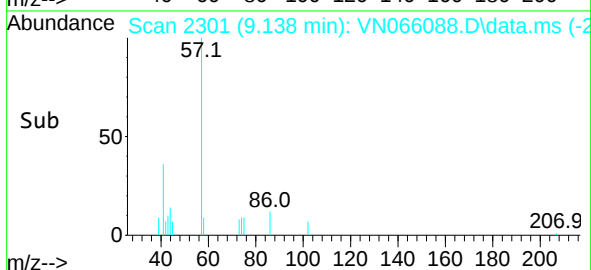

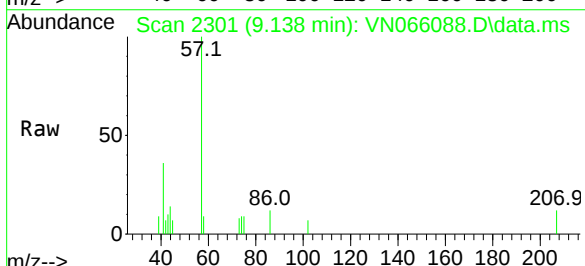




#50
Toluene-d8
Concen: 47.85 ug/l
RT: 10.058 min Scan# 2587
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampleId :
41700


Tgt Ion: 98 Resp: 225260
Ion Ratio Lower Upper
98 100
100 66.3 50.5 75.7

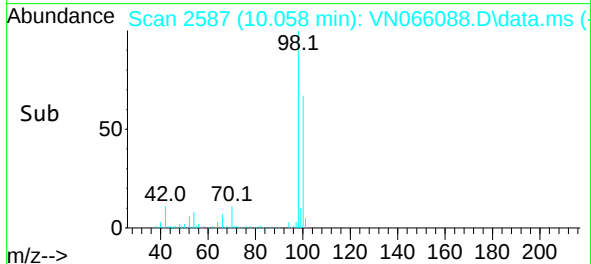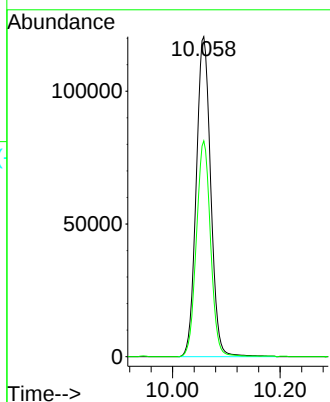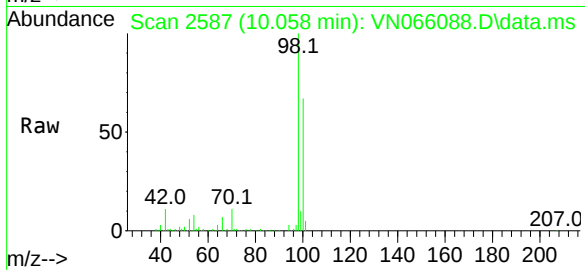

#51
4-Methyl-2-Pentanone
Concen: 1.74 ug/l
RT: 9.949 min Scan# 2553
Delta R.T. -0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 43 Resp: 2786
Ion Ratio Lower Upper
43 100
58 28.9 32.5 48.7#


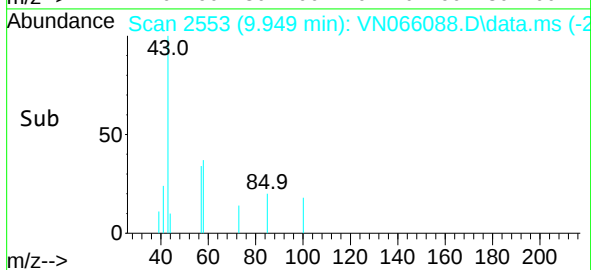
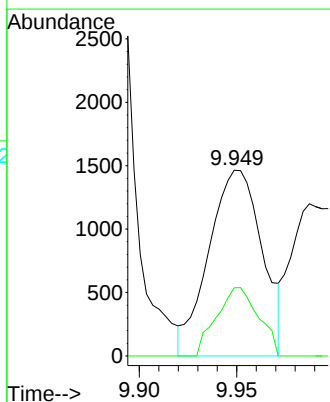
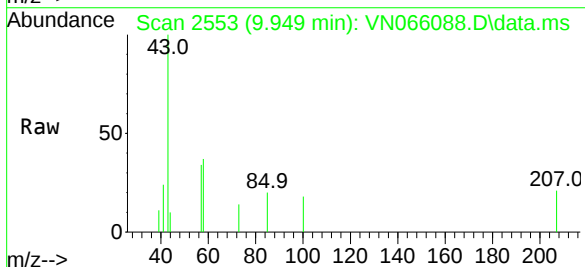




#52
Toluene
Concen: 1.68 ug/l
RT: 10.122 min Scan# 2607
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion: 92 Resp: 5775
Ion Ratio Lower Upper
92 100
91 174.4 140.7 211.1

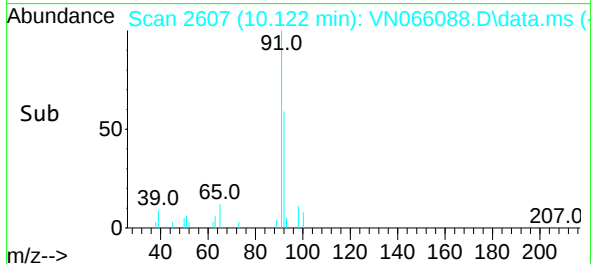

#54
cis-1,3-Dichloropropene
Concen: 6.64 ug/l
RT: 9.872 min Scan# 2529
Delta R.T. 0.065 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 75 Resp: 14665
Ion Ratio Lower Upper
75 100
77 0.0 24.9 37.3#
39 27.9 36.2 54.4#


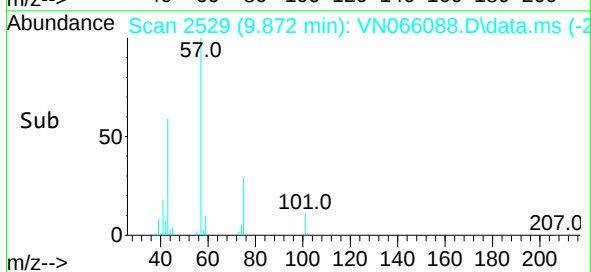




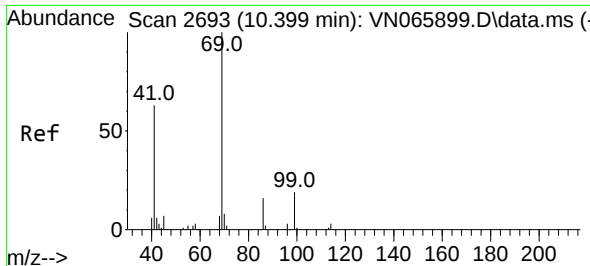

#56
Ethyl methacrylate
Concen: 0.36 ug/l
RT: 10.193 min Scan# 2629
Delta R.T. -0.206 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion: 69 Resp: 692
Ion Ratio Lower Upper
69 100
41 0.0 49.6 74.4#
39 14.5 28.0 42.0#

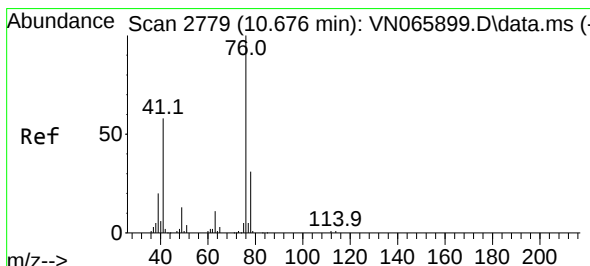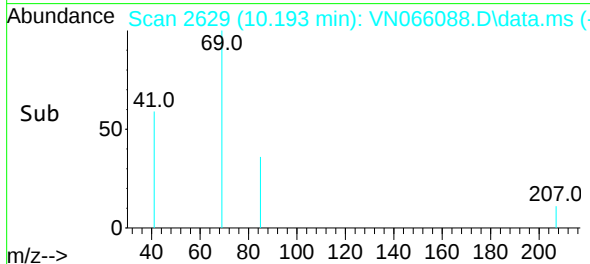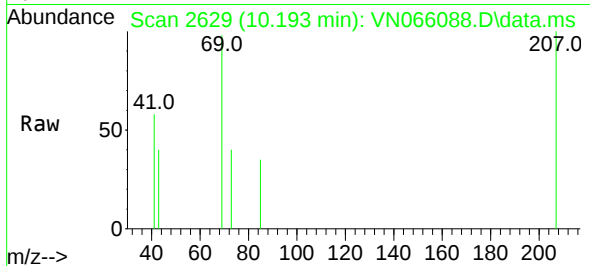

#57
1,3-Dichloropropane
Concen: 3.28 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.057 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51


Tgt Ion: 76 Resp: 7447
Ion Ratio Lower Upper
76 100
78 0.0 25.7 38.5#

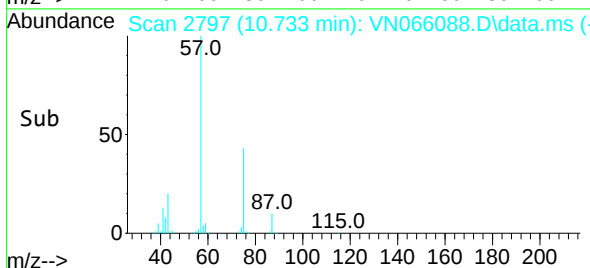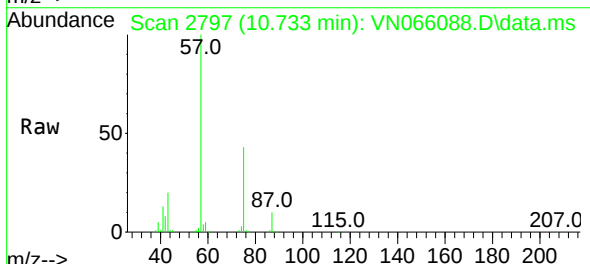



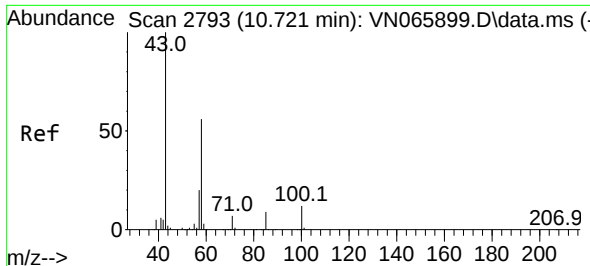


#59
2-Hexanone
Concen: 89.52 ug/l
RT: 10.733 min Scan# 2797
Delta R.T. 0.012 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampled :
41700



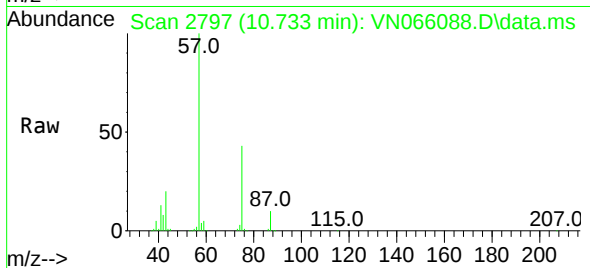



Tgt Ion: 43 Resp: 102036
Ion Ratio Lower Upper
43 100
58 19.8 28.1 84.3#

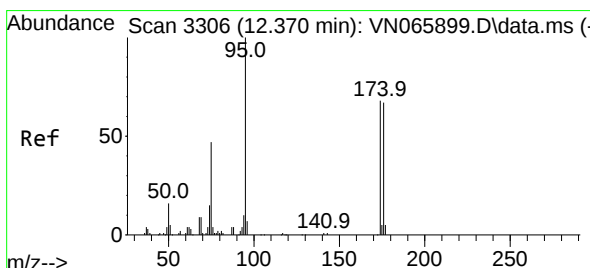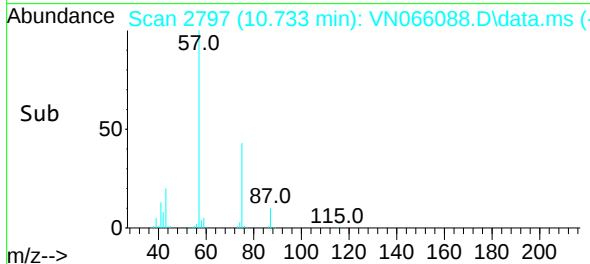

#62
4-Bromofluorobenzene
Concen: 47.26 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 95 Resp: 83521
Ion Ratio Lower Upper
95 100
174 73.4 0.0 169.0
176 71.3 0.0 162.4


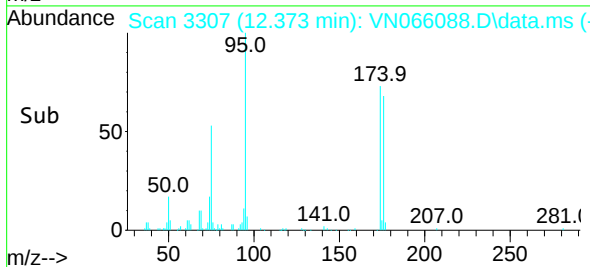

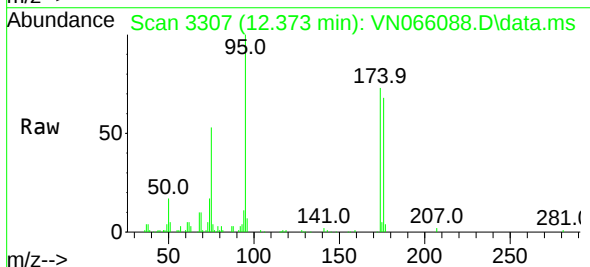


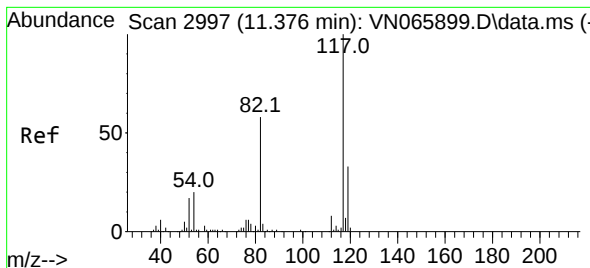

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampleId :
41700


Tgt Ion:117 Resp: 169203
Ion Ratio Lower Upper
117 100
82 57.4 43.7 65.5
119 31.5 26.1 39.1

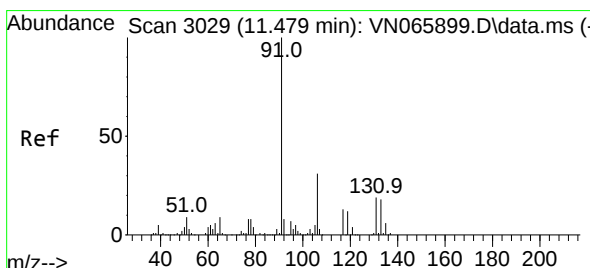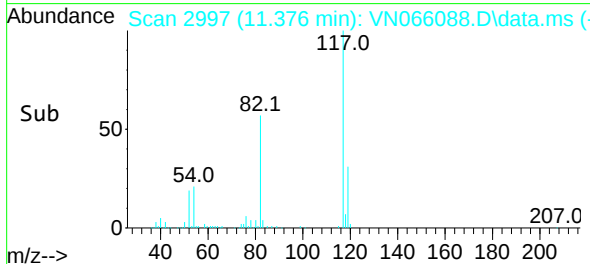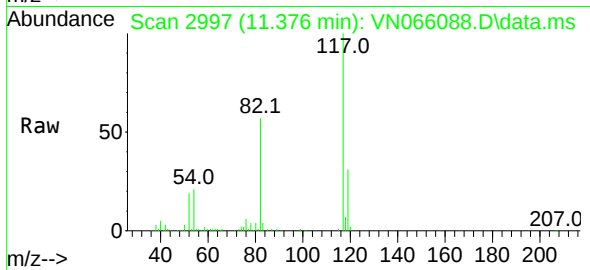

#67
Ethyl Benzene
Concen: 0.28 ug/l
RT: 11.479 min Scan# 3029
Delta R.T. 0.000 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 91 Resp: 1795
Ion Ratio Lower Upper
91 100
106 33.6 25.5 38.3


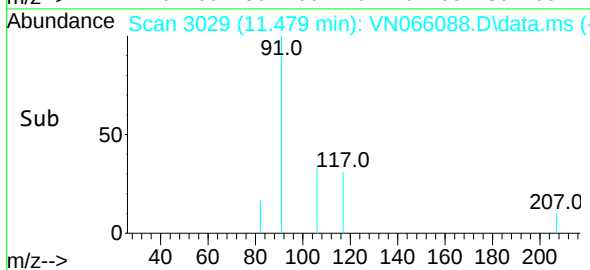

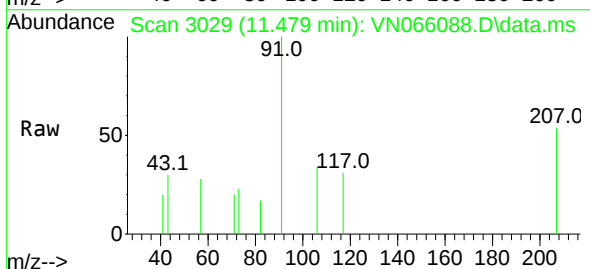




#68
m/p-Xylenes
Concen: 0.93 ug/l
RT: 11.585 min Scan# 3062
Delta R.T. -0.007 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion:106 Resp: 2228
Ion Ratio Lower Upper
106 100
91 230.1 161.4 242.0

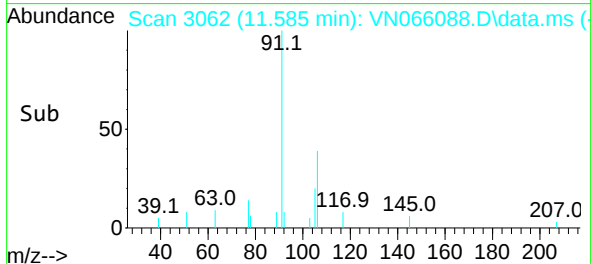

#69
o-Xylene
Concen: 0.55 ug/l
RT: 11.920 min Scan# 3166
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion:106 Resp: 1278
Ion Ratio Lower Upper
106 100
91 250.4 106.8 320.4


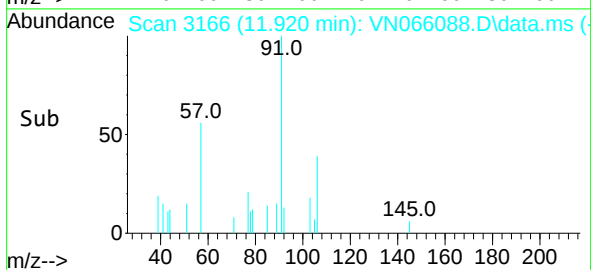

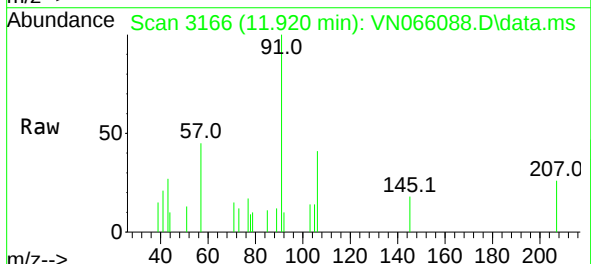


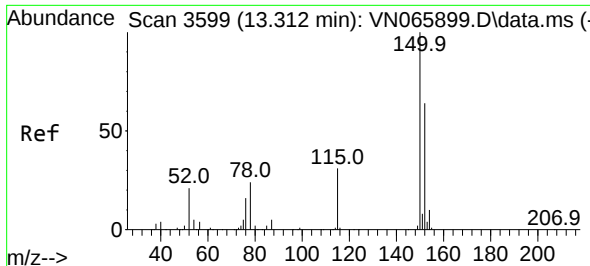

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.315 min Scan# 3600
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion:152 Resp: 73064
Ion Ratio Lower Upper
152 100
115 64.1 28.5 85.6
150 159.2 0.0 347.6

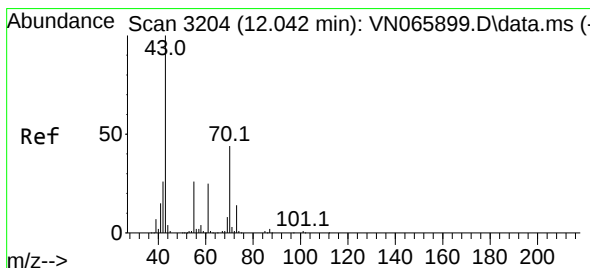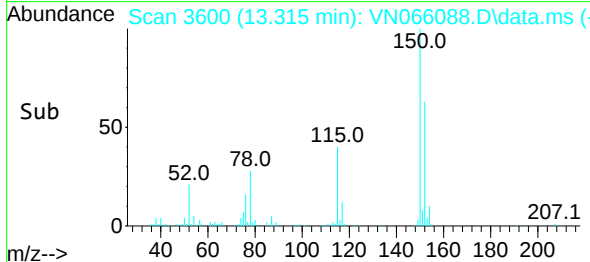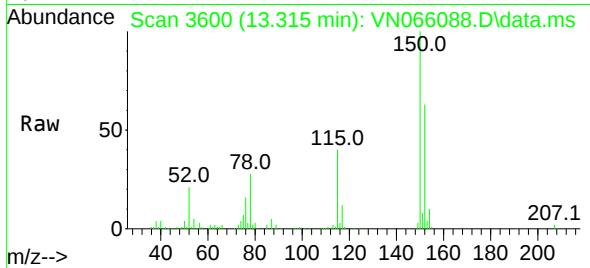

#74
N-ethyl acetate
Concen: 0.54 ug/l
RT: 12.026 min Scan# 3199
Delta R.T. -0.016 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 43 Resp: 1110
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 3.4 20.7 31.1#
61 0.0 19.1 28.7#


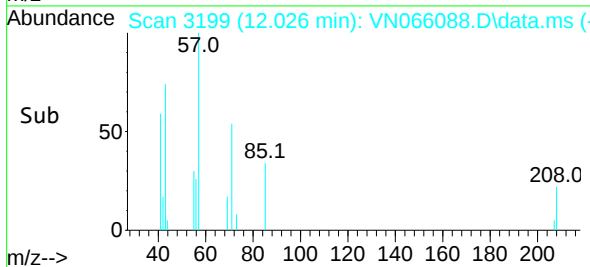

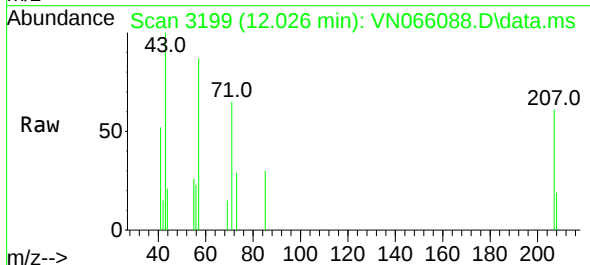


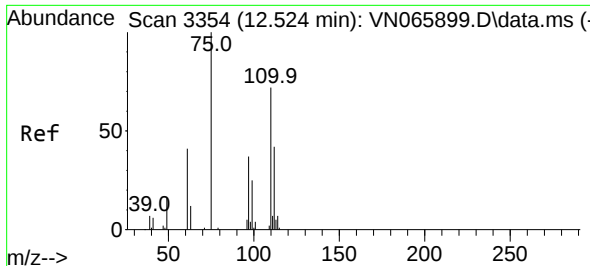

#76
1,2,3-Trichloropropane
Concen: 24.60 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion: 75 Resp: 43183
Ion Ratio Lower Upper
75 100
77 1.6 0.0 0.0#

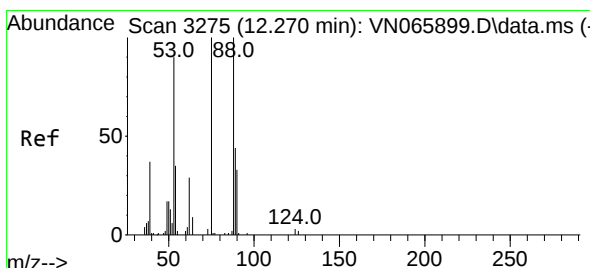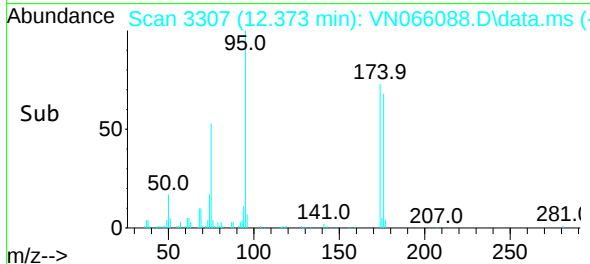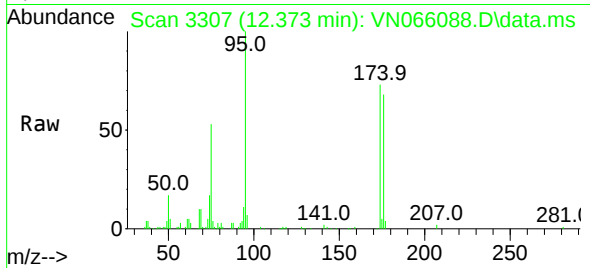

#81
trans-1,4-Dichloro-2-butene
Concen: 78.41 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 75 Resp: 43183
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#


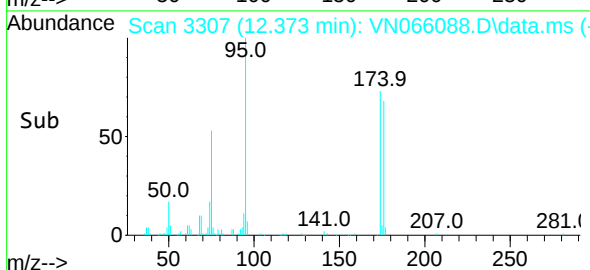

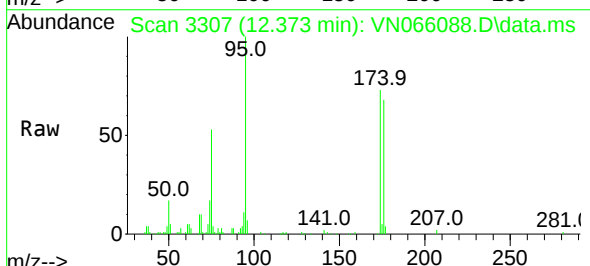




#84
1,2,4-Trimethylbenzene
Concen: 0.59 ug/l
RT: 13.013 min Scan# 3506
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51




Instrument :
MSVOA_N
ClientSampled :
41700


Tgt Ion:105 Resp: 2989
Ion Ratio Lower Upper
105 100
120 41.2 22.4 67.0

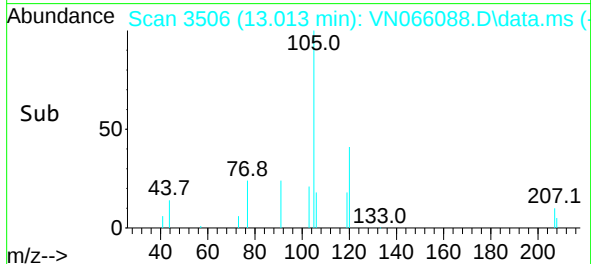

#85
sec-Butylbenzene
Concen: 0.55 ug/l
RT: 13.013 min Scan# 3506
Delta R.T. -0.129 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion:105 Resp: 2989
Ion Ratio Lower Upper
105 100
134 0.0 10.0 30.0#


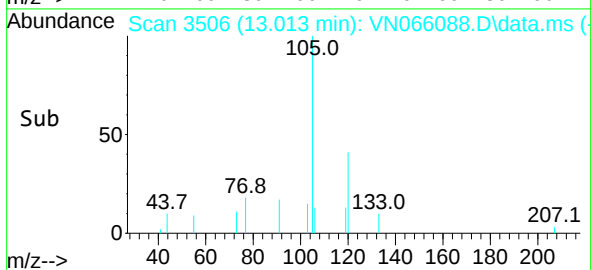

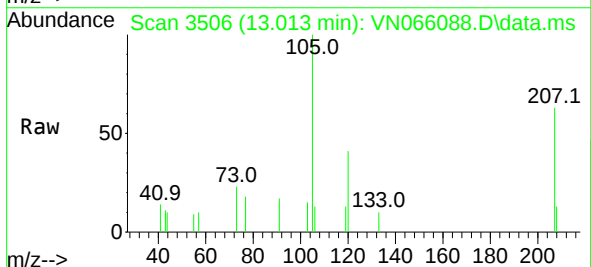




#92
1,2-Dibromo-3-Chloropropane
Concen: 1.02 ug/l
RT: 14.244 min Scan# 3889
Delta R.T. 0.006 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Instrument :
MSVOA_N
ClientSampled :
41700

Tgt Ion: 75 Resp: 61
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

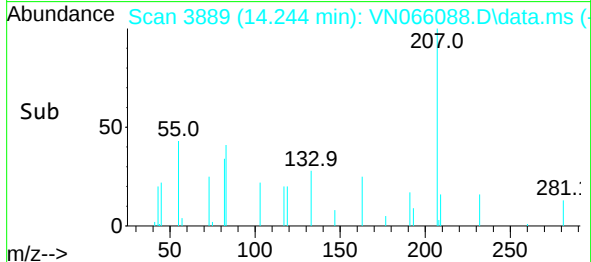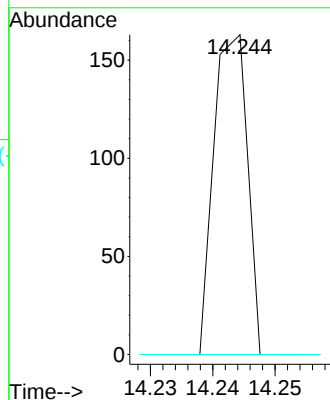

#95
Naphthalene
Concen: 4.45 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. 0.003 min
Lab File: VN066088.D
Acq: 1 Mar 2021 19:51

Tgt Ion: 128 Resp: 6301
Ion Ratio Lower Upper
128 100
127 12.5 10.2 15.2
129 10.9 8.6 13.0

