


Data Path : Z:\voasrv\HPCHEM1\MSVOA\_N\Data\VN030121\  
Data File : VN066067.D  
Acq On : 1 Mar 2021 9:17  
Operator : JC/MD  
Sample : BFB  
Misc : 5.00mL/MSVOA\_N/WATER  
ALS Vial : 1 Sample Multiplier: 1

Instrument :  
MSVOA\_N  
ClientSampleId :  
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA\_N\methods\82N021721W.M  
Title : SW846 8260  
Last Update : Wed Feb 17 15:48:13 2021

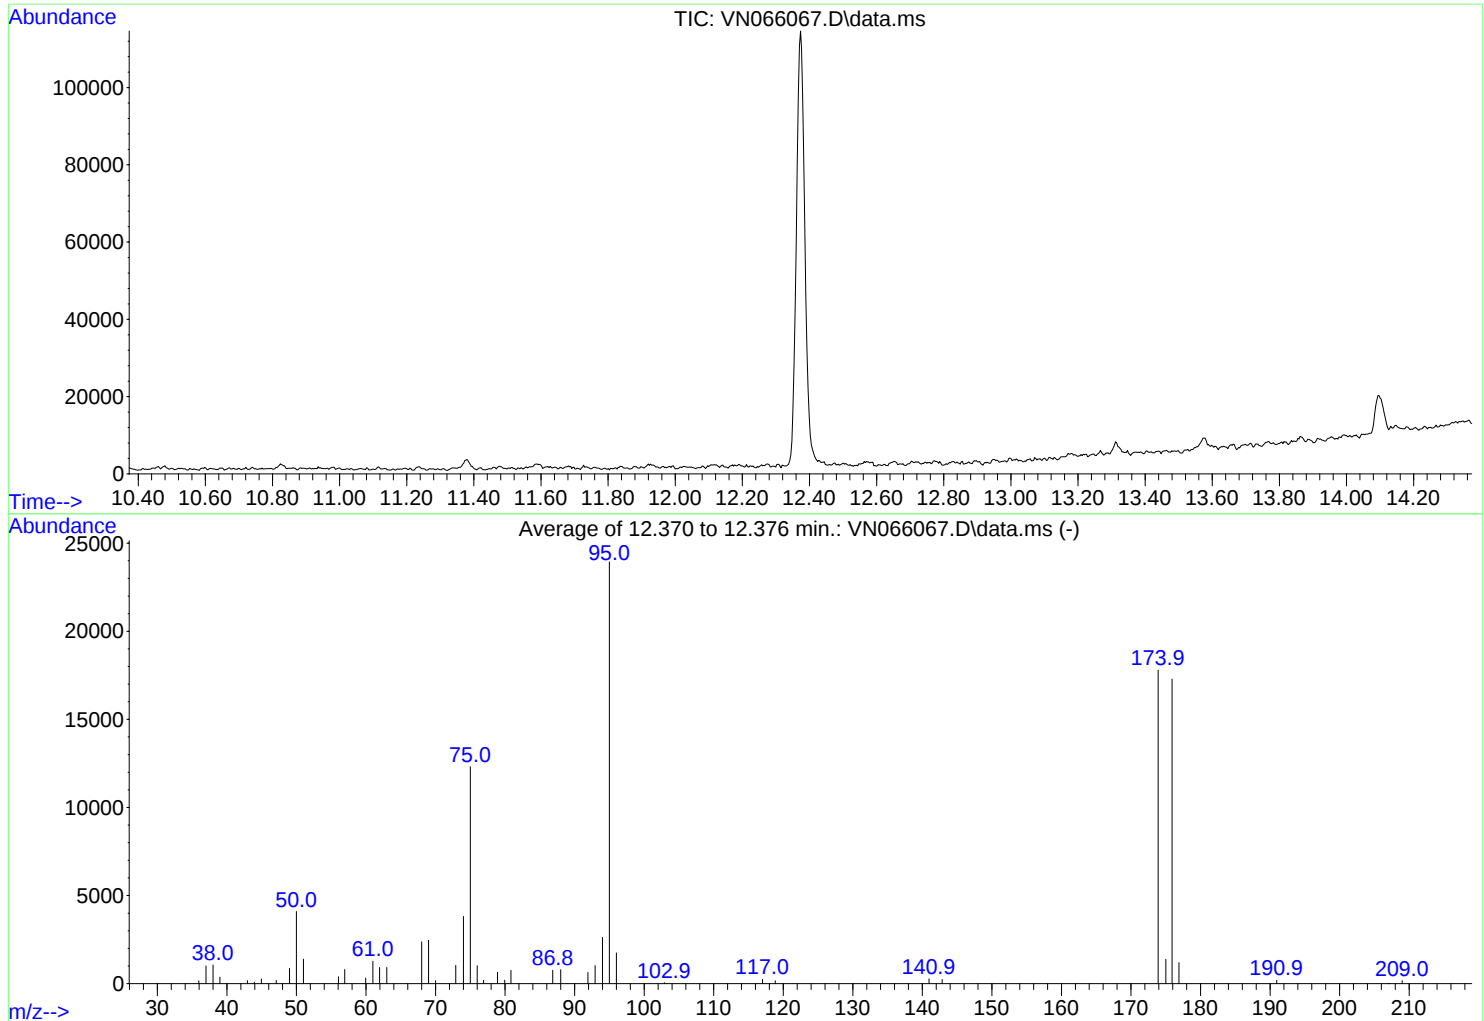

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3293

| Target<br>Mass | Rel. to<br>Mass | Lower<br>Limit% | Upper<br>Limit% | Rel.<br>Abn% | Raw<br>Abn | Result<br>Pass/Fail |
|----------------|-----------------|-----------------|-----------------|--------------|------------|---------------------|
| 50             | 95              | 15              | 40              | 17.1         | 4092       | PASS                |
| 75             | 95              | 30              | 60              | 51.5         | 12319      | PASS                |
| 95             | 95              | 100             | 100             | 100.0        | 23941      | PASS                |
| 96             | 95              | 5               | 9               | 7.3          | 1745       | PASS                |
| 173            | 174             | 0.00            | 2               | 0.0          | 0          | PASS                |
| 174            | 95              | 50              | 100             | 74.3         | 17787      | PASS                |
| 175            | 174             | 5               | 9               | 7.8          | 1381       | PASS                |
| 176            | 174             | 95              | 101             | 97.2         | 17291      | PASS                |
| 177            | 176             | 5               | 9               | 6.9          | 1189       | PASS                |