

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030122\
 Data File : VN071124.D
 Acq On : 01 Mar 2022 17:24
 Operator : JC\MD
 Sample : N1689-04
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 MW-40

Quant Time: Mar 02 03:31:27 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
 Quant Title : SW846 8260
 QLast Update : Mon Feb 21 07:57:15 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.081	168	912115	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	8.963	114	1465359	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.739	117	1317124	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.669	152	467999	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.434	65	555210	53.287	ug/l	0.00
Spiked Amount 50.000	Range 61 - 141		Recovery = 106.580%			
35) Dibromofluoromethane	8.016	113	422809	48.510	ug/l	0.00
Spiked Amount 50.000	Range 69 - 133		Recovery = 97.020%			
50) Toluene-d8	10.439	98	1776969	50.767	ug/l	0.00
Spiked Amount 50.000	Range 65 - 126		Recovery = 101.540%			
62) 4-Bromofluorobenzene	12.727	95	617638	49.366	ug/l	0.00
Spiked Amount 50.000	Range 58 - 135		Recovery = 98.740%			
Target Compounds						
					Qvalue	
3) Chloromethane	2.305	50	3073	0.258	ug/l #	82
11) Tert butyl alcohol	5.357	59	696827	366.974	ug/l	98
13) Acrolein	4.046	56	576	0.339	ug/l #	14
15) Acrylonitrile	5.610	53	3700	0.662	ug/l #	24
16) Acetone	4.293	43	18110	3.156	ug/l	95
18) Methyl Acetate	4.863	43	3139	Below Cal	#	70
19) Methyl tert-butyl Ether	5.616	73	275177	8.785	ug/l	94
22) Diisopropyl ether	6.493	45	213319	6.531	ug/l #	86
23) Vinyl Acetate	6.493	43	103990	3.761	ug/l #	72
25) 2-Butanone	7.340	43	4074	0.534	ug/l	91
29) Tetrahydrofuran	7.681	42	4852	0.981	ug/l #	32
31) Cyclohexane	8.092	56	28792	1.598	ug/l #	45
36) 1,1-Dichloropropene	8.081	75	68865	4.823	ug/l #	49
37) Ethyl Acetate	7.340	43	4074	0.266	ug/l #	68
38) Carbon Tetrachloride	8.081	117	89942	6.393	ug/l #	16
39) Methylcyclohexane	9.457	83	5706	0.311	ug/l #	93
40) Benzene	8.457	78	2184830	51.725	ug/l	99
43) Isopropyl Acetate	8.528	43	16837	0.697	ug/l #	55
51) 4-Methyl-2-Pentanone	10.328	43	3601	0.245	ug/l	92
52) Toluene	10.504	92	8346	0.314	ug/l	86
58) 2-Chloroethyl Vinyl ether	10.192	63	206	31.853	ug/l #	45
59) 2-Hexanone	11.122	43	12095	1.197	ug/l	63
67) Ethyl Benzene	11.839	91	19737	0.397	ug/l	99
68) m/p-Xylenes	11.951	106	8391	0.437	ug/l	89
69) o-Xylene	12.275	106	9427	0.503	ug/l	91
73) Isopropylbenzene	12.575	105	19938	0.529	ug/l	98
76) 1,2,3-Trichloropropane	12.727	75	315020	28.588	ug/l #	1
80) 1,3,5-Trimethylbenzene	13.057	105	7797	0.255	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.727	75	315020	92.640	ug/l #	5
84) 1,2,4-Trimethylbenzene	13.363	105	16648	0.554	ug/l	90
90) Hexachloroethane	14.274	117	1847	0.330	ug/l #	6
93) 1,2,4-Trichlorobenzene	15.269	180	838	2.092	ug/l #	34
95) Naphthalene	15.510	128	20694	5.880	ug/l	98
96) 1,2,3-Trichlorobenzene	15.692	180	823	2.614	ug/l #	54

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030122\
Data File : VN071124.D
Acq On : 01 Mar 2022 17:24
Operator : JC\MD
Sample : N1689-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Time: Mar 02 03:31:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 21 07:57:15 2022
Response via : Initial Calibration


Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


(#)=qualifier out of range (m)=manual integration (+)=signals summed						

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030122\
Data File : VN071124.D
Acq On : 01 Mar 2022 17:24
Operator : JC\MD
Sample : N1689-04
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 13 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Quant Time: Mar 02 03:31:27 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Quant Title : SW846 8260
QLast Update : Mon Feb 21 07:57:15 2022
Response via : Initial Calibration




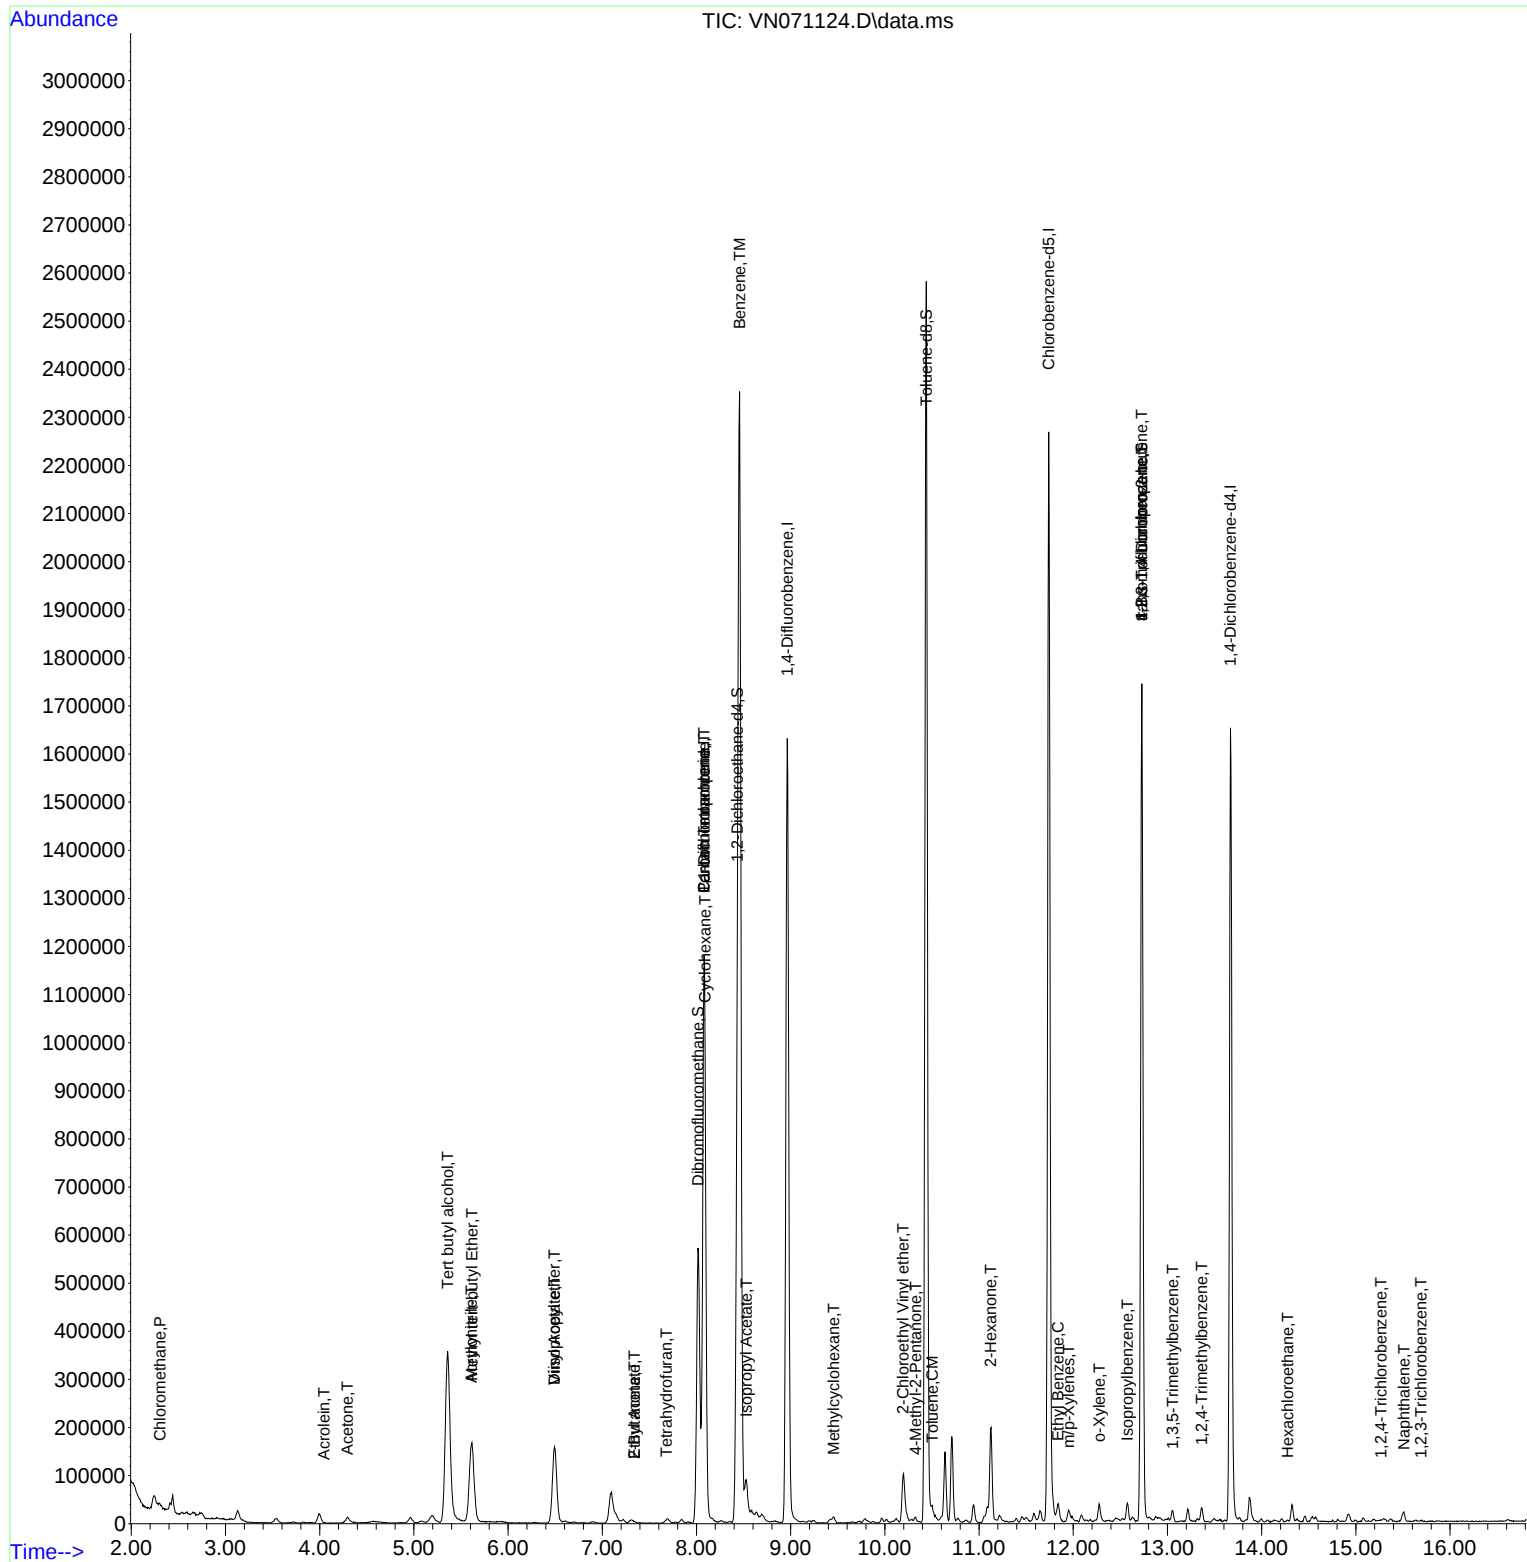




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.081 min Scan# 10
Delta R.T. -0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:168 Resp: 912115
Ion Ratio Lower Upper
168 100
99 56.6 41.3 61.9

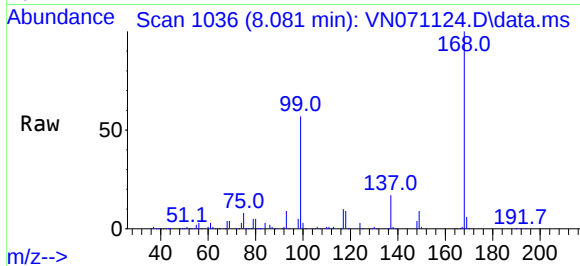

#3
Chloromethane
Concen: 0.258 ug/l
RT: 2.305 min Scan# 54
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 50 Resp: 3073
Ion Ratio Lower Upper
50 100
52 21.7 25.4 38.0#

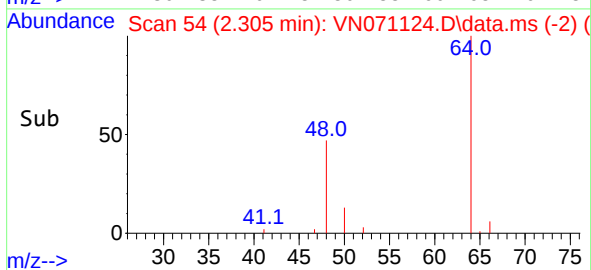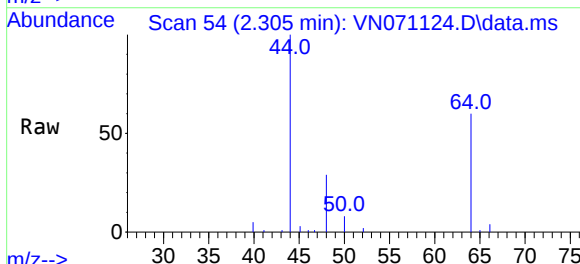



#11

Tert butyl alcohol

Concen: 366.974 ug/l

RT: 5.357 min Scan# 51

Delta R.T. -0.012 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion: 59 Resp: 696827

Ion Ratio Lower Upper

59 100

57 10.2 8.7 13.1

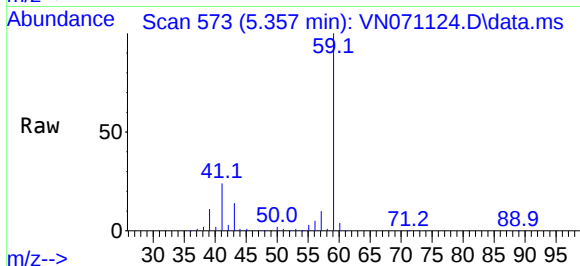

#13

Acrolein

Concen: 0.339 ug/l

RT: 4.046 min Scan# 350

Delta R.T. 0.012 min

Lab File: VN071124.D




Acq: 01 Mar 2022 17:24


Tgt Ion: 56 Resp: 576

Ion Ratio Lower Upper

56 100

55 0.0 56.6 85.0#


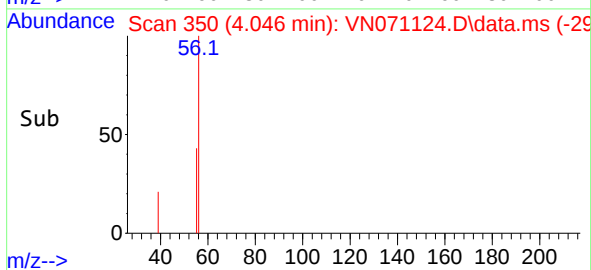

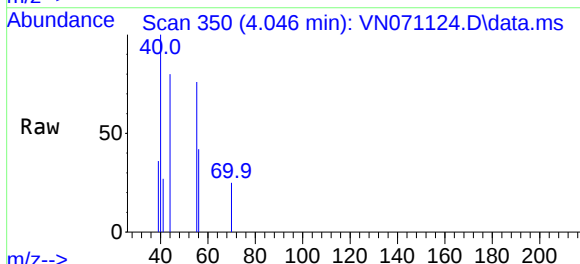




#15
Acrylonitrile
Concen: 0.662 ug/l
RT: 5.610 min Scan# 61
Delta R.T. 0.065 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 53 Resp: 3700
Ion Ratio Lower Upper
53 100
52 2.9 66.2 99.2#
51 65.4 29.6 44.4#



#16
Acetone
Concen: 3.156 ug/l
RT: 4.293 min Scan# 392
Delta R.T. 0.012 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 43 Resp: 18110
Ion Ratio Lower Upper
43 100
58 26.5 23.1 34.7

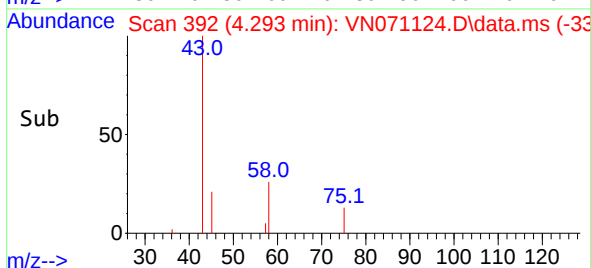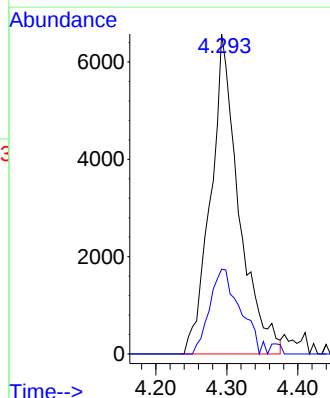



#18

Methyl Acetate

Concen: Below Cal

RT: 4.863 min Scan# 486

Delta R.T. 0.018 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion: 43 Resp: 3139

Ion Ratio Lower Upper

43 100

74 9.4 19.4 29.2#

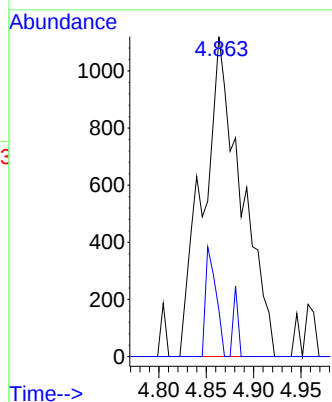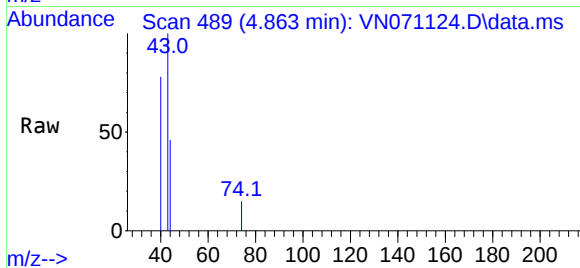

#19

Methyl tert-butyl Ether

Concen: 8.785 ug/l

RT: 5.616 min Scan# 617

Delta R.T. 0.006 min

Lab File: VN071124.D




Acq: 01 Mar 2022 17:24


Tgt Ion: 73 Resp: 275177

Ion Ratio Lower Upper

73 100

57 23.6 16.8 25.2


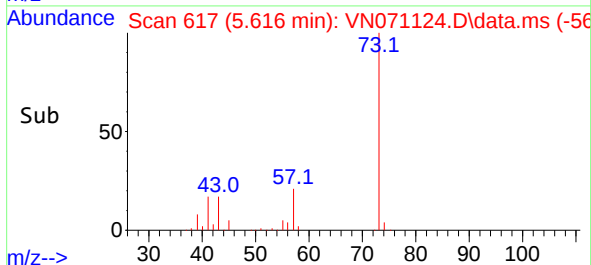

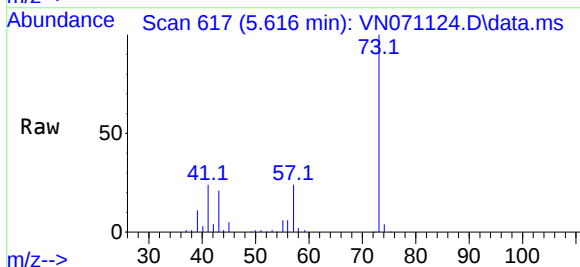




#22
Diisopropyl ether
Concen: 6.531 ug/l
RT: 6.493 min Scan# 766
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 45 Resp: 213319
Ion Ratio Lower Upper
45 100
43 47.9 51.7 77.5#
87 26.8 23.2 34.8
59 10.5 9.4 14.0



#23
Vinyl Acetate
Concen: 3.761 ug/l
RT: 6.493 min Scan# 766
Delta R.T. 0.065 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 43 Resp: 103990
Ion Ratio Lower Upper
43 100
86 0.0 8.5 12.7#

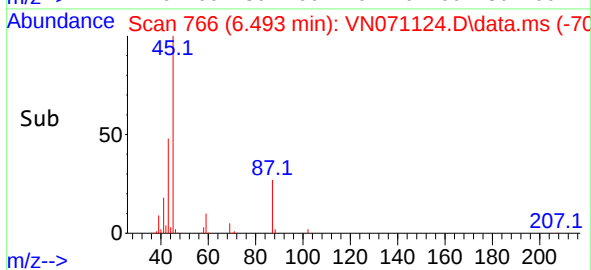



#25

2-Butanone

Concen: 0.534 ug/l

RT: 7.340 min Scan# 910

Delta R.T. 0.012 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24

Instrument :

MSVOA_N

ClientSampleId :





MW-40

Tgt Ion: 43 Resp: 4074

Ion Ratio Lower Upper

43 100

72 22.7 21.7 32.5

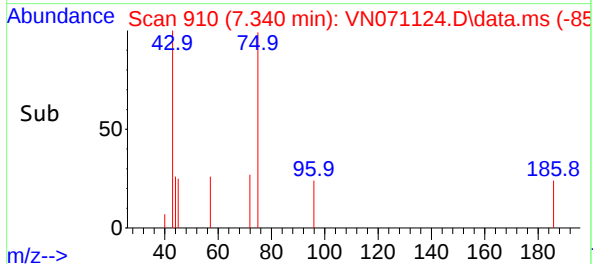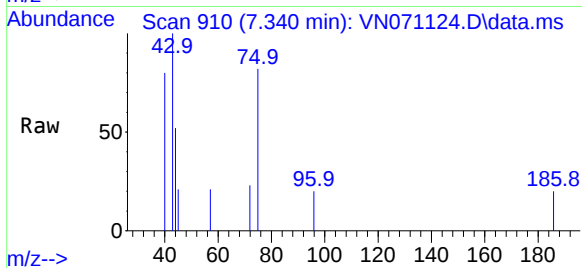

#29

Tetrahydrofuran

Concen: 0.981 ug/l

RT: 7.681 min Scan# 968

Delta R.T. 0.000 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24




Tgt Ion: 42 Resp: 4852


Ion Ratio Lower Upper

42 100

72 0.0 36.3 54.5#

71 0.0 34.7 52.1#


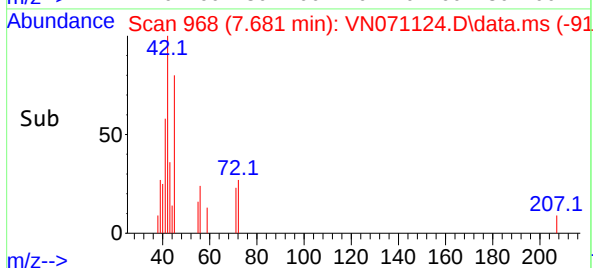
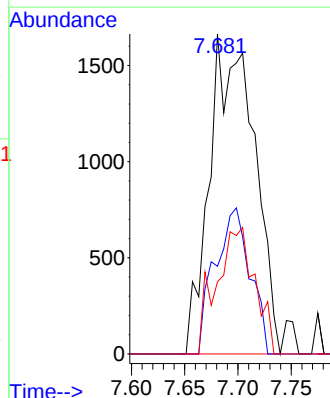
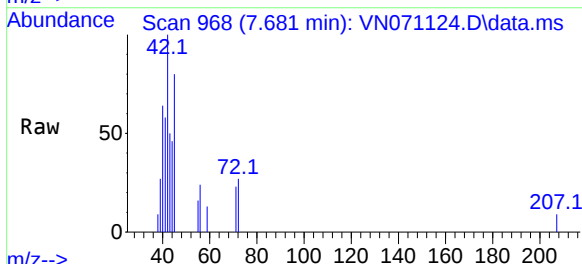


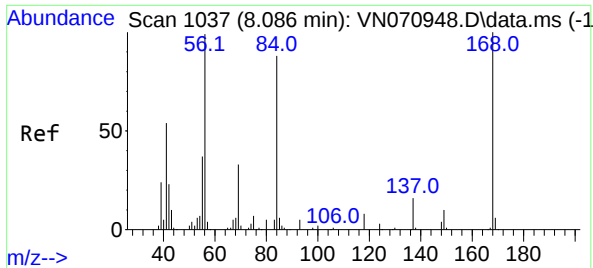

#31
Cyclohexane
Concen: 1.598 ug/l
RT: 8.092 min Scan# 1037
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 56 Resp: 28792
Ion Ratio Lower Upper
56 100
69 107.5 27.1 40.7#
84 118.3 73.4 110.0#

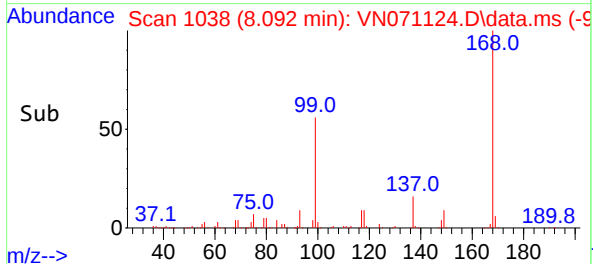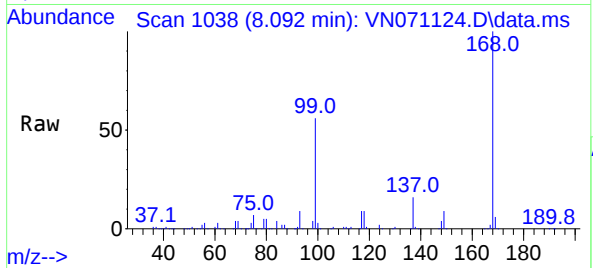

#33
1,2-Dichloroethane-d4
Concen: 53.287 ug/l
RT: 8.434 min Scan# 1096
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 65 Resp: 555210
Ion Ratio Lower Upper
65 100
67 52.8 0.0 103.0


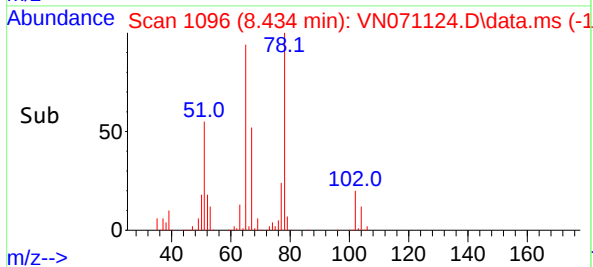

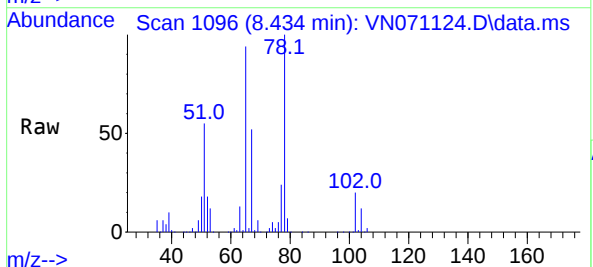




#34
1,4-Difluorobenzene
Concen: 50.000 ug/l
RT: 8.963 min Scan# 1186
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:114 Resp: 1465359
Ion Ratio Lower Upper
114 100
63 21.3 0.0 37.8
88 16.2 0.0 27.4

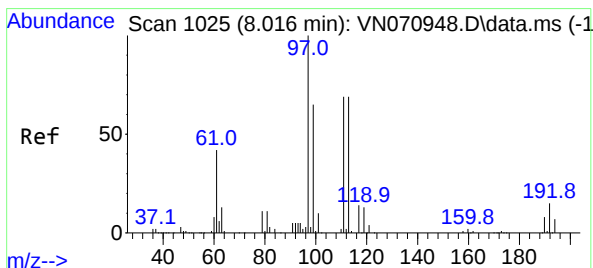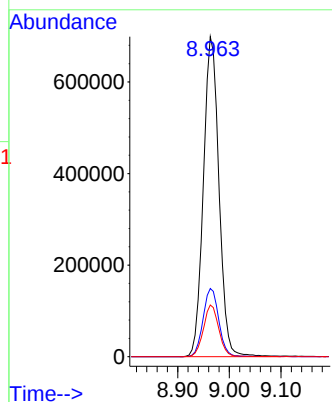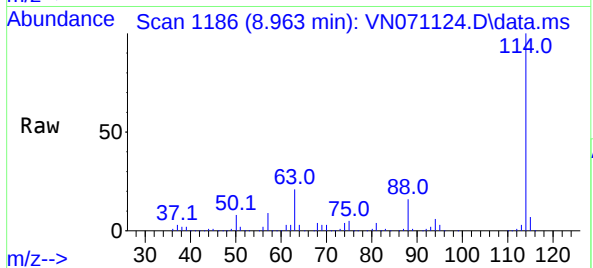

#35
Dibromofluoromethane
Concen: 48.510 ug/l
RT: 8.016 min Scan# 1025
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion:113 Resp: 422809
Ion Ratio Lower Upper
113 100
111 102.9 82.2 123.2
192 20.5 16.9 25.3

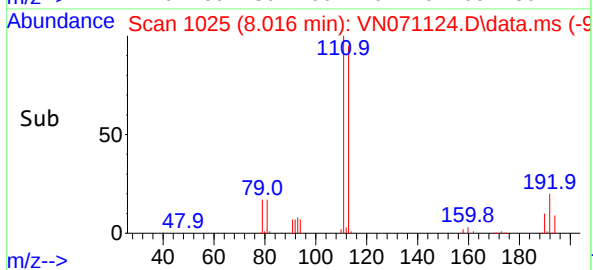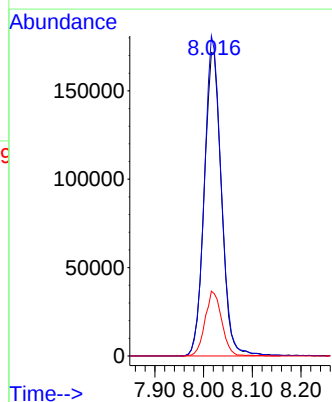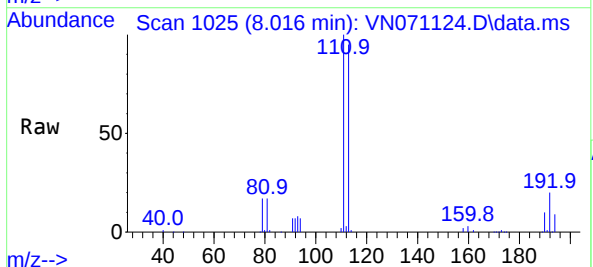

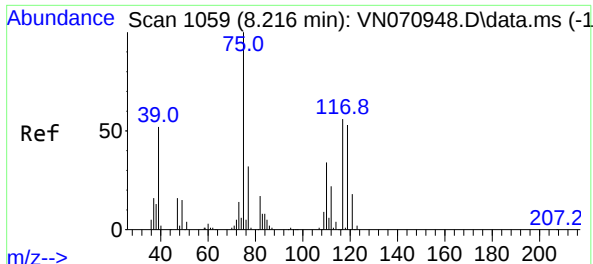

#36

1,1-Dichloropropene

Concen: 4.823 ug/l

RT: 8.081 min Scan# 1

Delta R.T. -0.135 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24

Instrument :

MSVOA_N

ClientSampleId :

MW-40





Tgt Ion: 75 Resp: 68865

Ion Ratio Lower Upper

75 100

110 9.1 18.4 55.2#

77 0.0 24.4 36.6#

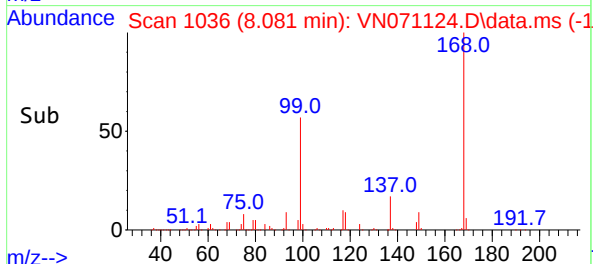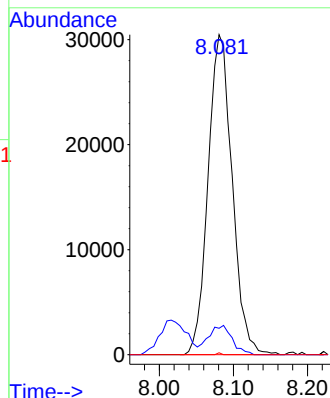

#37

Ethyl Acetate

Concen: 0.266 ug/l

RT: 7.340 min Scan# 910

Delta R.T. -0.065 min

Lab File: VN071124.D

Acq: 01 Mar 2022 17:24




Tgt Ion: 43 Resp: 4074


Ion Ratio Lower Upper

43 100

61 0.0 11.5 17.3#

70 0.0 7.9 11.9#


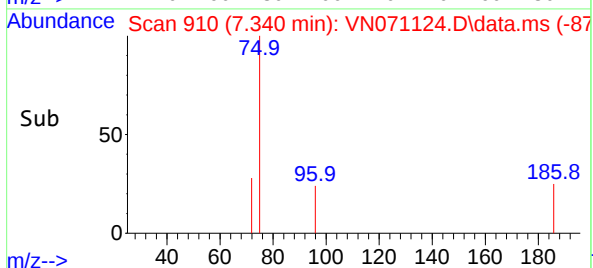
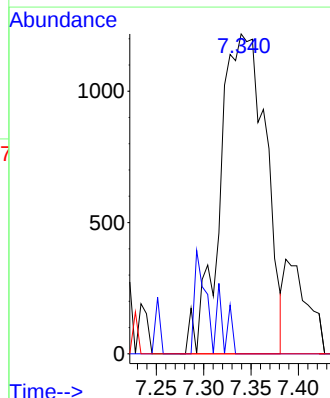
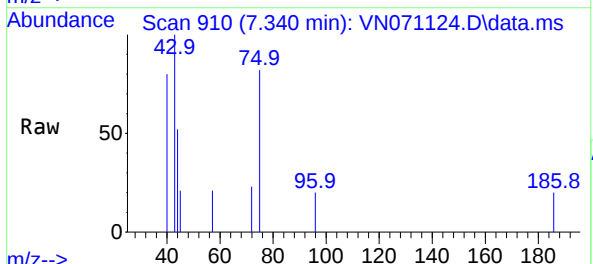




#38
Carbon Tetrachloride
Concen: 6.393 ug/l
RT: 8.081 min Scan# 11
Delta R.T. -0.117 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 89942
Ion Ratio Lower Upper
117 100
119 4.5 76.1 114.1#
121 0.0 24.2 36.2#

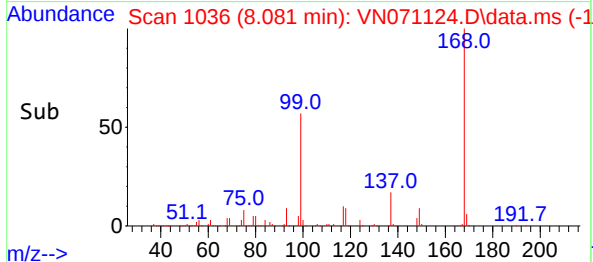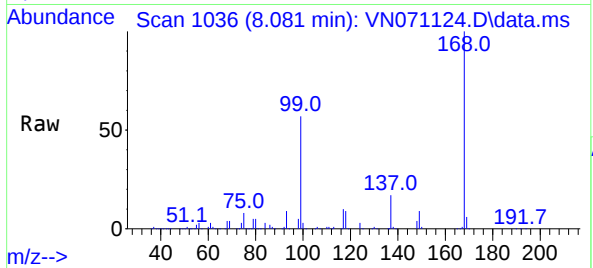

#39
Methylcyclohexane
Concen: 0.311 ug/l
RT: 9.457 min Scan# 1270
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 83 Resp: 5706
Ion Ratio Lower Upper
83 100
55 74.7 58.1 87.1
98 38.3 38.4 57.6#


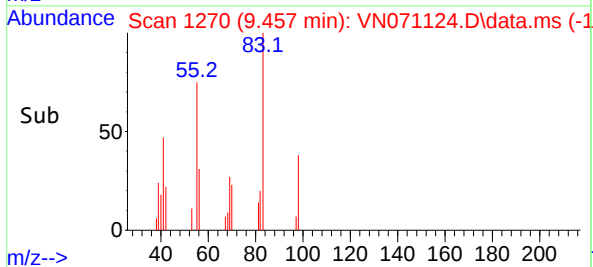

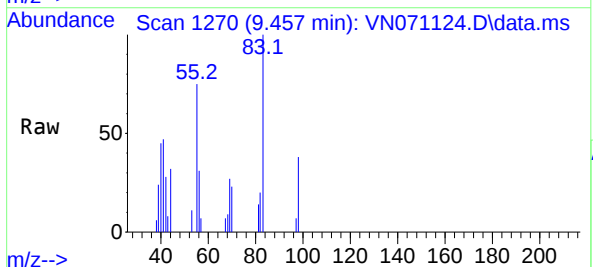




#40
Benzene
Concen: 51.725 ug/l
RT: 8.457 min Scan# 1100
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 78 Resp: 2184830
Ion Ratio Lower Upper
78 100
77 23.6 18.6 27.8

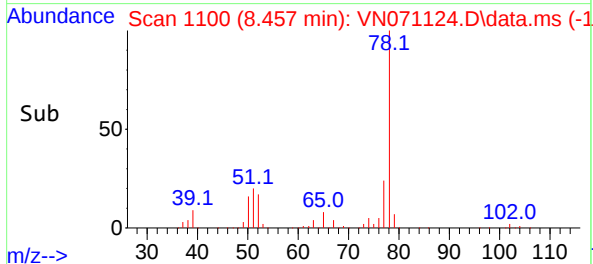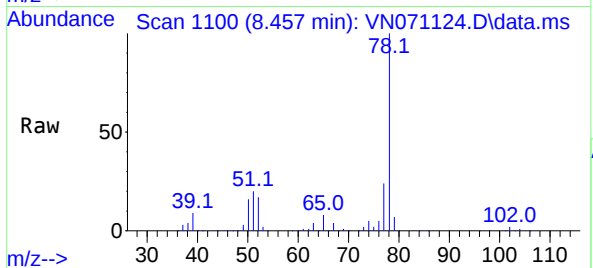

#43
Isopropyl Acetate
Concen: 0.697 ug/l
RT: 8.528 min Scan# 1112
Delta R.T. -0.029 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 43 Resp: 16837
Ion Ratio Lower Upper
43 100
61 0.0 20.4 30.6#
87 0.0 11.2 16.8#


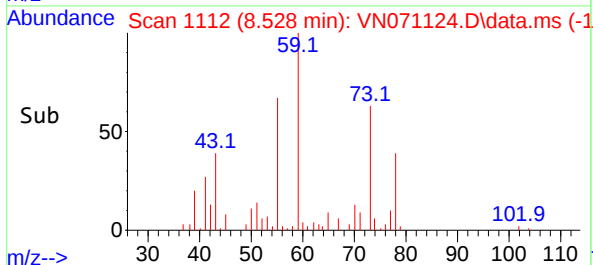

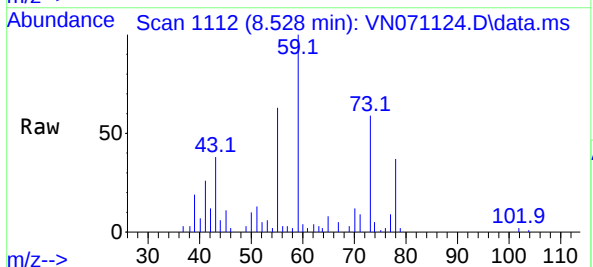




#50
Toluene-d8
Concen: 50.767 ug/l
RT: 10.439 min Scan# 1436
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 98 Resp: 1776969
Ion Ratio Lower Upper
98 100
100 66.1 50.4 75.6



#51
4-Methyl-2-Pentanone
Concen: 0.245 ug/l
RT: 10.328 min Scan# 1418
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 43 Resp: 3601
Ion Ratio Lower Upper
43 100
58 33.2 30.4 45.6


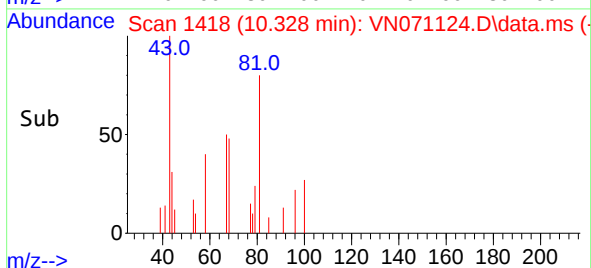






#52
Toluene
Concen: 0.314 ug/l
RT: 10.504 min Scan# 1447
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 92 Resp: 8346
Ion Ratio Lower Upper
92 100
91 157.6 142.0 213.0

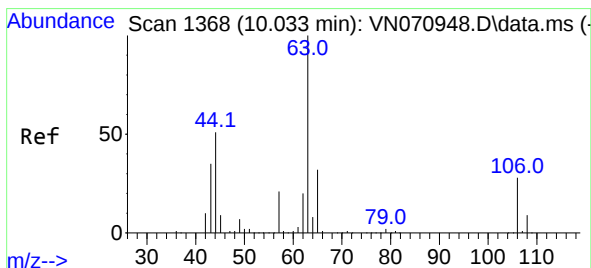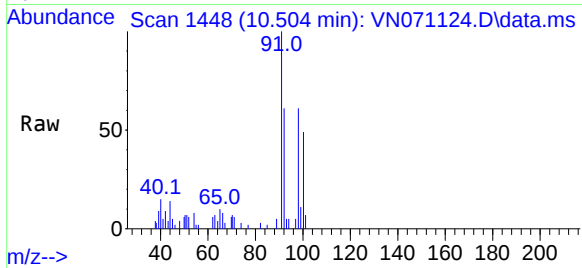

#58
2-Chloroethyl Vinyl ether
Concen: 31.853 ug/l
RT: 10.192 min Scan# 1395
Delta R.T. 0.159 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 63 Resp: 206
Ion Ratio Lower Upper
63 100
106 0.0 23.9 35.9#


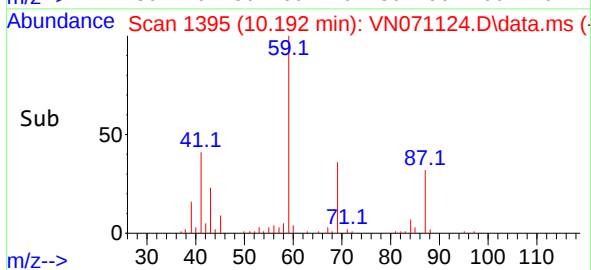

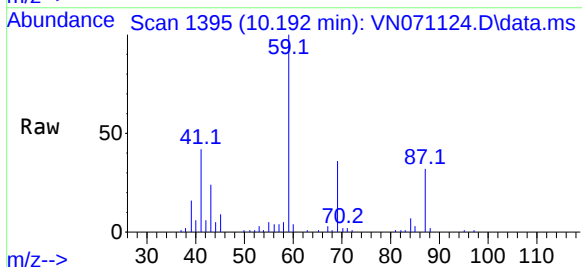




#59
2-Hexanone
Concen: 1.197 ug/l
RT: 11.122 min Scan# 11
Delta R.T. 0.042 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 43 Resp: 12095
Ion Ratio Lower Upper
43 100
58 80.1 26.9 80.7

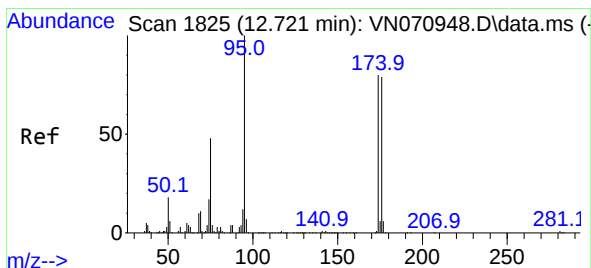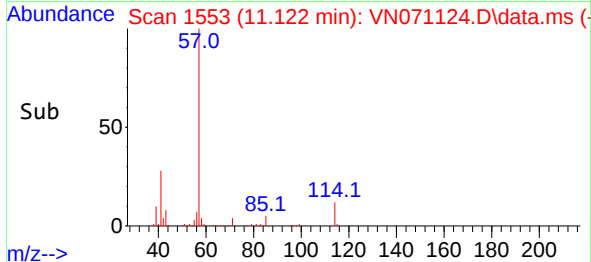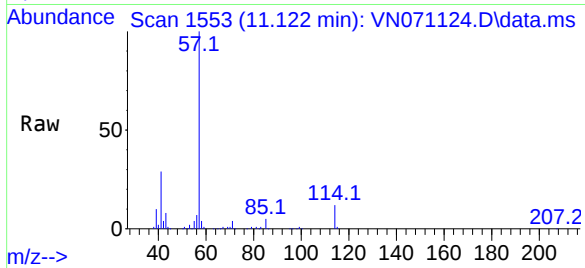

#62
4-Bromofluorobenzene
Concen: 49.366 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 95 Resp: 617638
Ion Ratio Lower Upper
95 100
174 80.0 0.0 187.2
176 76.5 0.0 181.4


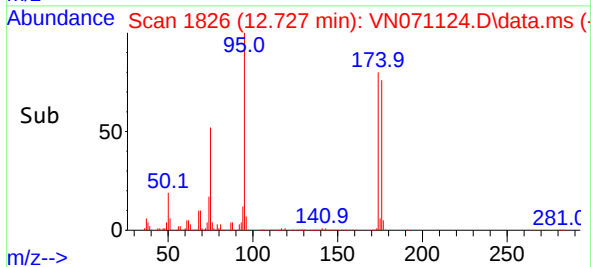

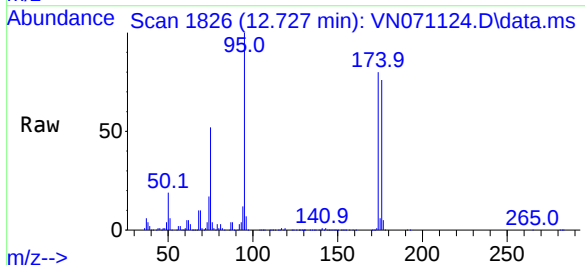




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.739 min Scan# 1658
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 1317124
Ion Ratio Lower Upper
117 100
82 57.1 42.4 63.6
119 31.6 25.4 38.2

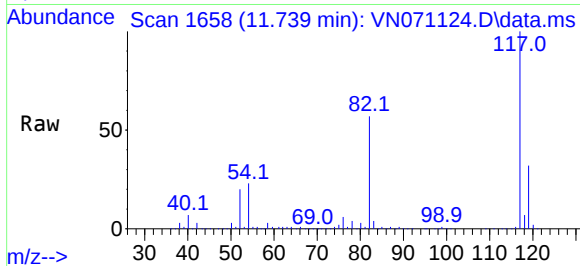

#67
Ethyl Benzene
Concen: 0.397 ug/l
RT: 11.839 min Scan# 1675
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 91 Resp: 19737
Ion Ratio Lower Upper
91 100
106 32.9 25.7 38.5


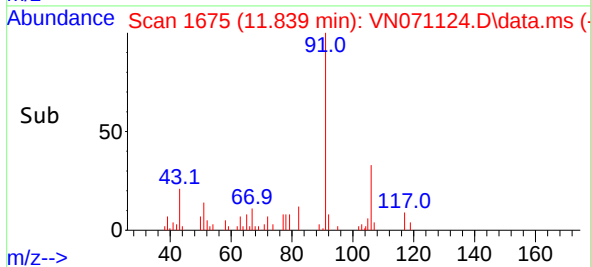

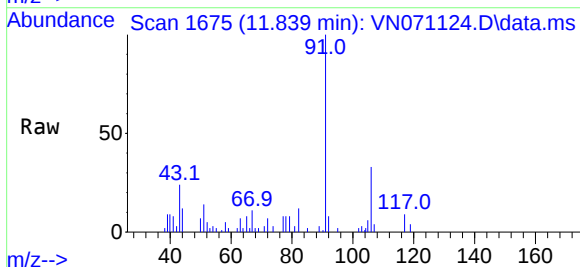




#68
m/p-Xylenes
Concen: 0.437 ug/l
RT: 11.951 min Scan# 1694
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:106 Resp: 8391
Ion Ratio Lower Upper
106 100
91 216.7 160.6 240.8

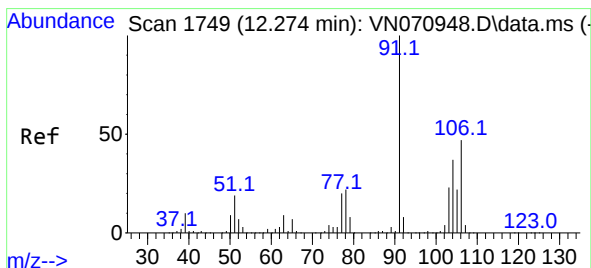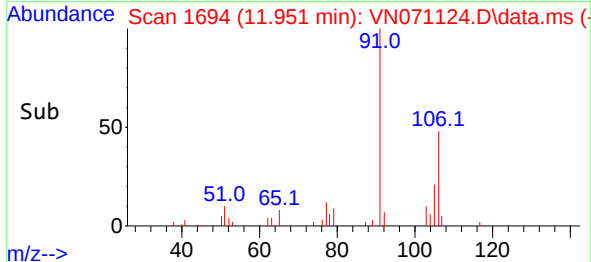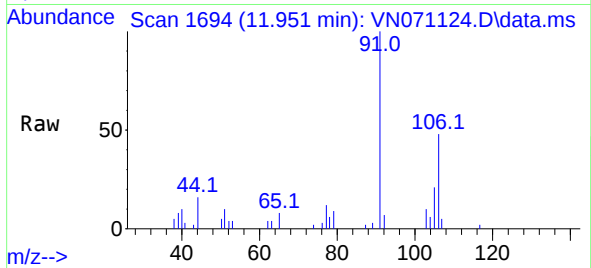

#69
o-Xylene
Concen: 0.503 ug/l
RT: 12.275 min Scan# 1749
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24


Tgt Ion:106 Resp: 9427
Ion Ratio Lower Upper
106 100
91 225.1 105.8 317.3

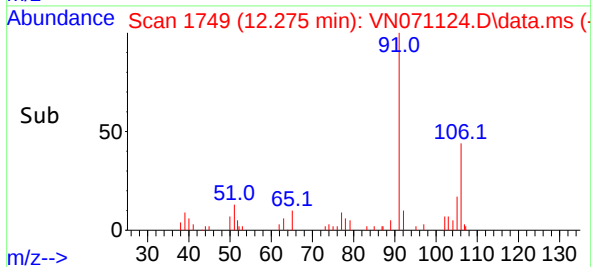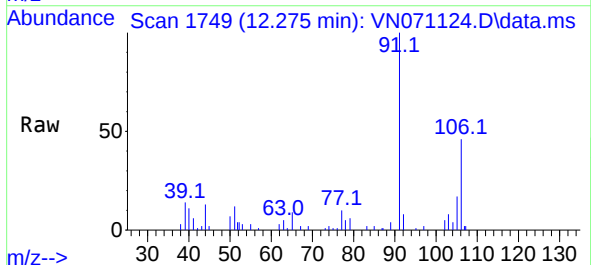






#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.669 min Scan# 1986
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24


Instrument :
MSVOA_N
ClientSampleId :
MW-40





Tgt Ion:152 Resp: 467999
Ion Ratio Lower Upper
152 100
115 58.5 27.5 82.5
150 156.3 0.0 344.4




#73
Isopropylbenzene
Concen: 0.529 ug/l
RT: 12.575 min Scan# 1800
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24



Tgt Ion:105 Resp: 19938
Ion Ratio Lower Upper
105 100
120 25.8 13.4 40.1



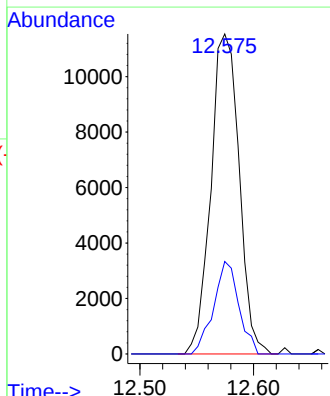





#76
1,2,3-Trichloropropane
Concen: 28.588 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. -0.141 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 315020
Ion Ratio Lower Upper
75 100
77 1.3 82.6 247.8#

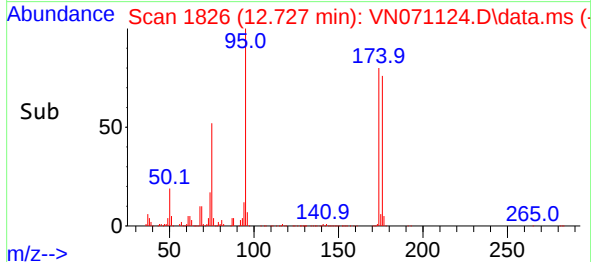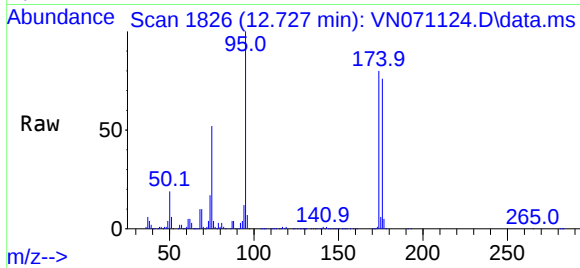

#80
1,3,5-Trimethylbenzene
Concen: 0.255 ug/l
RT: 13.057 min Scan# 1882
Delta R.T. 0.006 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 105 Resp: 7797
Ion Ratio Lower Upper
105 100
120 55.4 24.6 73.6


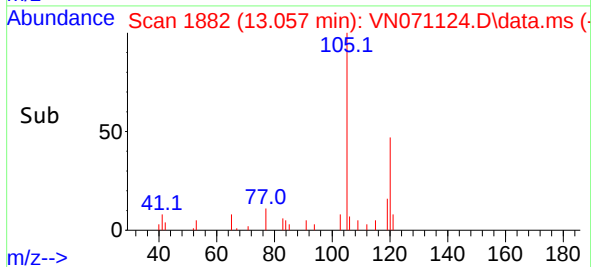

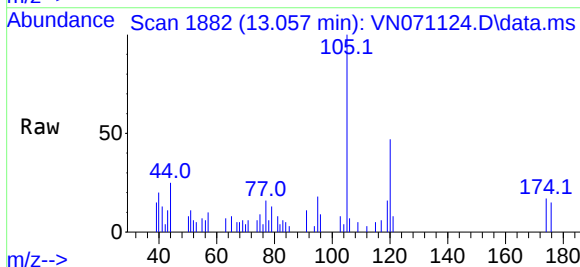




#81
trans-1,4-Dichloro-2-butene
Concen: 92.640 ug/l
RT: 12.727 min Scan# 1826
Delta R.T. 0.106 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion: 75 Resp: 315020
Ion Ratio Lower Upper
75 100
53 0.1 90.5 135.7#
89 0.0 38.2 57.4#

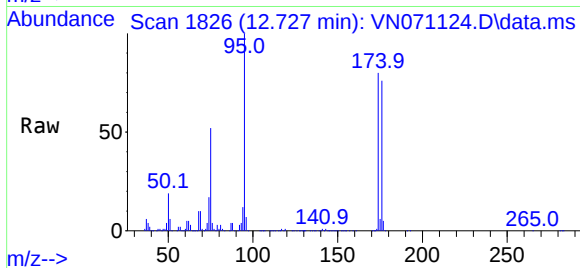

#84
1,2,4-Trimethylbenzene
Concen: 0.554 ug/l
RT: 13.363 min Scan# 1934
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion: 105 Resp: 16648
Ion Ratio Lower Upper
105 100
120 52.1 22.8 68.4


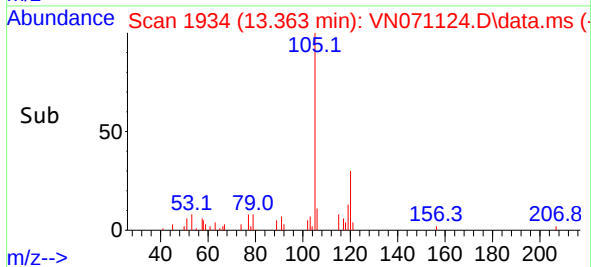

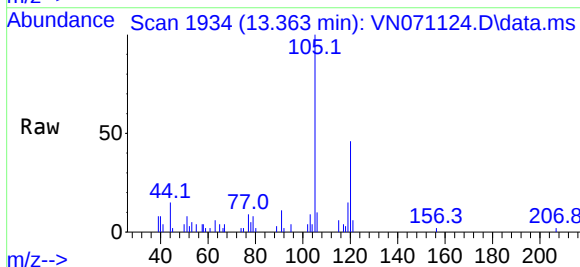




#90
Hexachloroethane
Concen: 0.330 ug/l
RT: 14.274 min Scan# 2077
Delta R.T. 0.071 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24




Instrument :
MSVOA_N
ClientSampleId :
MW-40


Tgt Ion:117 Resp: 1847
Ion Ratio Lower Upper
117 100
201 0.0 43.9 131.6#

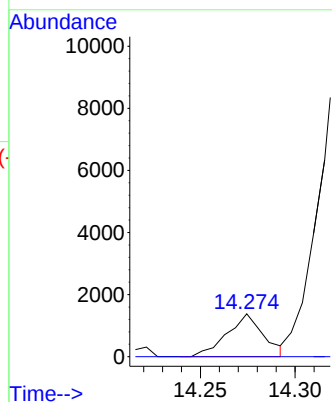

#93
1,2,4-Trichlorobenzene
Concen: 2.092 ug/l
RT: 15.269 min Scan# 2258
Delta R.T. 0.011 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion:180 Resp: 838
Ion Ratio Lower Upper
180 100
182 91.6 48.3 144.9
145 173.6 14.5 43.5#


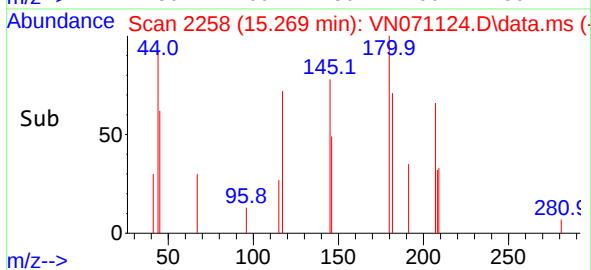






#95
Naphthalene
Concen: 5.880 ug/l
RT: 15.510 min Scan# 2297
Delta R.T. 0.012 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Instrument :
MSVOA_N
ClientSampleId :
MW-40

Tgt Ion:	128	Resp:	20694
Ion	Ratio	Lower	Upper
128	100		
127	13.7	10.5	15.7
129	9.9	8.7	13.1



#96
1,2,3-Trichlorobenzene
Concen: 2.614 ug/l
RT: 15.692 min Scan# 2330
Delta R.T. 0.000 min
Lab File: VN071124.D
Acq: 01 Mar 2022 17:24

Tgt Ion:	180	Resp:	823
Ion	Ratio	Lower	Upper
180	100		
182	55.3	47.4	142.2
145	64.9	15.0	45.1#

