

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030124\
 Data File : VN081275.D
 Acq On : 01 Mar 2024 10:50
 Operator : JC\MD
 Sample : VN0301WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0301WBL01

Quant Time: Mar 01 22:13:17 2024
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Quant Title : SW846 8260
 QLast Update : Fri Feb 16 23:45:20 2024
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	8.224	168	260547	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	495561	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	420264	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.794	152	167057	50.000	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	173028	54.180	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	=	108.360%
35) Dibromofluoromethane	8.165	113	145813	52.034	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	=	104.060%
50) Toluene-d8	10.565	98	440197	44.228	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	=	88.460%
62) 4-Bromofluorobenzene	12.853	95	152317	40.729	ug/l	0.00
Spiked Amount	50.000	Range	83 - 123	Recovery	=	81.460%#


Target Compounds	Qvalue


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030124\
Data File : VN081275.D
Acq On : 01 Mar 2024 10:50
Operator : JC\MD
Sample : VN0301WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0301WBL01

Quant Time: Mar 01 22:13:17 2024
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Quant Title : SW846 8260
QLast Update : Fri Feb 16 23:45:20 2024
Response via : Initial Calibration




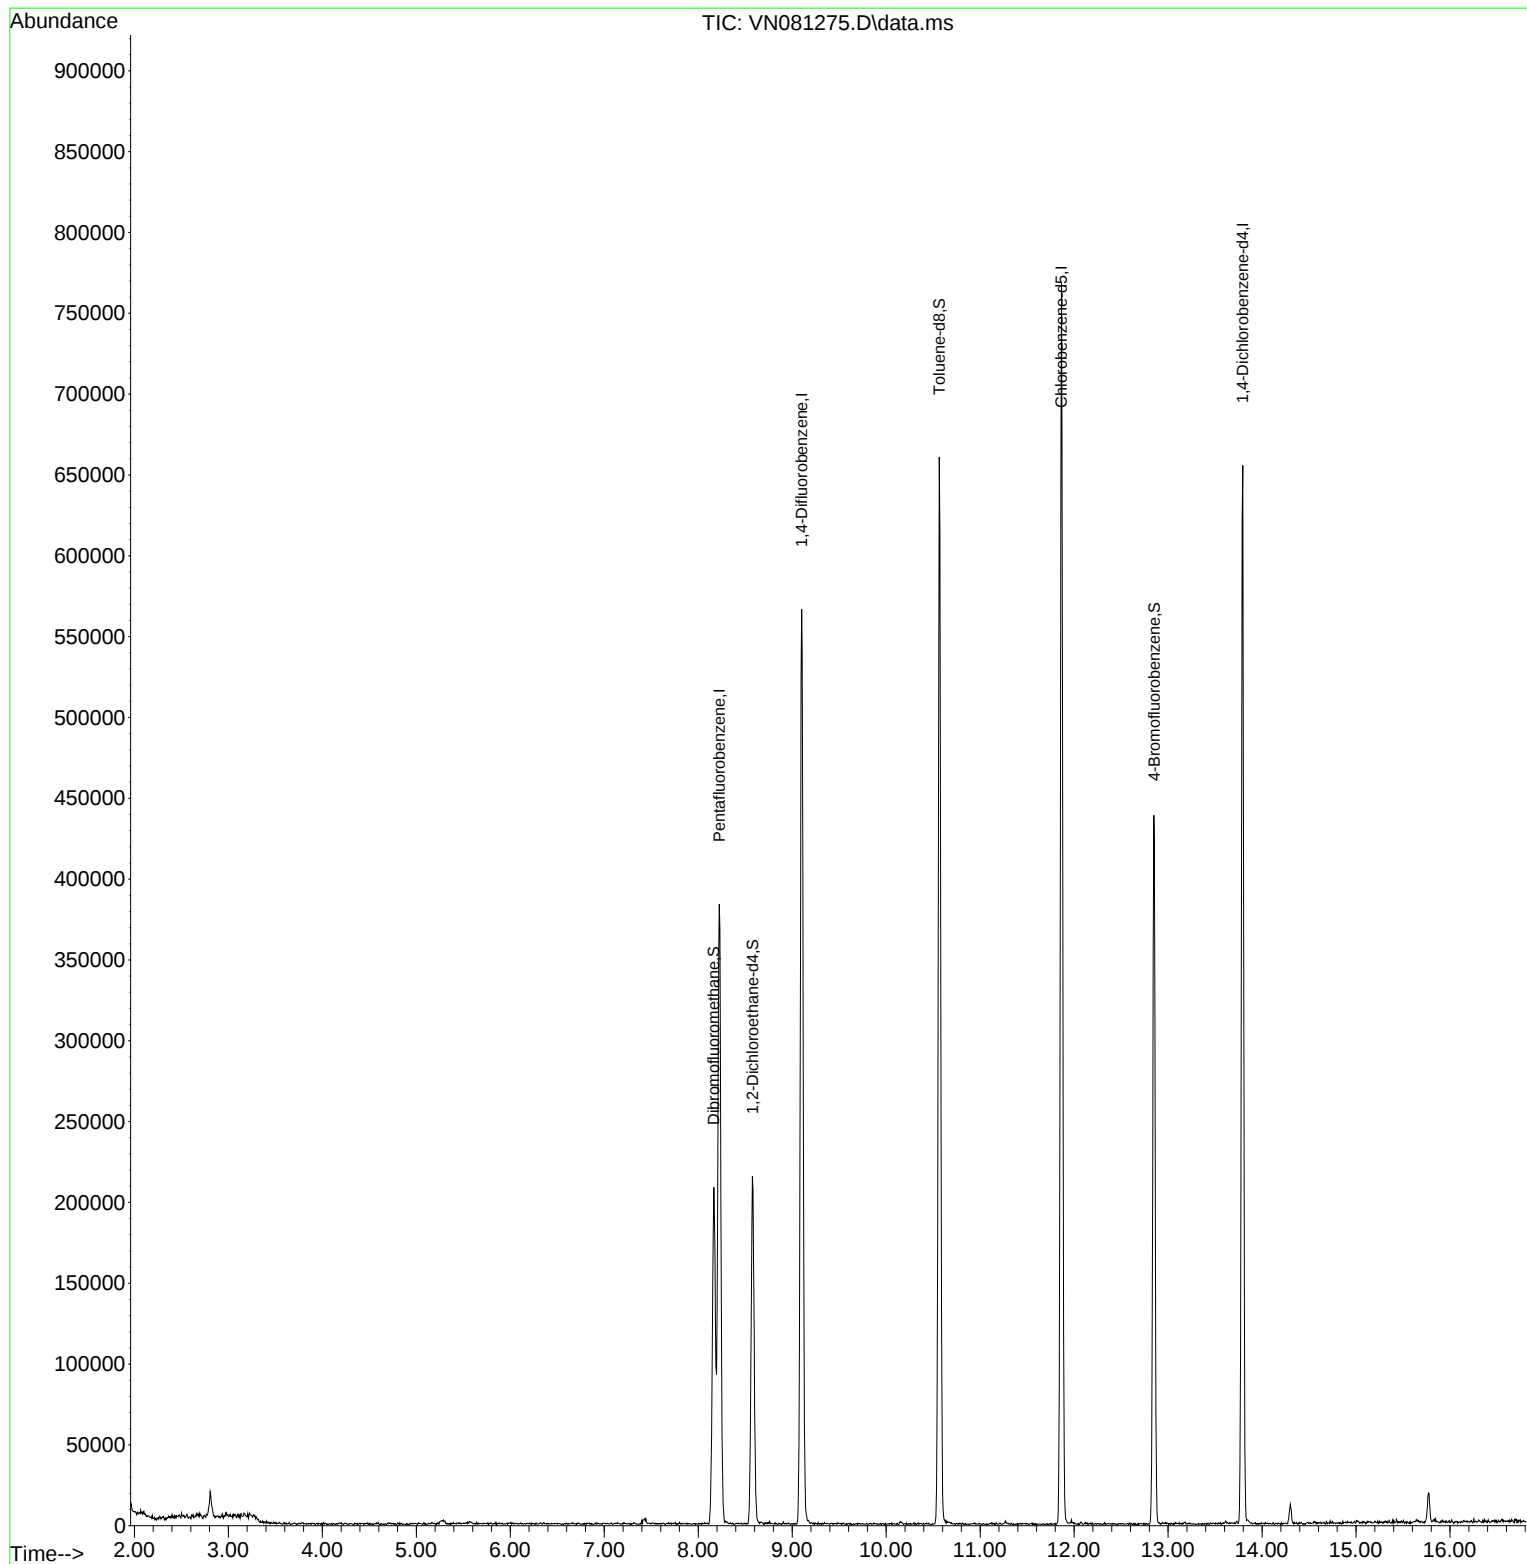


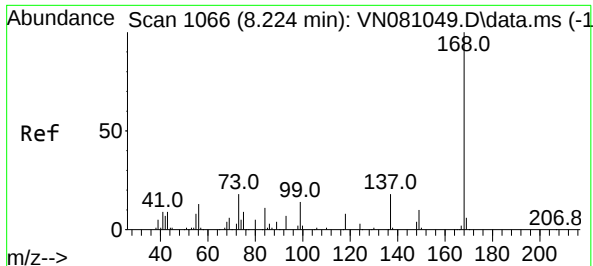

#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.000 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50




Instrument :
MSVOA_N
ClientSampleId :
VN0301WBL01


Tgt Ion:168 Resp: 260547
Ion Ratio Lower Upper
168 100
99 66.1 59.9 89.9

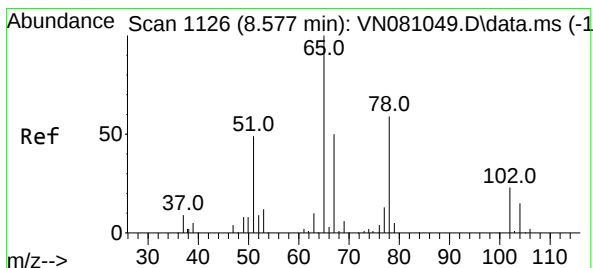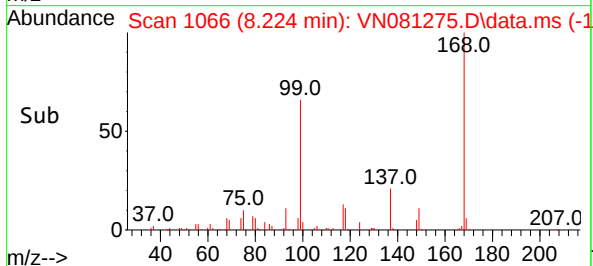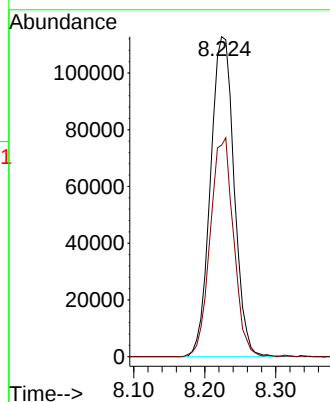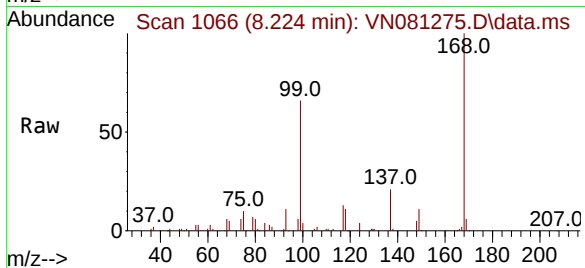

#33
1,2-Dichloroethane-d4
Concen: 54.180 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.000 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50

Tgt Ion: 65 Resp: 173028
Ion Ratio Lower Upper
65 100
67 51.0 0.0 102.4

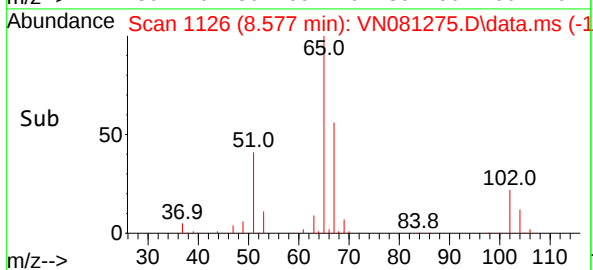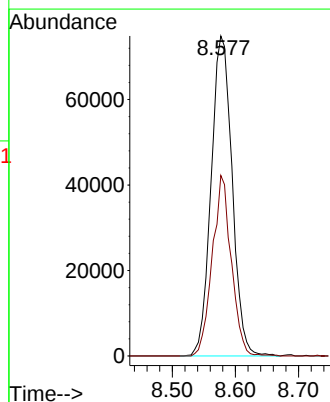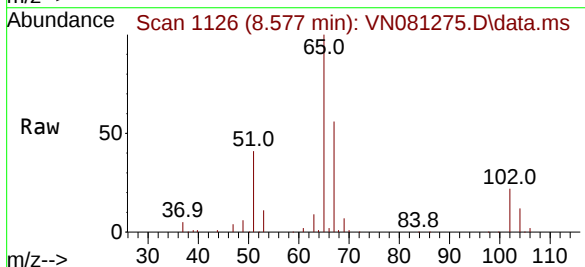

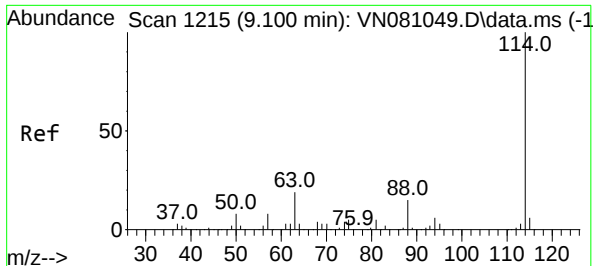

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.000 min

Lab File: VN081275.D

Acq: 01 Mar 2024 10:50

Instrument :

MSVOA_N

ClientSampleId :

VN0301WBL01





Tgt Ion:114 Resp: 495561

Ion Ratio Lower Upper

114 100

63 21.1 0.0 48.0

88 15.3 0.0 34.8

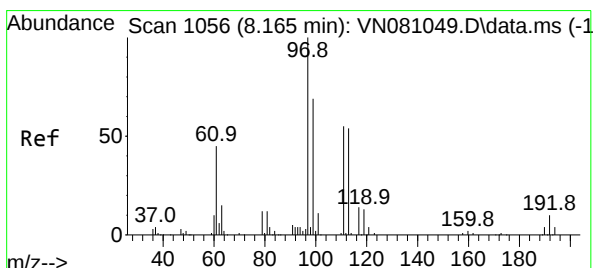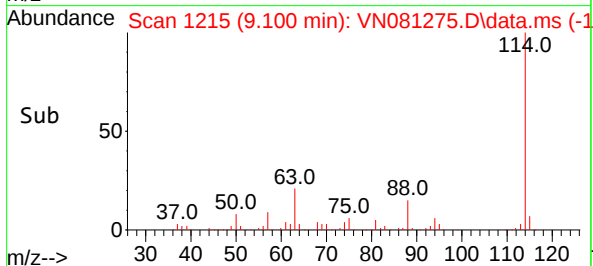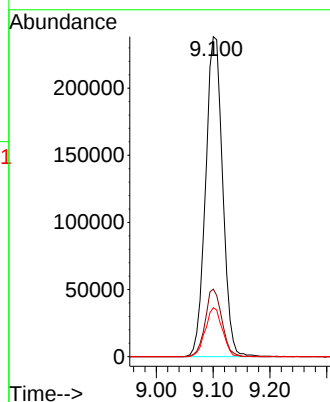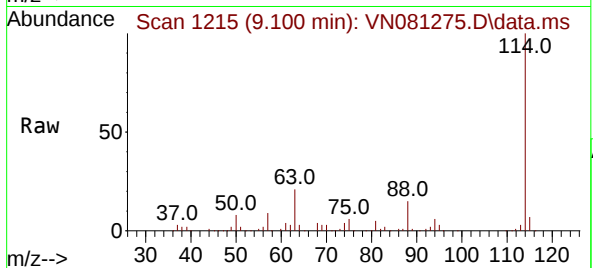

#35

Dibromofluoromethane

Concen: 52.034 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.000 min

Lab File: VN081275.D

Acq: 01 Mar 2024 10:50




Tgt Ion:113 Resp: 145813


Ion Ratio Lower Upper

113 100

111 103.4 82.2 123.4

192 15.1 12.5 18.7


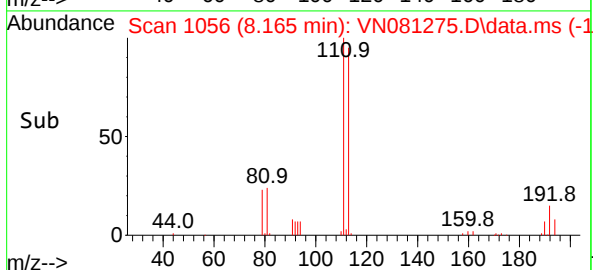
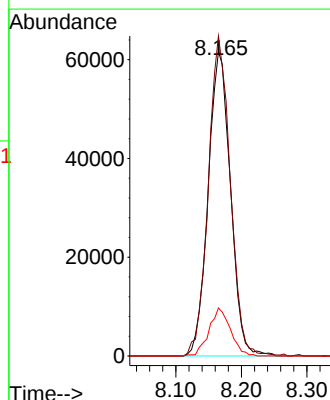
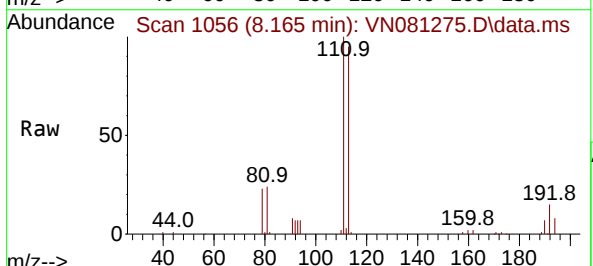


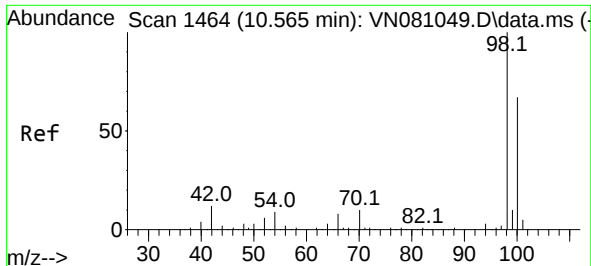

#50
Toluene-d8
Concen: 44.228 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.000 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50




Instrument :
MSVOA_N
ClientSampleId :
VN0301WBL01


Tgt Ion: 98 Resp: 440197
Ion Ratio Lower Upper
98 100
100 64.8 51.4 77.0

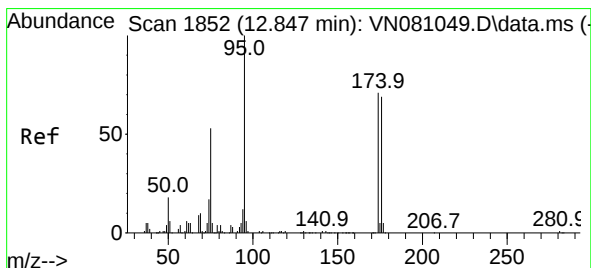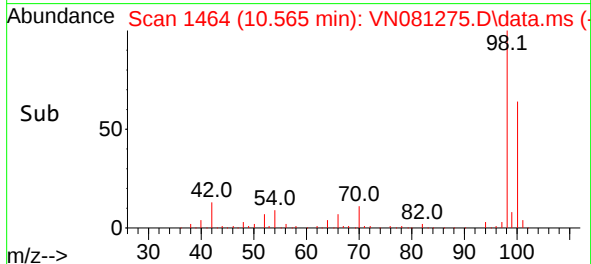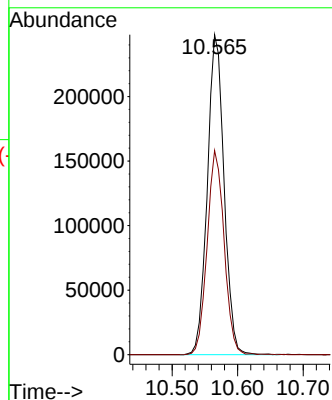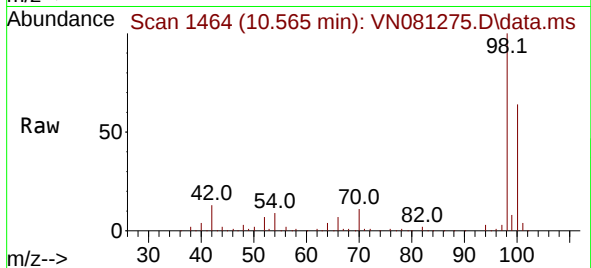

#62
4-Bromofluorobenzene
Concen: 40.729 ug/l
RT: 12.853 min Scan# 1853
Delta R.T. 0.006 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50

Tgt Ion: 95 Resp: 152317
Ion Ratio Lower Upper
95 100
174 69.7 0.0 120.4
176 68.1 0.0 121.0


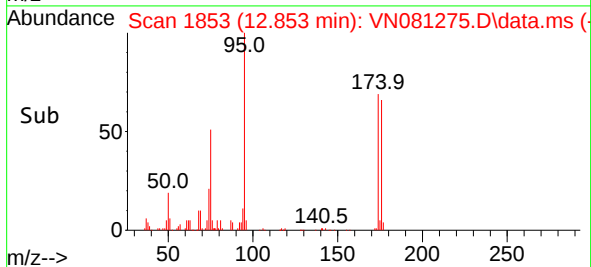
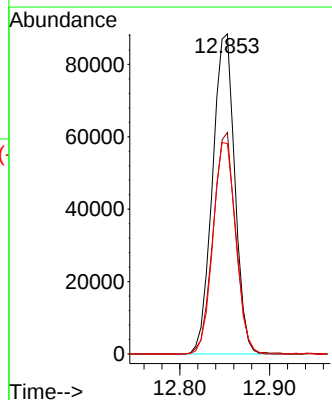
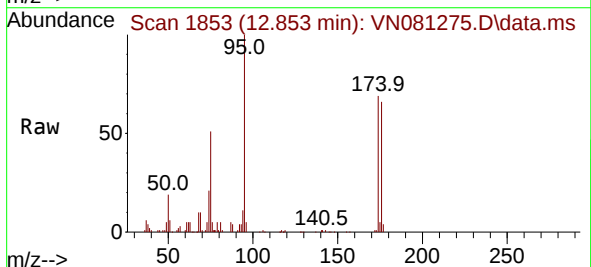


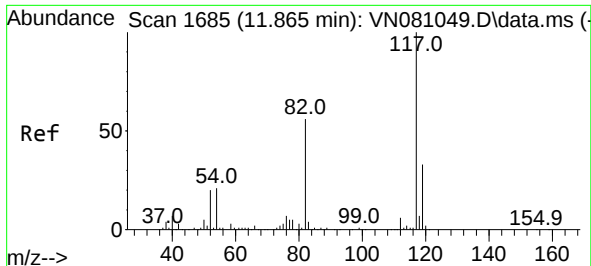

#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.000 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50

Instrument :
MSVOA_N
ClientSampleId :
VN0301WBL01

Tgt Ion:117 Resp: 420264
Ion Ratio Lower Upper
117 100
82 57.9 52.7 79.1
119 32.3 25.3 37.9

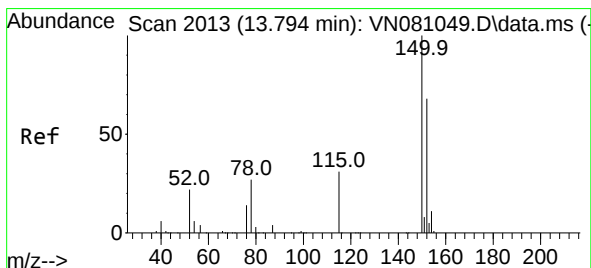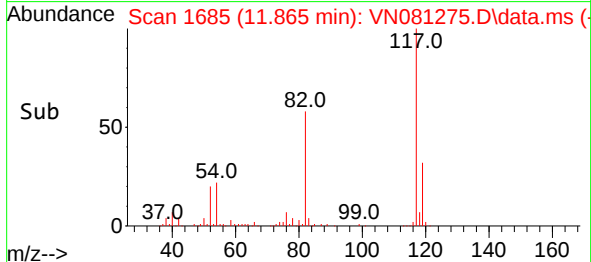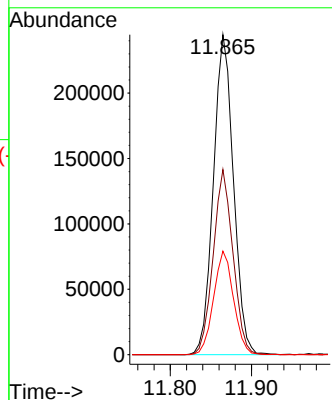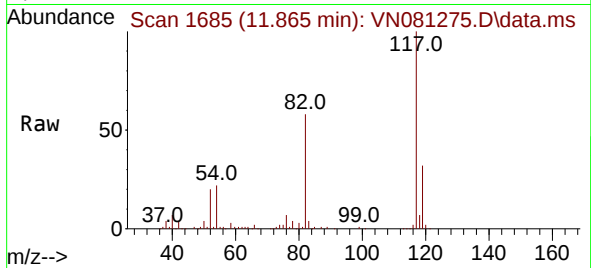

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.794 min Scan# 2013
Delta R.T. 0.000 min
Lab File: VN081275.D
Acq: 01 Mar 2024 10:50

Tgt Ion:152 Resp: 167057
Ion Ratio Lower Upper
152 100
115 63.0 32.3 96.8
150 159.1 0.0 339.8

