
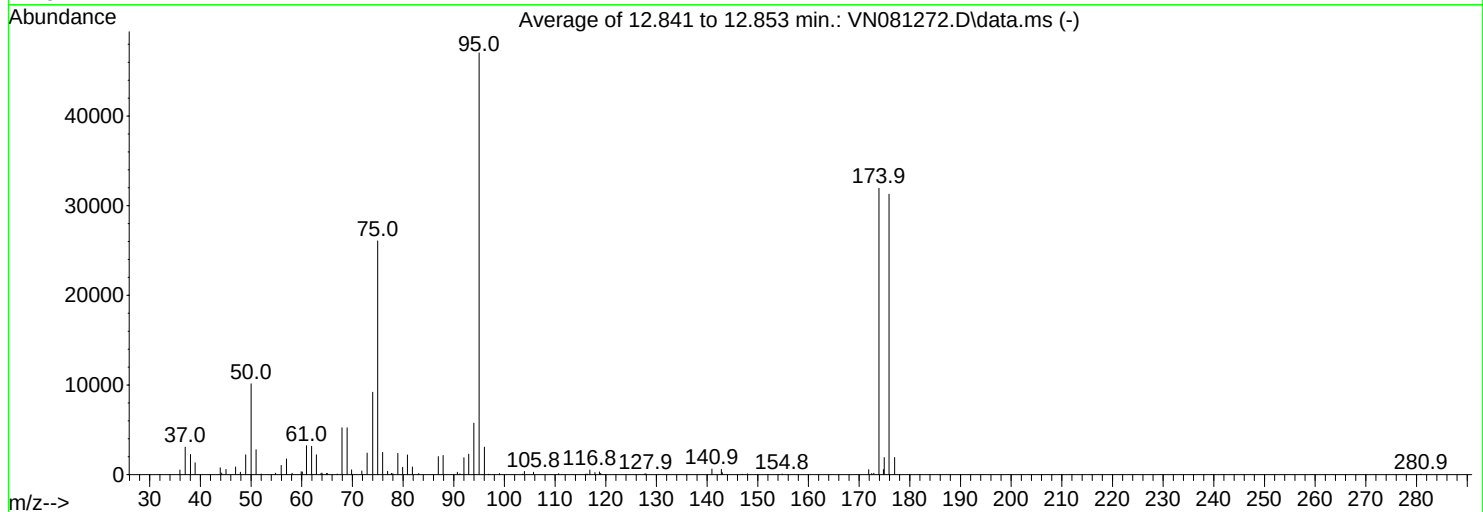


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030124\
Data File : VN081272.D
Acq On : 01 Mar 2024 09:06
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
Title : SW846 8260
Last Update : Fri Feb 16 23:45:20 2024

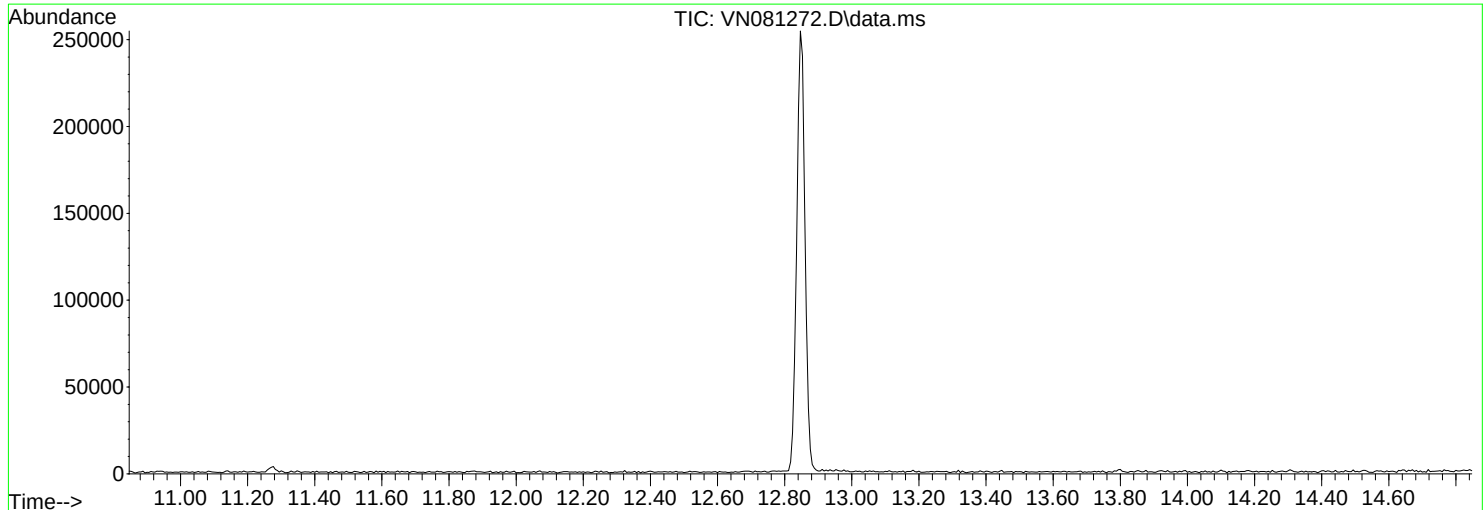

AutoFind: Scans 1851, 1852, 1853; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.6	10145	PASS
75	95	30	60	55.4	26080	PASS
95	95	100	100	100.0	47048	PASS
96	95	5	9	6.5	3066	PASS
173	174	0.00	2	0.5	171	PASS
174	95	50	100	67.9	31939	PASS
175	174	5	9	6.0	1918	PASS
176	174	95	101	98.0	31291	PASS
177	176	5	9	6.1	1905	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	516	51.00	2776	63.80	153	75.00	2608
37.00	3067	52.00	73	64.00	187	75.95	248
38.05	2256	54.85	154	64.90	147	76.95	38
38.95	1314	55.95	1034	65.10	123	77.70	15
43.90	772	57.00	1753	67.00	69	78.00	101
44.20	182	58.10	171	67.95	5239	78.95	2369
45.05	598	59.90	314	68.95	5231	79.90	820
46.95	858	60.10	313	69.85	542	80.85	2200
47.90	260	60.95	3227	71.85	410	81.85	863
48.95	2210	61.95	3154	72.90	2405	83.10	127
50.00	10145	62.90	2222	74.00	9201	86.95	2011

Average of 12.841 to 12.853 min.: VN081272.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
87.90	2145	103.95	365	140.95	628	174.95	1918
90.70	275	105.75	277	142.80	592	175.90	31291
91.20	97	110.70	104	143.00	219	177.00	1905
92.00	1901	116.10	74	146.90	62	280.90	58
92.95	2286	116.40	55	148.00	92		
93.95	5753	116.85	510	154.80	77		
95.00	47048	117.85	224	171.90	550		
96.05	3066	118.75	305	172.50	133		
96.90	58	119.00	141	172.90	171		
99.00	134	127.70	69	173.90	31939		
103.60	62	127.90	107	174.80	570		

Instrument :

MSVOA_N

ClientSampleId :

BFB