

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030219\
 Data File : VN054040.D
 Acq On : 1 Mar 2019 20:08
 Operator : JC/SP
 Sample : K1665-04
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 200029

Quant Time: Mar 02 05:38:34 2019
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 28 04:05:45 2019
 Response via : Initial Calibration


Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.67	168	615411	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.59	114	1166276	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.41	117	1130566	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	415171	50.00	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.03	65	416221	57.70	ug/l	0.00
Spiked Amount 50.000			Recovery	=	115.40%	
35) Dibromofluoromethane	7.59	113	374609	49.67	ug/l	0.00
Spiked Amount 50.000			Recovery	=	99.34%	
50) Toluene-d8	10.09	98	1473056	52.47	ug/l	0.00
Spiked Amount 50.000			Recovery	=	104.94%	
62) 4-Bromofluorobenzene	12.40	95	494956	52.92	ug/l	0.00
Spiked Amount 50.000			Recovery	=	105.84%	
Target Compounds						
20) Methylene Chloride	4.55	84	224184	31.399	ug/l	89
43) Isopropyl Acetate	8.17	43	34021	2.602	ug/l #	89
95) Naphthalene	15.13	128	10385	3.803	ug/l	97


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN030219\
Data File : VN054040.D
Acq On : 1 Mar 2019 20:08
Operator : JC/SP
Sample : K1665-04
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
200029

Quant Time: Mar 02 05:38:34 2019
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 28 04:05:45 2019
Response via : Initial Calibration

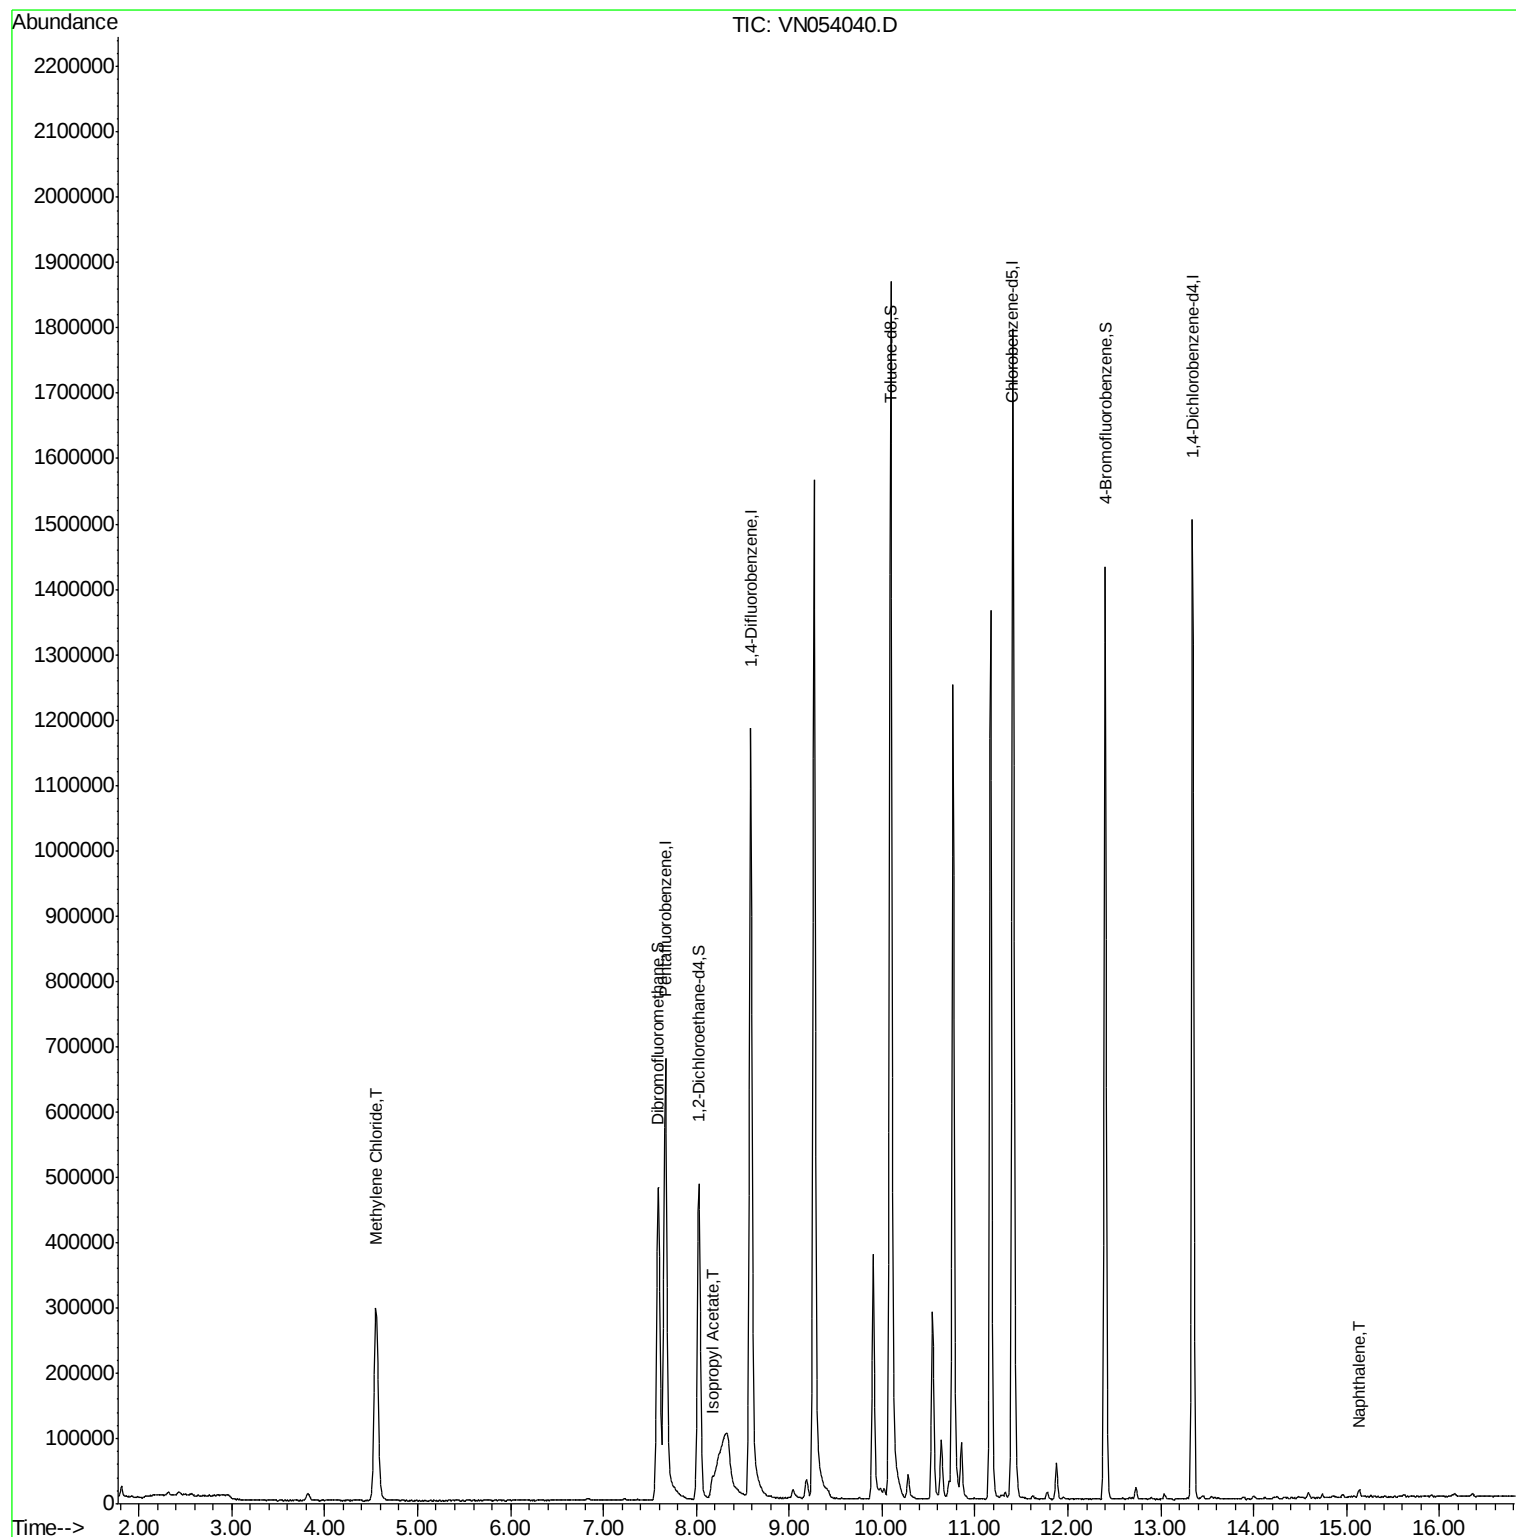

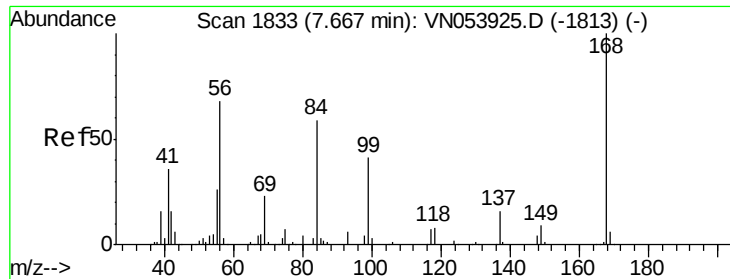

#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.67 min Scan# 1833

Delta R.T. 0.00 min

Lab File: VN054040.D

Acq: 1 Mar 2019 20:08

Instrument :

MSVOA_N

ClientSampleId :


200029

Tot Ion:168 Resp: 615411

Ion Ratio Lower Upper




168 100

99 51.2 36.9 55.3

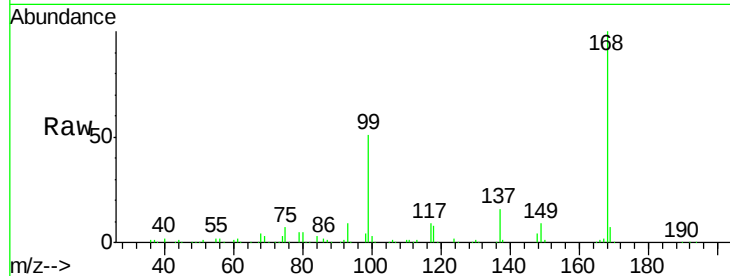

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VNO

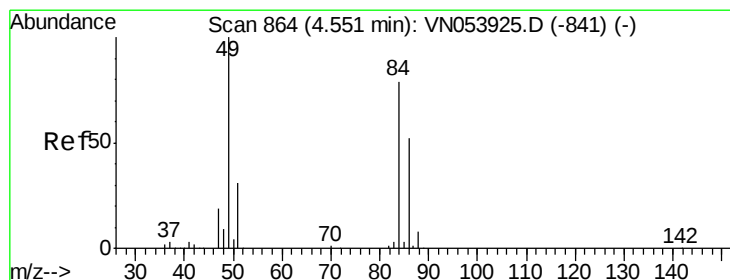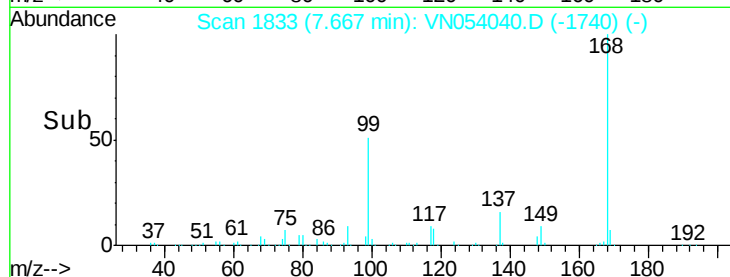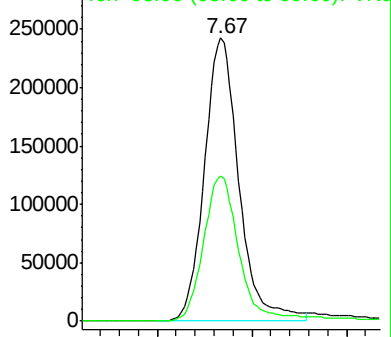

#20

Methylene Chloride

Concen: 31.399 ug/l

RT: 4.55 min Scan# 865

Delta R.T. 0.00 min

Lab File: VN054040.D

Acq: 1 Mar 2019 20:08

Tgt Ion: 84 Resp: 224184


Ion Ratio Lower Upper

84 100

49 130.0 89.7 134.5

51 39.4 27.8 41.8

86 65.2 51.3 76.9


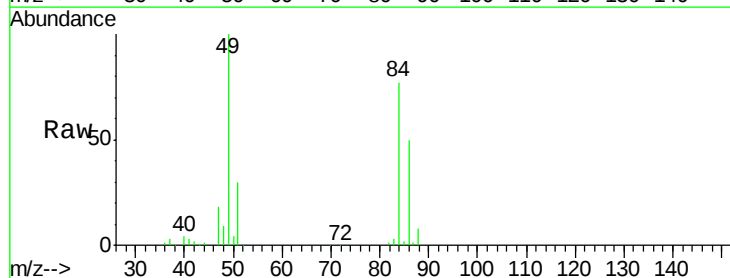



Abundance Ion 83.90 (83.60 to 84.60): VNO

Ion 48.90 (48.60 to 49.60): VNO

Ion 50.90 (50.60 to 51.60): VNO

Ion 85.90 (85.60 to 86.60): VNO



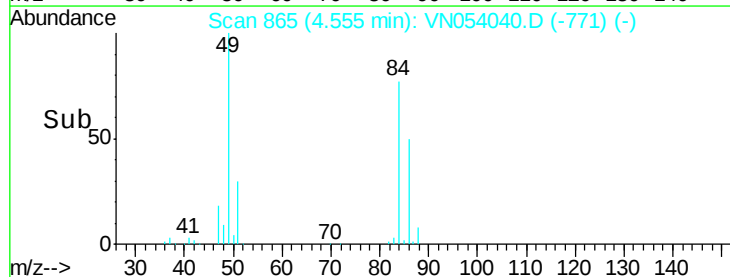
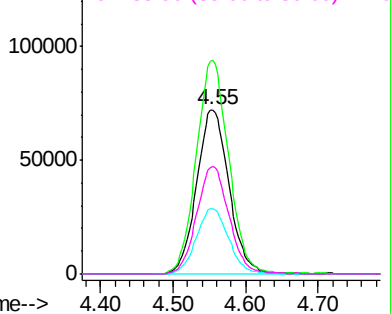


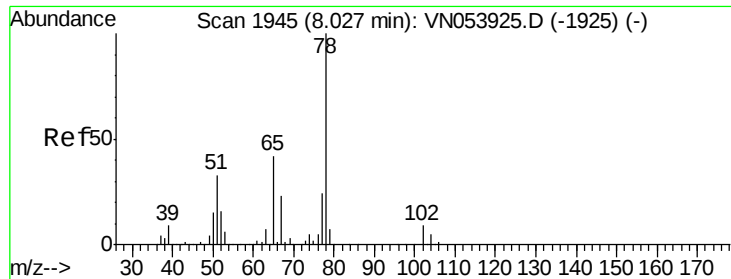

#33
 1,2-Dichloroethane-d4
 Concen: 57.696 ug/l
 RT: 8.03 min Scan# 1945
 Delta R.T. 0.00 min
 Lab File: VN054040.D
 Acq: 1 Mar 2019 20:08




Instrument :
 MSVOA_N
 ClientSampleId :
 200029


Tot Ion: 65 Resp: 416221
 Ion Ratio Lower Upper
 65 100
 67 53.9 0.0 111.8

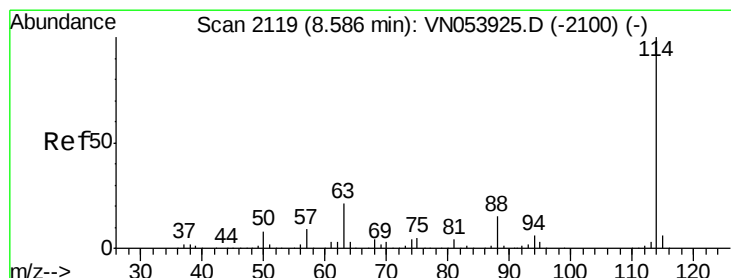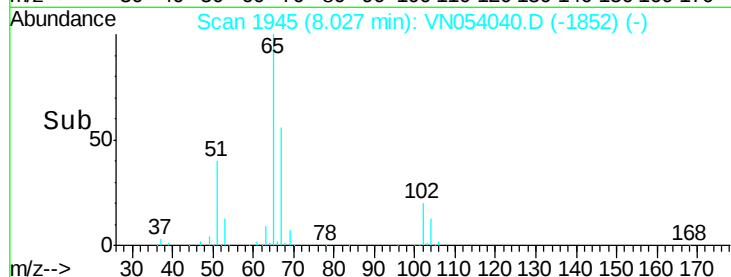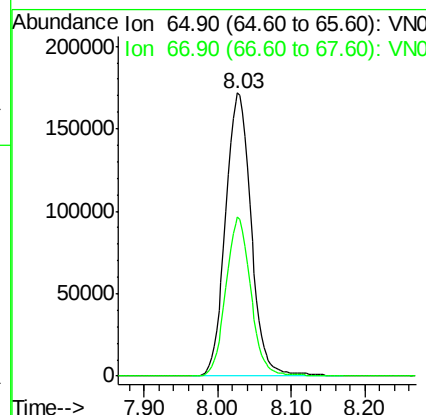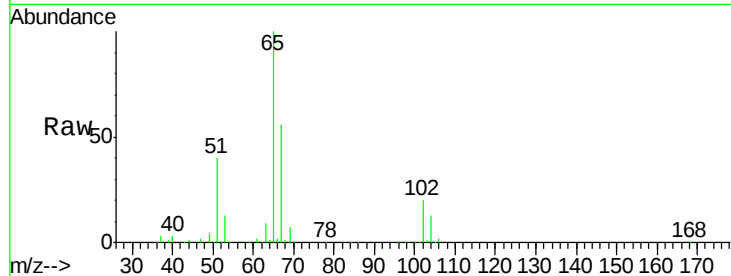

#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.59 min Scan# 2119
 Delta R.T. 0.00 min
 Lab File: VN054040.D
 Acq: 1 Mar 2019 20:08

Tgt Ion: 114 Resp: 1166276
 Ion Ratio Lower Upper
 114 100
 63 21.3 0.0 37.4
 88 16.1 0.0 30.4


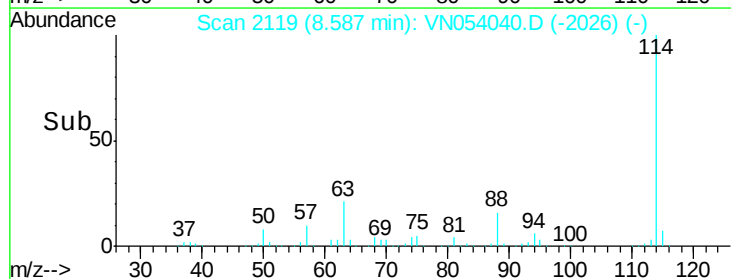
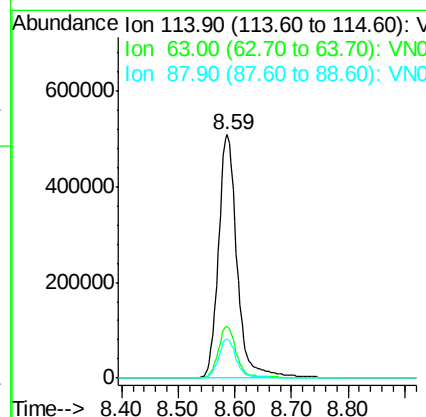
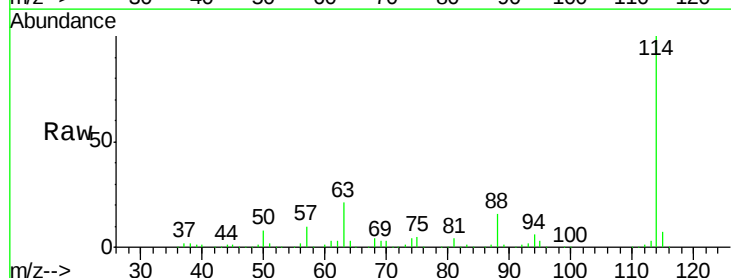


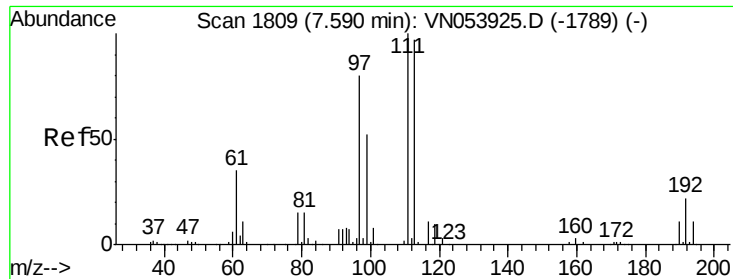

#35
 Dibromofluoromethane
 Concen: 49.671 ug/l
 RT: 7.59 min Scan# 1810
 Delta R.T. 0.00 min
 Lab File: VN054040.D
 Acq: 1 Mar 2019 20:08




Instrument :
 MSVOA_N
 ClientSampled :
 200029


Tot Ion:113 Resp: 374609
 Ion Ratio Lower Upper
 113 100
 111 102.4 81.1 121.7
 192 21.3 18.8 28.2

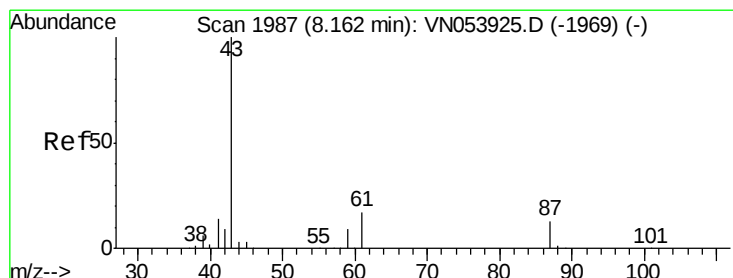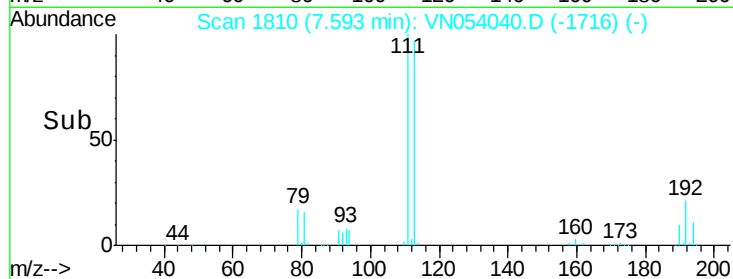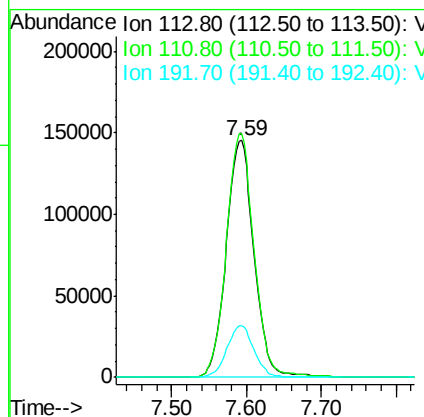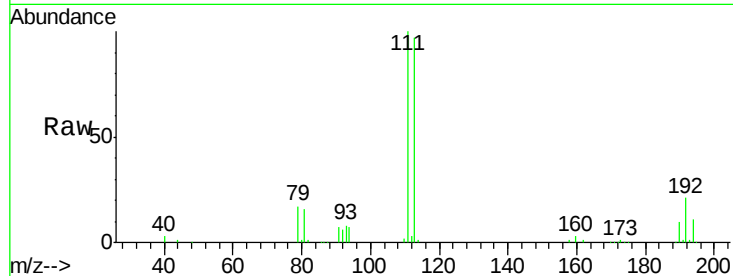

#43
 Isopropyl Acetate
 Concen: 2.602 ug/l
 RT: 8.17 min Scan# 1990
 Delta R.T. 0.01 min
 Lab File: VN054040.D
 Acq: 1 Mar 2019 20:08

Tgt Ion: 43 Resp: 34021
 Ion Ratio Lower Upper
 43 100
 61 15.8 17.4 26.0#
 87 11.1 11.5 17.3#

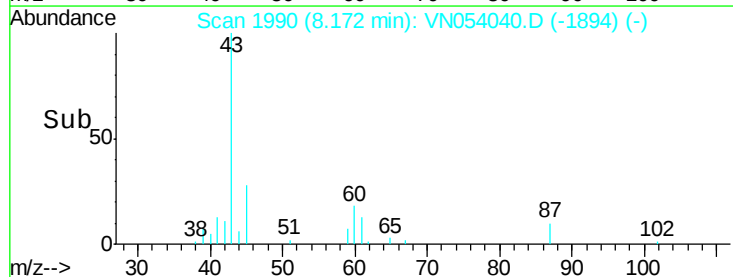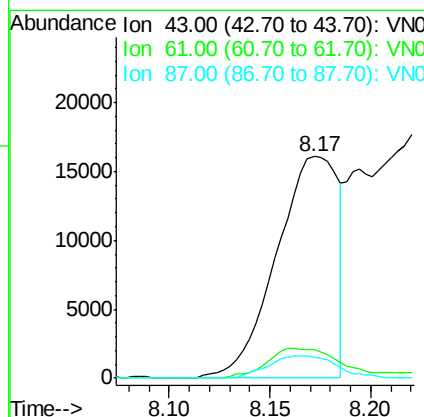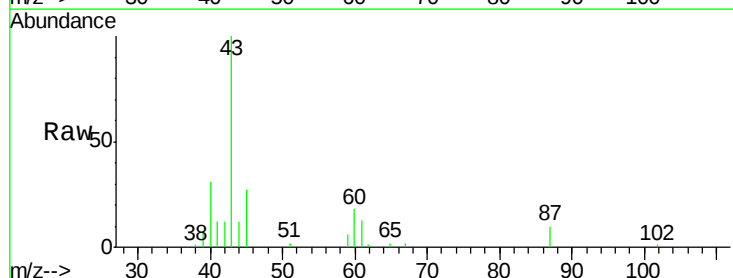

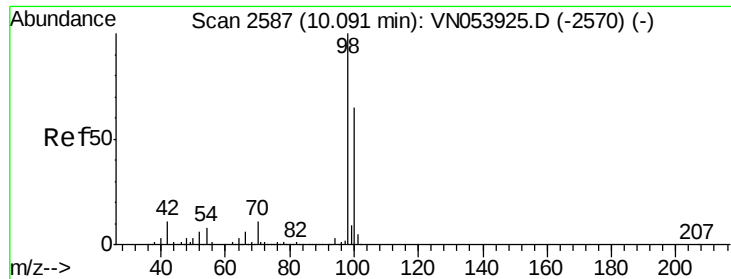

#50

Toluene-d8

Concen: 52.469 ug/l

RT: 10.09 min Scan# 2587

Delta R.T. 0.00 min

Lab File: VN054040.D

Acq: 1 Mar 2019 20:08

Instrument :

MSVOA_N

ClientSampled :





200029

Tot Ion: 98 Resp: 1473056

Ion Ratio Lower Upper

98 100

100 63.9 51.9 77.9

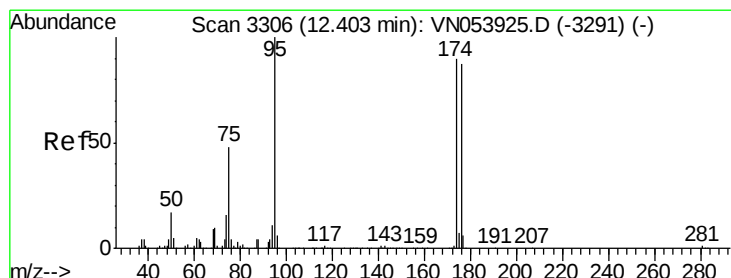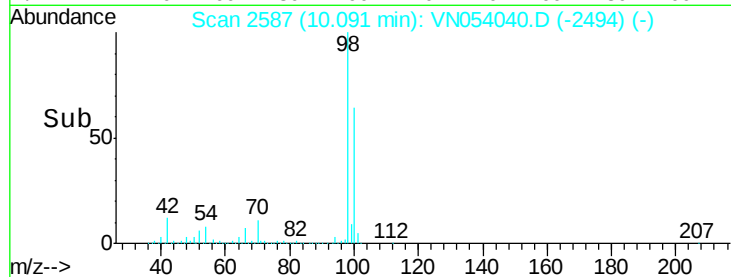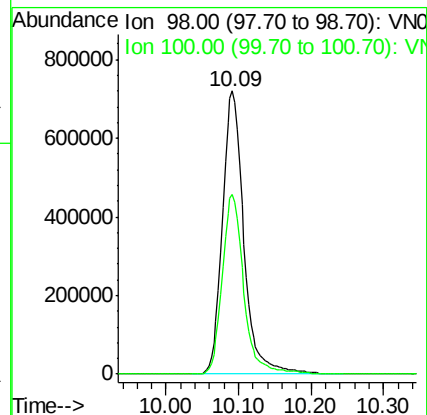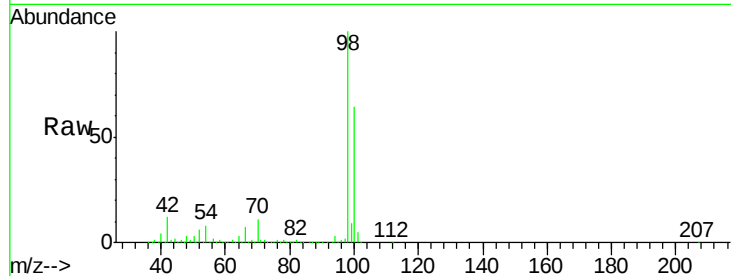

#62

4-Bromofluorobenzene

Concen: 52.915 ug/l

RT: 12.40 min Scan# 3305

Delta R.T. -0.00 min

Lab File: VN054040.D

Acq: 1 Mar 2019 20:08




Tgt Ion: 95 Resp: 494956


Ion Ratio Lower Upper

95 100

174 85.8 0.0 188.8

176 84.0 0.0 182.6

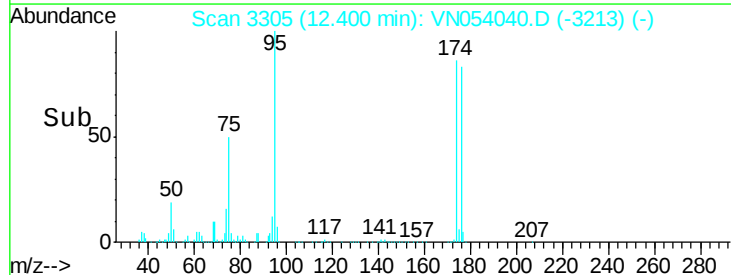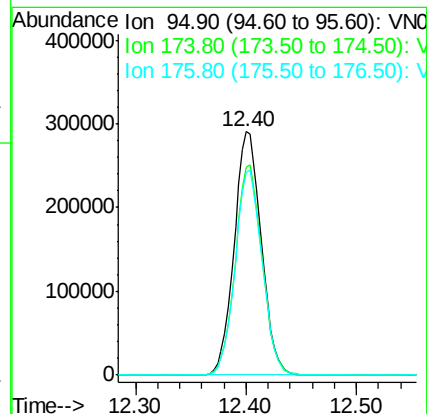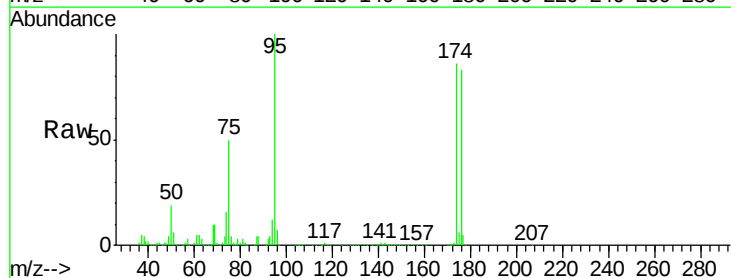


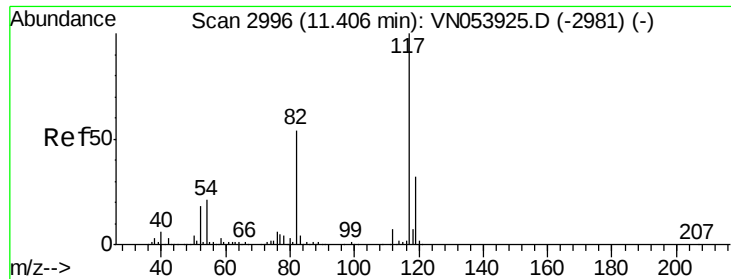




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.41 min Scan# 2996
Delta R.T. 0.00 min
Lab File: VN054040.D
Acq: 1 Mar 2019 20:08

Instrument :
MSVOA_N
ClientSampleId :
200029

Tot Ion:117 Resp: 1130566
Ion Ratio Lower Upper
117 100
82 55.7 41.4 62.2
119 32.6 25.3 37.9

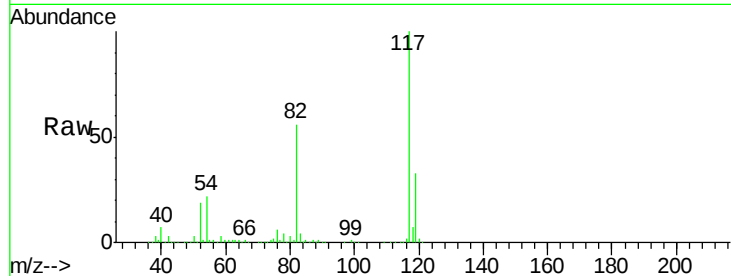


Abundance Ion 116.90 (116.60 to 117.60): V
Ion 82.00 (81.70 to 82.70): V
Ion 118.90 (118.60 to 119.60): V

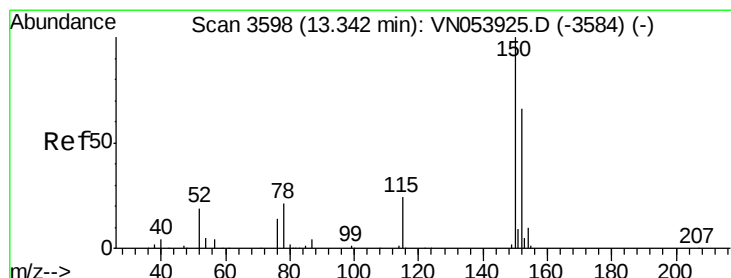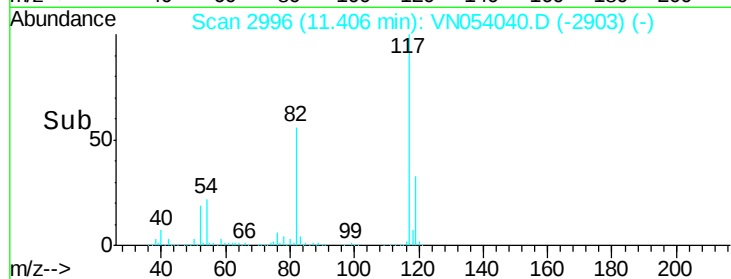
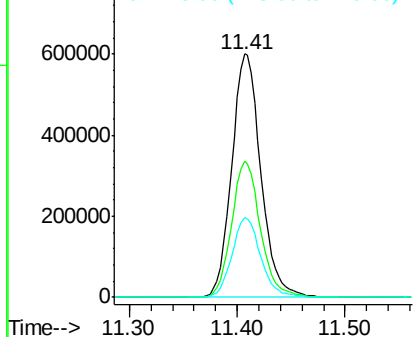



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.34 min Scan# 3598
Delta R.T. 0.00 min
Lab File: VN054040.D
Acq: 1 Mar 2019 20:08

Tgt Ion:152 Resp: 415171
Ion Ratio Lower Upper
152 100
115 57.0 27.2 81.6
150 155.3 0.0 348.2

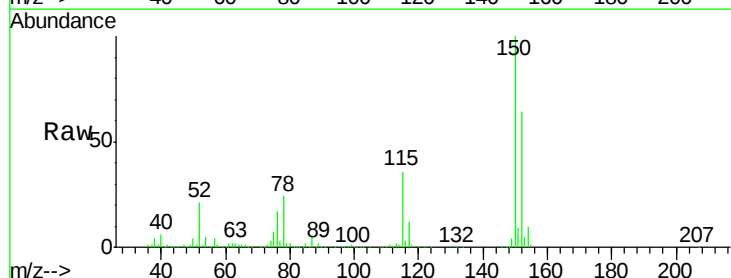

Abundance Ion 151.90 (151.60 to 152.60): V
Ion 114.90 (114.60 to 115.60): V
Ion 149.90 (149.60 to 150.60): V

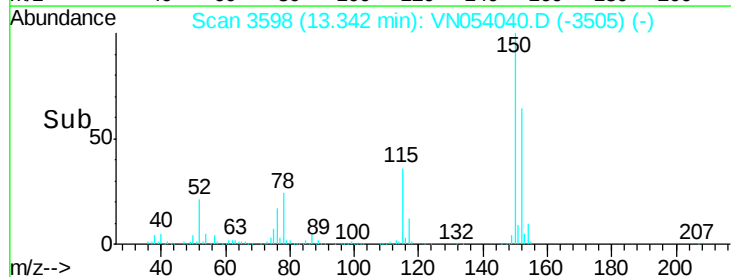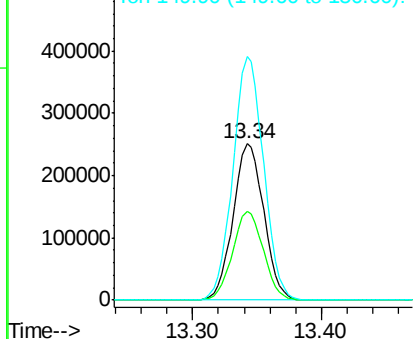

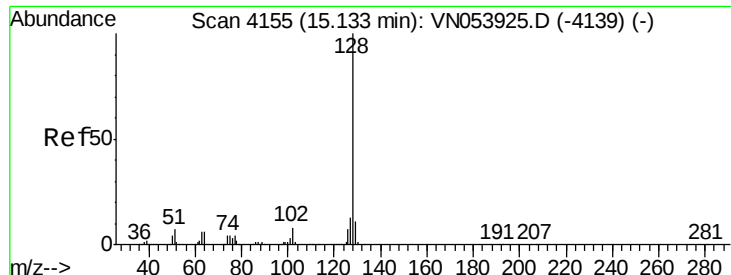

#95

Naphthalene

Concen: 3.803 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. 0.00 min

Lab File: VN054040.D

Acq: 1 Mar 2019 20:08

Instrument :

MSVOA_N

ClientSampleId :

200029


Tot Ion:128 Resp: 10385

Ion Ratio Lower Upper

128 100

127 12.2 10.2 15.2

129 12.5 8.6 12.8

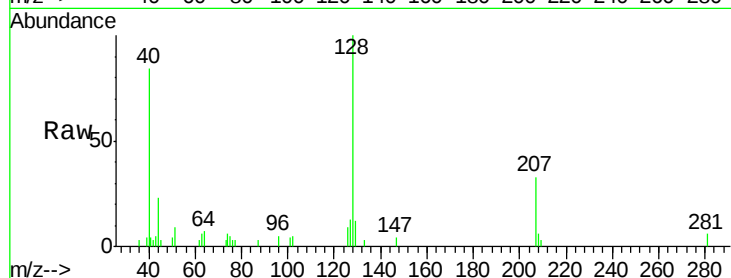

Abundance Ion 128.00 (127.70 to 128.70): V

Ion 127.00 (126.70 to 127.70): V

Ion 129.00 (128.70 to 129.70): V

