


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030219\
Data File : VN054031.D
Acq On : 1 Mar 2019 15:53
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Title : SW846 8260
Last Update : Thu Feb 28 04:05:45 2019

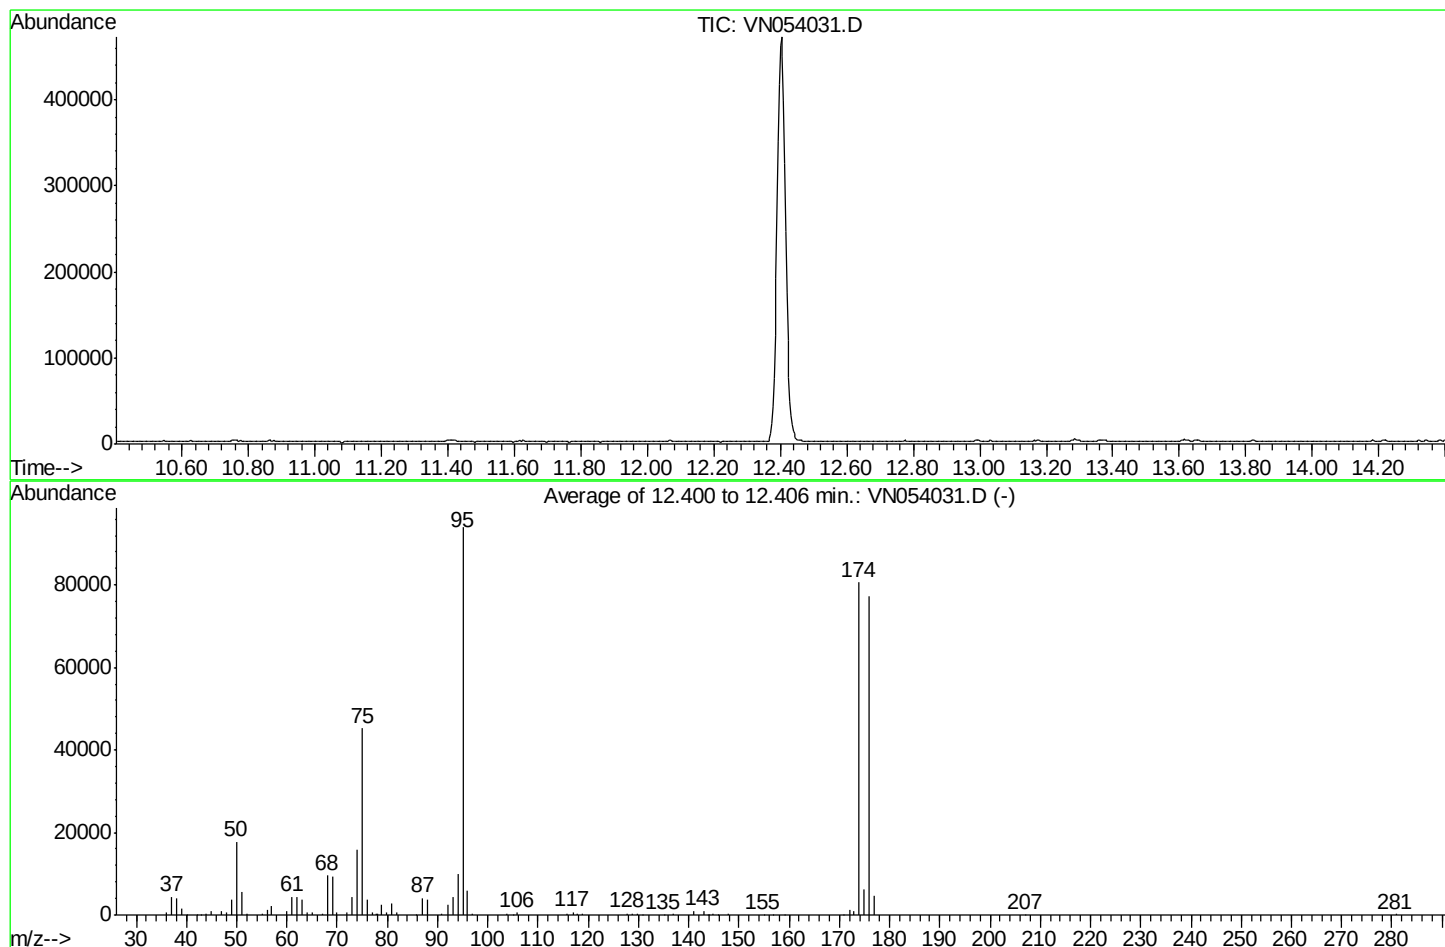

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.9	17725	PASS
75	95	30	60	48.2	45261	PASS
95	95	100	100	100.0	93981	PASS
96	95	5	9	6.4	6059	PASS
173	174	0.00	2	1.3	1020	PASS
174	95	50	100	85.7	80573	PASS
175	174	5	9	7.6	6087	PASS
176	174	95	101	95.8	77192	PASS
177	176	5	9	6.0	4666	PASS