

Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030220\
 Data File : VN060310.D
 Acq On : 2 Mar 2020 14:42
 Operator : JC/MD
 Sample : L1369-06
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :

Quant Time: Mar 03 05:46:43 2020
 Quant Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Quant Title : SW846 8260
 QLast Update : Thu Feb 27 13:52:50 2020
 Response via : Initial Calibration

Internal Standards	R.T.	QIon	Response	Conc	Units	Dev(Min)
1) Pentafluorobenzene	7.64	168	199648	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.57	114	324005	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.40	117	302697	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.34	152	144426	50.00	ug/l	0.00

System Monitoring Compounds	R.T.	QIon	Response	Conc	Units	Dev(Min)
33) 1,2-Dichloroethane-d4	8.00	65	128591	50.20	ug/l	0.00
Spiked Amount			Recovery	=	100.40%	
35) Dibromofluoromethane	7.57	113	87929	58.47	ug/l	0.00
Spiked Amount			Recovery	=	116.94%	
50) Toluene-d8	10.08	98	397402	52.21	ug/l	0.00
Spiked Amount			Recovery	=	104.42%	
62) 4-Bromofluorobenzene	12.40	95	149122	51.68	ug/l	0.00
Spiked Amount			Recovery	=	103.36%	


Target Compounds	R.T.	QIon	Response	Conc	Units	Qvalue
16) Acetone	3.79	43	20895	25.260	ug/l	99
17) Carbon Disulfide	4.03	76	93	Below Cal	#	75
18) Methyl Acetate	4.29	43	1738	0.630	ug/l #	52
20) Methylene Chloride	4.53	84	3717	1.636	ug/l	96
21) trans-1,2-Dichloroethene	5.02	96	64	Below Cal	#	1
25) 2-Butanone	6.81	43	1519	1.137	ug/l #	49
31) Cyclohexane	7.64	56	4354	Below Cal	#	7
36) 1,1-Dichloropropene	7.64	75	15582	5.046	ug/l #	50
37) Ethyl Acetate	6.81	43	1519	0.520	ug/l #	68
38) Carbon Tetrachloride	7.64	117	19438	6.465	ug/l #	16
43) Isopropyl Acetate	8.14	43	48068	9.391	ug/l #	91
45) 1,2-Dichloropropane	9.25	63	782	0.333	ug/l #	44
48) Methyl methacrylate	9.17	41	2797	1.198	ug/l #	13
51) 4-Methyl-2-Pentanone	9.97	43	4142	1.427	ug/l	94
52) Toluene	10.14	92	1296	0.230	ug/l	82
54) cis-1,3-Dichloropropene	9.89	75	20587	5.229	ug/l #	58
57) 1,3-Dichloropropane	10.75	76	3212	0.868	ug/l #	42
59) 2-Hexanone	10.75	43	47701	22.385	ug/l #	51
74) N-amyl acetate	12.02	43	3852	0.823	ug/l #	44
76) 1,2,3-Trichloropropane	12.40	75	76991	24.297	ug/l #	100
81) trans-1,4-Dichloro-2-buten	12.40	75	76991	67.072	ug/l #	8
87) 1,3-Dichlorobenzene	13.28	146	131	Below Cal	#	25
88) 1,4-Dichlorobenzene	13.35	146	171	Below Cal	#	1
90) Hexachloroethane	14.00	117	452	0.323	ug/l #	8
92) 1,2-Dibromo-3-Chloropropan	14.28	75	232	0.352	ug/l #	3
95) Naphthalene	15.13	128	8777	0.752	ug/l	99
96) 1,2,3-Trichlorobenzene	15.31	180	97	Below Cal	#	1

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\V0ASRV\HPCHEM1\MSVOA N\DATA\VN030220\
Data File : VN060310.D
Acq On : 2 Mar 2020 14:42
Operator : JC/MD
Sample : L1369-06
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :

Quant Time: Mar 03 05:46:43 2020
Quant Method : Z:\V0ASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Quant Title : SW846 8260
QLast Update : Thu Feb 27 13:52:50 2020
Response via : Initial Calibration

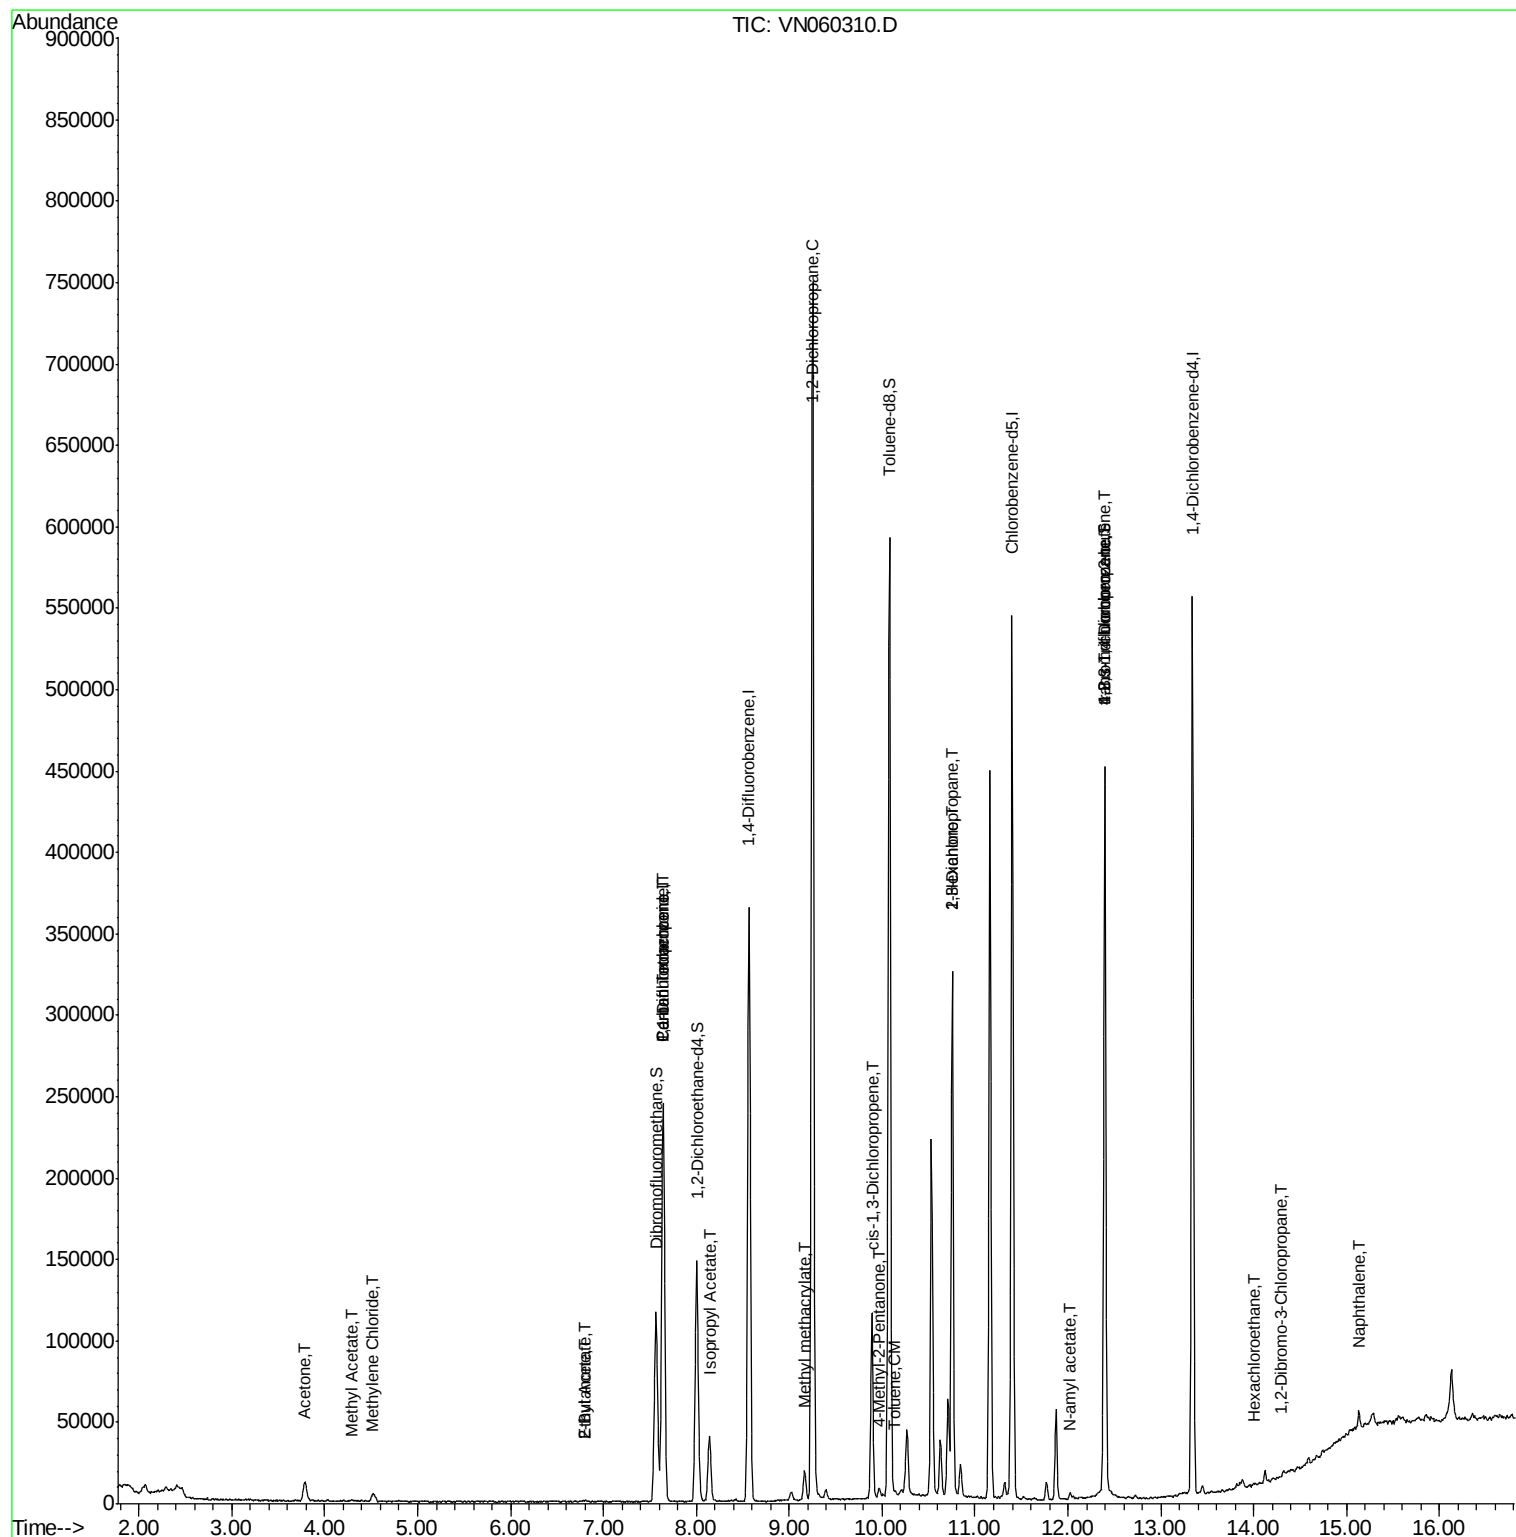



#1

Pentafluorobenzene

Concen: 50.000 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Instrument :
MSVOA_N
ClientSampled :

Tot Ion:168 Resp: 199648

Ion Ratio Lower Upper




168 100

99 56.0 44.7 67.1

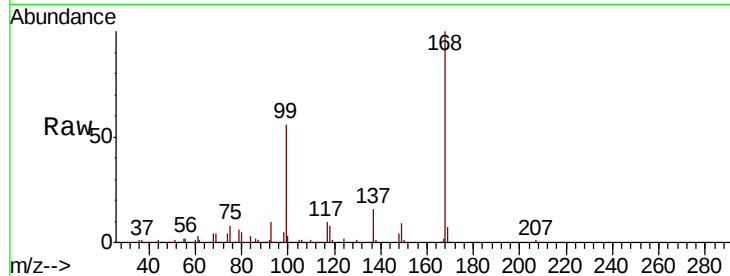

Abundance Ion 167.90 (167.60 to 168.60): V

Ion 98.90 (98.60 to 99.60): VN

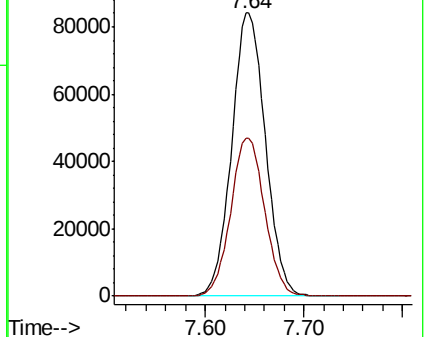

#16

Acetone

Concen: 25.260 ug/l

RT: 3.79 min Scan# 626

Delta R.T. 0.01 min

Lab File: VN060310.D


Acq: 2 Mar 2020 14:42

Tgt Ion: 43 Resp: 20895

Ion Ratio Lower Upper



43 100


58 30.0 24.6 36.8



Abundance Ion 43.00 (42.70 to 43.70): VN

Ion 58.00 (57.70 to 58.70): VN

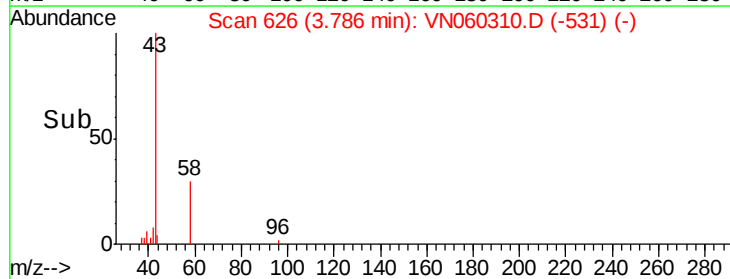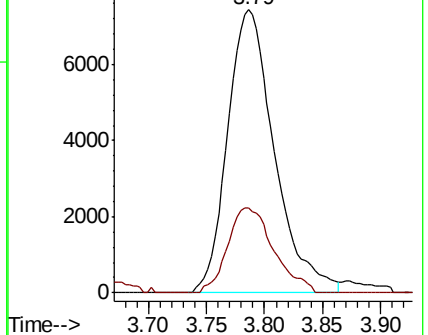



#17

Carbon Disulfide

Concen: Below Cal

RT: 4.03 min Scan# 702

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 76 Resp: 93

Ion Ratio Lower Upper

76 100

78 0.0 7.4 11.0#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

4.03

150



100

50

0

4.02 4.03 4.04

Time-->



#18

Methyl Acetate

Concen: 0.630 ug/l

RT: 4.29 min Scan# 782

Delta R.T. 0.00 min

Lab File: VN060310.D


Acq: 2 Mar 2020 14:42

Tgt Ion: 43 Resp: 1738

Ion Ratio Lower Upper

43 100

74 0.0 18.8 28.2#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 74.00 (73.70 to 74.70): VN0

600


400




200

0

4.25 4.30 4.35

Time-->









#20
Methvlene Chloride
Concen: 1.636 ua/l
RT: 4.53 min Scan# 856
Delta R.T. 0.00 min
Lab File: VN060310.D
Acq: 2 Mar 2020 14:42


Instrument :
MSVOA_N
ClientSampled :


Tot Ion:	84	Resp:	3717
Ion	Ratio	Lower	Upper
84	100		
49	128.2	99.3	148.9
51	39.1	30.1	45.1
86	69.5	51.1	76.7

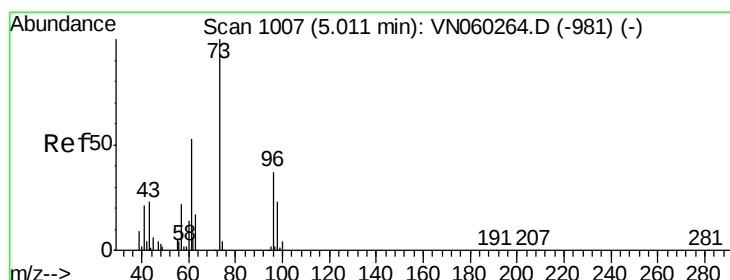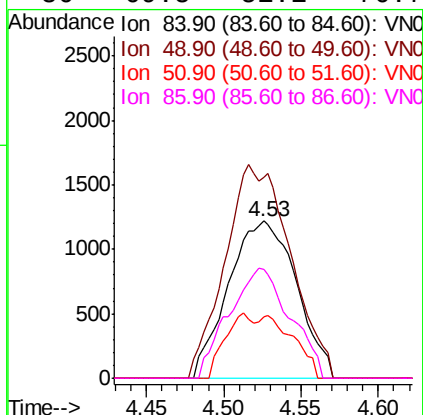

#21
trans-1,2-Dichloroethene
Concen: Below Cal
RT: 5.02 min Scan# 1010
Delta R.T. 0.01 min
Lab File: VN060310.D
Acq: 2 Mar 2020 14:42

Tgt Ion:	96	Resp:	64
Ion	Ratio	Lower	Upper
96	100		
61	0.0	113.8	170.8#
98	0.0	48.8	73.2#




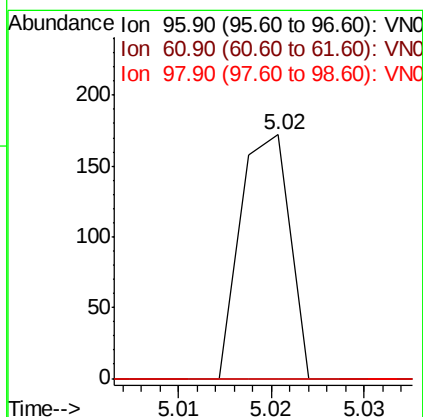




#25
 2-Butanone
 Concen: 1.137 ug/l
 RT: 6.81 min Scan# 1566
 Delta R.T. 0.01 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion: 43 Resp: 1519
 Ion Ratio Lower Upper
 43 100
 72 0.0 20.9 31.3#

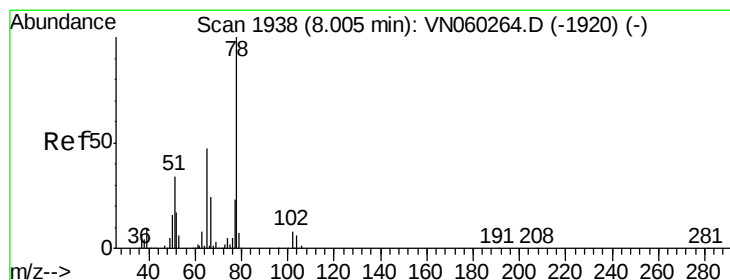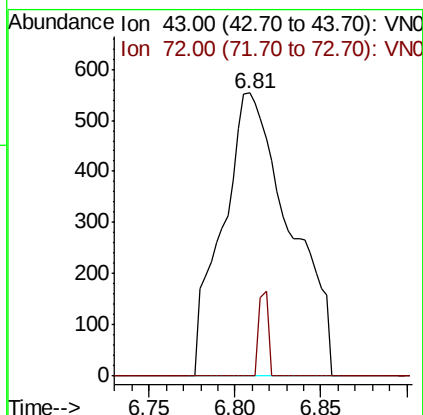

#33
 1,2-Dichloroethane-d4
 Concen: 50.201 ug/l
 RT: 8.00 min Scan# 1938
 Delta R.T. 0.00 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42

Tgt Ion: 65 Resp: 128591
 Ion Ratio Lower Upper
 65 100
 67 52.0 0.0 103.8

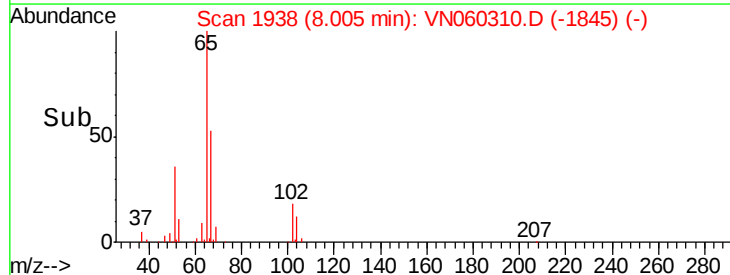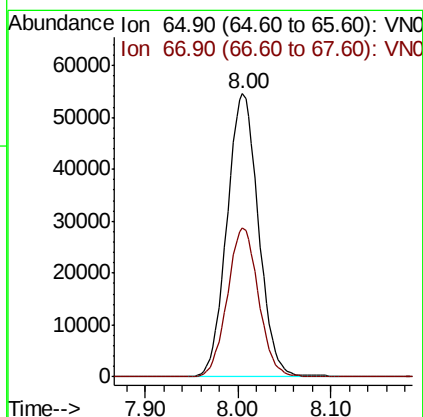







#34
 1,4-Difluorobenzene
 Concen: 50.000 ug/l
 RT: 8.57 min Scan# 2113
 Delta R.T. 0.00 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42

Instrument :
 MSVOA_N
 ClientSampleId :

Tot Ion	Ratio	Lower	Upper
114	100		
63	22.0	0.0	43.2
88	16.3	0.0	31.6




Abundance Ion 113.90 (113.60 to 114.60): V
 Ion 63.00 (62.70 to 63.70): VN
 Ion 87.90 (87.60 to 88.60): VN

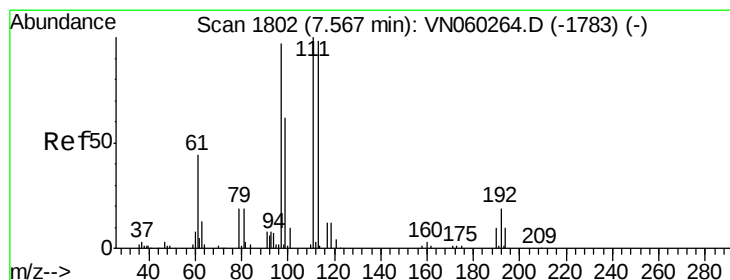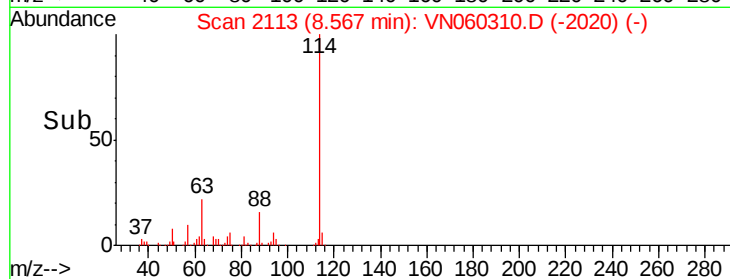
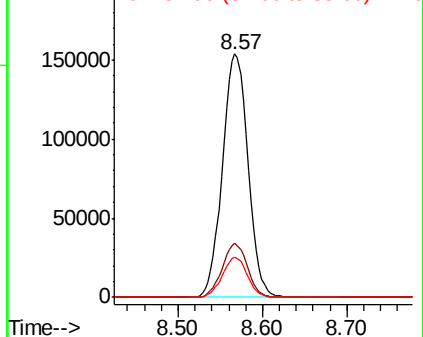



#35
 Dibromofluoromethane
 Concen: 58.466 ug/l
 RT: 7.57 min Scan# 1802
 Delta R.T. 0.00 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42

Tgt Ion	Ratio	Lower	Upper
113	100		
111	104.7	82.4	123.6
192	20.7	16.2	24.2



Abundance Ion 112.80 (112.50 to 113.50): V
 Ion 110.80 (110.50 to 111.50): V
 Ion 191.70 (191.40 to 192.40): V

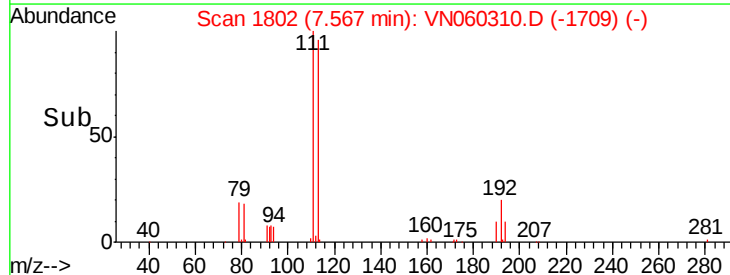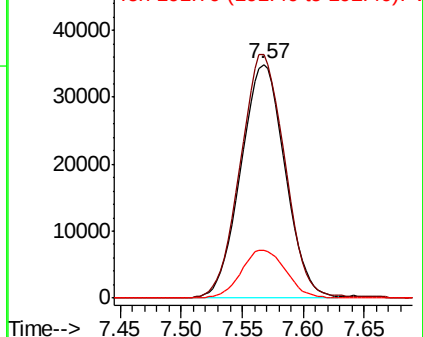



#36

1,1-Dichloropropene

Concen: 5.046 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.13 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N

ClientSampled :


Tot Ion: 75 Resp: 15582

Ion Ratio Lower Upper

75 100

110 8.4 17.3 52.0#




77 0.0 24.2 36.2#



Abundance Ion 74.90 (74.60 to 75.60): VN060310.D (-1772) (-)

Ion 109.90 (109.60 to 110.60): VN060310.D (-1772) (-)

Ion 76.90 (76.60 to 77.60): VN060310.D (-1772) (-)

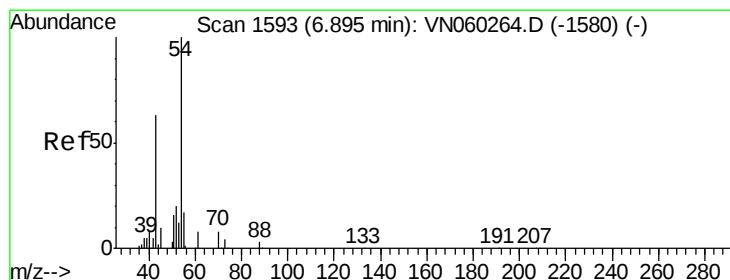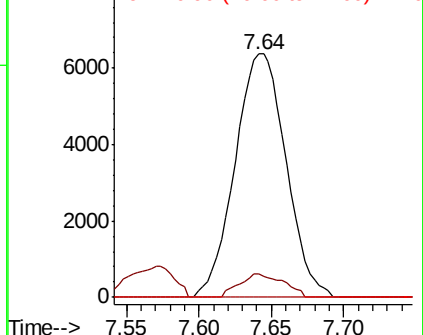

#37

Ethyl Acetate

Concen: 0.520 ug/l

RT: 6.81 min Scan# 1566

Delta R.T. -0.09 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 43 Resp: 1519

Ion Ratio Lower Upper

43 100

61 0.0 11.1 16.7#



70 0.0 8.4 12.6#




Abundance Ion 43.00 (42.70 to 43.70): VN060310.D (-1500) (-)

Ion 60.90 (60.60 to 61.60): VN060310.D (-1500) (-)

Ion 70.00 (69.70 to 70.70): VN060310.D (-1500) (-)

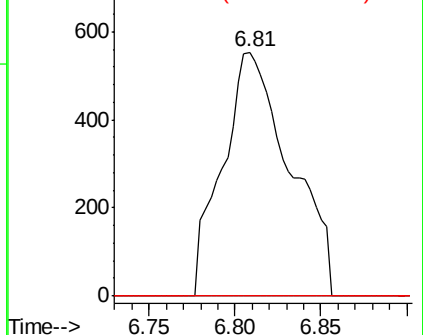



#38

Carbon Tetrachloride

Concen: 6.465 ug/l

RT: 7.64 min Scan# 1825

Delta R.T. -0.11 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:117 Resp: 19438

Ion Ratio Lower Upper

117 100

119 5.7 76.7 115.1#




121 0.0 24.5 36.7#



Abundance Ion 116.80 (116.50 to 117.50): V

Ion 118.80 (118.50 to 119.50): V

Ion 120.80 (120.50 to 121.50): V

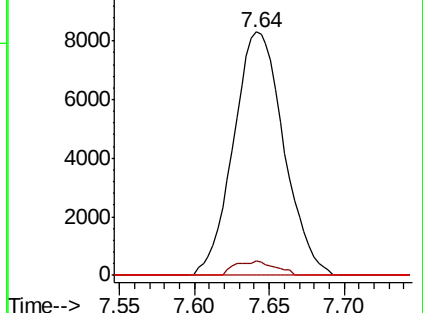

#43

Isopropyl Acetate

Concen: 9.391 ug/l

RT: 8.14 min Scan# 1981

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 43 Resp: 48068

Ion Ratio Lower Upper

43 100

61 19.8 20.9 31.3#



87 12.8 10.6 16.0




Abundance Ion 43.00 (42.70 to 43.70): V

Ion 61.00 (60.70 to 61.70): V

Ion 87.00 (86.70 to 87.70): V



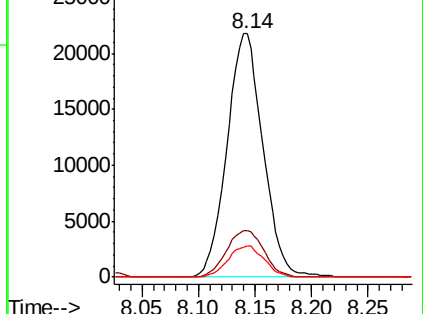



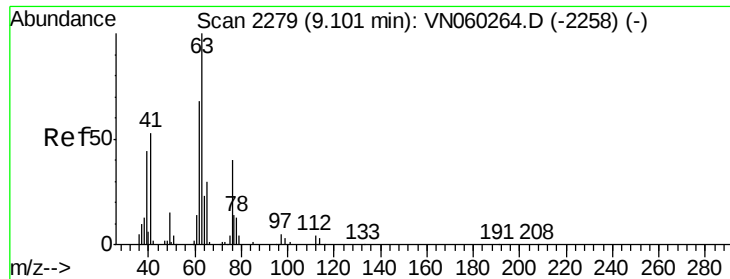

#45
 1,2-Dichloropropane
 Concen: 0.333 ug/l
 RT: 9.25 min Scan# 2325
 Delta R.T. 0.15 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42




Instrument :
 MSVOA_N
 ClientSampled :


Tot Ion: 63 Resp: 782
 Ion Ratio Lower Upper
 63 100
 65 0.0 24.4 36.6#

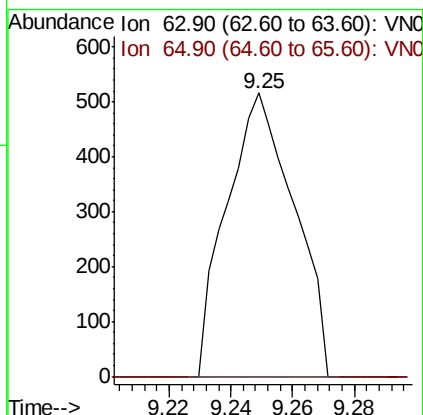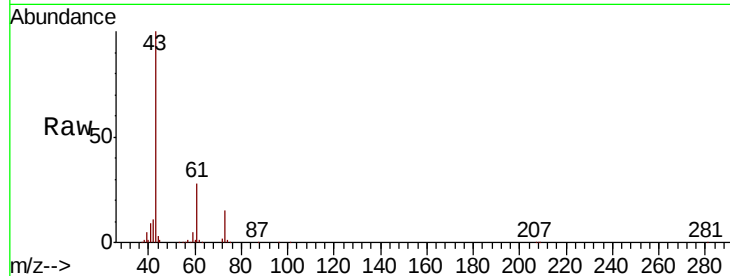

#48
 Methyl methacrylate
 Concen: 1.198 ug/l
 RT: 9.17 min Scan# 2299
 Delta R.T. -0.02 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42

Tgt Ion: 41 Resp: 2797
 Ion Ratio Lower Upper
 41 100
 69 0.0 66.7 100.1#
 39 0.0 50.1 75.1#

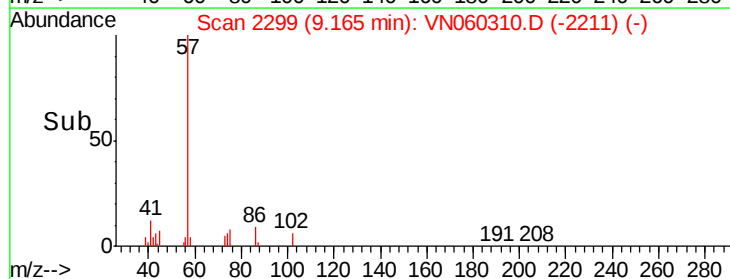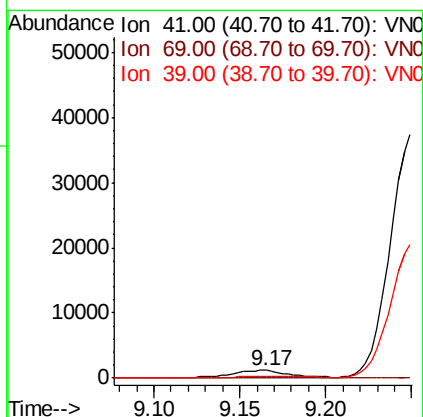



#50

Toluene-d8

Concen: 52.210 ug/l

RT: 10.08 min Scan# 2583

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 98 Resp: 397402

Ion Ratio Lower Upper

98 100

100 65.0 52.2 78.2



Abundance Ion 98.00 (97.70 to 98.70): VN060264.D (-2567) (-)

Ion 100.00 (99.70 to 100.70): VN060264.D (-2567) (-)

10.08

250000

200000



150000

100000

50000

0

Time-->



#51

4-Methyl-2-Pentanone

Concen: 1.427 ug/l

RT: 9.97 min Scan# 2549

Delta R.T. 0.00 min

Lab File: VN060310.D


Acq: 2 Mar 2020 14:42

Tgt Ion: 43 Resp: 4142

Ion Ratio Lower Upper

43 100

58 35.1 30.9 46.3



Abundance Ion 43.00 (42.70 to 43.70): VN060264.D (-2531) (-)

Ion 58.00 (57.70 to 58.70): VN060264.D (-2531) (-)

8000


6000


4000

2000

0

Time-->





#52

Toluene

Concen: 0.230 ug/l

RT: 10.14 min Scan# 2603

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 92 Resp: 1296

Ion Ratio Lower Upper




92 100

91 197.2 138.1 207.1

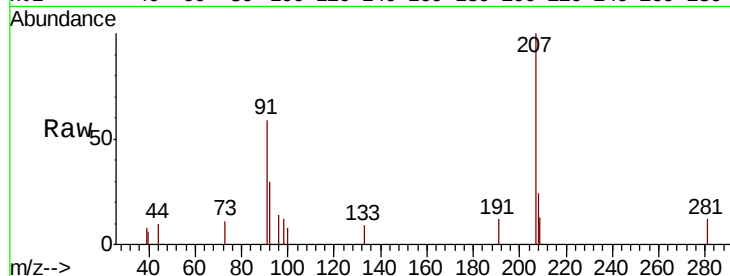

Abundance Ion 92.00 (91.70 to 92.70): VN0

Ion 91.00 (90.70 to 91.70): VN0

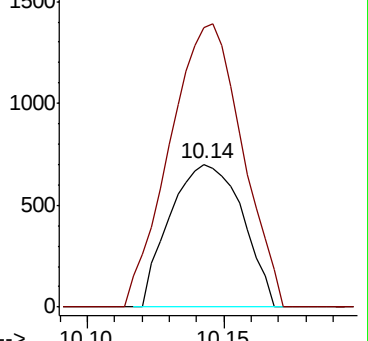

#54

cis-1,3-Dichloropropene

Concen: 5.229 ug/l

RT: 9.89 min Scan# 2525

Delta R.T. 0.07 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 75 Resp: 20587

Ion Ratio Lower Upper

75 100

77 0.0 24.8 37.2#



39 30.9 43.8 65.8#




Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 76.90 (76.60 to 77.60): VN0

Ion 39.00 (38.70 to 39.70): VN0

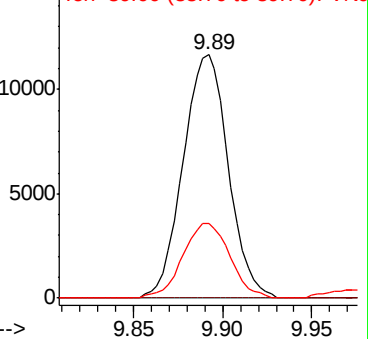



#57

1,3-Dichloropropane

Concen: 0.868 ug/l

RT: 10.75 min Scan# 2793

Delta R.T. 0.06 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N


ClientSampleId :

Tot Ion: 76 Resp: 3212

Ion Ratio Lower Upper




76 100

78 0.0 26.2 39.2#



Abundance Ion 75.90 (75.60 to 76.60): VN0

Ion 77.90 (77.60 to 78.60): VN0

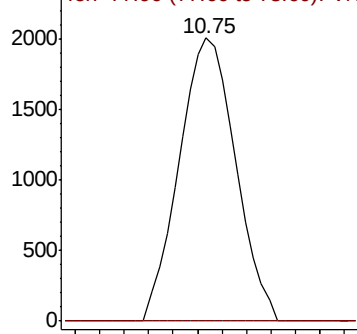

#59

2-Hexanone

Concen: 22.385 ug/l

RT: 10.75 min Scan# 2793

Delta R.T. 0.01 min

Lab File: VN060310.D


Acq: 2 Mar 2020 14:42

Tgt Ion: 43 Resp: 47701

Ion Ratio Lower Upper



43 100


58 18.5 26.5 79.5#



Abundance Ion 43.00 (42.70 to 43.70): VN0

Ion 58.00 (57.70 to 58.70): VN0

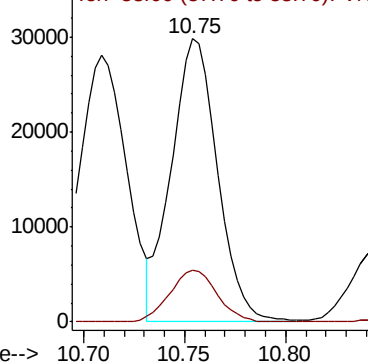

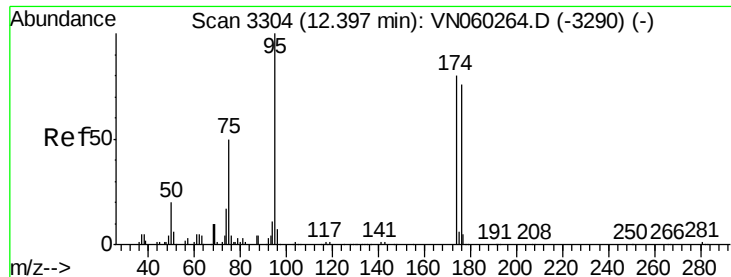

#62

4-Bromofluorobenzene

Concen: 51.682 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 95 Resp: 149122

Ion Ratio Lower Upper

95 100

174 79.8 0.0 159.2




176 78.4 0.0 153.8

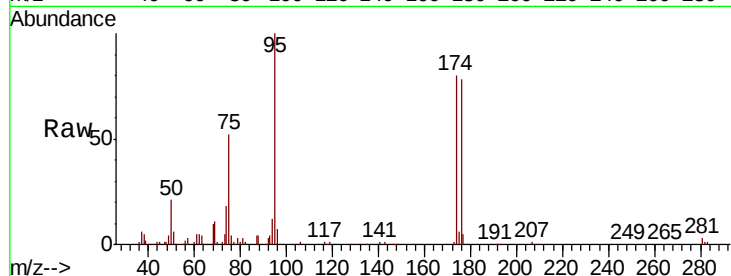

Abundance Ion 94.90 (94.60 to 95.60): VN060310.D (-3211) (-)

Ion 173.80 (173.50 to 174.50): VN060310.D (-3211) (-)

Ion 175.80 (175.50 to 176.50): VN060310.D (-3211) (-)

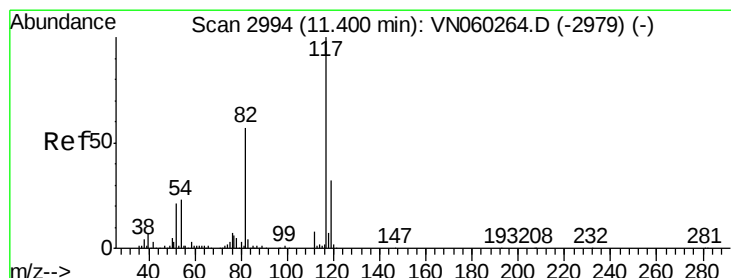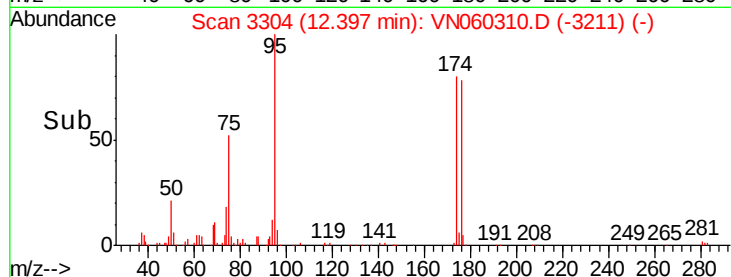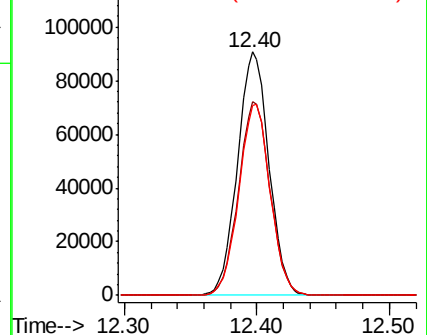

#63

Chlorobenzene-d5

Concen: 50.000 ug/l

RT: 11.40 min Scan# 2994

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 117 Resp: 302697

Ion Ratio Lower Upper

117 100

82 56.7 45.8 68.6



119 32.1 25.8 38.8

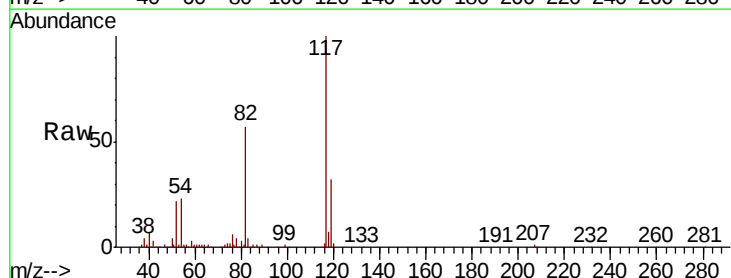


Abundance Ion 116.90 (116.60 to 117.60): VN060310.D (-2901) (-)

Ion 82.00 (81.70 to 82.70): VN060310.D (-2901) (-)

Ion 118.90 (118.60 to 119.60): VN060310.D (-2901) (-)

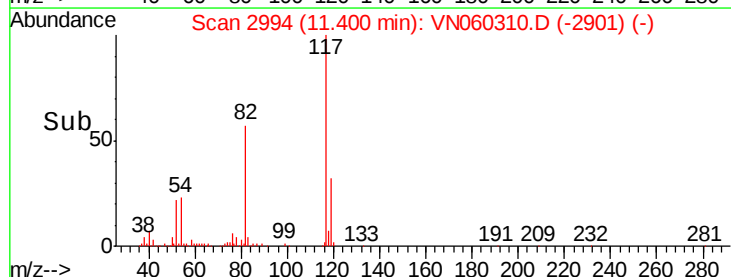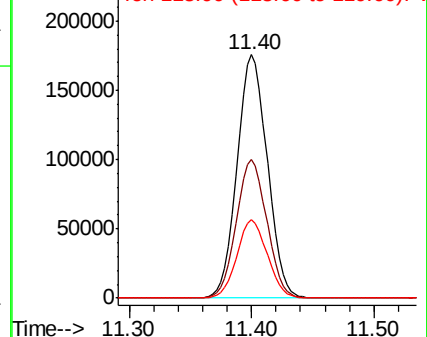

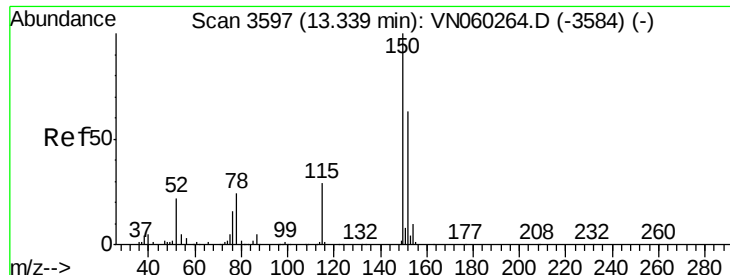

#72

1,4-Dichlorobenzene-d4

Concen: 50.000 ug/l

RT: 13.34 min Scan# 3597

Delta R.T. -0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion:152 Resp: 144426

Ion Ratio Lower Upper

152 100

115 57.9 30.0 90.0




150 155.0 0.0 349.6

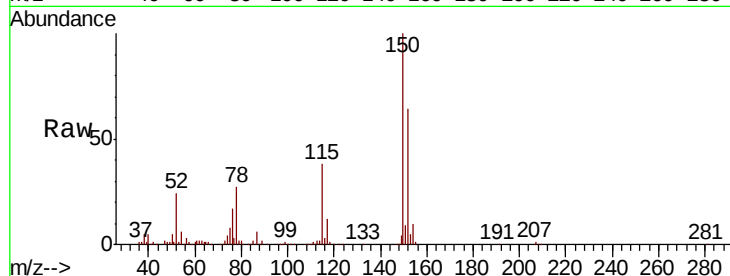

Abundance Ion 151.90 (151.60 to 152.60): V

Ion 114.90 (114.60 to 115.60): V

Ion 149.90 (149.60 to 150.60): V

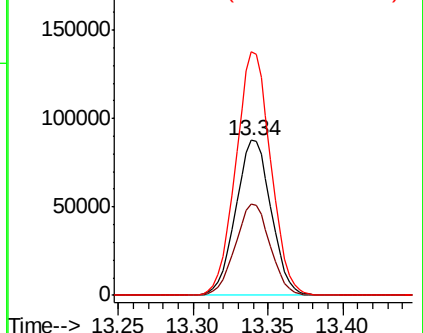

#74

N-ethyl acetate

Concen: 0.823 ug/l

RT: 12.02 min Scan# 3187

Delta R.T. -0.04 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Tgt Ion: 43 Resp: 3852


Ion Ratio Lower Upper

43 100

70 0.0 32.2 48.2#

55 0.0 18.2 27.4#

61 0.0 19.2 28.8#


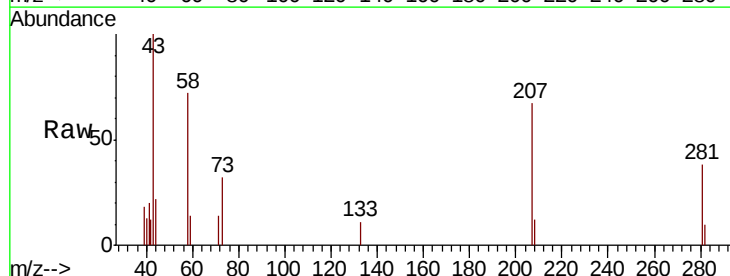



Abundance Ion 43.00 (42.70 to 43.70): VNO

Ion 70.00 (69.70 to 70.70): VNO

Ion 55.00 (54.70 to 55.70): VNO

Ion 61.00 (60.70 to 61.70): VNO

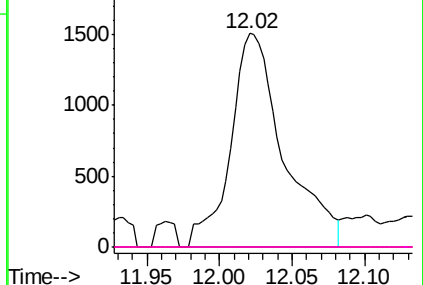

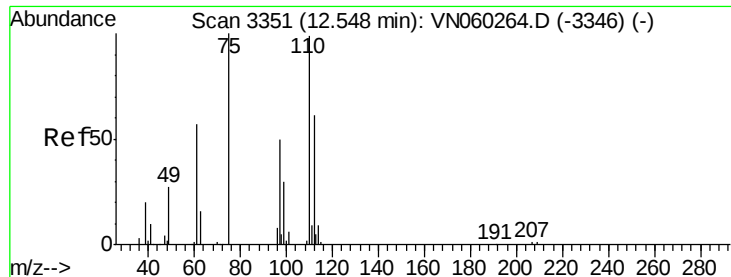

#76

1,2,3-Trichloropropane

Concen: 24.297 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. -0.15 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N


ClientSampled :

Tot Ion: 75 Resp: 76991

Ion Ratio Lower Upper




75 100

77 1.3 0.0 0.0#

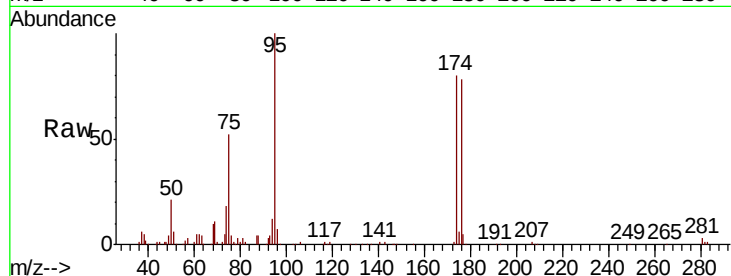

Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 77.00 (76.70 to 77.70): VN0

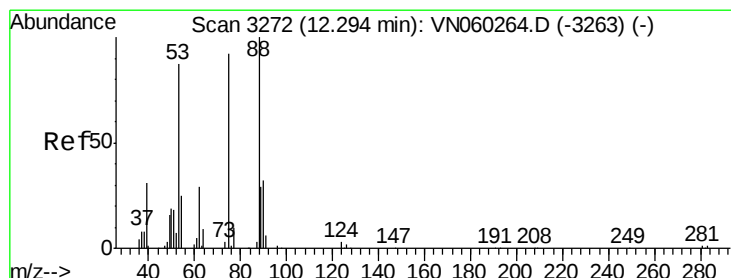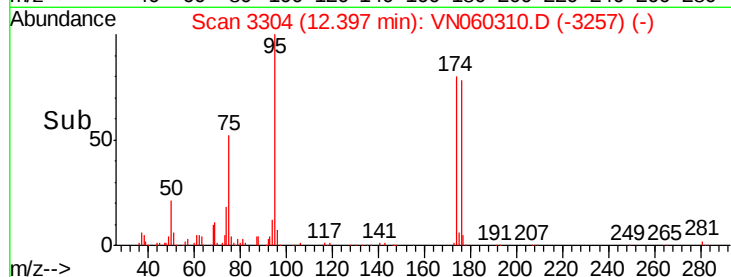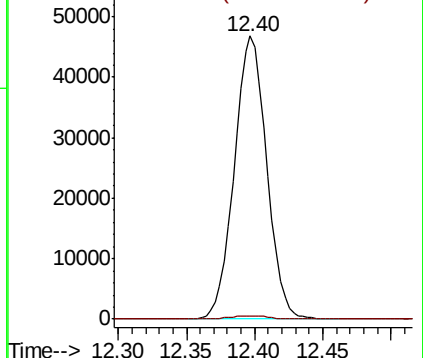

#81

trans-1,4-Dichloro-2-butene

Concen: 67.072 ug/l

RT: 12.40 min Scan# 3304

Delta R.T. 0.10 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 75 Resp: 76991

Ion Ratio Lower Upper

75 100

53 0.0 73.8 110.6#



89 0.0 57.1 85.7#

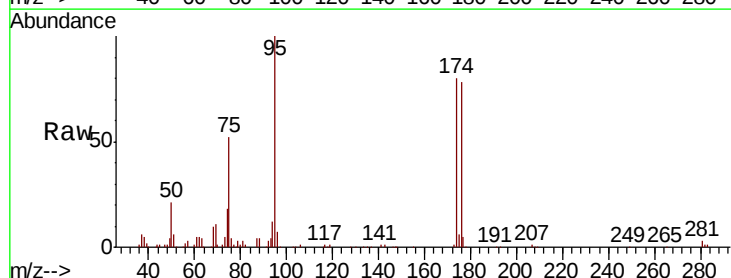


Abundance Ion 74.90 (74.60 to 75.60): VN0

Ion 53.00 (52.70 to 53.70): VN0

Ion 88.90 (88.60 to 89.60): VN0



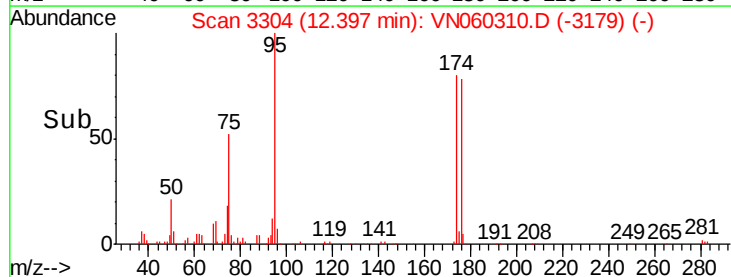
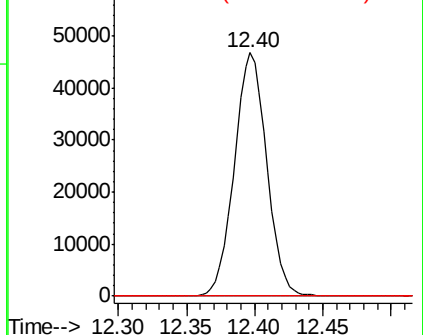




#88
 1,4-Dichlorobenzene
 Concen: Below Cal
 RT: 13.35 min Scan# 3602
 Delta R.T. -0.00 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42




Instrument :
 MSVOA_N
 ClientSampleId :


Tot Ion:146 Resp: 171
 Ion Ratio Lower Upper
 146 100
 111 1122.2 19.8 59.4#
 148 518.1 32.3 96.9#

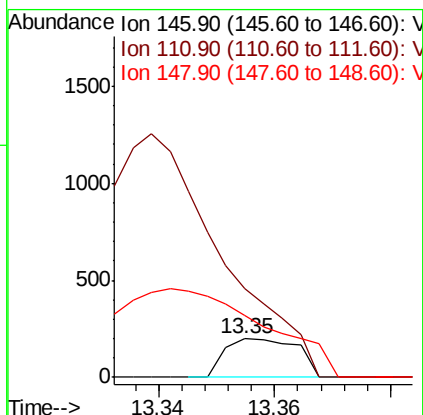

#90
 Hexachloroethane
 Concen: 0.323 ug/l
 RT: 14.00 min Scan# 3802
 Delta R.T. 0.13 min
 Lab File: VN060310.D
 Acq: 2 Mar 2020 14:42

Tgt Ion:117 Resp: 452
 Ion Ratio Lower Upper
 117 100
 201 0.0 41.0 123.0#

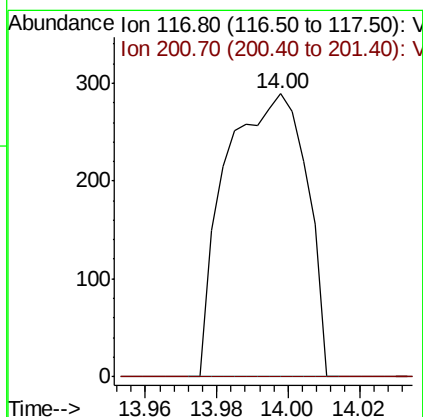

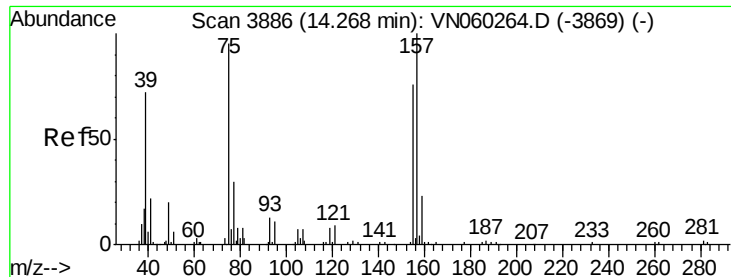

#92

1,2-Dibromo-3-Chloropropane

Concen: 0.352 ug/l

RT: 14.28 min Scan# 3890

Delta R.T. 0.01 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42

Instrument :

MSVOA_N

ClientSampleId :


Tot Ion: 75 Resp: 232

Ion Ratio Lower Upper

75 100

155 0.0 40.4 121.2#




157 0.0 52.5 157.5#

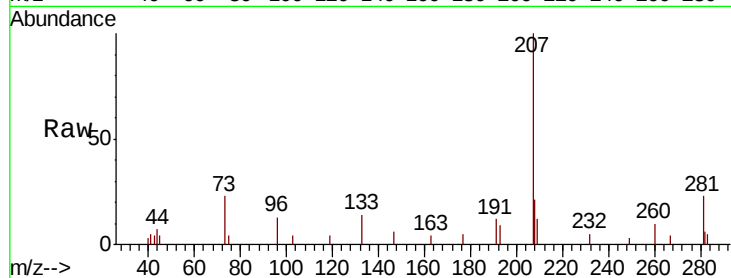

Abundance Ion 74.90 (74.60 to 75.60): VN060310.D (-3793) (-)

Ion 154.80 (154.50 to 155.50): VN060310.D (-3793) (-)

Ion 156.80 (156.50 to 157.50): VN060310.D (-3793) (-)

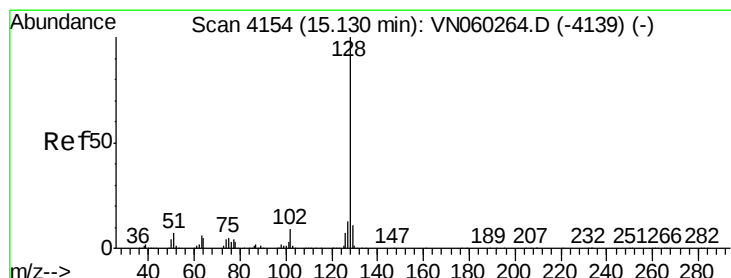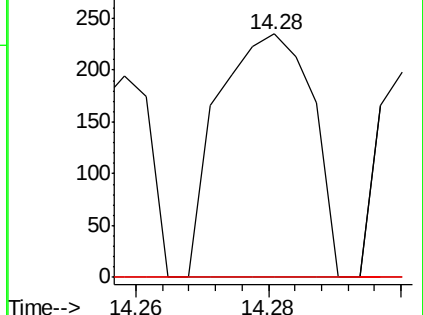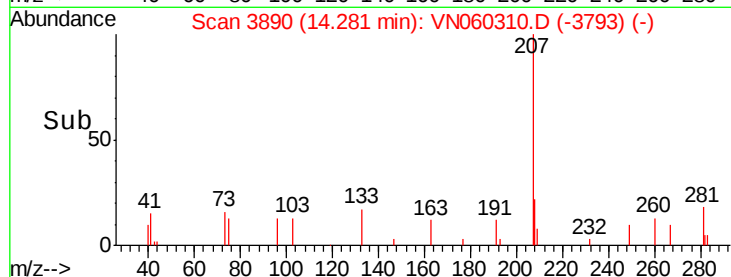

#95

Naphthalene

Concen: 0.752 ug/l

RT: 15.13 min Scan# 4155

Delta R.T. 0.00 min

Lab File: VN060310.D

Acq: 2 Mar 2020 14:42


Tgt Ion: 128 Resp: 8777

Ion Ratio Lower Upper

128 100

127 12.9 10.4 15.6

129 10.0 8.6 13.0

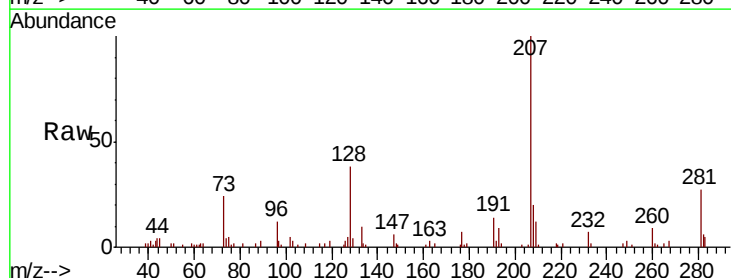

Abundance Ion 128.00 (127.70 to 128.70): VN060310.D (-4060) (-)

Ion 127.00 (126.70 to 127.70): VN060310.D (-4060) (-)

Ion 129.00 (128.70 to 129.70): VN060310.D (-4060) (-)

