


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN030220\
 Data File : VN060297.D
 Acq On : 2 Mar 2020 8:22
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
 Title : SW846 8260
 Last Update : Thu Feb 27 13:52:50 2020

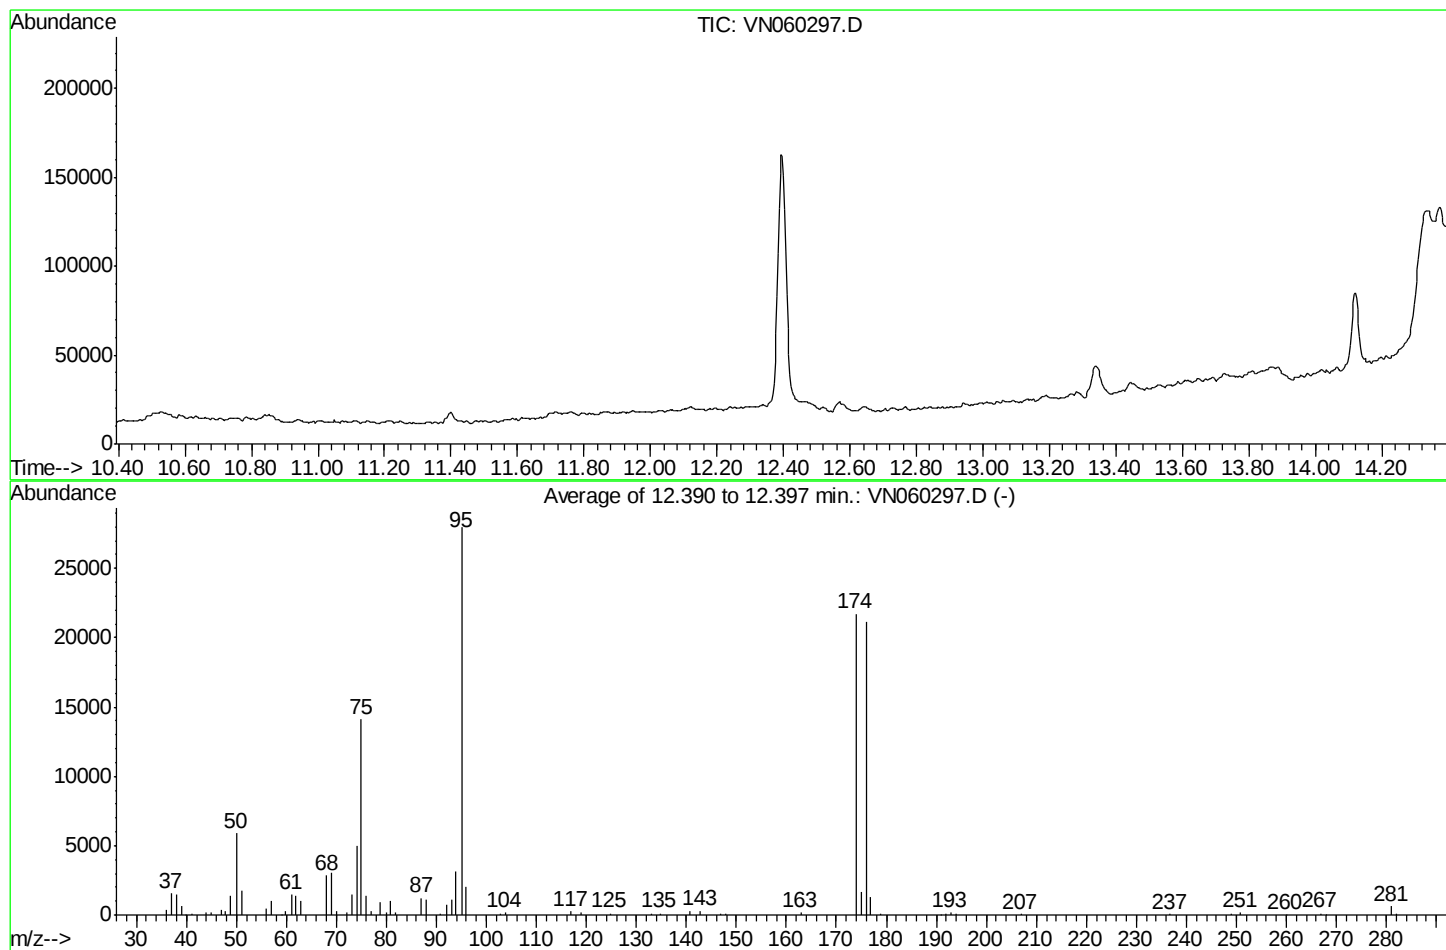

AutoFind: Scans 3302, 3303, 3304; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	21.0	5886	PASS
75	95	30	60	50.5	14115	PASS
95	95	100	100	100.0	27968	PASS
96	95	5	9	7.3	2030	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	77.6	21709	PASS
175	174	5	9	7.8	1691	PASS
176	174	95	101	97.3	21120	PASS
177	176	5	9	6.3	1324	PASS