


Chloromethane

Response Ratio

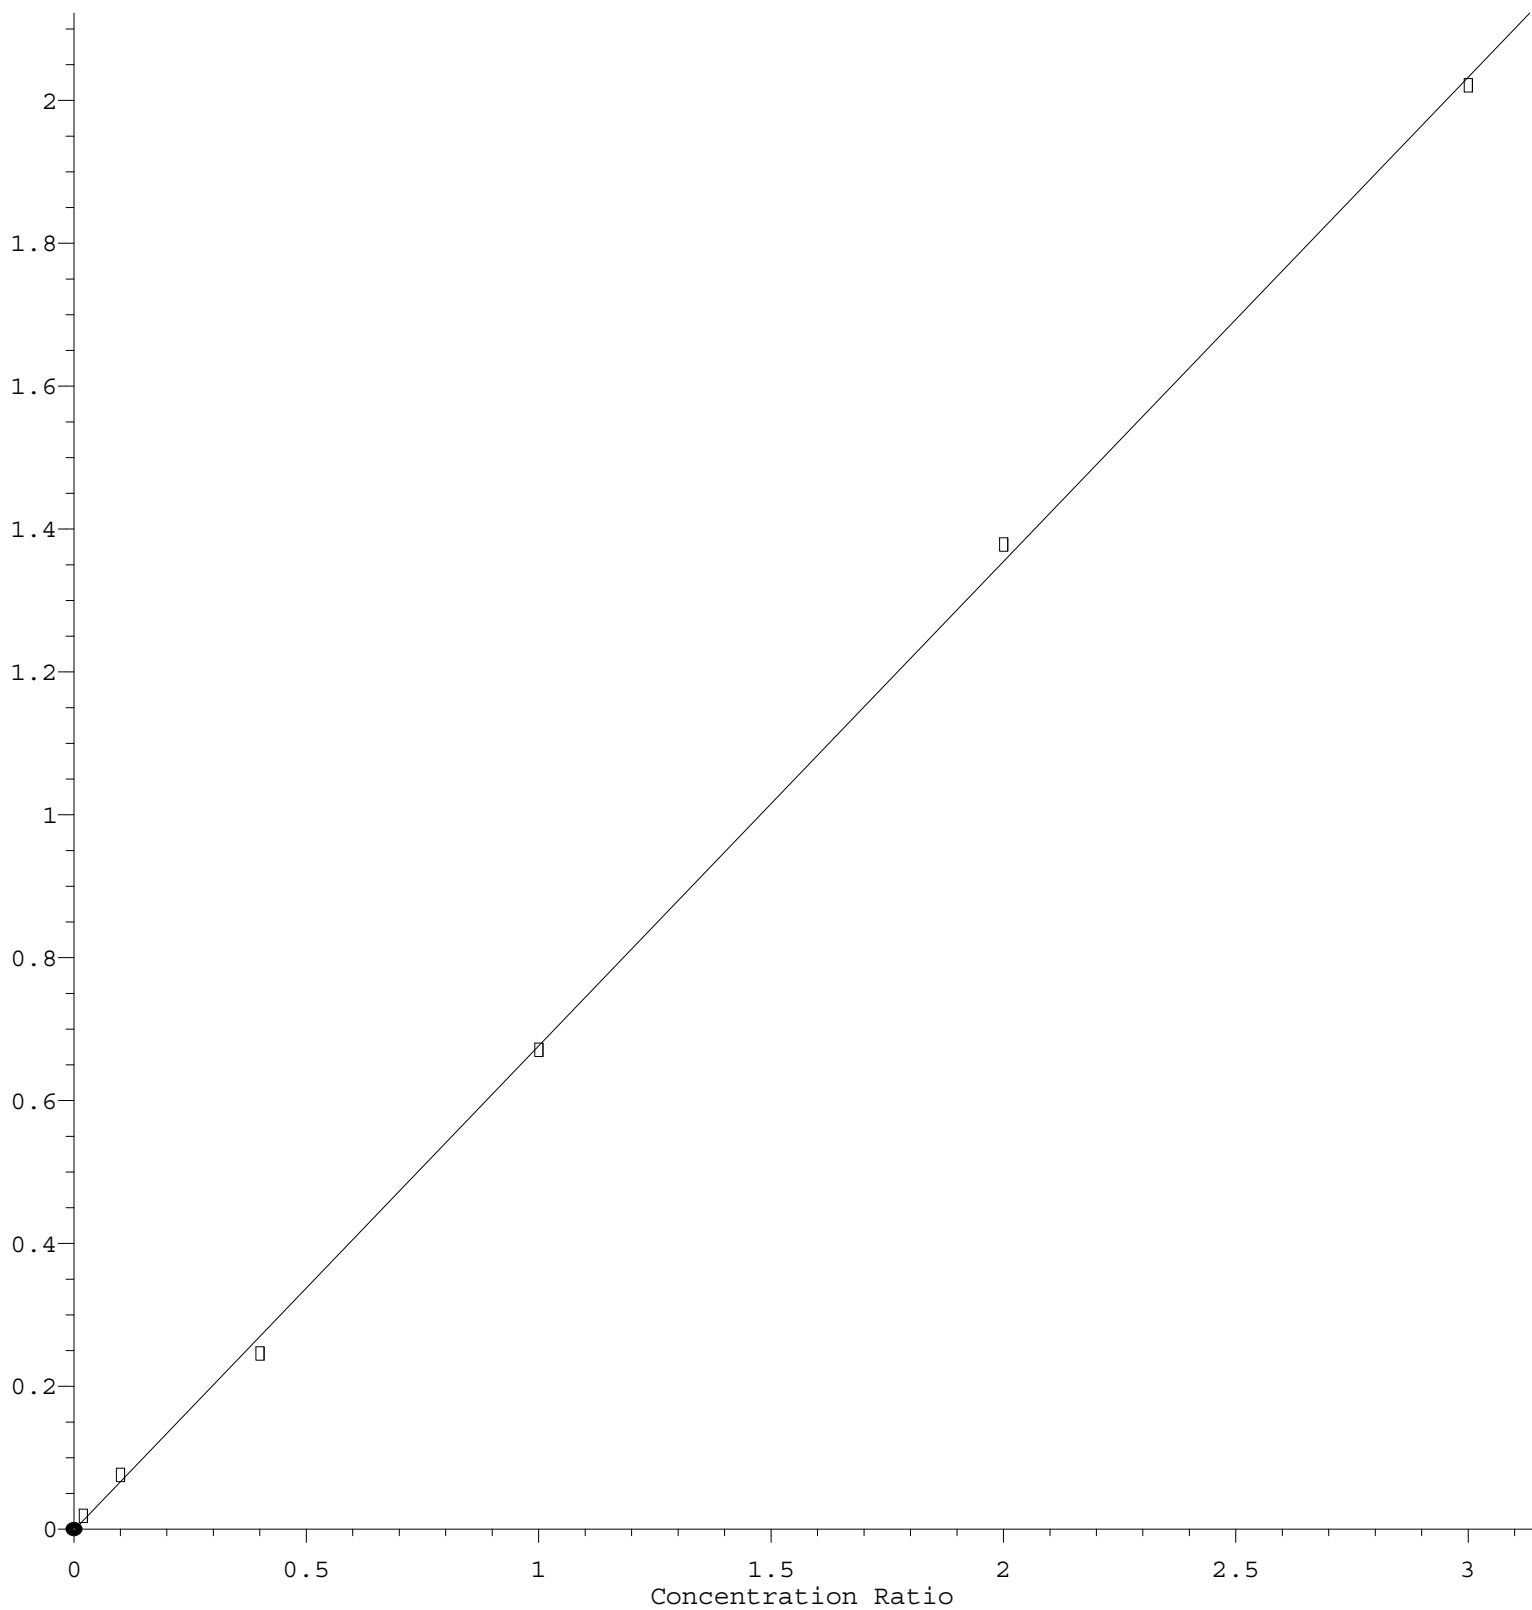

$$\text{Response} = 6.780\text{e-}001 * \text{Amt} - 1.660\text{e-}003$$


Coef of Det (r^2) = 0.999562 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M

Calibration Table Last Updated: Tue Mar 02 14:05:08 2021

Acrolein

Response Ratio

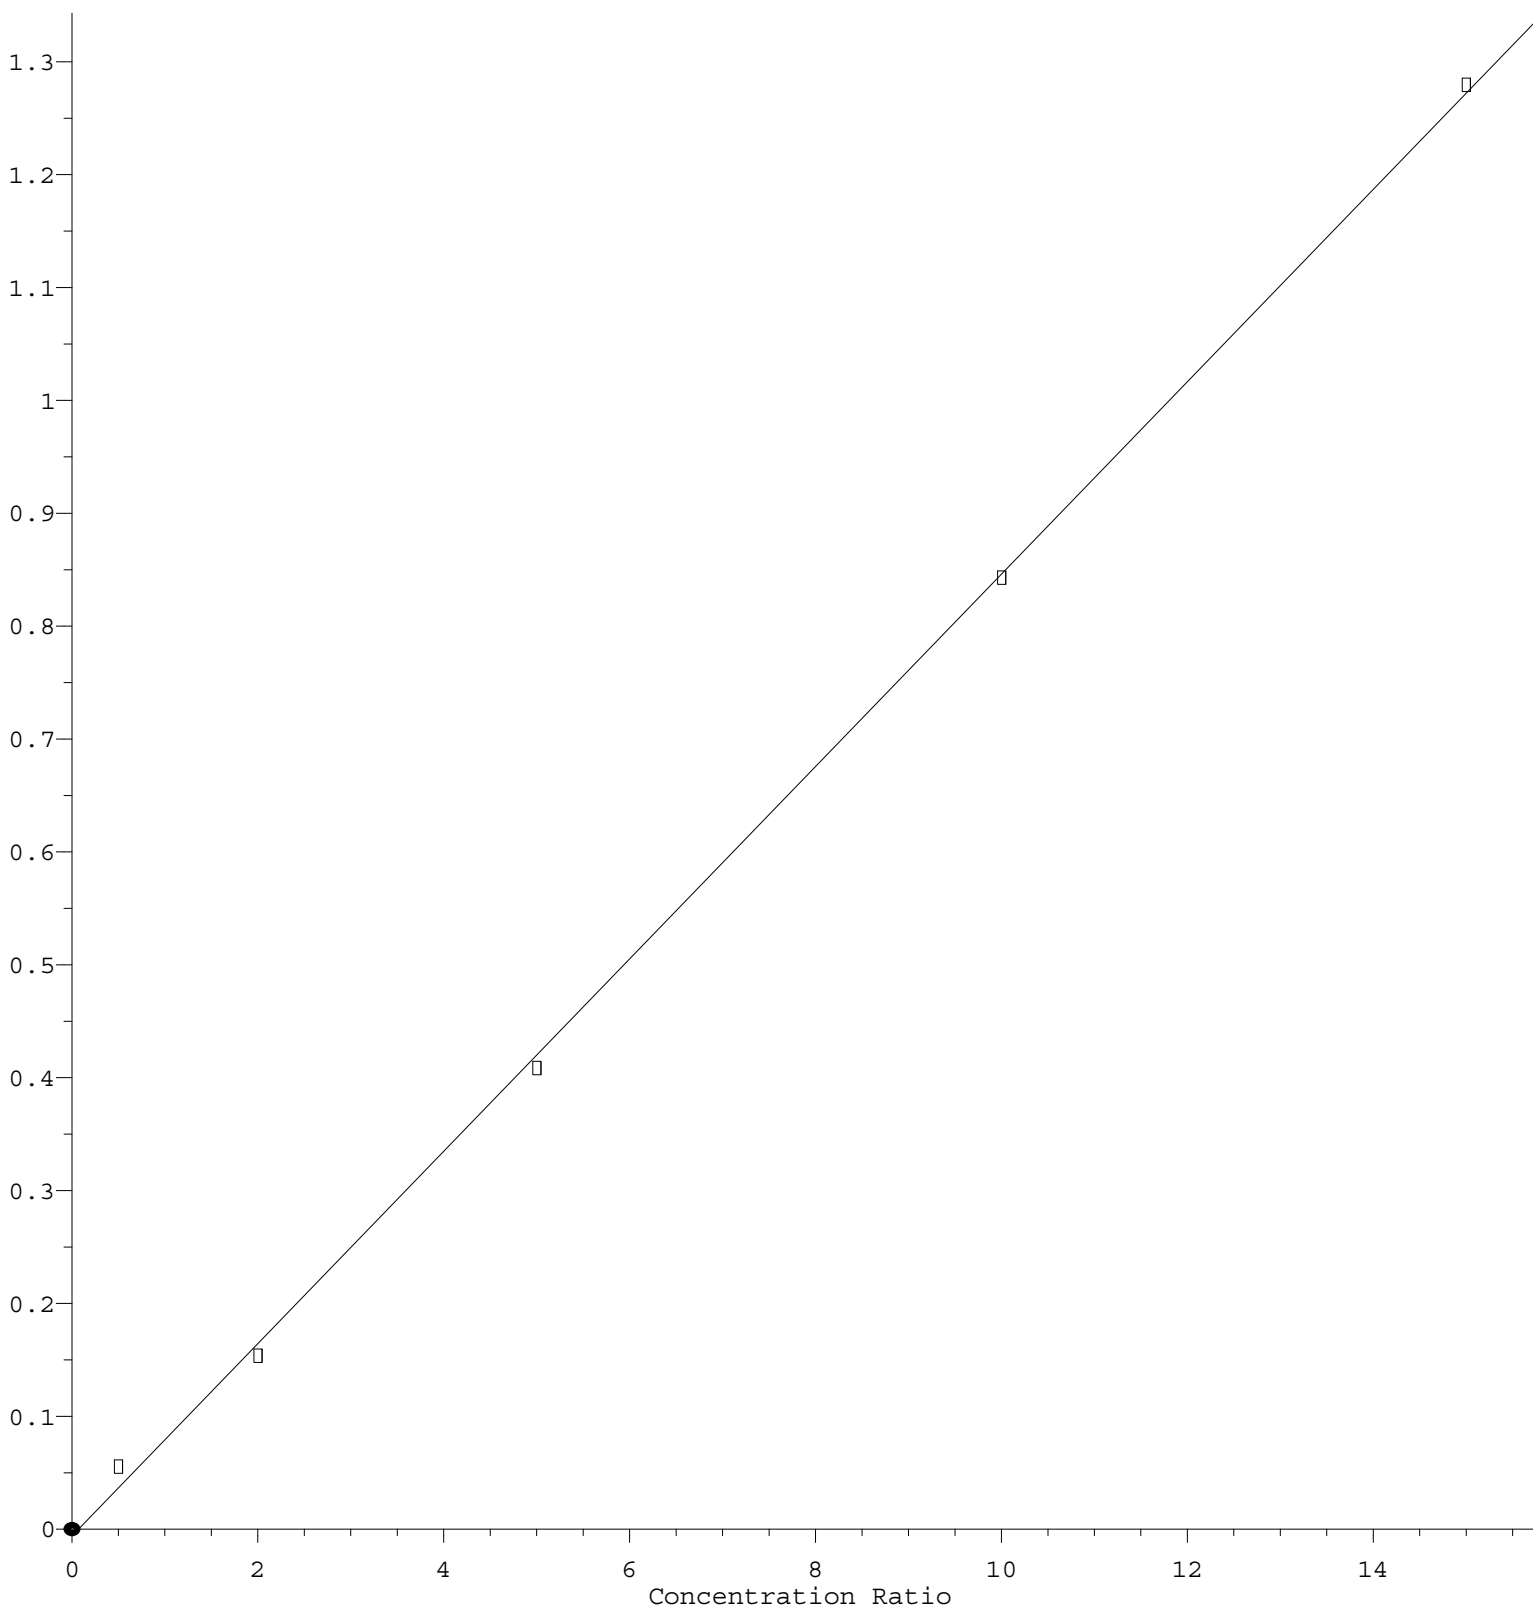

$$\text{Response} = 8.524\text{e-}002 * \text{Amt} - 6.093\text{e-}003$$


Coef of Det (r^2) = 0.999358 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M

Calibration Table Last Updated: Tue Mar 02 14:05:08 2021

Bromochloromethane

Response Ratio

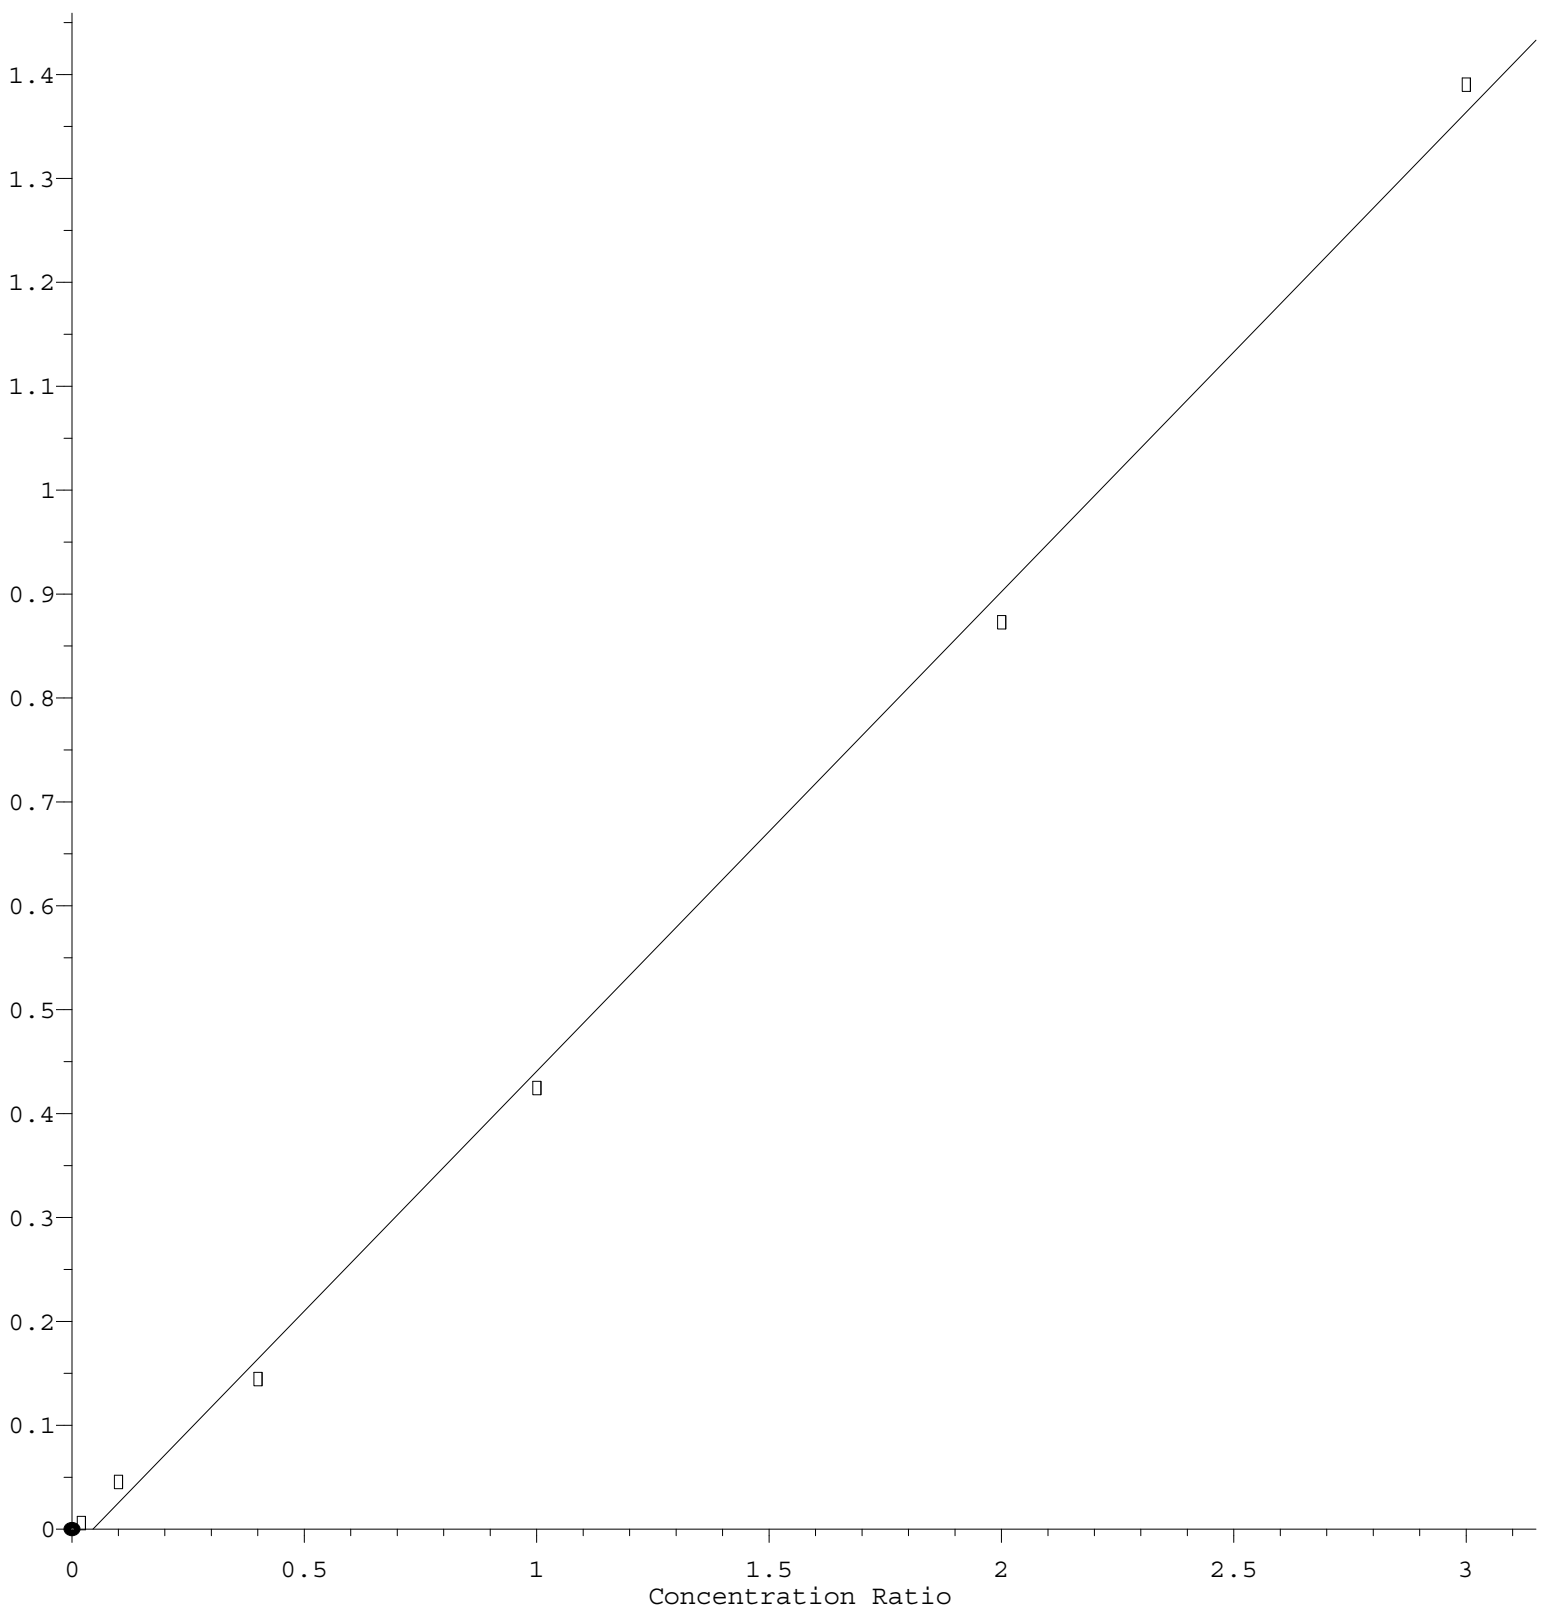


$$\text{Response} = 4.615\text{e-}001 * \text{Amt} - 2.100\text{e-}002$$

Coef of Det (r^2) = 0.998078 Curve Fit: Linear

Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M

Calibration Table Last Updated: Tue Mar 02 14:05:08 2021


1,4-Dioxane

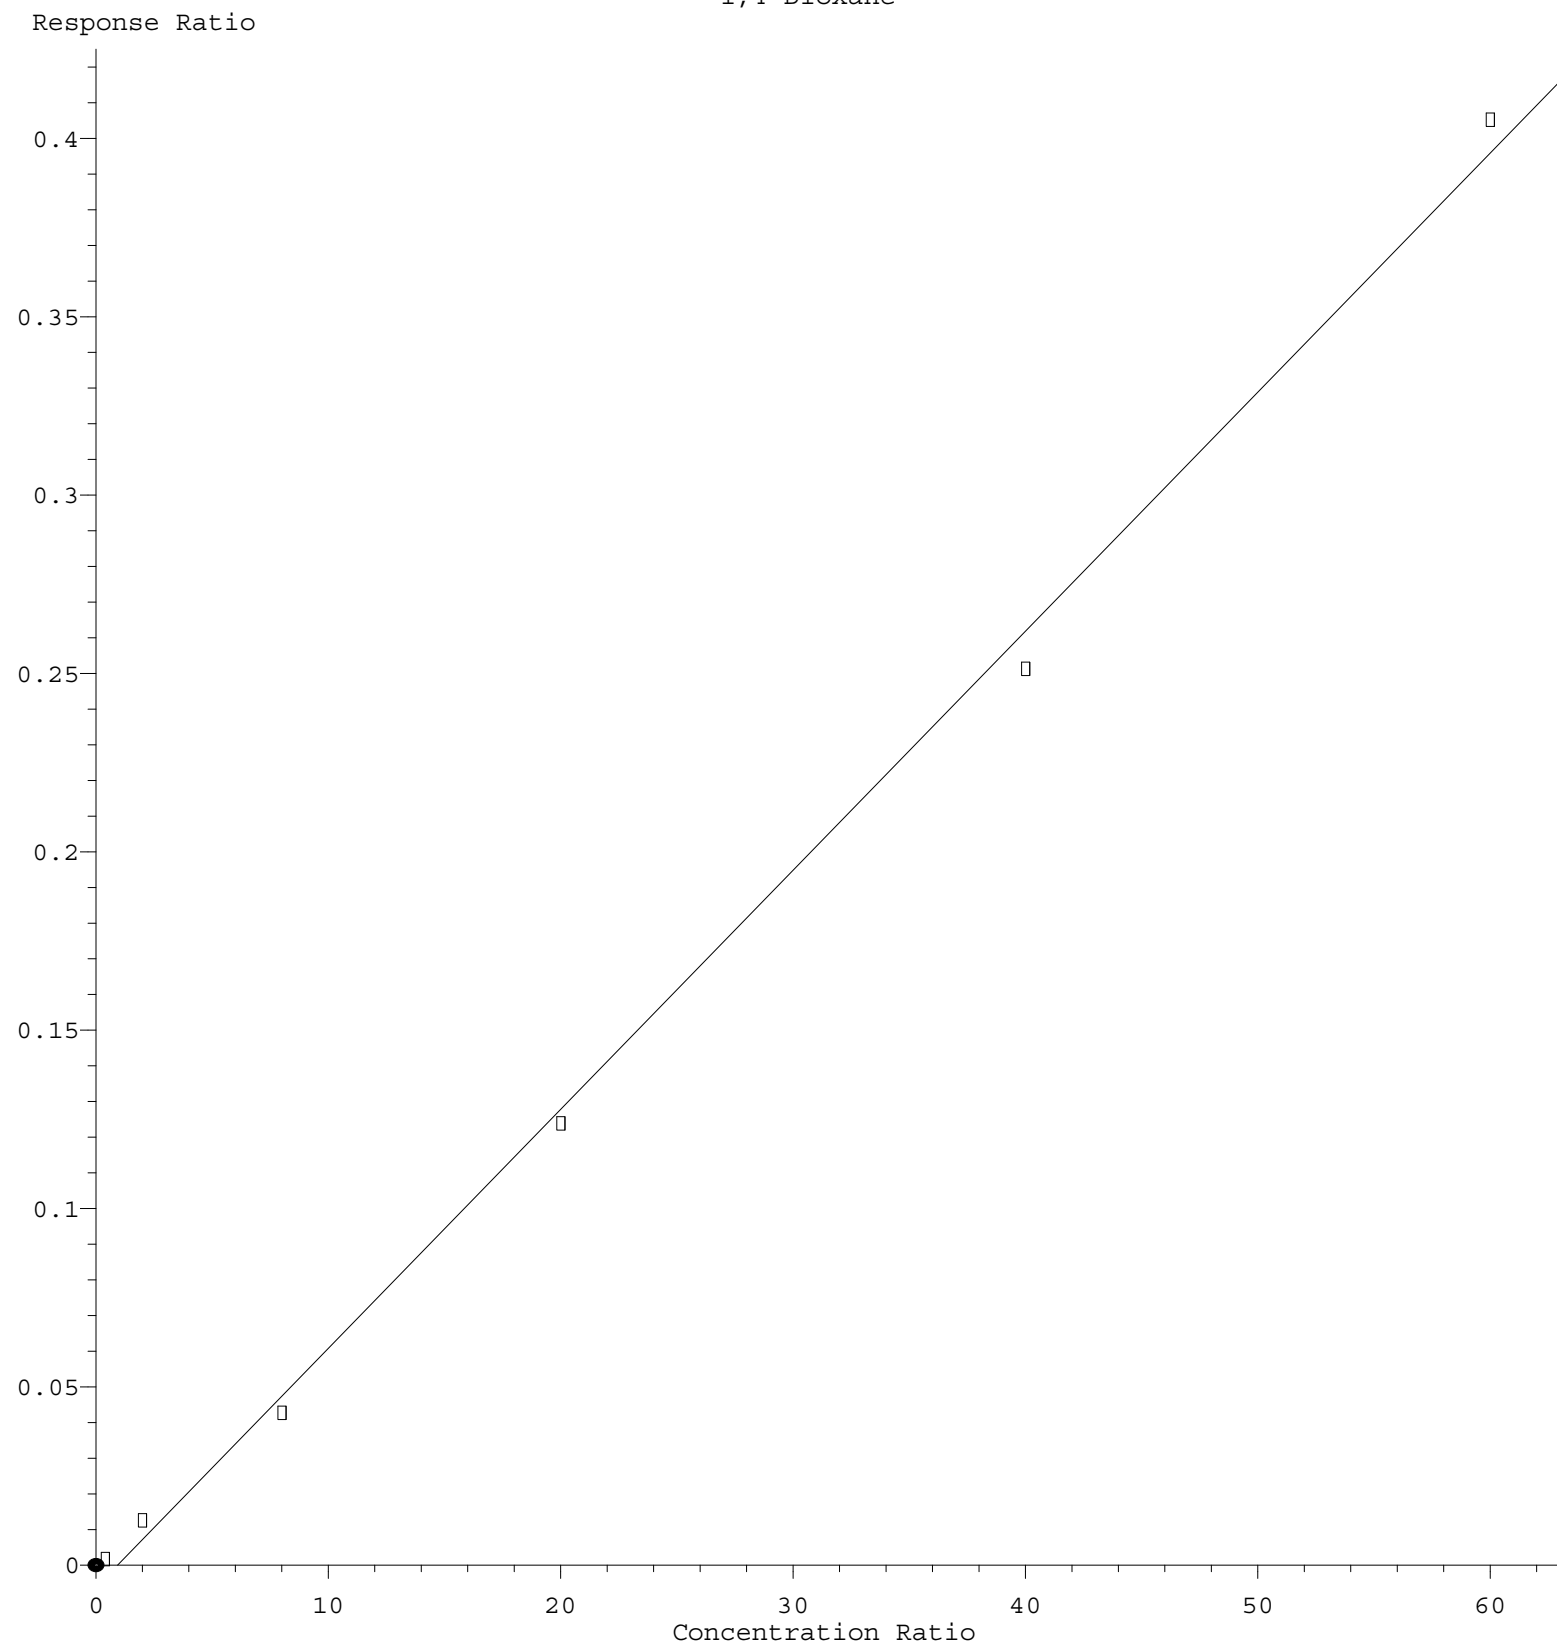

Response = $6.708 \times 10^{-3} \times \text{Amt} - 6.228 \times 10^{-3}$
 Coef of Det (r^2) = 0.997705 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M
 Calibration Table Last Updated: Tue Mar 02 14:05:08 2021


N-amyl acetate

Response Ratio

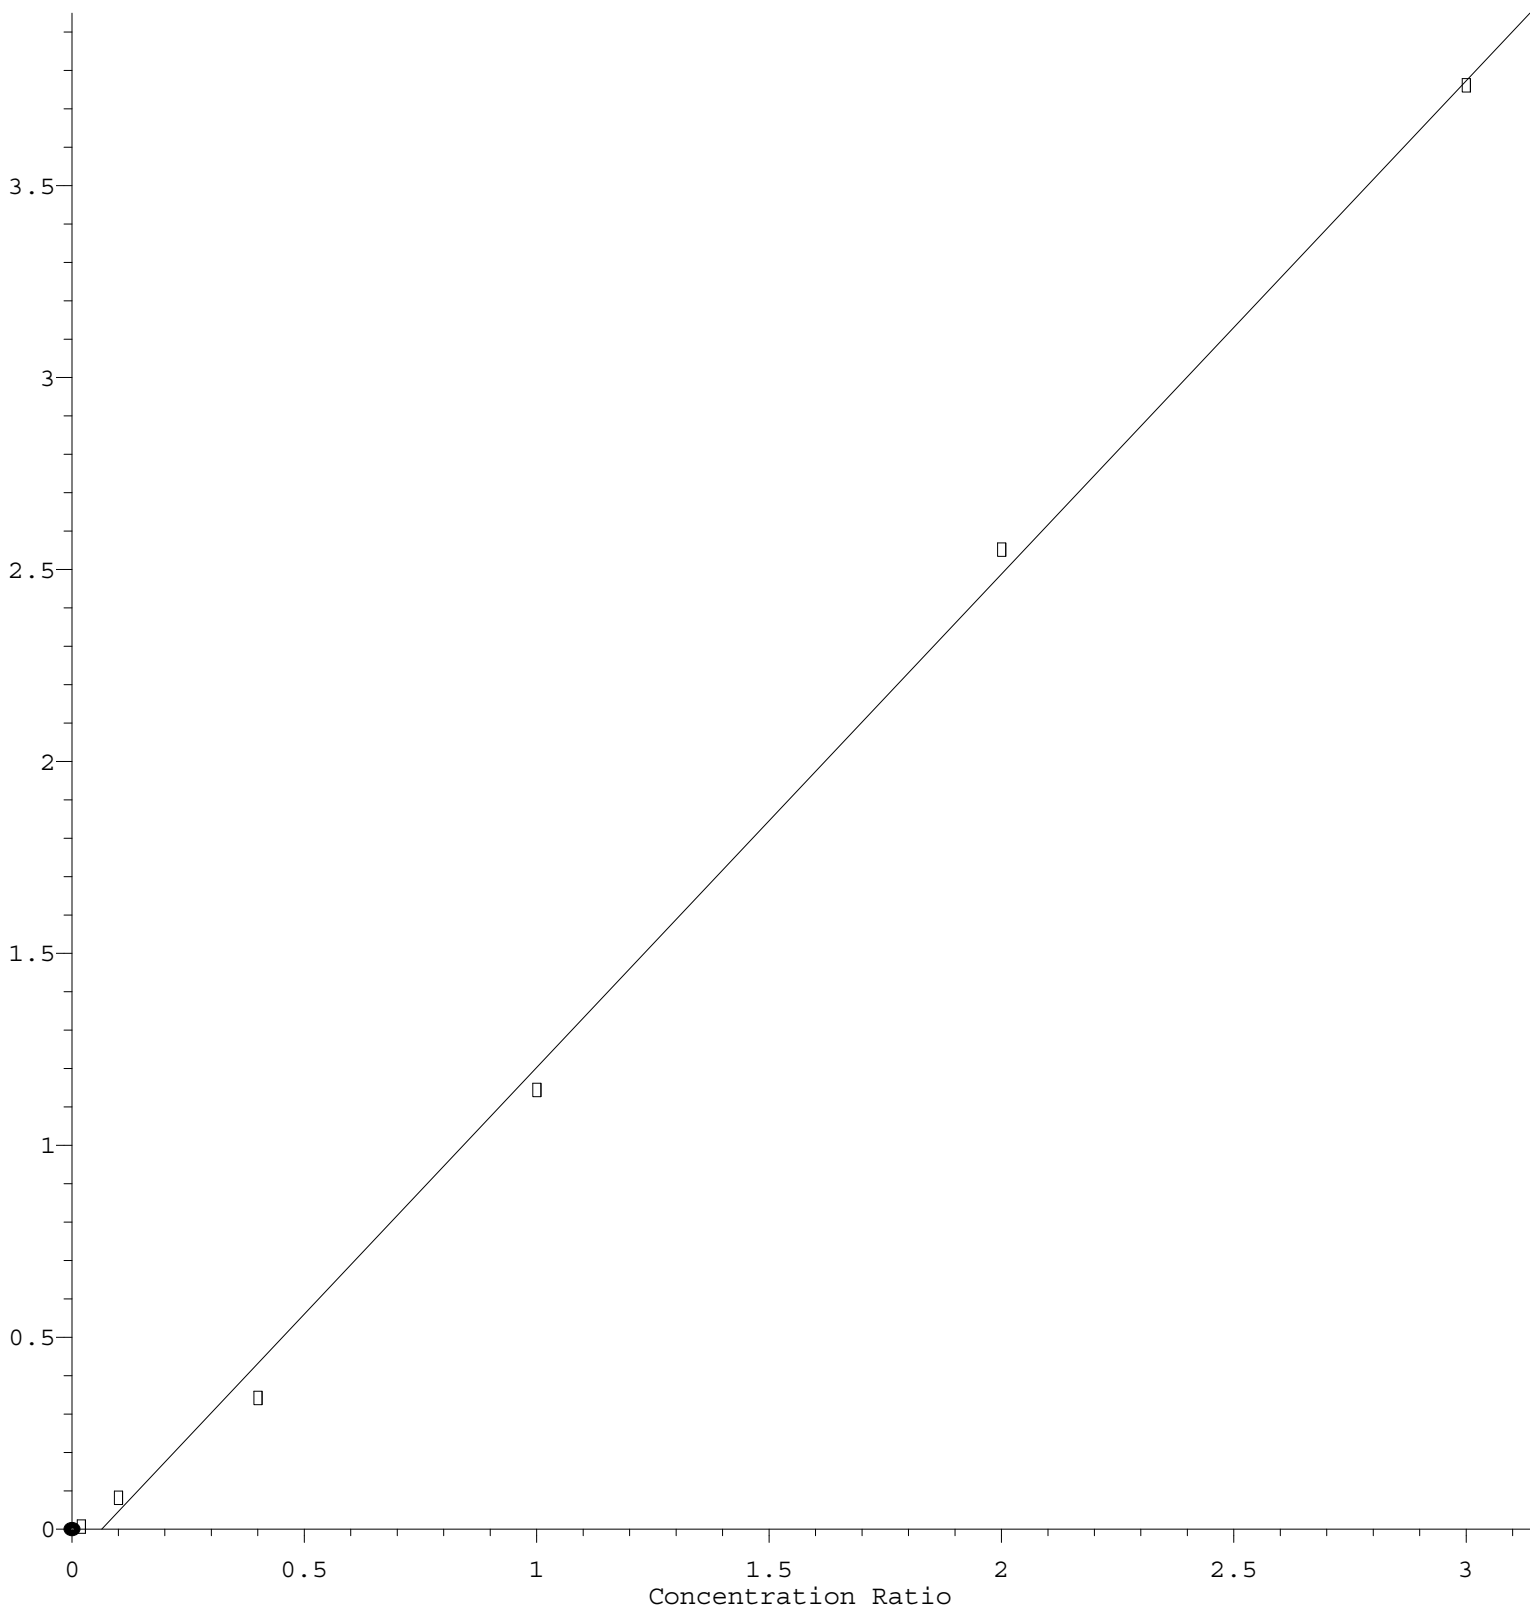

Response = 1.285e+000 * Amt - 8.207e-002
 Coef of Det (r^2) = 0.998209 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M
 Calibration Table Last Updated: Tue Mar 02 14:05:08 2021

1,2-Dibromo-3-Chloropropane

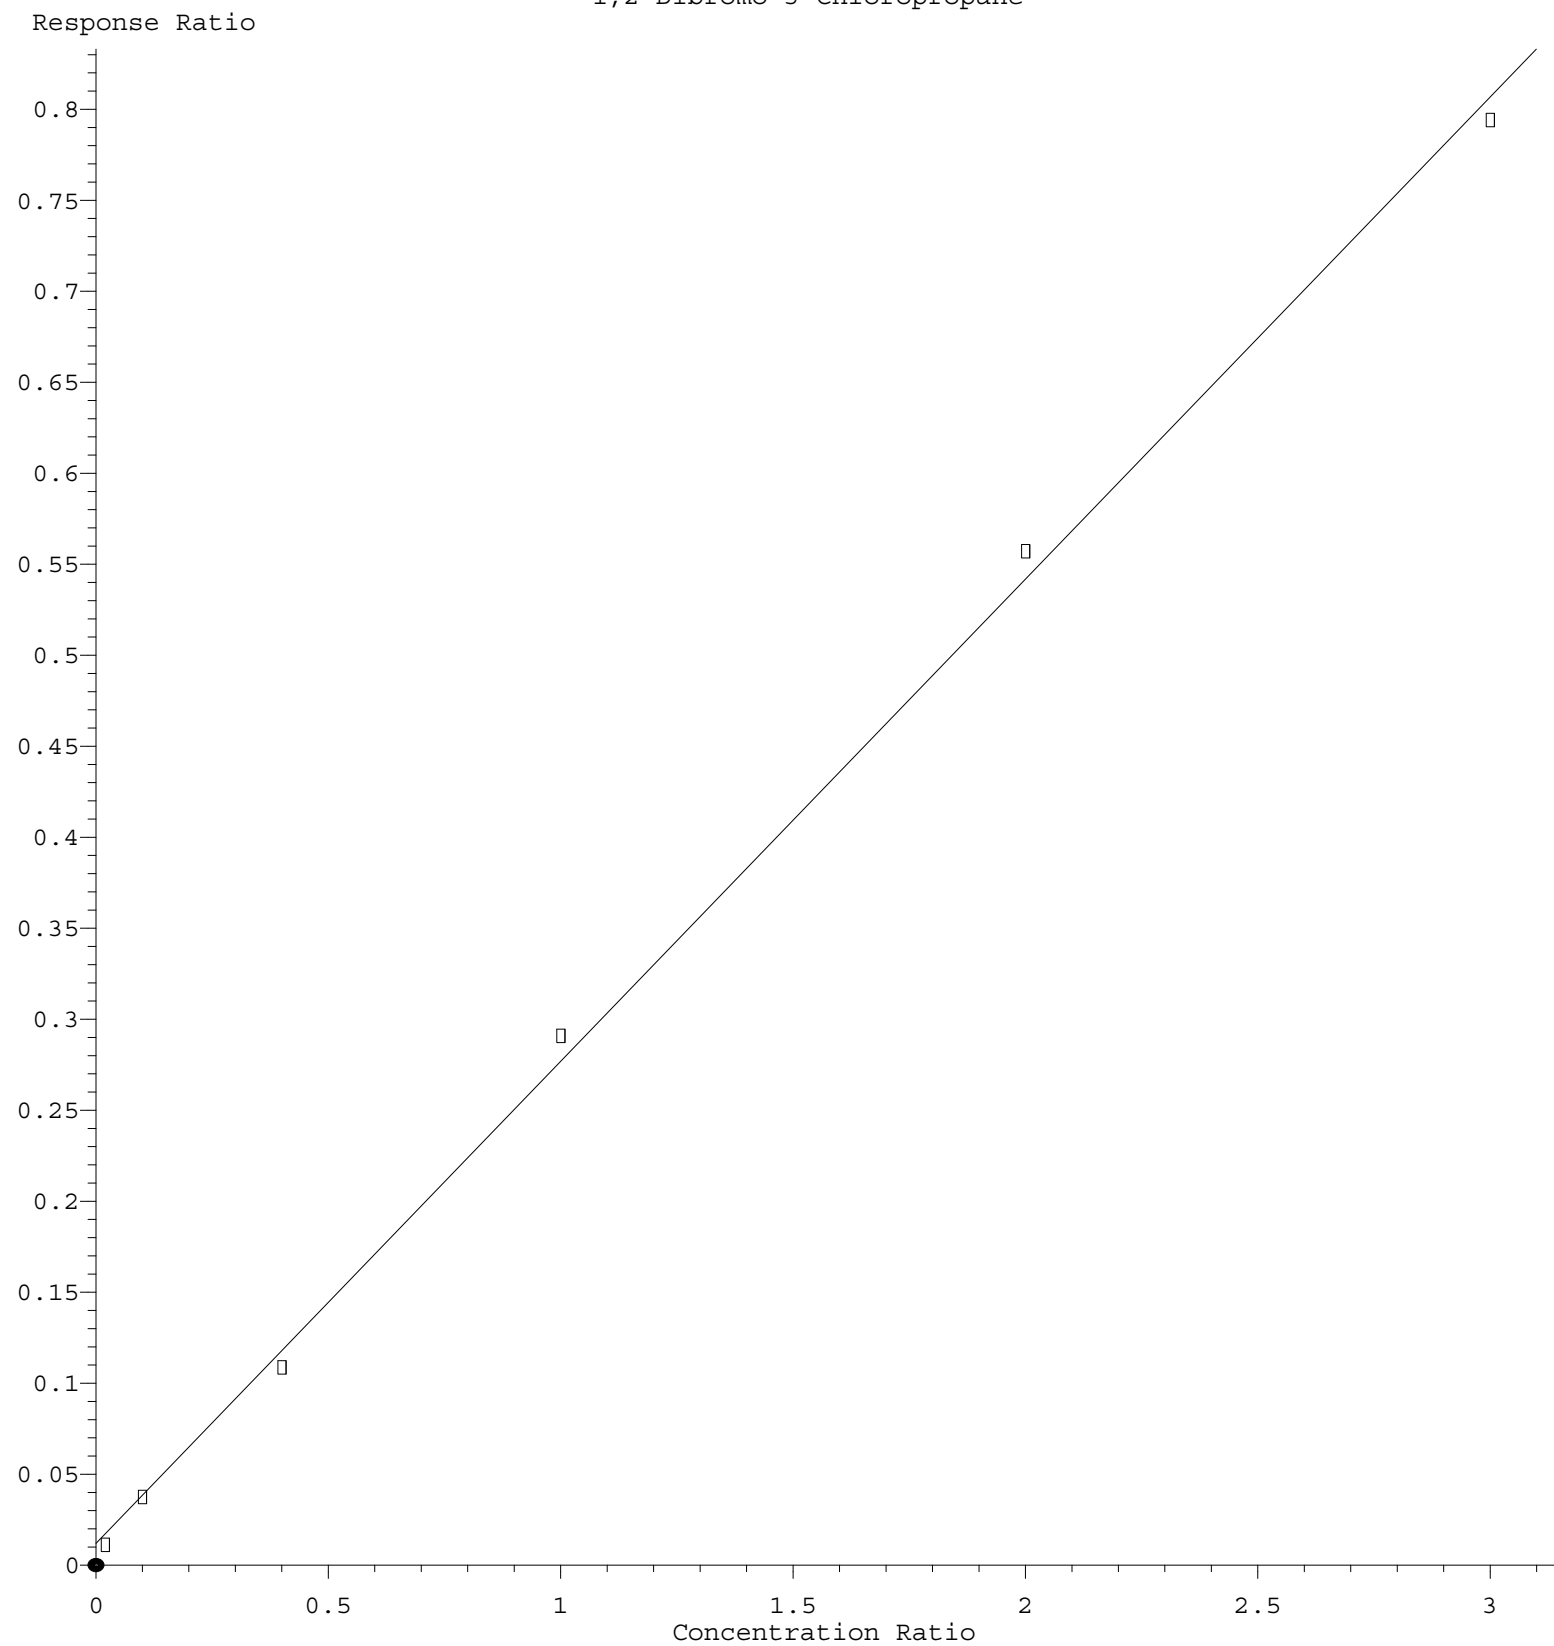

$\text{Response} = 2.652\text{e-}001 * \text{Amt} + 1.164\text{e-}002$
 Coef of Det (r^2) = 0.998571 Curve Fit: Linear
 Method Name: Z:\voasrv\HPCHEM1\MSVOA N\methods\82N030221W.M
 Calibration Table Last Updated: Tue Mar 02 14:05:08 2021