


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030221\
 Data File : VN066092.D
 Acq On : 2 Mar 2021 9:23
 Operator : JC/MD
 Sample : BFB
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030221W.M
 Title : SW846 8260
 Last Update : Tue Mar 02 14:05:08 2021

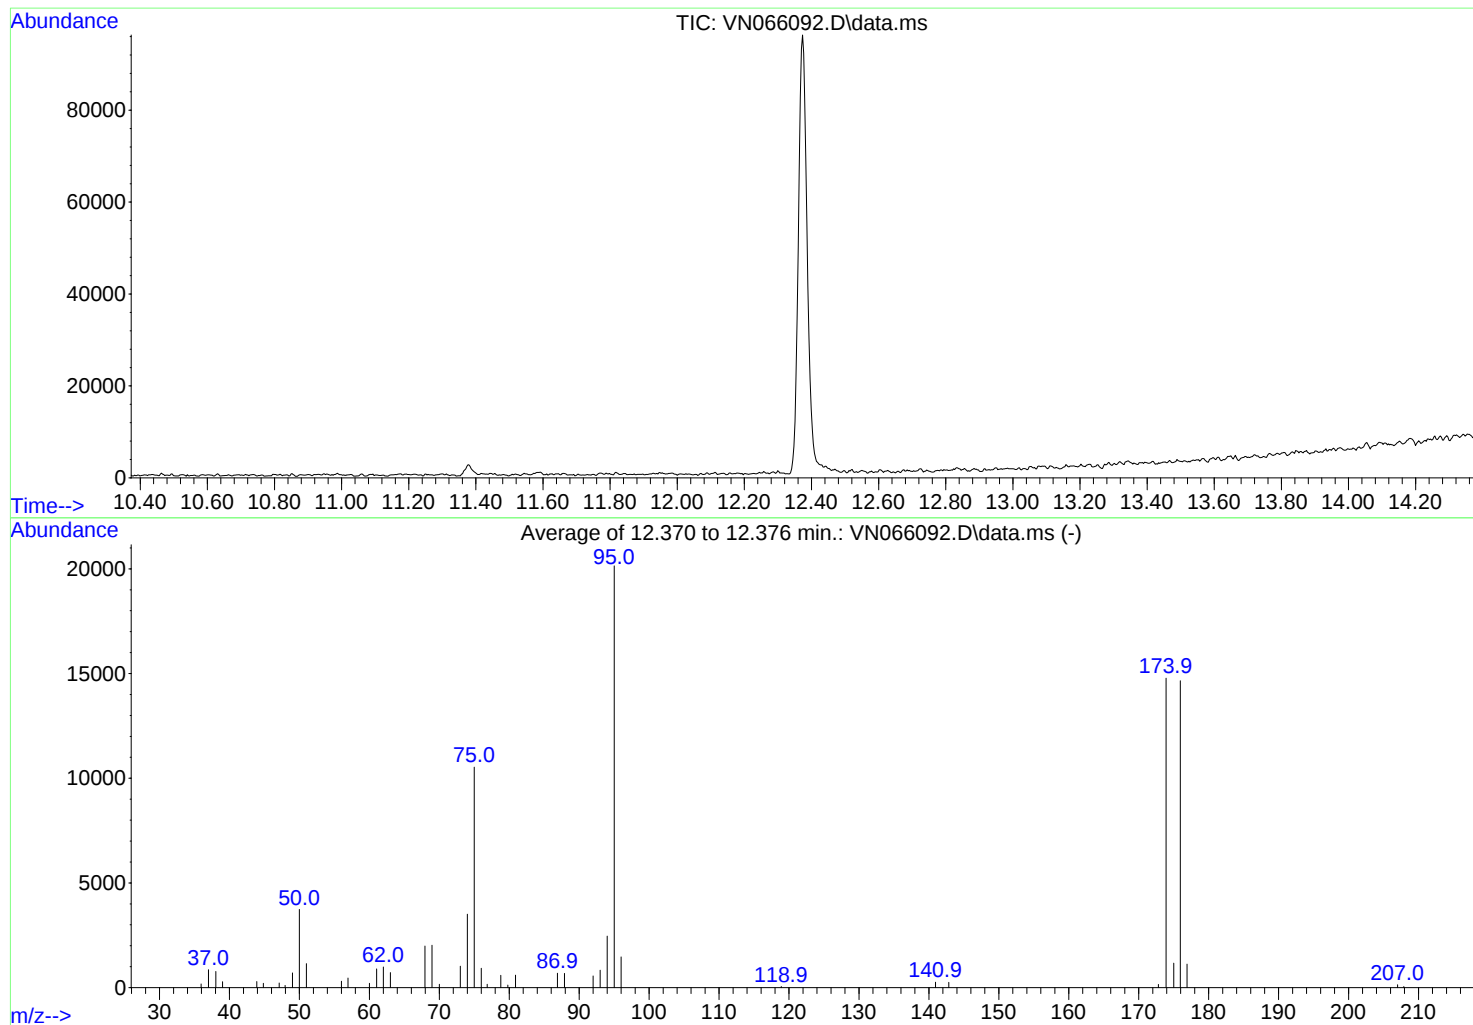

AutoFind: Scans 3306, 3307, 3308; Background Corrected with Scan 3294

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	3735	PASS
75	95	30	60	52.3	10529	PASS
95	95	100	100	100.0	20144	PASS
96	95	5	9	7.3	1471	PASS
173	174	0.00	2	1.0	152	PASS
174	95	50	100	73.4	14781	PASS
175	174	5	9	7.9	1166	PASS
176	174	95	101	99.1	14653	PASS
177	176	5	9	7.6	1120	PASS