


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030222\
Data File : VN071133.D
Acq On : 02 Mar 2022 09:44
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021522W.M
Title : SW846 8260
Last Update : Mon Feb 21 07:57:15 2022

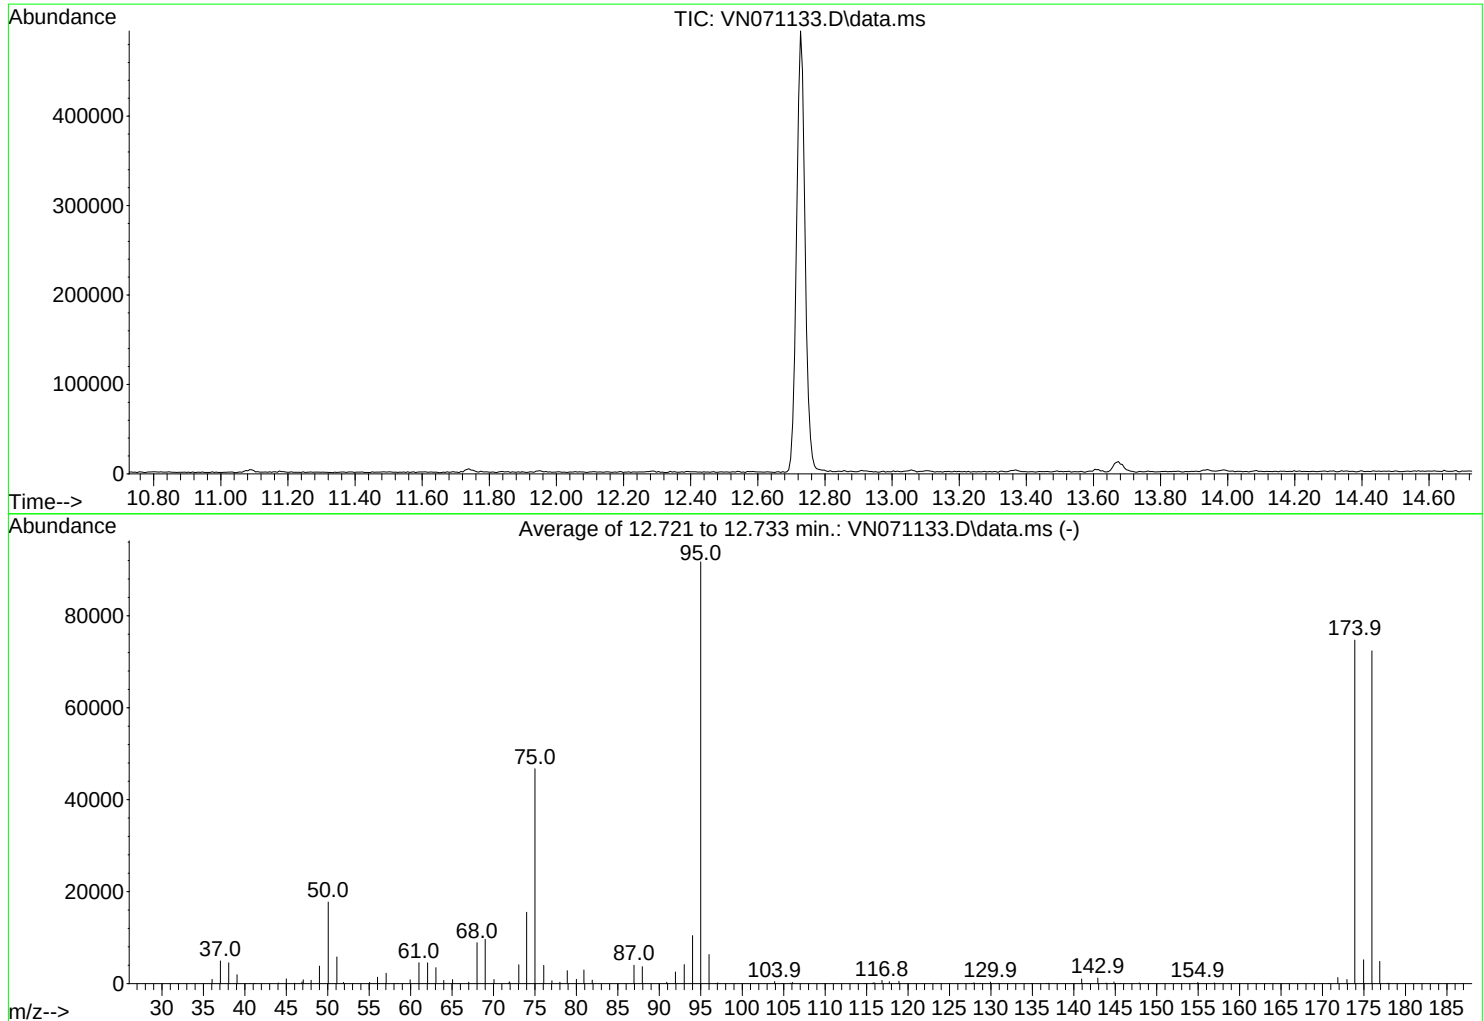

AutoFind: Scans 1825, 1826, 1827; Background Corrected with Scan 1817

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.4	17755	PASS
75	95	30	60	50.9	46725	PASS
95	95	100	100	100.0	91728	PASS
96	95	5	9	6.9	6345	PASS
173	174	0.00	2	1.2	922	PASS
174	95	50	100	81.5	74720	PASS
175	174	5	9	6.9	5184	PASS
176	174	95	101	96.9	72373	PASS
177	176	5	9	6.7	4854	PASS