

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030321\
 Data File : VN066126.D
 Acq On : 3 Mar 2021 16:08
 Operator : JC/MD
 Sample : M1507-07
 Misc : 5.00mL/MSVOA_N/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-30771-73-77

Quant Time: Mar 04 02:16:46 2021
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030221W.M
 Quant Title : SW846 8260
 QLast Update : Tue Mar 02 14:05:08 2021
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)

Internal Standards						
1) Pentafluorobenzene	7.624	168	64403	50.00	ug/l	0.00
34) 1,4-Difluorobenzene	8.547	114	119036	50.00	ug/l	0.00
63) Chlorobenzene-d5	11.376	117	118613	50.00	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.312	152	48847	50.00	ug/l	0.00

System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	7.987	65	48032	49.01	ug/l	0.00
Spiked Amount	50.000	Range	61 - 141	Recovery	=	98.02%
35) Dibromofluoromethane	7.553	113	37706	50.02	ug/l	0.00
Spiked Amount	50.000	Range	69 - 133	Recovery	=	100.04%
50) Toluene-d8	10.055	98	145872	49.68	ug/l	0.00
Spiked Amount	50.000	Range	65 - 126	Recovery	=	99.36%
62) 4-Bromofluorobenzene	12.373	95	60831	53.80	ug/l	0.00
Spiked Amount	50.000	Range	58 - 135	Recovery	=	107.60%


Target Compounds						Qvalue
3) Chloromethane	2.052	50	733	0.96	ug/l #	86
11) Tert butyl alcohol	4.727	59	2298	16.98	ug/l #	73
13) Acrolein	3.586	56	782	10.70	ug/l #	67
14) Allyl chloride	4.032	41	1200	1.18	ug/l #	73
16) Acetone	3.788	43	16370	55.88	ug/l	94
18) Methyl Acetate	4.280	43	872	1.39	ug/l #	65
20) Methylene Chloride	4.524	84	287	0.37	ug/l #	60
25) 2-Butanone	6.791	43	6535	16.82	ug/l	99
31) Cyclohexane	7.621	56	1669	1.42	ug/l #	48
36) 1,1-Dichloropropene	7.627	75	4681	4.18	ug/l #	43
37) Ethyl Acetate	6.791	43	6535	7.50	ug/l #	68
38) Carbon Tetrachloride	7.624	117	6309	4.90	ug/l #	12
40) Benzene	8.000	78	45571	13.79	ug/l	97
43) Isopropyl Acetate	7.974	43	649	0.40	ug/l #	1
48) Methyl methacrylate	9.129	41	1020	1.29	ug/l #	22
51) 4-Methyl-2-Pentanone	9.945	43	877	0.98	ug/l #	68
52) Toluene	10.122	92	35059	16.49	ug/l	93
53) t-1,3-Dichloropropene	10.119	75	545	0.38	ug/l #	1
67) Ethyl Benzene	11.479	91	9260	2.08	ug/l	91
68) m/p-Xylenes	11.588	106	15149	8.79	ug/l	93
69) o-Xylene	11.916	106	5958	3.54	ug/l	98
70) Styrene	11.933	104	970	0.37	ug/l #	1
74) N-amyl acetate	12.051	43	60	3.24	ug/l #	42
76) 1,2,3-Trichloropropane	12.373	75	30757	28.52	ug/l #	100
78) n-propylbenzene	12.560	91	982	0.23	ug/l #	75
80) 1,3,5-Trimethylbenzene	12.701	105	2161	0.61	ug/l	92
81) trans-1,4-Dichloro-2-b...	12.373	75	30757	83.91	ug/l #	12
84) 1,2,4-Trimethylbenzene	13.010	105	5058	1.46	ug/l	99
85) sec-Butylbenzene	13.010	105	5058	1.41	ug/l #	56
90) Hexachloroethane	13.900	117	168	0.33	ug/l #	12
92) 1,2-Dibromo-3-Chloropr...	14.251	75	29	Below	Cal #	1
95) Naphthalene	15.100	128	10080	3.70	ug/l #	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030321\
Data File : VN066126.D
Acq On : 3 Mar 2021 16:08
Operator : JC/MD
Sample : M1507-07
Misc : 5.00mL/MSVOA_N/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77

Quant Time: Mar 04 02:16:46 2021
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030221W.M
Quant Title : SW846 8260
QLast Update : Tue Mar 02 14:05:08 2021
Response via : Initial Calibration




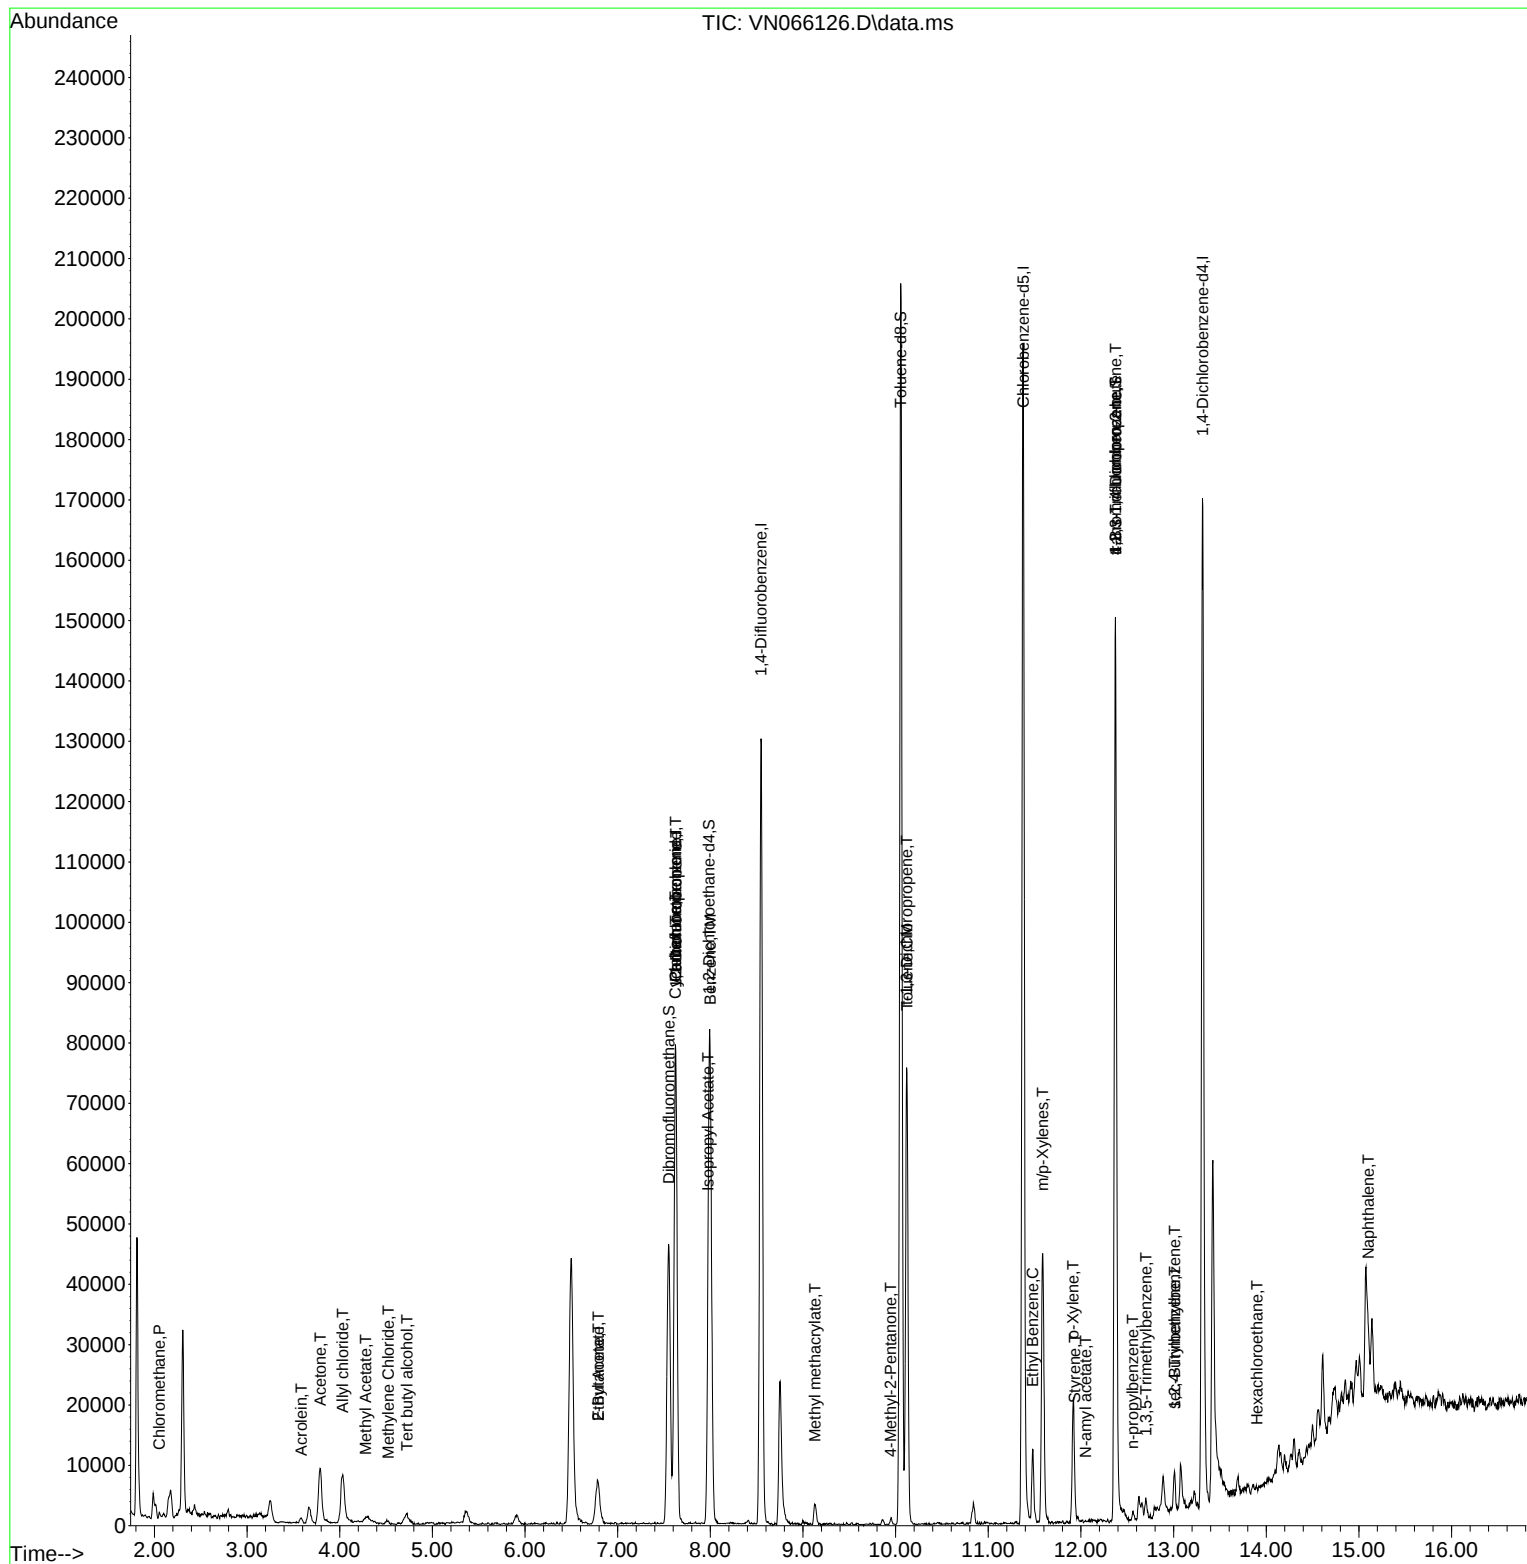




#1
Pentafluorobenzene
Concen: 50.00 ug/l
RT: 7.624 min Scan# 1830
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion:168 Resp: 64403
Ion Ratio Lower Upper
168 100
99 61.0 42.6 63.8

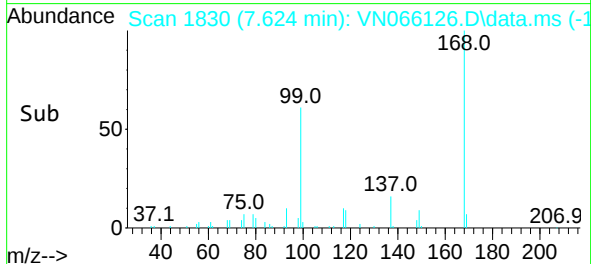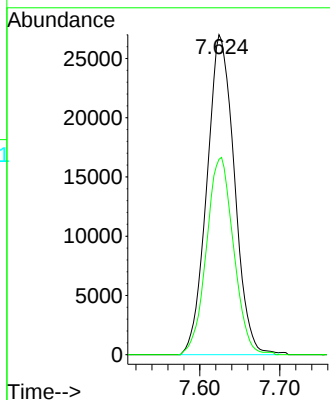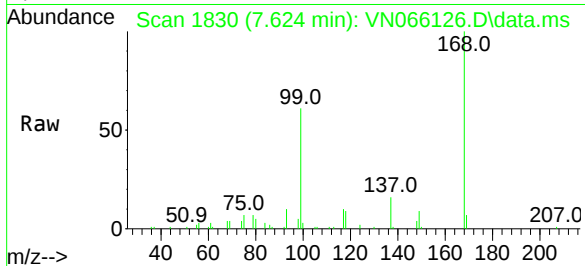

#3
Chloromethane
Concen: 0.96 ug/l
RT: 2.052 min Scan# 97
Delta R.T. -0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 50 Resp: 733
Ion Ratio Lower Upper
50 100
52 40.4 25.8 38.8#

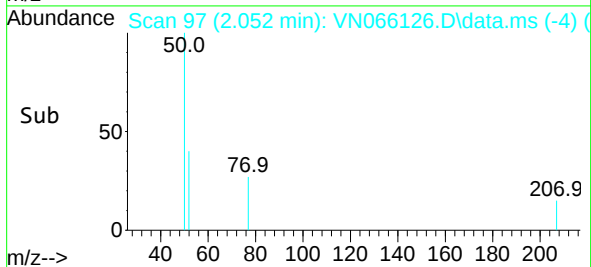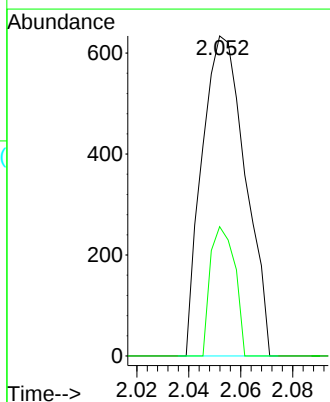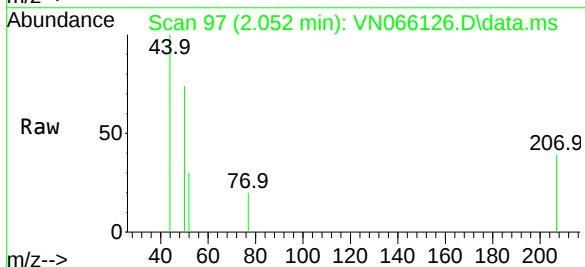







#11

Tert butyl alcohol
Concen: 16.98 ug/l
RT: 4.727 min Scan# 929
Delta R.T. -0.006 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77




Tgt Ion: 59 Resp: 2298
Ion Ratio Lower Upper
59 100
57 0.0 8.0 12.0#

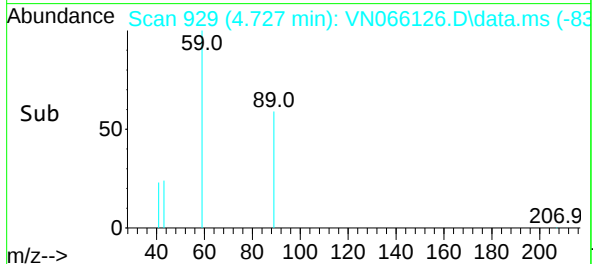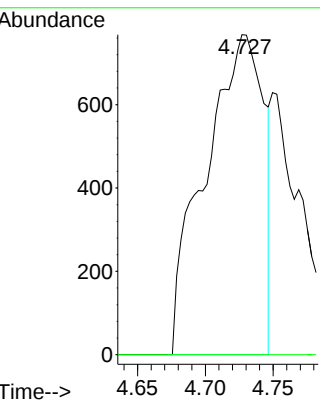


#13

Acrolein
Concen: 10.70 ug/l
RT: 3.586 min Scan# 574
Delta R.T. 0.010 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08


Tgt Ion: 56 Resp: 782
Ion Ratio Lower Upper
56 100
55 43.2 56.0 84.0#

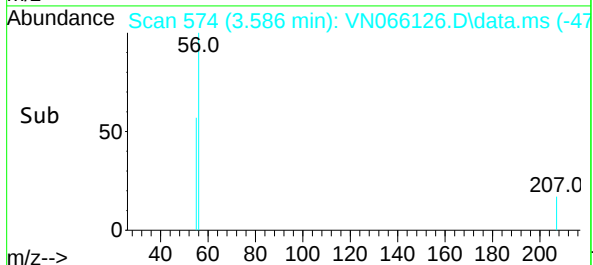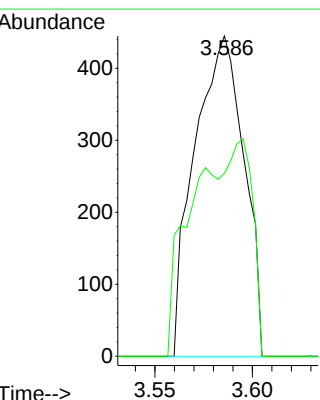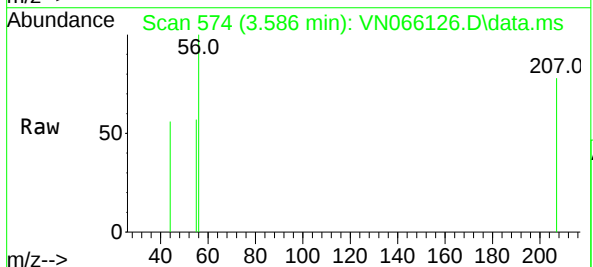






#14
 Allyl chloride
 Concen: 1.18 ug/l
 RT: 4.032 min Scan# 713
 Delta R.T. -0.253 min
 Lab File: VN066126.D
 Acq: 3 Mar 2021 16:08

Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-30771-73-77



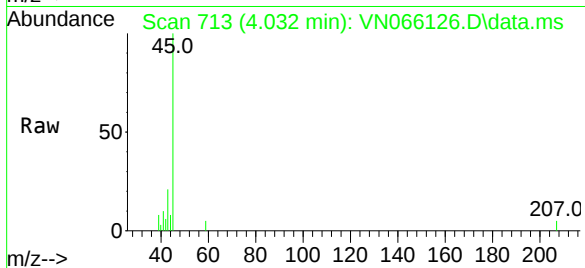



Tgt Ion: 41 Resp: 1200
 Ion Ratio Lower Upper
 41 100
 39 79.5 53.0 79.4#
 76 8.3 28.9 43.3#

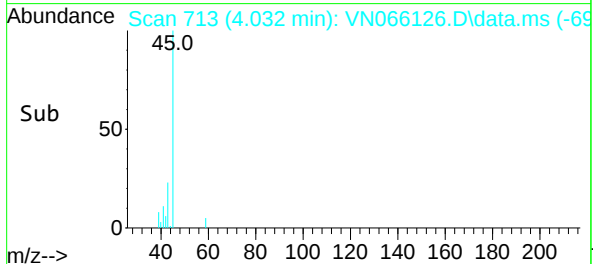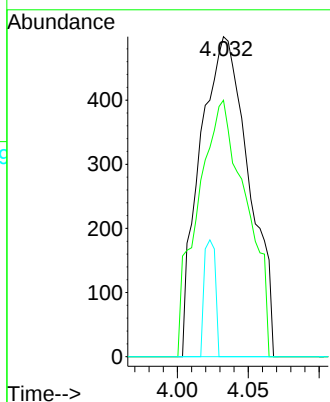

#16
 Acetone
 Concen: 55.88 ug/l
 RT: 3.788 min Scan# 637
 Delta R.T. 0.003 min
 Lab File: VN066126.D
 Acq: 3 Mar 2021 16:08

Tgt Ion: 43 Resp: 16370
 Ion Ratio Lower Upper
 43 100
 58 30.4 27.0 40.6

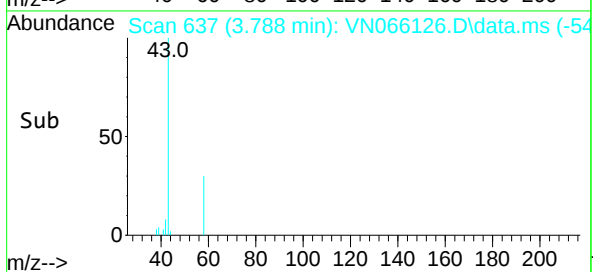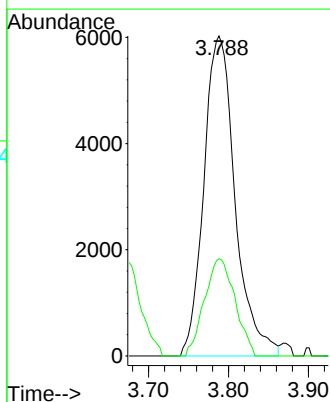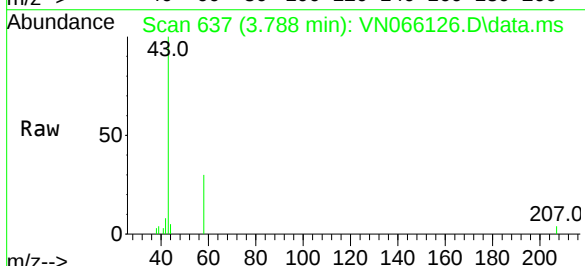



#18

Methyl Acetate

Concen: 1.39 ug/l

RT: 4.280 min Scan# 790

Delta R.T. -0.006 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Instrument :

MSVOA_N

ClientSampleId :





COMP-30771-73-77

Tgt Ion: 43 Resp: 872

Ion Ratio Lower Upper

43 100

74 7.0 19.5 29.3#

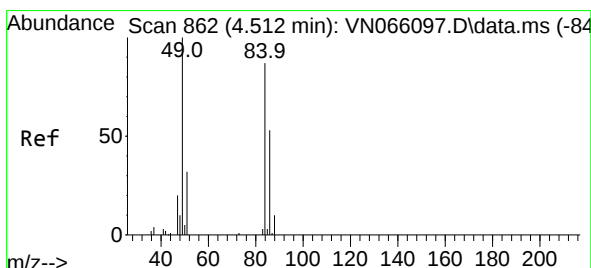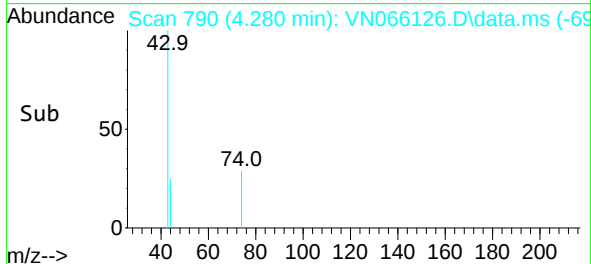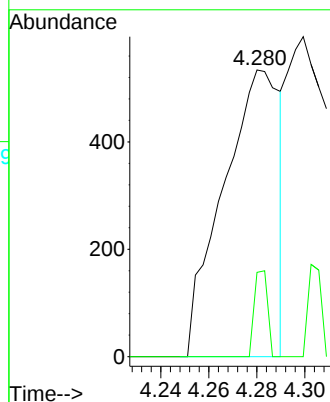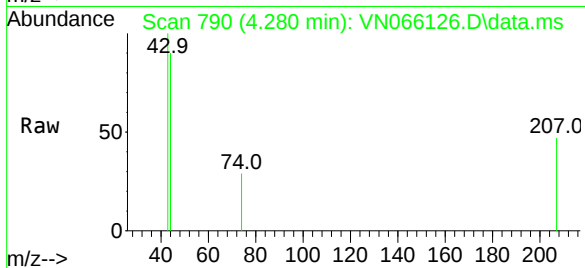

#20

Methylene Chloride

Concen: 0.37 ug/l

RT: 4.524 min Scan# 866

Delta R.T. 0.012 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Tgt Ion: 84 Resp: 287




Ion Ratio Lower Upper


84 100

49 106.5 94.6 141.8

51 0.0 29.9 44.9#

86 0.0 51.4 77.2#


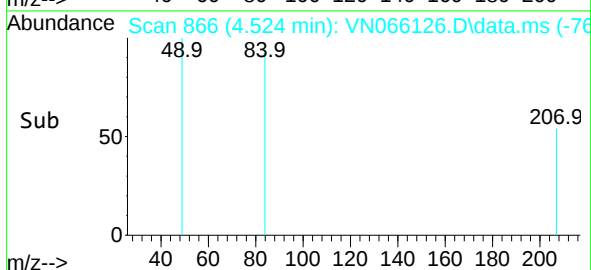
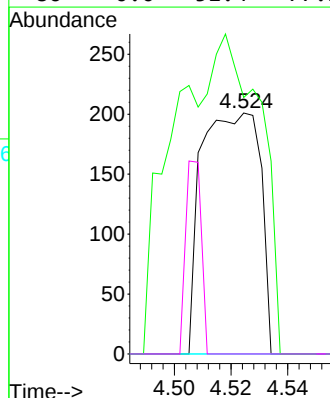
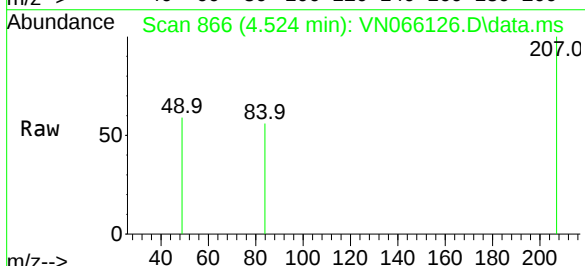




#25
2-Butanone
Concen: 16.82 ug/l
RT: 6.791 min Scan# 1571
Delta R.T. 0.003 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 43 Resp: 6535
Ion Ratio Lower Upper
43 100
72 29.5 23.1 34.7



#31
Cyclohexane
Concen: 1.42 ug/l
RT: 7.621 min Scan# 1829
Delta R.T. 0.007 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 56 Resp: 1669
Ion Ratio Lower Upper
56 100
69 124.7 26.6 39.8#
84 78.6 70.4 105.6


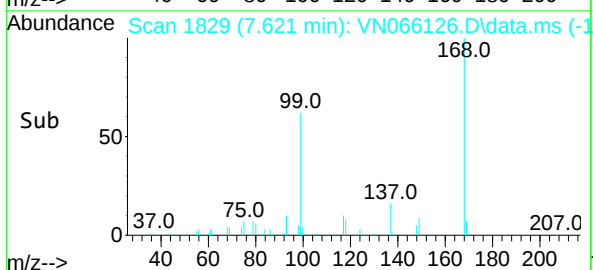
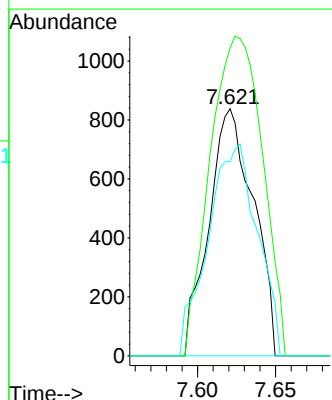





#33
1,2-Dichloroethane-d4
Concen: 49.01 ug/l
RT: 7.987 min Scan# 1943
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 65 Resp: 48032
Ion Ratio Lower Upper
65 100
67 50.5 0.0 107.2

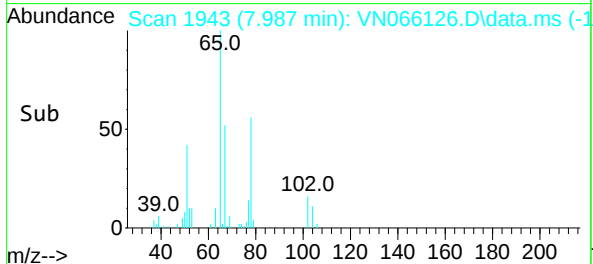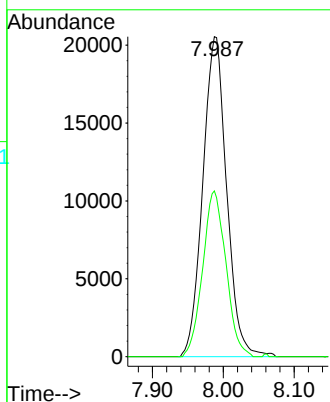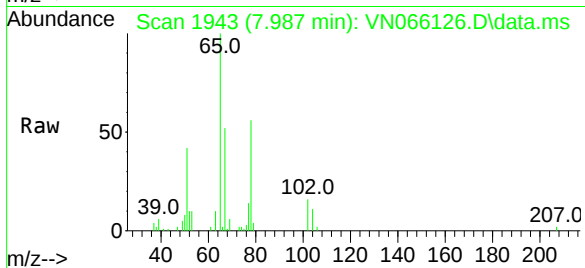

#34
1,4-Difluorobenzene
Concen: 50.00 ug/l
RT: 8.547 min Scan# 2117
Delta R.T. -0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 114 Resp: 119036
Ion Ratio Lower Upper
114 100
63 21.0 0.0 38.6
88 16.8 0.0 30.6

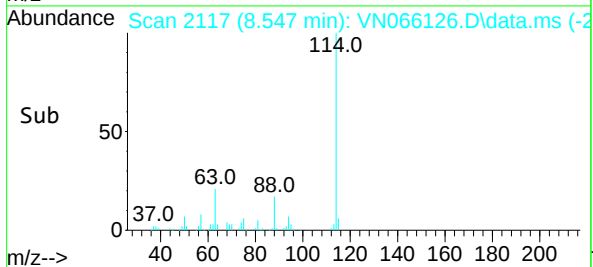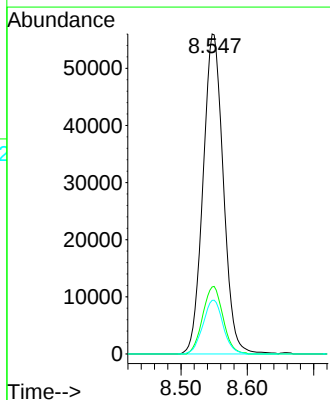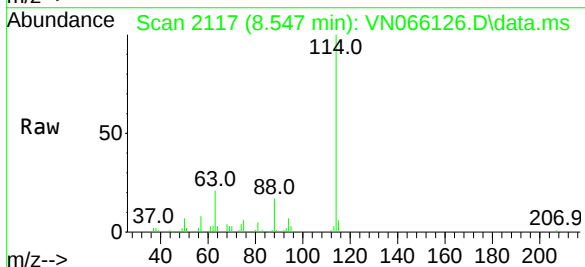



#35

Dibromofluoromethane

Concen: 50.02 ug/l

RT: 7.553 min Scan# 1808





Delta R.T. 0.003 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Tgt Ion:	113	Resp:	37706
Ion	Ratio	Lower	Upper
113	100		
111	101.0	82.2	123.2
192	18.1	15.4	23.0

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77

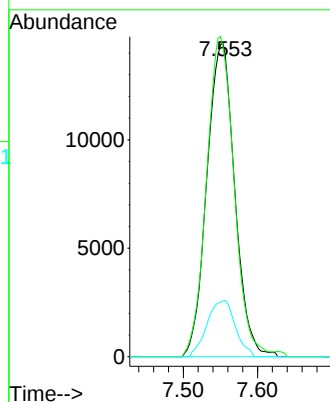

#36

1,1-Dichloropropene

Concen: 4.18 ug/l




RT: 7.627 min Scan# 1831


Delta R.T. -0.126 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Tgt Ion:	75	Resp:	4681
Ion	Ratio	Lower	Upper
75	100		
110	2.0	18.2	54.6#
77	0.0	24.9	37.3#

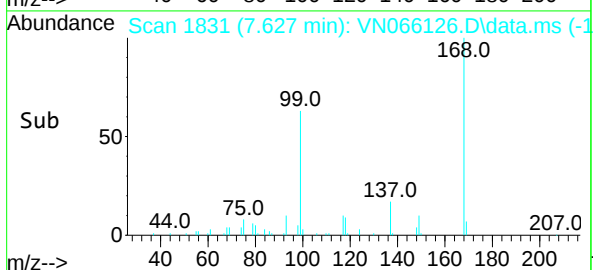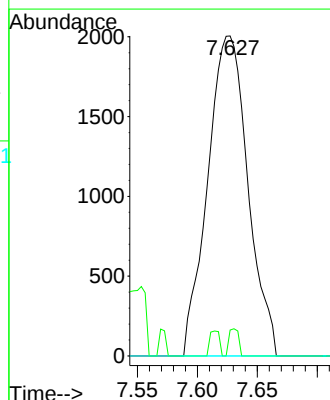



#37

Ethyl Acetate

Concen: 7.50 ug/l

RT: 6.791 min Scan# 1571





Delta R.T. -0.090 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77

Tgt Ion:	43	Resp:	6535
Ion	Ratio	Lower	Upper
43	100		
61	0.0	11.6	17.4#
70	0.0	8.6	13.0#

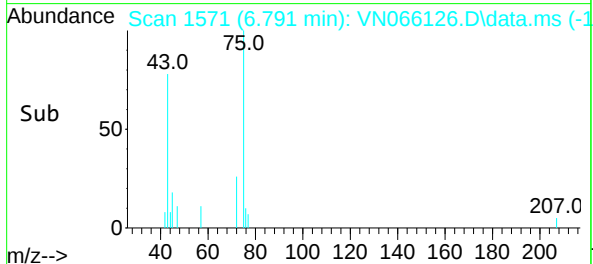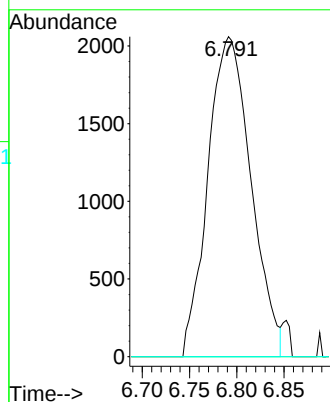

#38

Carbon Tetrachloride

Concen: 4.90 ug/l




RT: 7.624 min Scan# 1830


Delta R.T. -0.109 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Tgt Ion:	117	Resp:	6309
Ion	Ratio	Lower	Upper
117	100		
119	0.0	76.0	114.0#
121	0.0	24.5	36.7#


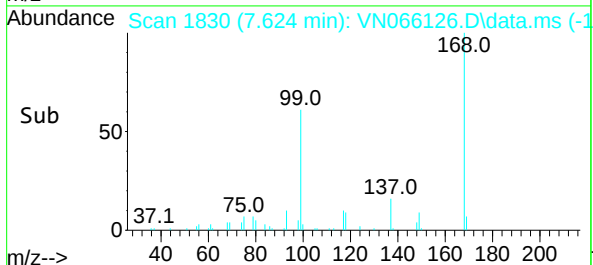
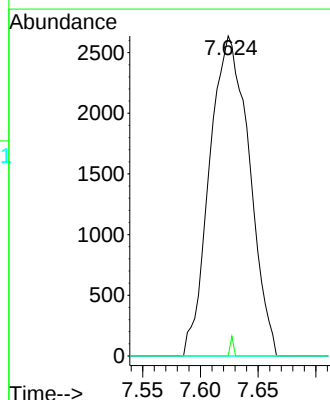
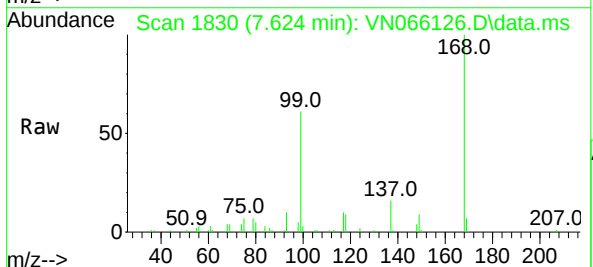




#40
Benzene
Concen: 13.79 ug/l
RT: 8.000 min Scan# 1947
Delta R.T. -0.003 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 78 Resp: 45571
Ion Ratio Lower Upper
78 100
77 25.3 19.0 28.4

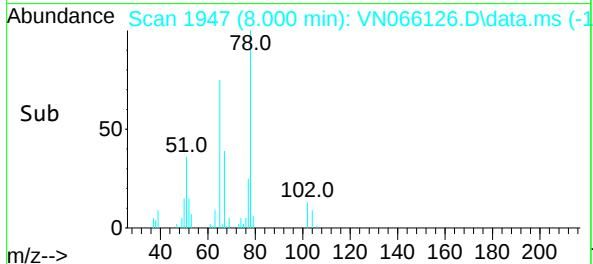

#43
Isopropyl Acetate
Concen: 0.40 ug/l
RT: 7.974 min Scan# 1939
Delta R.T. -0.148 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 43 Resp: 649
Ion Ratio Lower Upper
43 100
61 160.6 22.5 33.7#
87 0.0 11.1 16.7#

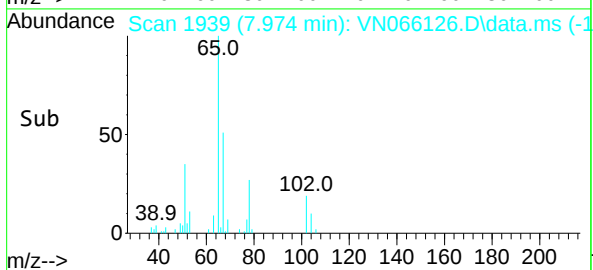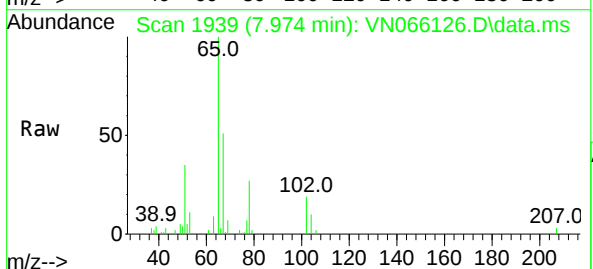



#48

Methyl methacrylate

Concen: 1.29 ug/l

RT: 9.129 min Scan# 2298

Delta R.T. -0.032 min

Lab File: VN066126.D

Acq: 3 Mar 2021 16:08

Tgt Ion: 41 Resp: 1020

Ion Ratio Lower Upper

41 100

69 0.0 75.9 113.9#





39 23.9 46.6 69.8#

Instrument :

MSVOA_N

ClientSampleId :

COMP-30771-73-77

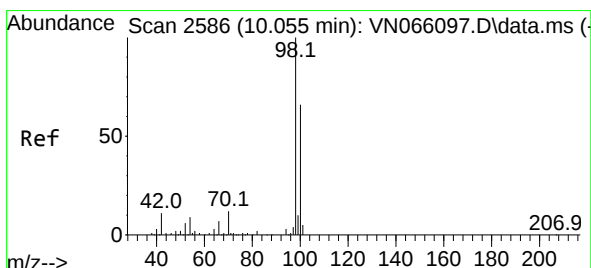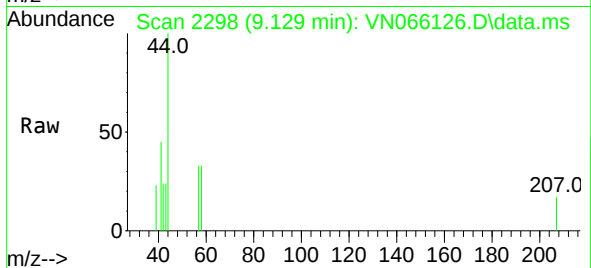

#50

Toluene-d8

Concen: 49.68 ug/l

RT: 10.055 min Scan# 2586

Delta R.T. -0.000 min

Lab File: VN066126.D




Acq: 3 Mar 2021 16:08


Tgt Ion: 98 Resp: 145872

Ion Ratio Lower Upper

98 100

100 64.8 50.5 75.7


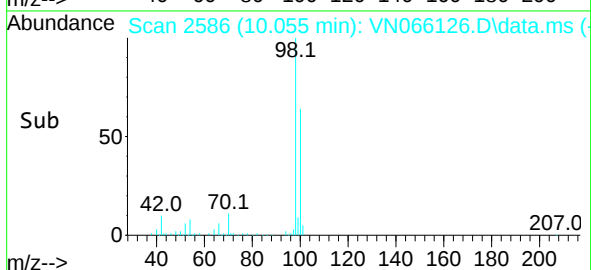
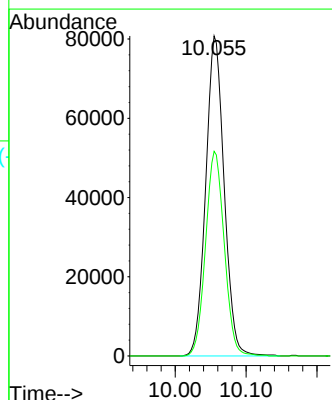





#51
4-Methyl-2-Pentanone
Concen: 0.98 ug/l
RT: 9.945 min Scan# 2552
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 43 Resp: 877
Ion Ratio Lower Upper
43 100
58 20.5 32.5 48.7#

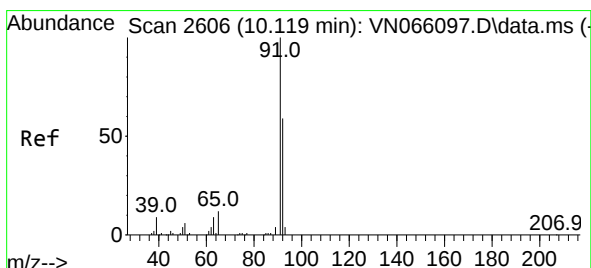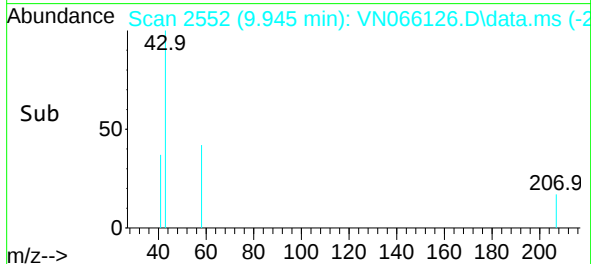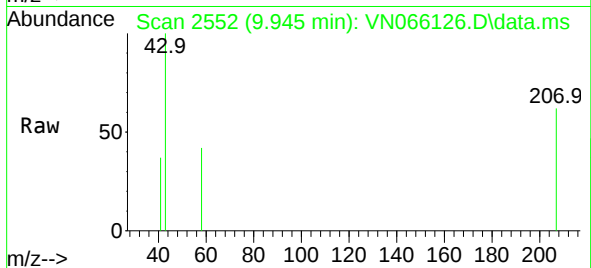

#52
Toluene
Concen: 16.49 ug/l
RT: 10.122 min Scan# 2607
Delta R.T. 0.003 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 92 Resp: 35059
Ion Ratio Lower Upper
92 100
91 165.6 140.7 211.1


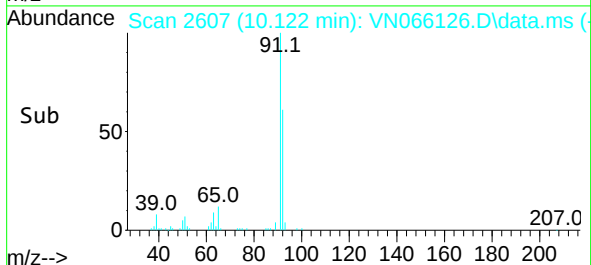
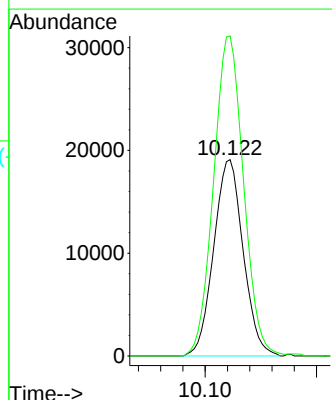
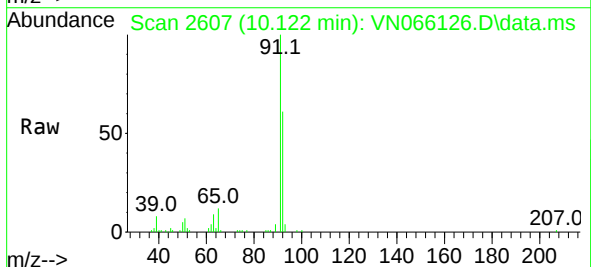




#53
t-1,3-Dichloropropene
Concen: 0.38 ug/l
RT: 10.119 min Scan# 2606
Delta R.T. -0.228 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 75 Resp: 545
Ion Ratio Lower Upper
75 100
77 134.3 26.2 39.4#

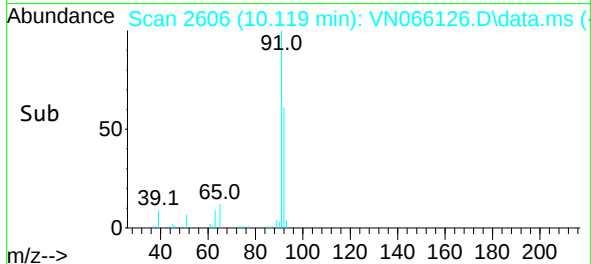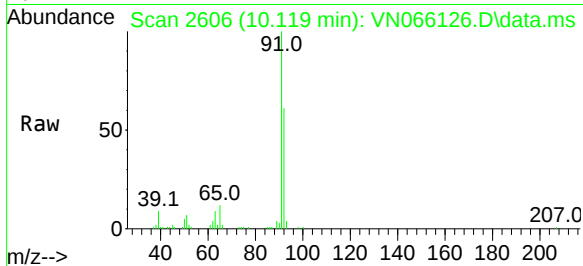

#62
4-Bromofluorobenzene
Concen: 53.80 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.003 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 95 Resp: 60831
Ion Ratio Lower Upper
95 100
174 71.4 0.0 169.0
176 69.7 0.0 162.4


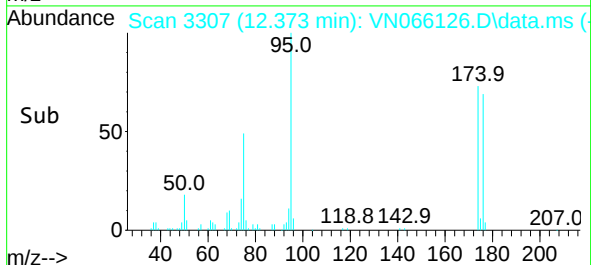
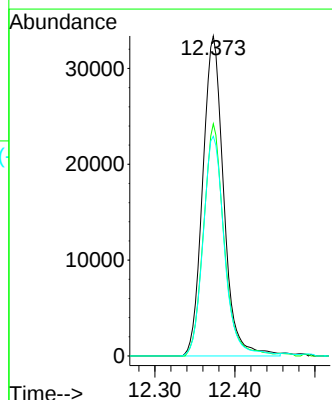
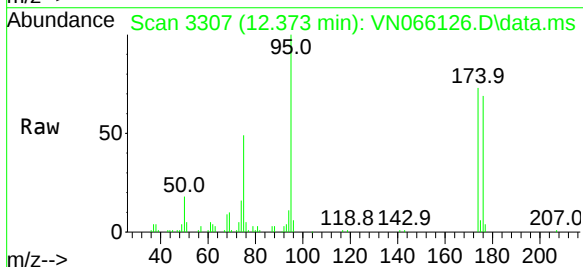


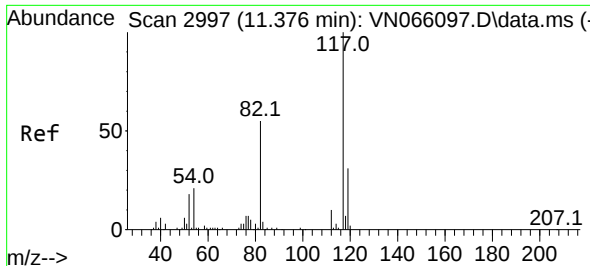

#63
Chlorobenzene-d5
Concen: 50.00 ug/l
RT: 11.376 min Scan# 2997
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion:117 Resp: 118613
Ion Ratio Lower Upper
117 100
82 57.1 43.7 65.5
119 32.3 26.1 39.1

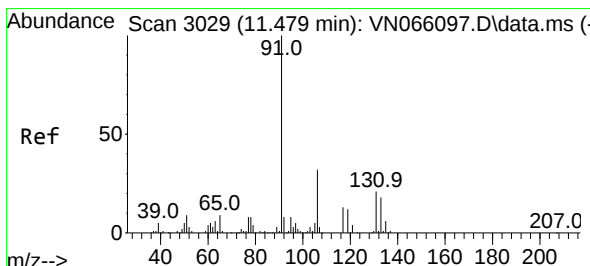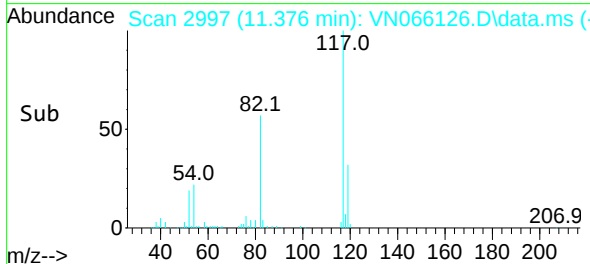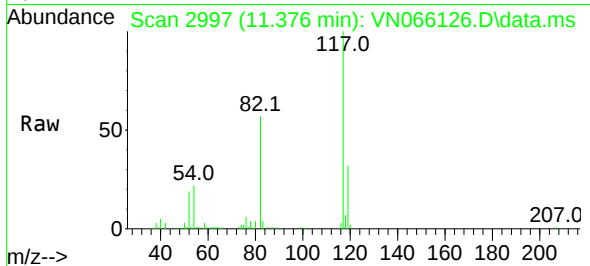

#67
Ethyl Benzene
Concen: 2.08 ug/l
RT: 11.479 min Scan# 3029
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 91 Resp: 9260
Ion Ratio Lower Upper
91 100
106 37.0 25.5 38.3


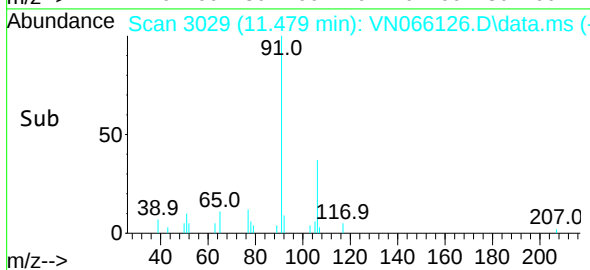

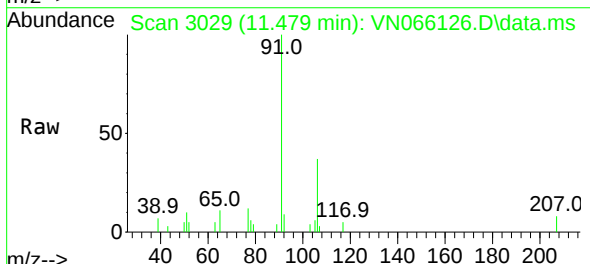


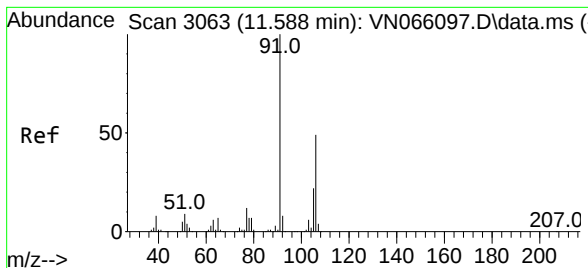

#68
m/p-Xylenes
Concen: 8.79 ug/l
RT: 11.588 min Scan# 3063
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion:106 Resp: 15149
Ion Ratio Lower Upper
106 100
91 211.9 161.4 242.0

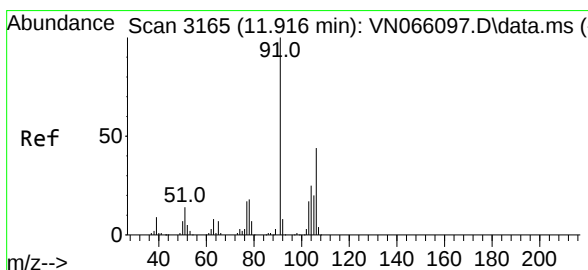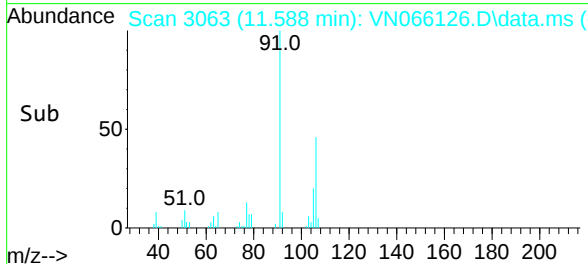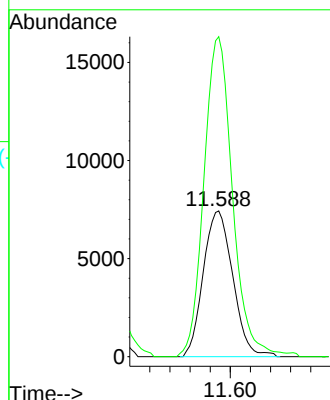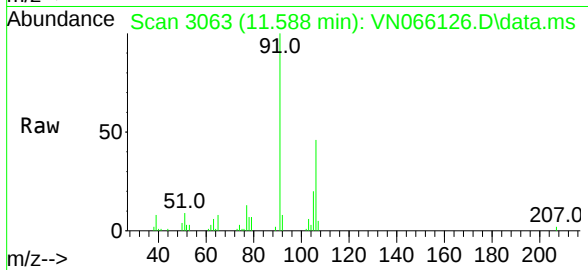

#69
o-Xylene
Concen: 3.54 ug/l
RT: 11.916 min Scan# 3165
Delta R.T. 0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion:106 Resp: 5958
Ion Ratio Lower Upper
106 100
91 217.2 106.8 320.4


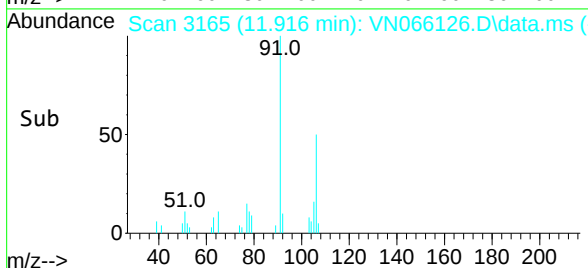
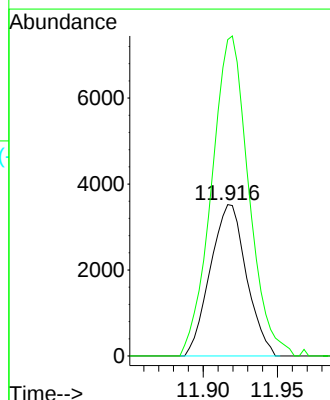
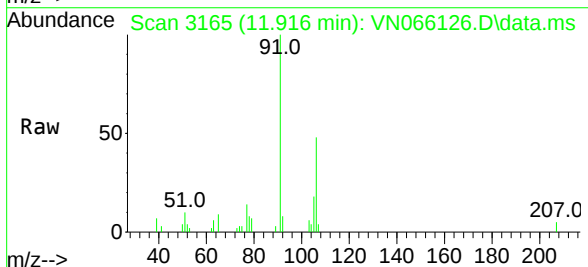


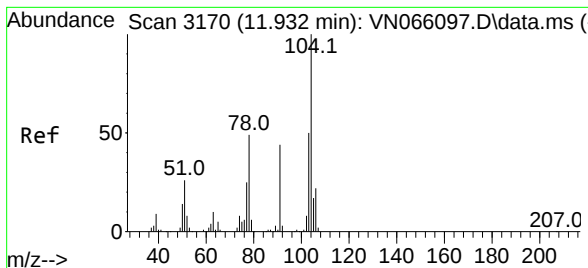

#70
Styrene
Concen: 0.37 ug/l
RT: 11.933 min Scan# 3170
Delta R.T. 0.001 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion:104 Resp: 970
Ion Ratio Lower Upper
104 100
78 132.4 39.0 58.4#
103 124.7 44.5 66.7#

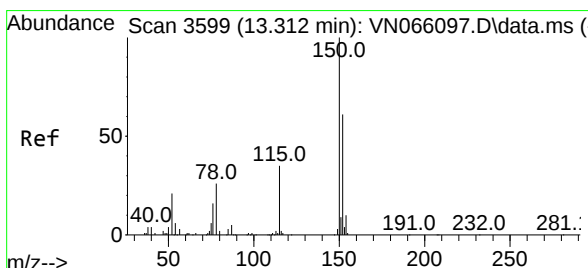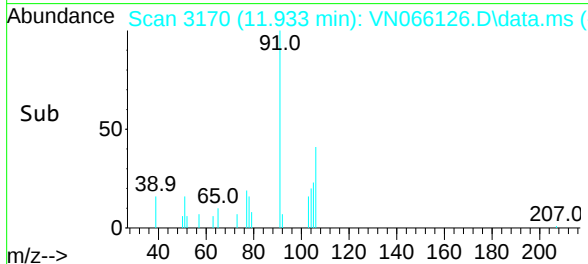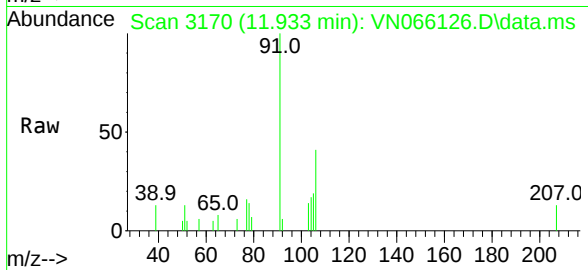

#72
1,4-Dichlorobenzene-d4
Concen: 50.00 ug/l
RT: 13.312 min Scan# 3599
Delta R.T. -0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08


Tgt Ion:152 Resp: 48847
Ion Ratio Lower Upper
152 100
115 62.3 28.5 85.6
150 157.1 0.0 347.6

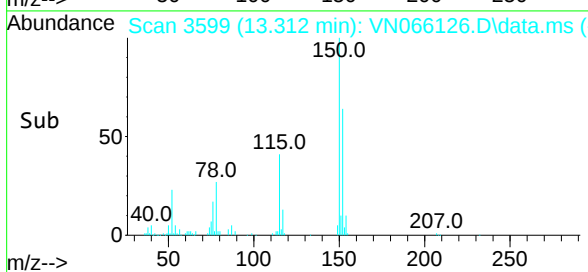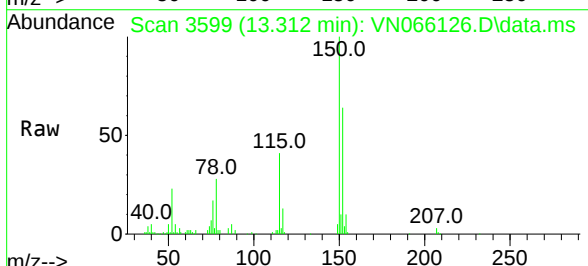






#74
N-amy1 acetate
Concen: 3.24 ug/l
RT: 12.051 min Scan# 3207
Delta R.T. 0.009 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77



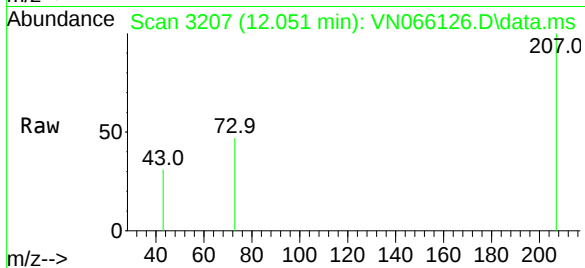



Tgt Ion: 43 Resp: 60
Ion Ratio Lower Upper
43 100
70 0.0 34.4 51.6#
55 0.0 20.7 31.1#
61 0.0 19.1 28.7#

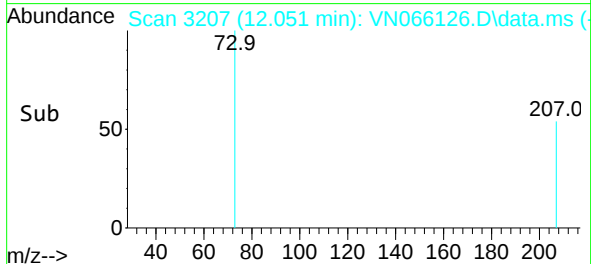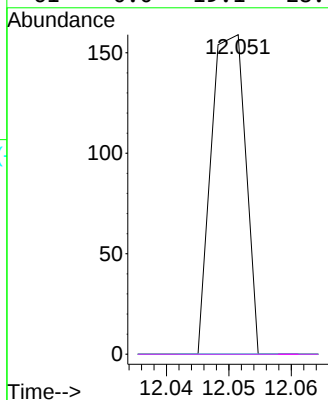

#76
1,2,3-Trichloropropane
Concen: 28.52 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. -0.151 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 75 Resp: 30757
Ion Ratio Lower Upper
75 100
77 0.5 0.0 0.0#


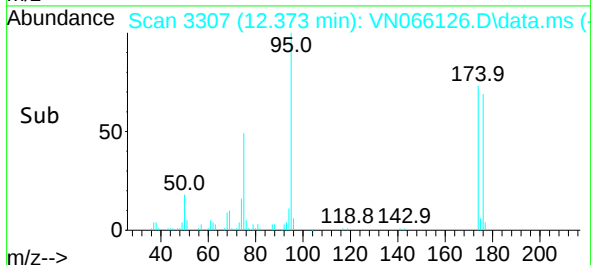
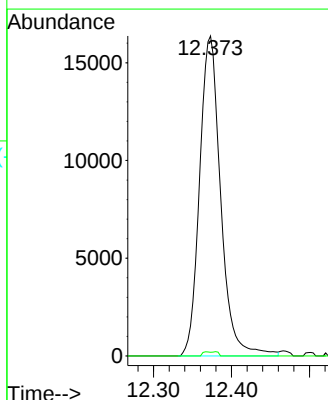
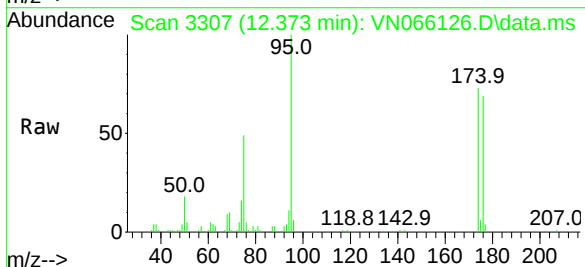




#78
n-propylbenzene
Concen: 0.23 ug/l
RT: 12.560 min Scan# 3365
Delta R.T. 0.001 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08




Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77


Tgt Ion: 91 Resp: 982
Ion Ratio Lower Upper
91 100
120 11.1 11.8 35.3#

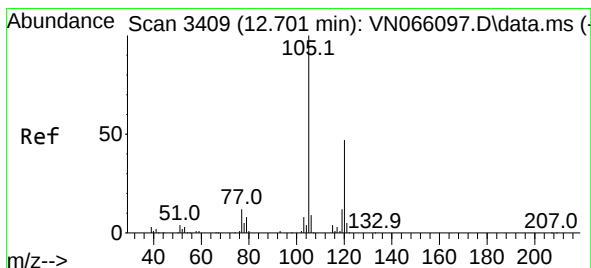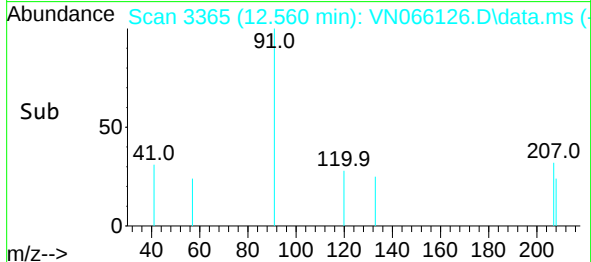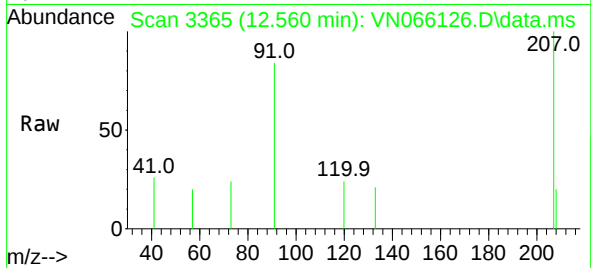

#80
1,3,5-Trimethylbenzene
Concen: 0.61 ug/l
RT: 12.701 min Scan# 3409
Delta R.T. -0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08


Tgt Ion: 105 Resp: 2161
Ion Ratio Lower Upper
105 100
120 43.3 24.3 72.8

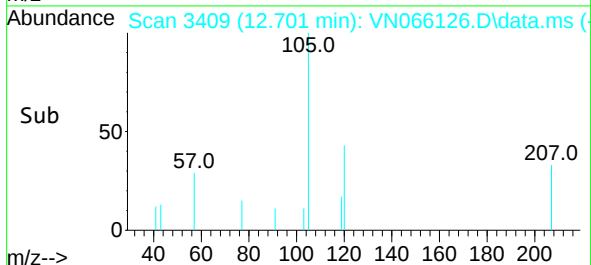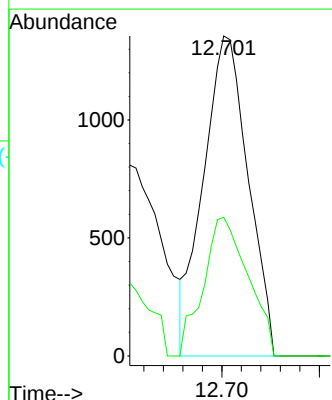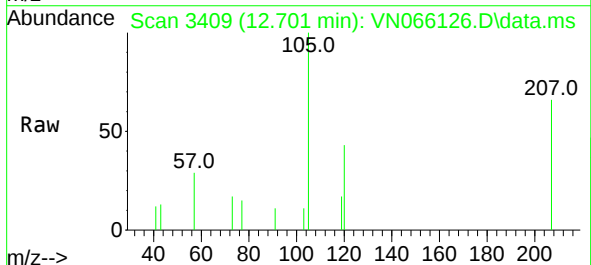



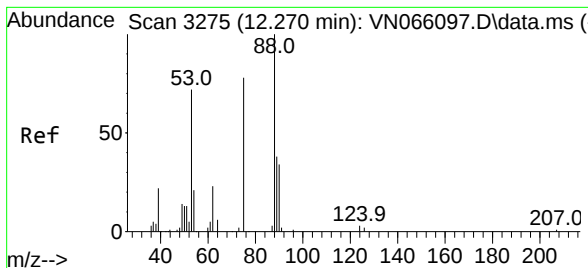


#81
trans-1,4-Dichloro-2-butene
Concen: 83.91 ug/l
RT: 12.373 min Scan# 3307
Delta R.T. 0.103 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77



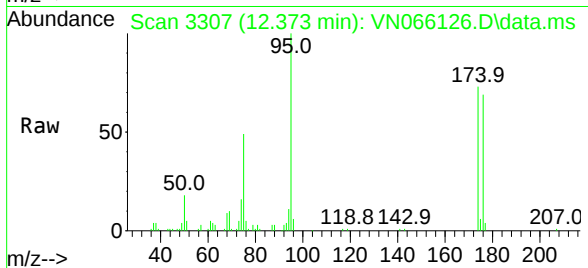



Tgt Ion: 75 Resp: 30757
Ion Ratio Lower Upper
75 100
53 0.0 74.6 111.8#
89 0.0 35.8 53.8#

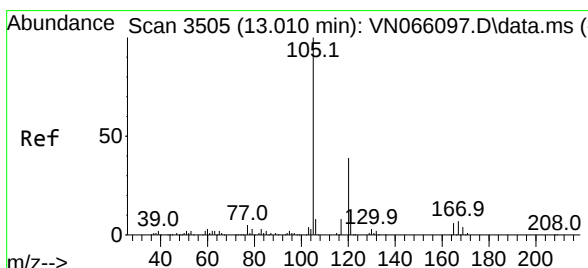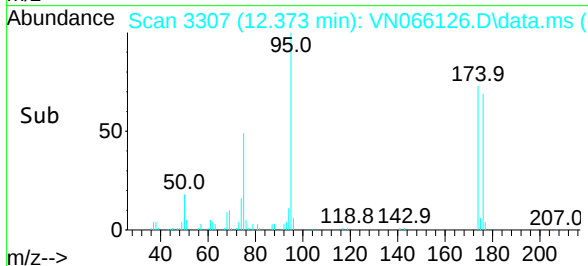

#84
1,2,4-Trimethylbenzene
Concen: 1.46 ug/l
RT: 13.010 min Scan# 3505
Delta R.T. -0.000 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 105 Resp: 5058
Ion Ratio Lower Upper
105 100
120 45.6 22.4 67.0


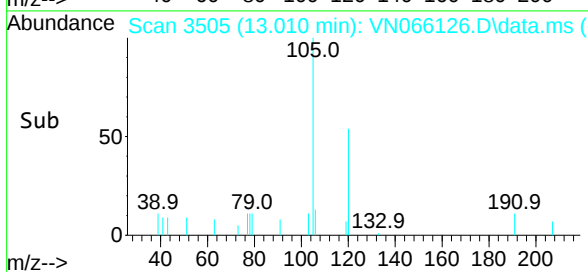

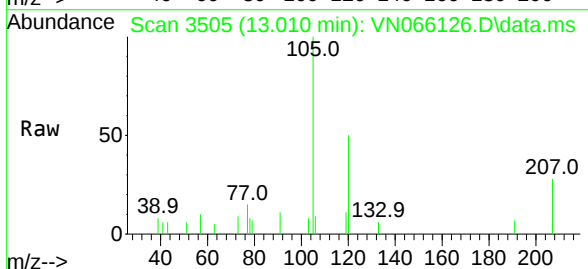


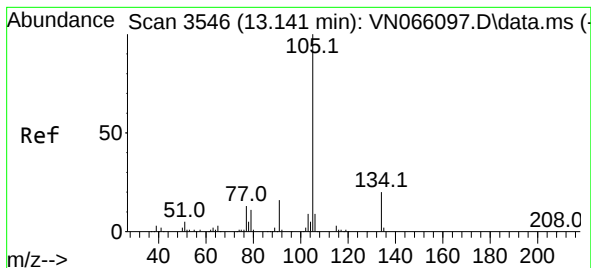

#85
 sec-Butylbenzene
 Concen: 1.41 ug/l
 RT: 13.010 min Scan# 3505
 Delta R.T. -0.131 min
 Lab File: VN066126.D
 Acq: 3 Mar 2021 16:08




Instrument :
 MSVOA_N
 ClientSampleId :
 COMP-30771-73-77


Tgt Ion:105 Resp: 5058
 Ion Ratio Lower Upper
 105 100
 134 0.0 10.0 30.0#

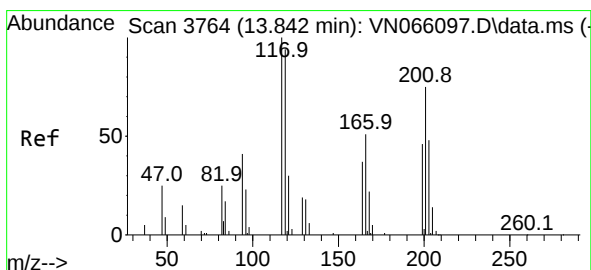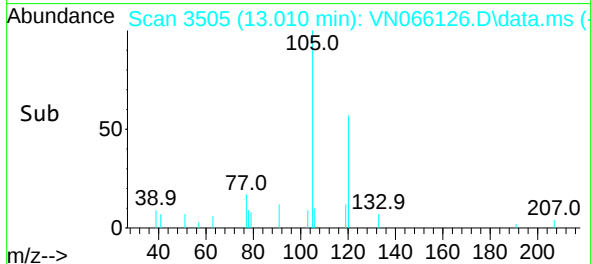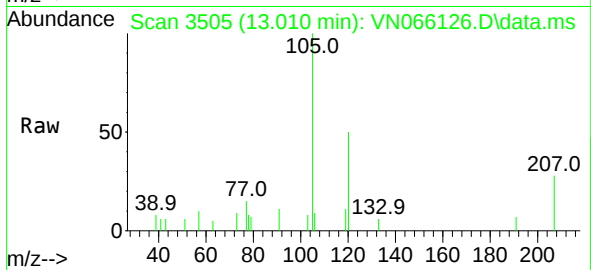

#90
 Hexachloroethane
 Concen: 0.33 ug/l
 RT: 13.900 min Scan# 3782
 Delta R.T. 0.058 min
 Lab File: VN066126.D
 Acq: 3 Mar 2021 16:08

Tgt Ion:117 Resp: 168
 Ion Ratio Lower Upper
 117 100
 201 0.0 37.8 113.3#


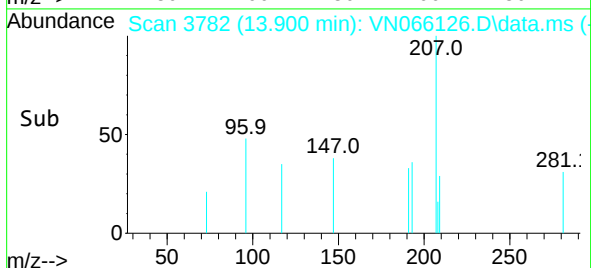
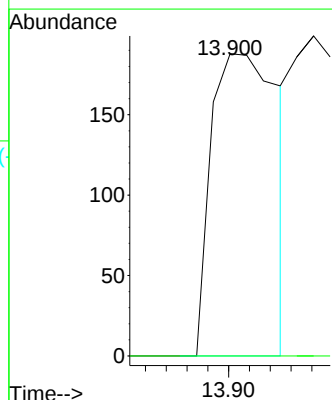
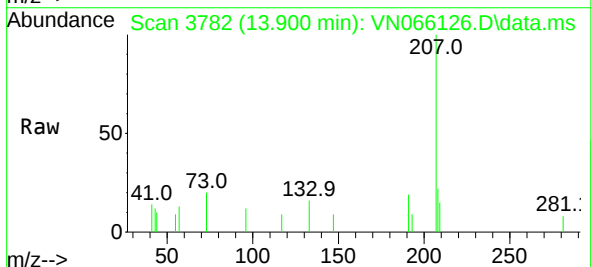


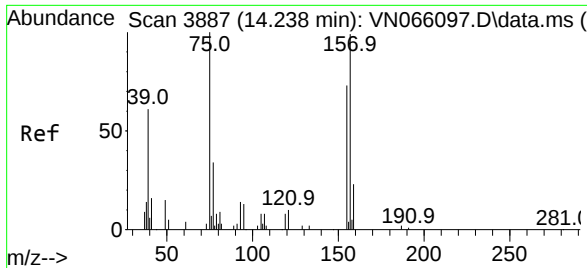

#92
1,2-Dibromo-3-Chloropropane
Concen: Below Cal
RT: 14.251 min Scan# 3891
Delta R.T. 0.013 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Instrument :
MSVOA_N
ClientSampleId :
COMP-30771-73-77

Tgt Ion: 75 Resp: 29
Ion Ratio Lower Upper
75 100
155 0.0 44.1 132.4#
157 0.0 56.0 168.2#

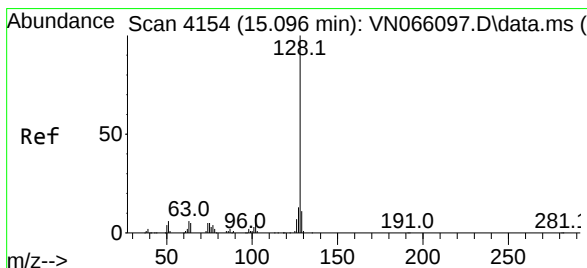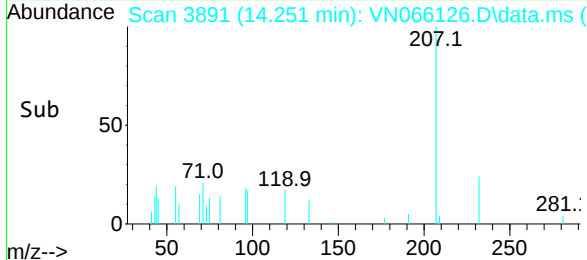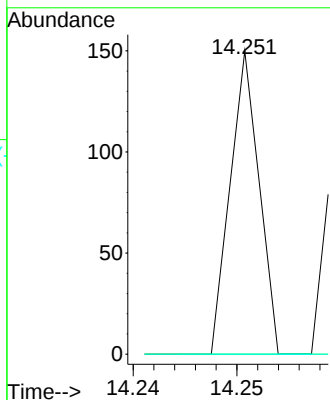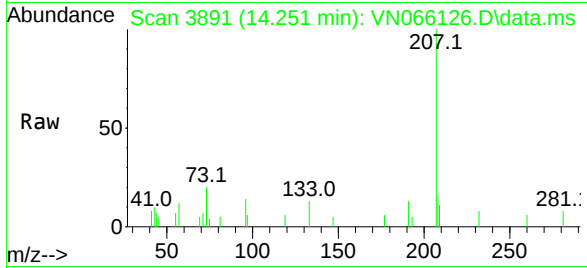

#95
Naphthalene
Concen: 3.70 ug/l
RT: 15.100 min Scan# 4155
Delta R.T. 0.004 min
Lab File: VN066126.D
Acq: 3 Mar 2021 16:08

Tgt Ion: 128 Resp: 10080
Ion Ratio Lower Upper
128 100
127 12.9 10.2 15.2
129 15.5 8.6 13.0#

