


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030419\
 Data File : VN054056.D
 Acq On : 4 Mar 2019 9:06
 Operator : JC/SP
 Sample : BFB
 Misc : 5.00mL/MSVOA N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Integration File: RTEINT3.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\624N030119W.M
 Title : METHOD 624 VOLATILE ORGANIC ANALYSIS
 Last Update : Tue Mar 05 00:48:50 2019

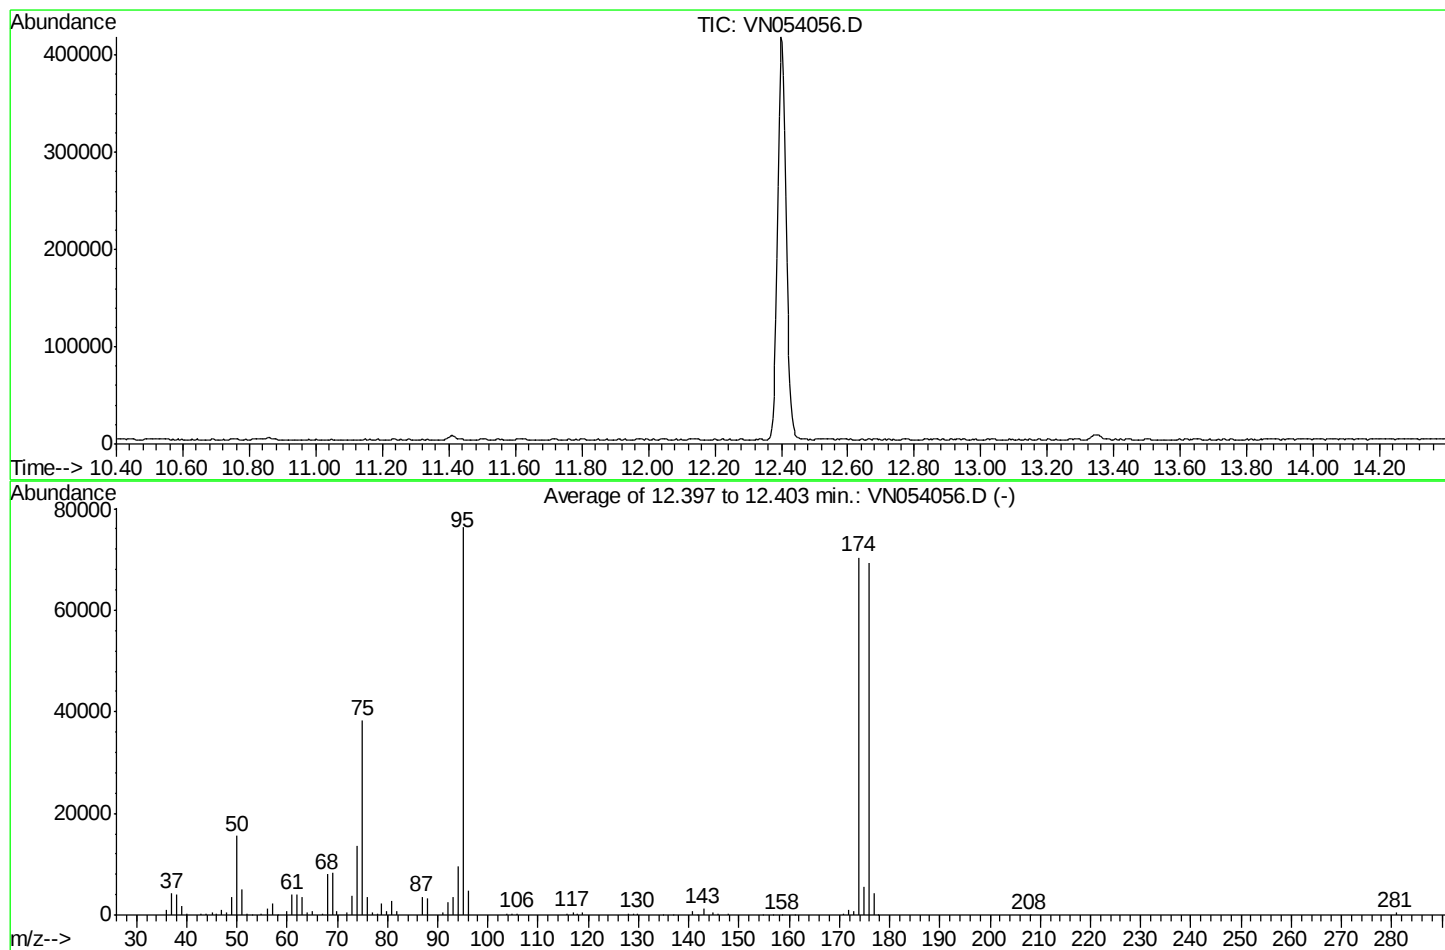

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.4	15557	PASS
75	95	30	60	50.2	38293	PASS
95	95	100	100	100.0	76325	PASS
96	95	5	9	6.3	4832	PASS
173	174	0.00	2	1.2	838	PASS
174	95	50	100	92.3	70440	PASS
175	174	5	9	8.0	5602	PASS
176	174	95	101	98.4	69314	PASS
177	176	5	9	6.3	4348	PASS