


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN030419\
Data File : VN054063.D
Acq On : 4 Mar 2019 13:49
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 8 Sample Multiplier: 1

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Title : SW846 8260
Last Update : Thu Feb 28 04:05:45 2019

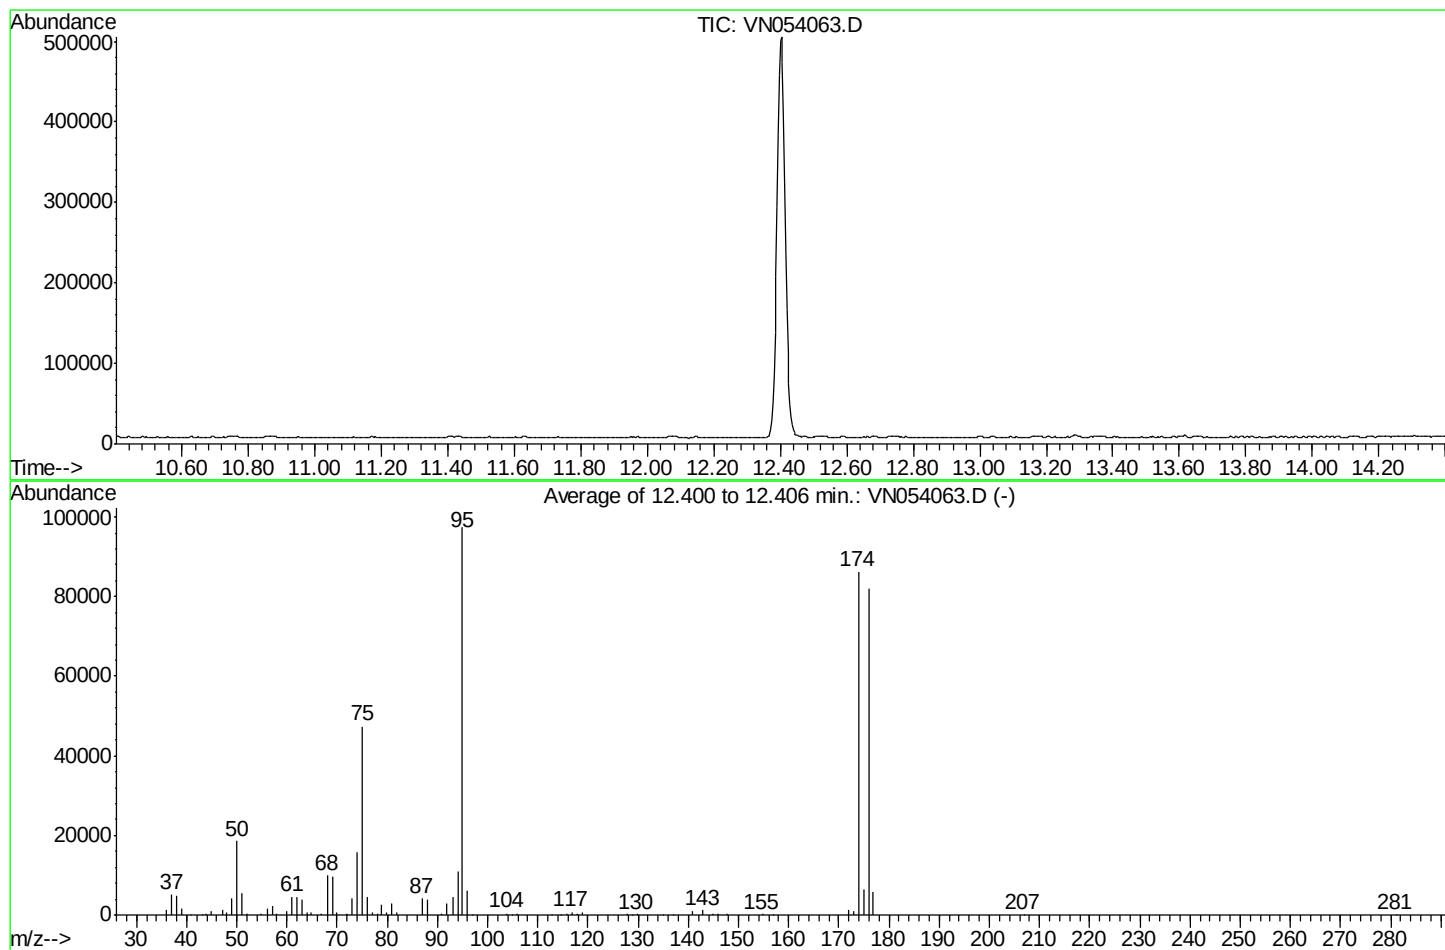

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.1	18632	PASS
75	95	30	60	48.7	47405	PASS
95	95	100	100	100.0	97402	PASS
96	95	5	9	6.3	6098	PASS
173	174	0.00	2	1.1	922	PASS
174	95	50	100	88.5	86237	PASS
175	174	5	9	7.6	6523	PASS
176	174	95	101	95.1	81976	PASS
177	176	5	9	7.2	5877	PASS