
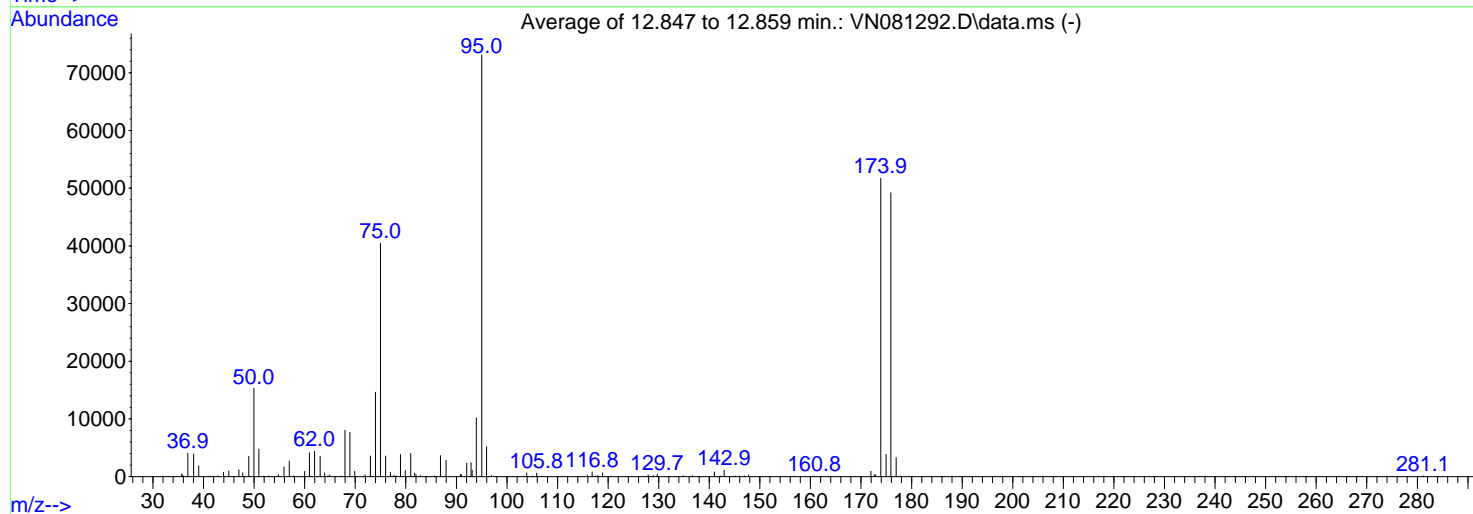


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030424\
 Data File : VN081292.D
 Acq On : 04 Mar 2024 09:33
 Operator : JC\MD
 Sample : BFB
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021624W.M
 Title : SW846 8260
 Last Update : Fri Feb 16 23:45:20 2024

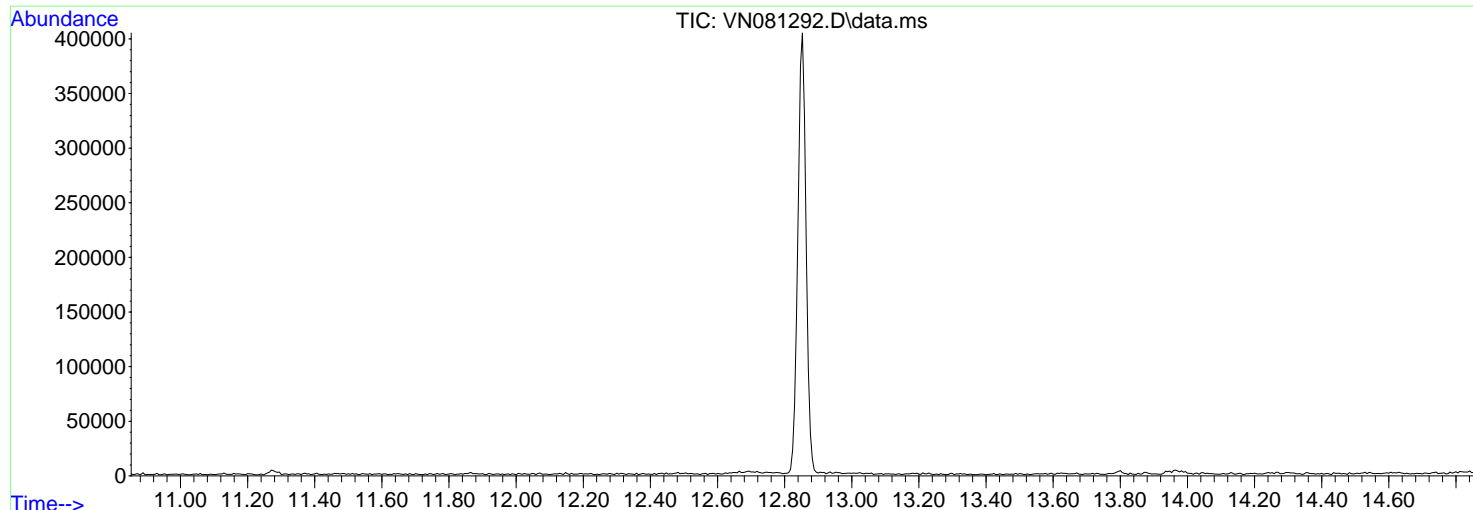

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.9	15307	PASS
75	95	30	60	55.3	40448	PASS
95	95	100	100	100.0	73112	PASS
96	95	5	9	7.1	5176	PASS
173	174	0.00	2	0.6	307	PASS
174	95	50	100	70.7	51712	PASS
175	174	5	9	7.5	3857	PASS
176	174	95	101	95.2	49237	PASS
177	176	5	9	6.7	3300	PASS

Average of 12.847 to 12.859 min.: VN081292.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.70	498	47.00	1174	60.00	909	69.90	92
35.90	257	47.75	656	60.95	4138	71.70	6
36.90	4059	48.95	3516	61.95	4409	71.95	34
38.05	3916	49.95	15307	63.05	3513	73.00	358
39.05	1864	50.95	4771	63.95	670	74.00	14620
40.00	50	51.80	84	64.60	140	75.00	40448
40.90	69	52.90	108	64.95	287	76.00	3583
42.00	93	54.80	328	65.90	90	76.95	739
42.85	148	55.90	1699	67.20	86	77.65	250
43.95	738	56.95	2688	67.95	8056	78.10	140
45.00	979	57.85	173	68.95	7692	78.95	3838

Instrument :
MSVOA_N
ClientSampleId :
BFB

Average of 12.847 to 12.859 min.: VN081292.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
79.90	1052	92.05	2324	106.80	62	130.00	59
80.95	4032	92.90	2424	110.80	62	134.85	168
81.75	608	93.10	1138	112.00	69	136.65	184
82.00	335	93.95	10190	115.90	287	141.00	805
82.90	157	95.00	73112	116.85	796	141.90	71
85.65	144	95.95	5176	117.50	99	142.30	128
86.85	3629	96.95	213	117.90	179	142.95	1100
87.95	2839	103.50	95	118.90	673	144.60	68
88.70	62	103.90	638	127.90	303	144.90	69
90.80	357	105.05	123	128.95	167	145.20	101
91.00	346	105.85	583	129.70	389	145.95	126

Average of 12.847 to 12.859 min.: VN081292.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
147.00	127	174.95	3857				
147.75	275	175.90	49237				
149.80	51	176.95	3300				
151.80	57	177.70	102				
154.90	62	281.15	133				
156.90	75						
160.80	81						
171.95	943						
172.65	313						
172.90	307						
173.90	51712						