


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030519\
Data File : VN054090.D
Acq On : 5 Mar 2019 10:02
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022519W.M
Title : SW846 8260
Last Update : Thu Feb 28 04:05:45 2019

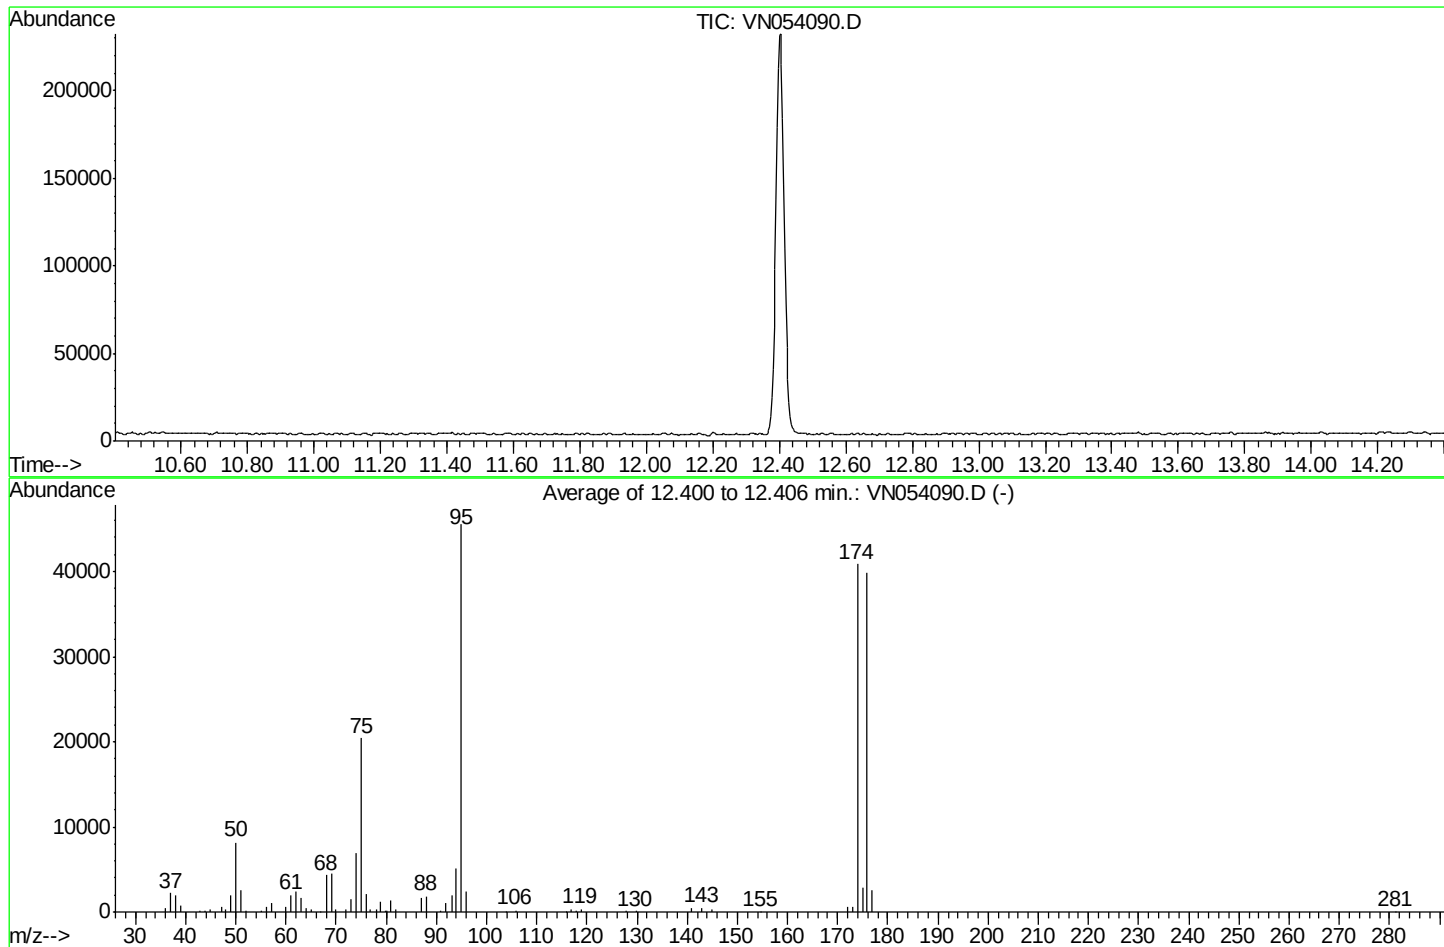

AutoFind: Scans 3305, 3306, 3307; Background Corrected with Scan 3292

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	17.9	8175	PASS
75	95	30	60	44.8	20413	PASS
95	95	100	100	100.0	45552	PASS
96	95	5	9	5.4	2444	PASS
173	174	0.00	2	1.5	601	PASS
174	95	50	100	89.7	40869	PASS
175	174	5	9	7.0	2869	PASS
176	174	95	101	97.4	39824	PASS
177	176	5	9	6.5	2607	PASS