


Data Path : Z:\voasrv\HPCHEM1\MSVOA N\Data\VN030520\
Data File : VN060356.D
Acq On : 5 Mar 2020 10:12
Operator : JC/MD
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N022720W.M
Title : SW846 8260
Last Update : Thu Feb 27 13:52:50 2020

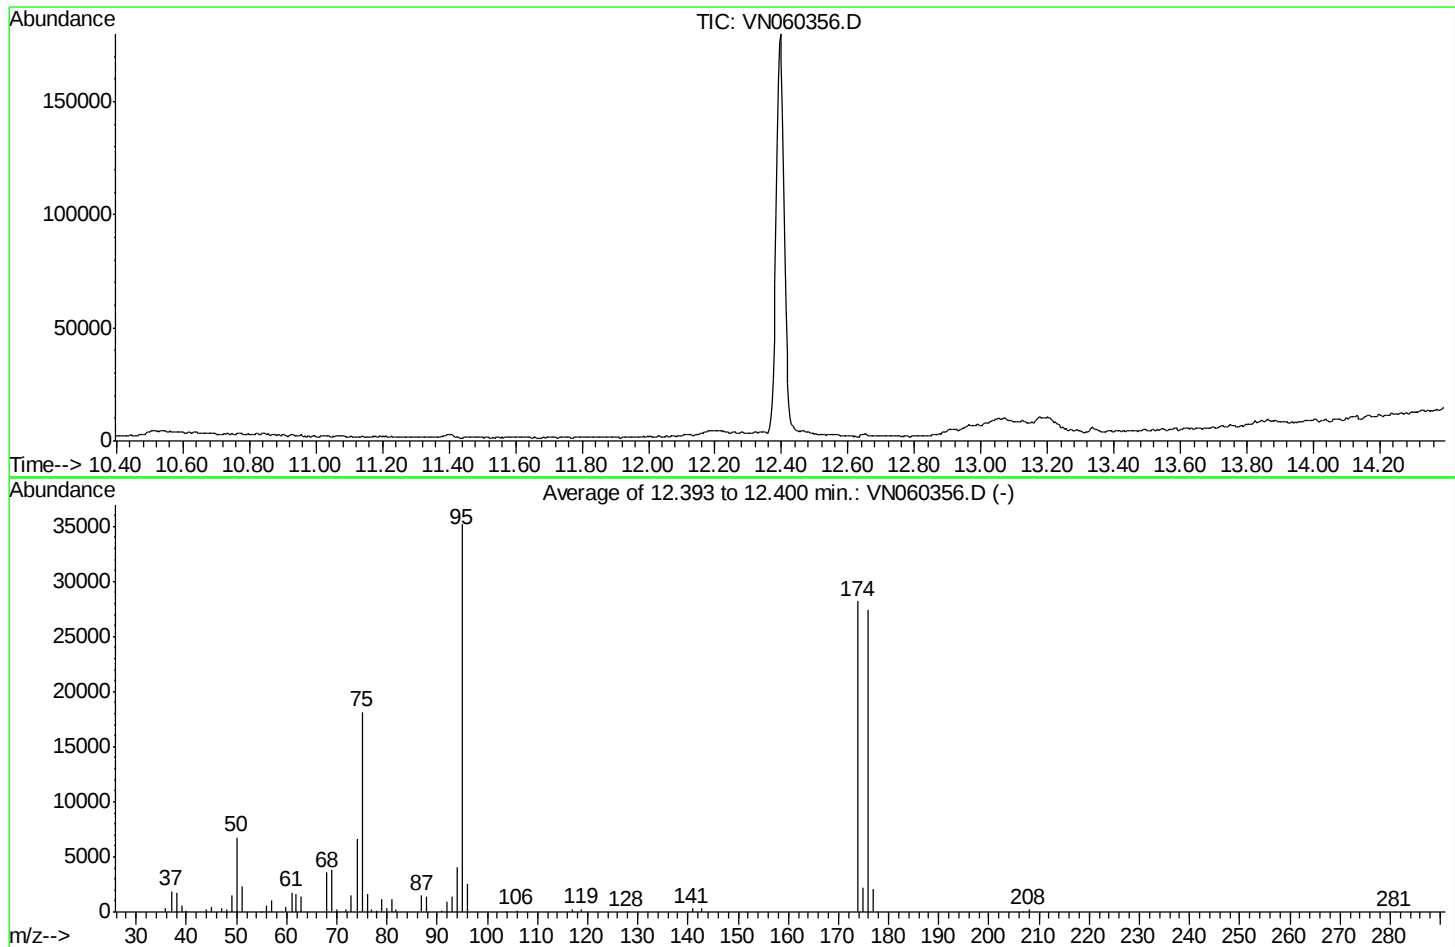

AutoFind: Scans 3303, 3304, 3305; Background Corrected with Scan 3290

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.3	6781	PASS
75	95	30	60	51.7	18173	PASS
95	95	100	100	100.0	35178	PASS
96	95	5	9	7.2	2530	PASS
173	174	0.00	2	0.0	0	PASS
174	95	50	100	80.1	28189	PASS
175	174	5	9	7.7	2180	PASS
176	174	95	101	97.3	27424	PASS
177	176	5	9	7.4	2039	PASS