


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030524\
Data File : VN081302.D
Acq On : 05 Mar 2024 09:31
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

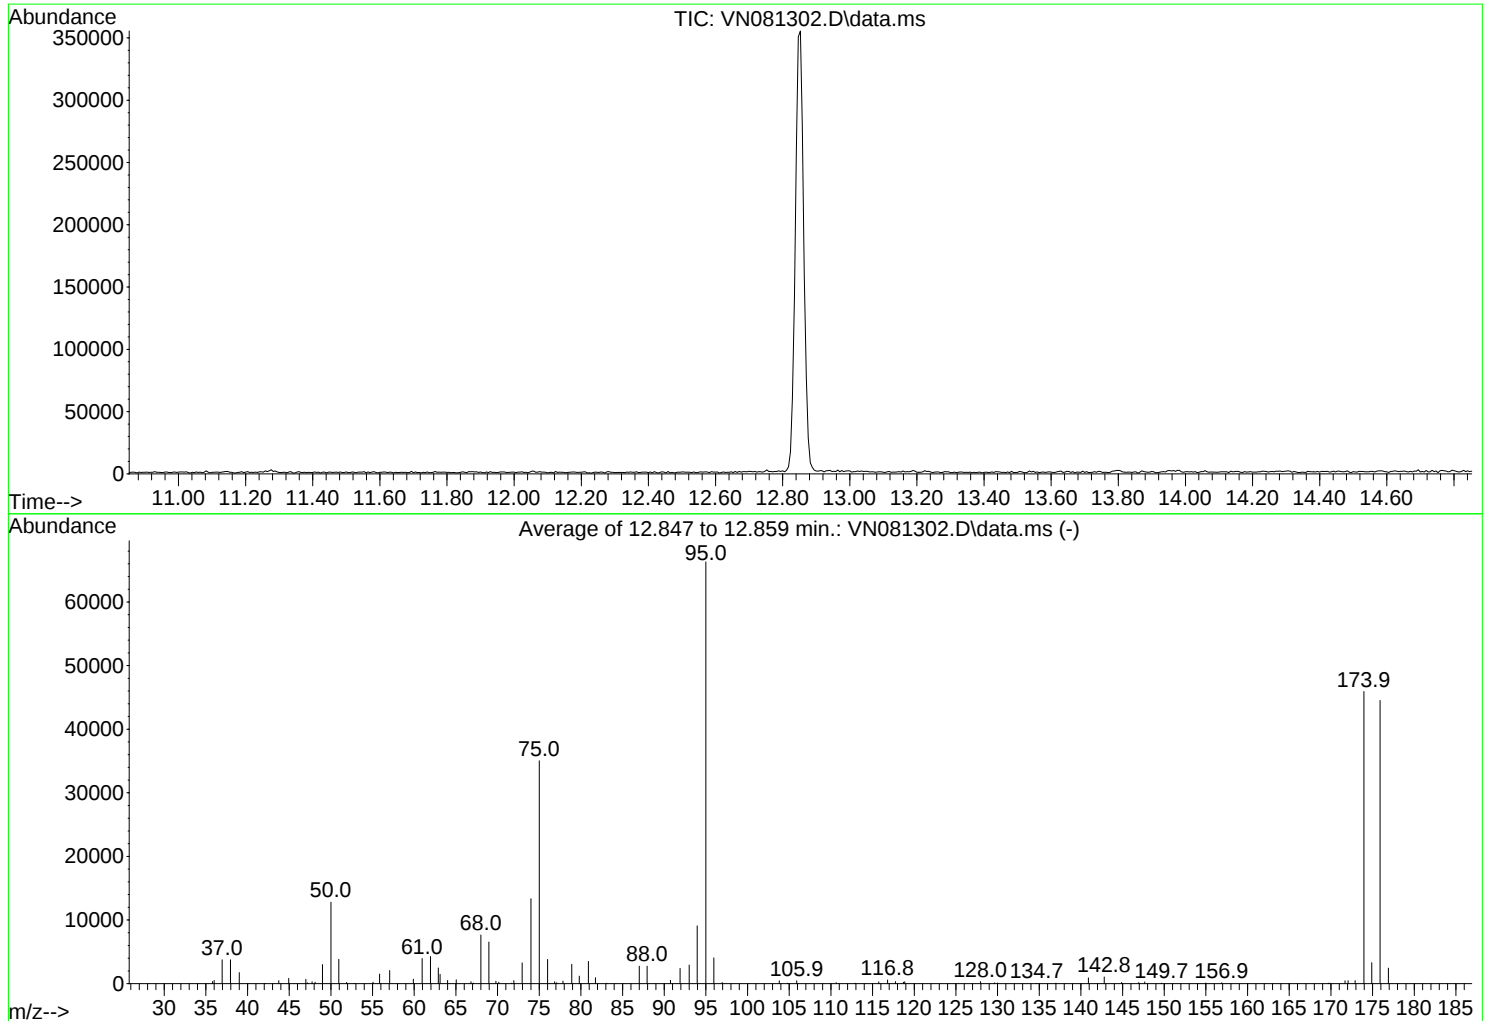

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.3	12805	PASS
75	95	30	60	52.9	35048	PASS
95	95	100	100	100.0	66312	PASS
96	95	5	9	6.1	4059	PASS
173	174	0.00	2	1.1	483	PASS
174	95	50	100	69.3	45944	PASS
175	174	5	9	7.2	3298	PASS
176	174	95	101	96.9	44523	PASS
177	176	5	9	5.5	2438	PASS

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.80	339	48.10	229	61.95	4287	71.70	71
36.00	510	49.00	2987	62.90	2479	71.95	49
36.95	3760	50.00	12805	63.10	1448	72.95	327
37.95	3745	50.95	3832	64.00	516	74.00	1336
39.00	1750	51.90	211	65.05	606	75.00	35048
42.10	63	52.80	60	66.80	312	76.00	3796
43.75	491	55.05	216	67.10	98	76.85	295
44.95	842	55.85	1519	68.00	7645	77.10	140
47.00	686	57.05	2064	68.95	6541	77.85	412
47.20	121	59.90	712	69.80	387	78.90	3039
47.75	309	60.95	3946	70.15	218	79.80	1182

Average of 12.847 to 12.859 min.: VN081302.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
80.90	3502	96.95	187	127.95	341	155.00	94
81.75	947	103.80	450	129.65	133	156.90	118
83.10	85	104.80	74	130.00	105	169.70	90
87.00	2732	105.90	459	134.70	58	169.90	67
87.95	2741	110.65	154	137.00	84	171.70	455
90.75	537	112.90	70	140.90	897	172.05	484
91.90	2391	115.75	274	142.80	1050	172.90	483
93.00	2923	116.80	580	144.90	203	173.95	45944
93.95	9074	117.75	331	146.95	183	174.90	3298
95.00	66312	118.70	225	147.65	274	175.90	44523
95.95	4059	118.85	304	149.70	87	176.90	2438

Instrument :

MSVOA_N

ClientSampleId :

BFB