


Data Path : Z:\VOASRV\HPCHEM1\MSVOA N\DATA\VN030619\
Data File : VN054109.D
Acq On : 6 Mar 2019 9:35
Operator : JC/SP
Sample : BFB
Misc : 5.00mL/MSVOA N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\VOASRV\HPCHEM1\MSVOA_N\METHODS\82N030619W.M
Title : SW846 8260
Last Update : Thu Mar 07 06:25:49 2019

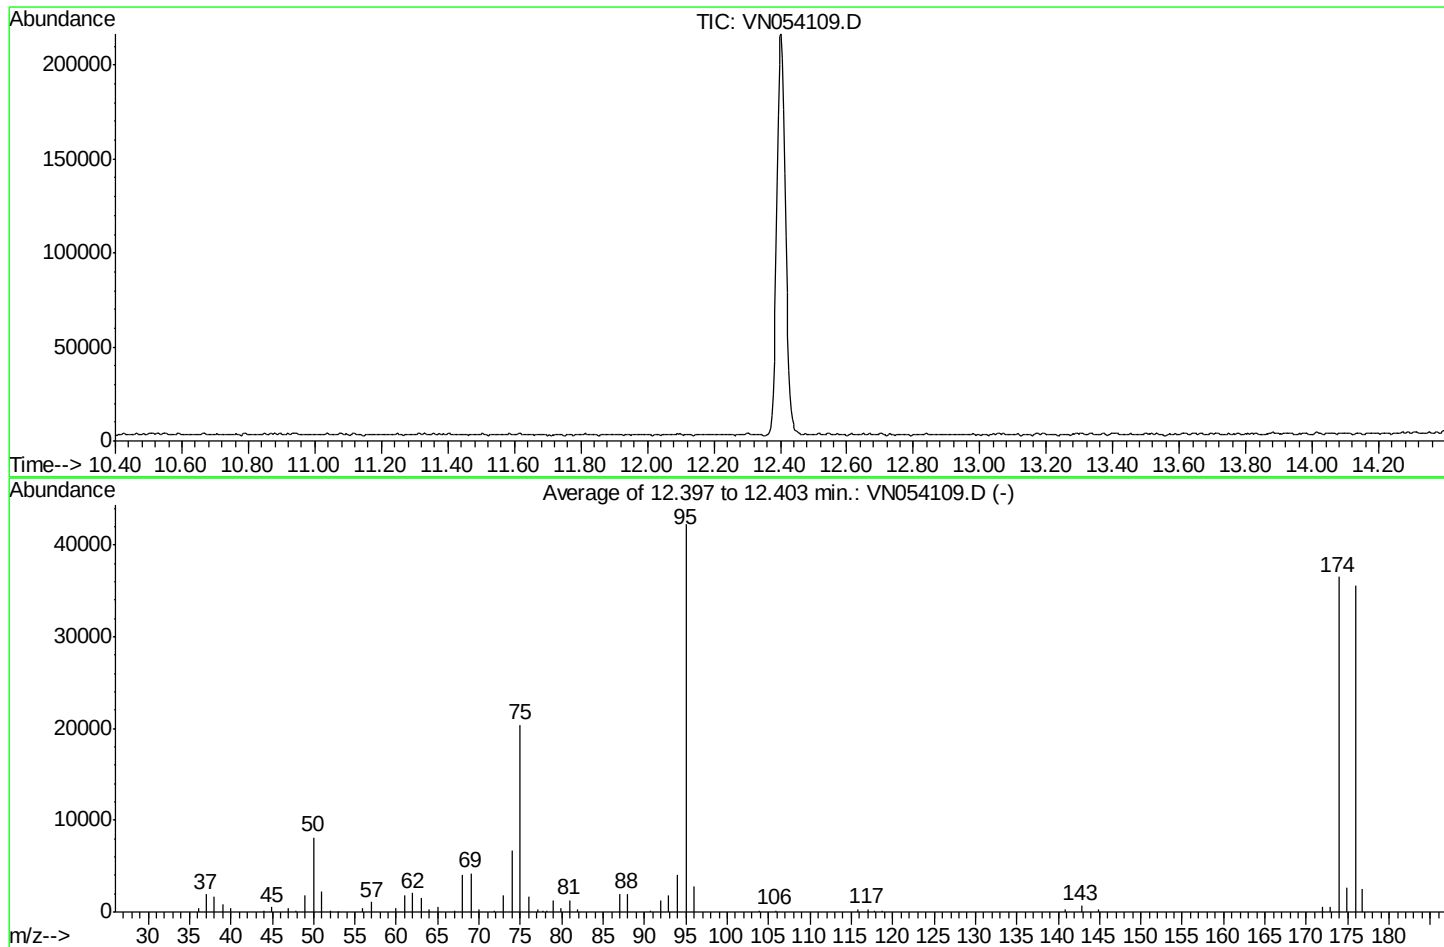

AutoFind: Scans 3304, 3305, 3306; Background Corrected with Scan 3291

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	19.2	8105	PASS
75	95	30	60	48.3	20416	PASS
95	95	100	100	100.0	42269	PASS
96	95	5	9	6.6	2798	PASS
173	174	0.00	2	1.4	506	PASS
174	95	50	100	86.4	36530	PASS
175	174	5	9	7.4	2707	PASS
176	174	95	101	97.5	35632	PASS
177	176	5	9	7.0	2495	PASS