
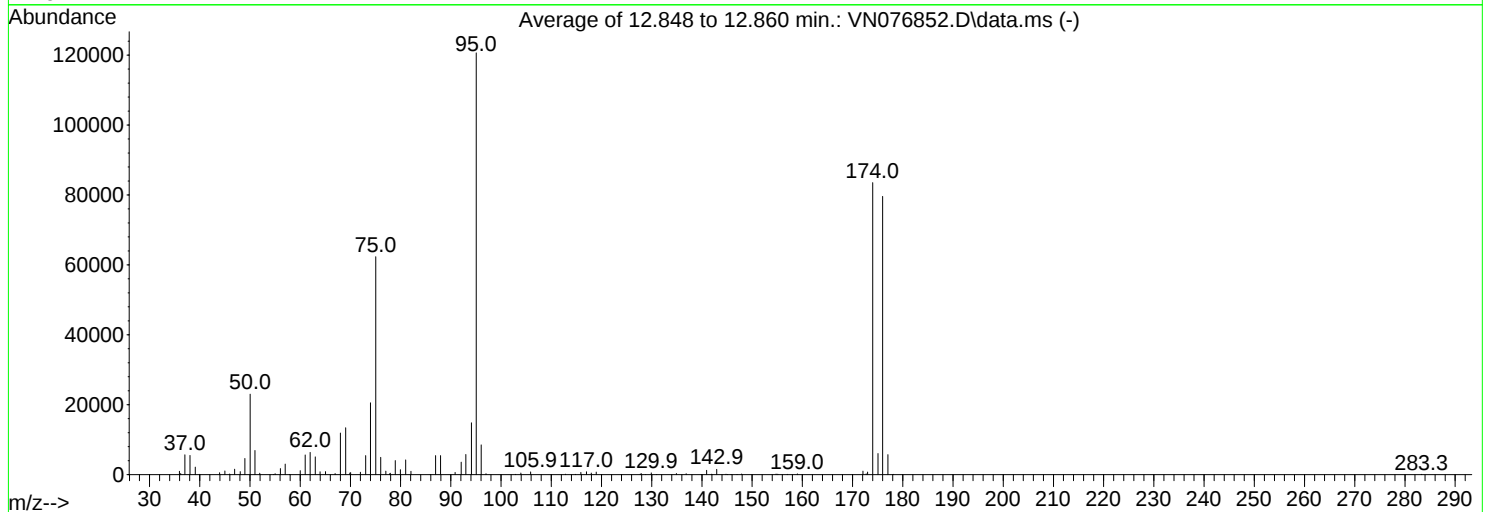


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030623\
Data File : VN076852.D
Acq On : 06 Mar 2023 16:15
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030623W.M
Title : SW846 8260
Last Update : Tue Mar 07 08:45:33 2023

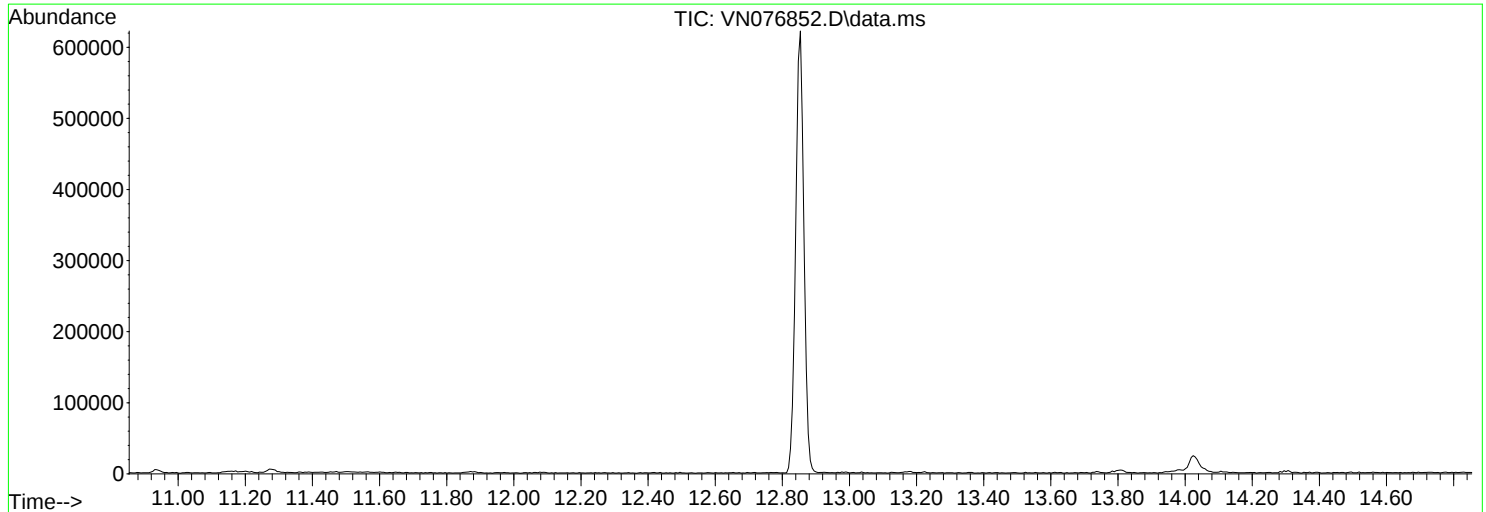

AutoFind: Scans 1855, 1856, 1857; Background Corrected with Scan 1847

Target	Rel. to	Lower	Upper	Rel.	Raw	Result
Mass	Mass	Limit%	Limit%	Abn%	Abn	Pass/Fail
50	95	15	40	19.1	23021	PASS
75	95	30	60	51.7	62357	PASS
95	95	100	100	100.0	120648	PASS
96	95	5	9	7.1	8520	PASS
173	174	0.00	2	0.9	732	PASS
174	95	50	100	69.2	83507	PASS
175	174	5	9	7.2	6040	PASS
176	174	95	101	95.3	79608	PASS
177	176	5	9	7.2	5738	PASS

Average of 12.848 to 12.860 min.: VN076852.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.95	958	49.00	4640	62.00	6387	74.00	2057
36.20	301	50.05	23021	63.00	5078	75.05	6235
37.05	5699	51.00	6915	63.95	805	76.05	492
38.05	5497	51.95	397	65.05	868	77.05	102
39.10	2141	54.70	52	66.95	321	77.80	230
40.00	75	55.00	256	68.00	11882	77.95	416
43.95	571	56.05	1743	69.05	13392	78.95	4038
45.00	1054	57.00	3033	69.90	451	79.95	1443
45.95	168	57.90	68	70.05	584	81.00	4221
46.95	1559	60.00	1124	72.00	690	82.05	970
48.05	852	61.00	5627	73.05	5428	85.90	60

Average of 12.848 to 12.860 min.: VN076852.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
86.95	5445	105.90	781	129.90	514	147.00	52
87.95	5453	112.85	156	131.00	56	147.90	192
90.85	620	114.80	87	134.90	320	154.75	182
92.05	3570	115.90	637	136.85	292	155.10	140
93.00	5755	117.00	828	139.90	64	157.00	106
94.10	14846	117.95	476	140.95	1219	159.00	229
95.05	120648	118.95	726	141.95	141	172.05	1010
96.05	8520	124.00	58	142.95	1512	172.70	211
97.00	279	127.70	118	144.80	149	173.00	732
102.90	115	127.90	321	145.10	60	174.00	83507
103.95	480	128.80	51	145.80	68	175.05	6040

Average of 12.848 to 12.860 min.: VN076852.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.00	79608						
177.05	5738						
178.10	109						
283.30	72						

Instrument :

MSVOA_N

ClientSampleId :

BFB