
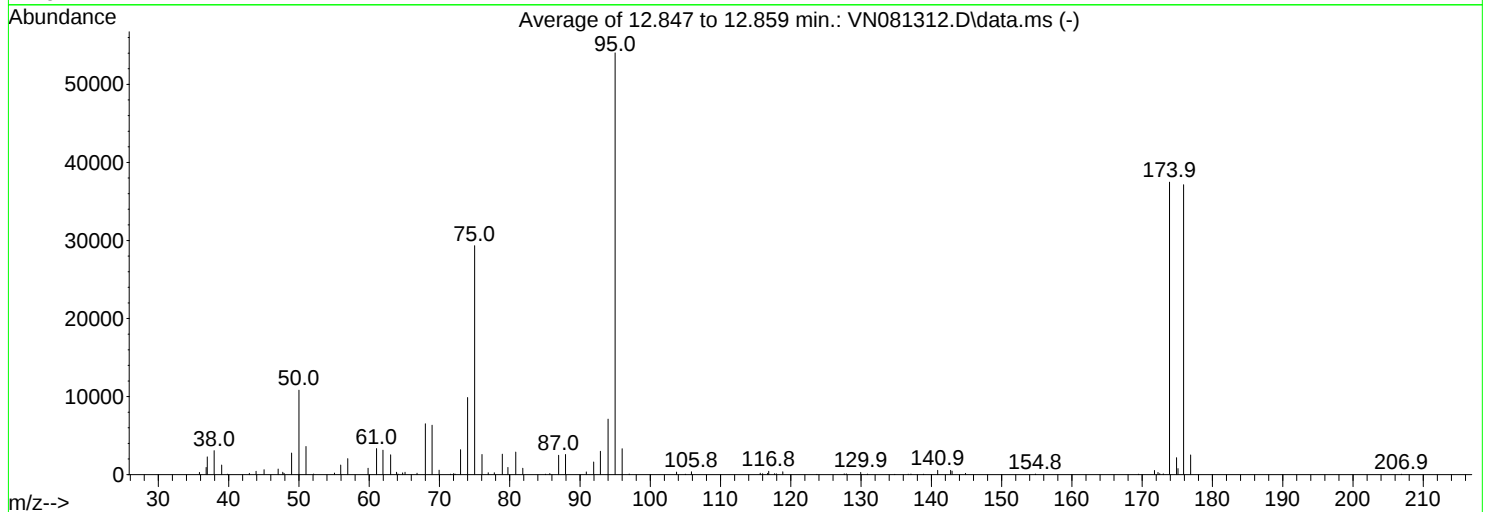


Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030624\
Data File : VN081312.D
Acq On : 06 Mar 2024 08:28
Operator : JC\MD
Sample : BFB
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
BFB

Integration File: RTEINT.P

Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N030524W.M
Title : SW846 8260
Last Update : Wed Mar 06 03:12:57 2024

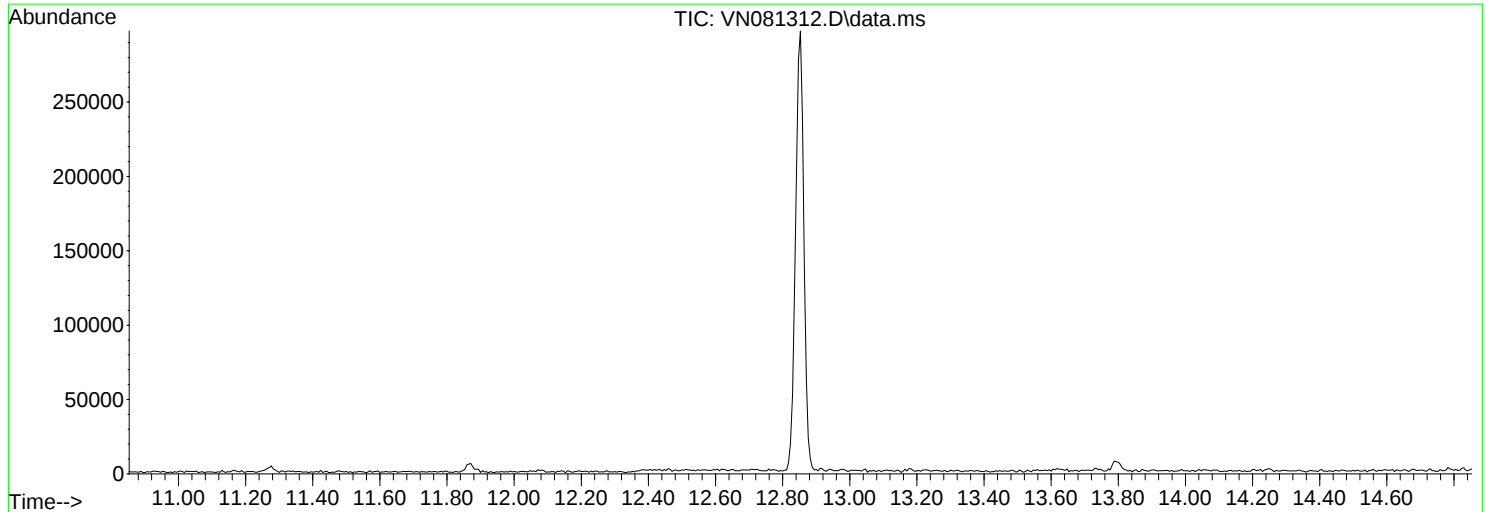

AutoFind: Scans 1852, 1853, 1854; Background Corrected with Scan 1843

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	20.0	10816	PASS
75	95	30	60	54.3	29328	PASS
95	95	100	100	100.0	54040	PASS
96	95	5	9	6.1	3317	PASS
173	174	0.00	2	0.3	98	PASS
174	95	50	100	69.4	37477	PASS
175	174	5	9	5.8	2177	PASS
176	174	95	101	99.1	37139	PASS
177	176	5	9	6.8	2522	PASS

Average of 12.847 to 12.859 min.: VN081312.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
35.85	292	47.90	174	63.05	2541	72.20	71
36.80	929	48.95	2775	63.90	298	73.00	319
36.95	2286	50.00	10816	64.10	83	74.00	987
37.95	3073	51.00	3608	64.75	237	75.00	2932
39.00	1232	52.10	91	65.10	315	76.05	2575
39.85	63	55.05	215	66.80	184	76.95	241
42.95	163	55.95	1227	68.00	6514	77.80	241
43.90	425	56.95	2061	68.95	6340	78.95	2618
45.05	637	59.85	825	69.95	579	79.75	914
47.05	717	61.05	3336	71.60	70	80.85	2890
47.70	314	61.95	3139	72.00	117	81.85	818

Average of 12.847 to 12.859 min.: VN081312.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
85.10	52	103.75	320	127.60	110	144.85	167
85.70	138	105.00	73	127.90	110	154.80	87
86.95	2472	105.85	373	129.95	289	169.50	56
87.95	2581	115.65	191	130.90	77	171.75	531
90.90	342	116.00	116	134.80	51	172.25	288
91.95	1614	116.70	175	136.70	65	172.50	123
92.90	2984	116.85	436	137.10	76	173.00	98
94.00	7116	117.70	125	138.90	61	173.90	37477
95.00	54040	117.95	102	140.90	558	174.90	2177
96.00	3317	118.85	374	142.75	549	175.10	789
97.00	89	123.70	50	142.95	461	175.90	37139

Average of 12.847 to 12.859 min.: VN081312.D\data.ms

BFB

Modified:subtracted

m/z	abund.	m/z	abund.	m/z	abund.	m/z	abund.
176.90	2522						
206.90	55						

Instrument :
MSVOA_N
ClientSampleId :
BFB