

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030625\
 Data File : VN085897.D
 Acq On : 06 Mar 2025 14:41
 Operator : JC\MD
 Sample : VN0306WBL01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 VN0306WBL01

Quant Time: Mar 07 00:37:26 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	132674	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	229960	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	211168	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	85128	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.577	65	101028	58.735	ug/l	0.00
Spiked Amount 50.000	Range 74 - 125		Recovery = 117.460%			
35) Dibromofluoromethane	8.165	113	88829	59.032	ug/l	0.00
Spiked Amount 50.000	Range 75 - 124		Recovery = 118.060%			
50) Toluene-d8	10.565	98	287556	52.524	ug/l	0.00
Spiked Amount 50.000	Range 86 - 113		Recovery = 105.040%			
62) 4-Bromofluorobenzene	12.847	95	85632	47.473	ug/l	0.00
Spiked Amount 50.000	Range 77 - 121		Recovery = 94.940%			
Target Compounds						Qvalue
3) Chloromethane	2.353	50	507	0.280	ug/l #	82
5) Bromomethane	2.965	94	787	0.642	ug/l	85
13) Acrolein	4.189	56	132	0.421	ug/l #	15
16) Acetone	4.436	43	240	0.441	ug/l #	40
17) Carbon Disulfide	4.718	76	1666	0.386	ug/l #	75
18) Methyl Acetate	5.030	43	494	0.264	ug/l #	72
25) 2-Butanone	7.506	43	170	0.212	ug/l #	45
31) Cyclohexane	8.224	56	2482	1.010	ug/l #	1
36) 1,1-Dichloropropene	8.224	75	10080	4.733	ug/l #	50
38) Carbon Tetrachloride	8.224	117	13885	5.487	ug/l #	18
43) Isopropyl Acetate	8.712	43	2383	0.231	ug/l #	53
59) 2-Hexanone	11.200	43	741	0.637	ug/l	71
70) Styrene	12.412	104	498	0.691	ug/l #	59
76) 1,2,3-Trichloropropane	12.847	75	42434	22.440	ug/l #	1
77) Bromobenzene	12.988	156	333	0.211	ug/l	88
79) 2-Chlorotoluene	13.223	91	910	0.204	ug/l	91
81) trans-1,4-Dichloro-2-b...	12.847	75	42434	65.475	ug/l #	12
82) 4-Chlorotoluene	13.223	91	910	0.206	ug/l	91
85) sec-Butylbenzene	13.612	105	1326	0.235	ug/l #	71
86) p-Isopropyltoluene	13.729	119	1137	0.861	ug/l #	81
87) 1,3-Dichlorobenzene	13.741	146	1051	0.356	ug/l	79
88) 1,4-Dichlorobenzene	13.741	146	1051	0.347	ug/l	81
89) n-Butylbenzene	14.053	91	1974	0.493	ug/l	91
91) 1,2-Dichlorobenzene	14.106	146	997	0.351	ug/l	83
92) 1,2-Dibromo-3-Chloropr...	14.717	75	124	0.336	ug/l	60
93) 1,2,4-Trichlorobenzene	15.400	180	1506	1.113	ug/l #	81
94) Hexachlorobutadiene	15.494	225	1245	1.514	ug/l	89
95) Naphthalene	15.641	128	6213	1.673	ug/l	96
96) 1,2,3-Trichlorobenzene	15.847	180	1795	1.322	ug/l	88

(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030625\
Data File : VN085897.D
Acq On : 06 Mar 2025 14:41
Operator : JC\MD
Sample : VN0306WBL01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01

Quant Time: Mar 07 00:37:26 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




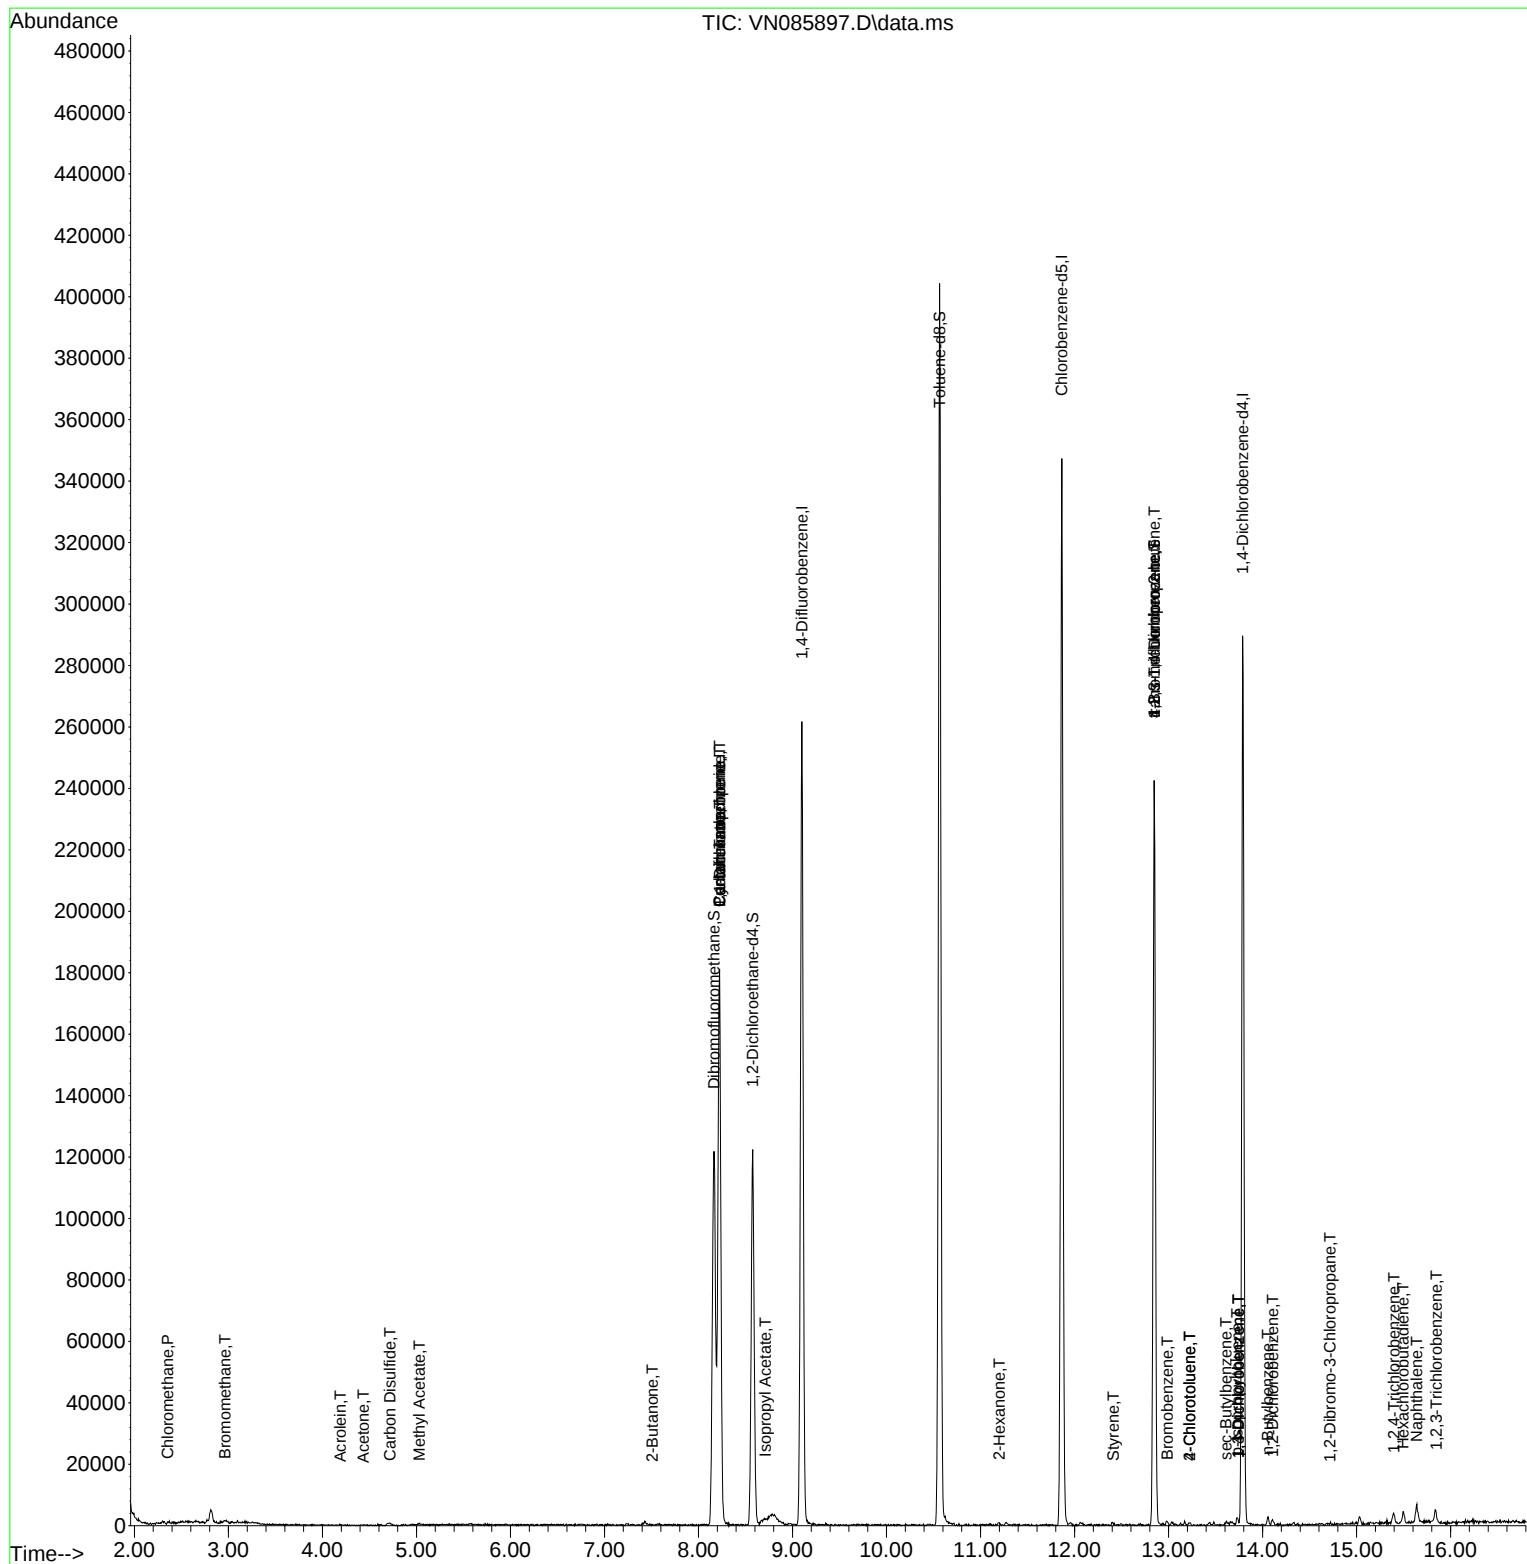




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 10
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion:168 Resp: 132674
Ion Ratio Lower Upper
168 100
99 59.3 47.9 71.9

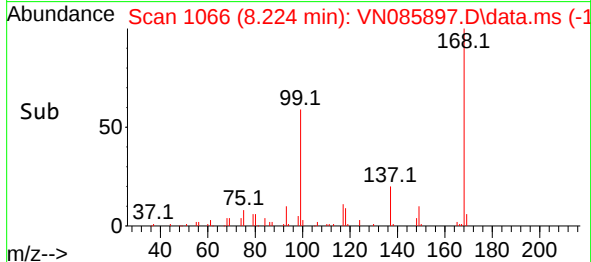

#3
Chloromethane
Concen: 0.280 ug/l
RT: 2.353 min Scan# 68
Delta R.T. -0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 50 Resp: 507
Ion Ratio Lower Upper
50 100
52 43.8 26.7 40.1#


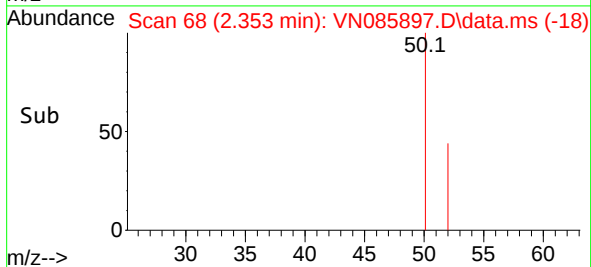

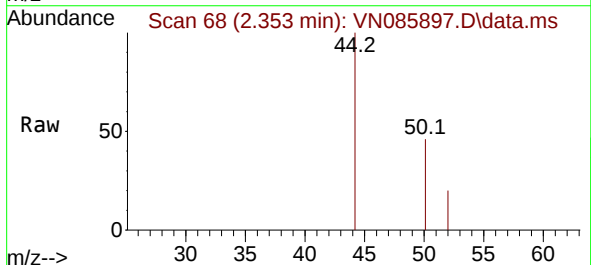


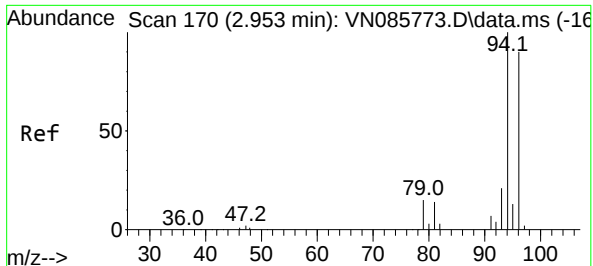

#5
Bromomethane
Concen: 0.642 ug/l
RT: 2.965 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion: 94 Resp: 787
Ion Ratio Lower Upper
94 100
96 75.5 71.7 107.5

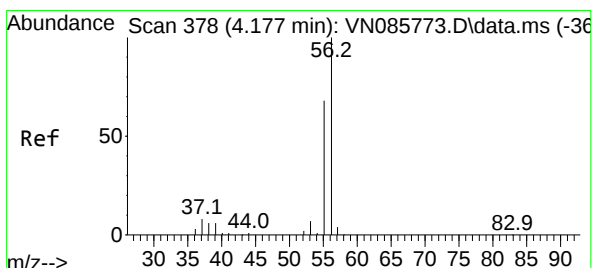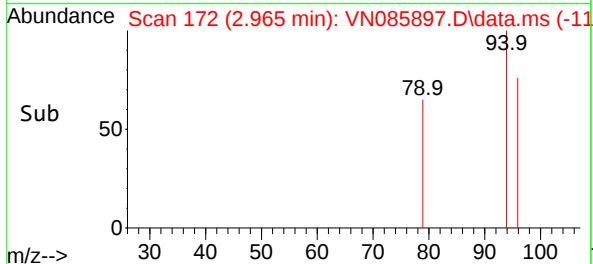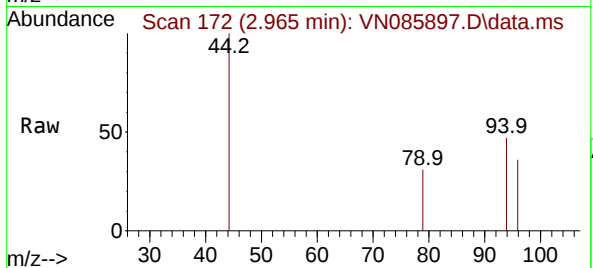

#13
Acrolein
Concen: 0.421 ug/l
RT: 4.189 min Scan# 380
Delta R.T. 0.012 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 56 Resp: 132
Ion Ratio Lower Upper
56 100
55 0.0 55.3 82.9#


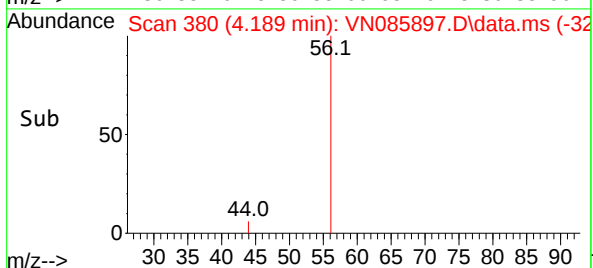

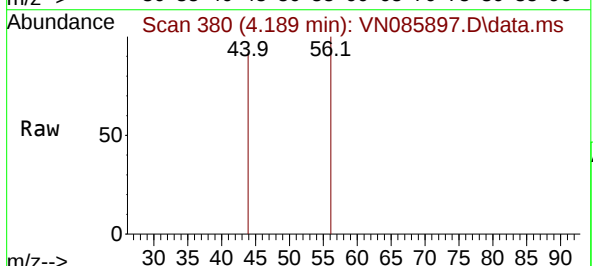




#16
Acetone
Concen: 0.441 ug/l
RT: 4.436 min Scan# 41
Delta R.T. 0.018 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion: 43 Resp: 240
Ion Ratio Lower Upper
43 100
58 0.0 27.5 41.3#



#17
Carbon Disulfide
Concen: 0.386 ug/l
RT: 4.718 min Scan# 470
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 76 Resp: 1666
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#

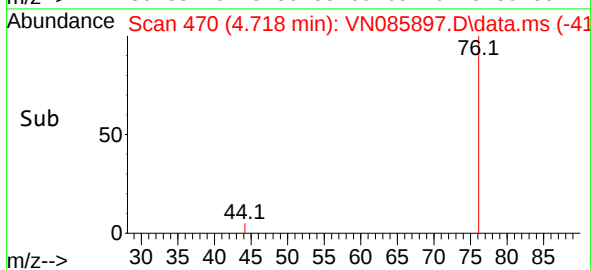



#18

Methyl Acetate

Concen: 0.264 ug/l

RT: 5.030 min Scan# 51

Delta R.T. 0.012 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :





VN0306WBL01

Tgt Ion: 43 Resp: 494

Ion Ratio Lower Upper

43 100

74 13.0 22.2 33.4#

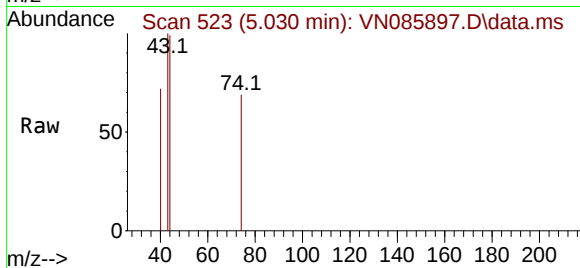

#25

2-Butanone

Concen: 0.212 ug/l

RT: 7.506 min Scan# 944

Delta R.T. 0.035 min

Lab File: VN085897.D




Acq: 06 Mar 2025 14:41


Tgt Ion: 43 Resp: 170

Ion Ratio Lower Upper

43 100

72 0.0 23.6 35.4#


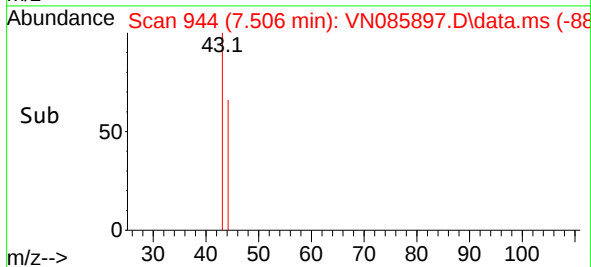

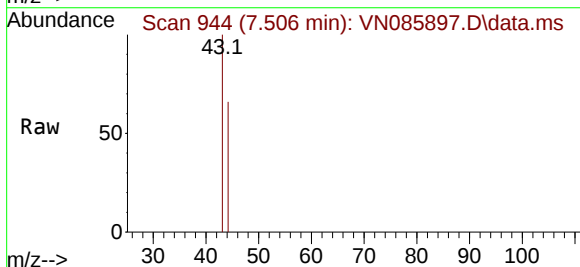




#31
Cyclohexane
Concen: 1.010 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.029 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion: 56 Resp: 2482
Ion Ratio Lower Upper
56 100
69 186.1 25.8 38.6#
84 171.9 74.5 111.7#



#33
1,2-Dichloroethane-d4
Concen: 58.735 ug/l
RT: 8.577 min Scan# 1126
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 65 Resp: 101028
Ion Ratio Lower Upper
65 100
67 51.3 0.0 106.2

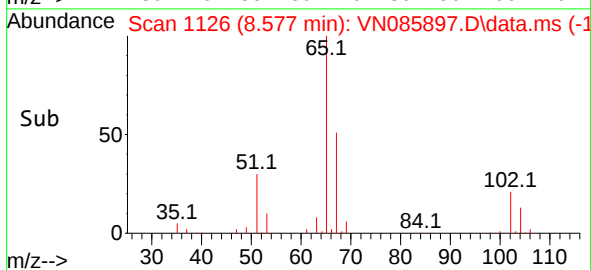

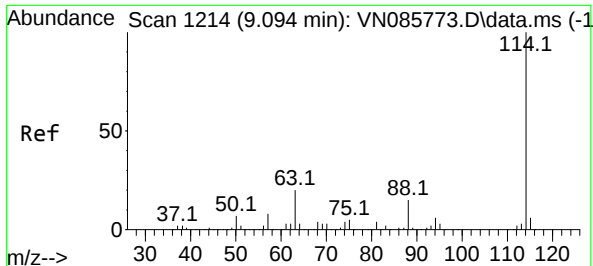

#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :

VN0306WBL01





Tgt Ion:114 Resp: 229960

Ion Ratio Lower Upper

114 100

63 20.3 0.0 39.2

88 15.7 0.0 30.0

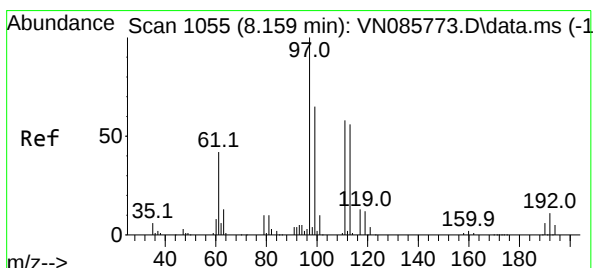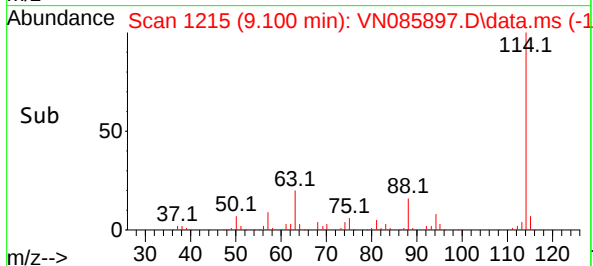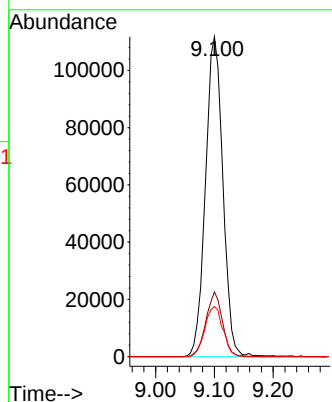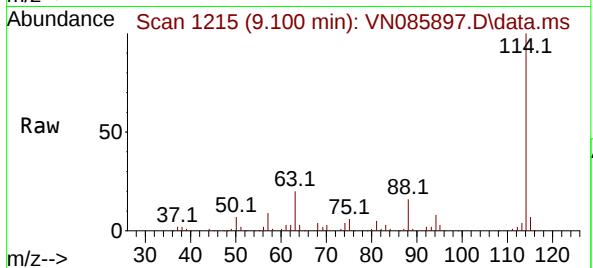

#35

Dibromofluoromethane

Concen: 59.032 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41




Tgt Ion:113 Resp: 88829


Ion Ratio Lower Upper

113 100

111 104.3 82.2 123.4

192 19.9 14.7 22.1

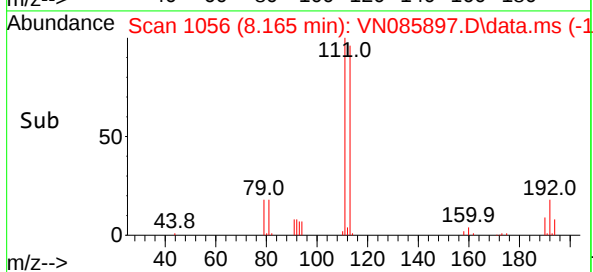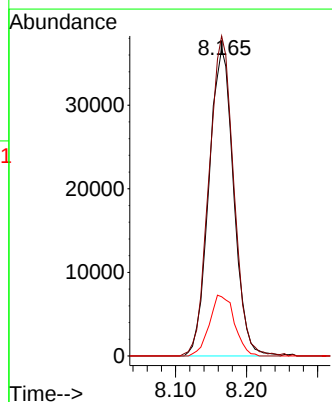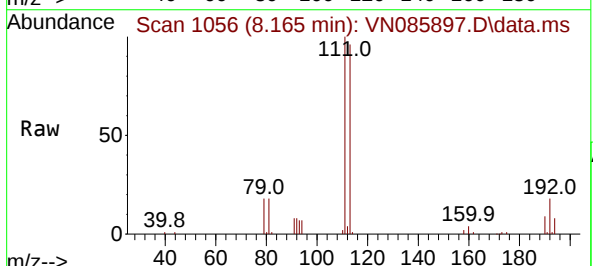

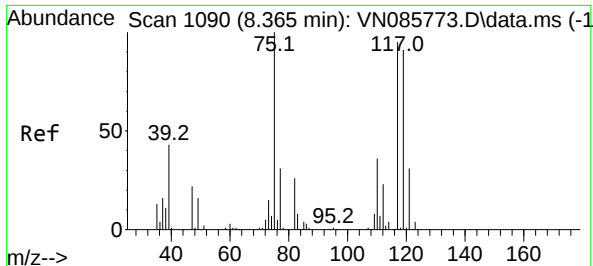

#36

1,1-Dichloropropene

Concen: 4.733 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.141 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :

VN0306WBL01





Tgt Ion: 75 Resp: 10080

Ion Ratio Lower Upper

75 100

110 8.7 17.3 52.0#

77 0.0 24.6 37.0#

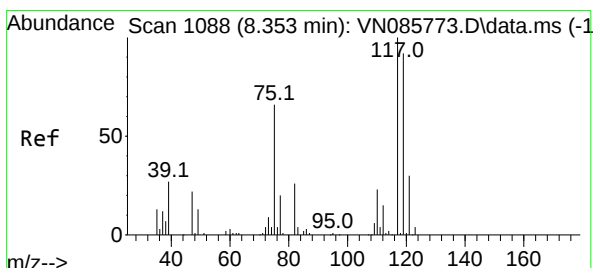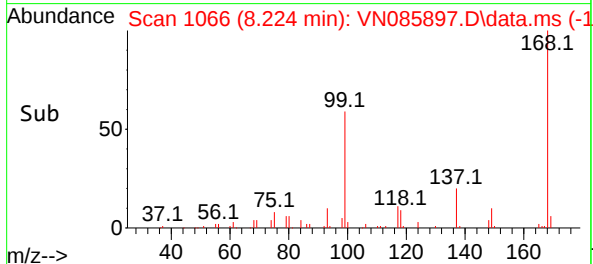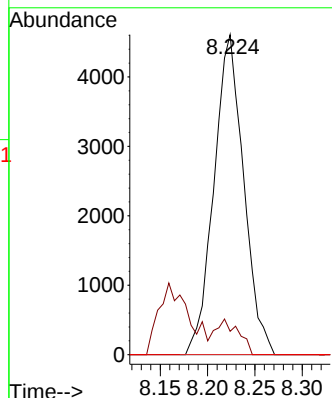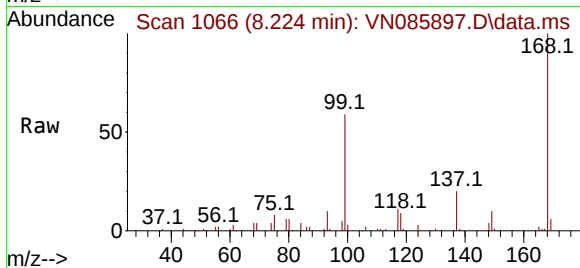

#38

Carbon Tetrachloride

Concen: 5.487 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.129 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41




Tgt Ion: 117 Resp: 13885


Ion Ratio Lower Upper

117 100

119 5.1 73.8 110.6#

121 0.0 24.3 36.5#


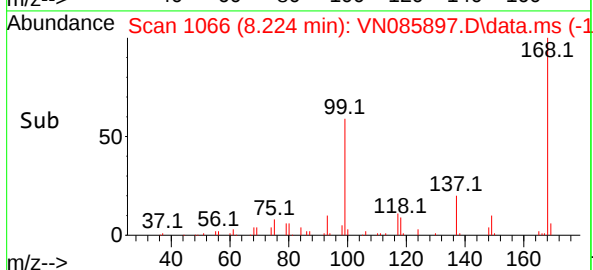

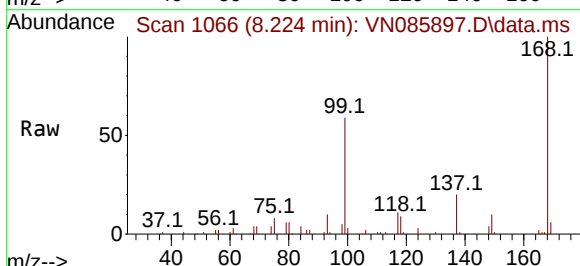




#43
Isopropyl Acetate
Concen: 0.231 ug/l
RT: 8.712 min Scan# 1144
Delta R.T. 0.029 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion: 43 Resp: 2383
Ion Ratio Lower Upper
43 100
61 0.0 22.6 34.0#
87 0.0 11.8 17.8#

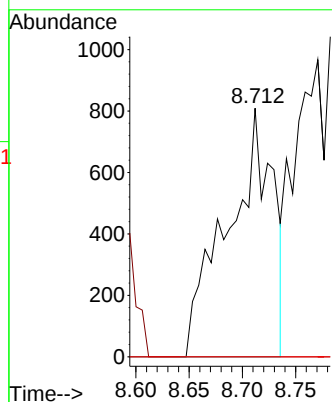

#50
Toluene-d8
Concen: 52.524 ug/l
RT: 10.565 min Scan# 1464
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 98 Resp: 287556
Ion Ratio Lower Upper
98 100
100 62.6 52.1 78.1

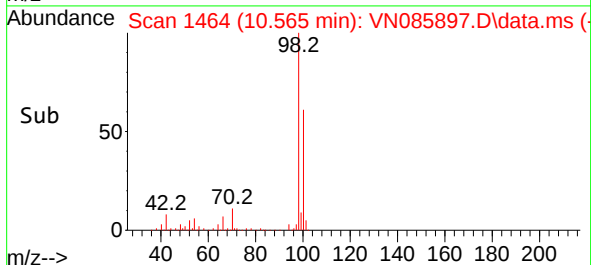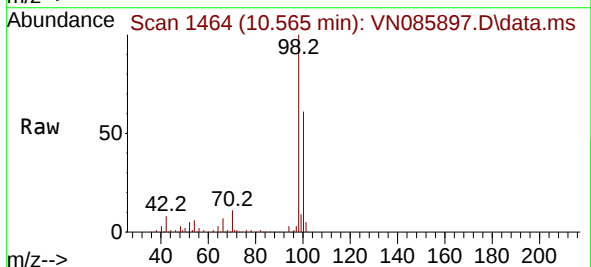



#59

2-Hexanone

Concen: 0.637 ug/l

RT: 11.200 min Scan# 11

Delta R.T. 0.012 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :





VN0306WBL01

Tgt Ion: 43 Resp: 741

Ion Ratio Lower Upper

43 100

58 37.7 29.8 89.5

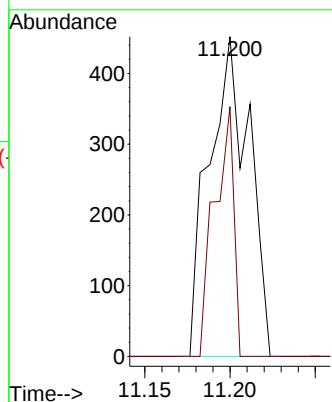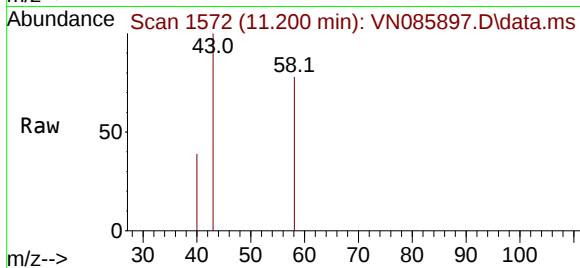

#62

4-Bromofluorobenzene

Concen: 47.473 ug/l

RT: 12.847 min Scan# 1852

Delta R.T. 0.006 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41




Tgt Ion: 95 Resp: 85632


Ion Ratio Lower Upper

95 100

174 83.0 0.0 152.4

176 80.0 0.0 146.6


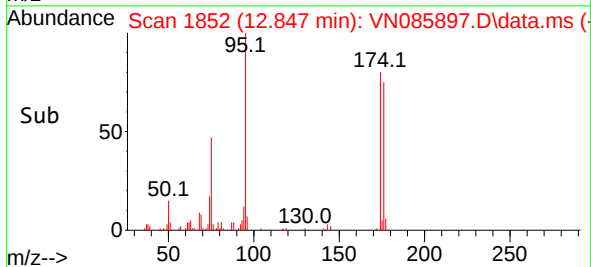
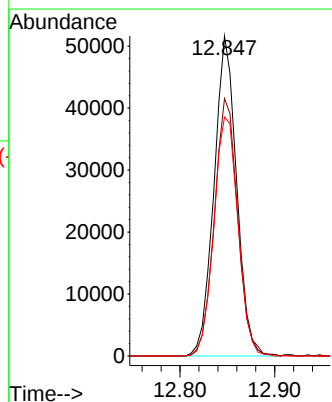
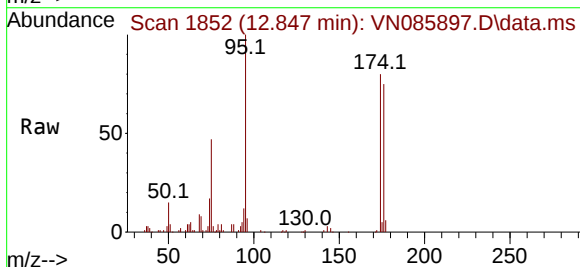




#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 117
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion:117 Resp: 211168
Ion Ratio Lower Upper
117 100
82 56.0 45.7 68.5
119 33.6 26.2 39.2



#70
Styrene
Concen: 0.691 ug/l
RT: 12.412 min Scan# 1778
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion:104 Resp: 498
Ion Ratio Lower Upper
104 100
78 0.0 39.0 58.6#
103 44.8 43.3 64.9


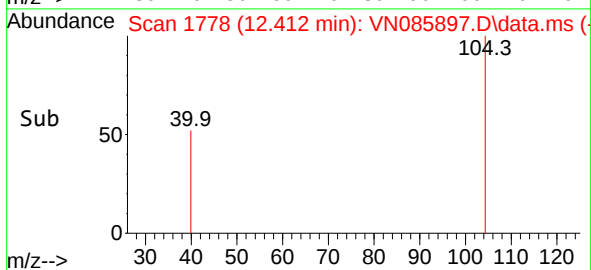

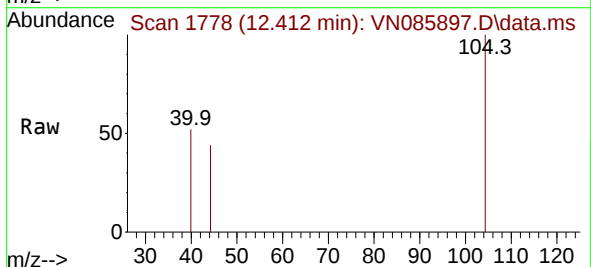


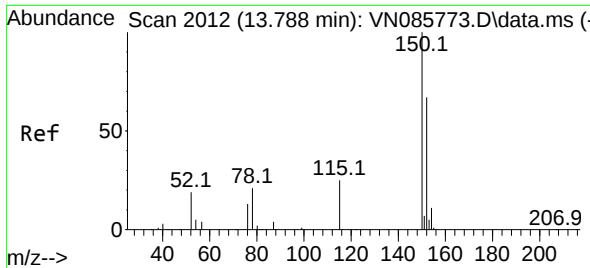

#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion:152 Resp: 85128
Ion Ratio Lower Upper
152 100
115 60.4 30.4 91.3
150 156.6 0.0 345.4

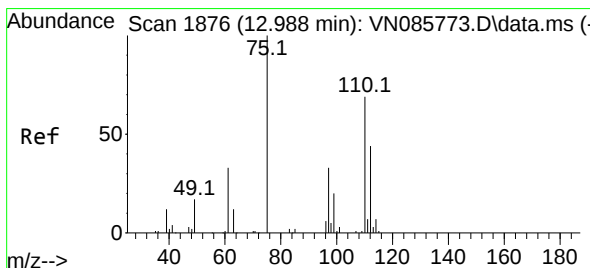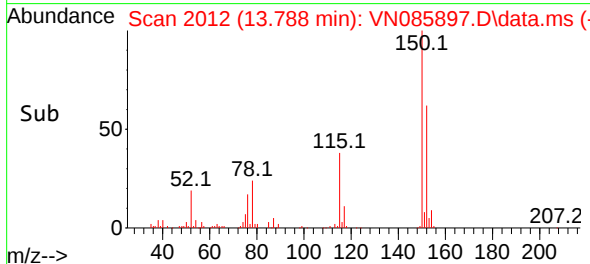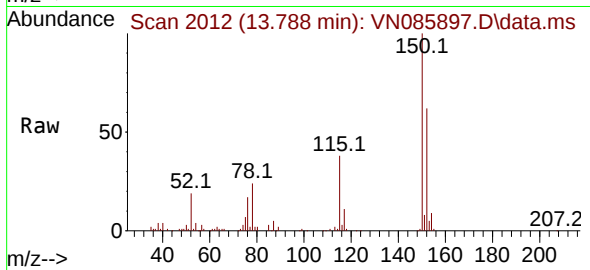

#76
1,2,3-Trichloropropane
Concen: 22.440 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 75 Resp: 42434
Ion Ratio Lower Upper
75 100
77 1.1 100.0 300.0#


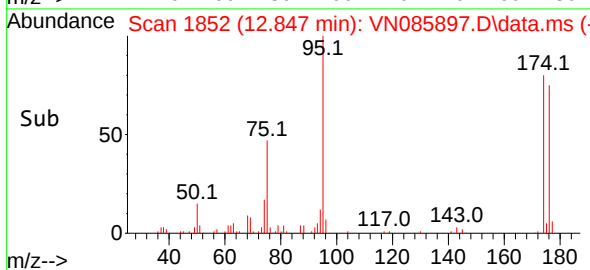

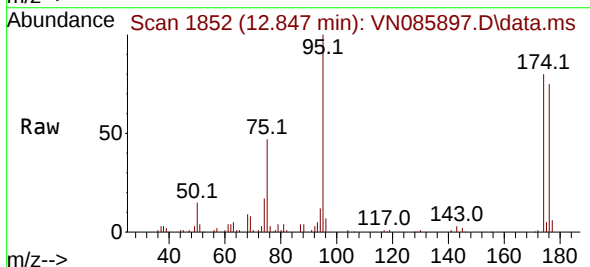




#77
Bromobenzene
Concen: 0.211 ug/l
RT: 12.988 min Scan# 11
Delta R.T. 0.012 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion:156 Resp: 333
Ion Ratio Lower Upper
156 100
77 233.0 104.1 312.3
158 100.3 48.1 144.4

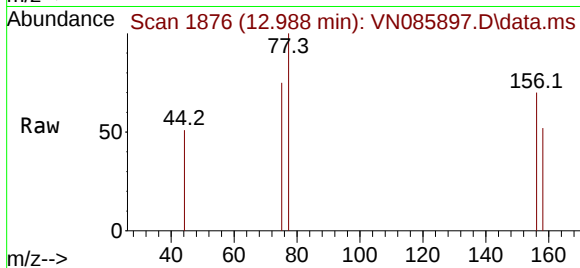

#79
2-Chlorotoluene
Concen: 0.204 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. 0.106 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 91 Resp: 910
Ion Ratio Lower Upper
91 100
126 27.6 16.4 49.1


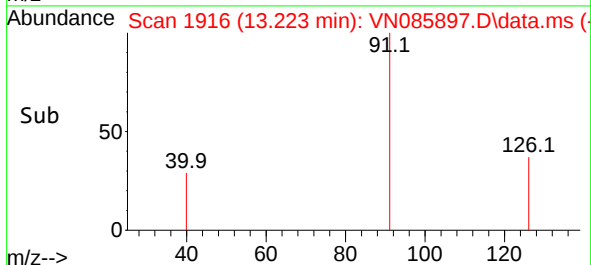

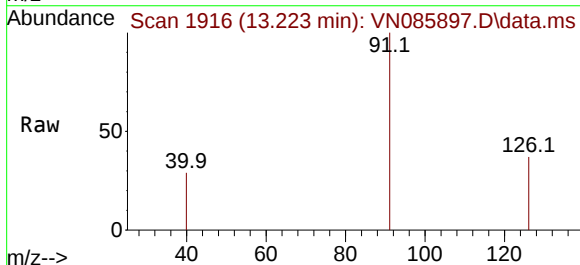




#81
trans-1,4-Dichloro-2-butene
Concen: 65.475 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.118 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion: 75 Resp: 42434
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.9 52.3#

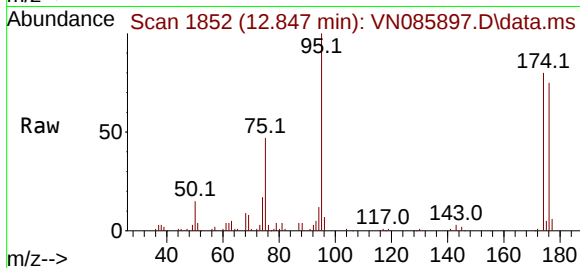

#82
4-Chlorotoluene
Concen: 0.206 ug/l
RT: 13.223 min Scan# 1916
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion: 91 Resp: 910
Ion Ratio Lower Upper
91 100
126 27.6 16.4 49.4


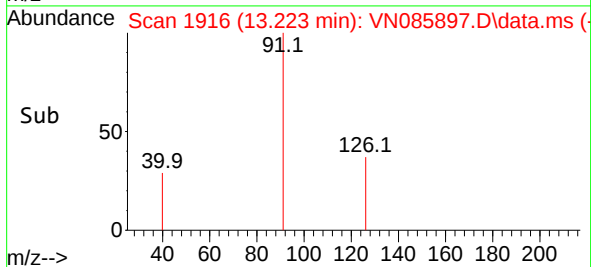

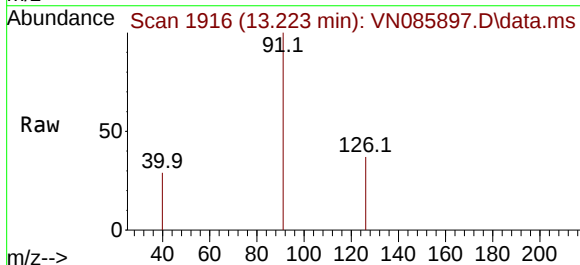




#85
 sec-Butylbenzene
 Concen: 0.235 ug/l
 RT: 13.612 min Scan# 1982
 Delta R.T. -0.000 min
 Lab File: VN085897.D
 Acq: 06 Mar 2025 14:41




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0306WBL01


Tgt Ion:105 Resp: 1326
 Ion Ratio Lower Upper
 105 100
 134 6.3 9.8 29.4#



#86
 p-Isopropyltoluene
 Concen: 0.861 ug/l
 RT: 13.729 min Scan# 2002
 Delta R.T. 0.006 min
 Lab File: VN085897.D
 Acq: 06 Mar 2025 14:41

Tgt Ion:119 Resp: 1137
 Ion Ratio Lower Upper
 119 100
 134 27.7 13.0 39.0
 91 5.5 11.7 35.1#

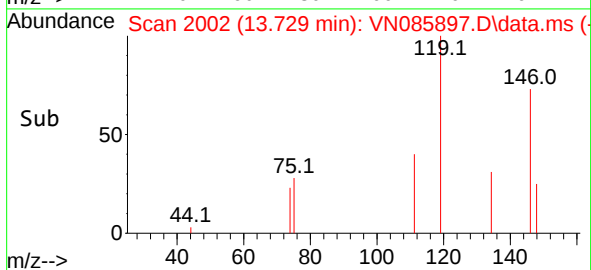



#87

1,3-Dichlorobenzene

Concen: 0.356 ug/l

RT: 13.741 min Scan# 2004

Delta R.T. 0.012 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :

VN0306WBL01





Tgt Ion:146 Resp: 1051

Ion Ratio Lower Upper

146 100

111 29.7 21.1 63.3

148 47.8 32.1 96.5

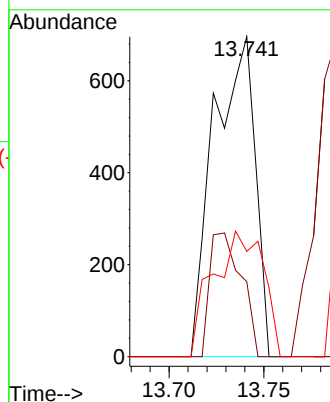

#88

1,4-Dichlorobenzene

Concen: 0.347 ug/l

RT: 13.741 min Scan# 2004

Delta R.T. -0.065 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41




Tgt Ion:146 Resp: 1051


Ion Ratio Lower Upper

146 100

111 29.7 20.4 61.3

148 47.8 31.8 95.4

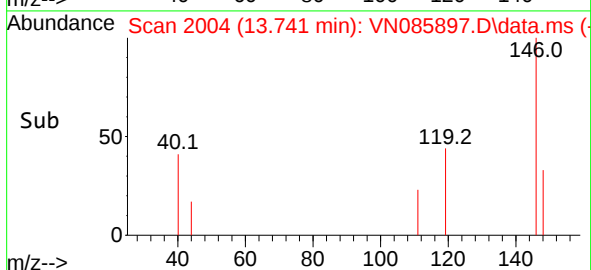

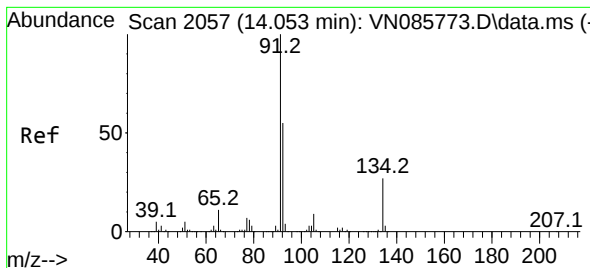

#89

n-Butylbenzene

Concen: 0.493 ug/l

RT: 14.053 min Scan# 2057

Delta R.T. -0.000 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41





Instrument :

MSVOA_N

ClientSampleId :

VN0306WBL01

Tgt Ion: 91	Resp:	1974
Ion	Ratio	Lower Upper
91	100	
92	56.8	27.1 81.3
134	14.5	12.7 38.1

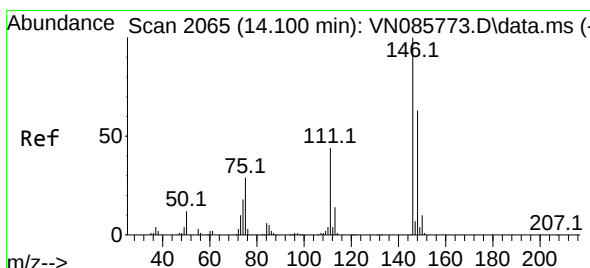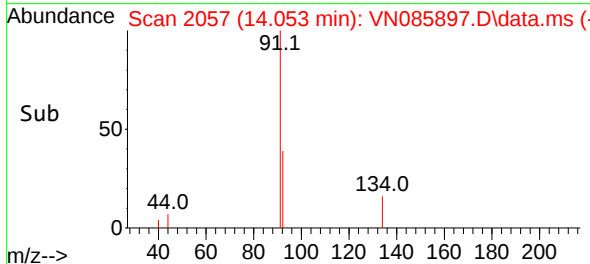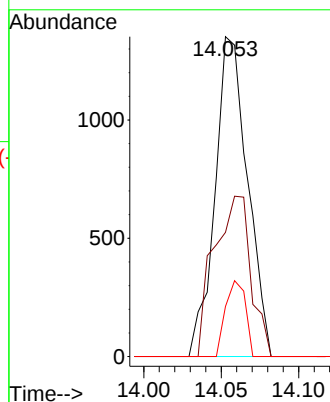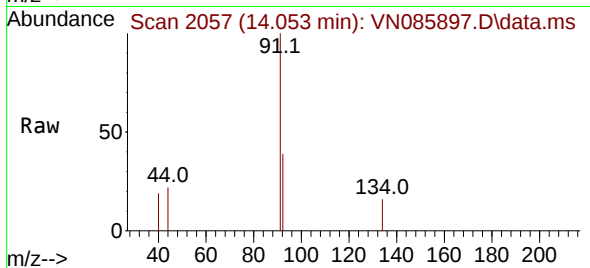

#91

1,2-Dichlorobenzene

Concen: 0.351 ug/l




RT: 14.106 min Scan# 2066


Delta R.T. 0.006 min

Lab File: VN085897.D

Acq: 06 Mar 2025 14:41

Tgt Ion: 146	Resp:	997
Ion	Ratio	Lower Upper
146	100	
111	25.8	21.4 64.3
148	72.6	32.0 96.2


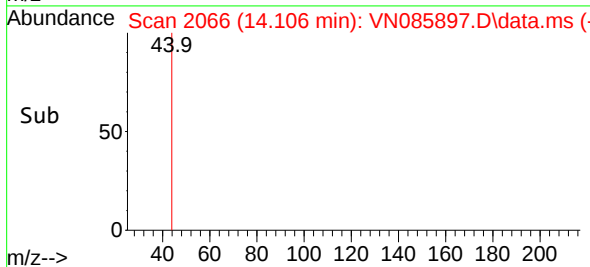
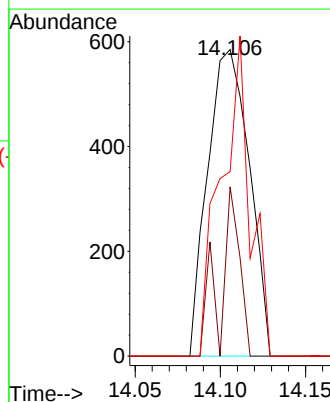
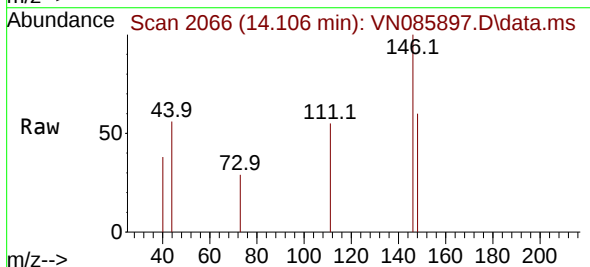




#92
 1,2-Dibromo-3-Chloropropane
 Concen: 0.336 ug/l
 RT: 14.717 min Scan# 2169
 Delta R.T. 0.006 min
 Lab File: VN085897.D
 Acq: 06 Mar 2025 14:41




Instrument :
 MSVOA_N
 ClientSampleId :
 VN0306WBL01


Tgt Ion: 75 Resp: 124
 Ion Ratio Lower Upper
 75 100
 155 53.2 39.9 119.6
 157 51.6 49.9 149.7

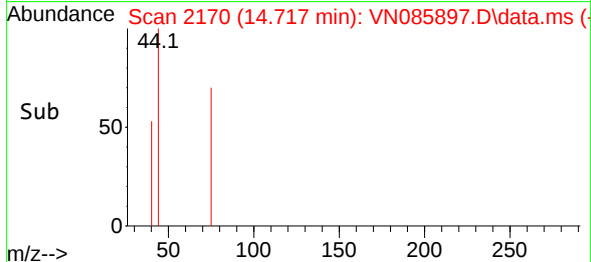

#93
 1,2,4-Trichlorobenzene
 Concen: 1.113 ug/l
 RT: 15.400 min Scan# 2286
 Delta R.T. 0.012 min
 Lab File: VN085897.D
 Acq: 06 Mar 2025 14:41

Tgt Ion: 180 Resp: 1506
 Ion Ratio Lower Upper
 180 100
 182 105.7 47.3 141.9
 145 10.3 16.2 48.5#


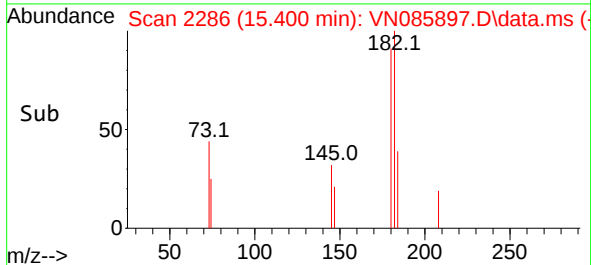

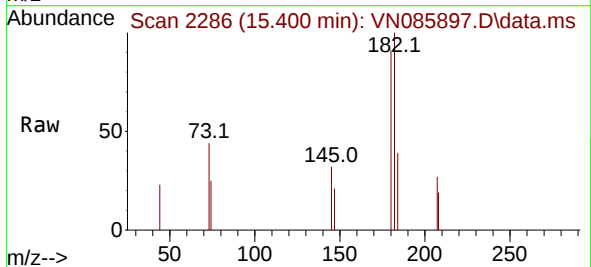




#94
Hexachlorobutadiene
Concen: 1.514 ug/l
RT: 15.494 min Scan# 21
Delta R.T. -0.000 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41




Instrument :
MSVOA_N
ClientSampleId :
VN0306WBL01


Tgt Ion:225 Resp: 1245
Ion Ratio Lower Upper
225 100
223 61.0 31.9 95.5
227 49.9 32.2 96.6

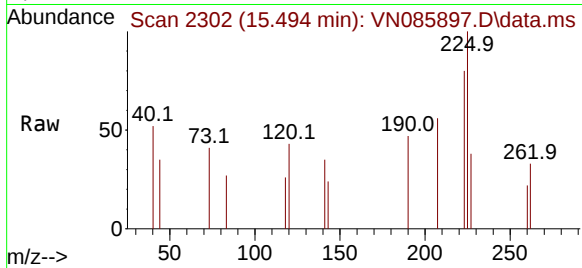

#95
Naphthalene
Concen: 1.673 ug/l
RT: 15.641 min Scan# 2327
Delta R.T. 0.006 min
Lab File: VN085897.D
Acq: 06 Mar 2025 14:41

Tgt Ion:128 Resp: 6213
Ion Ratio Lower Upper
128 100
127 14.1 10.2 15.2
129 13.0 8.7 13.1

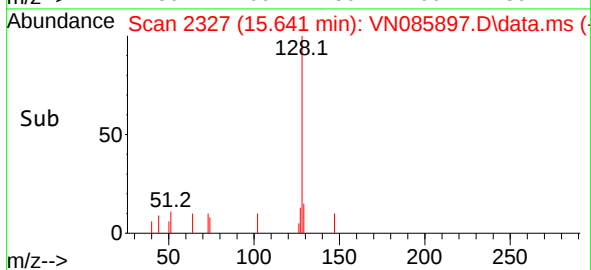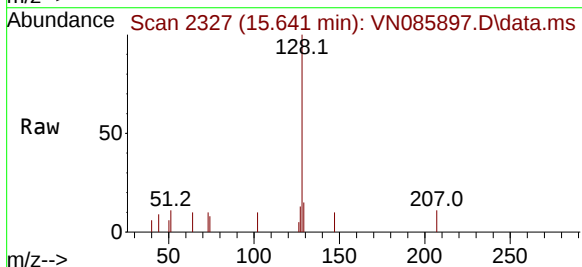



#96

1,2,3-Trichlorobenzene

Concen: 1.322 ug/l

RT: 15.847 min Scan# 21

Delta R.T. 0.012 min

Lab File: VN085897.D


Acq: 06 Mar 2025 14:41

Instrument :

MSVOA_N

ClientSampleId :

VN0306WBL01

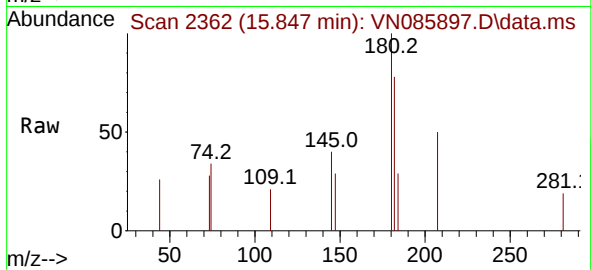

Tgt Ion:180 Resp: 1795

Ion Ratio Lower Upper

180 100

182 106.2 47.3 141.8

145 27.2 16.9 50.6

