

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030625\
 Data File : VN085899.D
 Acq On : 06 Mar 2025 15:30
 Operator : JC\MD
 Sample : PB166989ZHE#01
 Misc : 5.0mL/MSVOA_N/WATER
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 MSVOA_N
 ClientSampleId :
 PB166989ZHE#01

Quant Time: Mar 07 00:39:12 2025
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
 Quant Title : SW846 8260
 QLast Update : Wed Feb 19 03:43:32 2025
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) Pentafluorobenzene	8.224	168	151418	50.000	ug/l	0.00
34) 1,4-Difluorobenzene	9.100	114	266243	50.000	ug/l	0.00
63) Chlorobenzene-d5	11.865	117	269996	50.000	ug/l	0.00
72) 1,4-Dichlorobenzene-d4	13.788	152	97889	50.000	ug/l	0.00
System Monitoring Compounds						
33) 1,2-Dichloroethane-d4	8.576	65	109310	55.683	ug/l	0.00
Spiked Amount	50.000	Range	74 - 125	Recovery	= 111.360%	
35) Dibromofluoromethane	8.165	113	96008	55.108	ug/l	0.00
Spiked Amount	50.000	Range	75 - 124	Recovery	= 110.220%	
50) Toluene-d8	10.565	98	352300	55.581	ug/l	0.00
Spiked Amount	50.000	Range	86 - 113	Recovery	= 111.160%	
62) 4-Bromofluorobenzene	12.847	95	108983	52.185	ug/l	0.00
Spiked Amount	50.000	Range	77 - 121	Recovery	= 104.360%	
Target Compounds						
					Qvalue	
11) Tert butyl alcohol	5.524	59	175	0.725	ug/l #	72
16) Acetone	4.436	43	32452	52.245	ug/l	89
17) Carbon Disulfide	4.712	76	1042	0.212	ug/l #	75
18) Methyl Acetate	5.030	43	2192	1.026	ug/l #	60
20) Methylene Chloride	5.271	84	1240	0.621	ug/l #	90
25) 2-Butanone	7.482	43	3320	3.633	ug/l	99
29) Tetrahydrofuran	7.841	42	175	0.297	ug/l #	53
31) Cyclohexane	8.224	56	3246	1.158	ug/l #	17
36) 1,1-Dichloropropene	8.218	75	11064	4.487	ug/l #	51
37) Ethyl Acetate	7.565	43	1448	0.714	ug/l #	75
38) Carbon Tetrachloride	8.224	117	15358	5.242	ug/l #	18
43) Isopropyl Acetate	8.682	43	48615	13.251	ug/l #	91
45) 1,2-Dichloropropane	9.735	63	916	0.480	ug/l #	43
48) Methyl methacrylate	9.741	41	61475	40.795	ug/l #	37
51) 4-Methyl-2-Pentanone	10.447	43	7302	3.733	ug/l #	74
54) cis-1,3-Dichloropropene	10.359	75	29069	9.959	ug/l #	61
56) Ethyl methacrylate	10.876	69	117	0.509	ug/l #	30
57) 1,3-Dichloropropane	11.200	76	3868	1.258	ug/l #	42
59) 2-Hexanone	11.200	43	41673	30.965	ug/l #	55
70) Styrene	12.412	104	529	0.673	ug/l #	60
74) N-amyl acetate	12.470	43	982	0.415	ug/l #	37
76) 1,2,3-Trichloropropane	12.847	75	52796	24.280	ug/l #	1
81) trans-1,4-Dichloro-2-b...	12.847	75	52796	70.844	ug/l #	12
86) p-Isopropyltoluene	13.723	119	694	0.750	ug/l #	69
89) n-Butylbenzene	14.058	91	1276	0.277	ug/l	87
93) 1,2,4-Trichlorobenzene	15.400	180	1155	0.743	ug/l	92
94) Hexachlorobutadiene	15.500	225	692	0.732	ug/l	91
95) Naphthalene	15.647	128	4095	0.959	ug/l #	91
96) 1,2,3-Trichlorobenzene	15.835	180	1217	0.779	ug/l	94


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_N\Data\VN030625\
Data File : VN085899.D
Acq On : 06 Mar 2025 15:30
Operator : JC\MD
Sample : PB166989ZHE#01
Misc : 5.0mL/MSVOA_N/WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01

Quant Time: Mar 07 00:39:12 2025
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_N\methods\82N021825W.M
Quant Title : SW846 8260
QLast Update : Wed Feb 19 03:43:32 2025
Response via : Initial Calibration




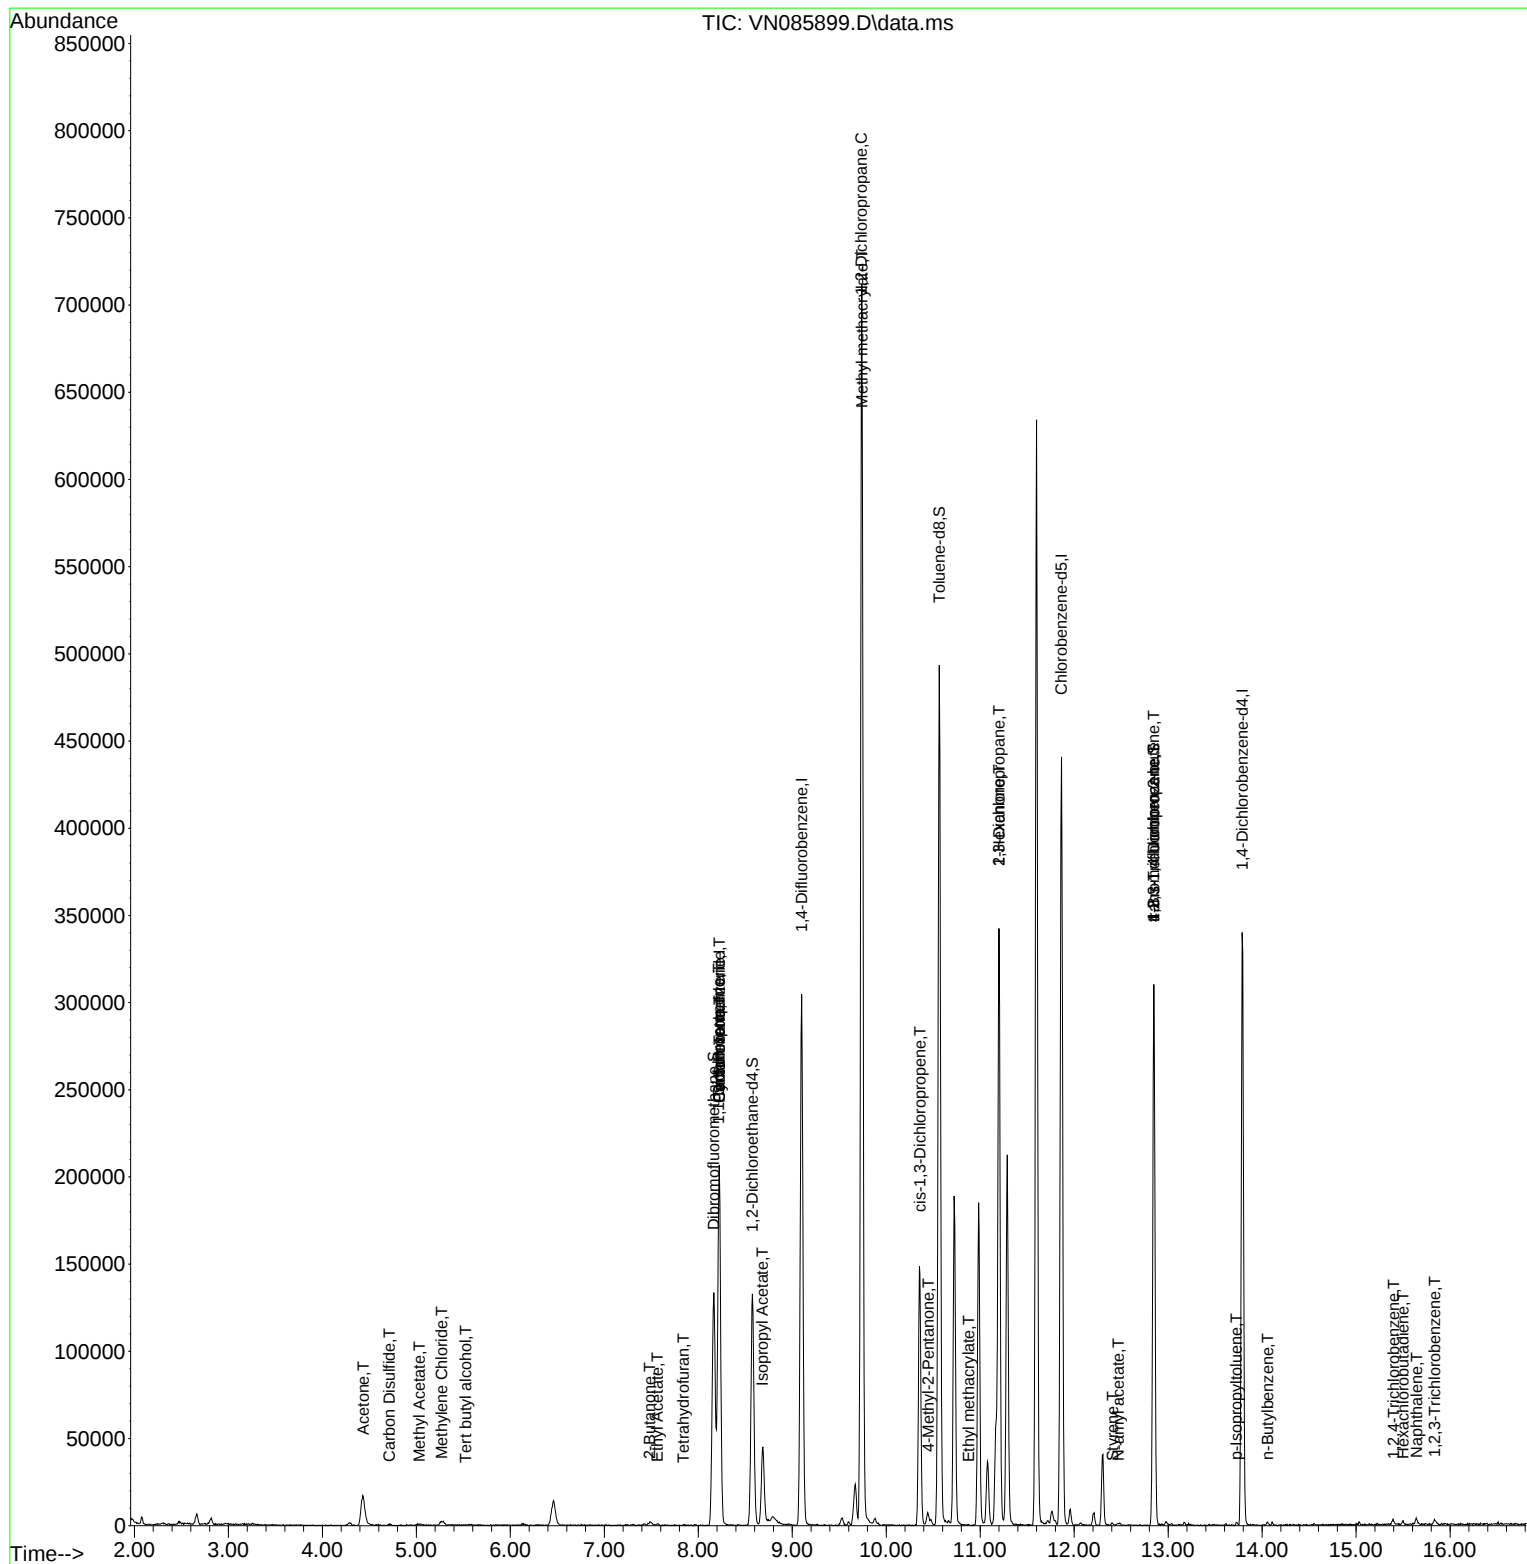




#1
Pentafluorobenzene
Concen: 50.000 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. 0.006 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion:168 Resp: 151418
Ion Ratio Lower Upper
168 100
99 57.2 47.9 71.9

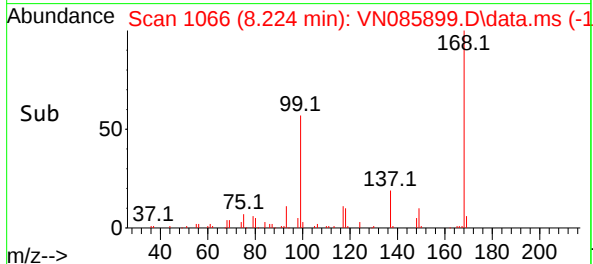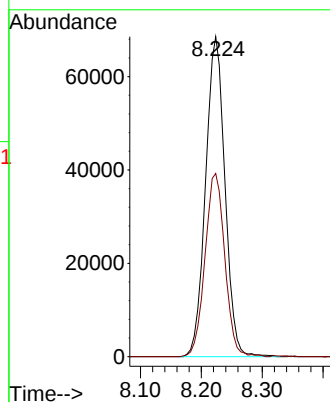

#11
Tert butyl alcohol
Concen: 0.725 ug/l
RT: 5.524 min Scan# 607
Delta R.T. 0.018 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 59 Resp: 175
Ion Ratio Lower Upper
59 100
57 0.0 8.3 12.5#


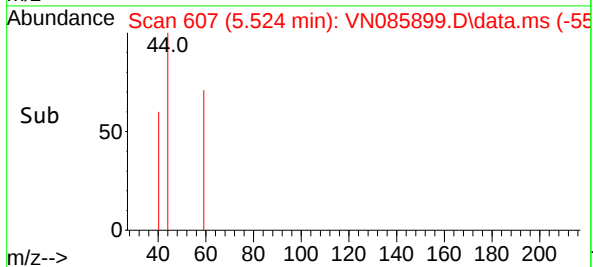
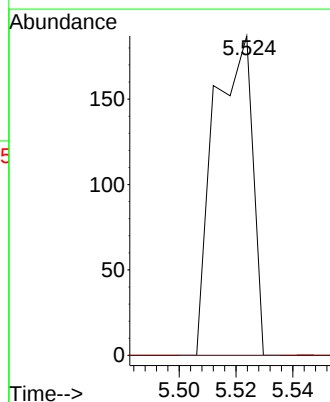
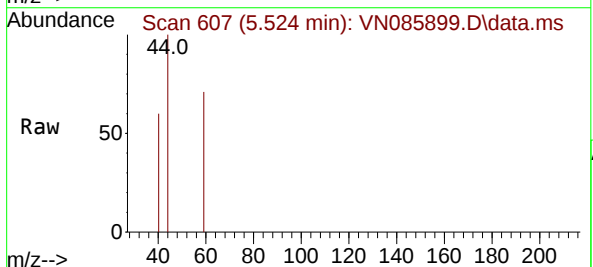




#16
Acetone
Concen: 52.245 ug/l
RT: 4.436 min Scan# 419
Delta R.T. 0.018 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion: 43 Resp: 32452
Ion Ratio Lower Upper
43 100
58 40.7 27.5 41.3

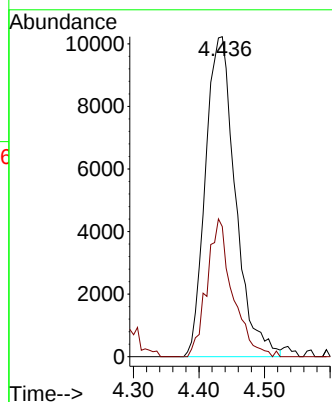

#17
Carbon Disulfide
Concen: 0.212 ug/l
RT: 4.712 min Scan# 469
Delta R.T. -0.000 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 76 Resp: 1042
Ion Ratio Lower Upper
76 100
78 0.0 7.4 11.0#


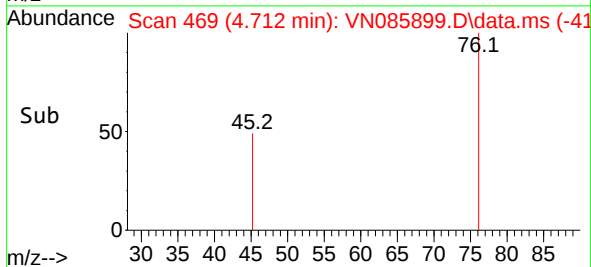
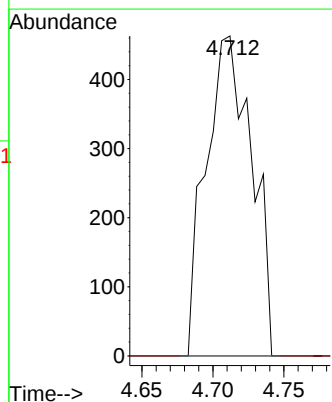
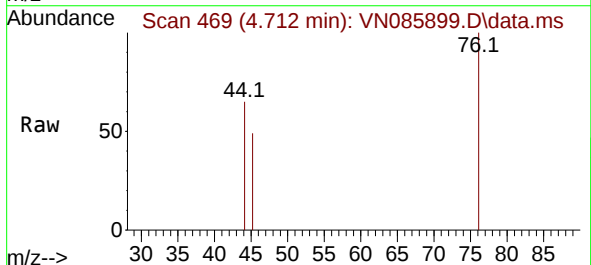




#18
Methyl Acetate
Concen: 1.026 ug/l
RT: 5.030 min Scan# 51
Delta R.T. 0.012 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion: 43 Resp: 2192
Ion Ratio Lower Upper
43 100
74 6.9 22.2 33.4#

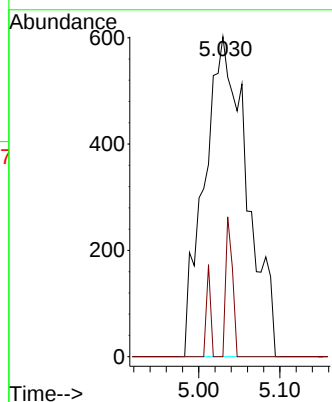

#20
Methylene Chloride
Concen: 0.621 ug/l
RT: 5.271 min Scan# 564
Delta R.T. -0.000 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 84 Resp: 1240
Ion Ratio Lower Upper
84 100
49 119.1 88.4 132.6
51 35.9 26.6 40.0
86 76.6 51.0 76.6#

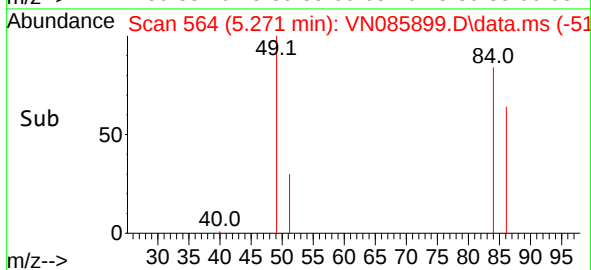



#25

2-Butanone

Concen: 3.633 ug/l

RT: 7.482 min Scan# 94

Delta R.T. 0.012 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :





PB166989ZHE#01

Tgt Ion: 43 Resp: 3320

Ion Ratio Lower Upper

43 100

72 30.0 23.6 35.4

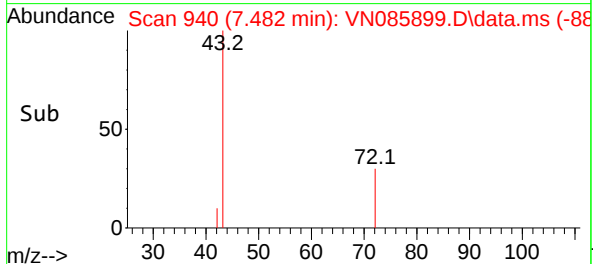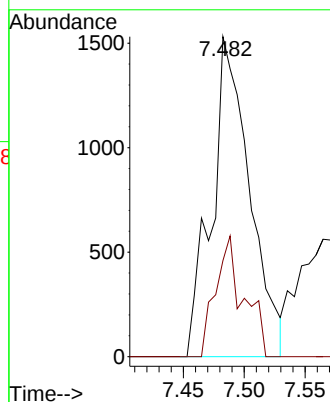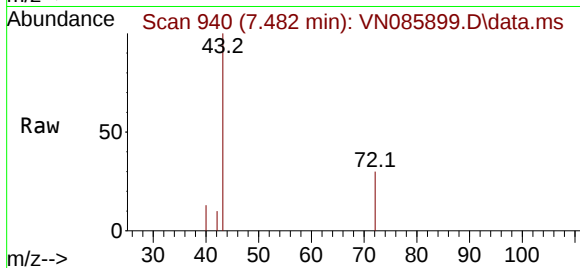

#29

Tetrahydrofuran

Concen: 0.297 ug/l

RT: 7.841 min Scan# 1001

Delta R.T. 0.012 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30




Tgt Ion: 42 Resp: 175


Ion Ratio Lower Upper

42 100

72 0.0 40.0 60.0#

71 33.7 37.0 55.4#

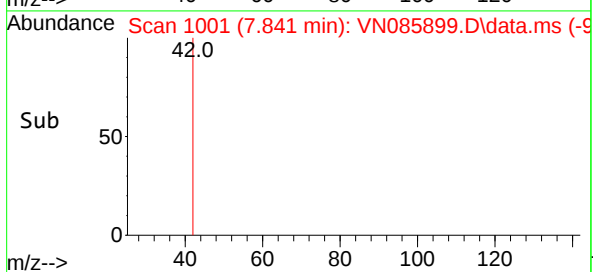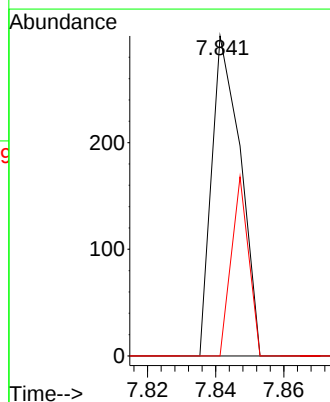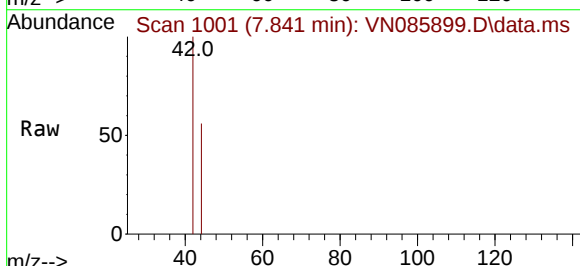



#31

Cyclohexane

Concen: 1.158 ug/l

RT: 8.224 min Scan# 1066

Delta R.T. -0.030 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :

PB166989ZHE#01





Tgt Ion: 56 Resp: 3246

Ion Ratio Lower Upper

56 100

69 169.3 25.8 38.6#

84 119.3 74.5 111.7#

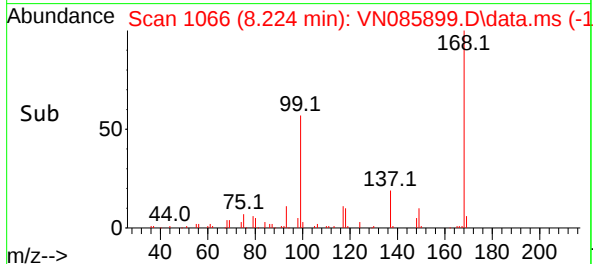

#33

1,2-Dichloroethane-d4

Concen: 55.683 ug/l

RT: 8.576 min Scan# 1126

Delta R.T. 0.006 min

Lab File: VN085899.D




Acq: 06 Mar 2025 15:30


Tgt Ion: 65 Resp: 109310

Ion Ratio Lower Upper

65 100

67 52.9 0.0 106.2

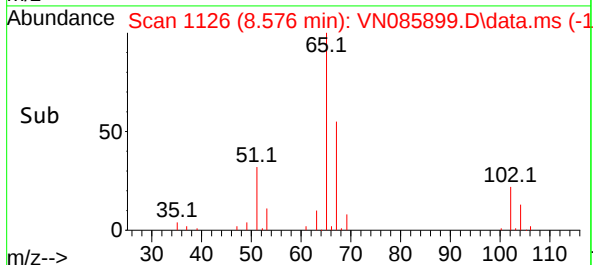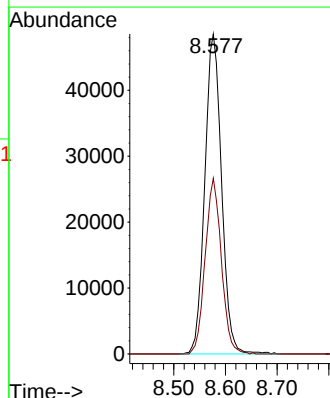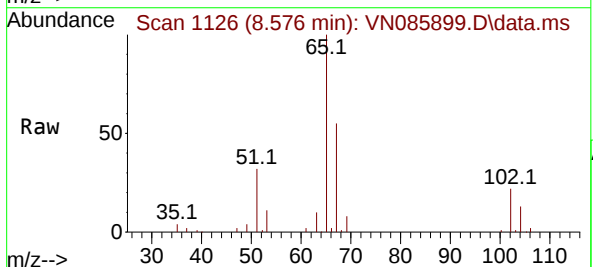



#34

1,4-Difluorobenzene

Concen: 50.000 ug/l

RT: 9.100 min Scan# 1

Delta R.T. 0.006 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :

PB166989ZHE#01





Tgt Ion:114 Resp: 266243

Ion Ratio Lower Upper

114 100

63 18.6 0.0 39.2

88 15.8 0.0 30.0

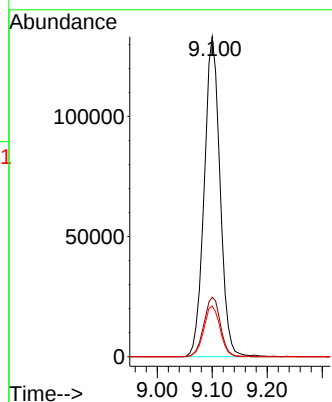

#35

Dibromofluoromethane

Concen: 55.108 ug/l

RT: 8.165 min Scan# 1056

Delta R.T. 0.006 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30




Tgt Ion:113 Resp: 96008


Ion Ratio Lower Upper

113 100

111 102.3 82.2 123.4

192 19.4 14.7 22.1

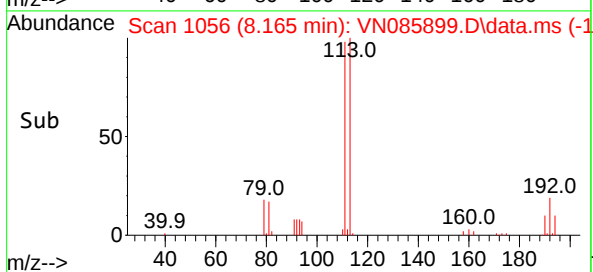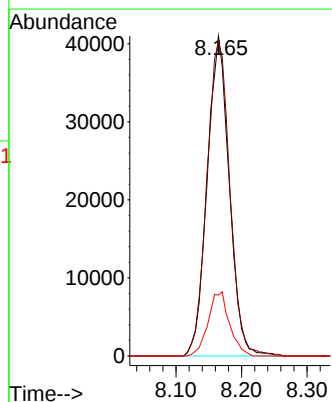



#36

1,1-Dichloropropene

Concen: 4.487 ug/l

RT: 8.218 min Scan# 1

Delta R.T. -0.147 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :

PB166989ZHE#01





Tgt Ion: 75 Resp: 11064

Ion Ratio Lower Upper

75 100

110 10.5 17.3 52.0#

77 0.0 24.6 37.0#

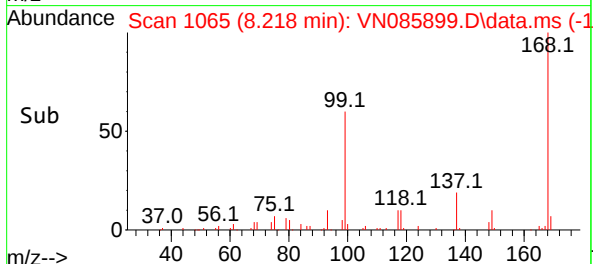

#37

Ethyl Acetate

Concen: 0.714 ug/l

RT: 7.565 min Scan# 954

Delta R.T. 0.012 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30




Tgt Ion: 43 Resp: 1448


Ion Ratio Lower Upper

43 100

61 0.0 12.2 18.2#


70 7.7 9.5 14.3#

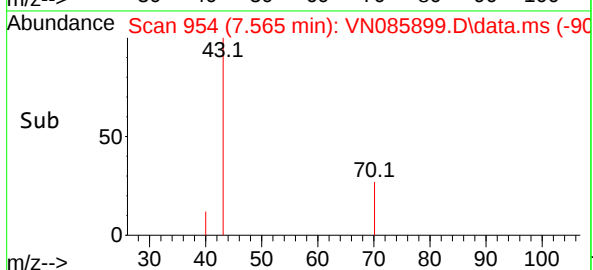






#38
Carbon Tetrachloride
Concen: 5.242 ug/l
RT: 8.224 min Scan# 1066
Delta R.T. -0.130 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01



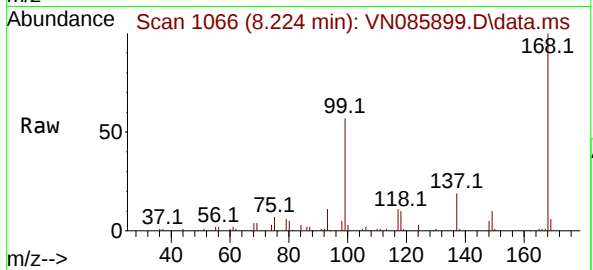



Tgt Ion:117 Resp: 15358
Ion Ratio Lower Upper
117 100
119 5.0 73.8 110.6#
121 0.0 24.3 36.5#

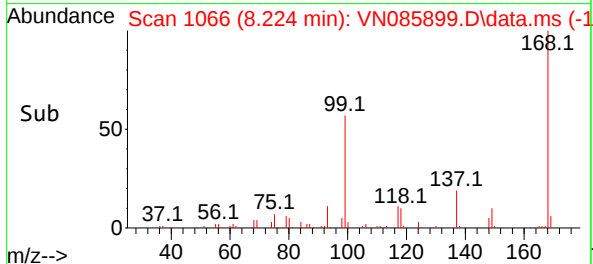

#43
Isopropyl Acetate
Concen: 13.251 ug/l
RT: 8.682 min Scan# 1144
Delta R.T. -0.001 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 43 Resp: 48615
Ion Ratio Lower Upper
43 100
61 21.8 22.6 34.0#
87 15.6 11.8 17.8

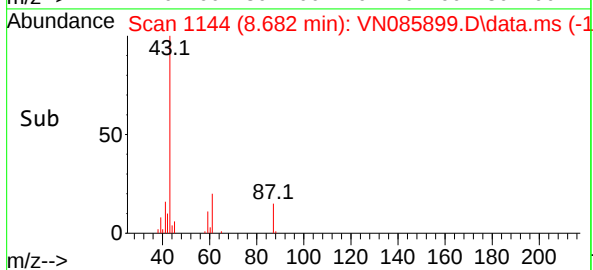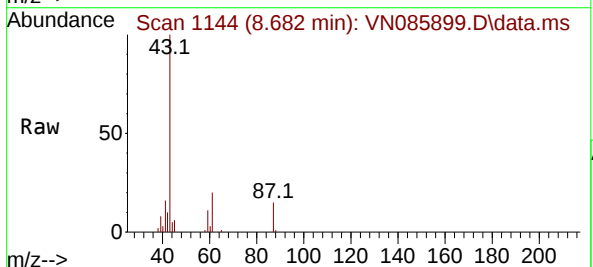



#45

1,2-Dichloropropane

Concen: 0.480 ug/l

RT: 9.735 min Scan# 11

Delta R.T. 0.117 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :





PB166989ZHE#01

Tgt Ion: 63 Resp: 916

Ion Ratio Lower Upper

63 100

65 0.0 25.1 37.7#

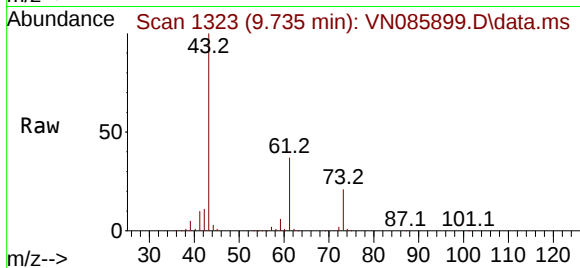

#48

Methyl methacrylate

Concen: 40.795 ug/l

RT: 9.741 min Scan# 1324

Delta R.T. 0.065 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30




Tgt Ion: 41 Resp: 61475


Ion Ratio Lower Upper

41 100

69 0.1 76.0 114.0#

39 52.7 42.3 63.5

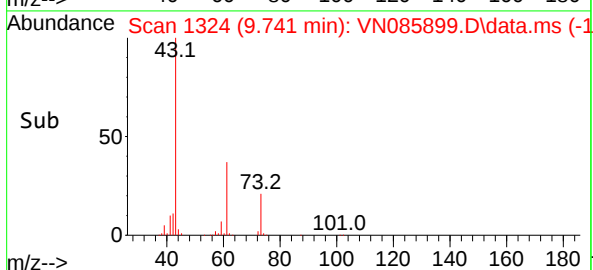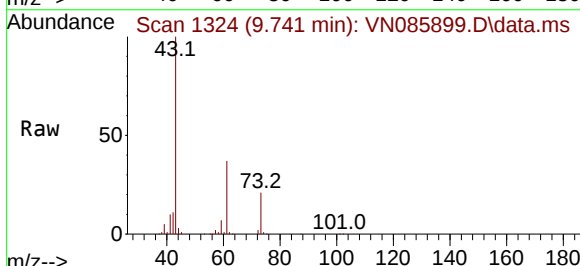

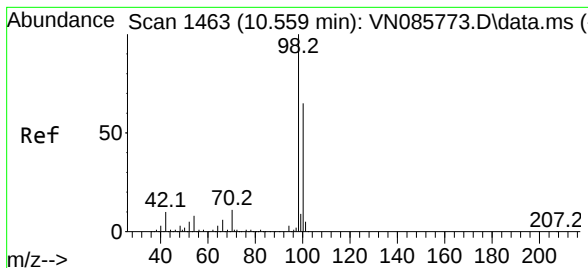

#50

Toluene-d8

Concen: 55.581 ug/l

RT: 10.565 min Scan# 1464

Delta R.T. 0.006 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :





PB166989ZHE#01

Tgt Ion: 98 Resp: 352300

Ion Ratio Lower Upper

98 100

100 65.3 52.1 78.1

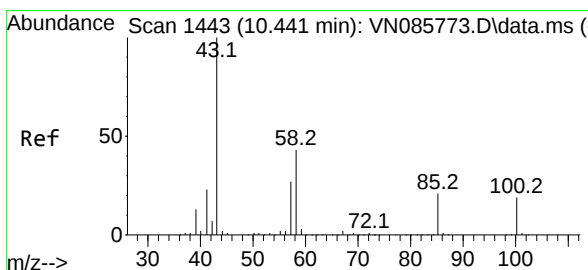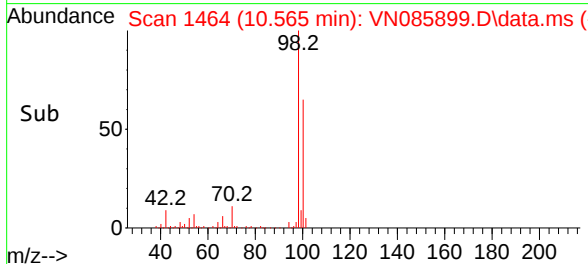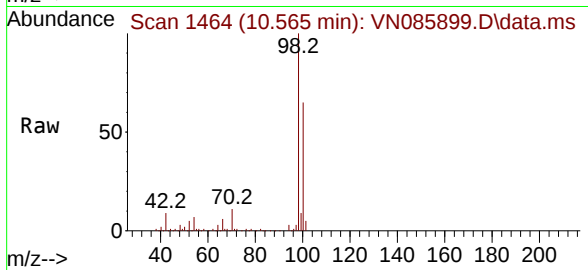

#51

4-Methyl-2-Pentanone

Concen: 3.733 ug/l

RT: 10.447 min Scan# 1444

Delta R.T. 0.006 min

Lab File: VN085899.D




Acq: 06 Mar 2025 15:30


Tgt Ion: 43 Resp: 7302

Ion Ratio Lower Upper

43 100

58 26.5 34.6 52.0#


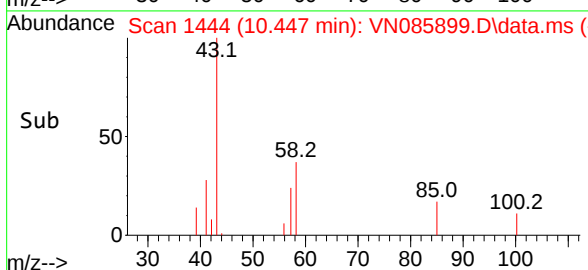

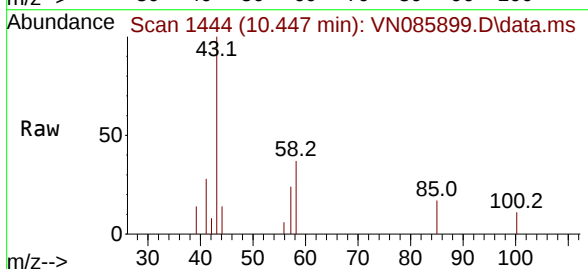




#54
 cis-1,3-Dichloropropene
 Concen: 9.959 ug/l
 RT: 10.359 min Scan# 1429
 Delta R.T. 0.053 min
 Lab File: VN085899.D
 Acq: 06 Mar 2025 15:30




Instrument :
 MSVOA_N
 ClientSampleId :
 PB166989ZHE#01


Tgt Ion: 75 Resp: 29069
 Ion Ratio Lower Upper
 75 100
 77 0.0 26.1 39.1#
 39 25.9 33.4 50.0#



#56
 Ethyl methacrylate
 Concen: 0.509 ug/l
 RT: 10.876 min Scan# 1517
 Delta R.T. 0.005 min
 Lab File: VN085899.D
 Acq: 06 Mar 2025 15:30

Tgt Ion: 69 Resp: 117
 Ion Ratio Lower Upper
 69 100
 41 0.0 46.0 69.0#
 39 0.0 22.0 33.0#

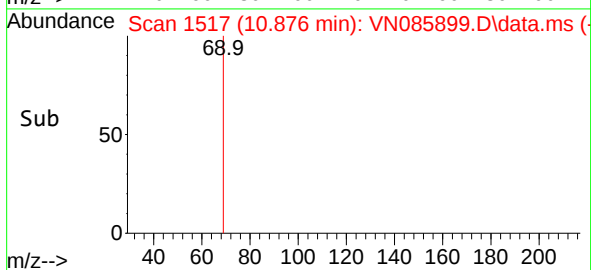



#57

1,3-Dichloropropane

Concen: 1.258 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.041 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :





PB166989ZHE#01

Tgt Ion: 76 Resp: 3868

Ion Ratio Lower Upper

76 100

78 0.0 25.9 38.9#

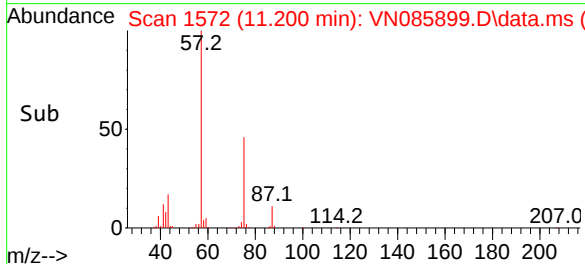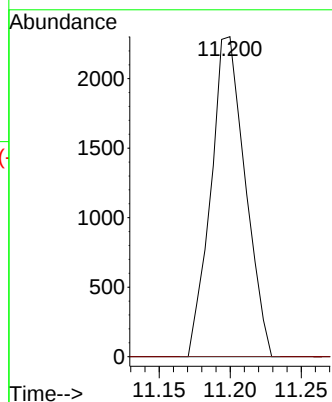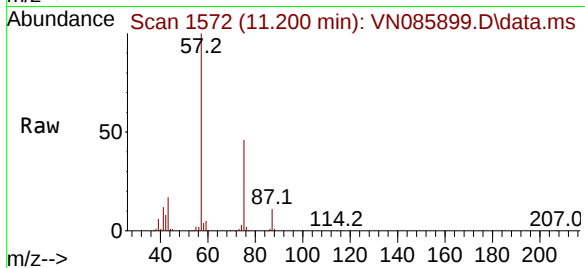

#59

2-Hexanone

Concen: 30.965 ug/l

RT: 11.200 min Scan# 1572

Delta R.T. 0.012 min

Lab File: VN085899.D




Acq: 06 Mar 2025 15:30


Tgt Ion: 43 Resp: 41673

Ion Ratio Lower Upper

43 100

58 25.4 29.8 89.5#


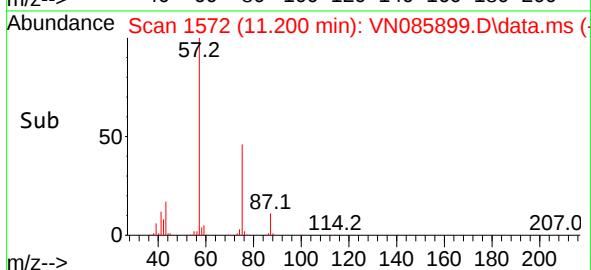

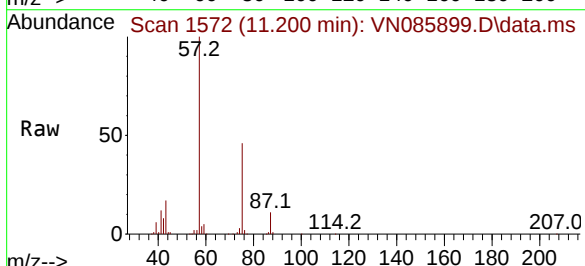




#62
4-Bromofluorobenzene
Concen: 52.185 ug/l
RT: 12.847 min Scan# 1851
Delta R.T. 0.006 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion: 95 Resp: 108983
Ion Ratio Lower Upper
95 100
174 80.1 0.0 152.4
176 76.6 0.0 146.6



#63
Chlorobenzene-d5
Concen: 50.000 ug/l
RT: 11.865 min Scan# 1685
Delta R.T. 0.006 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 117 Resp: 269996
Ion Ratio Lower Upper
117 100
82 54.7 45.7 68.5
119 32.5 26.2 39.2




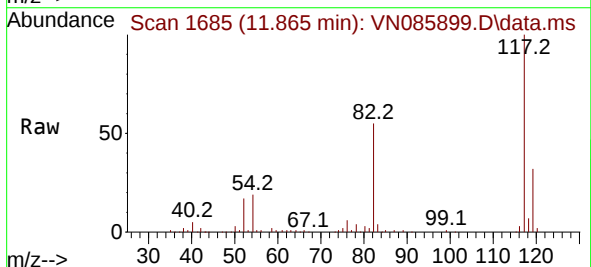




#70
Styrene
Concen: 0.673 ug/l
RT: 12.412 min Scan# 11
Delta R.T. 0.006 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion:104 Resp: 529
Ion Ratio Lower Upper
104 100
78 26.1 39.0 58.6#
103 21.0 43.3 64.9#



#72
1,4-Dichlorobenzene-d4
Concen: 50.000 ug/l
RT: 13.788 min Scan# 2012
Delta R.T. -0.000 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion:152 Resp: 97889
Ion Ratio Lower Upper
152 100
115 61.4 30.4 91.3
150 159.7 0.0 345.4


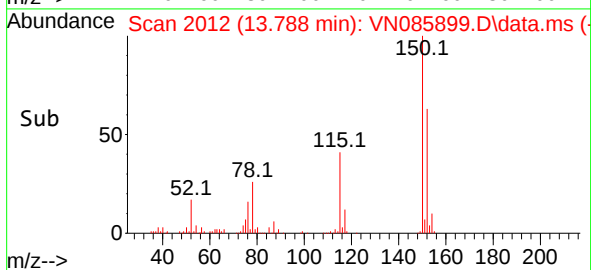

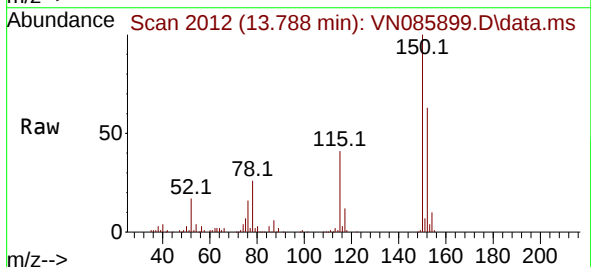




#74
N-amy1 acetate
Concen: 0.415 ug/l
RT: 12.470 min Scan# 11
Delta R.T. -0.018 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion: 43	Resp: 982
Ion Ratio	Lower Upper
43 100	
70 0.0	41.0 61.4#
55 0.0	24.6 36.8#
61 0.0	21.6 32.4#

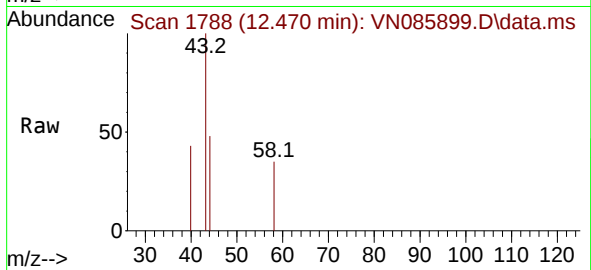

#76
1,2,3-Trichloropropane
Concen: 24.280 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. -0.141 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 75	Resp: 52796
Ion Ratio	Lower Upper
75 100	
77 1.3	100.0 300.0#


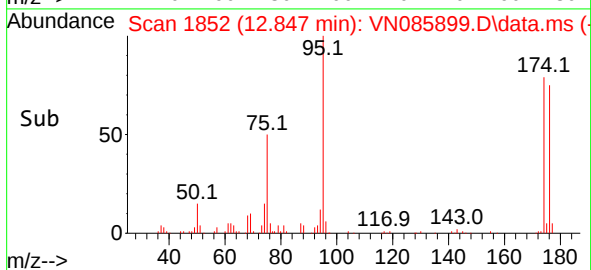

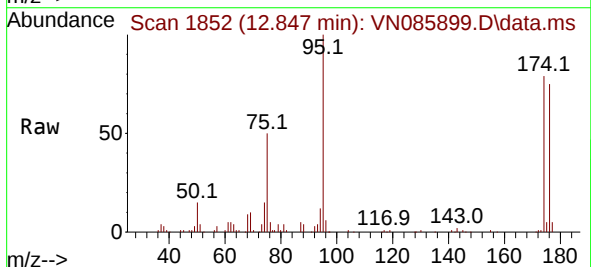




#81
trans-1,4-Dichloro-2-butene
Concen: 70.844 ug/l
RT: 12.847 min Scan# 1852
Delta R.T. 0.117 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion: 75 Resp: 52796
Ion Ratio Lower Upper
75 100
53 0.0 74.2 111.4#
89 0.0 34.9 52.3#

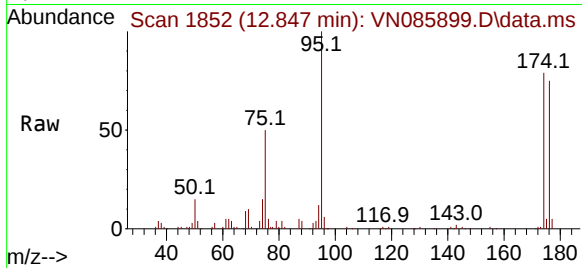

#86
p-Isopropyltoluene
Concen: 0.750 ug/l
RT: 13.723 min Scan# 2001
Delta R.T. 0.000 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion: 119 Resp: 694
Ion Ratio Lower Upper
119 100
134 8.1 13.0 39.0#
91 10.4 11.7 35.1#

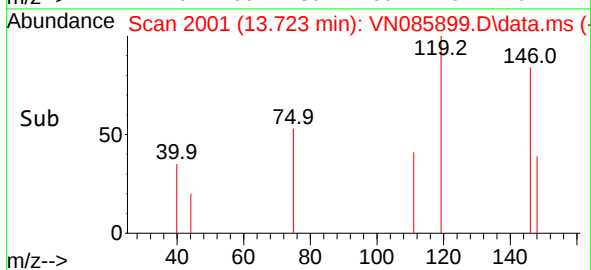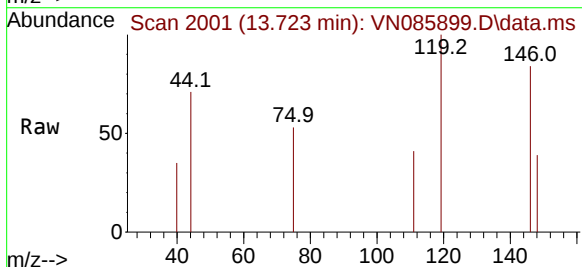



#89

n-Butylbenzene

Concen: 0.277 ug/l

RT: 14.058 min Scan# 2058

Delta R.T. 0.006 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30

Instrument :

MSVOA_N

ClientSampleId :

PB166989ZHE#01





Tgt Ion: 91 Resp: 1276

Ion Ratio Lower Upper

91 100

92 46.5 27.1 81.3

134 16.1 12.7 38.1



#93

1,2,4-Trichlorobenzene

Concen: 0.743 ug/l

RT: 15.400 min Scan# 2286

Delta R.T. 0.012 min

Lab File: VN085899.D

Acq: 06 Mar 2025 15:30




Tgt Ion: 180 Resp: 1155


Ion Ratio Lower Upper

180 100

182 89.1 47.3 141.9

145 23.6 16.2 48.5


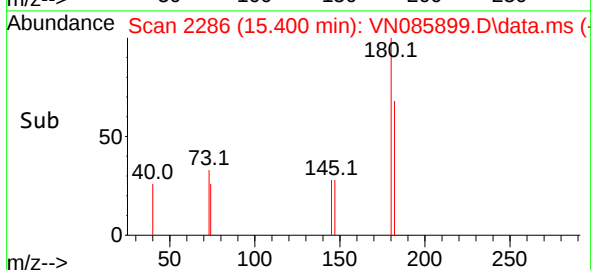






#94
Hexachlorobutadiene
Concen: 0.732 ug/l
RT: 15.500 min Scan# 21
Delta R.T. 0.006 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30




Instrument :
MSVOA_N
ClientSampleId :
PB166989ZHE#01


Tgt Ion:225 Resp: 692
Ion Ratio Lower Upper
225 100
223 61.1 31.9 95.5
227 53.5 32.2 96.6

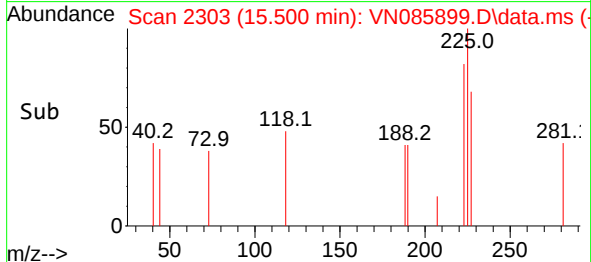

#95
Naphthalene
Concen: 0.959 ug/l
RT: 15.647 min Scan# 2328
Delta R.T. 0.012 min
Lab File: VN085899.D
Acq: 06 Mar 2025 15:30

Tgt Ion:128 Resp: 4095
Ion Ratio Lower Upper
128 100
127 8.8 10.2 15.2#
129 7.7 8.7 13.1#

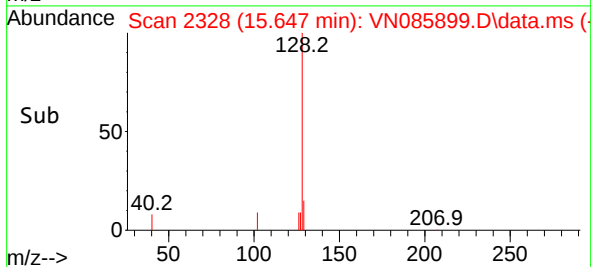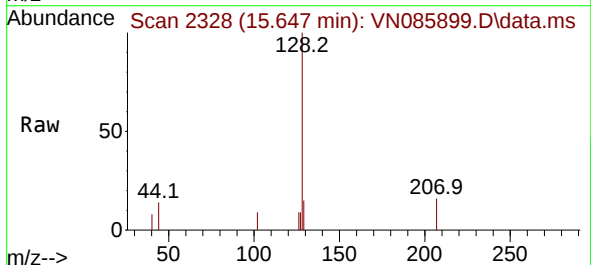



#96
 1,2,3-Trichlorobenzene
 Concen: 0.779 ug/l
 RT: 15.835 min Scan# 21
 Delta R.T. -0.000 min
 Lab File: VN085899.D
 Acq: 06 Mar 2025 15:30

Instrument :
 MSVOA_N
 ClientSampleId :
 PB166989ZHE#01

Tgt Ion:	180	Resp:	1217
Ion	Ratio	Lower	Upper
180	100		
182	99.8	47.3	141.8
145	28.6	16.9	50.6

